


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN082919\  
 Data File : BN007505.D  
 Acq On : 29 Aug 2019 16:55  
 Operator : HP/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-SIM-BN082319.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Aug 29 12:18:45 2019

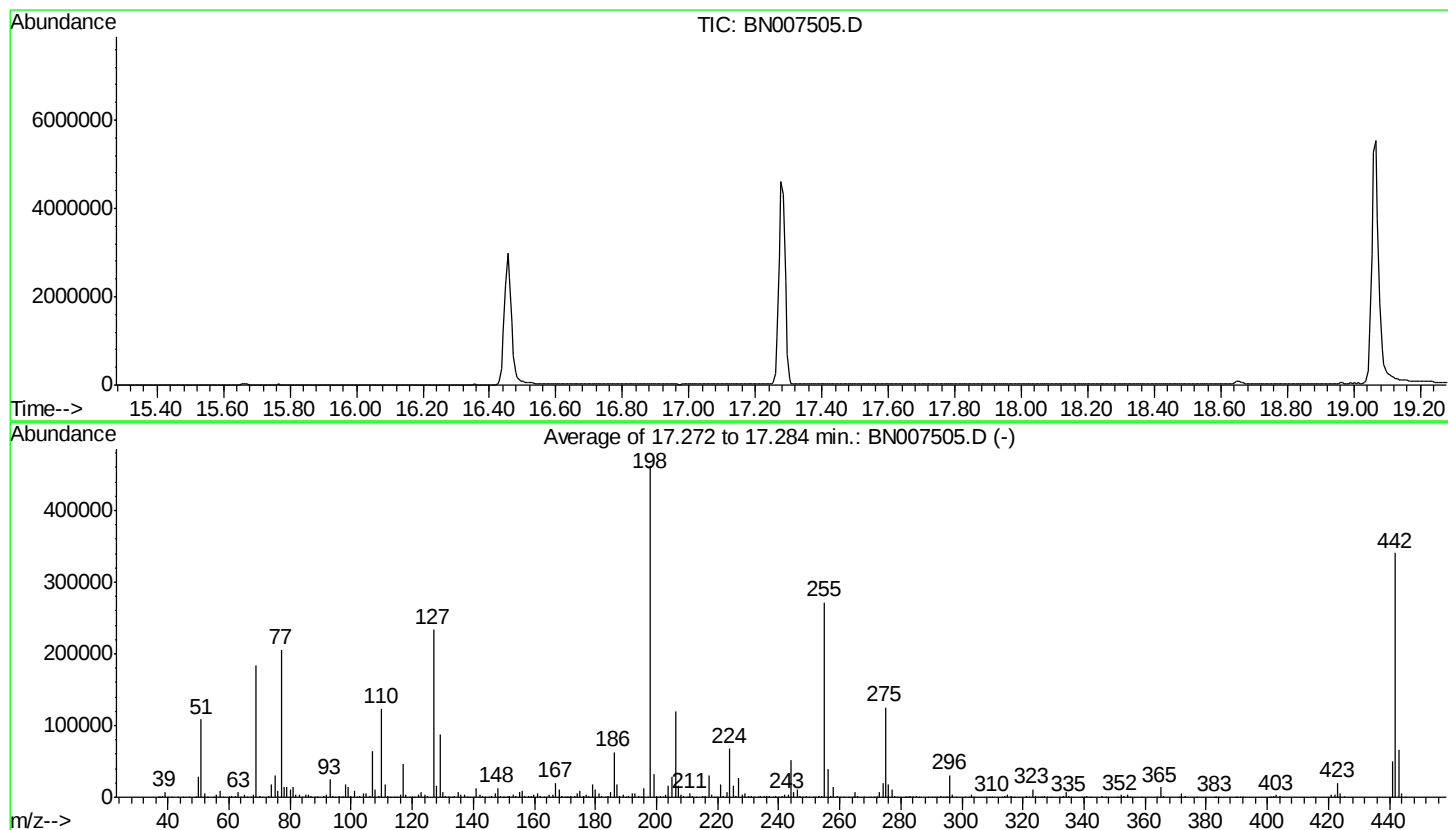

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2447

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 23.5      | 108528  | PASS             |
| 68          | 69           | 0.00         | 2            | 1.8       | 3378    | PASS             |
| 69          | 198          | 0.00         | 100          | 39.7      | 183732  | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 1027    | PASS             |
| 127         | 198          | 10           | 80           | 50.5      | 233365  | PASS             |
| 197         | 198          | 0.00         | 2            | 0.2       | 818     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 462442  | PASS             |
| 199         | 198          | 5            | 9            | 6.8       | 31410   | PASS             |
| 275         | 198          | 10           | 60           | 27.0      | 124978  | PASS             |
| 365         | 198          | 1            | 100          | 3.0       | 13692   | PASS             |
| 441         | 198          | 0.01         | 100          | 11.0      | 50936   | PASS             |
| 442         | 198          | 50           | 100          | 73.7      | 340885  | PASS             |
| 443         | 442          | 15           | 24           | 19.3      | 65949   | PASS             |