
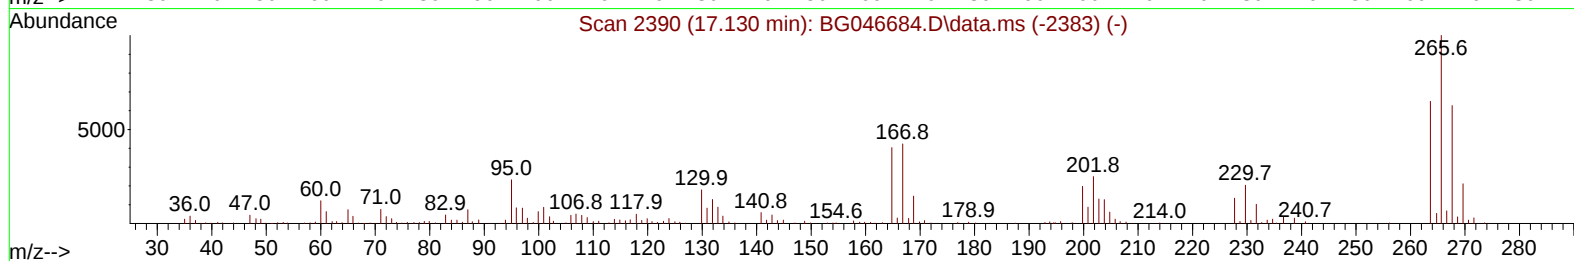
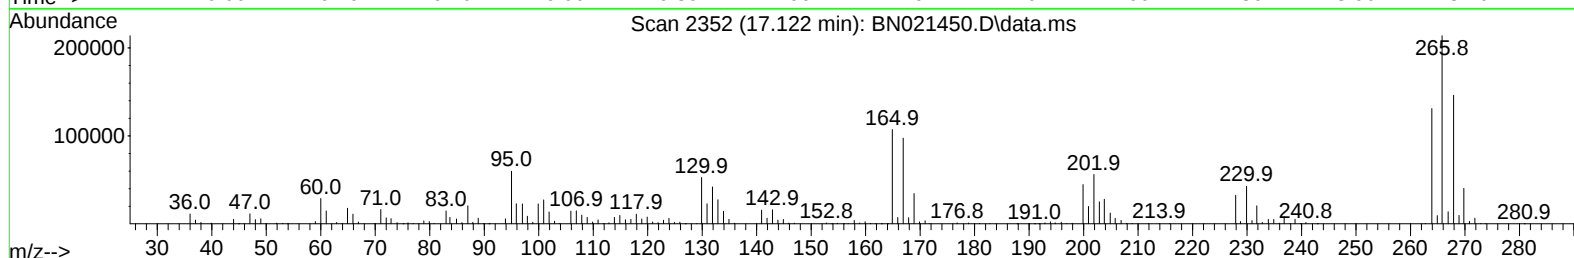


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083022\
 Data File : BN021450.D
 Acq On : 30 Aug 2022 09:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 02:53:58 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 31 02:53:53 2022
 Response via : Initial Calibration

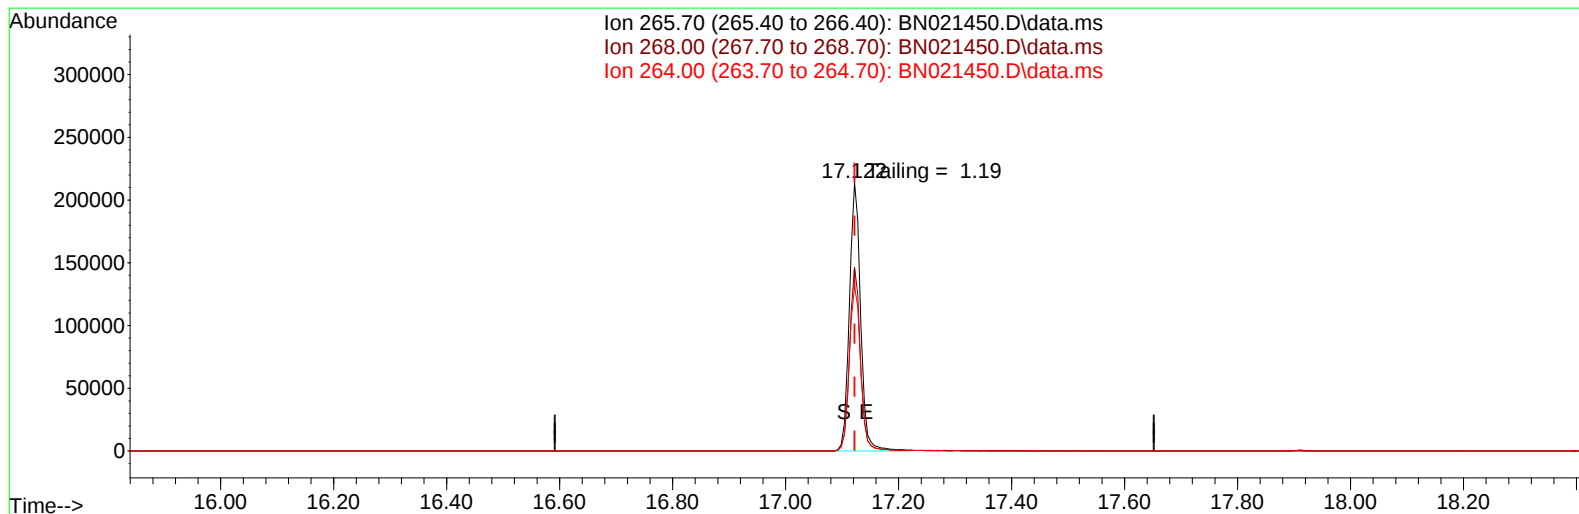

TIC: BN021450.D\data.ms

(70) Pentachlorophenol (C)




17.122min (0.000) 21868.80 ng

response 298277

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.40
264.00	61.60	61.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083022\
Data File : BN021450.D
Acq On : 30 Aug 2022 09:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 02:53:58 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 02:53:53 2022
Response via : Initial Calibration

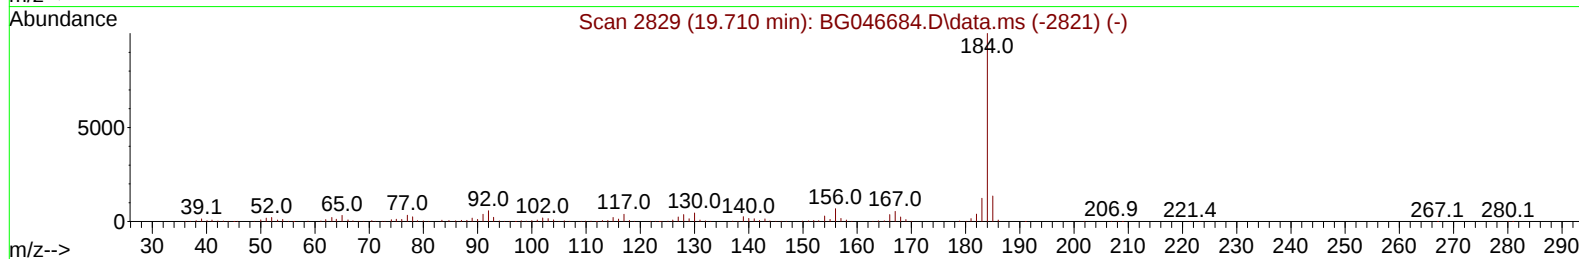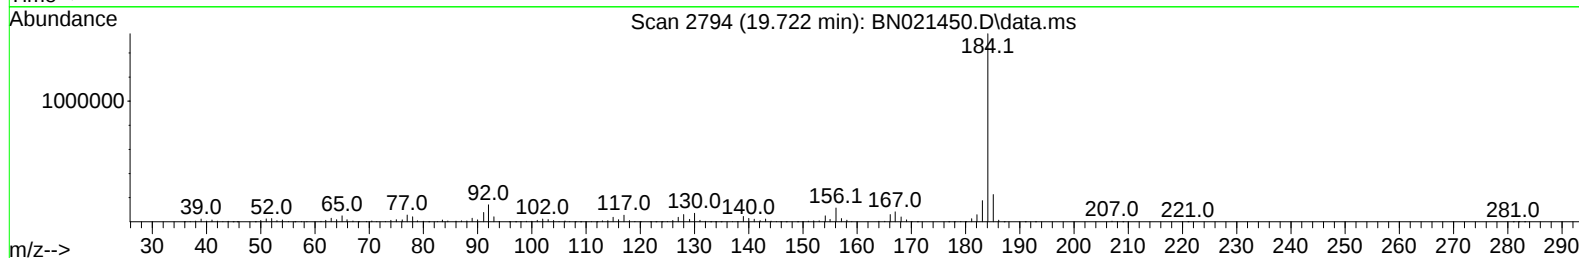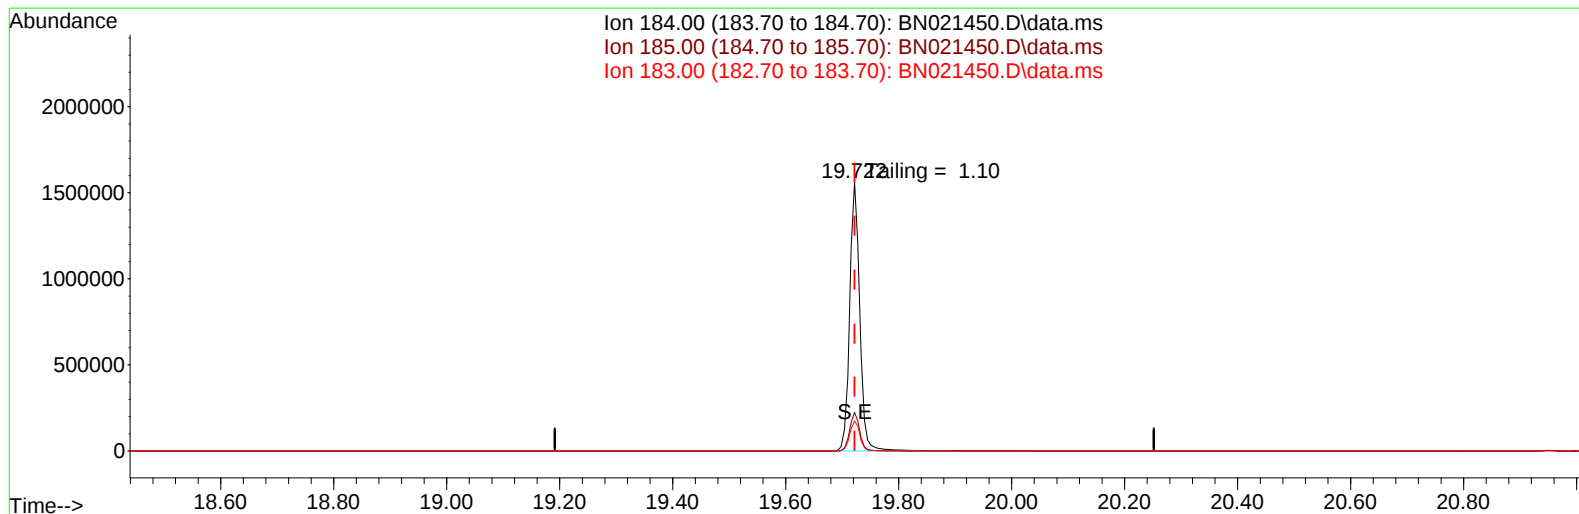

TIC: BN021450.D\data.ms

(77) Benzidine

19.722min (0.000) 0.00 ng

response 1949261

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.46
183.00	13.20	11.25
0.00	0.00	0.00