
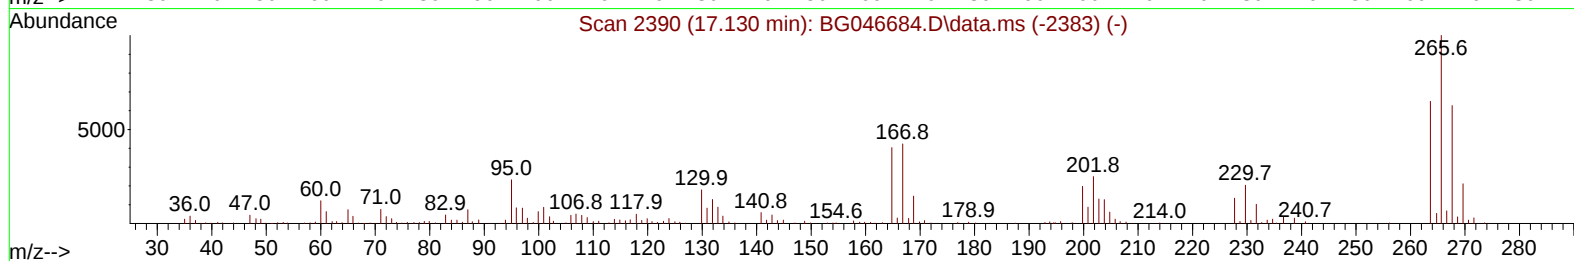
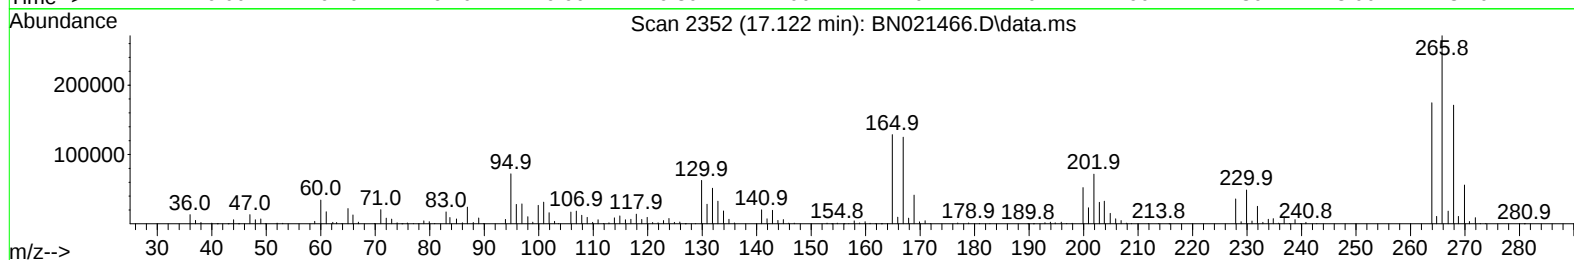


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083022\
Data File : BN021466.D
Acq On : 30 Aug 2022 22:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 02:55:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 02:53:53 2022
Response via : Initial Calibration

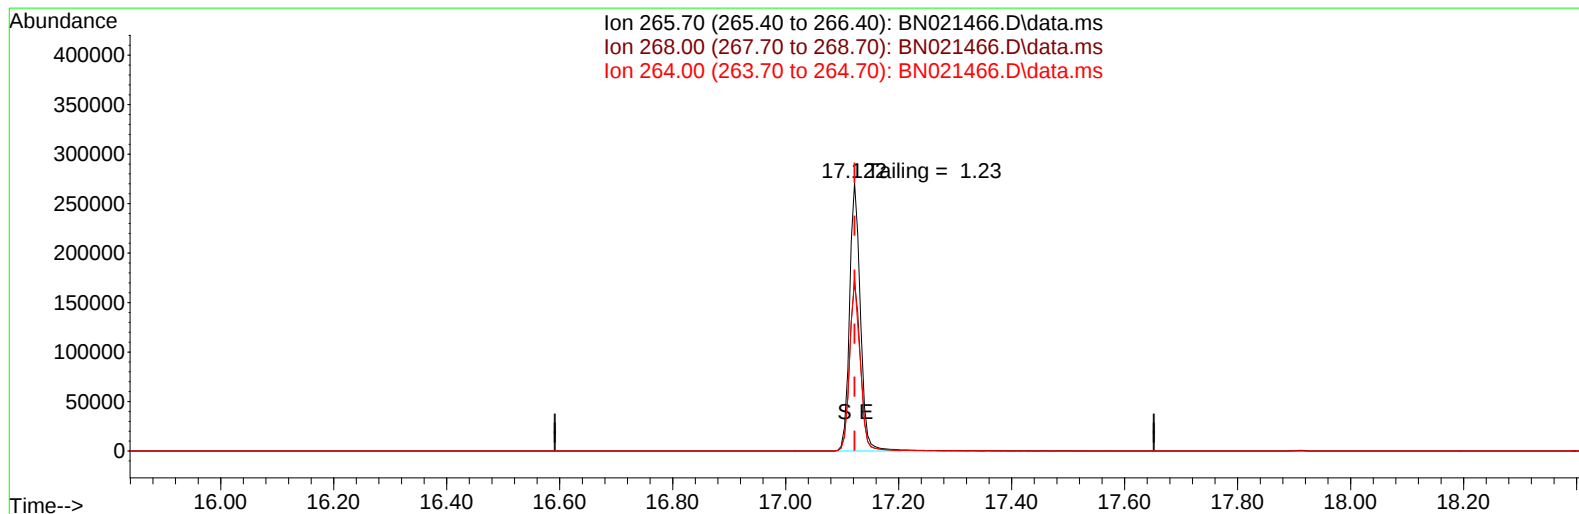

TIC: BN021466.D\data.ms

(70) Pentachlorophenol (C)




17.122min (-0.000) 22830.54 ng

response 362995

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.07
264.00	61.60	64.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083022\
 Data File : BN021466.D
 Acq On : 30 Aug 2022 22:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 02:55:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 31 02:53:53 2022
 Response via : Initial Calibration

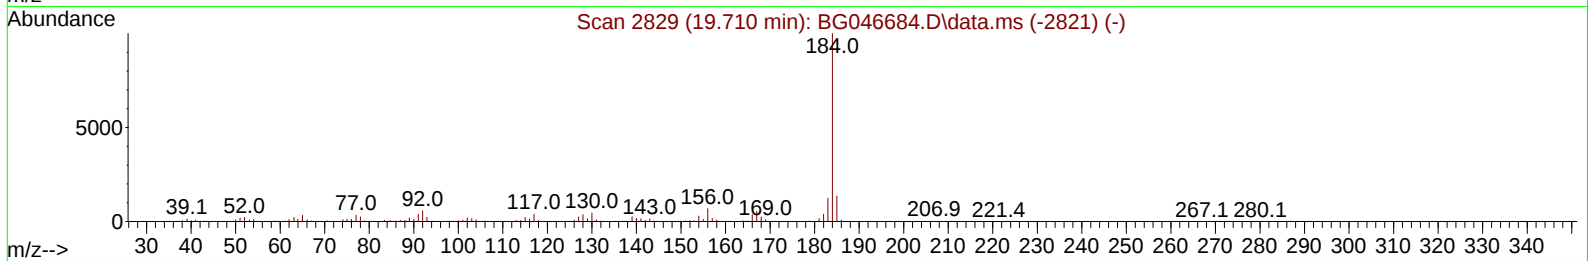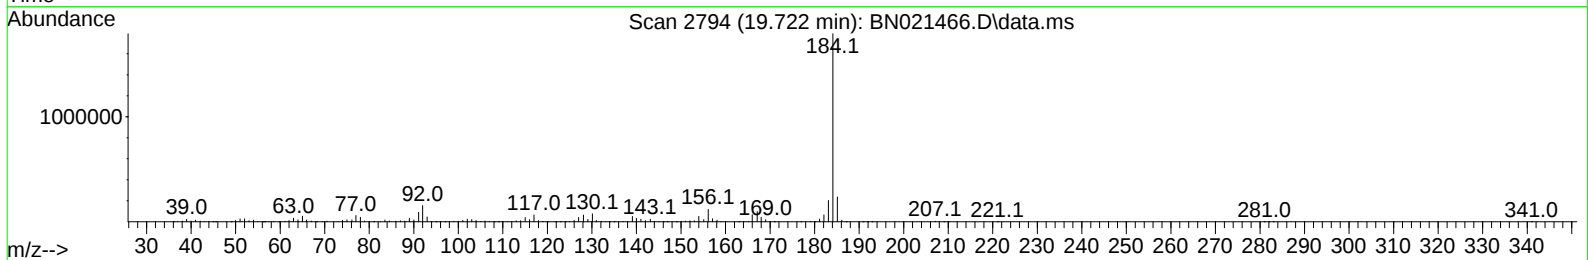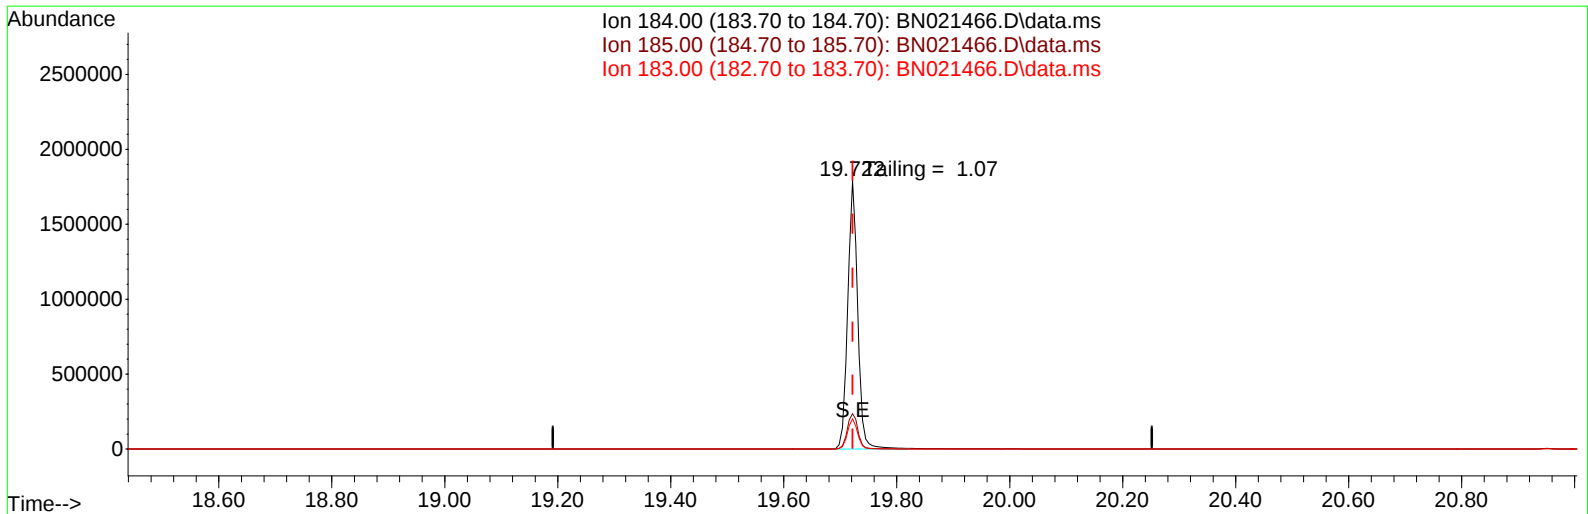

TIC: BN021466.D\data.ms

(77) Benzidine

19.722min (-0.000) 0.00 ng

response 2217341

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.17
183.00	13.20	11.29
0.00	0.00	0.00