

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083022\
 Data File : BN021467.D
 Acq On : 30 Aug 2022 23:10
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Aug 31 01:23:41 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 29 16:30:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.076	152	5141	0.400	ng	0.00
7) Naphthalene-d8	10.909	136	16322	0.400	ng	# 0.00
13) Acenaphthene-d10	14.729	164	9223	0.400	ng	0.00
19) Phenanthrene-d10	17.480	188	19396	0.400	ng	0.00
29) Chrysene-d12	21.664	240	14266	0.400	ng	0.00
35) Perylene-d12	24.185	264	10604	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.599	112	4236	0.421	ng	0.00
5) Phenol-d6	7.224	99	5255	0.410	ng	0.00
8) Nitrobenzene-d5	9.243	82	3945	0.358	ng	-0.01
11) 2-Methylnaphthalene-d10	12.490	152	14780	0.402	ng	0.00
14) 2,4,6-Tribromophenol	16.219	330	1045	0.345	ng	0.00
15) 2-Fluorobiphenyl	13.360	172	14851	0.368	ng	0.00
27) Fluoranthene-d10	19.506	212	17697	0.355	ng	0.00
31) Terphenyl-d14	20.097	244	12200	0.381	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.411	88	2497	0.388	ng	# 88
3) n-Nitrosodimethylamine	3.750	42	2139	0.369	ng	95
6) bis(2-Chloroethyl)ether	7.491	93	6100	0.378	ng	98
9) Naphthalene	10.952	128	17840	0.369	ng	99
10) Hexachlorobutadiene	11.240	225	3090	0.369	ng	# 100
12) 2-Methylnaphthalene	12.187	142	2503	0.438	ng	# 96
16) Acenaphthylene	14.451	152	14918	0.344	ng	100
17) Acenaphthene	14.793	154	11009	0.361	ng	99
18) Fluorene	15.776	166	13762	0.366	ng	99
21) 4-Bromophenyl-phenylether	16.660	248	4271	0.352	ng	# 79
22) Hexachlorobenzene	16.772	284	5180	0.349	ng	99
23) Atrazine	16.926	200	2393	0.338	ng	98
24) Pentachlorophenol	17.121	266	1022	0.432	ng	99
25) Phenanthrene	17.521	178	23785	0.355	ng	100
26) Anthracene	17.613	178	18414	0.346	ng	99
28) Fluoranthene	19.535	202	24419	0.351	ng	100
30) Pyrene	19.898	202	28397	0.373	ng	97
32) Benzo(a)anthracene	21.646	228	17932	0.361	ng	100
33) Chrysene	21.700	228	21487	0.363	ng	99
34) Bis(2-ethylhexyl)phtha...	21.557	149	7306	0.365	ng	99
36) Indeno(1,2,3-cd)pyrene	26.843	276	17184	0.359	ng	100
37) Benzo(b)fluoranthene	23.407	252	18333	0.351	ng	99
38) Benzo(k)fluoranthene	23.457	252	17808	0.338	ng	99
39) Benzo(a)pyrene	24.071	252	13664	0.375	ng	97
40) Dibenzo(a,h)anthracene	26.866	278	13756	0.357	ng	97
41) Benzo(g,h,i)perylene	27.658	276	14046	0.332	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083022\
Data File : BN021467.D
Acq On : 30 Aug 2022 23:10
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Aug 31 01:23:41 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 29 16:30:43 2022
Response via : Initial Calibration



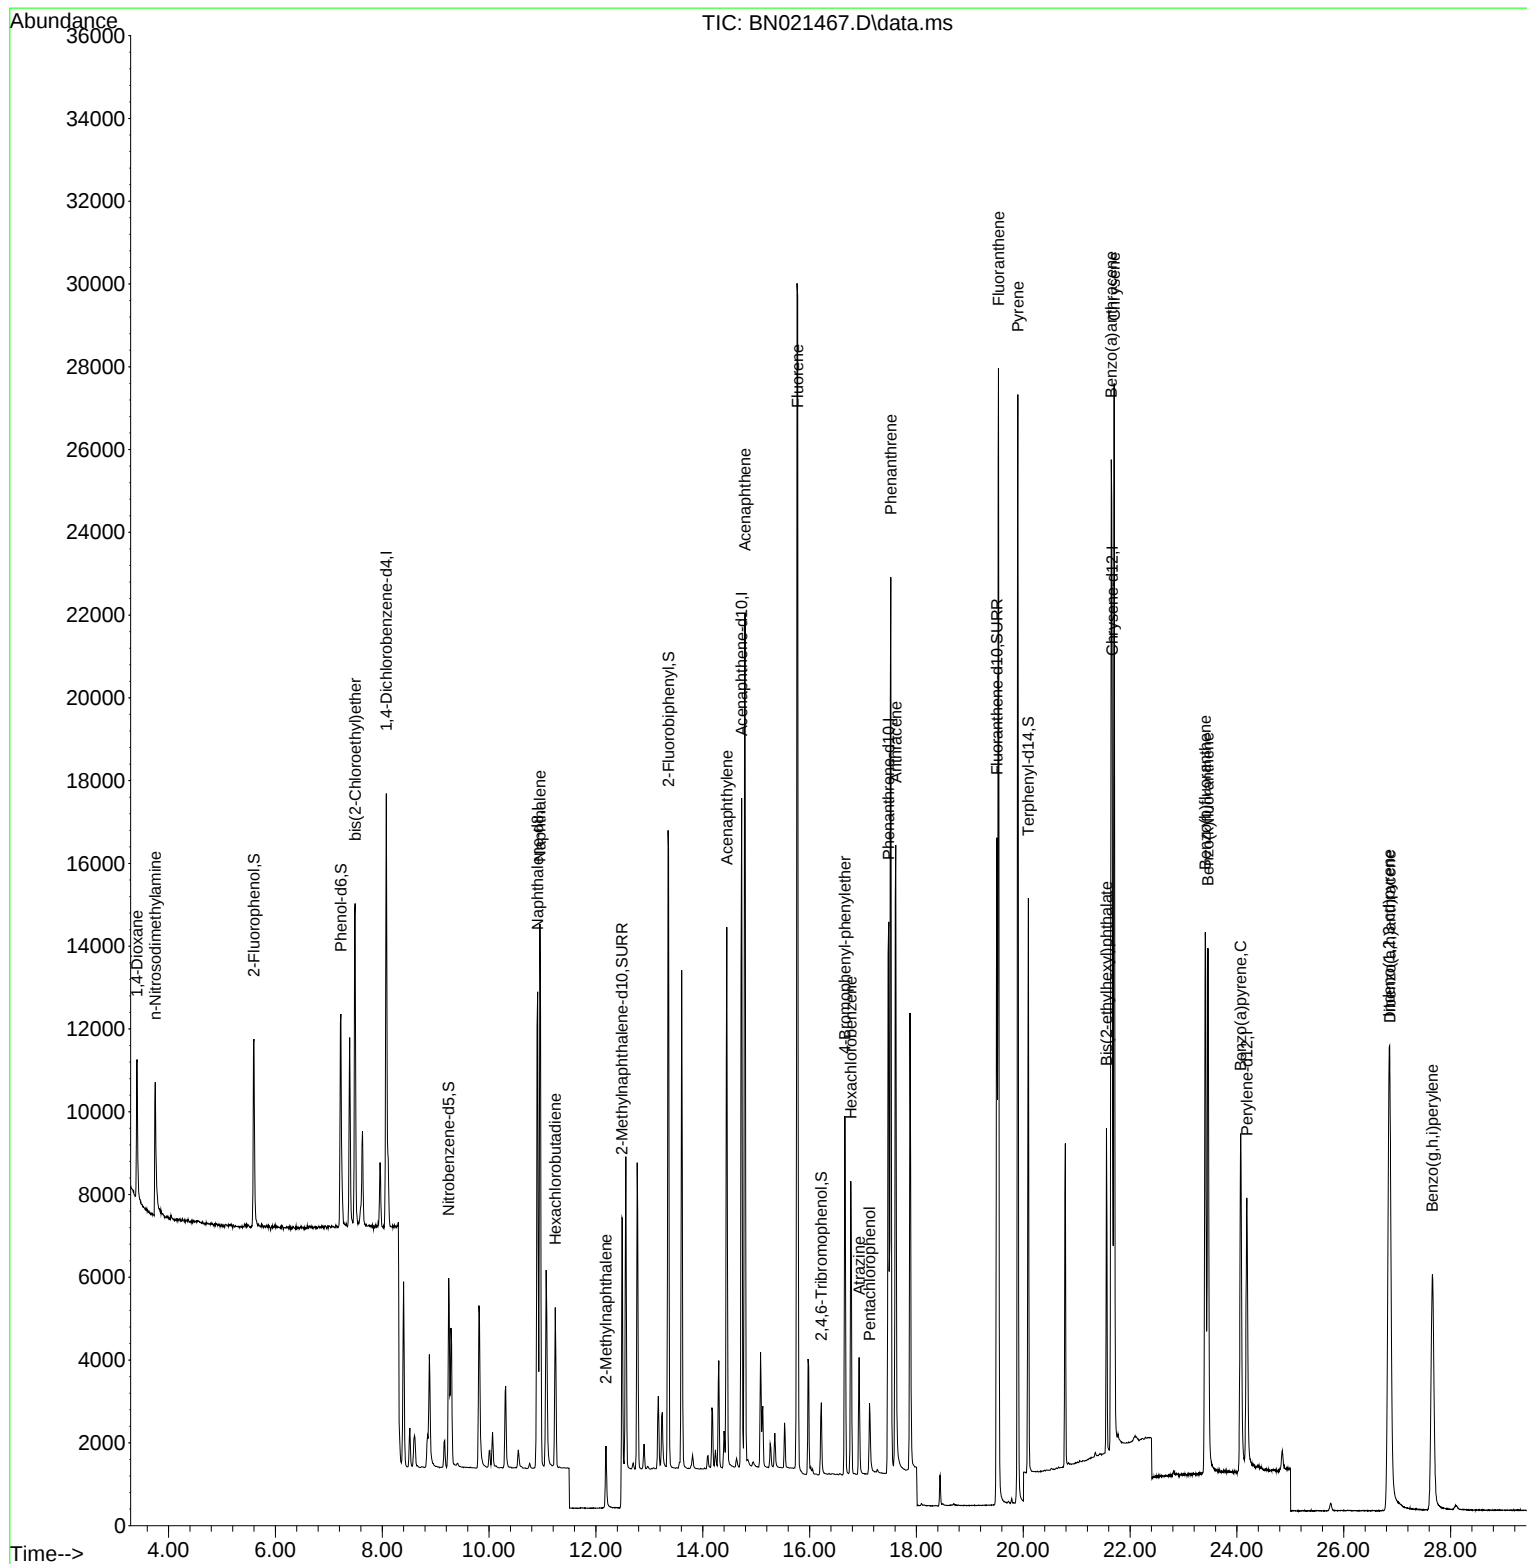




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 8.076 min Scan# 60
 Delta R.T. -0.007 min
 Lab File: BN021467.D
 Acq: 30 Aug 2022 23:10




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion:152 Resp: 5141
 Ion Ratio Lower Upper
 152 100
 150 154.4 121.4 182.0
 115 60.0 48.6 72.8

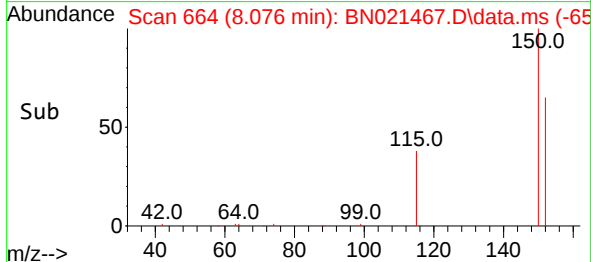

#2
 1,4-Dioxane
 Concen: 0.388 ng
 RT: 3.411 min Scan# 18
 Delta R.T. 0.000 min
 Lab File: BN021467.D
 Acq: 30 Aug 2022 23:10

Tgt Ion: 88 Resp: 2497
 Ion Ratio Lower Upper
 88 100
 43 26.0 35.8 53.8#
 58 72.8 57.1 85.7


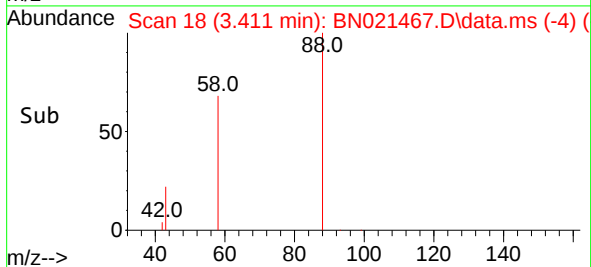

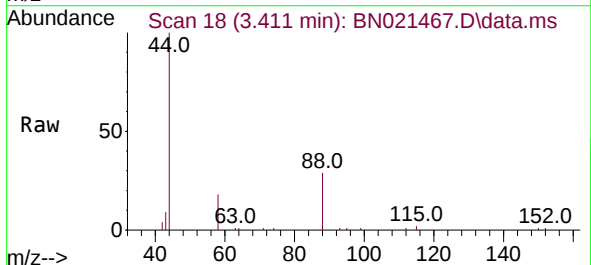




#3
 n-Nitrosodimethylamine
 Concen: 0.369 ng
 RT: 3.750 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN021467.D
 Acq: 30 Aug 2022 23:10




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion: 42 Resp: 2139
 Ion Ratio Lower Upper
 42 100
 74 135.5 113.0 169.6
 44 10.8 10.5 15.7

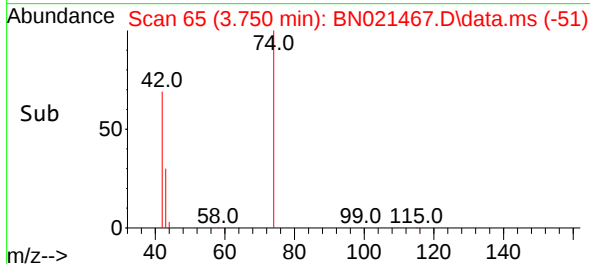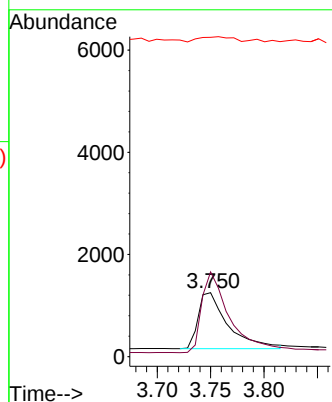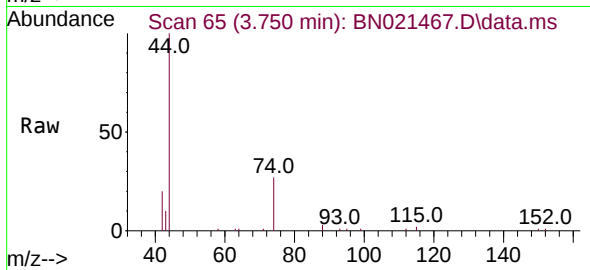

#4
 2-Fluorophenol
 Concen: 0.421 ng
 RT: 5.599 min Scan# 321
 Delta R.T. 0.000 min
 Lab File: BN021467.D
 Acq: 30 Aug 2022 23:10

Tgt Ion: 112 Resp: 4236
 Ion Ratio Lower Upper
 112 100
 64 55.4 43.5 65.3
 63 29.0 22.6 34.0


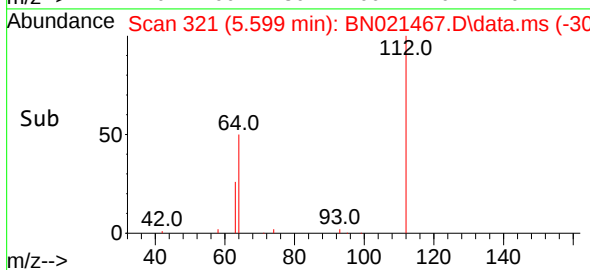
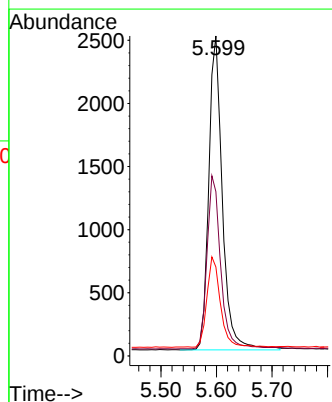
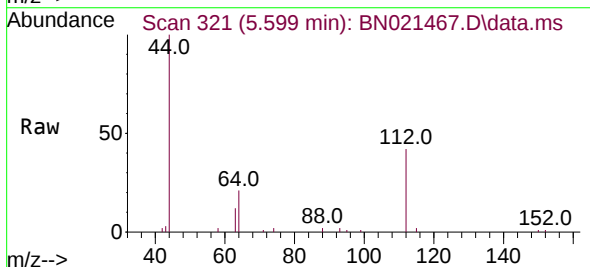




#5
Phenol-d6
Concen: 0.410 ng
RT: 7.224 min Scan# 54
Delta R.T. 0.000 min
Lab File: BN021467.D
Acq: 30 Aug 2022 23:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	99	Resp:	5255
Ion	Ratio	Lower	Upper
99	100		
42	18.2	15.5	23.3
71	31.4	24.2	36.2

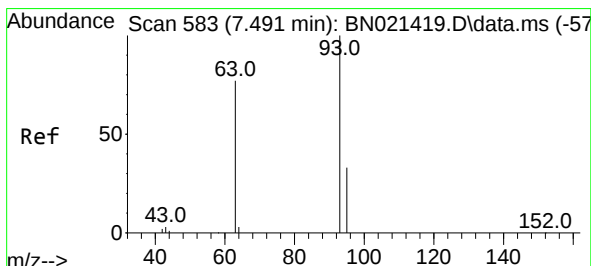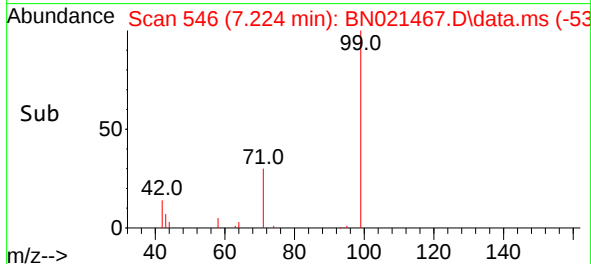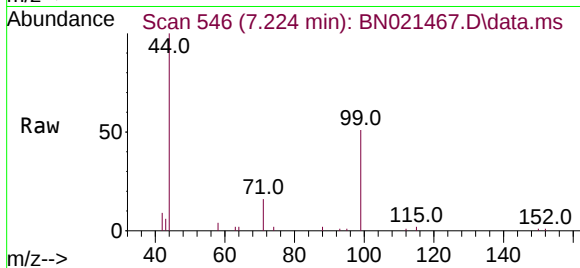

#6
bis(2-Chloroethyl)ether
Concen: 0.378 ng
RT: 7.491 min Scan# 583
Delta R.T. 0.000 min
Lab File: BN021467.D
Acq: 30 Aug 2022 23:10

Tgt Ion:	93	Resp:	6100
Ion	Ratio	Lower	Upper
93	100		
63	74.8	57.8	86.8
95	32.3	25.9	38.9


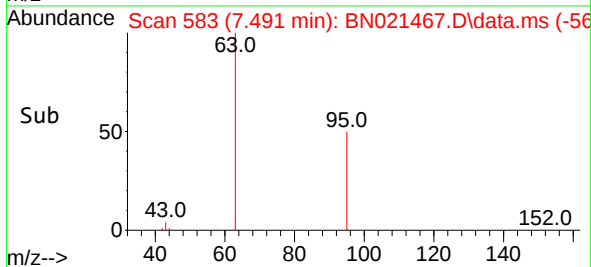

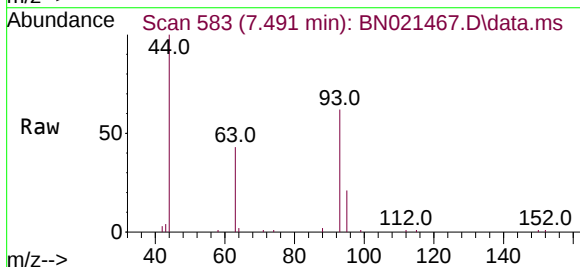


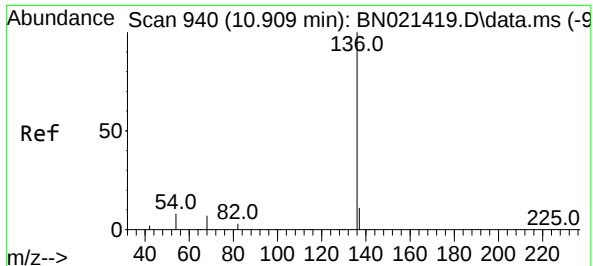

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.909 min Scan# 94
Delta R.T. -0.000 min
Lab File: BN021467.D
Acq: 30 Aug 2022 23:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	136	Resp:	16322
Ion Ratio	Lower	Upper	
136	100		
137	11.4	9.3	13.9
54	6.4	6.9	10.3#
68	5.7	6.1	9.1#

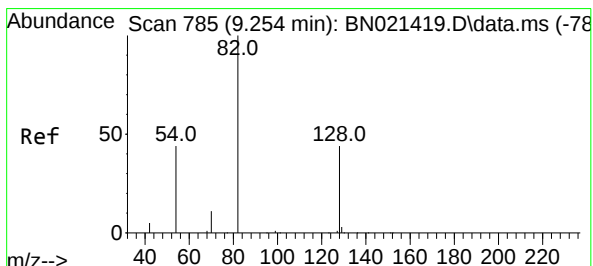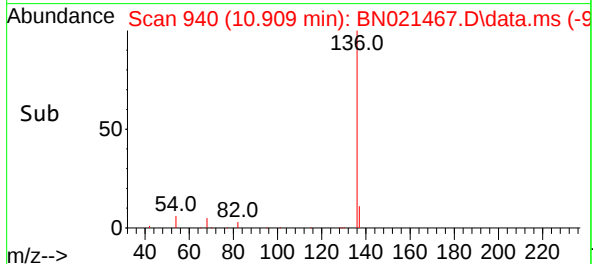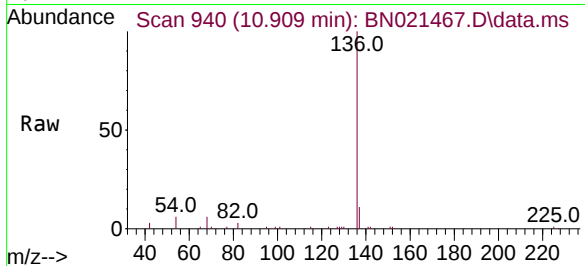

#8
Nitrobenzene-d5
Concen: 0.358 ng
RT: 9.243 min Scan# 784
Delta R.T. -0.011 min
Lab File: BN021467.D
Acq: 30 Aug 2022 23:10

Tgt Ion:	82	Resp:	3945
Ion Ratio	Lower	Upper	
82	100		
128	37.9	30.9	46.3
54	51.6	42.7	64.1


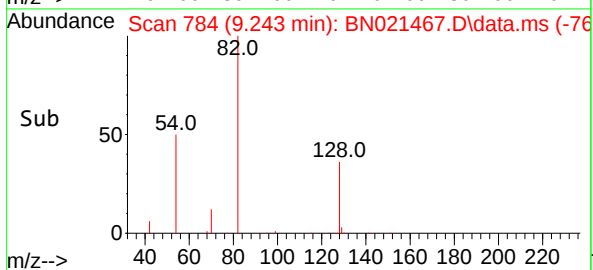

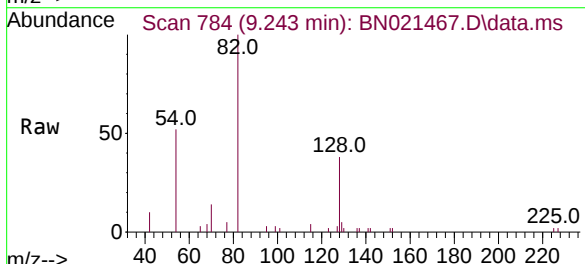


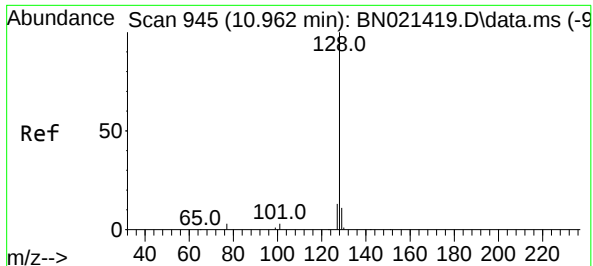

#9
Naphthalene
Concen: 0.369 ng
RT: 10.952 min Scan# 944
Delta R.T. -0.011 min
Lab File: BN021467.D
Acq: 30 Aug 2022 23:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:128 Resp: 17840
Ion Ratio Lower Upper
128 100
129 11.4 9.3 13.9
127 13.2 11.0 16.4

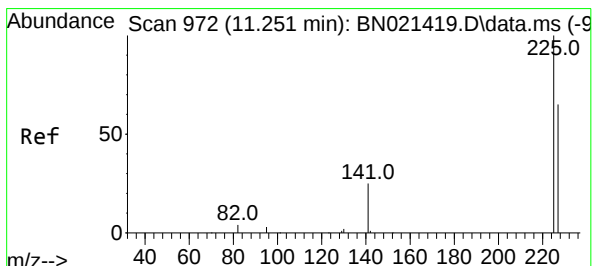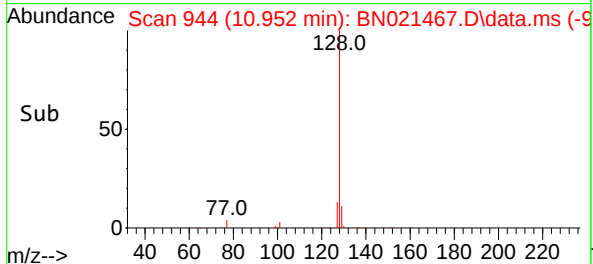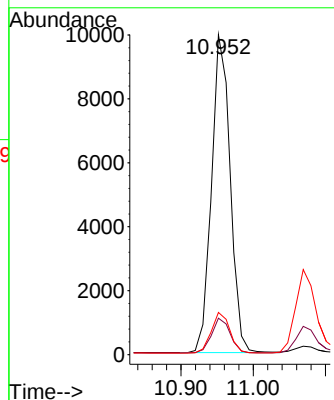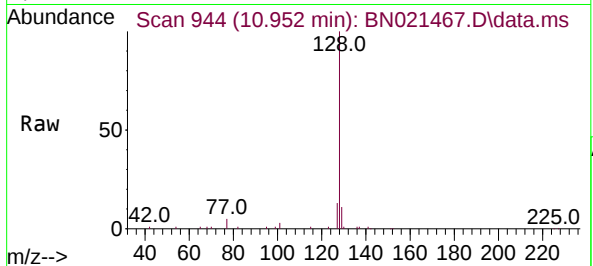

#10
Hexachlorobutadiene
Concen: 0.369 ng
RT: 11.240 min Scan# 971
Delta R.T. -0.011 min
Lab File: BN021467.D
Acq: 30 Aug 2022 23:10

Tgt Ion:225 Resp: 3090
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.0 51.2 76.8


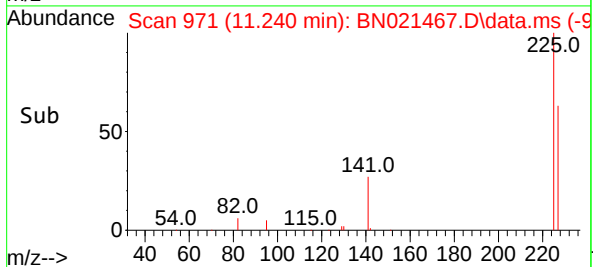
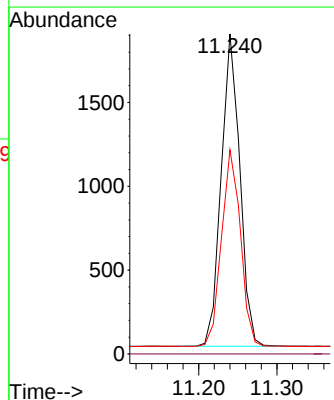
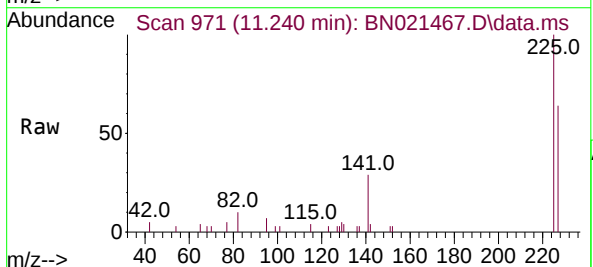




#11
2-Methylnaphthalene-d10
Concen: 0.402 ng
RT: 12.490 min Scan# 1176
Delta R.T. -0.007 min
Lab File: BN021467.D
Acq: 30 Aug 2022 23:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:152 Resp: 14780
Ion Ratio Lower Upper
152 100
151 18.4 14.5 21.7

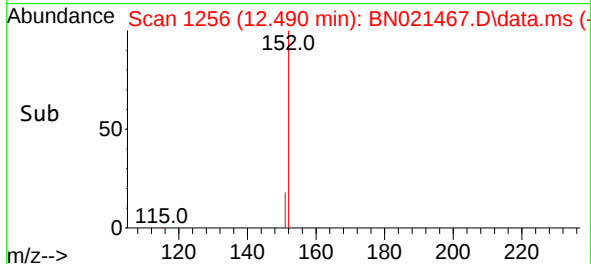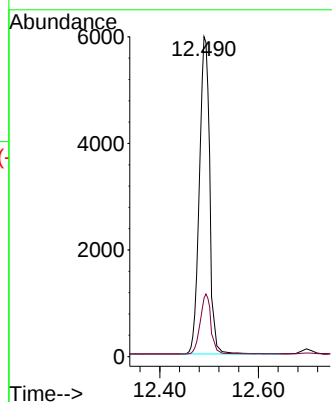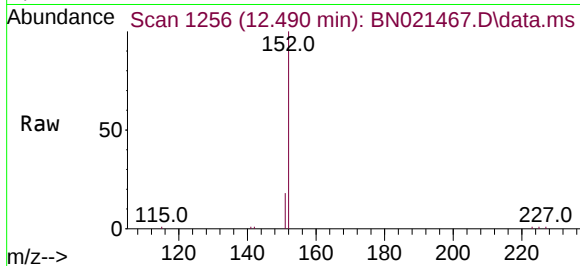

#12
2-Methylnaphthalene
Concen: 0.438 ng
RT: 12.187 min Scan# 1176
Delta R.T. -0.004 min
Lab File: BN021467.D
Acq: 30 Aug 2022 23:10

Tgt Ion:142 Resp: 2503
Ion Ratio Lower Upper
142 100
141 14.0 12.2 18.2
115 7.7 7.9 11.9#


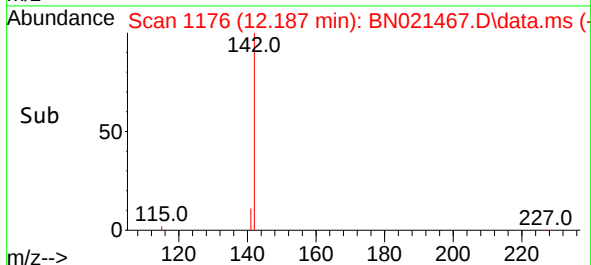

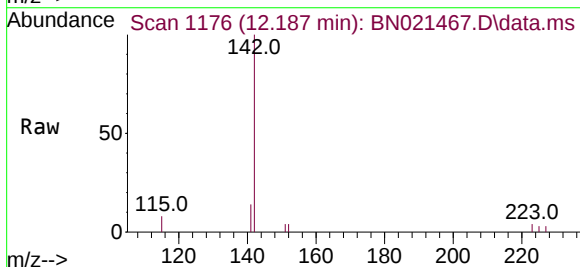




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.729 min Scan# 1468
Delta R.T. 0.001 min
Lab File: BN021467.D
Acq: 30 Aug 2022 23:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:164 Resp: 9223
Ion Ratio Lower Upper
164 100
162 103.0 82.2 123.4
160 49.2 39.5 59.3

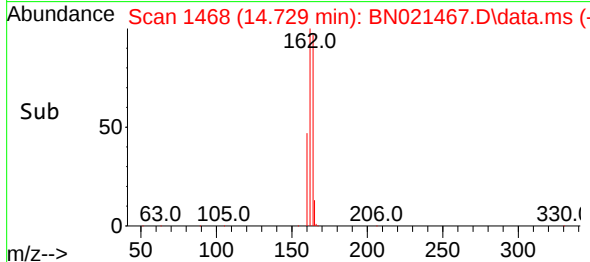

#14
2,4,6-Tribromophenol
Concen: 0.345 ng
RT: 16.219 min Scan# 1609
Delta R.T. 0.001 min
Lab File: BN021467.D
Acq: 30 Aug 2022 23:10

Tgt Ion:330 Resp: 1045
Ion Ratio Lower Upper
330 100
332 96.1 79.3 118.9
141 42.8 37.1 55.7


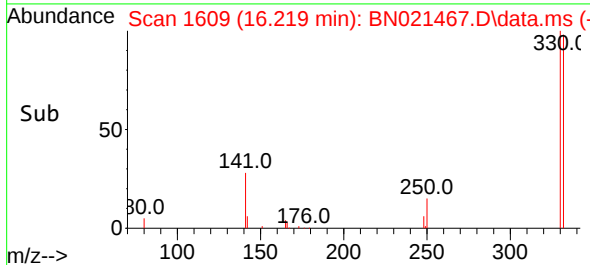

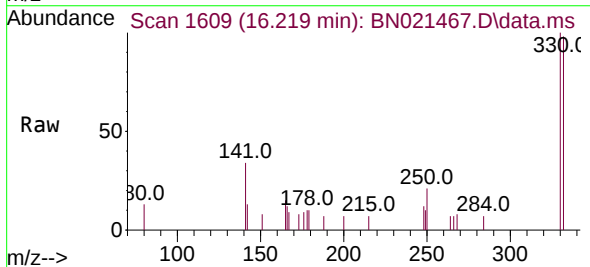


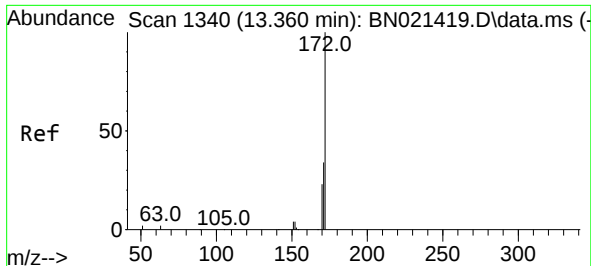

#15
2-Fluorobiphenyl
Concen: 0.368 ng
RT: 13.360 min Scan# 1340
Delta R.T. 0.000 min
Lab File: BN021467.D
Acq: 30 Aug 2022 23:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:172 Resp: 14851
Ion Ratio Lower Upper
172 100
171 33.6 27.8 41.6
170 22.3 18.6 28.0

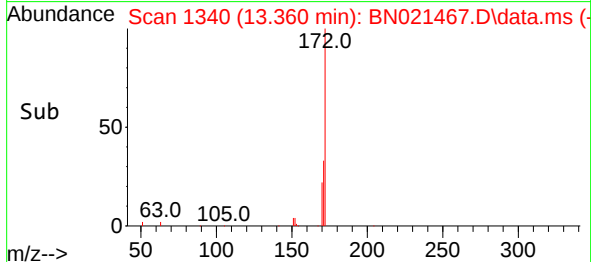

#16
Acenaphthylene
Concen: 0.344 ng
RT: 14.451 min Scan# 1442
Delta R.T. 0.000 min
Lab File: BN021467.D
Acq: 30 Aug 2022 23:10

Tgt Ion:152 Resp: 14918
Ion Ratio Lower Upper
152 100
151 19.3 15.4 23.2
153 13.0 10.3 15.5


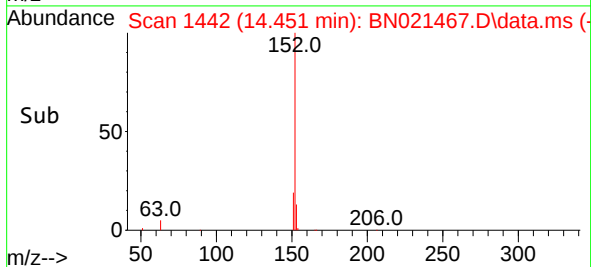

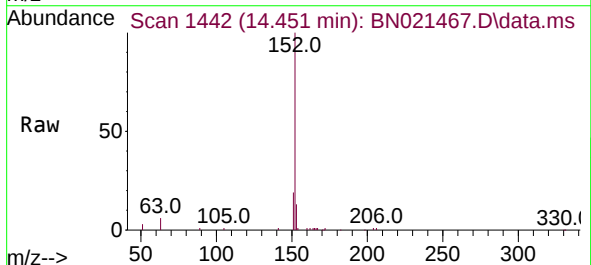




#17
Acenaphthene
Concen: 0.361 ng
RT: 14.793 min Scan# 1474
Delta R.T. 0.000 min
Lab File: BN021467.D
Acq: 30 Aug 2022 23:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:154 Resp: 11009
Ion Ratio Lower Upper
154 100
153 113.2 89.5 134.3
152 57.6 45.5 68.3

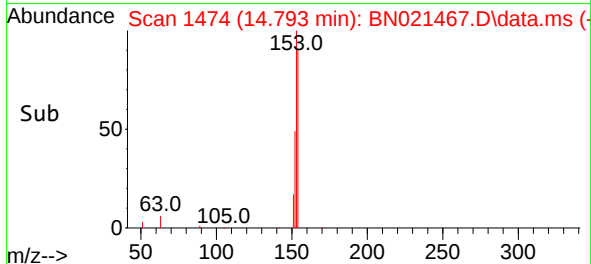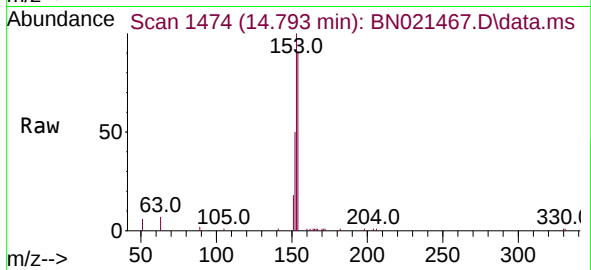

#18
Fluorene
Concen: 0.366 ng
RT: 15.776 min Scan# 1566
Delta R.T. 0.000 min
Lab File: BN021467.D
Acq: 30 Aug 2022 23:10

Tgt Ion:166 Resp: 13762
Ion Ratio Lower Upper
166 100
165 97.8 78.7 118.1
167 13.5 10.6 16.0

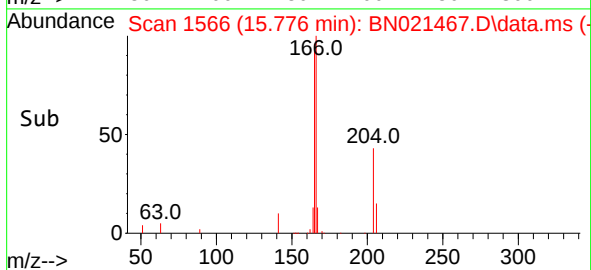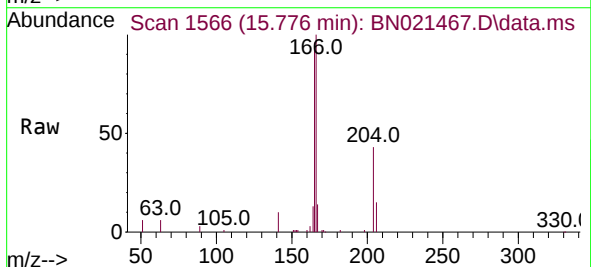



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.480 min Scan# 1732

Delta R.T. 0.000 min

Lab File: BN021467.D

Acq: 30 Aug 2022 23:10

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:188 Resp: 19396

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 9.9 9.5 14.3

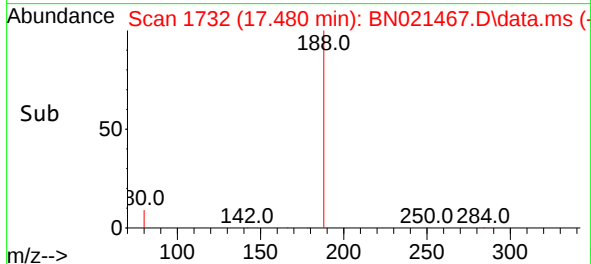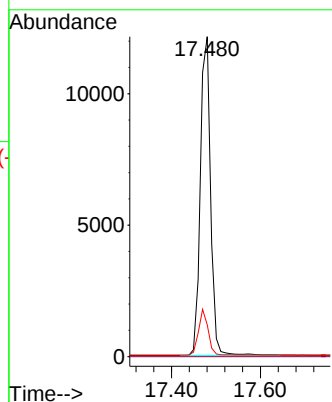

#21

4-Bromophenyl-phenylether

Concen: 0.352 ng

RT: 16.660 min Scan# 1652

Delta R.T. -0.010 min

Lab File: BN021467.D

Acq: 30 Aug 2022 23:10




Tgt Ion:248 Resp: 4271


Ion Ratio Lower Upper

248 100

250 95.1 81.8 122.6

141 81.4 38.5 57.7#


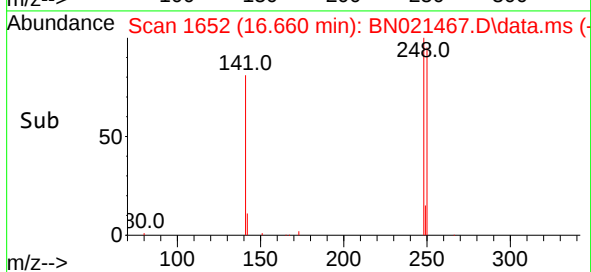
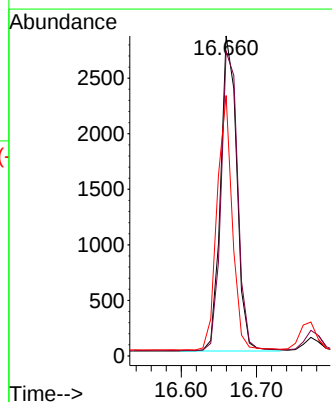
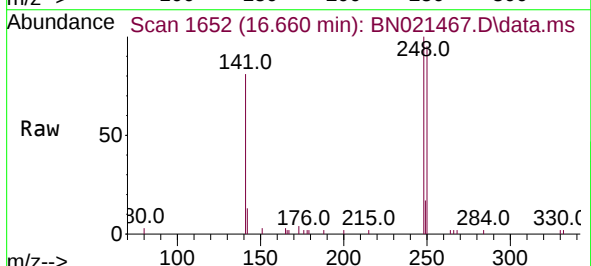


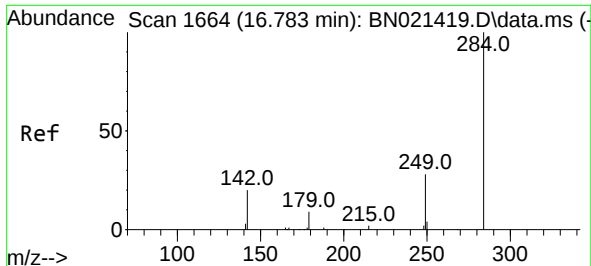

#22
Hexachlorobenzene
Concen: 0.349 ng
RT: 16.772 min Scan# 1663
Delta R.T. -0.010 min
Lab File: BN021467.D
Acq: 30 Aug 2022 23:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:284 Resp: 5180
Ion Ratio Lower Upper
284 100
142 40.9 32.3 48.5
249 31.6 25.4 38.2

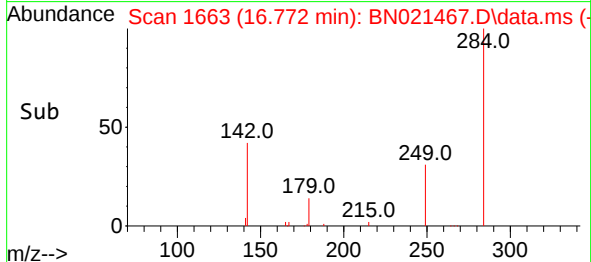

#23
Atrazine
Concen: 0.338 ng
RT: 16.926 min Scan# 1678
Delta R.T. 0.000 min
Lab File: BN021467.D
Acq: 30 Aug 2022 23:10

Tgt Ion:200 Resp: 2393
Ion Ratio Lower Upper
200 100
173 30.0 24.3 36.5
215 45.6 38.4 57.6

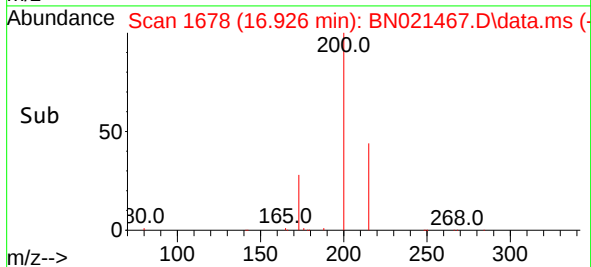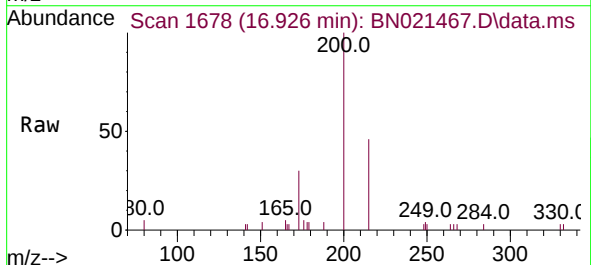



#24

Pentachlorophenol

Concen: 0.432 ng

RT: 17.121 min Scan# 1697

Delta R.T. -0.010 min

Lab File: BN021467.D

Acq: 30 Aug 2022 23:10

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:266 Resp: 1022

Ion Ratio Lower Upper

266 100

264 60.9 49.0 73.6

268 64.7 50.9 76.3

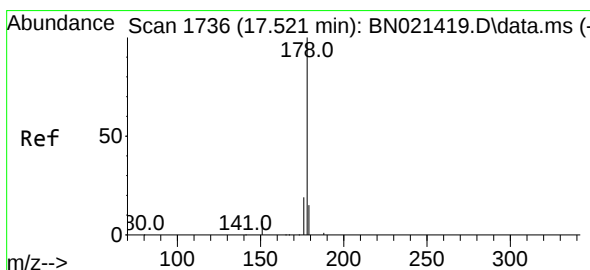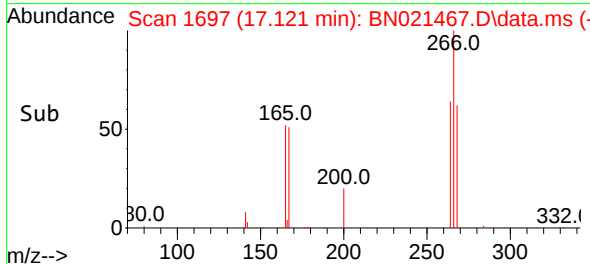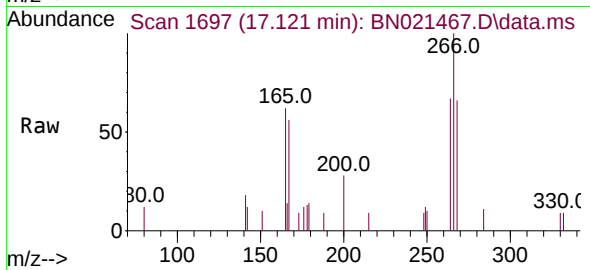

#25

Phenanthrene

Concen: 0.355 ng

RT: 17.521 min Scan# 1736

Delta R.T. 0.000 min

Lab File: BN021467.D

Acq: 30 Aug 2022 23:10




Tgt Ion:178 Resp: 23785


Ion Ratio Lower Upper

178 100

176 19.2 15.4 23.2

179 15.4 12.2 18.4


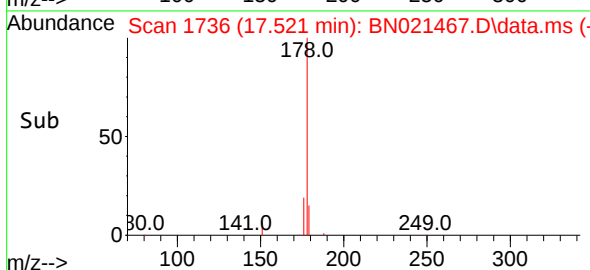

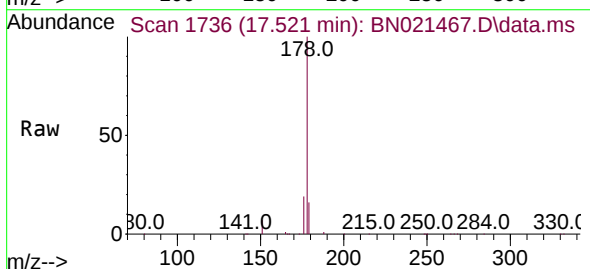


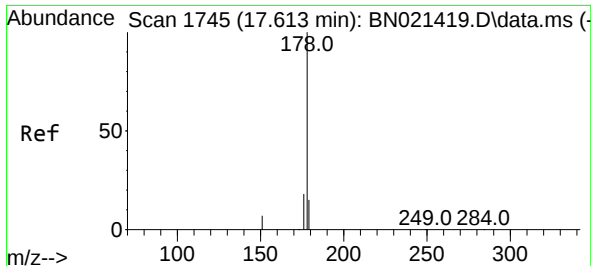

#26
 Anthracene
 Concen: 0.346 ng
 RT: 17.613 min Scan# 1745
 Delta R.T. 0.000 min
 Lab File: BN021467.D
 Acq: 30 Aug 2022 23:10




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion:	178	Resp:	18414
Ion Ratio	Lower	Upper	
178	100		
176	18.8	14.6	22.0
179	15.1	12.2	18.2

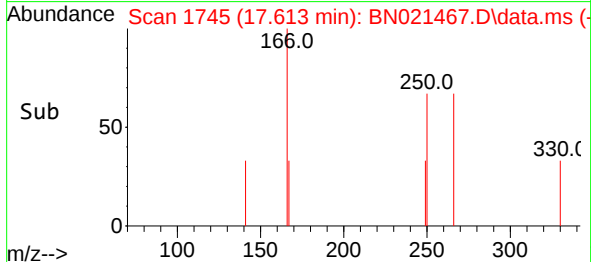

#27
 Fluoranthene-d10
 Concen: 0.355 ng
 RT: 19.506 min Scan# 2138
 Delta R.T. -0.004 min
 Lab File: BN021467.D
 Acq: 30 Aug 2022 23:10

Tgt Ion:	212	Resp:	17697
Ion Ratio	Lower	Upper	
212	100		
106	17.9	14.2	21.2
104	9.9	7.8	11.6


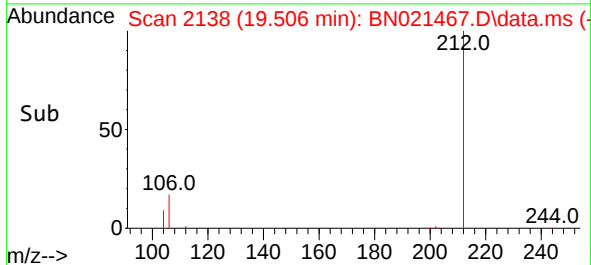

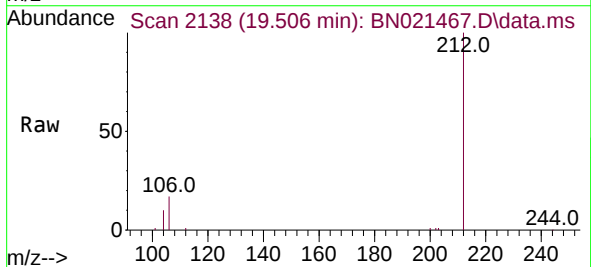




#28
Fluoranthene
Concen: 0.351 ng
RT: 19.535 min Scan# 2146
Delta R.T. -0.004 min
Lab File: BN021467.D
Acq: 30 Aug 2022 23:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:202 Resp: 24419
Ion Ratio Lower Upper
202 100
101 13.7 10.9 16.3
203 17.1 13.8 20.6

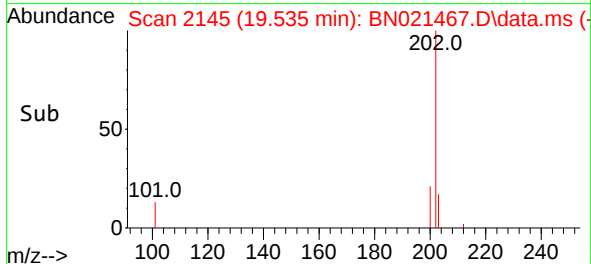

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.664 min Scan# 2442
Delta R.T. 0.000 min
Lab File: BN021467.D
Acq: 30 Aug 2022 23:10

Tgt Ion:240 Resp: 14266
Ion Ratio Lower Upper
240 100
120 13.3 10.2 15.4
236 27.2 22.1 33.1

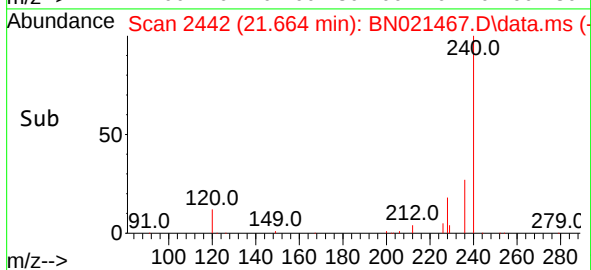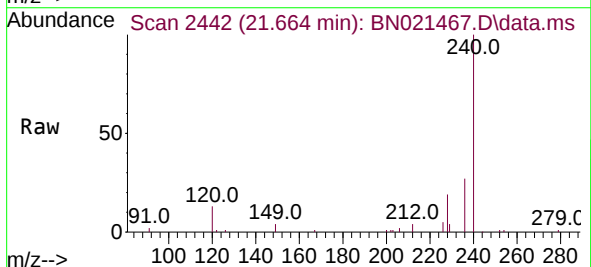



#30

Pyrene

Concen: 0.373 ng

RT: 19.898 min Scan# 2231

Delta R.T. -0.004 min

Lab File: BN021467.D

Acq: 30 Aug 2022 23:10

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:202 Resp: 28397

Ion Ratio Lower Upper

202 100

200 17.9 13.9 20.9

203 17.1 11.9 17.9

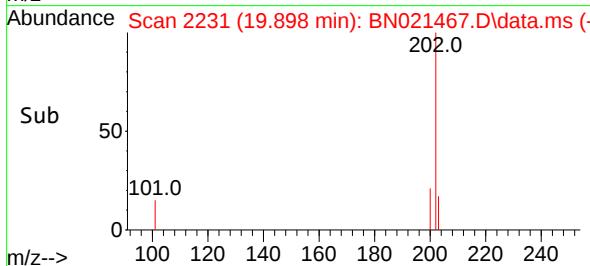

#31

Terphenyl-d14

Concen: 0.381 ng

RT: 20.097 min Scan# 2267

Delta R.T. 0.000 min

Lab File: BN021467.D

Acq: 30 Aug 2022 23:10




Tgt Ion:244 Resp: 12200


Ion Ratio Lower Upper

244 100

212 8.2 6.5 9.7

122 11.9 9.1 13.7


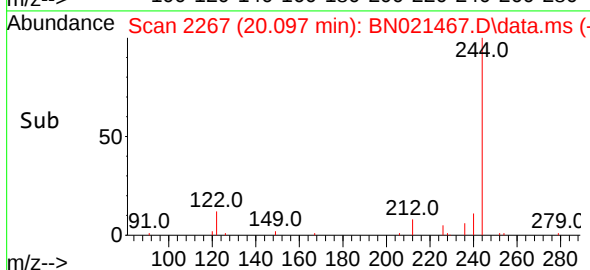

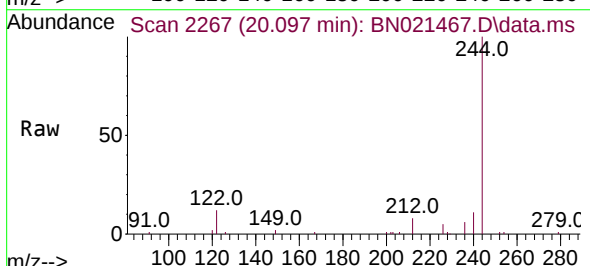




#32
Benzo(a)anthracene
Concen: 0.361 ng
RT: 21.646 min Scan# 2441
Delta R.T. -0.009 min
Lab File: BN021467.D
Acq: 30 Aug 2022 23:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:228 Resp: 17932
Ion Ratio Lower Upper
228 100
226 27.7 22.0 33.0
229 19.9 15.9 23.9

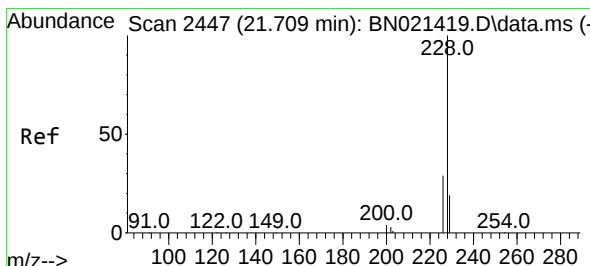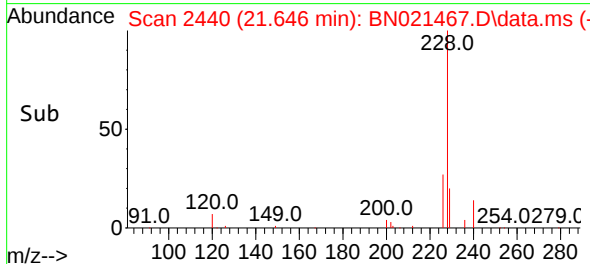

#33
Chrysene
Concen: 0.363 ng
RT: 21.700 min Scan# 2446
Delta R.T. -0.009 min
Lab File: BN021467.D
Acq: 30 Aug 2022 23:10

Tgt Ion:228 Resp: 21487
Ion Ratio Lower Upper
228 100
226 31.1 24.2 36.2
229 20.0 15.9 23.9


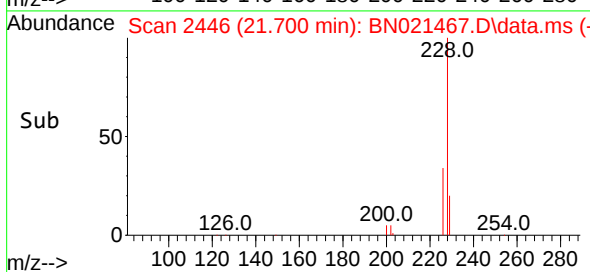

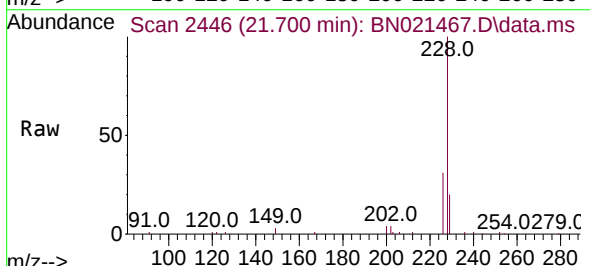


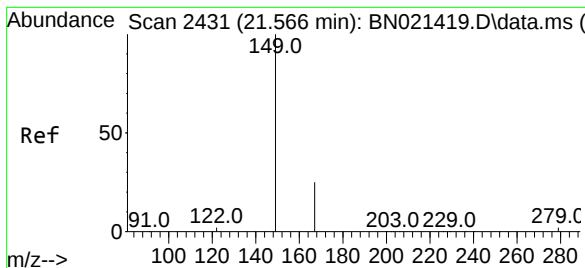

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.365 ng
 RT: 21.557 min Scan# 2431
 Delta R.T. -0.009 min
 Lab File: BN021467.D
 Acq: 30 Aug 2022 23:10




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Tgt Ion:149 Resp: 7306
 Ion Ratio Lower Upper
 149 100
 167 26.0 21.4 32.0
 279 2.5 2.2 3.2

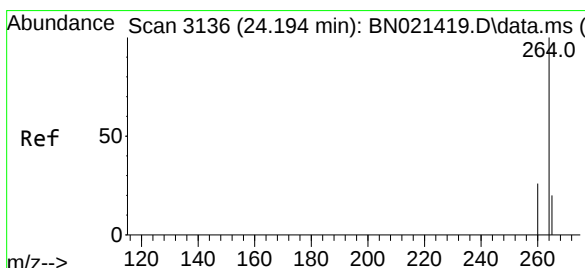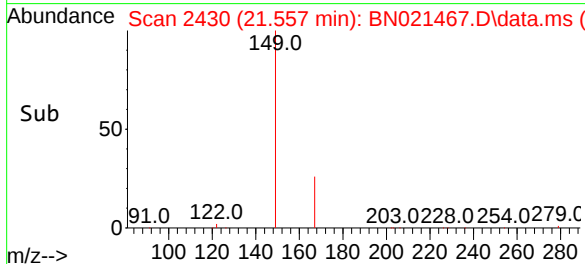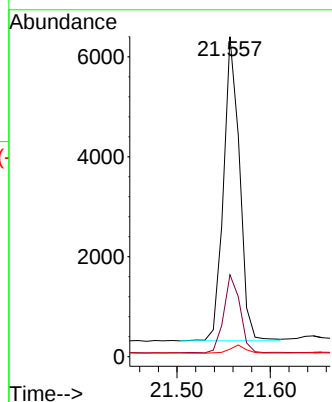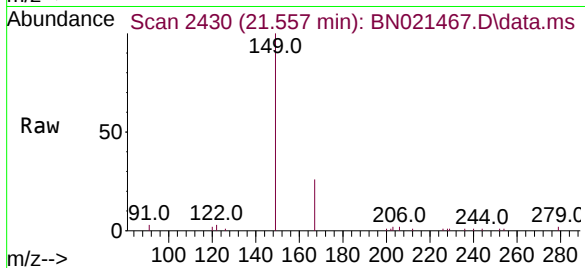

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 24.185 min Scan# 3133
 Delta R.T. -0.009 min
 Lab File: BN021467.D
 Acq: 30 Aug 2022 23:10

Tgt Ion:264 Resp: 10604
 Ion Ratio Lower Upper
 264 100
 260 26.5 21.0 31.6
 265 34.7 32.2 48.2


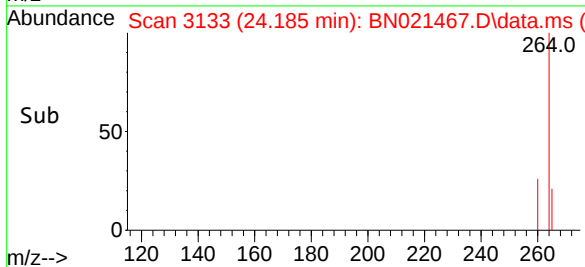
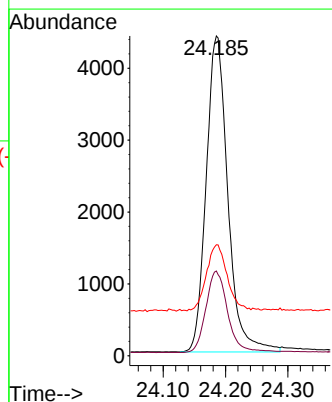
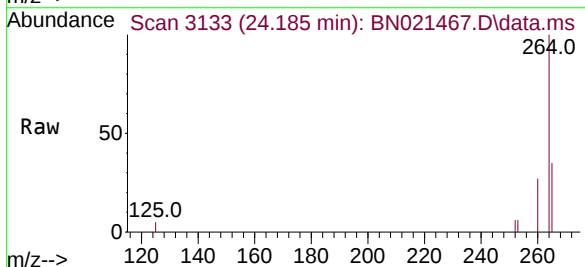




#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.359 ng
 RT: 26.843 min Scan# 4044
 Delta R.T. -0.006 min
 Lab File: BN021467.D
 Acq: 30 Aug 2022 23:10




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion:276 Resp: 17184
 Ion Ratio Lower Upper
 276 100
 138 34.0 27.4 41.2
 277 24.9 19.9 29.9

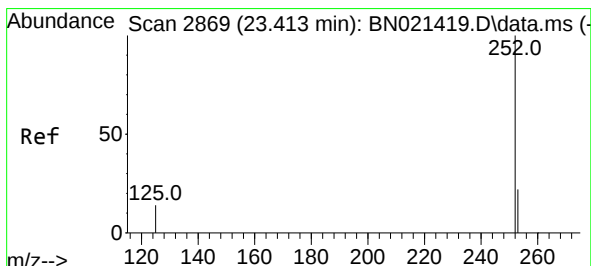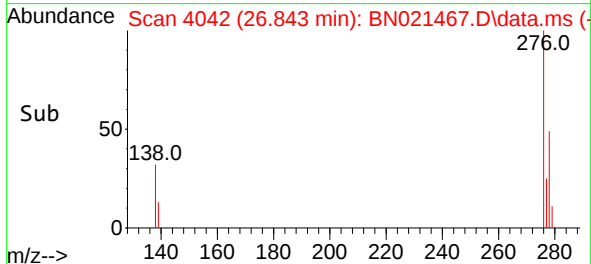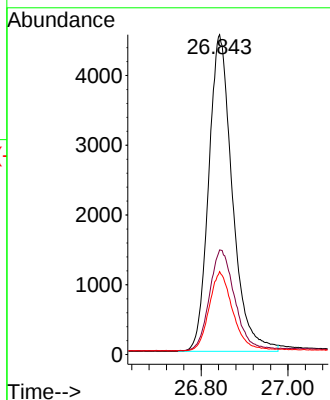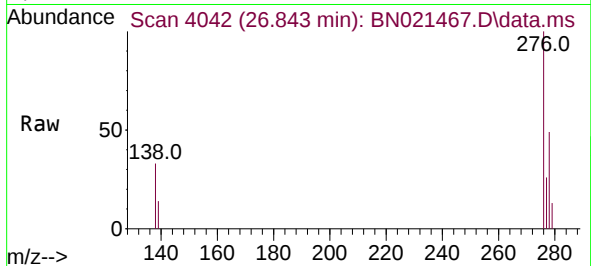

#37
 Benzo(b)fluoranthene
 Concen: 0.351 ng
 RT: 23.407 min Scan# 2867
 Delta R.T. -0.006 min
 Lab File: BN021467.D
 Acq: 30 Aug 2022 23:10

Tgt Ion:252 Resp: 18333
 Ion Ratio Lower Upper
 252 100
 253 24.1 19.8 29.6
 125 16.3 13.7 20.5


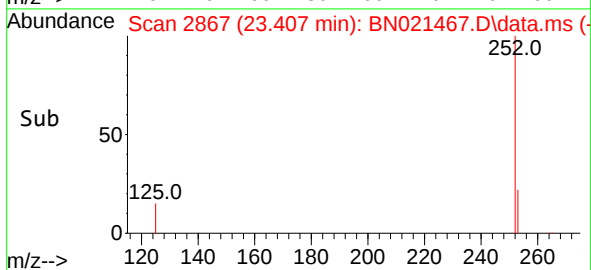
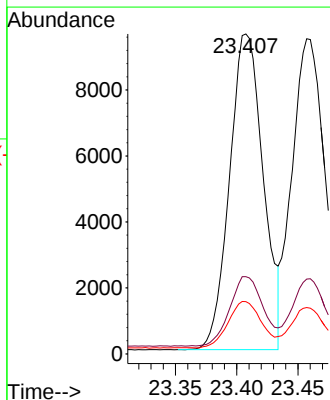
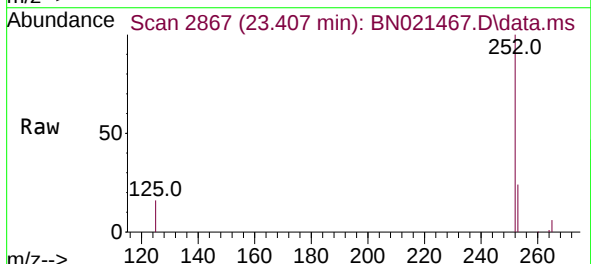




#38
Benzo(k)fluoranthene
Concen: 0.338 ng
RT: 23.457 min Scan# 2884
Delta R.T. -0.009 min
Lab File: BN021467.D
Acq: 30 Aug 2022 23:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:252 Resp: 17808
Ion Ratio Lower Upper
252 100
253 23.7 19.5 29.3
125 14.7 12.3 18.5

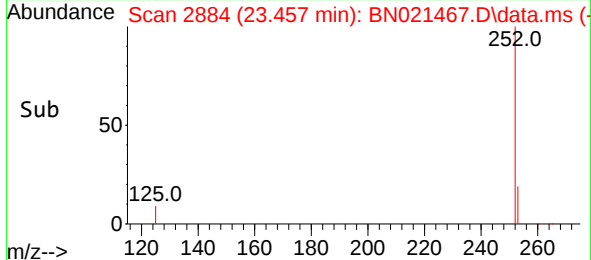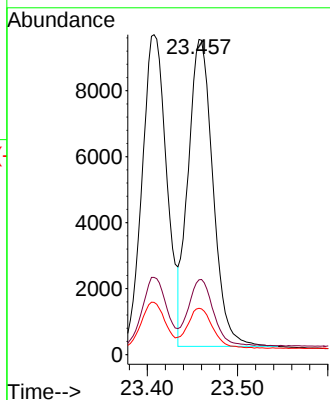

#39
Benzo(a)pyrene
Concen: 0.375 ng
RT: 24.071 min Scan# 3094
Delta R.T. -0.006 min
Lab File: BN021467.D
Acq: 30 Aug 2022 23:10

Tgt Ion:252 Resp: 13664
Ion Ratio Lower Upper
252 100
253 25.5 21.1 31.7
125 22.8 16.6 25.0


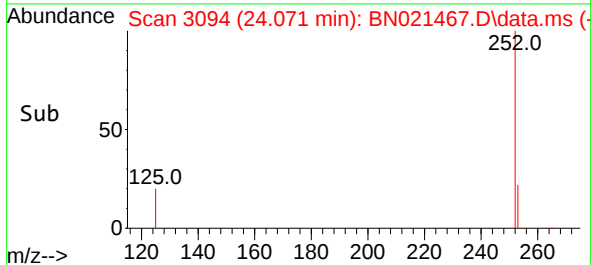
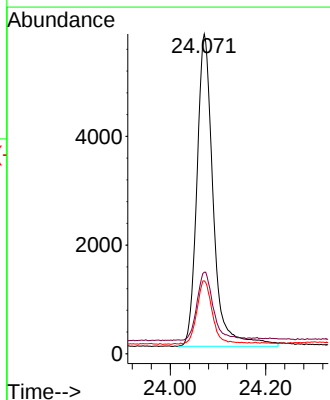
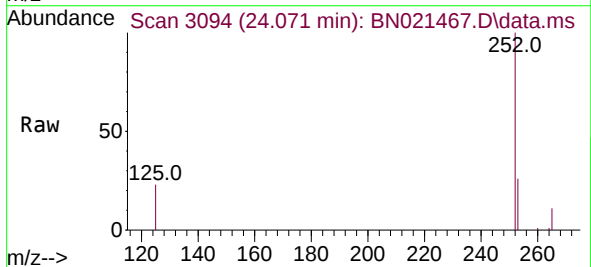




#40
Dibenzo(a,h)anthracene
Concen: 0.357 ng
RT: 26.866 min Scan# 4053
Delta R.T. -0.009 min
Lab File: BN021467.D
Acq: 30 Aug 2022 23:10

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:278 Resp: 13756
Ion Ratio Lower Upper
278 100
139 24.4 21.8 32.6
279 25.9 20.4 30.6

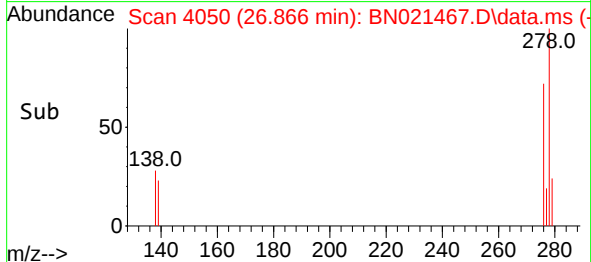

#41
Benzo(g,h,i)perylene
Concen: 0.332 ng
RT: 27.658 min Scan# 4321
Delta R.T. -0.012 min
Lab File: BN021467.D
Acq: 30 Aug 2022 23:10

Tgt Ion:276 Resp: 14046
Ion Ratio Lower Upper
276 100
277 24.5 19.7 29.5
138 29.6 23.7 35.5

