


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083022\
 Data File : BN021466.D
 Acq On : 30 Aug 2022 22:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 29 16:30:43 2022

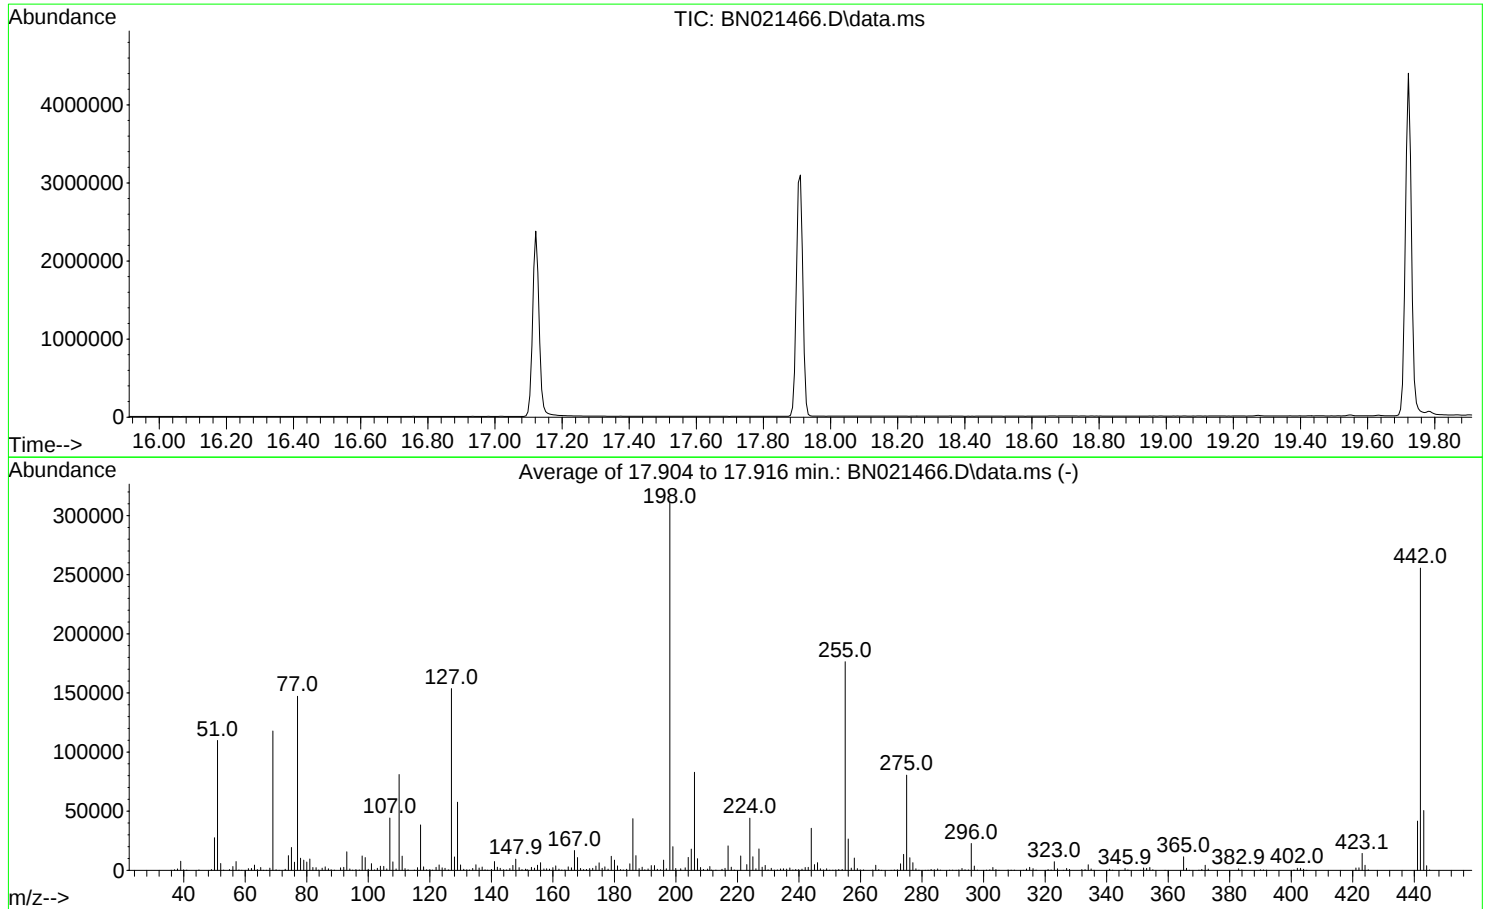




AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	109813	PASS
68	69	0.00	2	1.6	1875	PASS
69	198	0.00	100	37.9	117840	PASS
70	69	0.00	2	0.4	522	PASS
127	198	10	80	49.4	153659	PASS
197	198	0.00	2	0.4	1302	PASS
198	198	100	100	100.0	311125	PASS
199	198	5	9	6.4	19915	PASS
275	198	10	60	25.9	80440	PASS
365	198	1	100	3.7	11403	PASS
441	198	0.01	100	13.4	41621	PASS
442	442	50	100	100.0	255595	PASS
443	442	15	24	19.8	50581	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083022\
Data File : BN021466.D
Acq On : 30 Aug 2022 22:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 31 02:55:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 02:53:53 2022
Response via : Initial Calibration

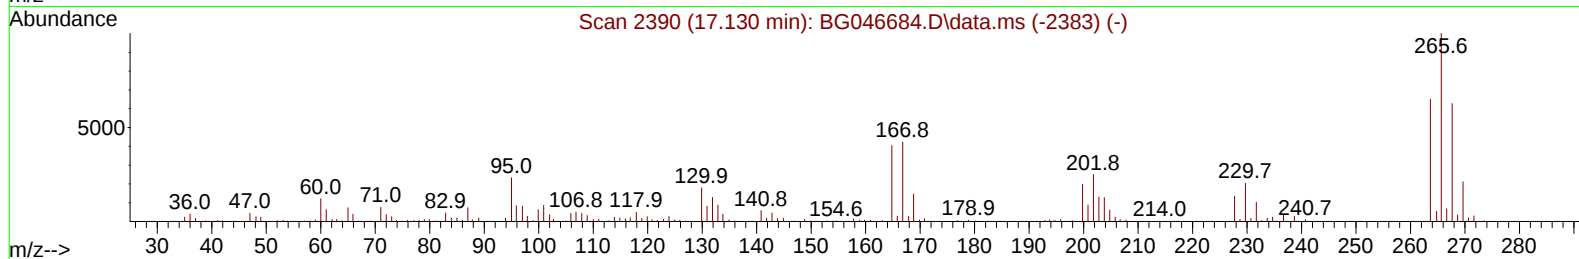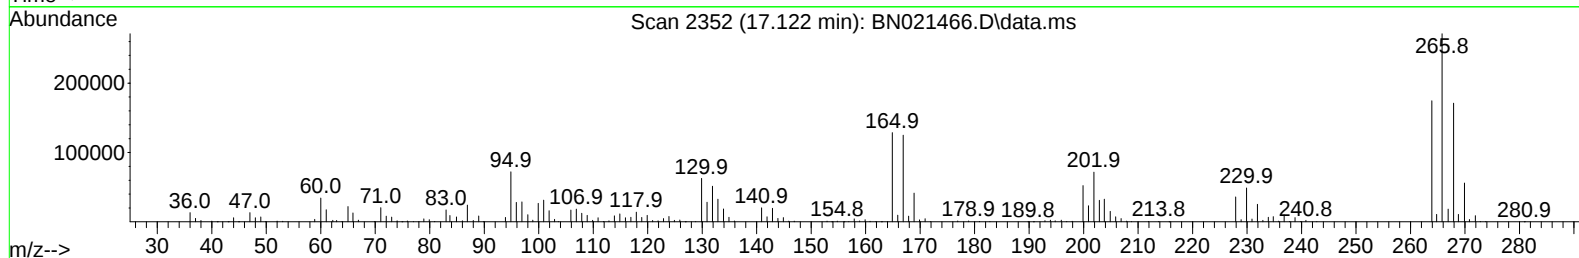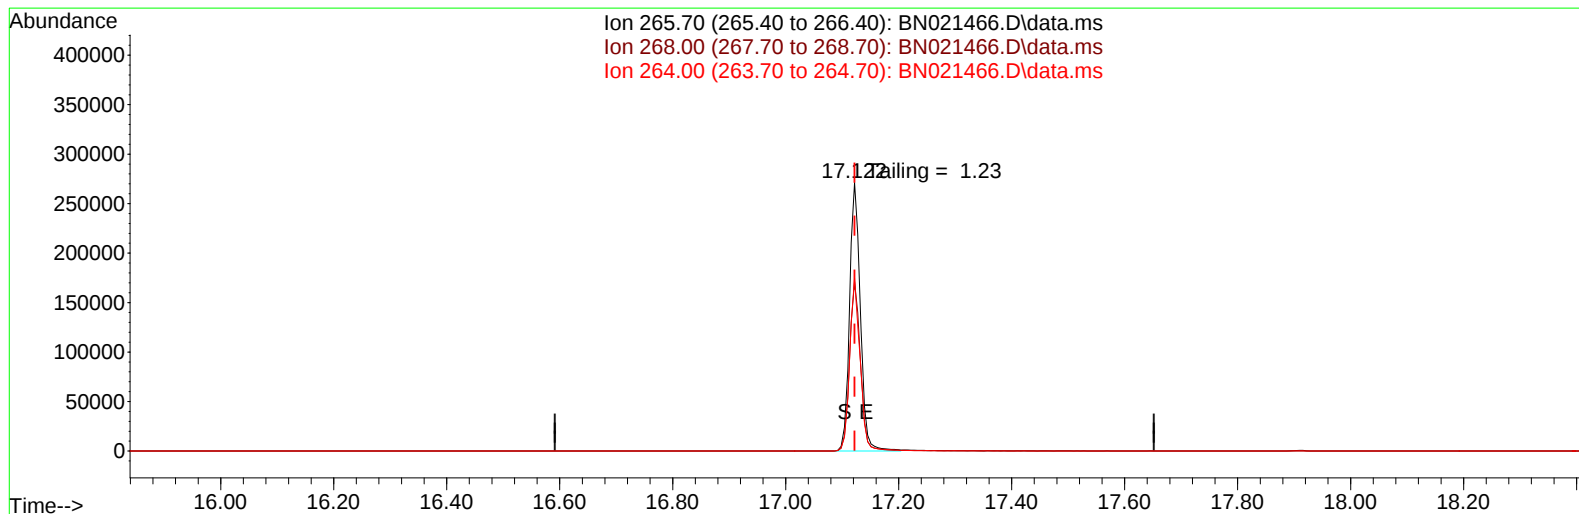

TIC: BN021466.D\data.ms

(70) Pentachlorophenol (C)

17.122min (-0.000) 22830.54 ng




response 362995

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.07
264.00	61.60	64.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083022\
Data File : BN021466.D
Acq On : 30 Aug 2022 22:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 31 02:55:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 02:53:53 2022
Response via : Initial Calibration

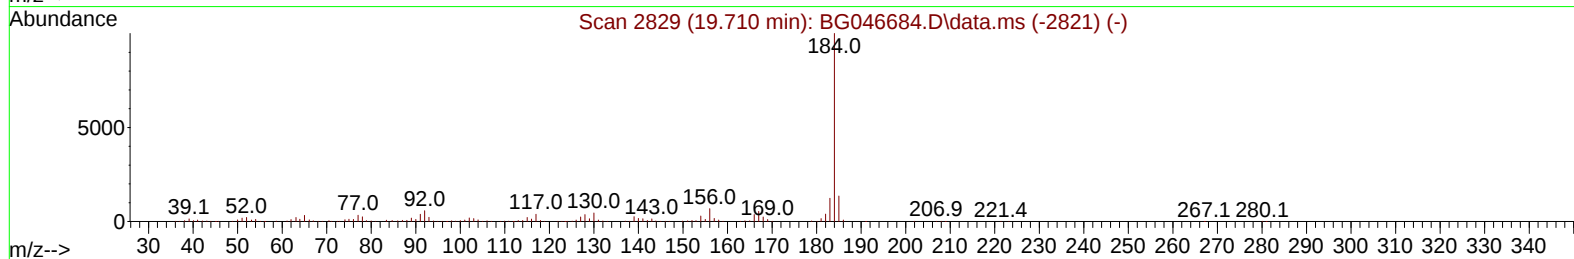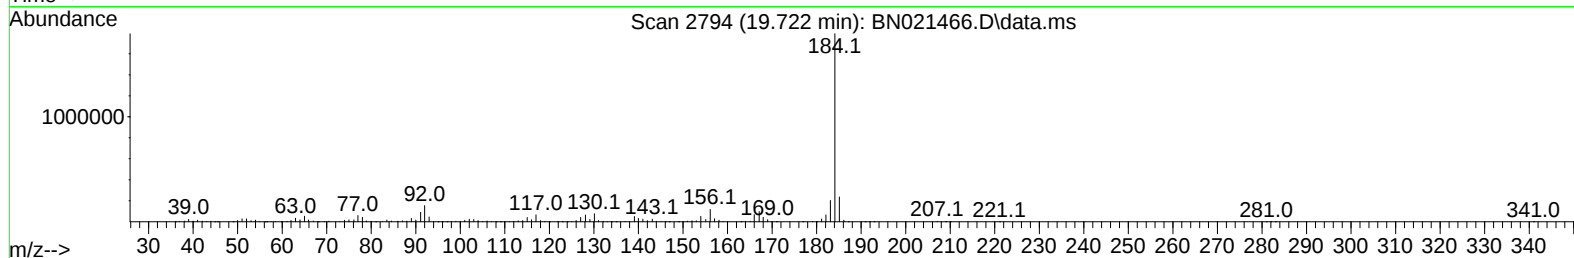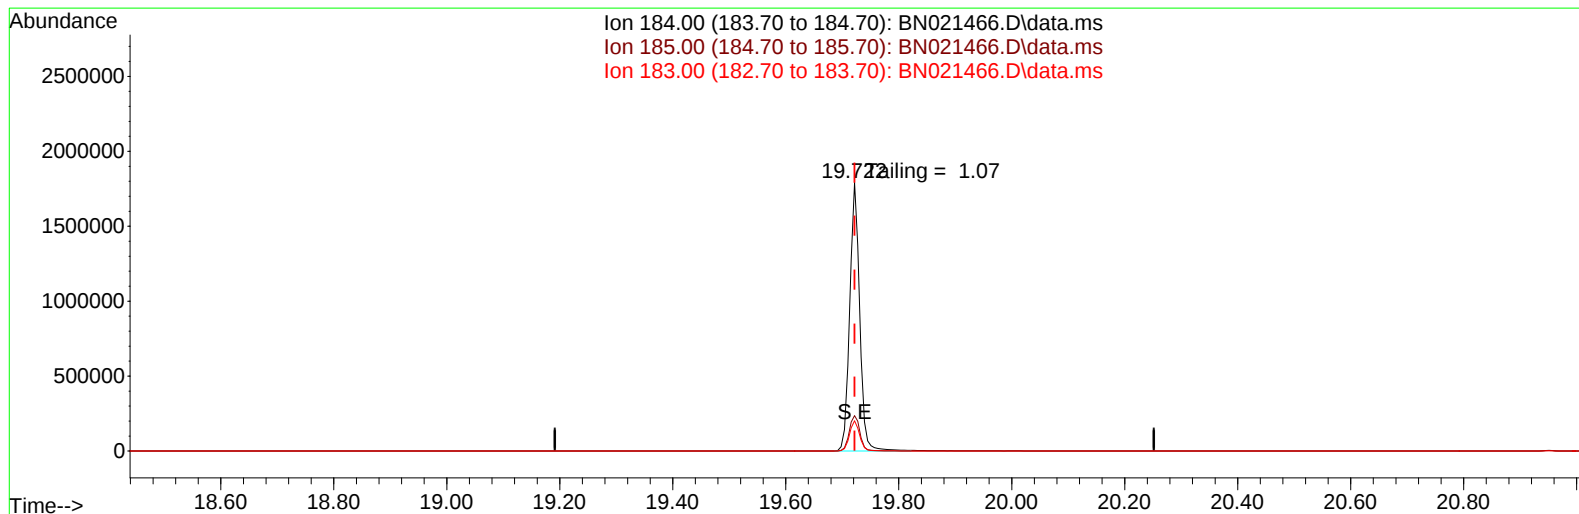

TIC: BN021466.D\data.ms

(77) Benzidine

19.722min (-0.000) 0.00 ng

response 2217341

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.17
183.00	13.20	11.29
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/30/2022	BNA_N	<u>BN021466.D</u>
Compound Name	Response	Retention Time
DDT	1007716	20.951
DDD	13255	20.51
DDE	455	19.998
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13710	1021426	1.34

Instrument :
BNA_N
ClientSampleId :
DFTPP