


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN090120\
Data File : BN011685.D
Acq On : 01 Sep 2020 15:28
Operator : CG/JU
Sample : L3843-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE7

Manual Integrations
APPROVED

mohammad
9/2/2020 1:59:52 PM

Quant Time: Sep 01 16:01:28 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 01 13:14:23 2020
Response via : Initial Calibration

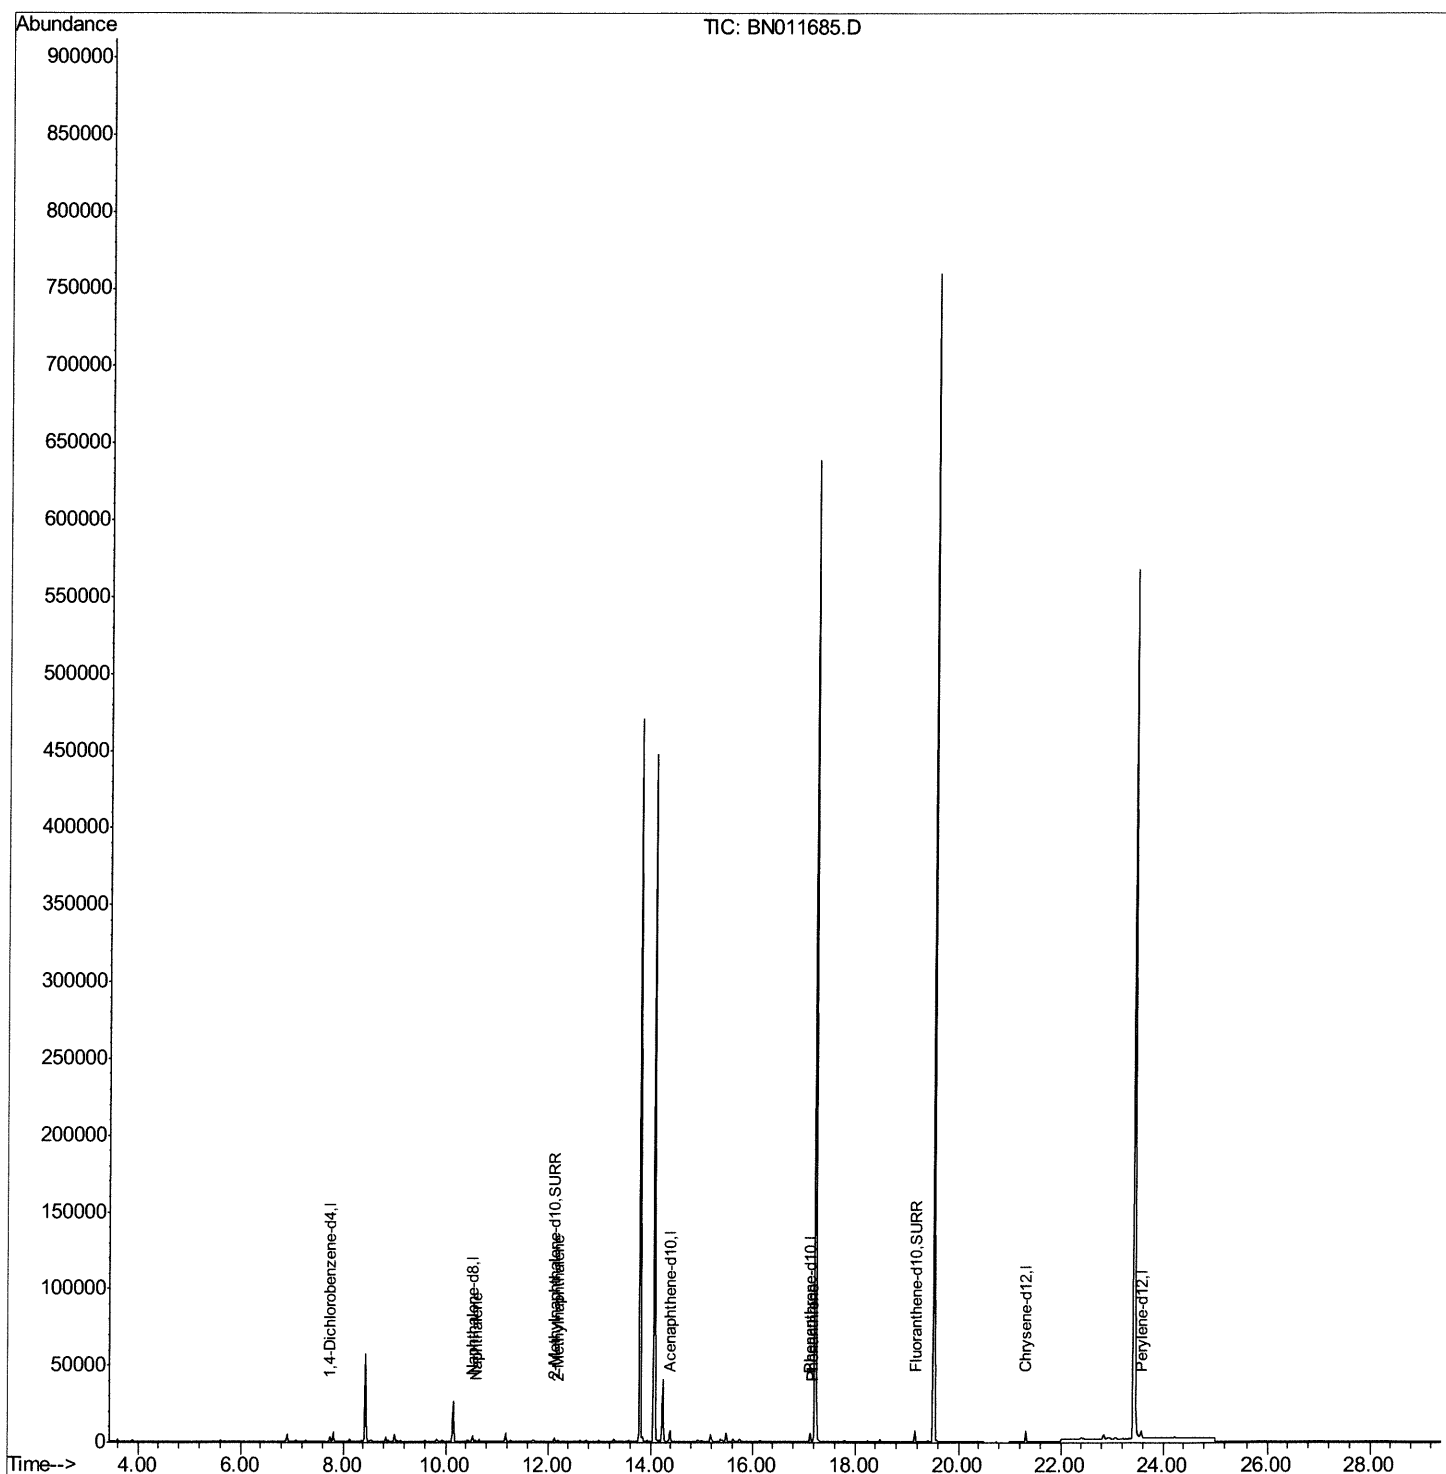

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN090120\
 Data File : BN011685.D
 Acq On : 01 Sep 2020 15:28
 Operator : CG/JU
 Sample : L3843-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE7

Manual Integrations
 APPROVED

mohammad
 9/2/2020 1:59:52 PM

Quant Time: Sep 01 16:00:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 01 13:14:23 2020
 Response via : Initial Calibration

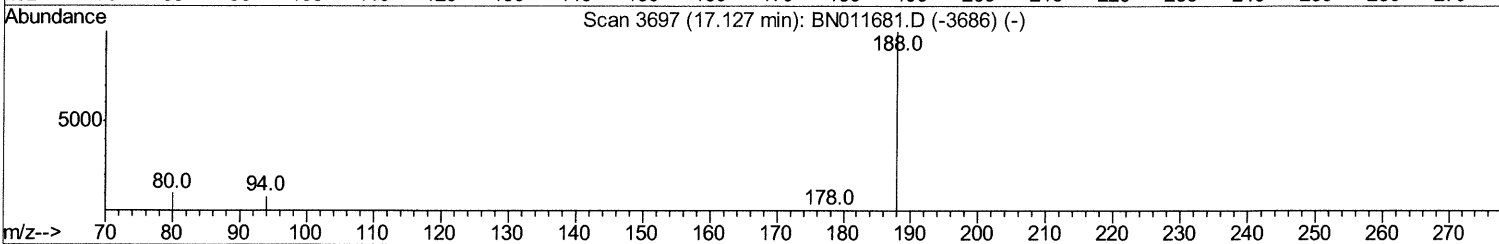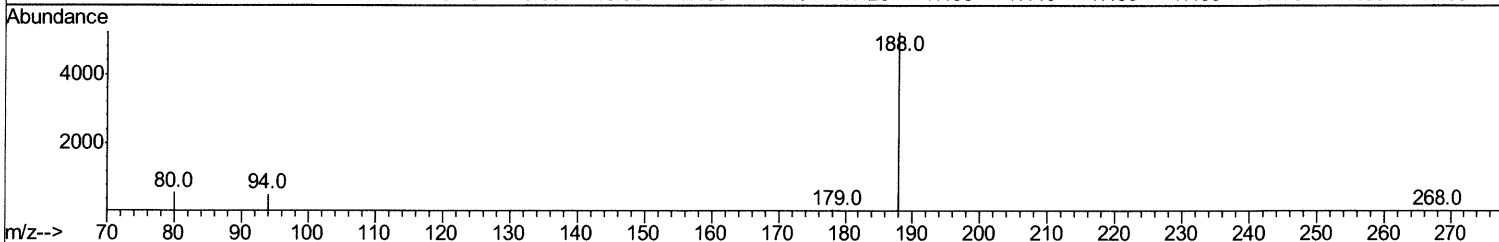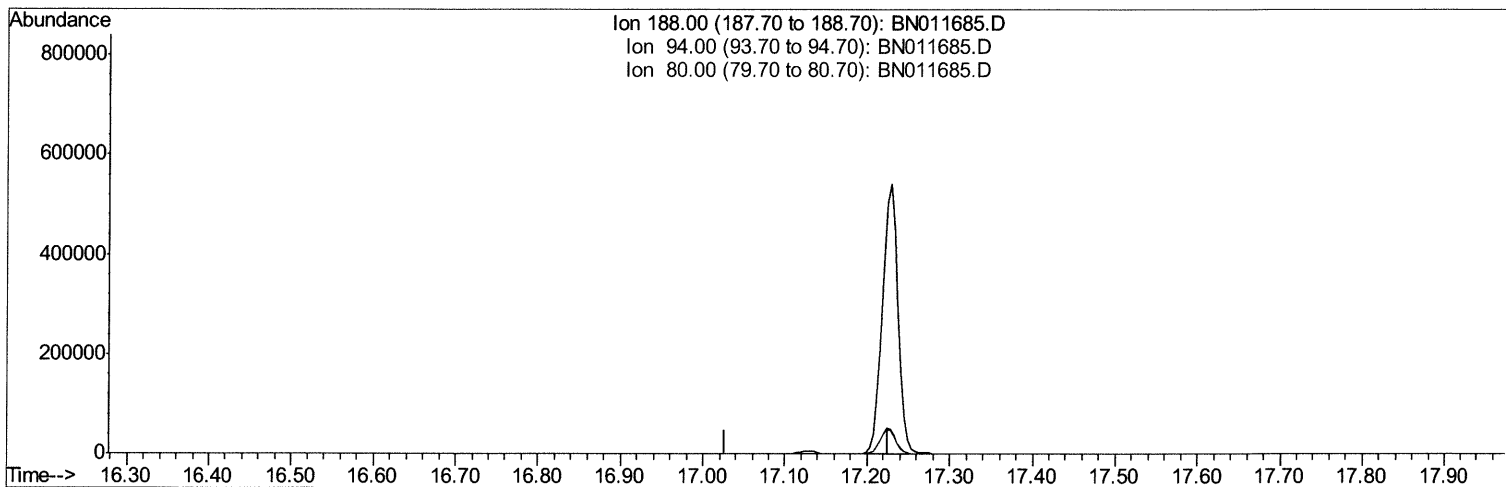

TIC: BN011685.D

(10) Phenanthrene-d10 (I)

17.127min (-17.127) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	8.20	0.00#
80.00	9.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN090120\
Data File : BN011685.D
Acq On : 01 Sep 2020 15:28
Operator : CG/JU
Sample : L3843-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE7

Manual Integrations
APPROVED

mohammad
9/2/2020 1:59:52 PM

Quant Time: Sep 01 16:00:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 01 13:14:23 2020
Response via : Initial Calibration

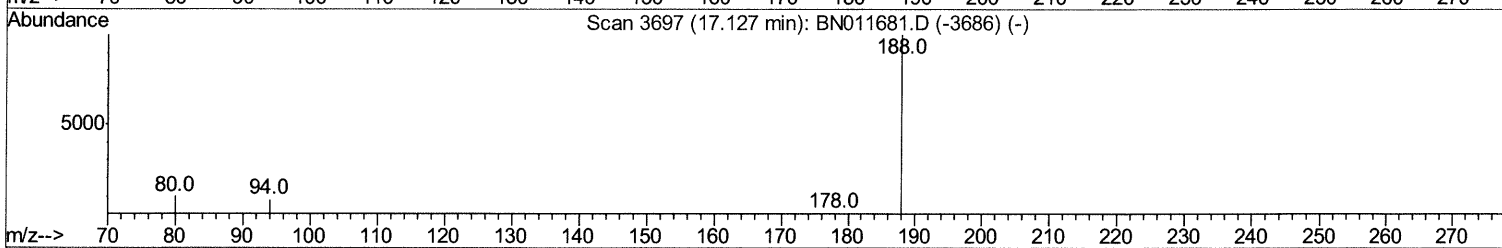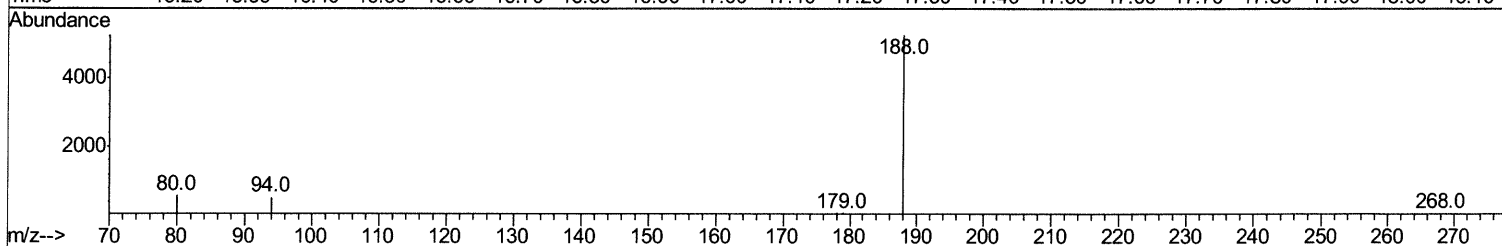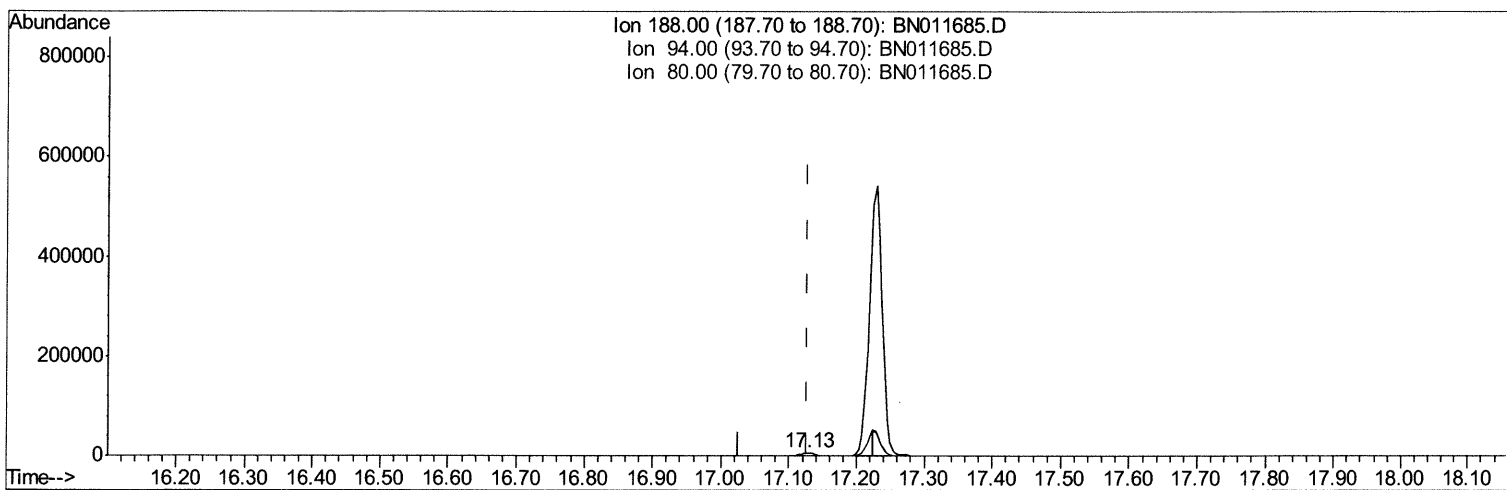

TIC: BN011685.D

(10) Phenanthrene-d10 (I)

17.127min (-0.000) 0.40ng/ul m 09/11/20 JU

response 7395

Ion	Exp%	Act%
188.00	100	100
94.00	8.20	9.82
80.00	9.00	11.06#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN090120\
 Data File : BN011685.D
 Acq On : 01 Sep 2020 15:28
 Operator : CG/JU
 Sample : L3843-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE7

Manual Integrations
 APPROVED

mohammad
 9/2/2020 1:59:52 PM

Quant Time: Sep 01 16:01:28 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 01 13:14:23 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	1492	0.40	ng/ul	0.00
2) Naphthalene-d8	10.53	136	5685	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.38	164	3595	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.13	188	7395m>	0.40	ng/ul>	0.00
16) Chrysene-d12	21.32	240	6387	0.40	ng/ul	0.00
20) Perylene-d12	23.57	264	6779	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.12	152	3118	0.39	ng/ul	0.00
14) Fluoranthene-d10	19.16	212	7820	0.38	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.58	128	1196	0.072	ng/ul#	86
5) 2-Methylnaphthalene	12.19	142	414	0.040	ng/ul	96
12) Phenanthrene	17.17	178	593	0.024	ng/ul#	80

(#) = qualifier out of range (m) = manual integration (+) = signals summed