
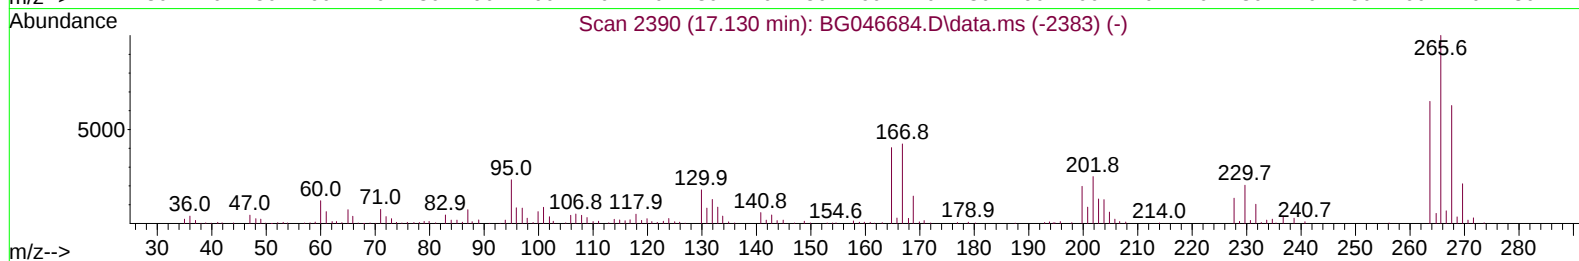
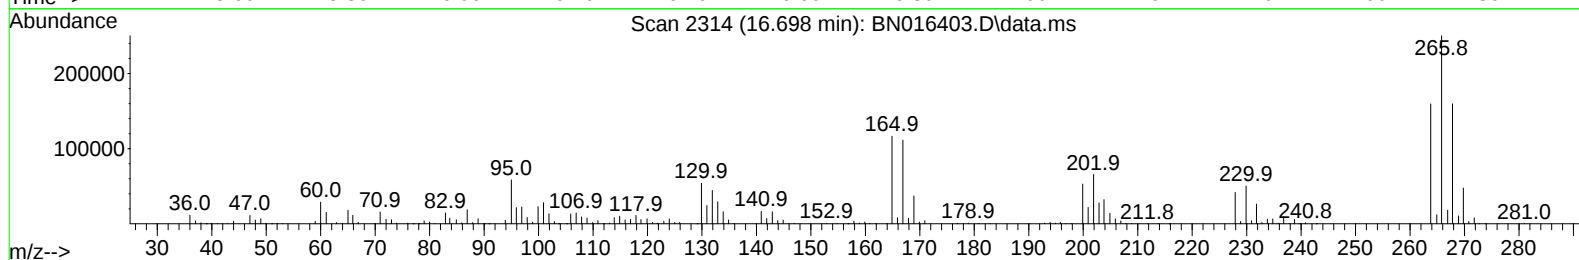


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092221\
Data File : BN016403.D
Acq On : 22 Sep 2021 09:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 10:44:28 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 21 13:04:53 2021
Response via : Initial Calibration

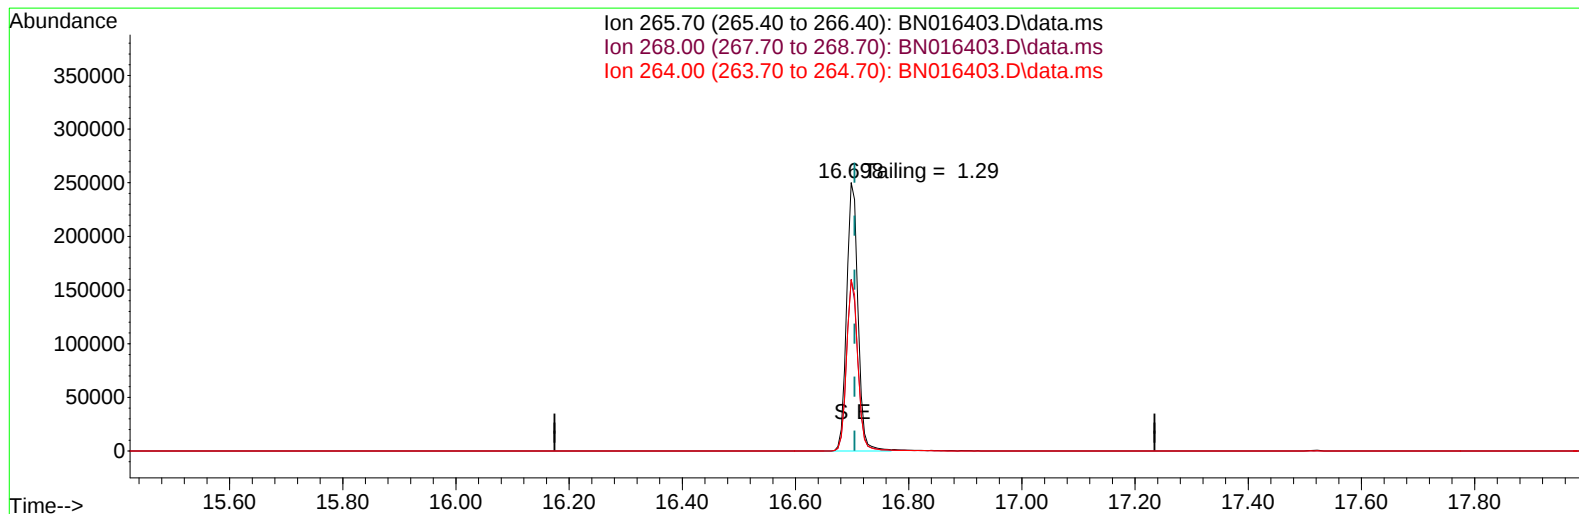

TIC: BN016403.D\data.ms

(70) Pentachlorophenol (C)




16.698min (-0.006) 21521.99 ng

response 351648

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.92
264.00	61.60	63.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092221\
Data File : BN016403.D
Acq On : 22 Sep 2021 09:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 10:44:28 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 21 13:04:53 2021
Response via : Initial Calibration

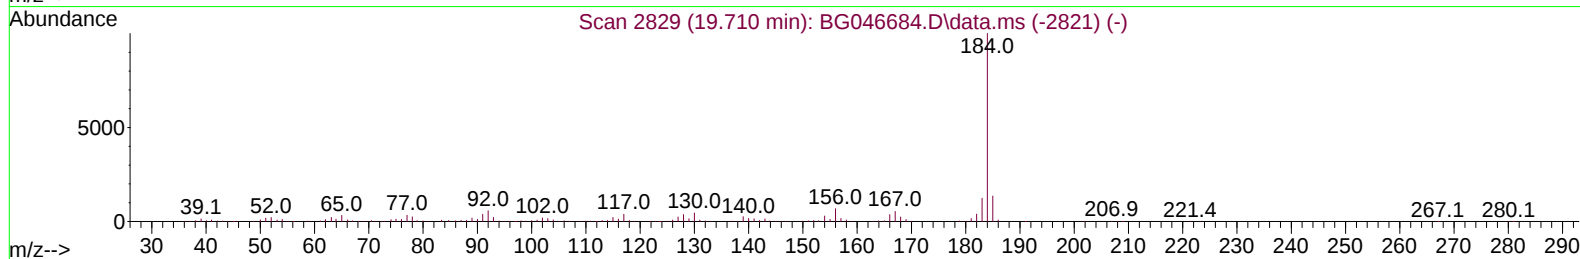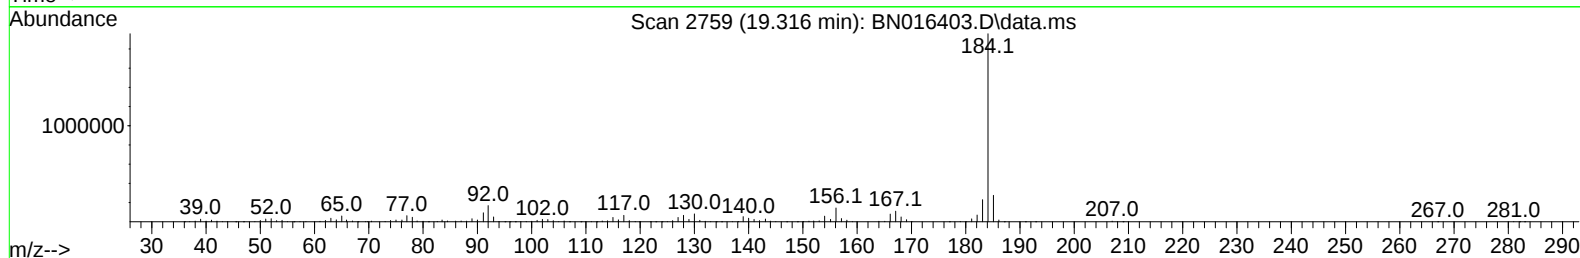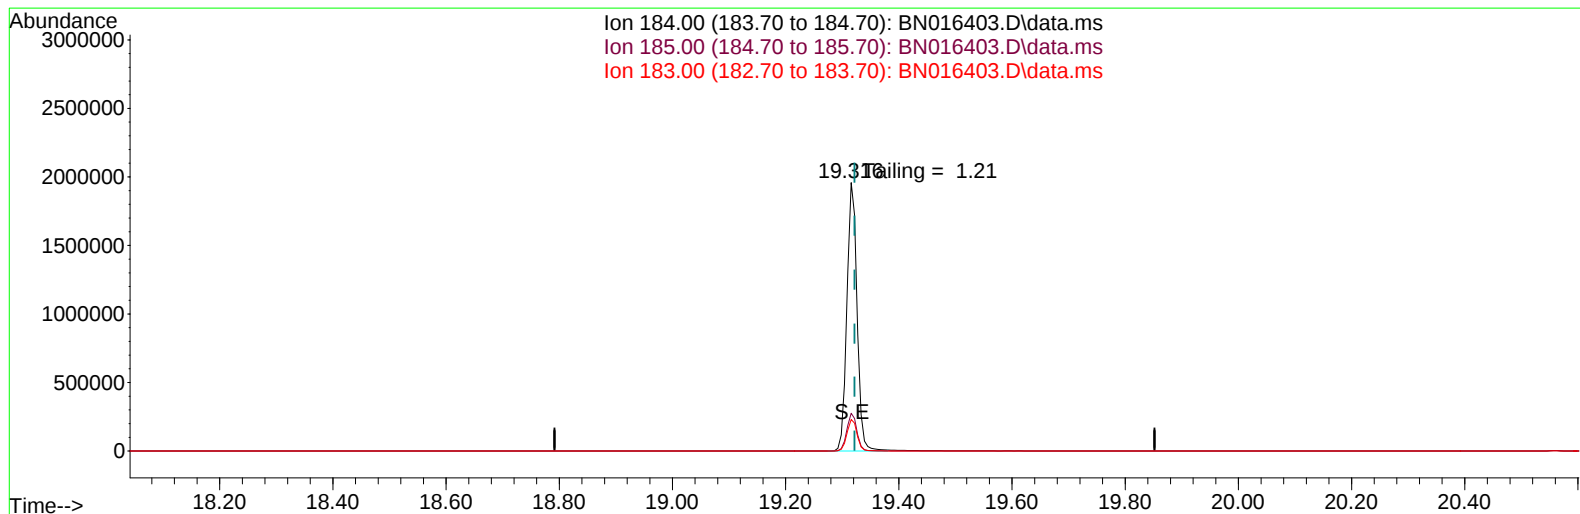

TIC: BN016403.D\data.ms

(77) Benzidine

19.316min (-0.006) 0.00 ng

response 2473272

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.07
183.00	13.20	11.77
0.00	0.00	0.00