


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092221\
 Data File : BN016403.D
 Acq On : 22 Sep 2021 09:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 21 13:21:55 2021

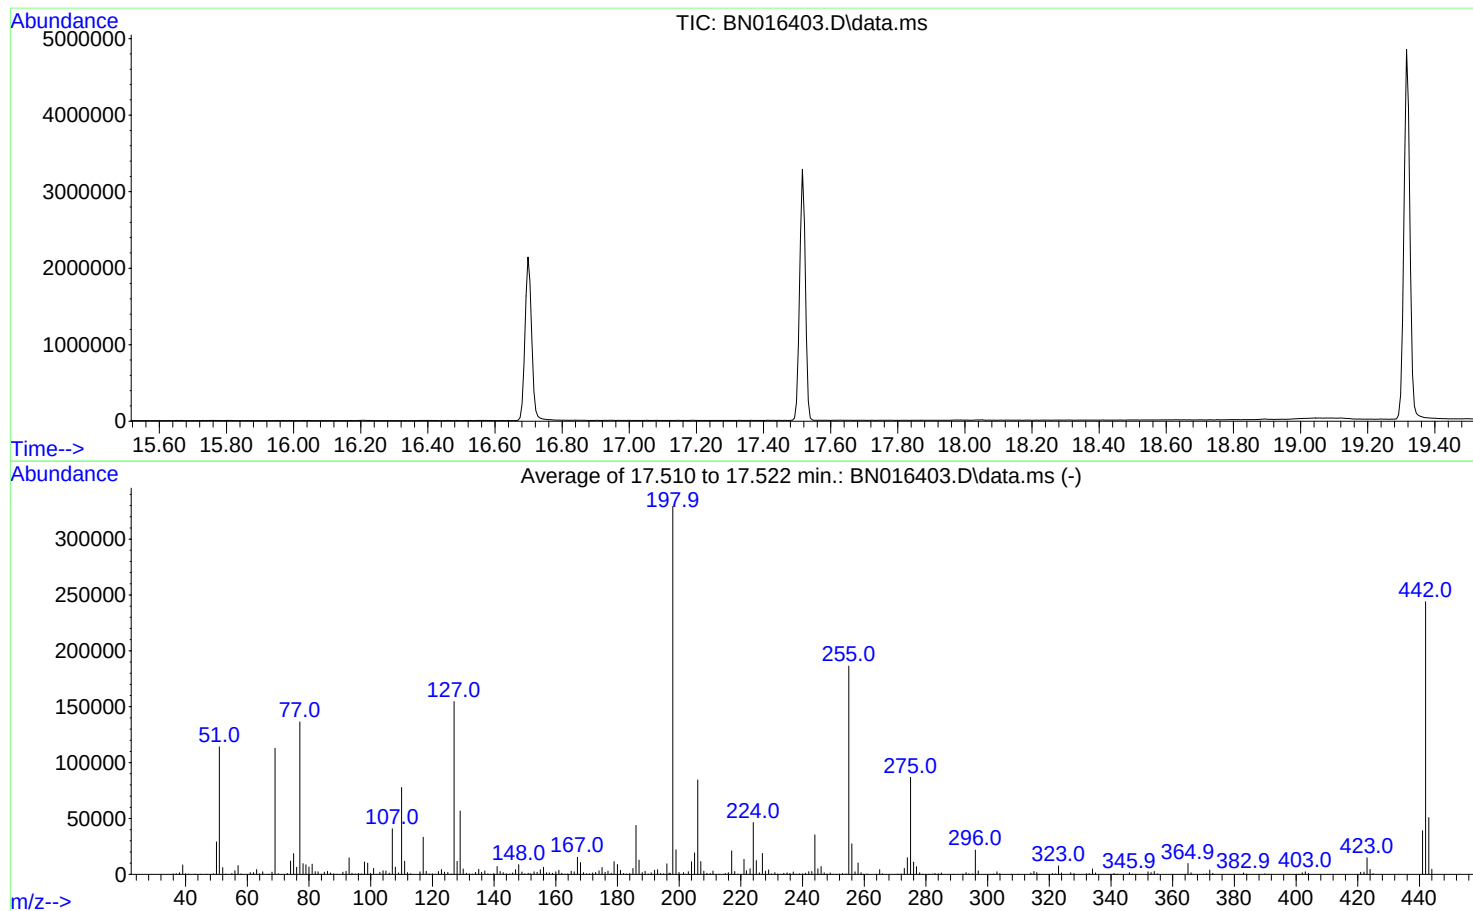




AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	114062	PASS
68	69	0.00	2	1.8	2059	PASS
69	198	0.00	100	34.3	112883	PASS
70	69	0.00	2	0.6	629	PASS
127	198	10	80	47.0	154560	PASS
197	198	0.00	2	0.4	1175	PASS
198	198	100	100	100.0	329152	PASS
199	198	5	9	6.7	22099	PASS
275	198	10	60	26.4	86739	PASS
365	198	1	100	3.0	9823	PASS
441	198	0.01	100	11.9	39061	PASS
442	442	50	100	100.0	244011	PASS
443	442	15	24	20.9	50899	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092221\
Data File : BN016403.D
Acq On : 22 Sep 2021 09:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 22 10:44:28 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 21 13:04:53 2021
Response via : Initial Calibration

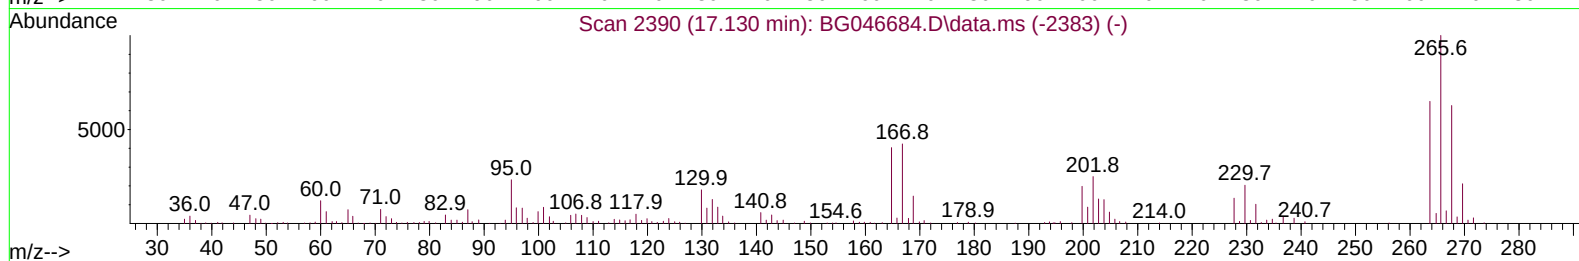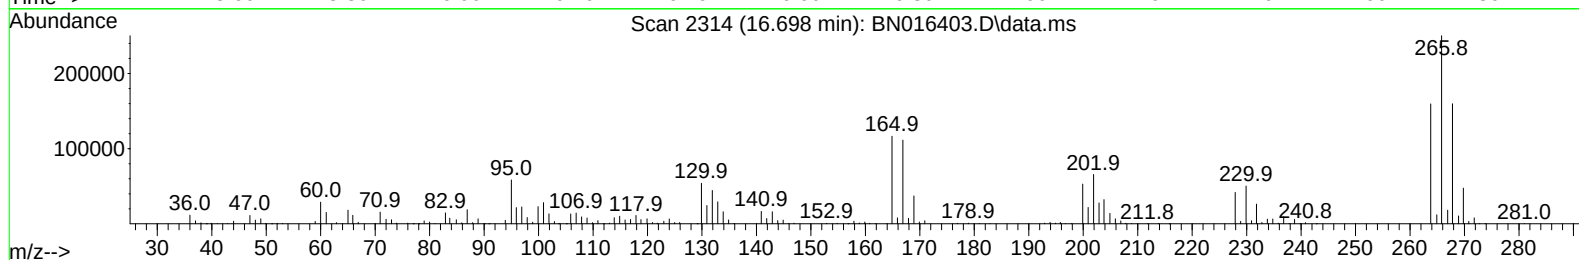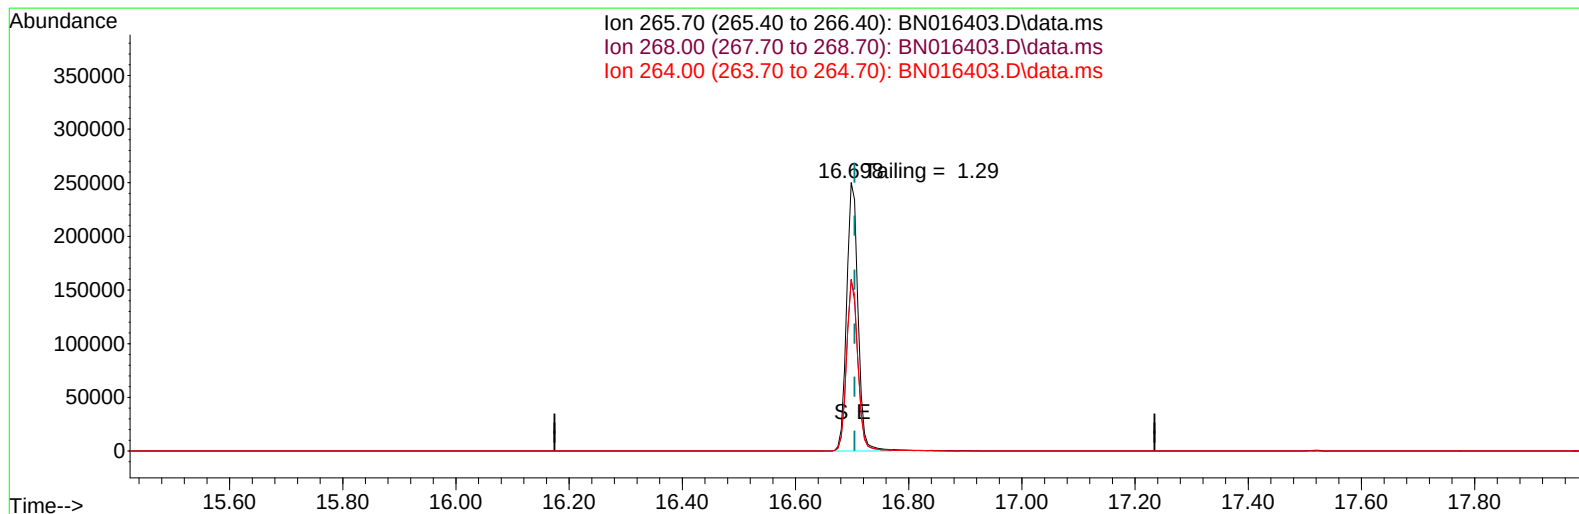

TIC: BN016403.D\data.ms

(70) Pentachlorophenol (C)

16.698min (-0.006) 21521.99 ng




response 351648

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.92
264.00	61.60	63.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092221\
Data File : BN016403.D
Acq On : 22 Sep 2021 09:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 22 10:44:28 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 21 13:04:53 2021
Response via : Initial Calibration

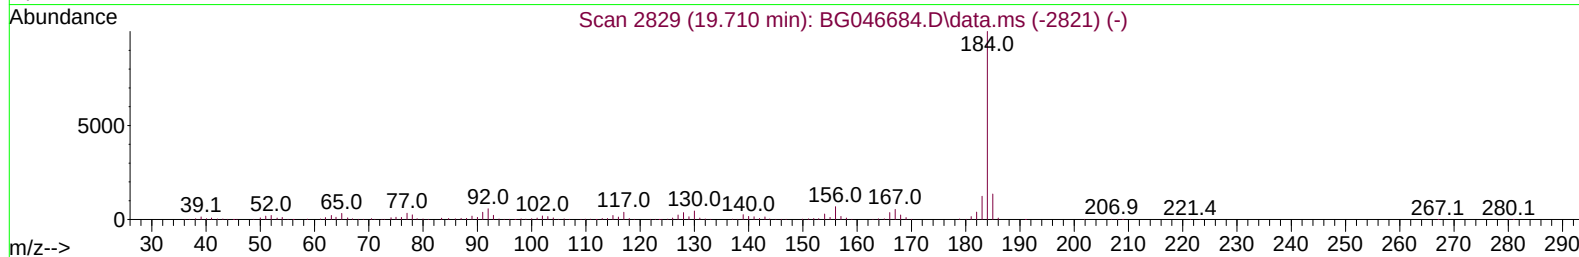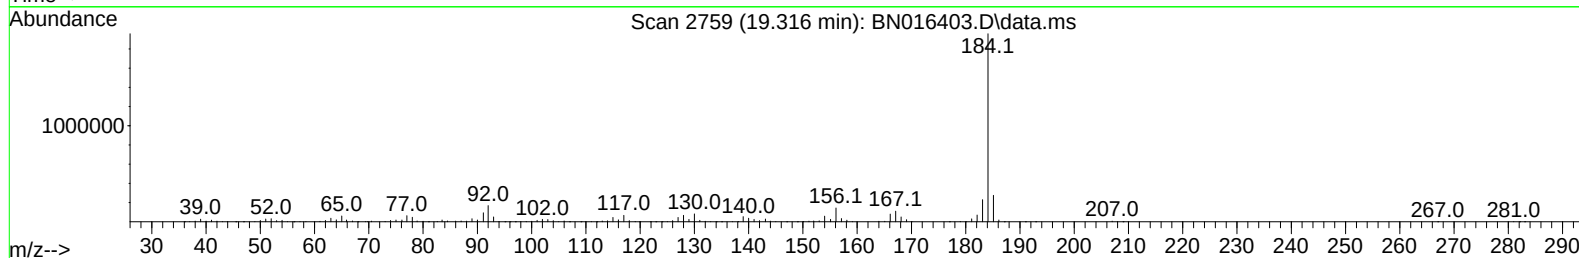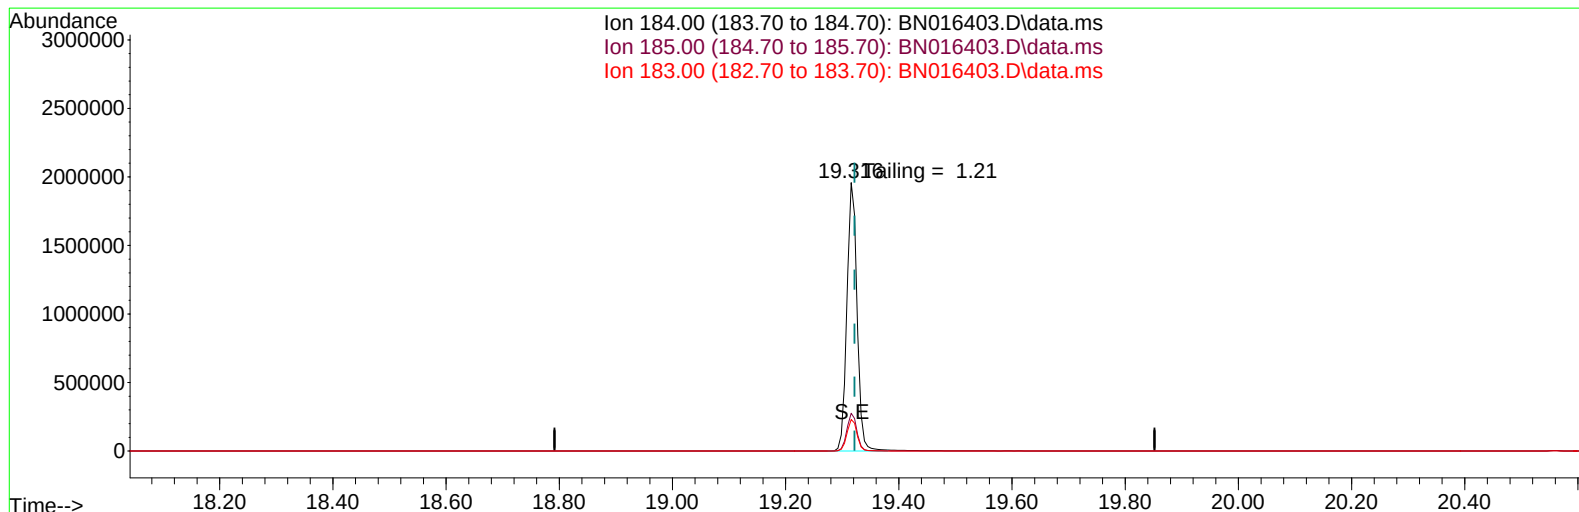

TIC: BN016403.D\data.ms

(77) Benzidine

19.316min (-0.006) 0.00 ng

response 2473272

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.07
183.00	13.20	11.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/22/2021	BNA_N	<u>BN016403.D</u>
Compound Name	Response	Retention Time
DDT	1082521	20.95
DDD	13127	20.11
DDE	0	19.61
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13127	1095648	1.20

Instrument :
BNA_N
ClientSampleId :
DFTPP