

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092321\
 Data File : BN016412.D
 Acq On : 22 Sep 2021 16:42
 Operator : CG/JU
 Sample : SSTD00515
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD005215

Quant Time: Sep 23 01:59:52 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN092321MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 23 01:47:54 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.657	152	200908	20.000	ng/u1	0.00
20) Naphthalene-d8	10.434	136	848801	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.298	164	524984	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.051	188	1086769	20.000	ng/u1	0.00
79) Chrysene-d12	21.257	240	1058480	20.000	ng/u1	0.00
88) Perylene-d12	23.515	264	1052401	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.211	96	10017	2.602	ng/uL	0.00
4) Pyridine-d5	3.605	84	52126	4.645	ng/u1	0.00
7) Phenol-d5	6.834	99	69828	4.606	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.005	67	44992	5.567	ng/u1	0.00
11) 2-Chlorophenol-d4	7.193	132	57468	4.473	ng/u1	0.00
15) 4-Methylphenol-d8	8.363	113	53106	4.346	ng/u1	0.00
21) Nitrobenzene-d5	8.804	128	23048	3.721	ng/u1	0.00
24) 2-Nitrophenol-d4	9.522	143	21705	3.129	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.057	165	50332	3.976	ng/u1	0.00
31) 4-Chloroaniline-d4	10.575	131	77455	4.460	ng/u1	0.00
46) Dimethylphthalate-d6	13.716	166	158058	4.689	ng/u1	0.00
49) Acenaphthylene-d8	13.987	160	198617	4.498	ng/u1	0.00
54) 4-Nitrophenol-d4	14.498	143	21753	3.350	ng/u1	0.00
60) Fluorene-d10	15.292	176	145350	4.892	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.416	200	14898	2.513	ng/u1	0.00
73) Anthracene-d10	17.145	188	219764	4.659	ng/u1	0.00
81) Pyrene-d10	19.451	212	239684	4.776	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.368	264	228017	4.425	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.246	88	10261	2.367	ng/uL#	85
5) Pyridine	3.622	79	61959	5.555	ng/u1#	84
6) Benzaldehyde	6.805	77	45988	5.062	ng/u1	95
8) Phenol	6.857	94	74529	4.825	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.093	93	61268	5.228	ng/u1	96
12) 2-Chlorophenol	7.222	128	59722	4.624	ng/u1	95
13) 2-Methylphenol	8.099	108	53003	4.440	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.187	45	85994	5.556	ng/u1	98
16) Acetophenone	8.475	105	89074	4.794	ng/u1#	94
17) N-Nitroso-di-n-propyla...	8.457	70	41370	4.806	ng/u1	97
18) 4-Methylphenol	8.422	108	58165	4.506	ng/u1	96
19) Hexachloroethane	8.722	117	23826	4.671	ng/u1	90
22) Nitrobenzene	8.846	77	59598	4.722	ng/u1	93
23) Isophorone	9.369	82	106670	4.350	ng/u1	97
25) 2-Nitrophenol	9.551	139	25484	3.442	ng/u1	94
26) 2,4-Dimethylphenol	9.622	107	62308	4.516	ng/u1	99
27) Bis(2-Chloroethoxy)met...	9.863	93	78819	5.077	ng/u1	97
29) 2,4-Dichlorophenol	10.081	162	51940	4.173	ng/u1	98
30) Naphthalene	10.481	128	206729	4.991	ng/u1	99
32) 4-Chloroaniline	10.598	127	81457	4.613	ng/u1	99
33) Hexachlorobutadiene	10.769	225	35029	4.220	ng/u1	97
34) Caprolactam	11.351	113	11841	2.799	ng/u1	97
35) 4-Chloro-3-methylphenol	11.728	107	52124	4.050	ng/u1	99
36) 2-Methylnaphthalene	12.104	142	134759	4.771	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092321\
 Data File : BN016412.D
 Acq On : 22 Sep 2021 16:42
 Operator : CG/JU
 Sample : SSTD00515
 Misc :
 ALS Vial : 2 Sample Multiplier: 1


Instrument :
 BNA_N
 ClientSampleId :
 SSTD005215


Quant Time: Sep 23 01:59:52 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN092321MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 23 01:47:54 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.322	142	138894	4.810	ng/ul	96
39) 1,2,4,5-Tetrachloroben...	12.475	216	68345	4.635	ng/ul#	94
40) Hexachlorocyclopentadiene	12.451	237	35010	4.141	ng/ul	99
41) 2,4,6-Trichlorophenol	12.716	196	37885	4.009	ng/ul	95
42) 2,4,5-Trichlorophenol	12.787	196	41181	4.028	ng/ul	96
43) 1,1'-Biphenyl	13.128	154	183301	5.172	ng/ul	98
44) 2-Chloronaphthalene	13.163	162	138818	4.941	ng/ul	98
45) 2-Nitroaniline	13.375	65	24943	3.492	ng/ul	93
47) Dimethylphthalate	13.763	163	164506	4.881	ng/ul	99
48) 2,6-Dinitrotoluene	13.881	165	22075	3.088	ng/ul#	76
50) Acenaphthylene	14.016	152	217454	4.767	ng/ul	98
51) 3-Nitroaniline	14.204	138	25628	3.238	ng/ul	83
52) Acenaphthene	14.357	153	149855	5.148	ng/ul	97
53) 2,4-Dinitrophenol	14.410	184	9282	2.424	ng/ul#	89
55) 4-Nitrophenol	14.510	109	17551	4.043	ng/ul	90
56) Dibenzofuran	14.698	168	213818	5.083	ng/ul	93
57) 2,4-Dinitrotoluene	14.669	165	31767	3.083	ng/ul	92
58) 2,3,4,6-Tetrachlorophenol	14.928	232	31784	3.792	ng/ul#	91
59) Diethylphthalate	15.139	149	169760	5.093	ng/ul	98
61) Fluorene	15.351	166	171007	5.037	ng/ul	94
62) 4-Chlorophenyl-phenyle...	15.351	204	83498	4.839	ng/ul	95
63) 4-Nitroaniline	15.369	138	25860	3.142	ng/ul#	86
66) 4,6-Dinitro-2-methylph...	15.428	198	15438	2.755	ng/ul#	91
67) N-Nitrosodiphenylamine	15.569	169	139245	4.713	ng/ul	99
68) 4-Bromophenyl-phenylether	16.251	248	48122	4.547	ng/ul	96
69) Hexachlorobenzene	16.351	284	54501	4.424	ng/ul#	92
70) Atrazine	16.528	200	41870	3.777	ng/ul	93
71) Pentachlorophenol	16.698	266	23423	3.727	ng/ul	93
72) Phenanthrene	17.092	178	273364	5.024	ng/ul	99
74) Anthracene	17.180	178	265948	4.756	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	13.087	216	71463	4.658	ng/ul	95
76) Pentachlorobenzene	14.616	250	70139	4.621	ng/ul	97
77) Carbazole	17.457	167	230429	4.635	ng/ul	98
78) Di-n-butylphthalate	18.039	149	237690	4.086	ng/ul	99
80) Fluoranthene	19.116	202	297298	4.818	ng/ul	96
82) Pyrene	19.480	202	323218	5.085	ng/ul	98
83) Butylbenzylphthalate	20.410	149	79177	3.107	ng/ul	92
84) 3,3'-Dichlorobenzidine	21.180	252	80401	3.766	ng/ul	98
85) Benzo(a)anthracene	21.239	228	303295	4.786	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.192	149	136498	3.668	ng/ul#	94
87) Chrysene	21.292	228	302116	4.891	ng/ul	97
89) Di-n-octyl phthalate	22.086	149	190445	3.002	ng/ul	100
90) Benzo(b)fluoranthene	22.880	252	282113	4.529	ng/ul	99
91) Benzo(k)fluoranthene	22.880	252	282113	4.930	ng/ul	98
93) Benzo(a)pyrene	23.415	252	275163	4.572	ng/ul	96
94) Indeno(1,2,3-cd)pyrene	26.504	276	258047	3.807	ng/ul	100
95) Dibenzo(a,h)anthracene	25.833	278	267179	4.580	ng/ul#	97
96) Benzo(g,h,i)perylene	26.504	276	258047	4.492	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Sep 23 01:59:52 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN092321MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 23 01:47:54 2021
Response via : Initial Calibration




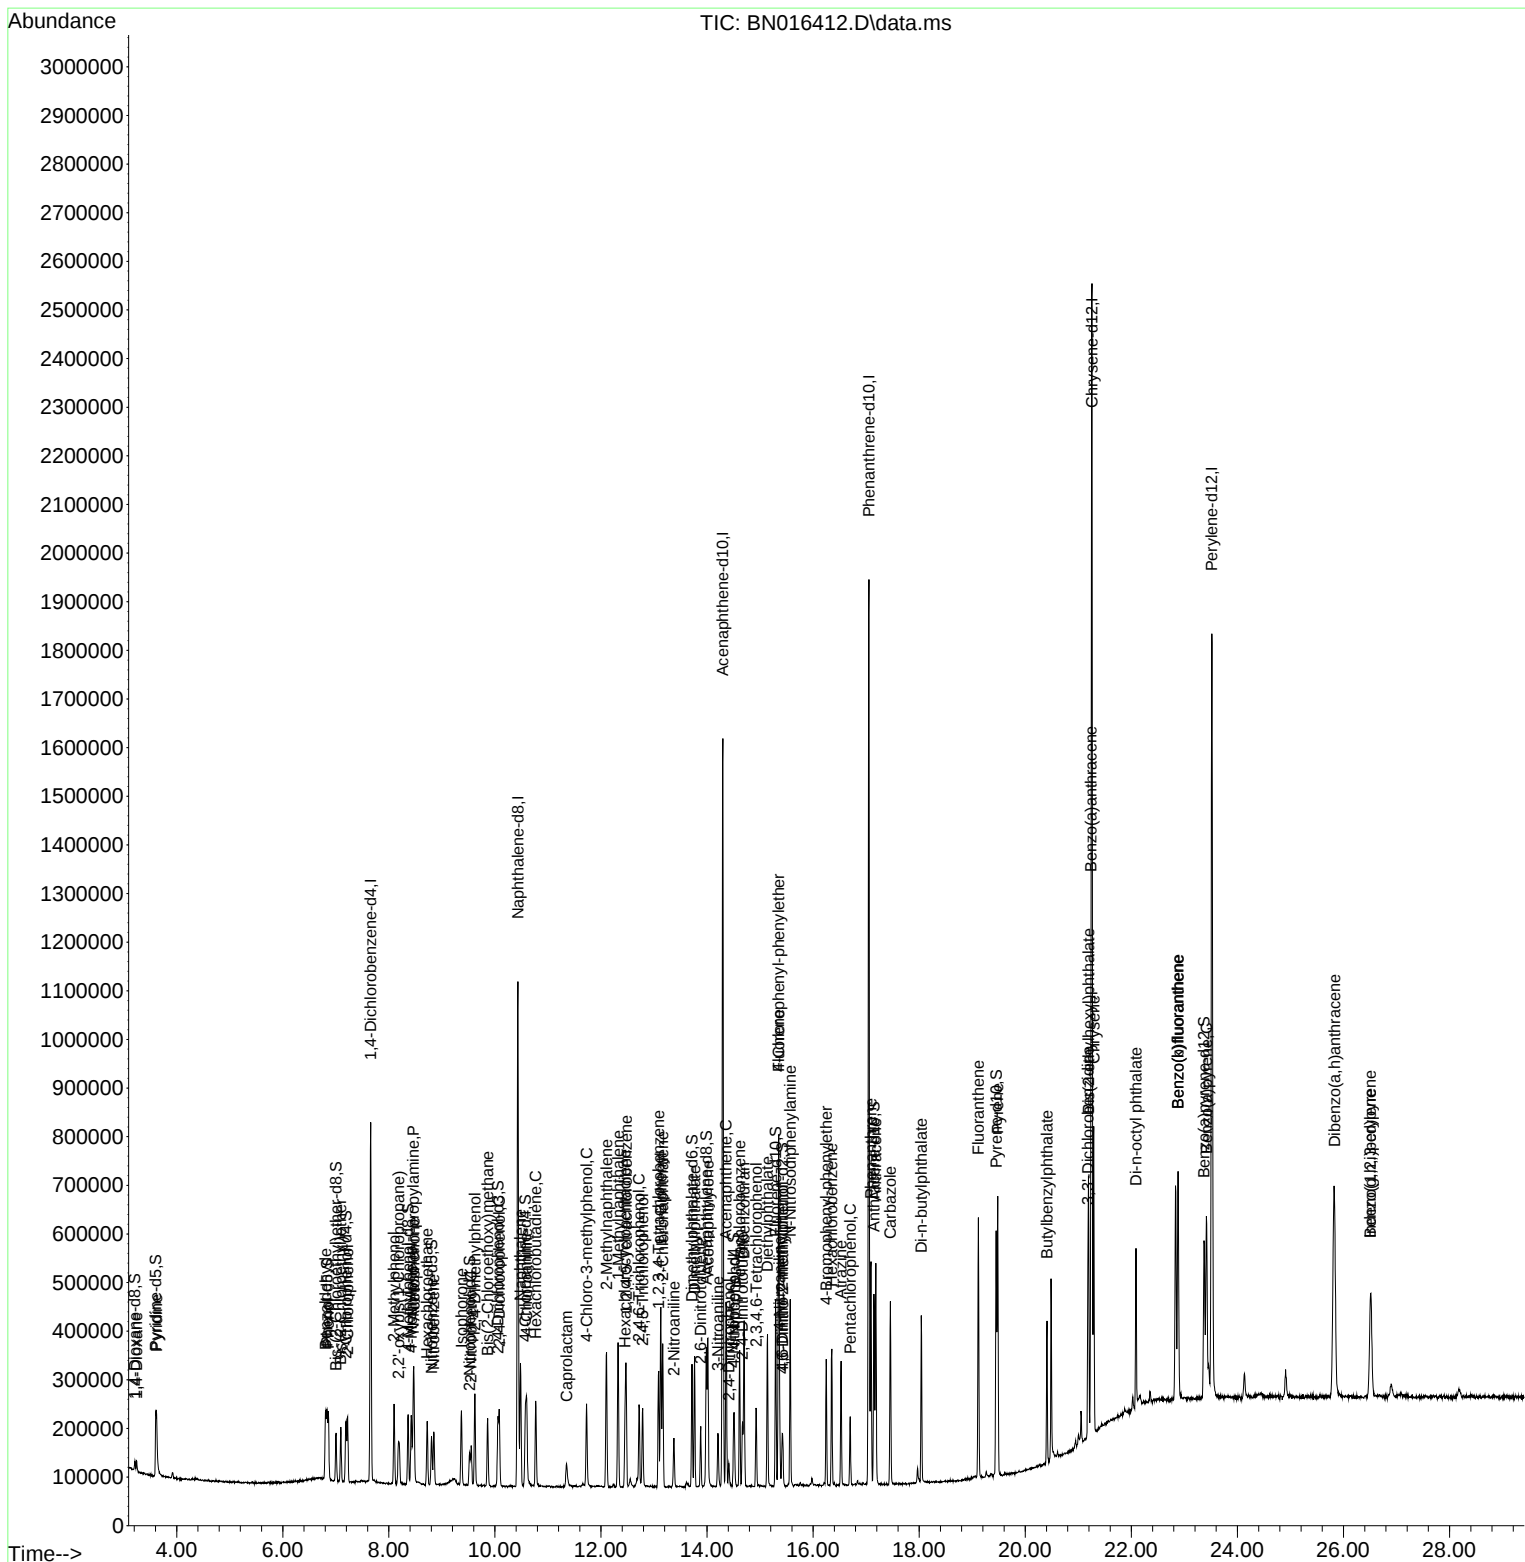




#2
1,4-Dioxane
Concen: 2.367 ng/uL
RT: 3.246 min Scan# 27
Delta R.T. 0.006 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion: 88 Resp: 10261
Ion Ratio Lower Upper
88 100
43 25.6 23.2 34.8
58 52.8 54.3 81.5#

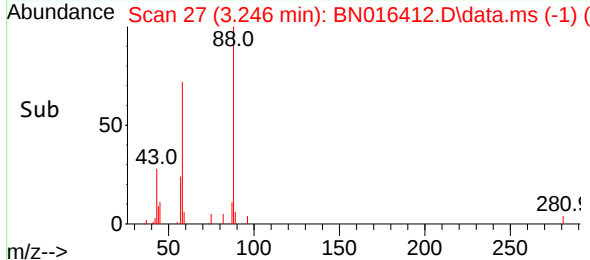

#5
Pyridine
Concen: 5.555 ng/uL
RT: 3.622 min Scan# 91
Delta R.T. 0.006 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion: 79 Resp: 61959
Ion Ratio Lower Upper
79 100
52 78.3 66.8 100.2
51 61.2 30.7 46.1#




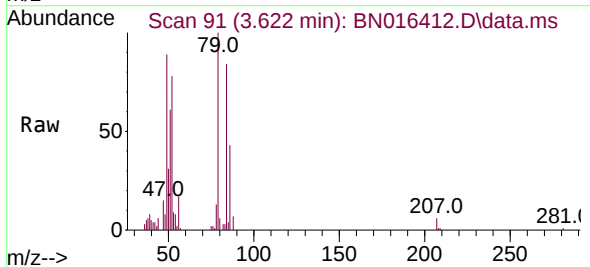




#6
Benzaldehyde
Concen: 5.062 ng/ul
RT: 6.805 min Scan# 632
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:	77	Resp:	45988
Ion	Ratio	Lower	Upper
77	100		
105	102.4	83.7	125.5
106	94.9	82.2	123.2

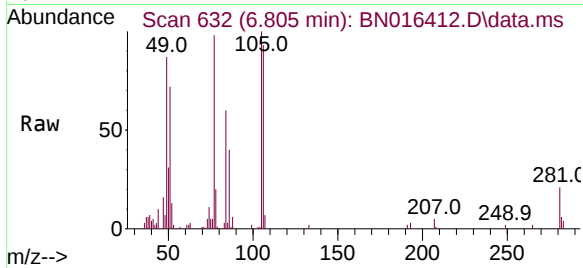

#8
Phenol
Concen: 4.825 ng/ul
RT: 6.857 min Scan# 641
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:	94	Resp:	74529
Ion	Ratio	Lower	Upper
94	100		
65	27.0	21.5	32.3
66	34.2	28.6	42.8


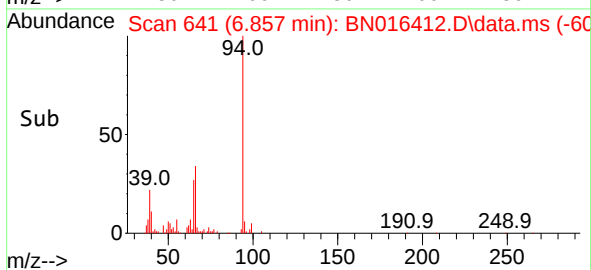

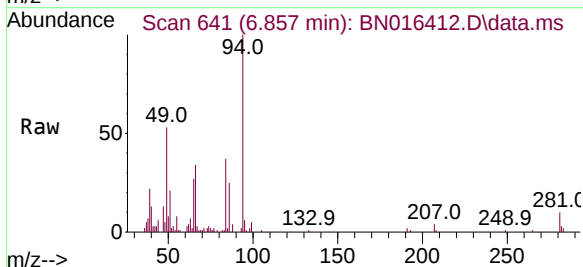




#10
Bis(2-Chloroethyl)ether
Concen: 5.228 ng/ul
RT: 7.093 min Scan# 681
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:	93	Resp:	61268
Ion	Ratio	Lower	Upper
93	100		
63	78.4	59.3	88.9
95	32.9	26.3	39.5

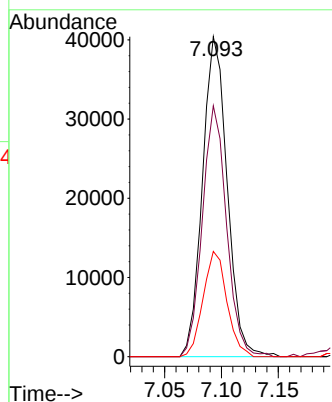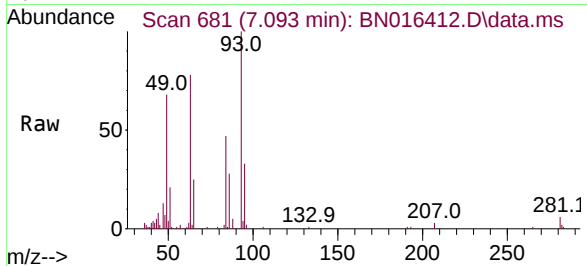

#12
2-Chlorophenol
Concen: 4.624 ng/ul
RT: 7.222 min Scan# 703
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:	128	Resp:	59722
Ion	Ratio	Lower	Upper
128	100		
64	46.1	33.4	50.2
130	32.7	25.4	38.0


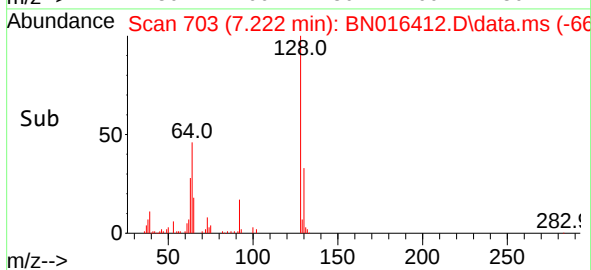

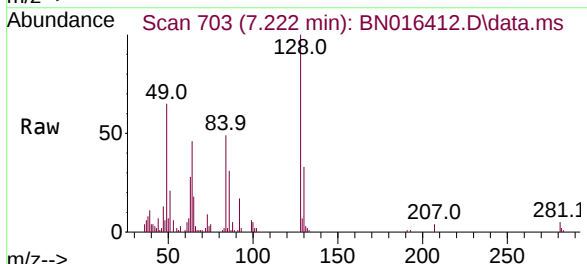




#13
2-Methylphenol
Concen: 4.440 ng/ul
RT: 8.099 min Scan# 852
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:108 Resp: 53003
Ion Ratio Lower Upper
108 100
107 90.5 71.5 107.3

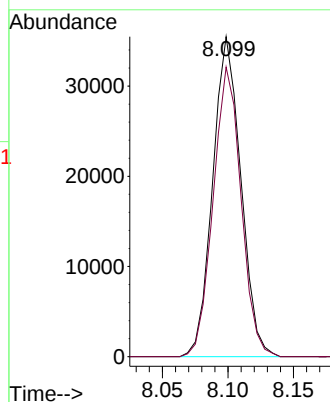

#14
2,2'-oxybis(1-Chloropropane)
Concen: 5.556 ng/ul
RT: 8.187 min Scan# 867
Delta R.T. -0.006 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion: 45 Resp: 85994
Ion Ratio Lower Upper
45 100
77 14.4 11.0 16.4
79 11.6 8.4 12.6




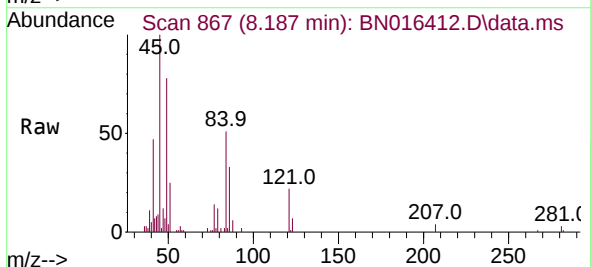




#16
Acetophenone
Concen: 4.794 ng/ul
RT: 8.475 min Scan# 916
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:105 Resp: 89074
Ion Ratio Lower Upper
105 100
77 74.0 59.0 88.4
51 37.5 20.3 30.5#

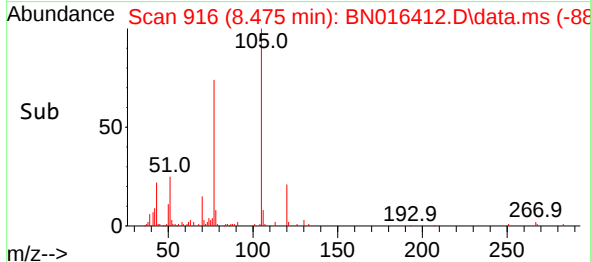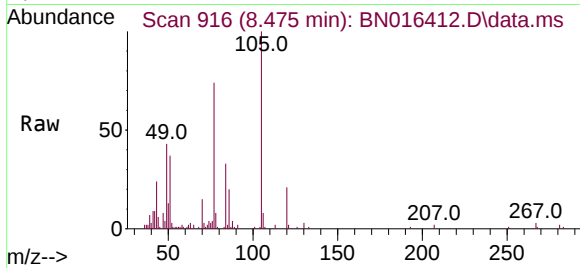

#17
N-Nitroso-di-n-propylamine
Concen: 4.806 ng/ul
RT: 8.457 min Scan# 913
Delta R.T. -0.006 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion: 70 Resp: 41370
Ion Ratio Lower Upper
70 100
42 56.1 45.1 67.7
101 9.7 8.9 13.3
130 21.1 19.9 29.9


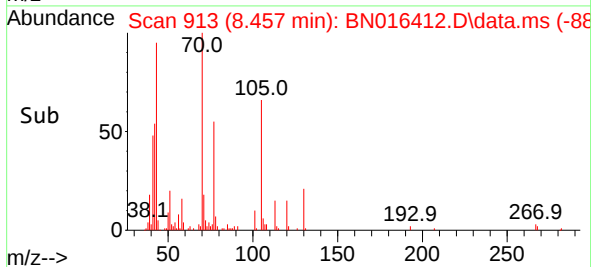

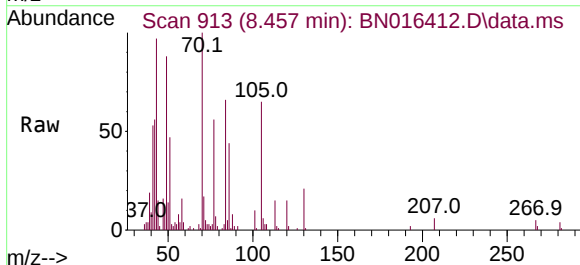




#18
4-Methylphenol
Concen: 4.506 ng/ul
RT: 8.422 min Scan# 907
Delta R.T. -0.006 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:108 Resp: 58165
Ion Ratio Lower Upper
108 100
107 112.9 87.0 130.4

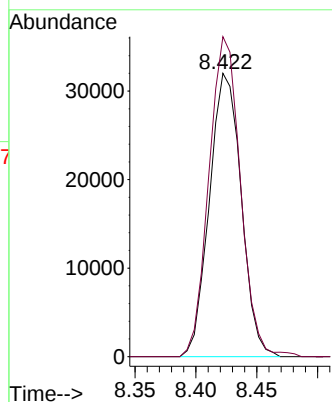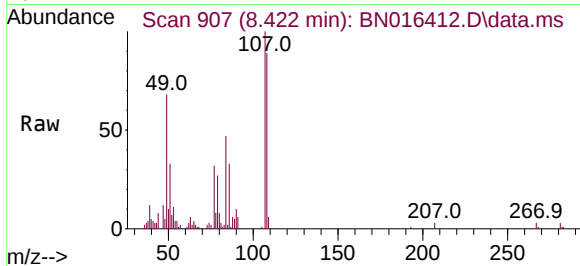

#19
Hexachloroethane
Concen: 4.671 ng/ul
RT: 8.722 min Scan# 958
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:117 Resp: 23826
Ion Ratio Lower Upper
117 100
201 92.1 82.6 123.8
199 57.5 52.0 78.0


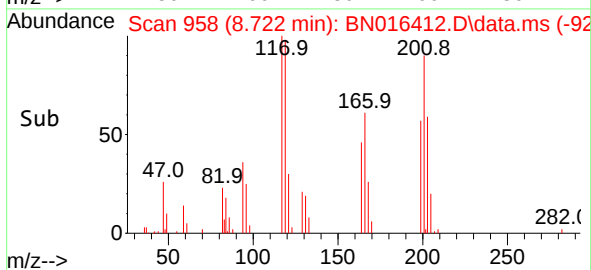

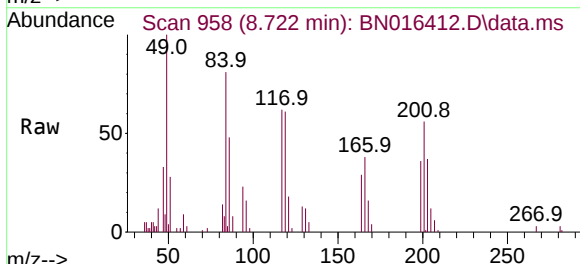




#22
Nitrobenzene
Concen: 4.722 ng/ul
RT: 8.846 min Scan# 979
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion: 77	Resp: 59598
Ion Ratio	Lower Upper
77 100	
123 45.6	41.1 61.7
65 12.8	11.0 16.6

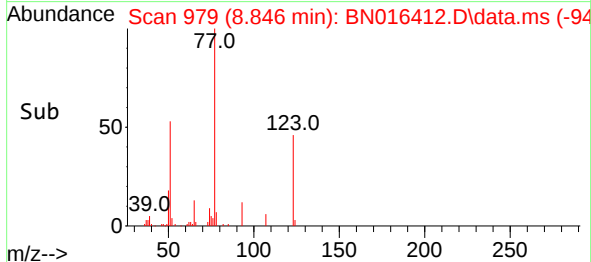

#23
Isophorone
Concen: 4.350 ng/ul
RT: 9.369 min Scan# 1068
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion: 82	Resp: 106670
Ion Ratio	Lower Upper
82 100	
95 6.1	6.1 9.1
138 18.4	15.8 23.8


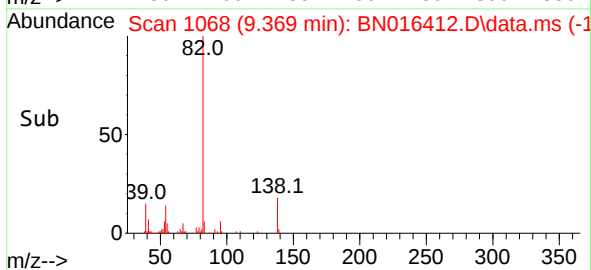




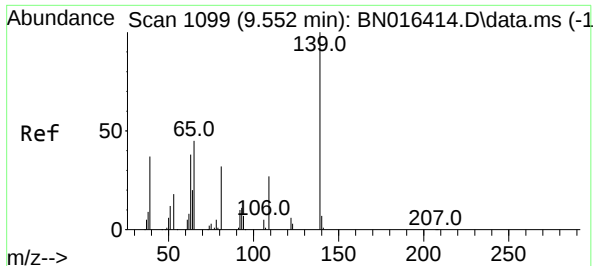

#25
2-Nitrophenol
Concen: 3.442 ng/ul
RT: 9.551 min Scan# 1099
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:139	Resp:	25484
Ion Ratio	Lower	Upper
139	100	
65	50.5	35.8 53.6
109	28.6	23.4 35.0

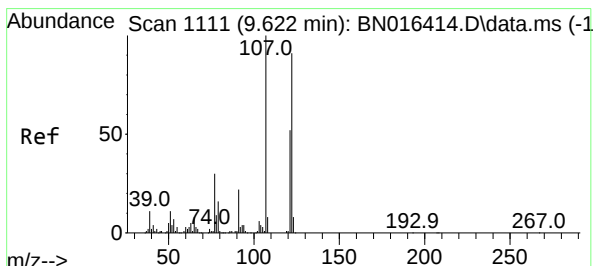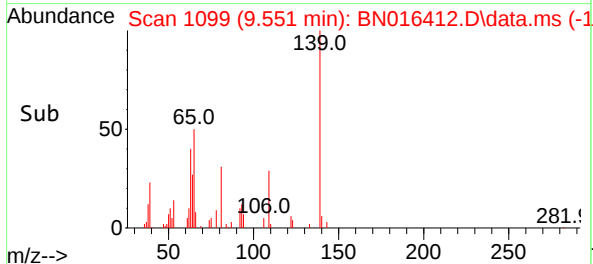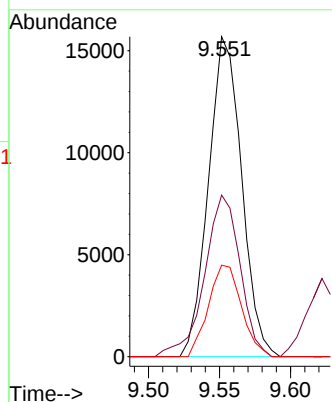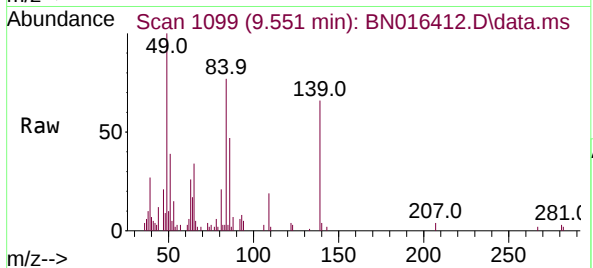

#26
2,4-Dimethylphenol
Concen: 4.516 ng/ul
RT: 9.622 min Scan# 1111
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:107	Resp:	62308
Ion Ratio	Lower	Upper
107	100	
121	54.2	41.8 62.8
122	88.5	71.1 106.7

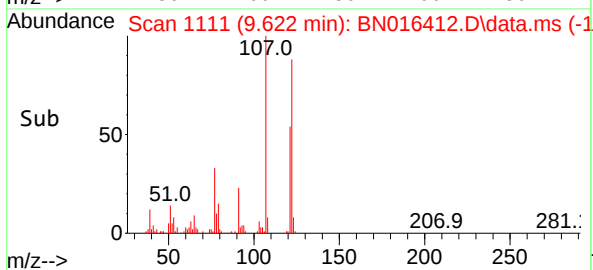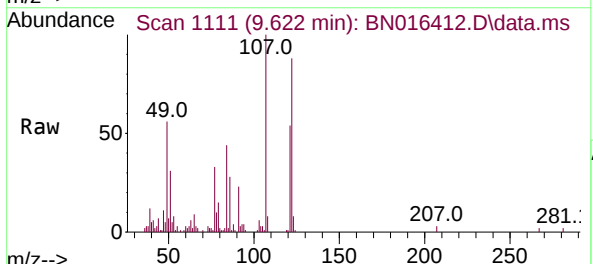




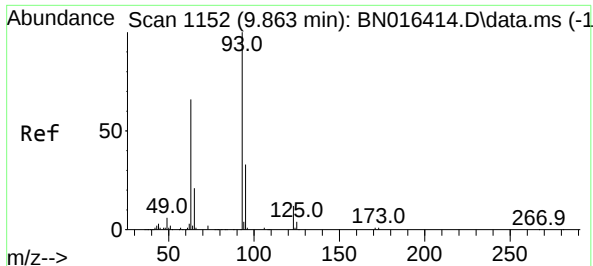


#27

Bis(2-Chloroethoxy)methane
Concen: 5.077 ng/ul
RT: 9.863 min Scan# 1152
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Instrument :
BNA_N
ClientSampleId :
SSTD005215




Tgt Ion:	93	Resp:	78819
Ion	Ratio	Lower	Upper
93	100		
95	32.8	24.9	37.3
123	11.0	9.4	14.0

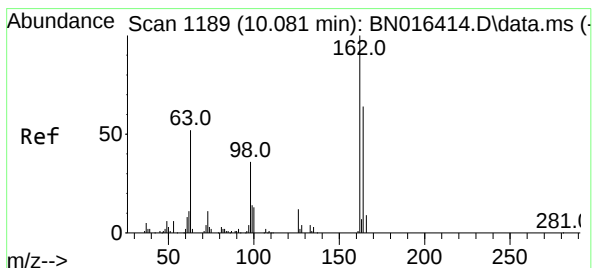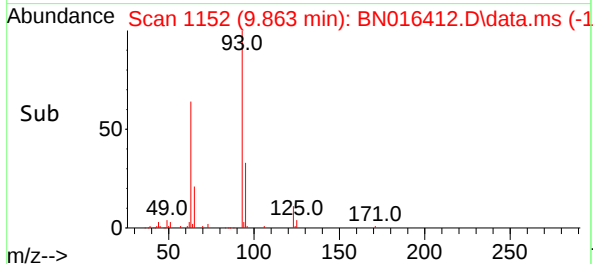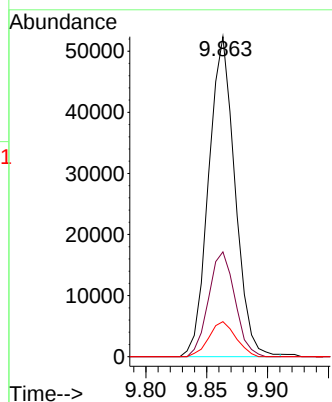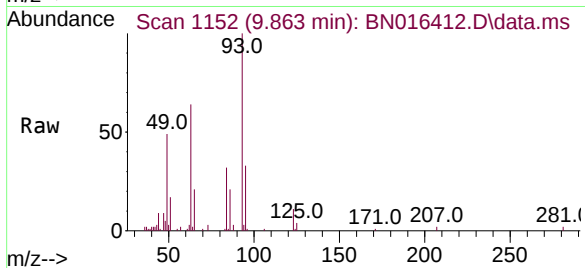


#29

2,4-Dichlorophenol
Concen: 4.173 ng/ul
RT: 10.081 min Scan# 1189
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:	162	Resp:	51940
Ion	Ratio	Lower	Upper
162	100		
164	64.6	51.7	77.5
98	36.0	26.3	39.5


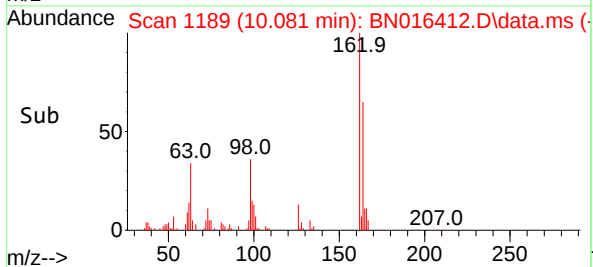

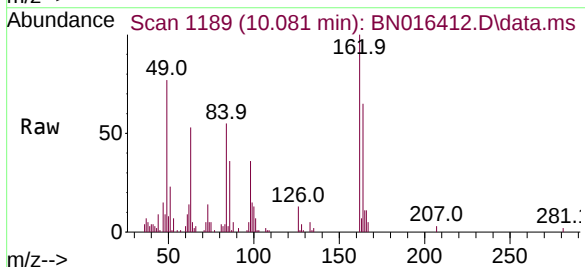




#30
Naphthalene
Concen: 4.991 ng/ul
RT: 10.481 min Scan# 1257
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:128 Resp: 206729
Ion Ratio Lower Upper
128 100
129 10.9 9.0 13.4
127 12.2 10.2 15.4



#32
4-Chloroaniline
Concen: 4.613 ng/ul
RT: 10.598 min Scan# 1277
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:127 Resp: 81457
Ion Ratio Lower Upper
127 100
129 32.6 25.8 38.8



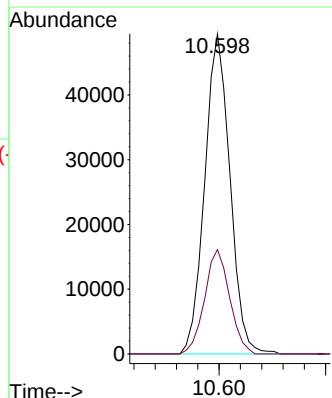





#33
Hexachlorobutadiene
Concen: 4.220 ng/ul
RT: 10.769 min Scan# 1306
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:	225	Resp:	35029
Ion Ratio	Lower	Upper	
225	100		
223	62.3	49.8	74.6
227	66.8	49.8	74.6

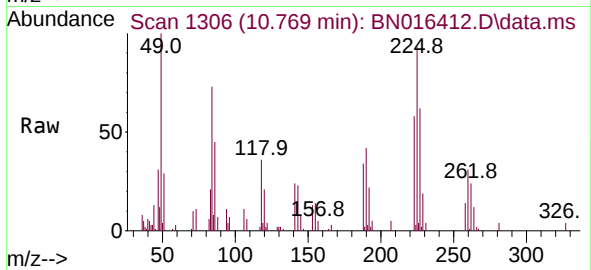

#34
Caprolactam
Concen: 2.799 ng/ul
RT: 11.351 min Scan# 1405
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:	113	Resp:	11841
Ion Ratio	Lower	Upper	
113	100		
55	157.9	123.8	185.8
56	115.7	89.4	134.2


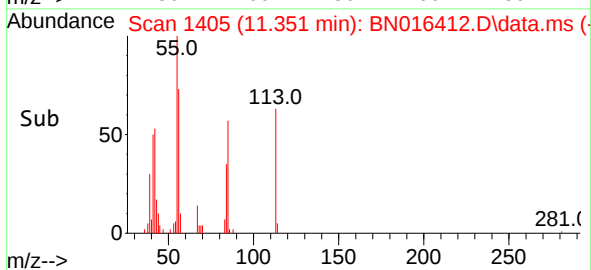

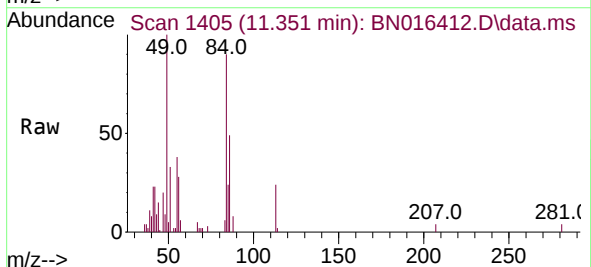




#35
4-Chloro-3-methylphenol
Concen: 4.050 ng/ul
RT: 11.728 min Scan# 1469
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:107 Resp: 52124
Ion Ratio Lower Upper
107 100
144 26.8 21.8 32.8
142 85.0 67.3 100.9



#36
2-Methylnaphthalene
Concen: 4.771 ng/ul
RT: 12.104 min Scan# 1533
Delta R.T. 0.006 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:142 Resp: 134759
Ion Ratio Lower Upper
142 100
141 90.3 71.3 106.9


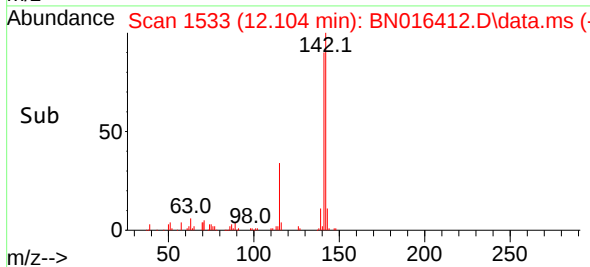




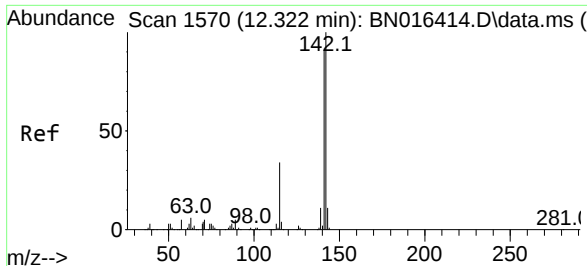

#37
1-Methylnaphthalene
Concen: 4.810 ng/ul
RT: 12.322 min Scan# 1570
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:142 Resp: 138894
Ion Ratio Lower Upper
142 100
141 94.2 71.9 107.9
116 3.6 2.7 4.1

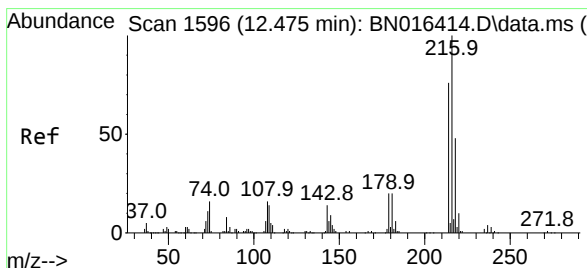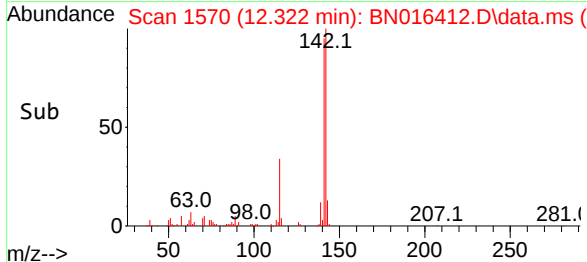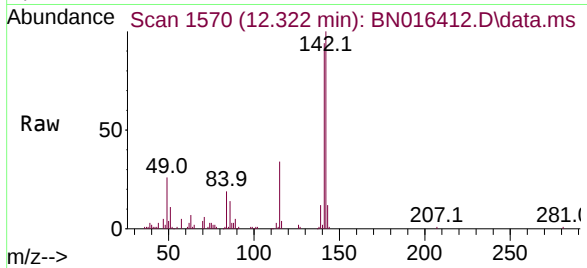

#39
1,2,4,5-Tetrachlorobenzene
Concen: 4.635 ng/ul
RT: 12.475 min Scan# 1596
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:216 Resp: 68345
Ion Ratio Lower Upper
216 100
214 81.9 61.8 92.6
179 22.0 15.8 23.8
108 17.3 11.4 17.0#


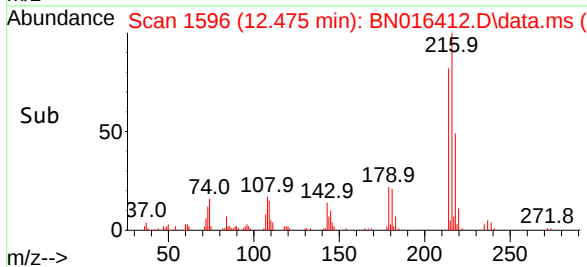
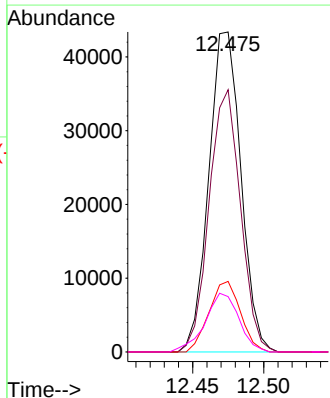
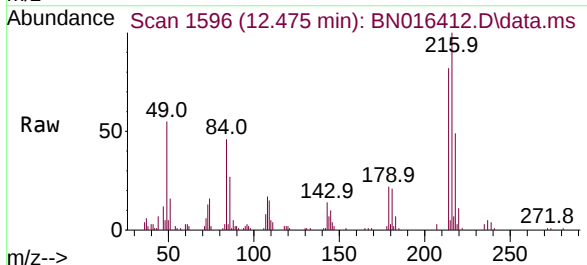




#40
Hexachlorocyclopentadiene
Concen: 4.141 ng/ul
RT: 12.451 min Scan# 1592
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:	237	Resp:	35010
Ion Ratio	Lower	Upper	
237	100		
235	66.4	52.7	79.1
272	12.7	11.8	17.8

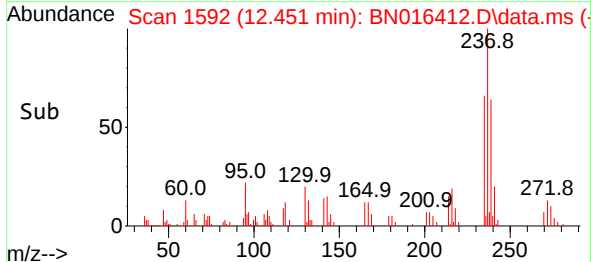

#41
2,4,6-Trichlorophenol
Concen: 4.009 ng/ul
RT: 12.716 min Scan# 1637
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:	196	Resp:	37885
Ion Ratio	Lower	Upper	
196	100		
198	88.7	75.2	112.8
200	29.1	24.2	36.4


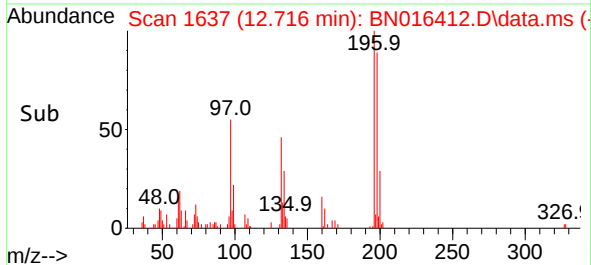

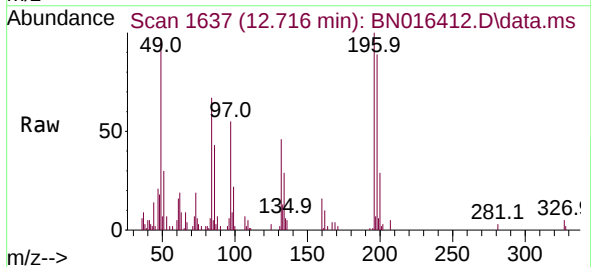




#42
2,4,5-Trichlorophenol
Concen: 4.028 ng/ul
RT: 12.787 min Scan# 1649
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:196 Resp: 41181
Ion Ratio Lower Upper
196 100
198 95.9 72.5 108.7
200 30.9 24.6 37.0



#43
1,1'-Biphenyl
Concen: 5.172 ng/ul
RT: 13.128 min Scan# 1707
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:154 Resp: 183301
Ion Ratio Lower Upper
154 100
153 41.1 32.1 48.1
76 13.5 9.1 13.7


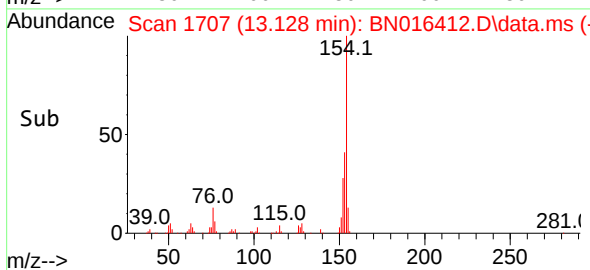






#44
2-Chloronaphthalene
Concen: 4.941 ng/ul
RT: 13.163 min Scan# 1713
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:162 Resp: 138818
Ion Ratio Lower Upper
162 100
164 32.9 26.2 39.4
127 39.5 30.1 45.1

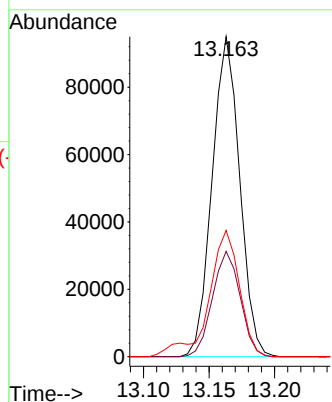

#45
2-Nitroaniline
Concen: 3.492 ng/ul
RT: 13.375 min Scan# 1749
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion: 65 Resp: 24943
Ion Ratio Lower Upper
65 100
92 75.8 57.8 86.8
138 114.8 99.6 149.4


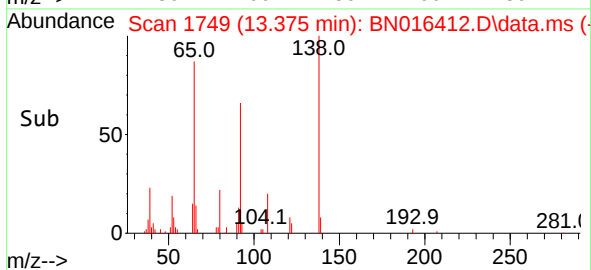






#47
Dimethylphthalate
Concen: 4.881 ng/ul
RT: 13.763 min Scan# 1815
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:163 Resp: 164506
Ion Ratio Lower Upper
163 100
194 4.4 3.3 4.9
164 10.1 8.2 12.4

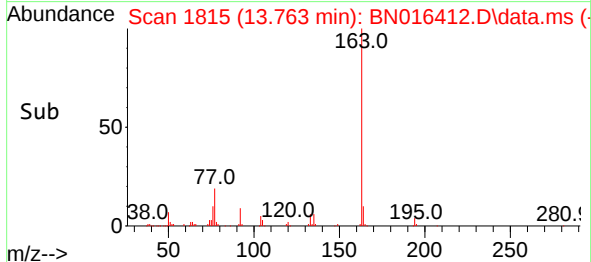

#48
2,6-Dinitrotoluene
Concen: 3.088 ng/ul
RT: 13.881 min Scan# 1835
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:165 Resp: 22075
Ion Ratio Lower Upper
165 100
89 62.2 35.6 53.4#
121 26.1 14.8 22.2#


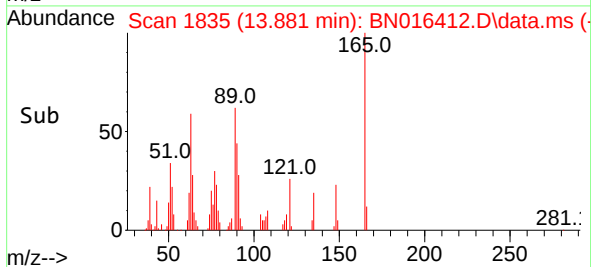

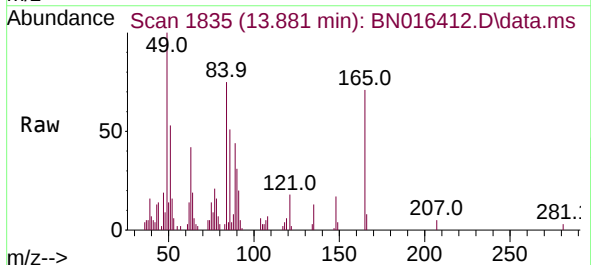




#50
Acenaphthylene
Concen: 4.767 ng/ul
RT: 14.016 min Scan# 1858
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:152 Resp: 217454
Ion Ratio Lower Upper
152 100
151 20.3 14.8 22.2
153 12.9 10.3 15.5

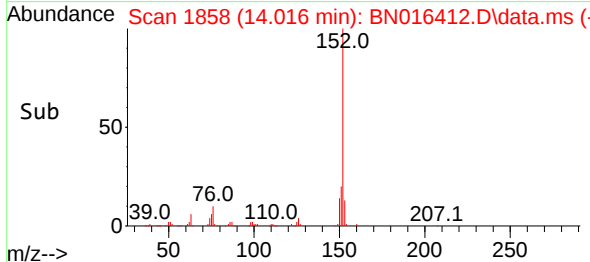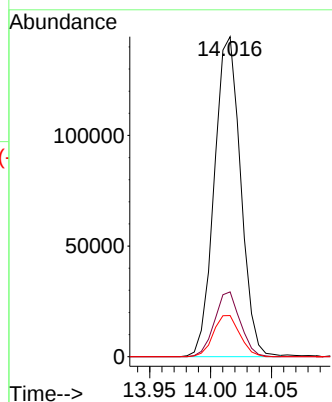

#51
3-Nitroaniline
Concen: 3.238 ng/ul
RT: 14.204 min Scan# 1890
Delta R.T. -0.006 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:138 Resp: 25628
Ion Ratio Lower Upper
138 100
108 11.5 9.0 13.4
92 122.5 82.3 123.5


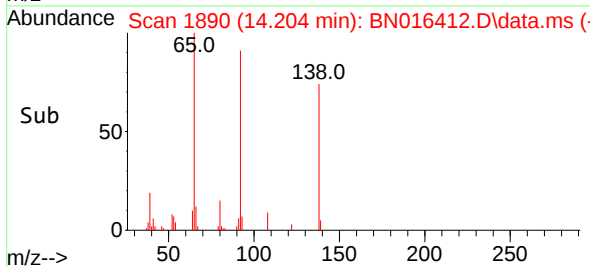






#52
Acenaphthene
Concen: 5.148 ng/ul
RT: 14.357 min Scan# 1916
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:153 Resp: 149855
Ion Ratio Lower Upper
153 100
152 47.2 36.6 54.8
154 85.9 70.9 106.3



#53
2,4-Dinitrophenol
Concen: 2.424 ng/ul
RT: 14.410 min Scan# 1925
Delta R.T. -0.006 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:184 Resp: 9282
Ion Ratio Lower Upper
184 100
63 68.1 45.2 67.8#
154 60.0 51.8 77.8


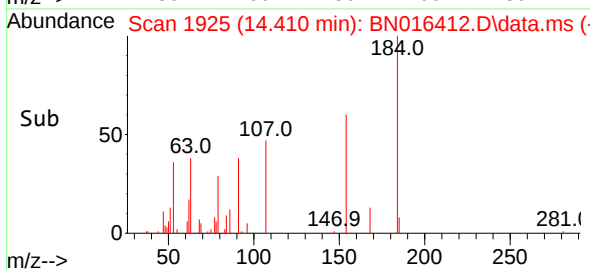






#55
4-Nitrophenol
Concen: 4.043 ng/ul
RT: 14.510 min Scan# 1942
Delta R.T. -0.006 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:109 Resp: 17551
Ion Ratio Lower Upper
109 100
139 139.2 129.5 194.3
65 136.9 109.0 163.4

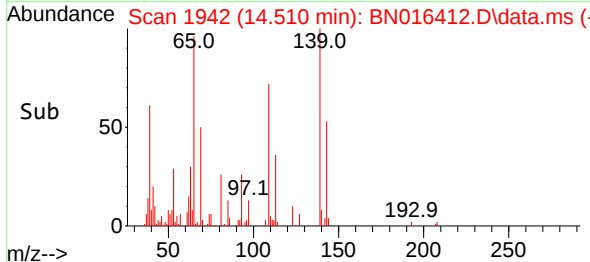

#56
Dibenzofuran
Concen: 5.083 ng/ul
RT: 14.698 min Scan# 1974
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:168 Resp: 213818
Ion Ratio Lower Upper
168 100
139 38.3 27.6 41.4



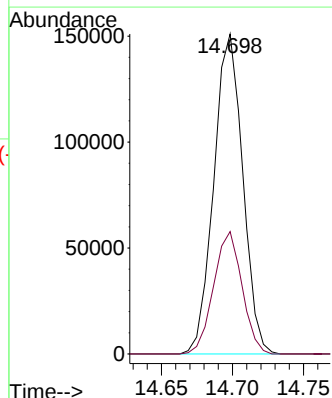





#57
2,4-Dinitrotoluene
Concen: 3.083 ng/ul
RT: 14.669 min Scan# 1969
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:165 Resp: 31767
Ion Ratio Lower Upper
165 100
63 43.0 30.4 45.6
182 3.1 2.5 3.7

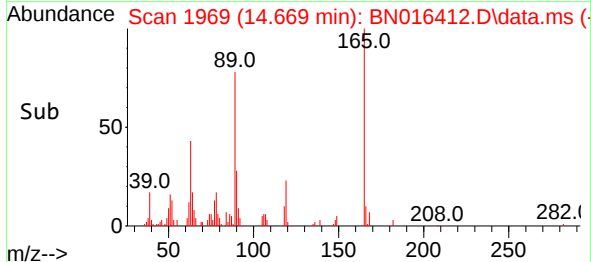

#58
2,3,4,6-Tetrachlorophenol
Concen: 3.792 ng/ul
RT: 14.928 min Scan# 2013
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:232 Resp: 31784
Ion Ratio Lower Upper
232 100
131 43.8 29.1 43.7#
130 2.0 1.7 2.5
166 29.7 21.6 32.4


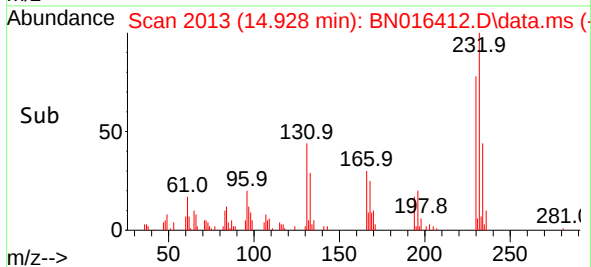

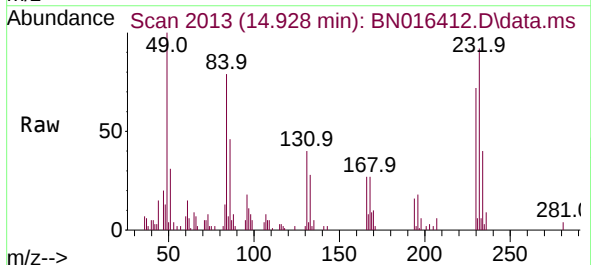




#59
Diethylphthalate
Concen: 5.093 ng/ul
RT: 15.139 min Scan# 2049
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:149 Resp: 169760
Ion Ratio Lower Upper
149 100
177 22.5 19.0 28.4
150 12.3 10.2 15.4



#61
Fluorene
Concen: 5.037 ng/ul
RT: 15.351 min Scan# 2085
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:166 Resp: 171007
Ion Ratio Lower Upper
166 100
165 100.5 74.8 112.2
167 13.1 10.6 15.8


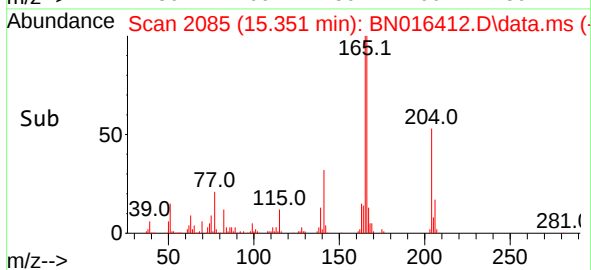






#62
4-Chlorophenyl-phenylether
Concen: 4.839 ng/ul
RT: 15.351 min Scan# 2085
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:204 Resp: 83498
Ion Ratio Lower Upper
204 100
206 31.8 27.6 41.4
141 61.3 45.5 68.3

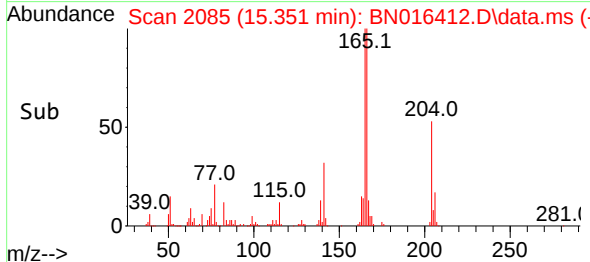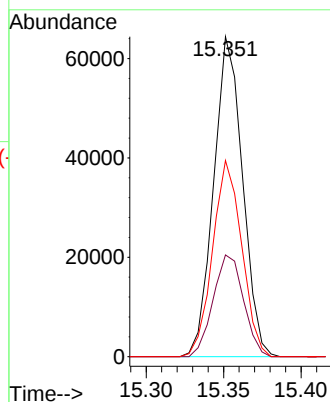

#63
4-Nitroaniline
Concen: 3.142 ng/ul
RT: 15.369 min Scan# 2088
Delta R.T. -0.006 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:138 Resp: 25860
Ion Ratio Lower Upper
138 100
92 56.5 35.5 53.3#
108 69.6 49.4 74.2


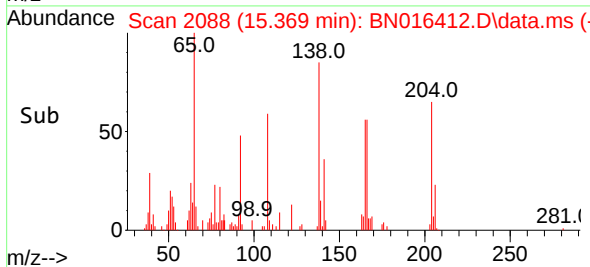






#66
4,6-Dinitro-2-methylphenol
Concen: 2.755 ng/ul
RT: 15.428 min Scan# 2098
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:198 Resp: 15438
Ion Ratio Lower Upper
198 100
182 8.1 4.2 6.4#
77 26.3 17.5 26.3#



#67
N-Nitrosodiphenylamine
Concen: 4.713 ng/ul
RT: 15.569 min Scan# 2122
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:169 Resp: 139245
Ion Ratio Lower Upper
169 100
168 64.5 51.6 77.4
167 34.9 27.1 40.7


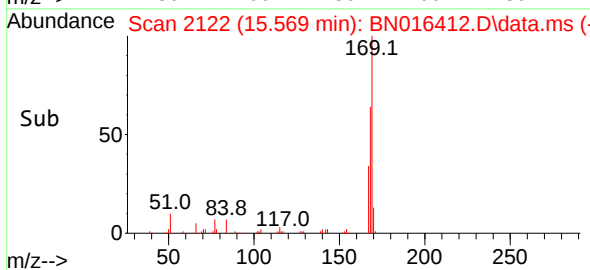




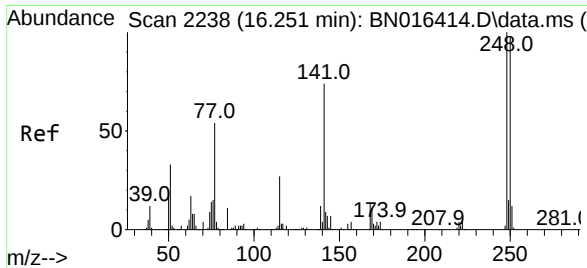

#68
4-Bromophenyl-phenylether
Concen: 4.547 ng/ul
RT: 16.251 min Scan# 2238
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:248 Resp: 48122
Ion Ratio Lower Upper
248 100
250 91.2 76.4 114.6
141 74.0 57.0 85.6

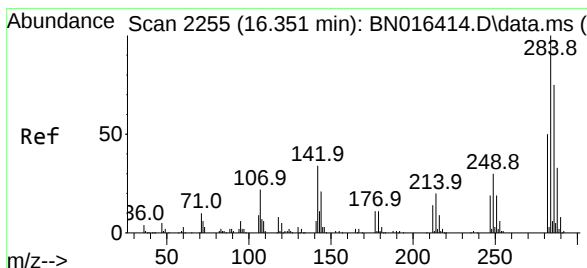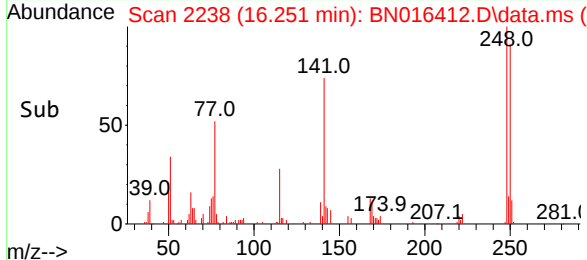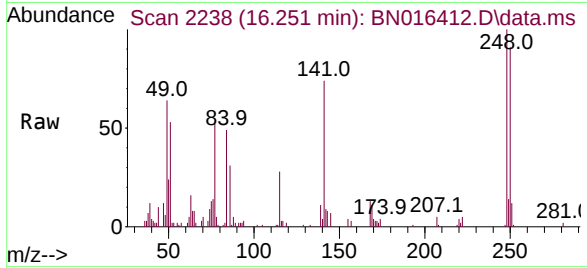

#69
Hexachlorobenzene
Concen: 4.424 ng/ul
RT: 16.351 min Scan# 2255
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:284 Resp: 54501
Ion Ratio Lower Upper
284 100
142 38.7 25.3 37.9#
249 32.3 24.3 36.5


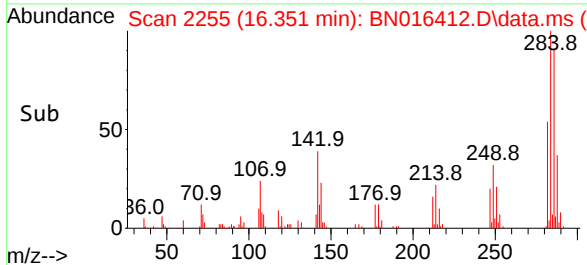

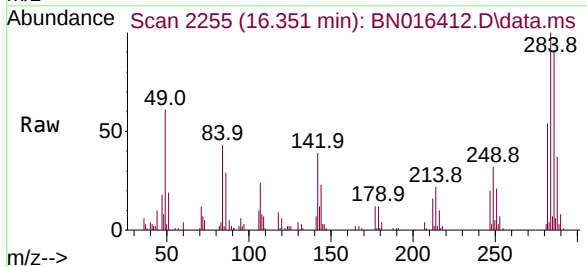


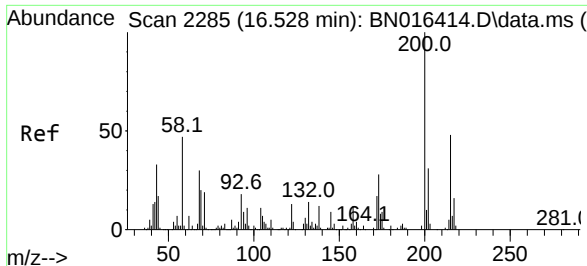

#70
Atrazine
Concen: 3.777 ng/ul
RT: 16.528 min Scan# 2285
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:200 Resp: 41870
Ion Ratio Lower Upper
200 100
173 27.3 22.6 34.0
215 46.2 42.0 63.0

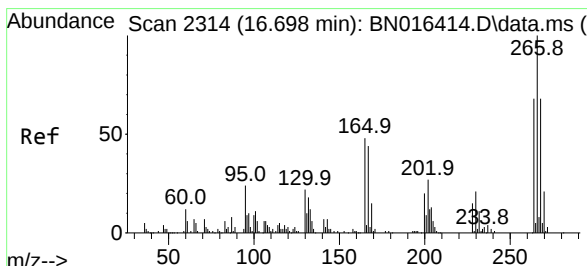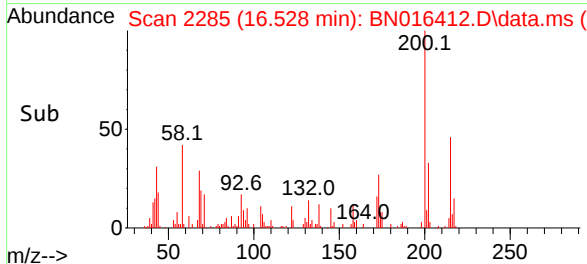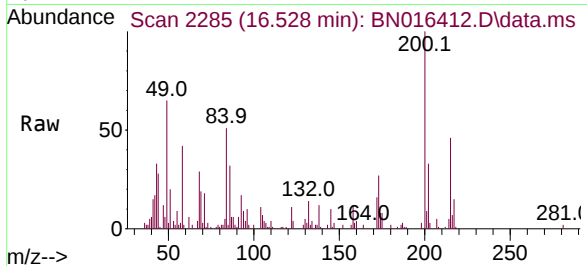

#71
Pentachlorophenol
Concen: 3.727 ng/ul
RT: 16.698 min Scan# 2314
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:266 Resp: 23423
Ion Ratio Lower Upper
266 100
264 56.0 50.7 76.1
268 65.7 49.8 74.6


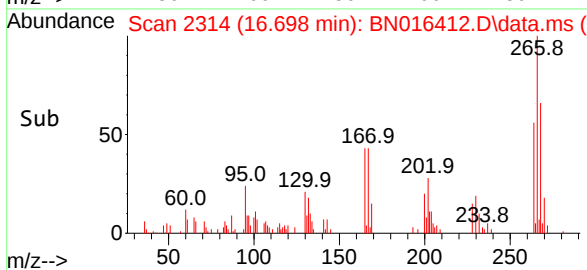

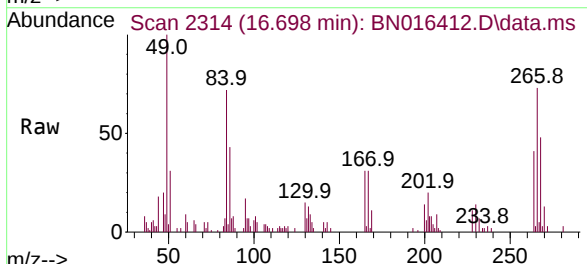


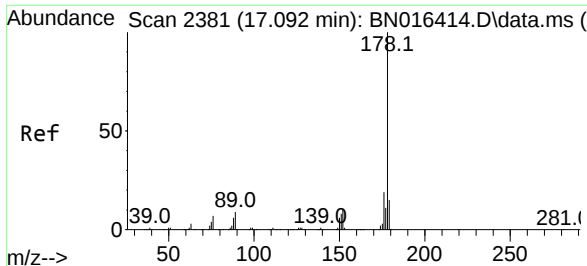

#72
Phenanthrene
Concen: 5.024 ng/ul
RT: 17.092 min Scan# 2381
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:178 Resp: 273364
Ion Ratio Lower Upper
178 100
179 15.0 12.2 18.2
176 18.0 14.7 22.1

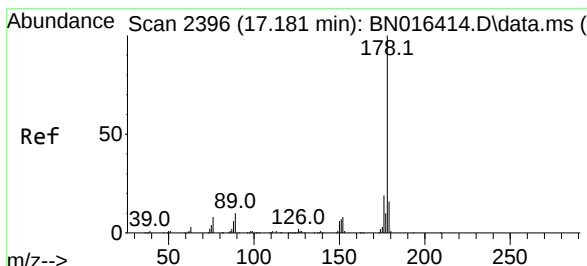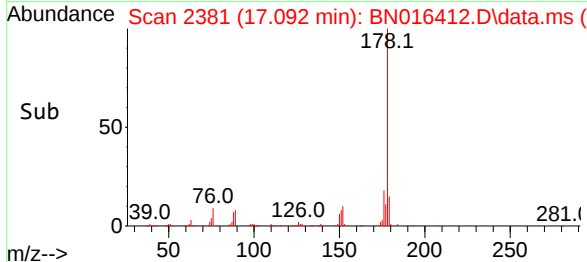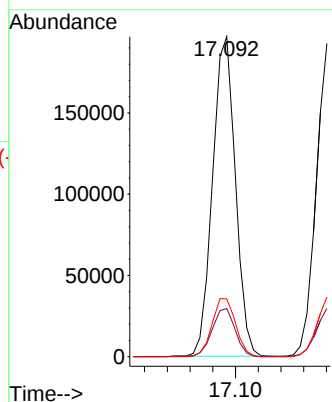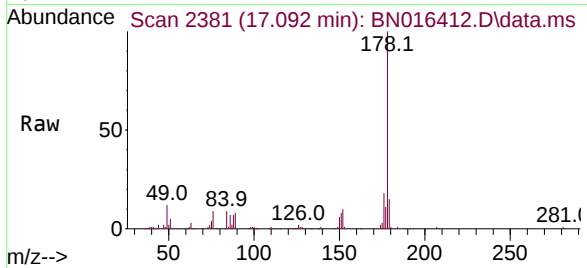

#74
Anthracene
Concen: 4.756 ng/ul
RT: 17.180 min Scan# 2396
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:178 Resp: 265948
Ion Ratio Lower Upper
178 100
179 15.4 12.4 18.6
176 19.0 14.2 21.4


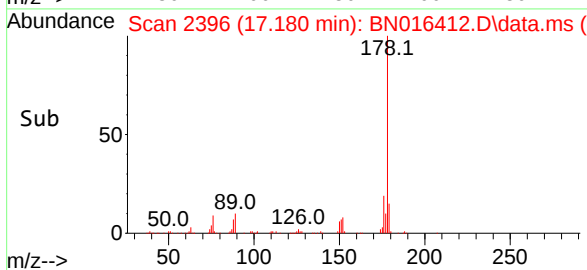

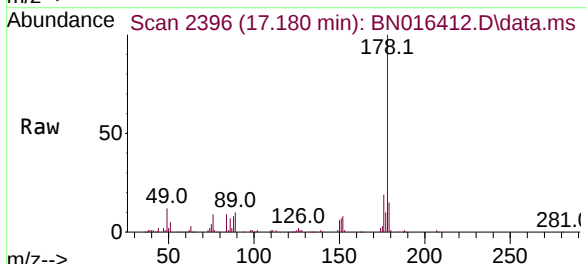




#75
1,2,3,4-Tetrachlorobenzene
Concen: 4.658 ng/uL
RT: 13.087 min Scan# 1700
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:	216	Resp:	71463
Ion Ratio	Lower	Upper	
216	100		
214	78.1	60.6	90.8
218	45.4	40.2	60.4

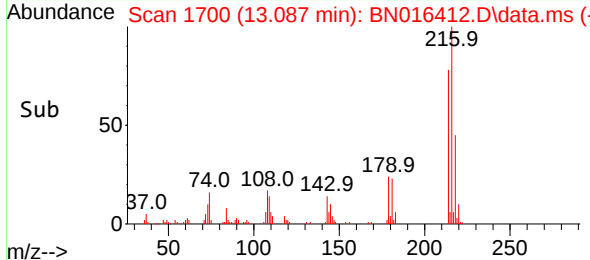

#76
Pentachlorobenzene
Concen: 4.621 ng/uL
RT: 14.616 min Scan# 1960
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:	250	Resp:	70139
Ion Ratio	Lower	Upper	
250	100		
248	65.7	51.1	76.7
252	68.6	52.1	78.1




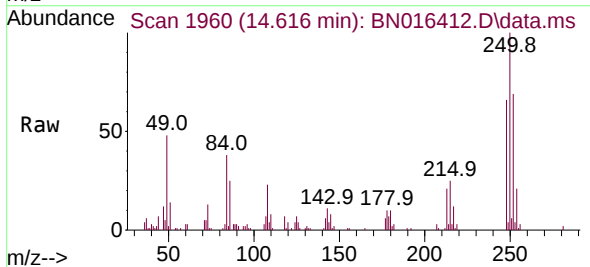


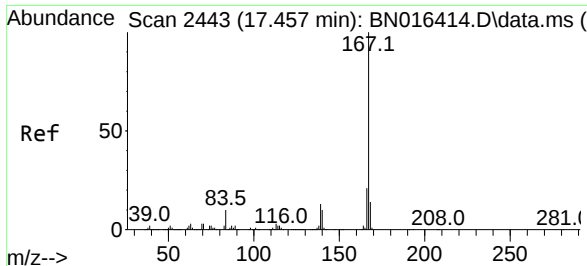

#77
 Carbazole
 Concen: 4.635 ng/ul
 RT: 17.457 min Scan# 2443
 Delta R.T. -0.000 min
 Lab File: BN016412.D
 Acq: 22 Sep 2021 16:42




Instrument :
 BNA_N
 ClientSampleId :
 SST005215


Tgt Ion:167 Resp: 230429
 Ion Ratio Lower Upper
 167 100
 166 20.4 16.8 25.2
 139 13.5 9.8 14.6

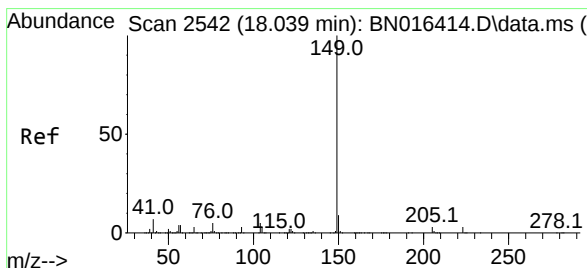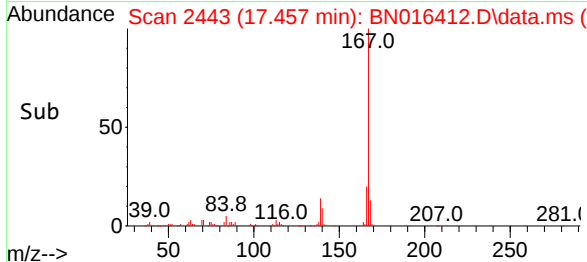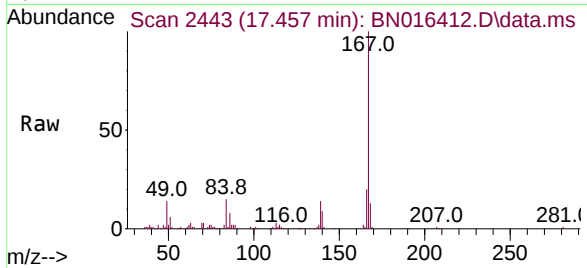

#78
 Di-n-butylphthalate
 Concen: 4.086 ng/ul
 RT: 18.039 min Scan# 2542
 Delta R.T. -0.000 min
 Lab File: BN016412.D
 Acq: 22 Sep 2021 16:42

Tgt Ion:149 Resp: 237690
 Ion Ratio Lower Upper
 149 100
 150 9.2 7.3 10.9
 104 5.1 3.5 5.3


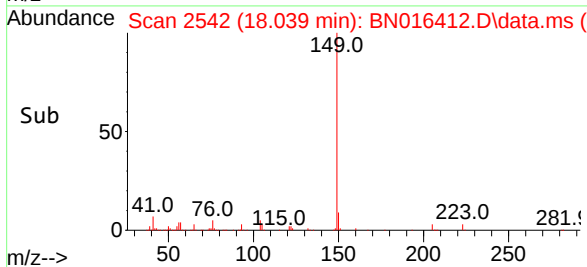

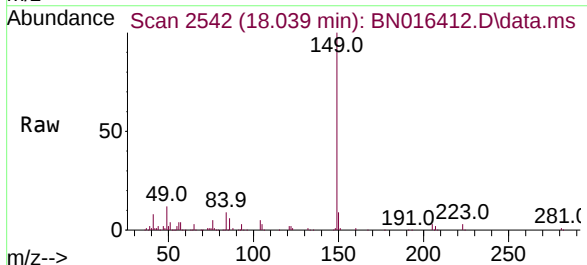




#80
 Fluoranthene
 Concen: 4.818 ng/ul
 RT: 19.116 min Scan# 2725
 Delta R.T. -0.000 min
 Lab File: BN016412.D
 Acq: 22 Sep 2021 16:42




Instrument :
 BNA_N
 ClientSampleId :
 SST005215


Tgt Ion:202 Resp: 297298
 Ion Ratio Lower Upper
 202 100
 101 12.5 8.7 13.1
 100 9.1 6.6 9.8

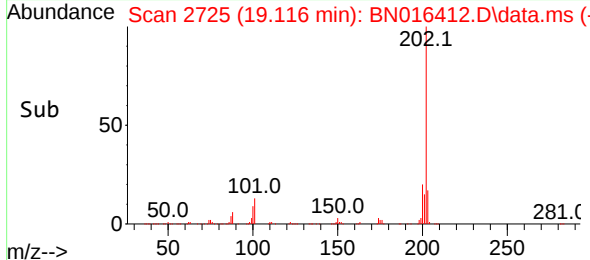

#82
 Pyrene
 Concen: 5.085 ng/ul
 RT: 19.480 min Scan# 2787
 Delta R.T. -0.000 min
 Lab File: BN016412.D
 Acq: 22 Sep 2021 16:42

Tgt Ion:202 Resp: 323218
 Ion Ratio Lower Upper
 202 100
 101 13.8 10.5 15.7
 100 11.3 8.6 13.0




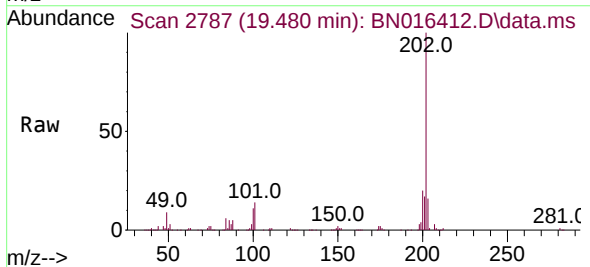




#83
Butylbenzylphthalate
Concen: 3.107 ng/ul
RT: 20.410 min Scan# 2945
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:149 Resp: 79177
Ion Ratio Lower Upper
149 100
91 71.4 50.6 76.0
206 22.1 18.5 27.7



#84
3,3'-Dichlorobenzidine
Concen: 3.766 ng/ul
RT: 21.180 min Scan# 3076
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:252 Resp: 80401
Ion Ratio Lower Upper
252 100
254 59.4 48.6 72.8
126 11.2 7.9 11.9


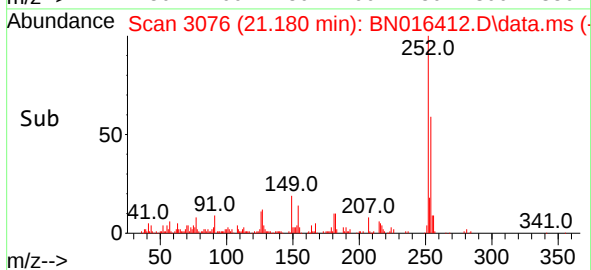






#85
Benzo(a)anthracene
Concen: 4.786 ng/ul
RT: 21.239 min Scan# 3086
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:228 Resp: 303295
Ion Ratio Lower Upper
228 100
229 18.8 15.7 23.5
226 26.1 20.6 31.0

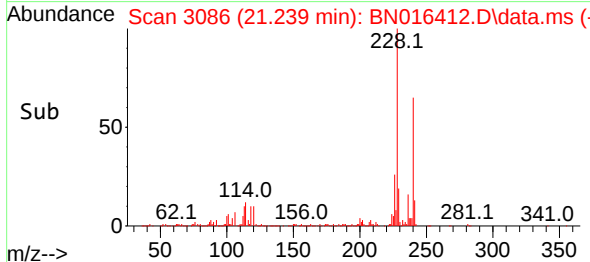

#86
Bis(2-ethylhexyl)phthalate
Concen: 3.668 ng/ul
RT: 21.192 min Scan# 3078
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:149 Resp: 136498
Ion Ratio Lower Upper
149 100
167 26.8 24.2 36.4
279 3.6 4.2 6.2#


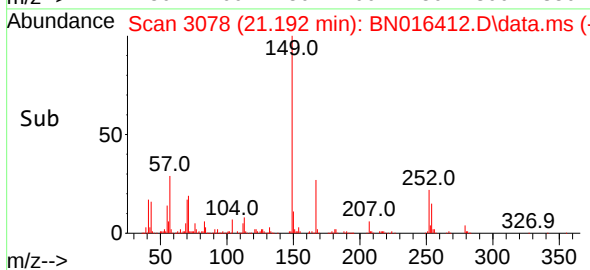






#87
Chrysene
Concen: 4.891 ng/ul
RT: 21.292 min Scan# 3095
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:228 Resp: 302116
Ion Ratio Lower Upper
228 100
226 31.2 23.4 35.0
229 19.2 14.9 22.3

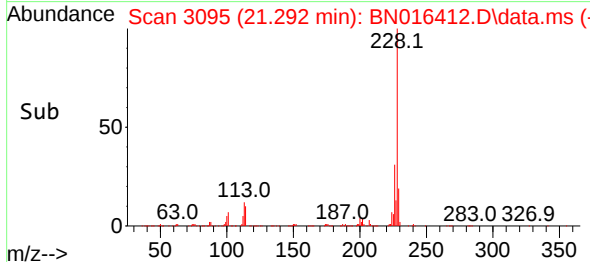

#89
Di-n-octyl phthalate
Concen: 3.002 ng/ul
RT: 22.086 min Scan# 3230
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:149 Resp: 190445


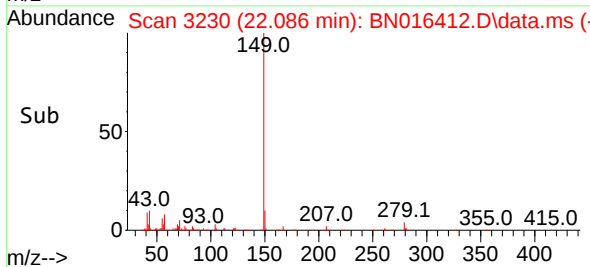






#90
Benzo(b)fluoranthene
Concen: 4.529 ng/ul
RT: 22.880 min Scan# 3365
Delta R.T. 0.041 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:252 Resp: 282113
Ion Ratio Lower Upper
252 100
253 21.9 17.6 26.4
125 11.3 7.8 11.8

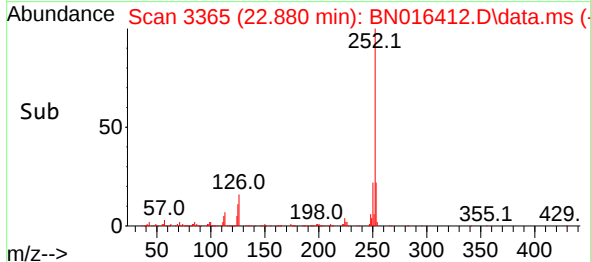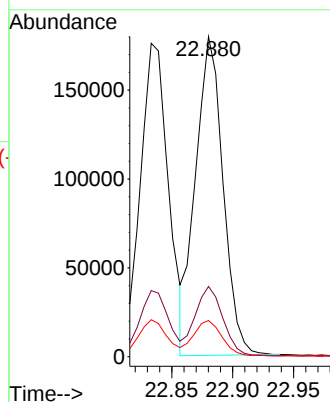

#91
Benzo(k)fluoranthene
Concen: 4.930 ng/ul
RT: 22.880 min Scan# 3365
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:252 Resp: 282113
Ion Ratio Lower Upper
252 100
253 21.9 17.0 25.4
125 11.3 7.8 11.6


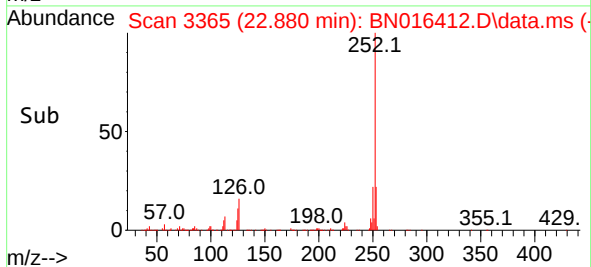

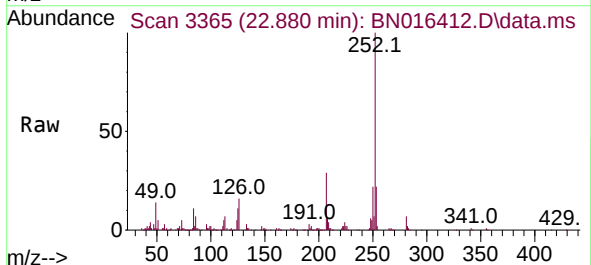




#93
Benzo(a)pyrene
Concen: 4.572 ng/ul
RT: 23.415 min Scan# 3456
Delta R.T. -0.000 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42




Instrument :
BNA_N
ClientSampleId :
SSTD005215


Tgt Ion:252 Resp: 275163
Ion Ratio Lower Upper
252 100
253 23.2 17.4 26.0
125 13.0 8.9 13.3

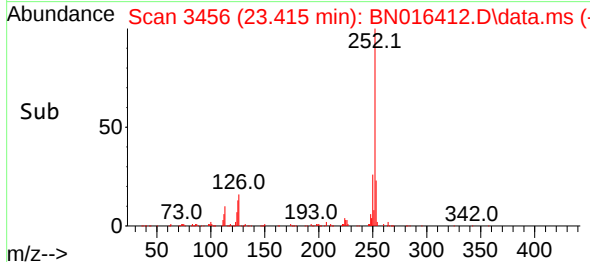

#94
Indeno(1,2,3-cd)pyrene
Concen: 3.807 ng/ul
RT: 26.504 min Scan# 3981
Delta R.T. -0.012 min
Lab File: BN016412.D
Acq: 22 Sep 2021 16:42

Tgt Ion:276 Resp: 258047
Ion Ratio Lower Upper
276 100
138 23.8 19.4 29.0
277 23.1 18.6 27.8


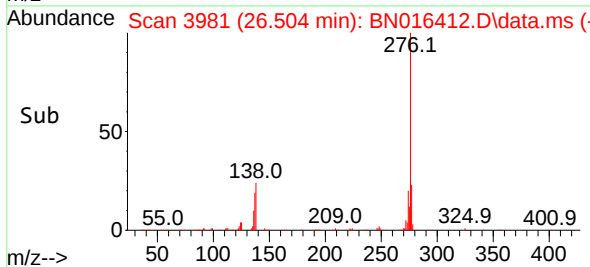




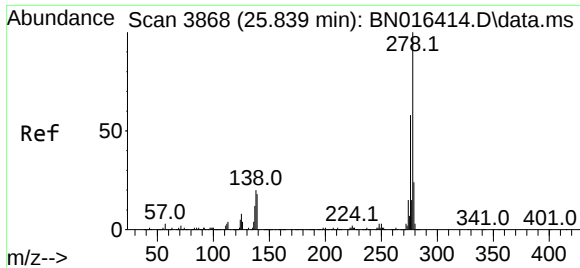

#95
 Dibenzo(a,h)anthracene
 Concen: 4.580 ng/ul
 RT: 25.833 min Scan# 3867
 Delta R.T. -0.006 min
 Lab File: BN016412.D
 Acq: 22 Sep 2021 16:42

Instrument :
 BNA_N
 ClientSampleId :
 SSTD005215

Tgt Ion:	278	Resp:	267179
Ion Ratio	Lower	Upper	
278	100		
139	18.5	12.2	18.4#
279	22.7	18.2	27.2

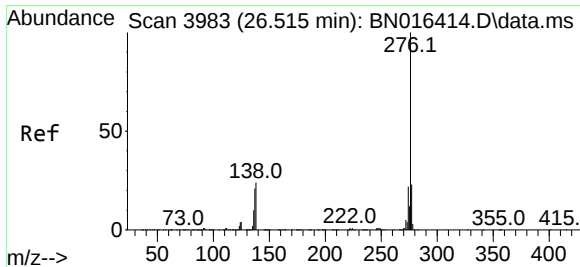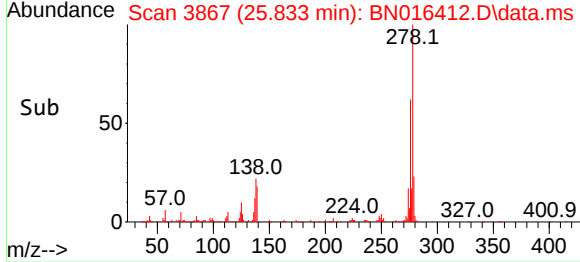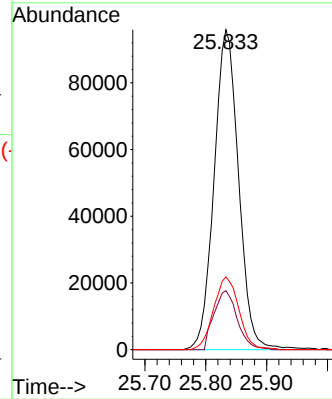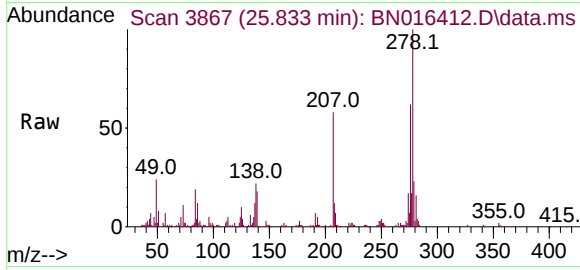

#96
 Benzo(g,h,i)perylene
 Concen: 4.492 ng/ul
 RT: 26.504 min Scan# 3981
 Delta R.T. -0.012 min
 Lab File: BN016412.D
 Acq: 22 Sep 2021 16:42

Tgt Ion:	276	Resp:	258047
Ion Ratio	Lower	Upper	
276	100		
138	23.8	17.4	26.0
277	23.1	18.4	27.6

