

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092821\
 Data File : BN016565.D
 Acq On : 28 Sep 2021 20:13
 Operator : CG/JU
 Sample : SSTDIC5.0
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDIC5.0

Quant Time: Sep 29 01:18:32 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN092821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 28 18:30:42 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.661	152	37073	0.400	ng	0.00
7) Naphthalene-d8	10.419	136	145053	0.400	ng	# 0.00
13) Acenaphthene-d10	14.281	164	75234	0.400	ng	0.00
19) Phenanthrene-d10	17.042	188	137044	0.400	ng	# 0.00
29) Chrysene-d12	21.249	240	126300	0.400	ng	# 0.00
35) Perylene-d12	23.509	264	122752	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.264	112	429910	5.698	ng	-0.02
5) Phenol-d6	6.840	99	462888	4.959	ng	0.00
8) Nitrobenzene-d5	8.797	82	480470	5.758	ng	0.00
11) 2-Methylnaphthalene-d10	12.016	152	1011851	4.954	ng	0.00
14) 2,4,6-Tribromophenol	15.779	330	196909	10.596	ng	0.00
15) 2-Fluorobiphenyl	12.911	172	1433013	4.104	ng	0.00
27) Fluoranthene-d10	19.078	212	1832563	4.784	ng	0.00
31) Terphenyl-d14	19.693	244	1433949	5.616	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.272	88	79801	4.663	ng	# 54
3) n-Nitrosodimethylamine	3.585	42	146516	4.457	ng	# 53
6) bis(2-Chloroethyl)ether	7.098	93	453703	4.604	ng	90
9) Naphthalene	10.470	128	1862840	4.608	ng	100
10) Hexachlorobutadiene	10.762	225	354331	4.170	ng	# 98
12) 2-Methylnaphthalene	12.092	142	1164288	4.906	ng	100
16) Acenaphthylene	14.002	152	1731492	4.999	ng	100
17) Acenaphthene	14.345	154	1099246	4.716	ng	# 89
18) Fluorene	15.335	166	1292249	4.617	ng	99
20) 4,6-Dinitro-2-methylph...	15.423	198	91609	11.651	ng	# 70
21) 4-Bromophenyl-phenylether	16.239	248	433215	5.097	ng	# 72
22) Hexachlorobenzene	16.348	284	460081	4.498	ng	95
23) Atrazine	16.519	200	345692	10.152	ng	98
24) Pentachlorophenol	16.689	266	233777	8.746	ng	99
25) Phenanthrene	17.078	178	1987265	4.459	ng	100
26) Anthracene	17.164	178	1870627	5.076	ng	100
28) Fluoranthene	19.108	202	2140278	4.398	ng	# 97
30) Pyrene	19.475	202	2245880	6.140	ng	99
32) Benzo(a)anthracene	21.227	228	2175247	6.492	ng	99
33) Chrysene	21.281	228	2075012	5.070	ng	99
34) Bis(2-ethylhexyl)phtha...	21.185	149	902308	14.397	ng	99
36) Indeno(1,2,3-cd)pyrene	25.798	276	2288389	5.931	ng	97
37) Benzo(b)fluoranthene	22.827	252	2192773	5.778	ng	99
38) Benzo(k)fluoranthene	22.872	252	2086820	4.713	ng	99
39) Benzo(a)pyrene	23.409	252	2001041	6.627	ng	99
40) Dibenzo(a,h)anthracene	25.822	278	1880529	5.485	ng	98
41) Benzo(g,h,i)perylene	26.504	276	1978921	6.254	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092821\
Data File : BN016565.D
Acq On : 28 Sep 2021 20:13
Operator : CG/JU
Sample : SSTDICC5.0
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Quant Time: Sep 29 01:18:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN092821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 28 18:30:42 2021
Response via : Initial Calibration




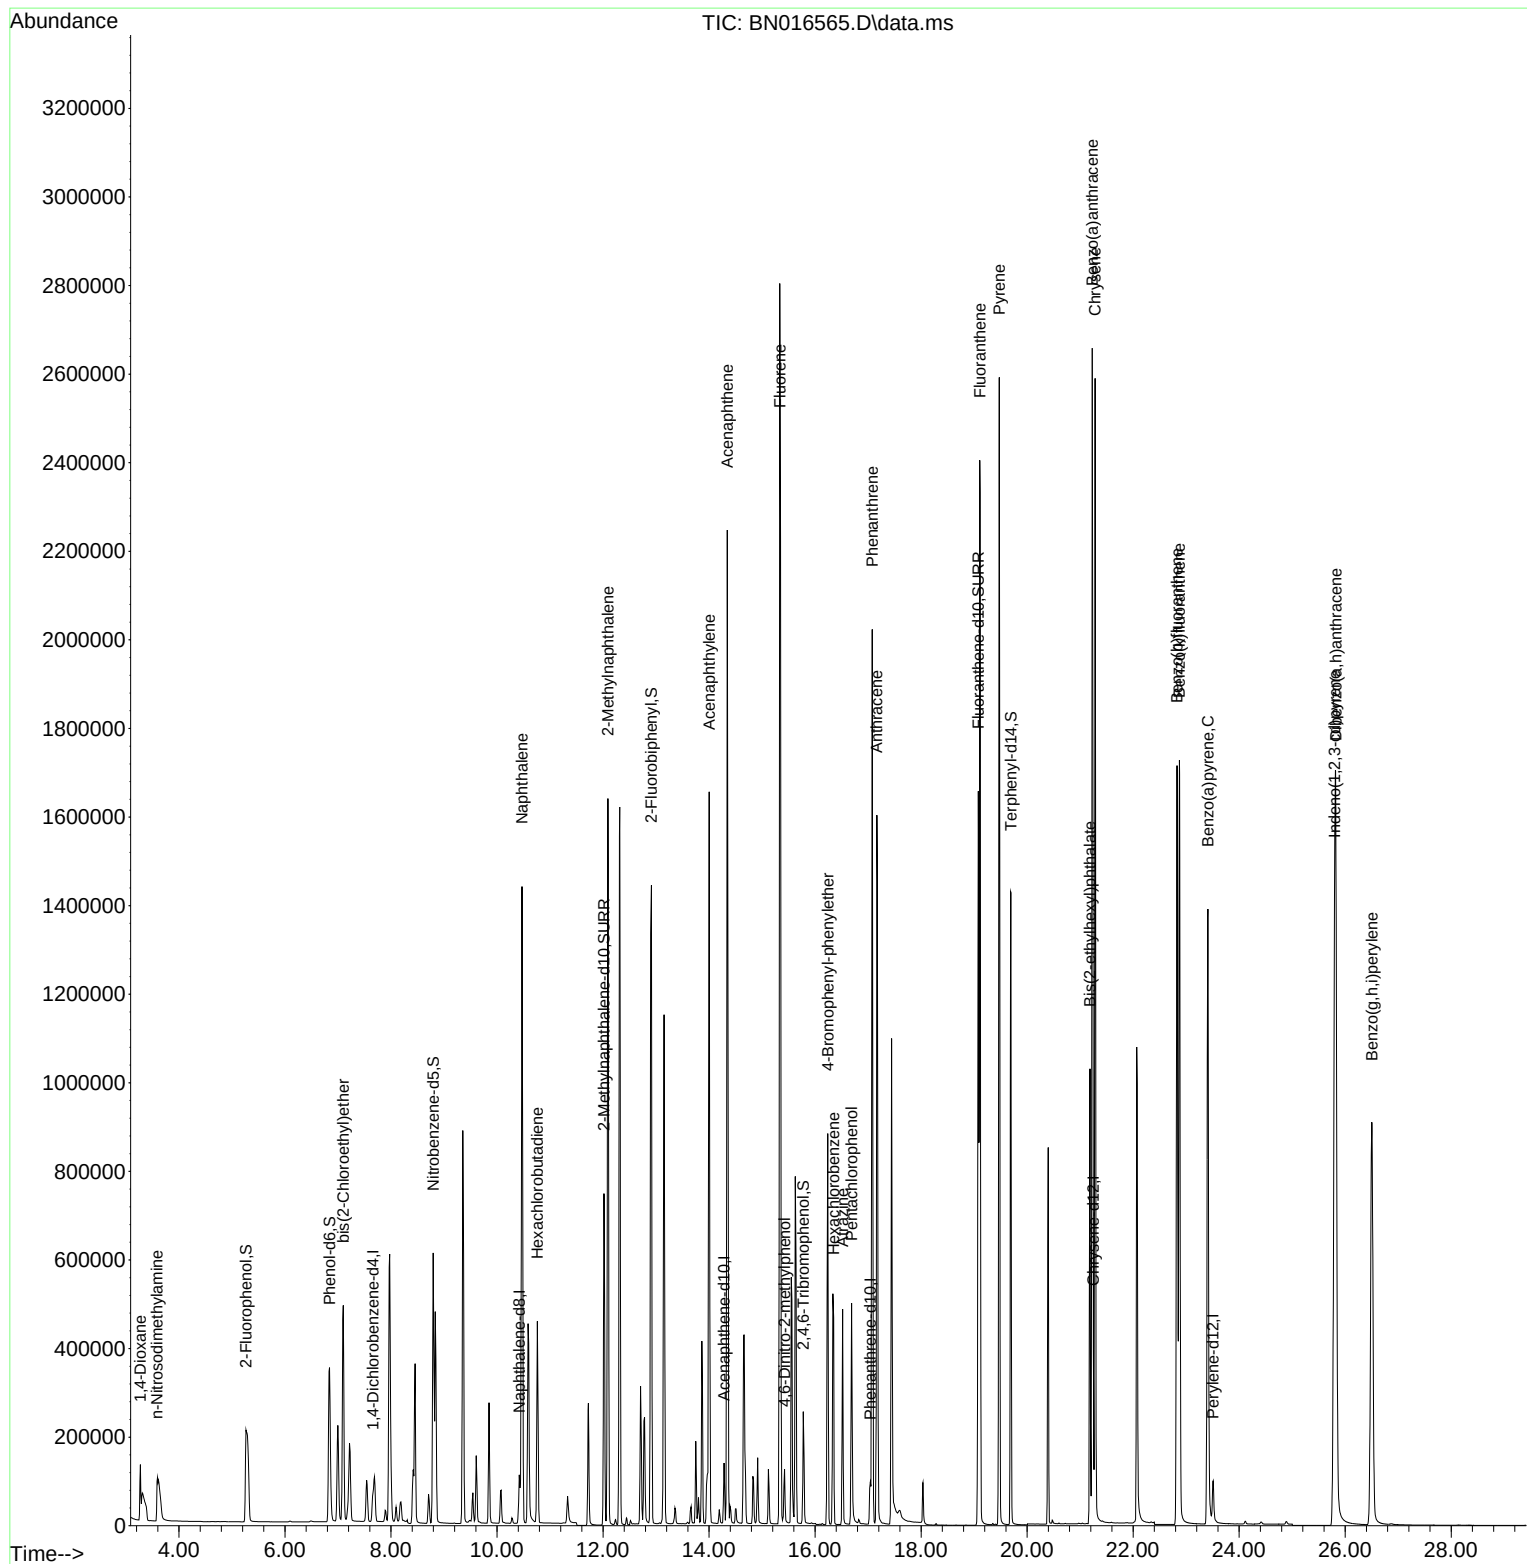




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.661 min Scan# 497
 Delta R.T. -0.000 min
 Lab File: BN016565.D
 Acq: 28 Sep 2021 20:13




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:152 Resp: 37073
 Ion Ratio Lower Upper
 152 100
 150 162.6 125.1 187.7
 115 57.7 45.8 68.8

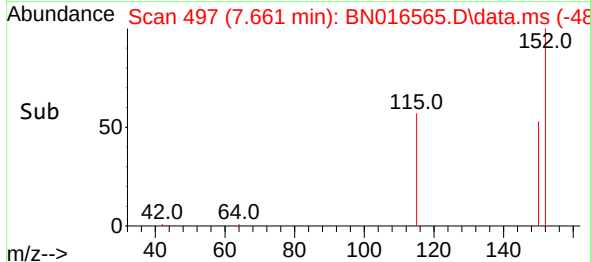

#2
 1,4-Dioxane
 Concen: 4.663 ng
 RT: 3.272 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN016565.D
 Acq: 28 Sep 2021 20:13

Tgt Ion: 88 Resp: 79801
 Ion Ratio Lower Upper
 88 100
 43 28.3 75.8 113.8#
 58 75.8 81.6 122.4#




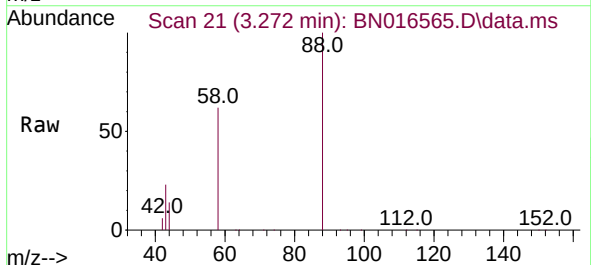


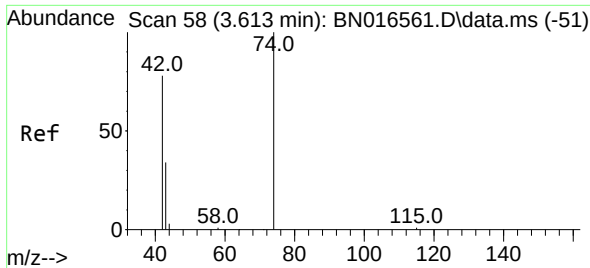

#3
n-Nitrosodimethylamine
Concen: 4.457 ng
RT: 3.585 min Scan# 55
Delta R.T. -0.028 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 42 Resp: 146516
Ion Ratio Lower Upper
42 100
74 143.2 77.5 116.3#
44 6.8 0.0 0.0#

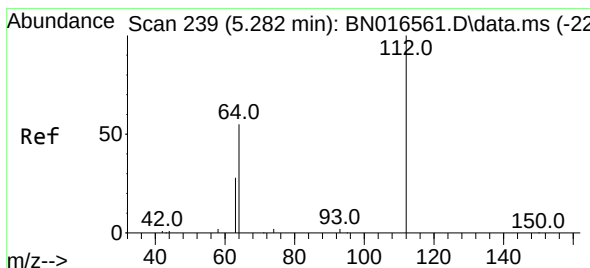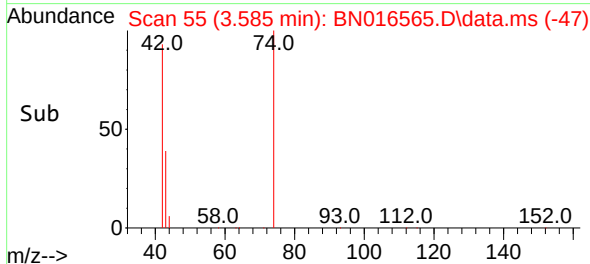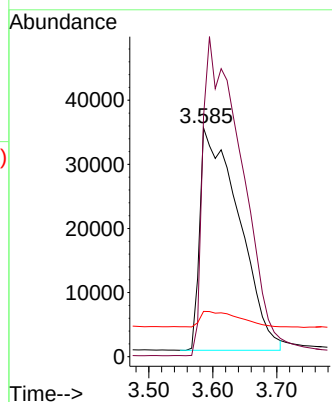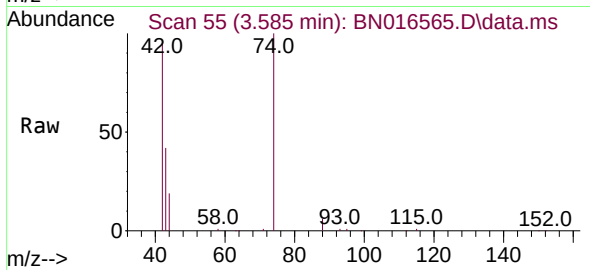

#4
2-Fluorophenol
Concen: 5.698 ng
RT: 5.264 min Scan# 237
Delta R.T. -0.019 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13

Tgt Ion: 112 Resp: 429910
Ion Ratio Lower Upper
112 100
64 54.9 48.4 72.6
63 27.8 25.4 38.2


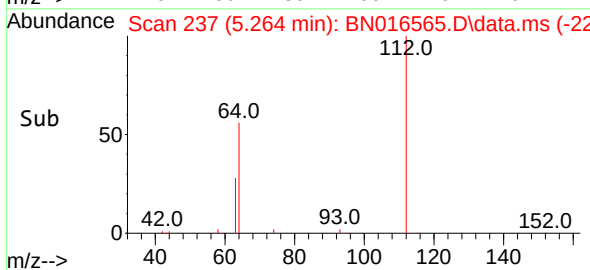
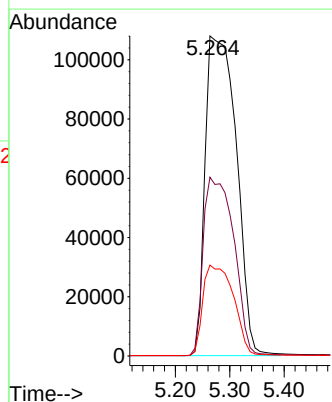
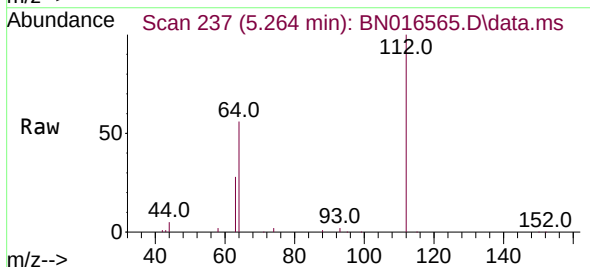


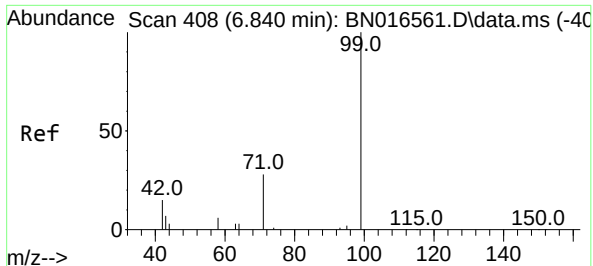

#5
Phenol-d6
Concen: 4.959 ng
RT: 6.840 min Scan# 408
Delta R.T. -0.000 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 99 Resp: 462888
Ion Ratio Lower Upper
99 100
42 17.4 19.6 29.4#
71 29.4 24.2 36.2

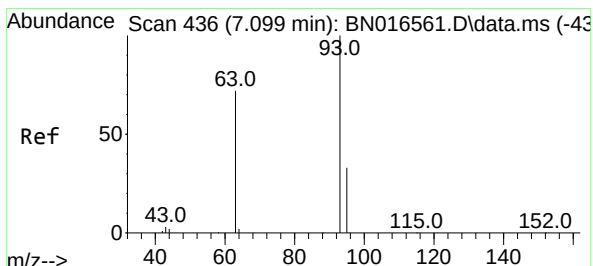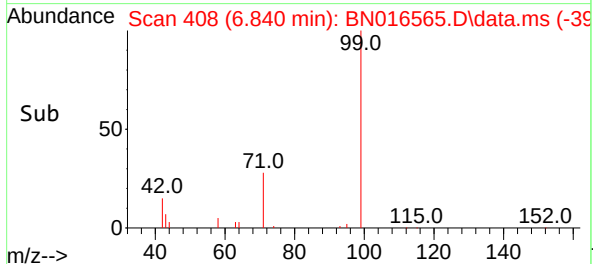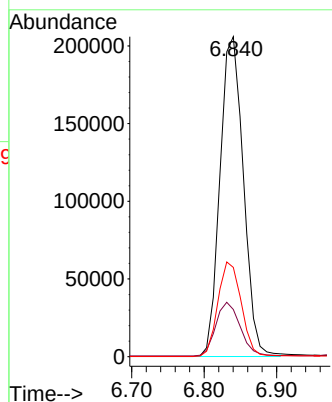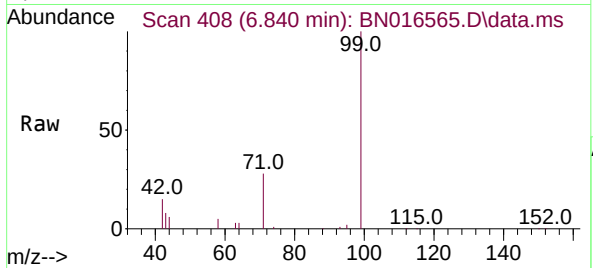

#6
bis(2-Chloroethyl)ether
Concen: 4.604 ng
RT: 7.098 min Scan# 436
Delta R.T. -0.000 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13

Tgt Ion: 93 Resp: 453703
Ion Ratio Lower Upper
93 100
63 74.9 70.0 105.0
95 32.6 26.3 39.5


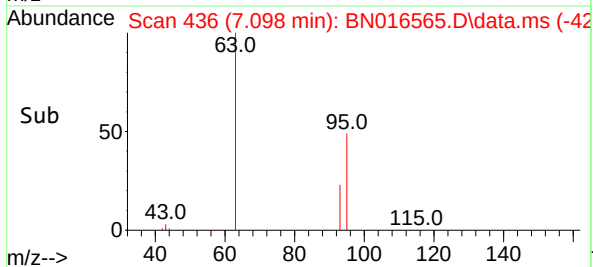

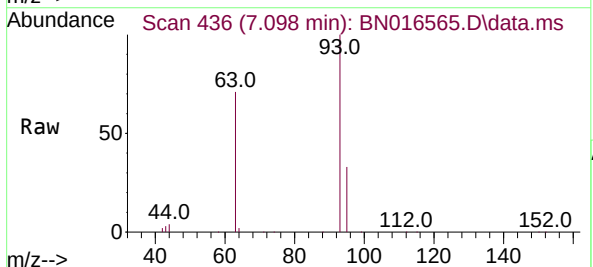




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.419 min Scan# 734
Delta R.T. -0.000 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	136	Resp:	145053
Ion Ratio	Lower	Upper	
136	100		
137	11.0	8.8	13.2
54	8.2	5.8	8.6
68	6.6	3.6	5.4

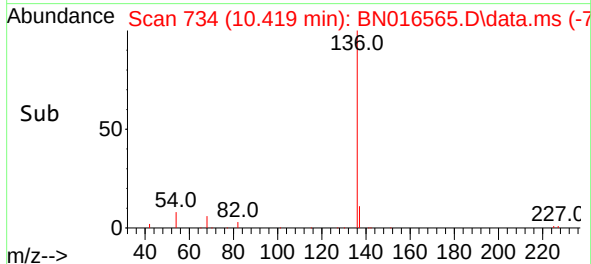

#8
Nitrobenzene-d5
Concen: 5.758 ng
RT: 8.797 min Scan# 606
Delta R.T. -0.000 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13

Tgt Ion:	82	Resp:	480470
Ion Ratio	Lower	Upper	
82	100		
128	42.8	27.4	41.2
54	48.1	58.5	87.7


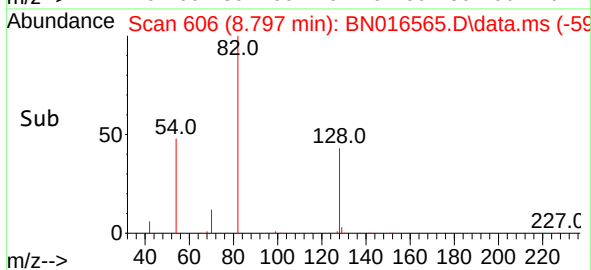






#9
Naphthalene
Concen: 4.608 ng
RT: 10.470 min Scan# 738
Delta R.T. -0.000 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:128 Resp: 1862840
Ion Ratio Lower Upper
128 100
129 11.1 8.9 13.3
127 12.7 10.1 15.1

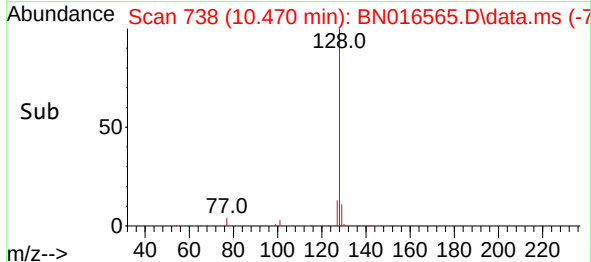

#10
Hexachlorobutadiene
Concen: 4.170 ng
RT: 10.762 min Scan# 761
Delta R.T. -0.000 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13

Tgt Ion:225 Resp: 354331
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.3 50.4 75.6







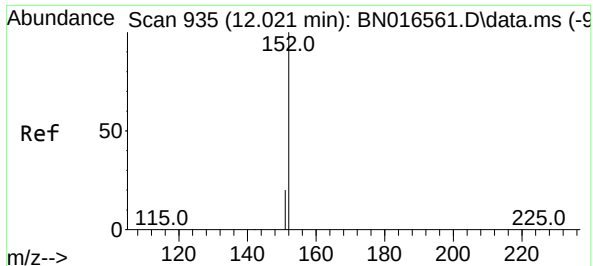

#11
2-Methylnaphthalene-d10
Concen: 4.954 ng
RT: 12.016 min Scan# 934
Delta R.T. -0.005 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:152 Resp: 1011851
Ion Ratio Lower Upper
152 100
151 20.1 16.6 25.0

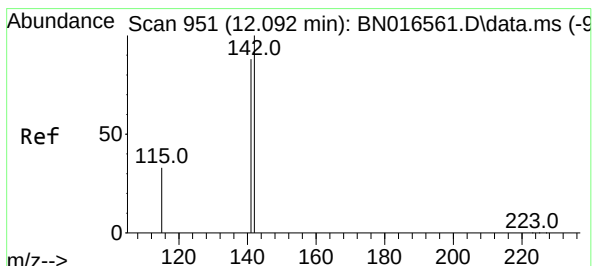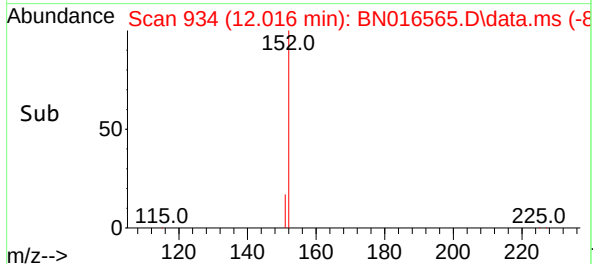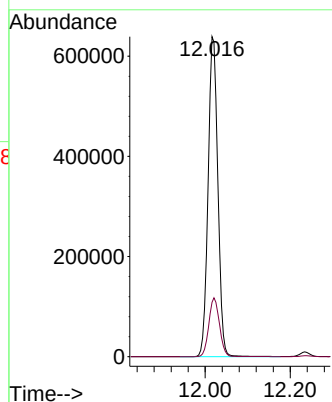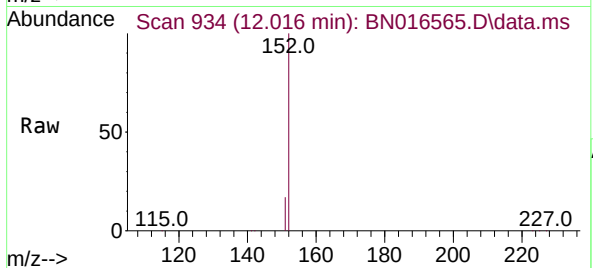

#12
2-Methylnaphthalene
Concen: 4.906 ng
RT: 12.092 min Scan# 951
Delta R.T. -0.000 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13

Tgt Ion:142 Resp: 1164288
Ion Ratio Lower Upper
142 100
141 87.5 69.9 104.9
115 33.0 27.0 40.4


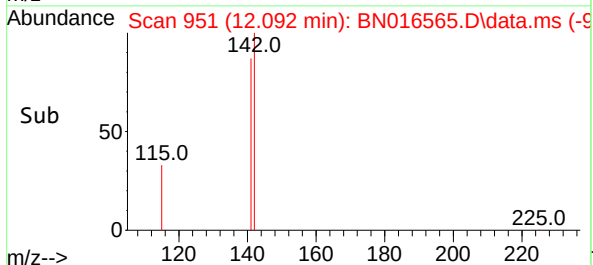

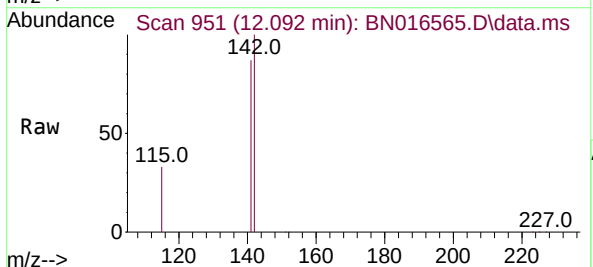




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.281 min Scan# 1184
Delta R.T. -0.000 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:164 Resp: 75234
Ion Ratio Lower Upper
164 100
162 102.2 79.4 119.0
160 47.1 46.6 70.0

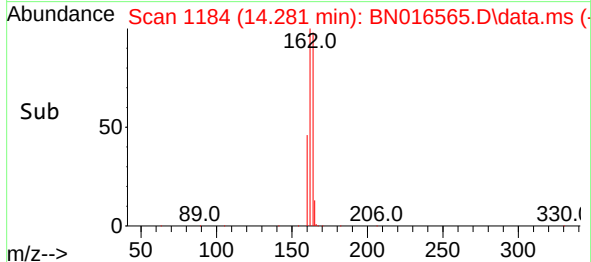

#14
2,4,6-Tribromophenol
Concen: 10.596 ng
RT: 15.779 min Scan# 1302
Delta R.T. -0.000 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13

Tgt Ion:330 Resp: 196909
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 34.1 34.4 51.6#


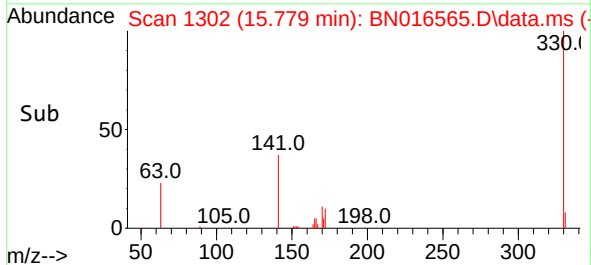






#15
2-Fluorobiphenyl
Concen: 4.104 ng
RT: 12.911 min Scan# 1076
Delta R.T. -0.000 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:172 Resp: 1433013
Ion Ratio Lower Upper
172 100
171 32.9 27.4 41.2
170 21.5 18.9 28.3

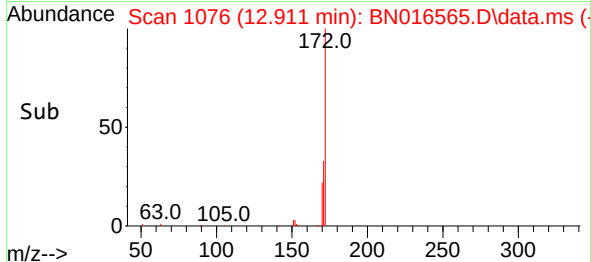

#16
Acenaphthylene
Concen: 4.999 ng
RT: 14.002 min Scan# 1162
Delta R.T. -0.000 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13

Tgt Ion:152 Resp: 1731492
Ion Ratio Lower Upper
152 100
151 19.3 15.4 23.0
153 13.2 10.4 15.6




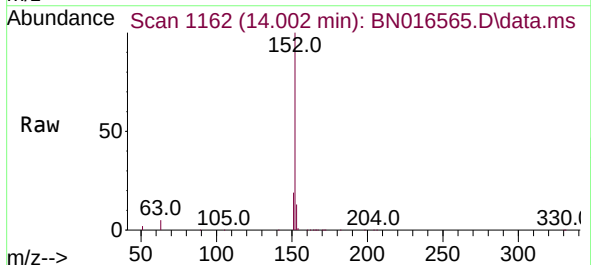


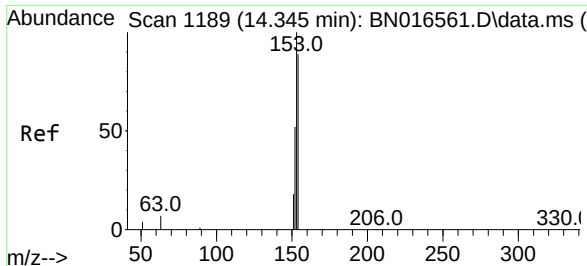

#17
Acenaphthene
Concen: 4.716 ng
RT: 14.345 min Scan# 1189
Delta R.T. -0.000 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:154 Resp: 1099246
Ion Ratio Lower Upper
154 100
153 108.7 91.0 136.4
152 52.4 55.8 83.6#

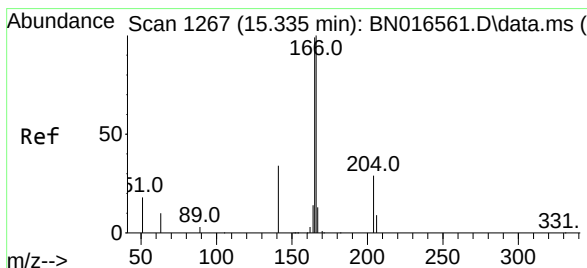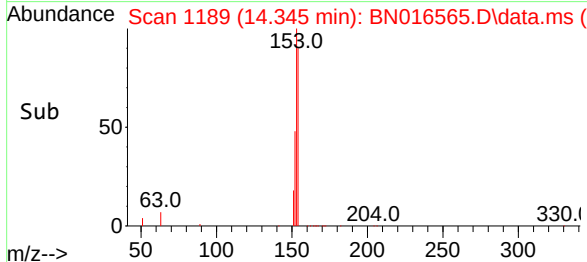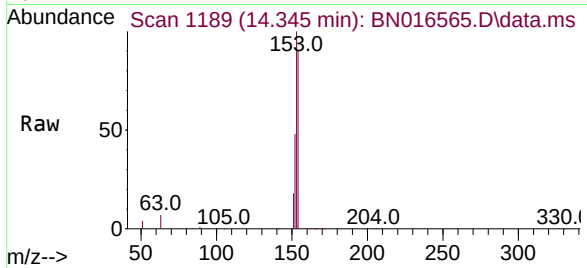

#18
Fluorene
Concen: 4.617 ng
RT: 15.335 min Scan# 1267
Delta R.T. -0.000 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13

Tgt Ion:166 Resp: 1292249
Ion Ratio Lower Upper
166 100
165 96.0 77.6 116.4
167 13.6 10.7 16.1


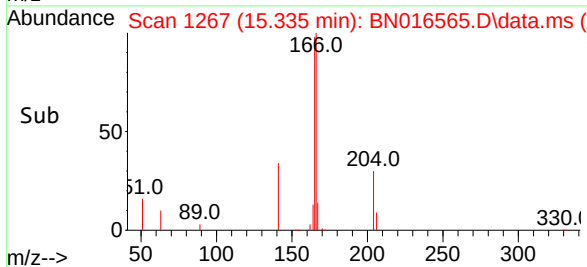

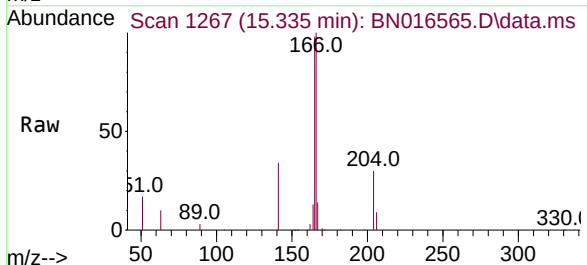




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.042 min Scan# 1405
Delta R.T. -0.000 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:188 Resp: 137044
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 6.8 6.9 10.3#

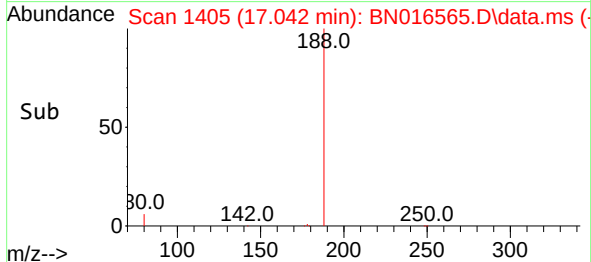

#20
4,6-Dinitro-2-methylphenol
Concen: 11.651 ng
RT: 15.423 min Scan# 1274
Delta R.T. -0.013 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13

Tgt Ion:198 Resp: 91609
Ion Ratio Lower Upper
198 100
182 7.8 17.5 26.3#
77 0.0 0.0 0.0




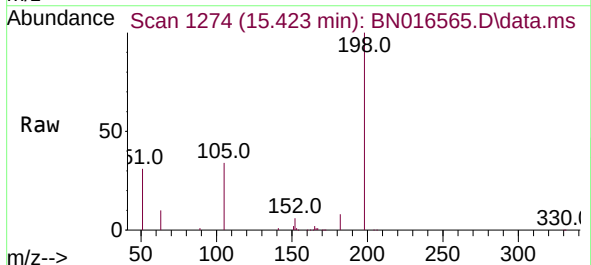


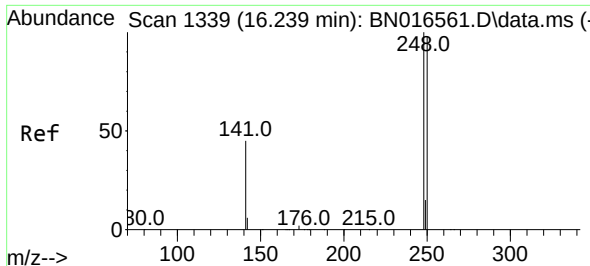

#21
4-Bromophenyl-phenylether
Concen: 5.097 ng
RT: 16.239 min Scan# 1339
Delta R.T. -0.000 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:248 Resp: 433215
Ion Ratio Lower Upper
248 100
250 100.4 71.8 107.6
141 45.7 69.7 104.5#

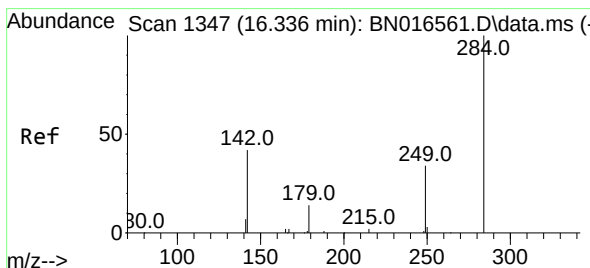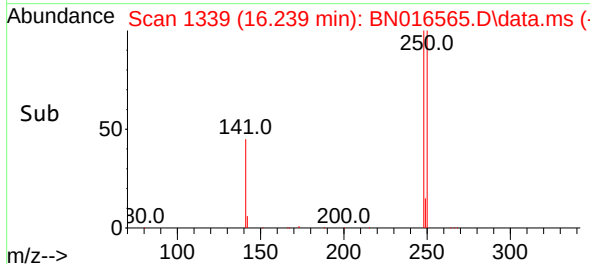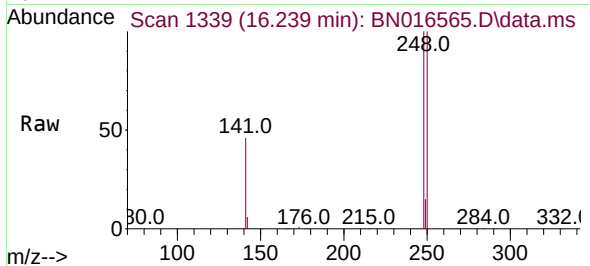

#22
Hexachlorobenzene
Concen: 4.498 ng
RT: 16.348 min Scan# 1348
Delta R.T. 0.012 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13

Tgt Ion:284 Resp: 460081
Ion Ratio Lower Upper
284 100
142 34.9 30.7 46.1
249 29.7 25.8 38.8


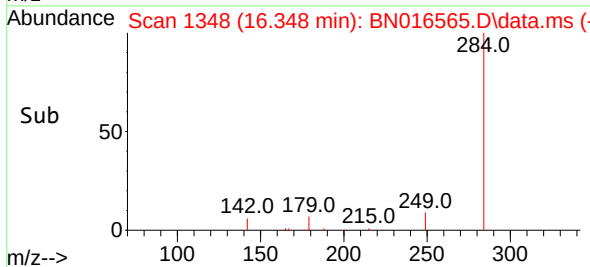

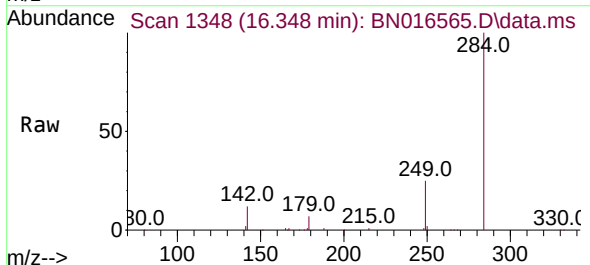


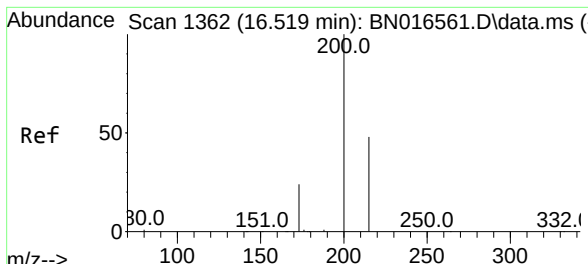

#23
 Atrazine
 Concen: 10.152 ng
 RT: 16.519 min Scan# 1362
 Delta R.T. -0.000 min
 Lab File: BN016565.D
 Acq: 28 Sep 2021 20:13




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:	200	Resp:	345692
Ion Ratio	Lower	Upper	
200	100		
173	25.4	22.6	34.0
215	48.1	38.2	57.4

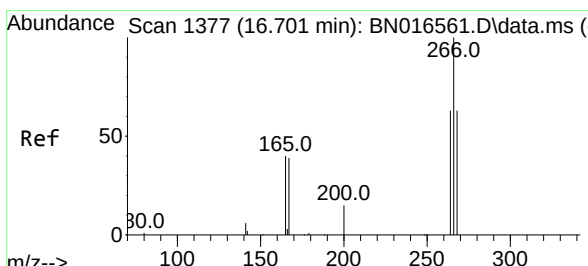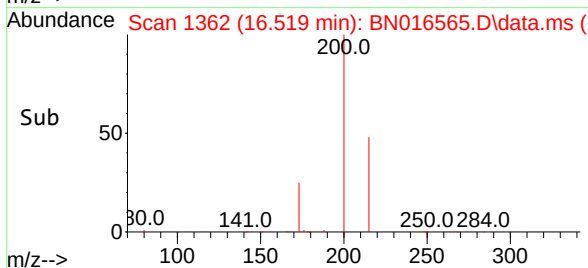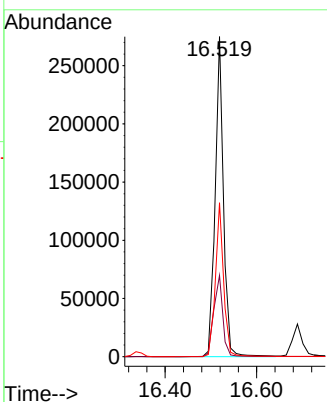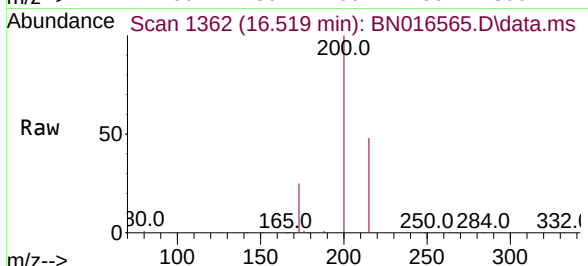

#24
 Pentachlorophenol
 Concen: 8.746 ng
 RT: 16.689 min Scan# 1376
 Delta R.T. -0.012 min
 Lab File: BN016565.D
 Acq: 28 Sep 2021 20:13

Tgt Ion:	266	Resp:	233777
Ion Ratio	Lower	Upper	
266	100		
264	62.5	50.2	75.2
268	64.1	51.8	77.8


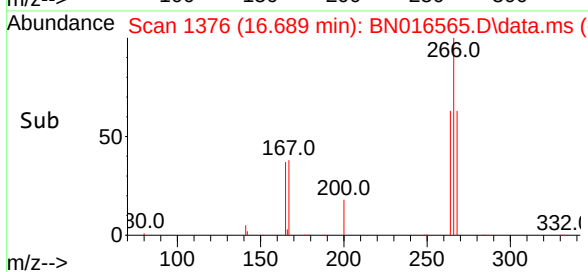
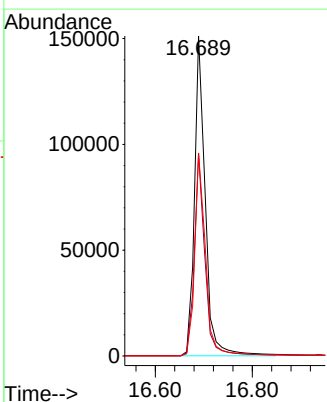
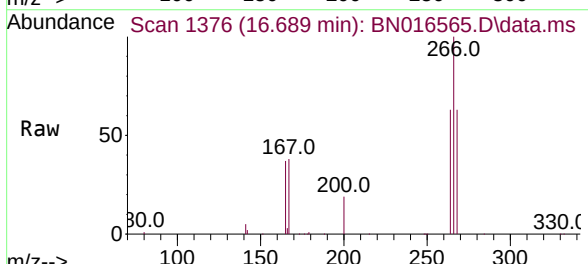


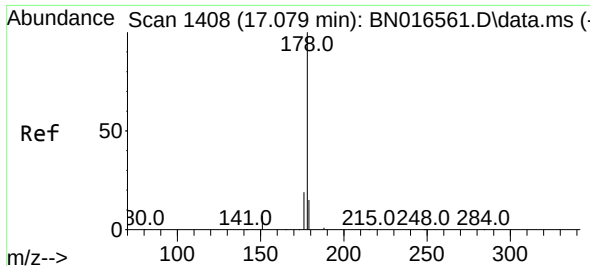

#25
Phenanthrene
Concen: 4.459 ng
RT: 17.078 min Scan# 1408
Delta R.T. -0.000 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:178 Resp: 1987265
Ion Ratio Lower Upper
178 100
176 18.8 15.0 22.6
179 15.6 12.3 18.5

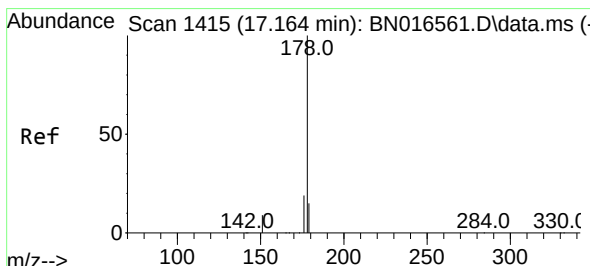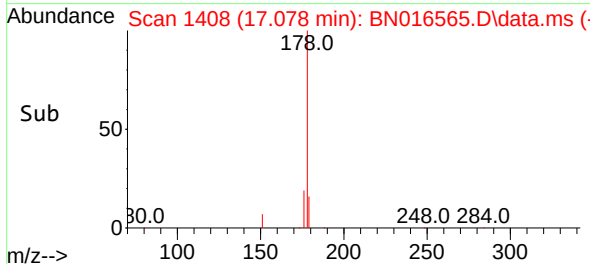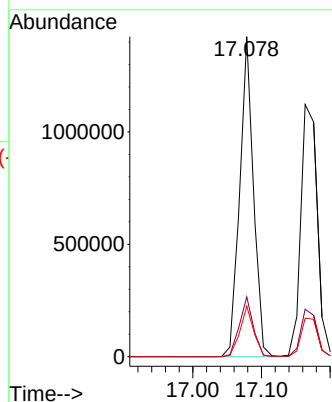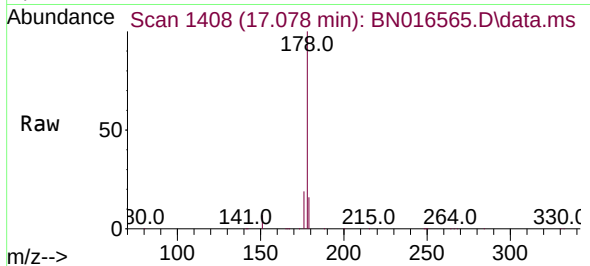

#26
Anthracene
Concen: 5.076 ng
RT: 17.164 min Scan# 1415
Delta R.T. -0.000 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13

Tgt Ion:178 Resp: 1870627
Ion Ratio Lower Upper
178 100
176 18.3 14.6 21.8
179 15.6 12.2 18.4


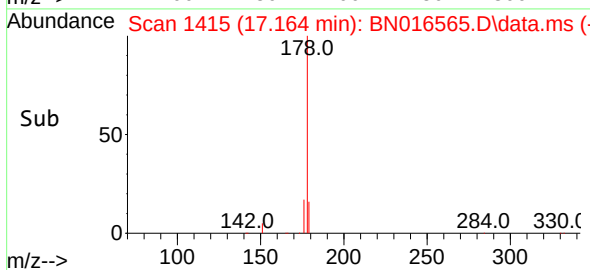

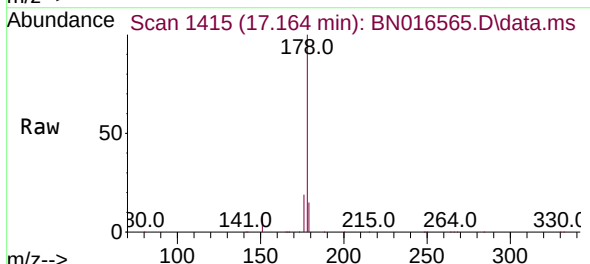


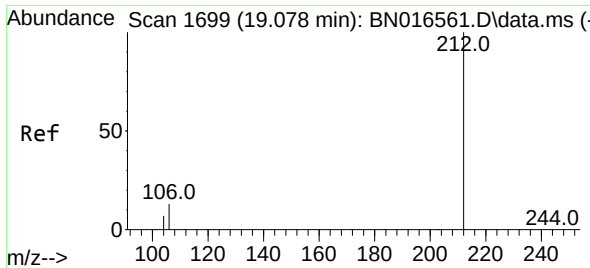

#27
Fluoranthene-d10
Concen: 4.784 ng
RT: 19.078 min Scan# 1699
Delta R.T. -0.000 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:212 Resp: 1832563
Ion Ratio Lower Upper
212 100
106 14.1 8.8 13.2#
104 7.7 5.0 7.4#

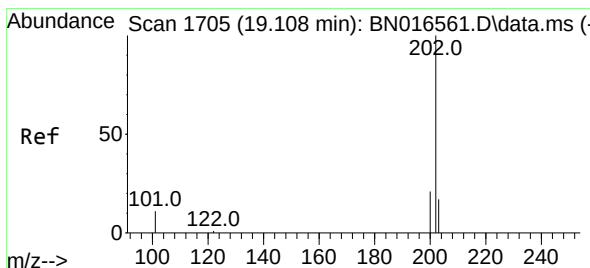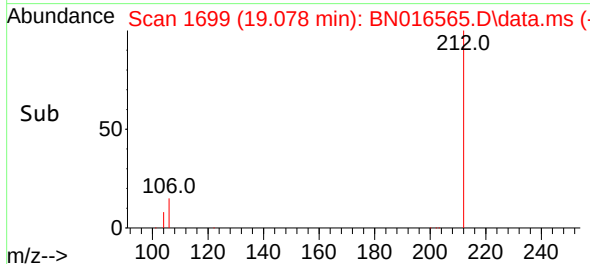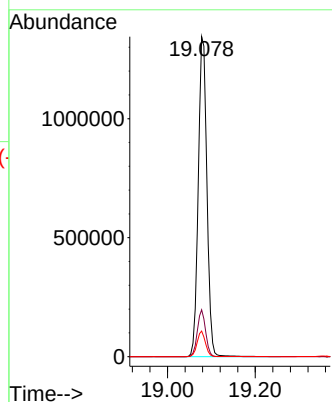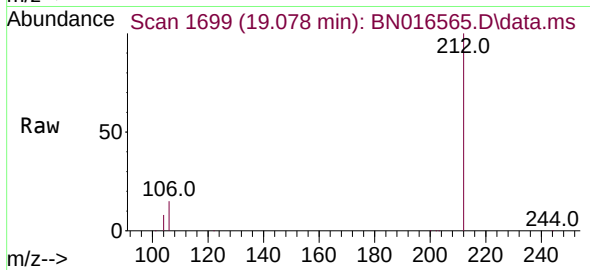

#28
Fluoranthene
Concen: 4.398 ng
RT: 19.108 min Scan# 1705
Delta R.T. -0.000 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13

Tgt Ion:202 Resp: 2140278
Ion Ratio Lower Upper
202 100
101 11.7 7.5 11.3#
203 17.7 13.9 20.9


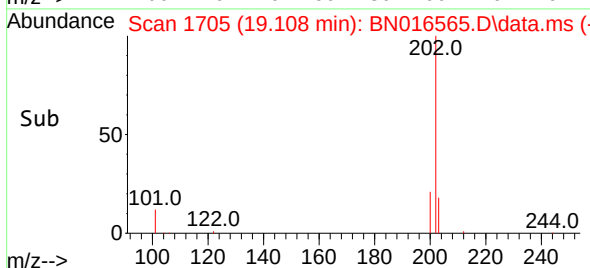

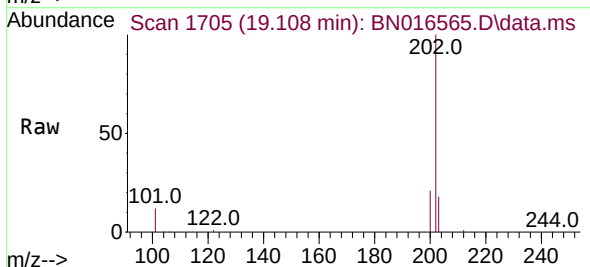




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.249 min Scan# 2003
Delta R.T. -0.000 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:240 Resp: 126300
Ion Ratio Lower Upper
240 100
120 7.7 9.0 13.4#
236 25.9 21.7 32.5

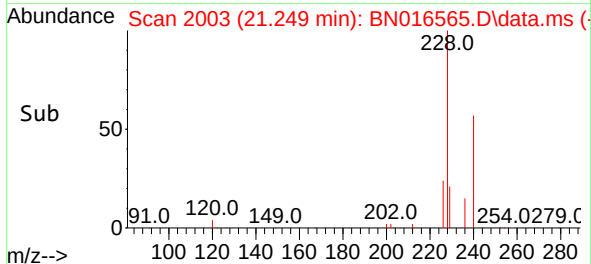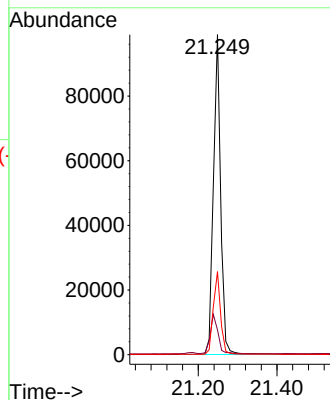

#30
Pyrene
Concen: 6.140 ng
RT: 19.475 min Scan# 1779
Delta R.T. -0.000 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13

Tgt Ion:202 Resp: 2245880
Ion Ratio Lower Upper
202 100
200 20.7 16.3 24.5
203 17.8 13.9 20.9



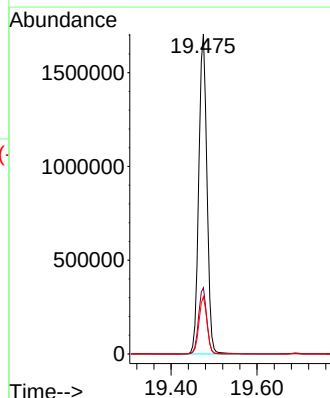
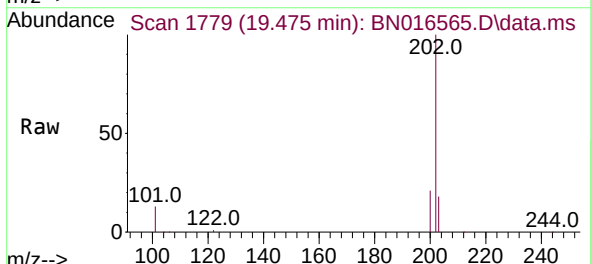




#31
 Terphenyl-d14
 Concen: 5.616 ng
 RT: 19.693 min Scan# 1823
 Delta R.T. -0.000 min
 Lab File: BN016565.D
 Acq: 28 Sep 2021 20:13




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:244 Resp: 1433949
 Ion Ratio Lower Upper
 244 100
 212 7.4 6.1 9.1
 122 11.9 8.4 12.6

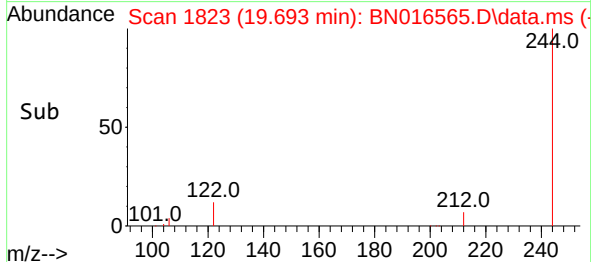

#32
 Benzo(a)anthracene
 Concen: 6.492 ng
 RT: 21.227 min Scan# 2001
 Delta R.T. -0.000 min
 Lab File: BN016565.D
 Acq: 28 Sep 2021 20:13

Tgt Ion:228 Resp: 2175247
 Ion Ratio Lower Upper
 228 100
 226 27.3 21.2 31.8
 229 20.0 15.6 23.4

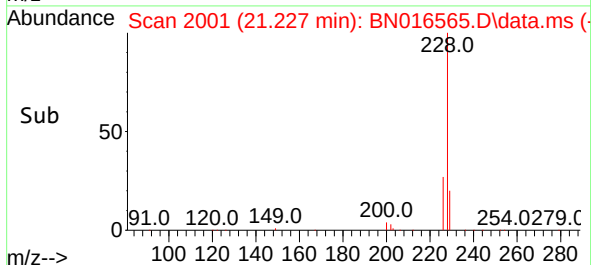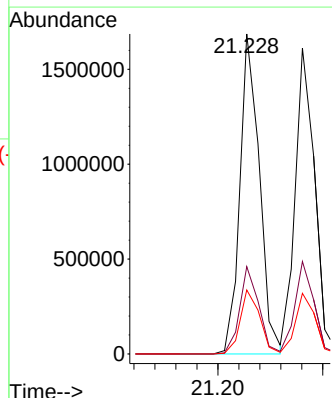

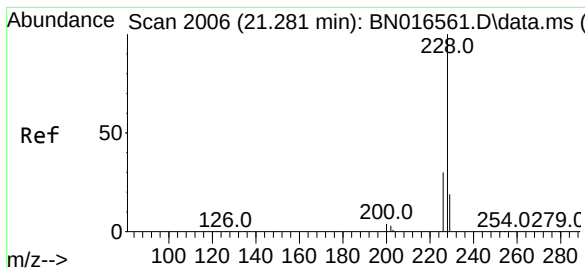

#33

Chrysene

Concen: 5.070 ng

RT: 21.281 min Scan# 2006

Delta R.T. -0.000 min

Lab File: BN016565.D

Acq: 28 Sep 2021 20:13

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:228 Resp: 2075012

Ion Ratio Lower Upper

228 100

226 30.2 23.1 34.7

229 19.8 15.8 23.8

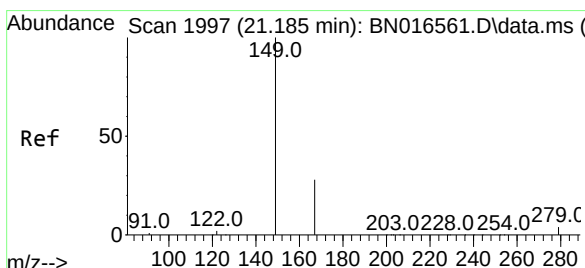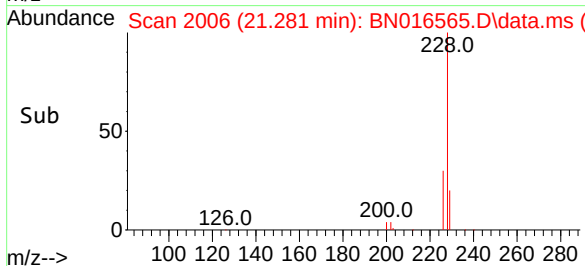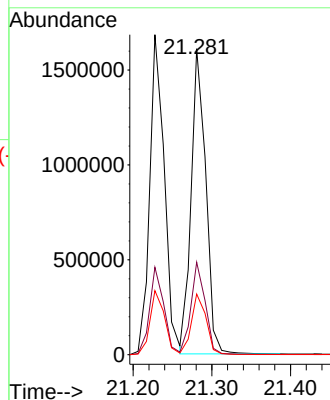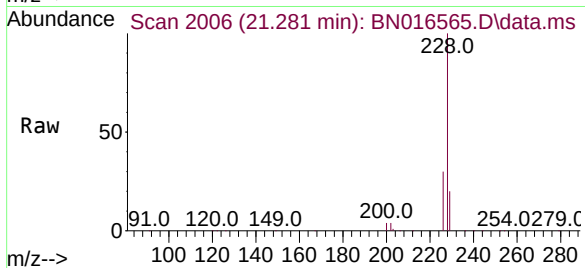

#34

Bis(2-ethylhexyl)phthalate

Concen: 14.397 ng

RT: 21.185 min Scan# 1997

Delta R.T. -0.000 min

Lab File: BN016565.D

Acq: 28 Sep 2021 20:13




Tgt Ion:149 Resp: 902308


Ion Ratio Lower Upper

149 100

167 27.6 21.4 32.2

279 3.7 3.1 4.7

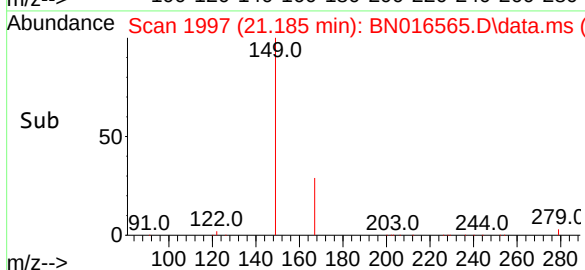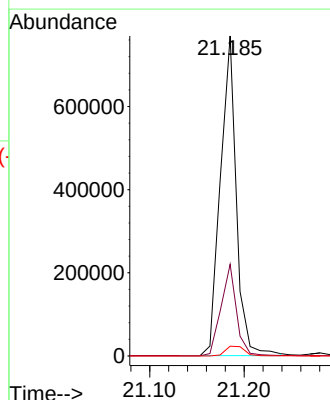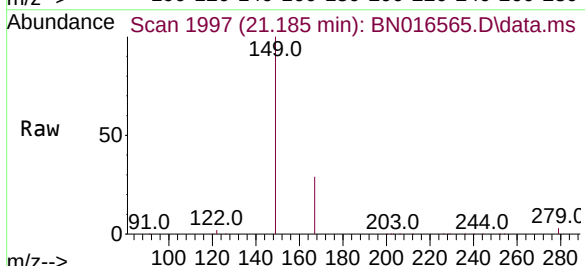







#35
Perylene-d12
Concen: 0.400 ng
RT: 23.509 min Scan# 2434
Delta R.T. -0.000 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:264 Resp: 122752




Ion	Ratio	Lower	Upper
264	100		
260	24.7	19.9	29.9
265	23.5	20.7	31.1

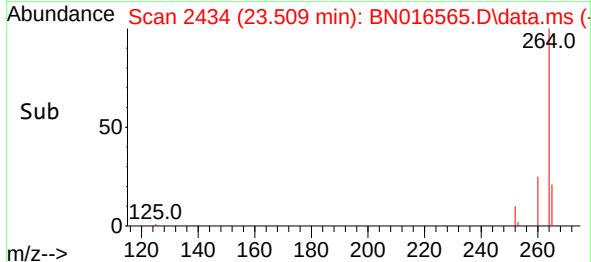


#36
Indeno(1,2,3-cd)pyrene
Concen: 5.931 ng
RT: 25.798 min Scan# 3103
Delta R.T. 0.003 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13

Tgt Ion:276 Resp: 2288389

Ion	Ratio	Lower	Upper
276	100		
138	25.8	18.2	27.2
277	25.1	19.8	29.8




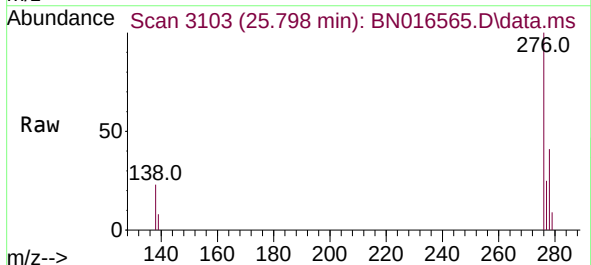




#37
Benzo(b)fluoranthene
Concen: 5.778 ng
RT: 22.827 min Scan# 2235
Delta R.T. 0.003 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:252 Resp: 2192773
Ion Ratio Lower Upper
252 100
253 22.2 17.8 26.6
125 10.3 7.3 10.9

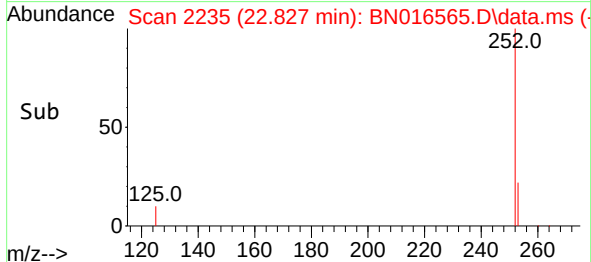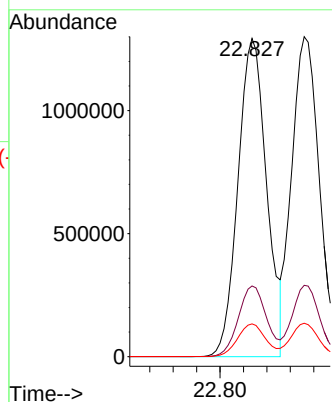

#38
Benzo(k)fluoranthene
Concen: 4.713 ng
RT: 22.872 min Scan# 2248
Delta R.T. 0.003 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13

Tgt Ion:252 Resp: 2086820
Ion Ratio Lower Upper
252 100
253 22.3 17.8 26.6
125 10.5 7.4 11.0




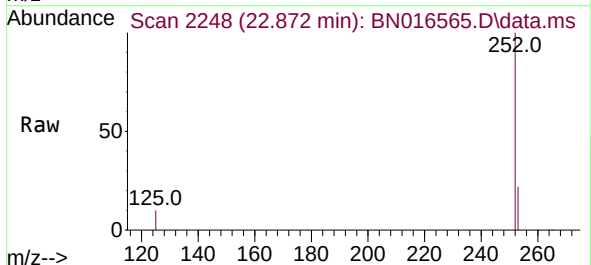




#39
Benzo(a)pyrene
Concen: 6.627 ng
RT: 23.409 min Scan# 2405
Delta R.T. 0.003 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:252 Resp: 2001041
Ion Ratio Lower Upper
252 100
253 22.1 17.9 26.9
125 11.2 8.2 12.4

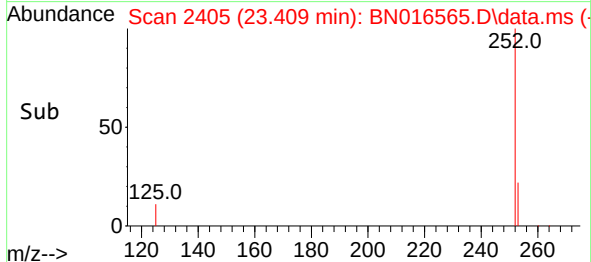

#40
Dibenzo(a,h)anthracene
Concen: 5.485 ng
RT: 25.822 min Scan# 3110
Delta R.T. 0.003 min
Lab File: BN016565.D
Acq: 28 Sep 2021 20:13

Tgt Ion:278 Resp: 1880529
Ion Ratio Lower Upper
278 100
139 17.1 12.1 18.1
279 23.8 19.2 28.8

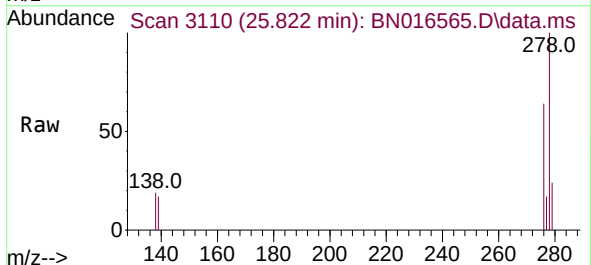

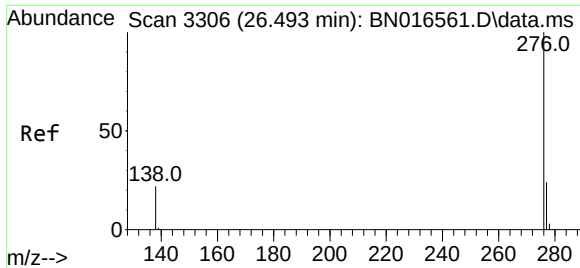

#41
 Benzo(g,h,i)perylene
 Concen: 6.254 ng
 RT: 26.504 min Scan# 3309
 Delta R.T. 0.010 min
 Lab File: BN016565.D
 Acq: 28 Sep 2021 20:13

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Tgt Ion:276 Resp: 1978921

Ion	Ratio	Lower	Upper
276	100		
277	23.7	18.9	28.3
138	22.0	15.7	23.5

