
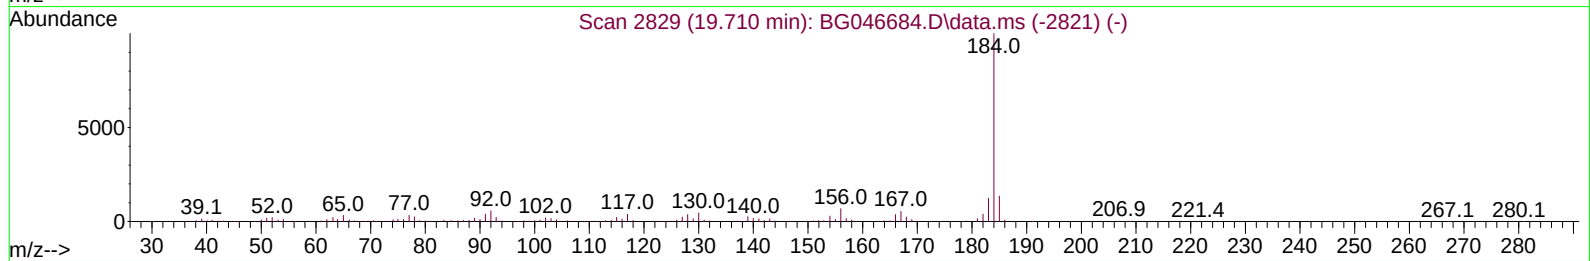
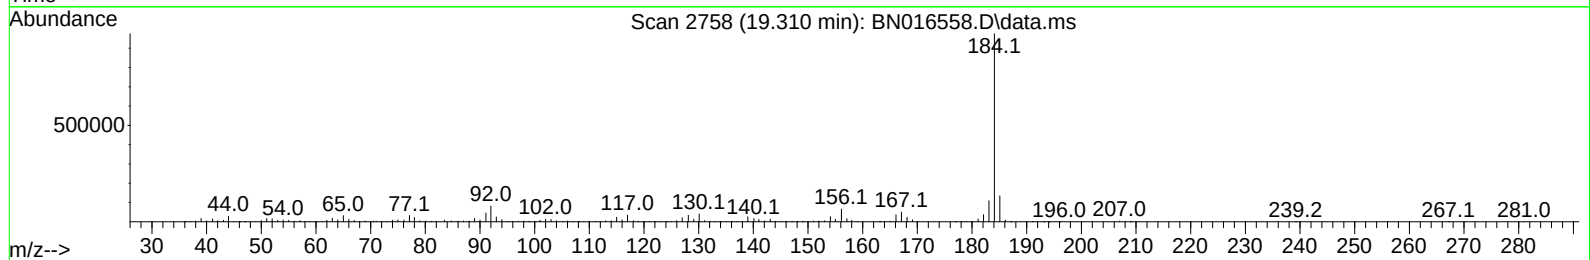


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092821\
 Data File : BN016558.D
 Acq On : 28 Sep 2021 15:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 28 17:48:08 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 28 17:48:03 2021
 Response via : Initial Calibration

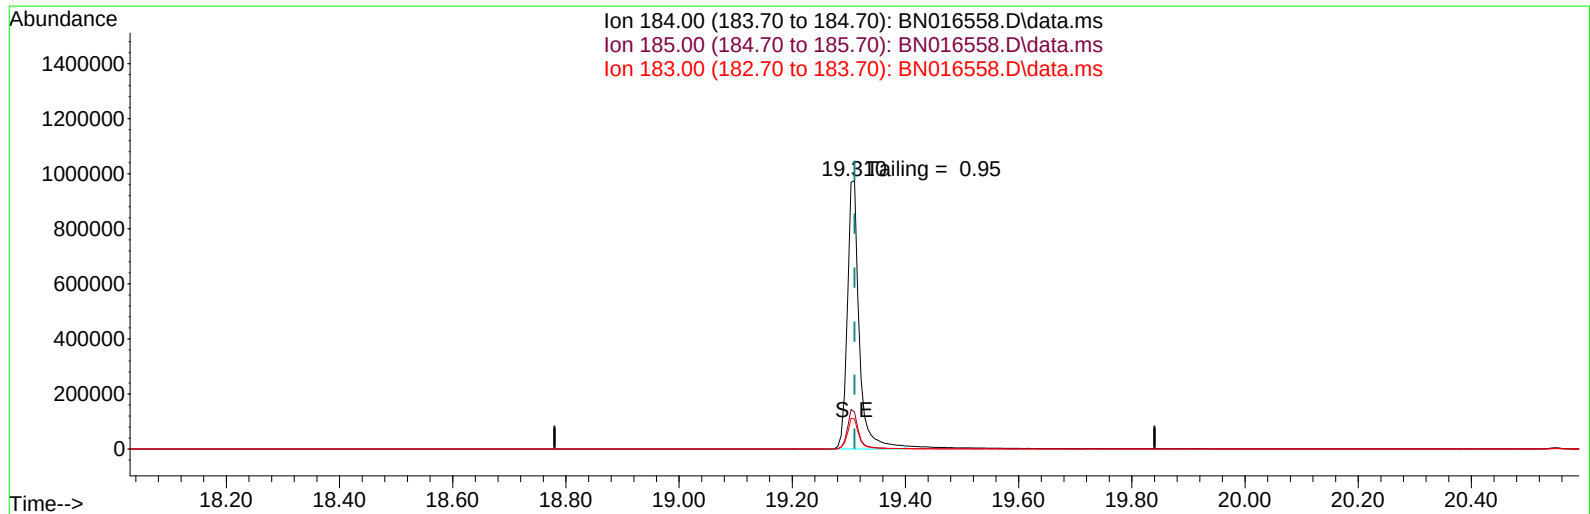

TIC: BN016558.D\data.ms

(77) Benzidine




19.310min (0.000) 153176.07 ng

response 1477895

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.78
183.00	13.20	11.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092821\
Data File : BN016558.D
Acq On : 28 Sep 2021 15:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 28 17:48:08 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 28 17:48:03 2021
Response via : Initial Calibration

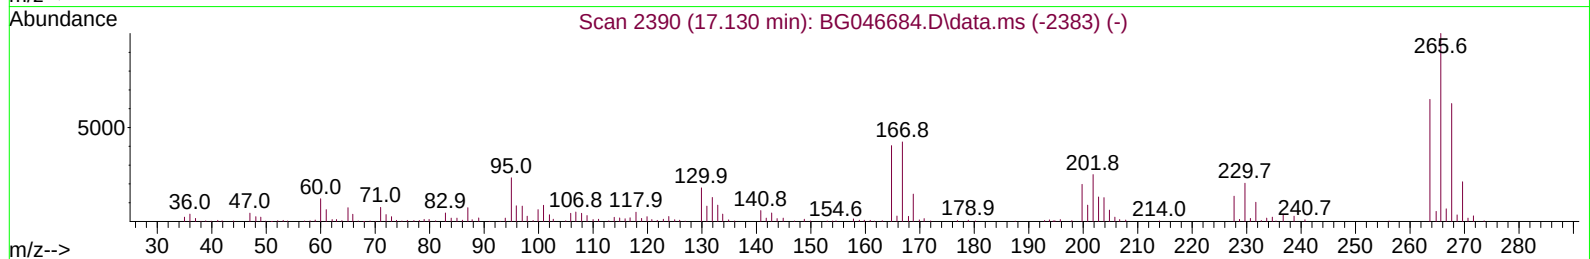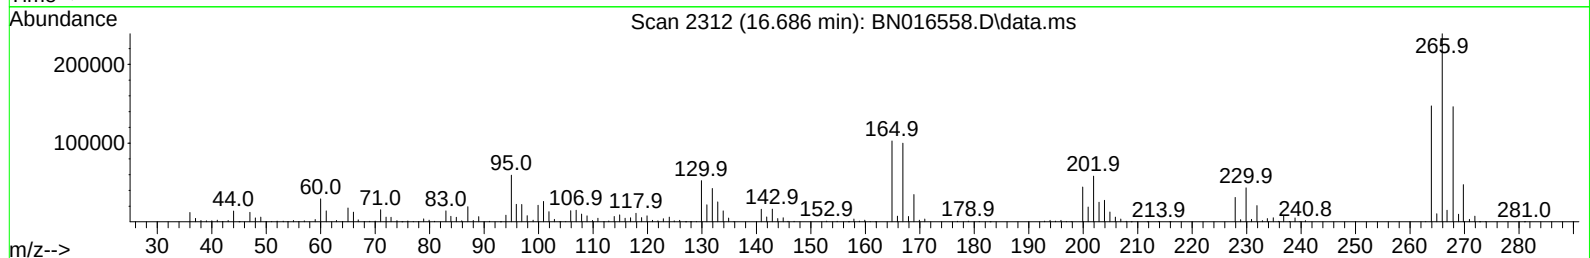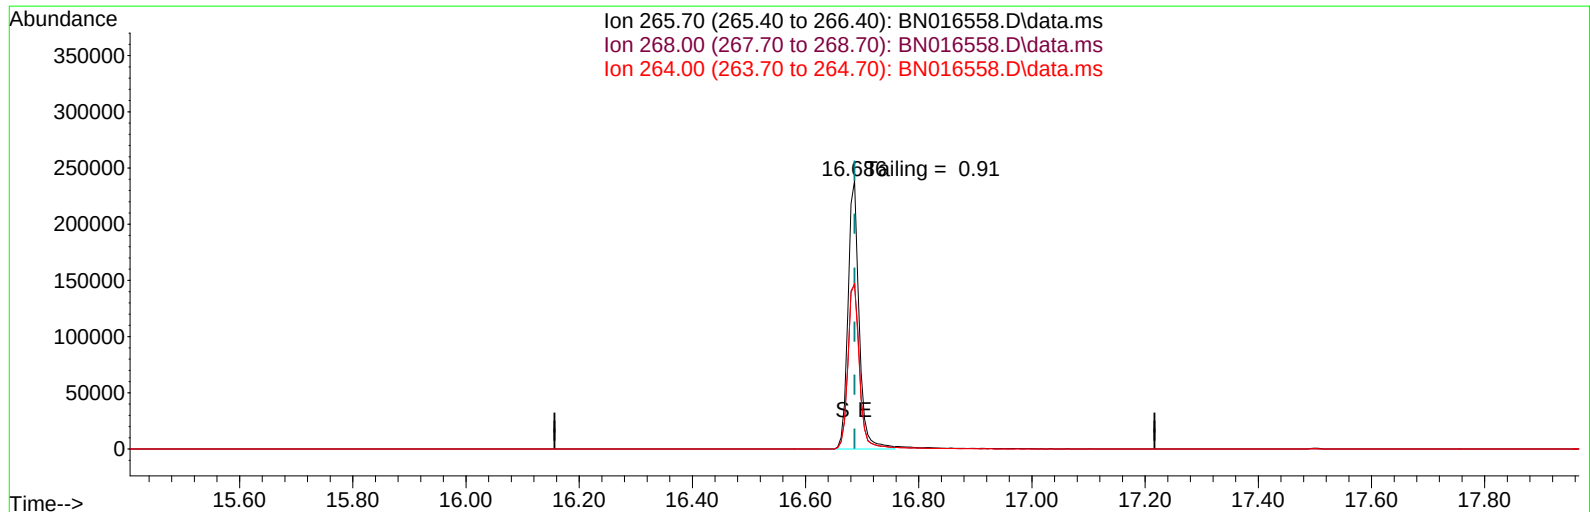

TIC: BN016558.D\data.ms

(70) Pentachlorophenol (C)

16.686min (0.000) 26355.98 ng

response 329902

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.27
264.00	61.60	61.70
0.00	0.00	0.00