
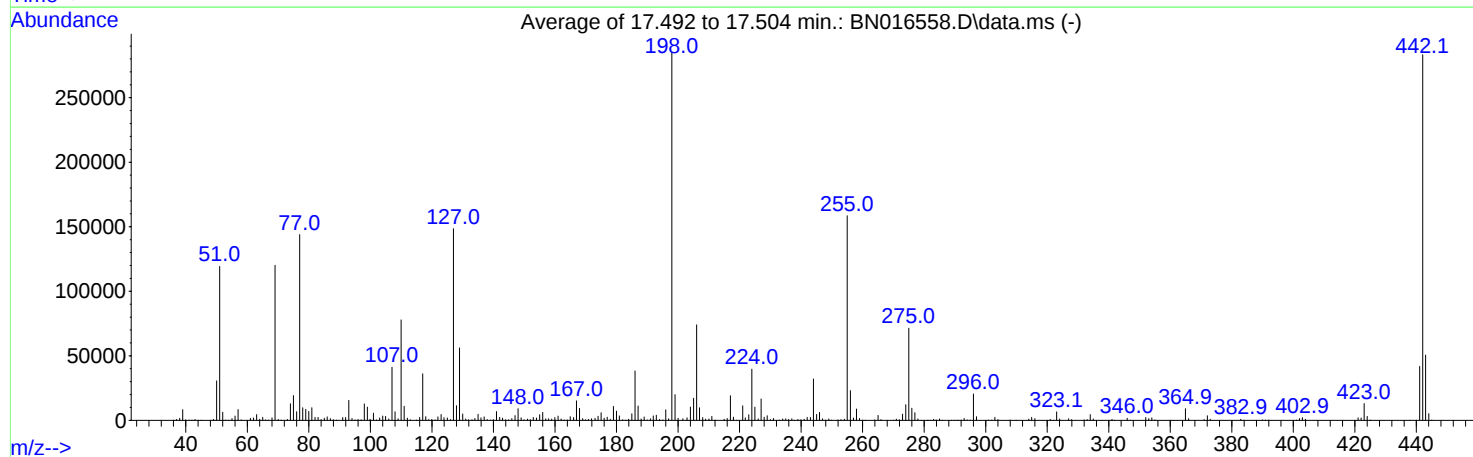


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092821\
 Data File : BN016558.D
 Acq On : 28 Sep 2021 15:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN092821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 29 10:56:17 2021

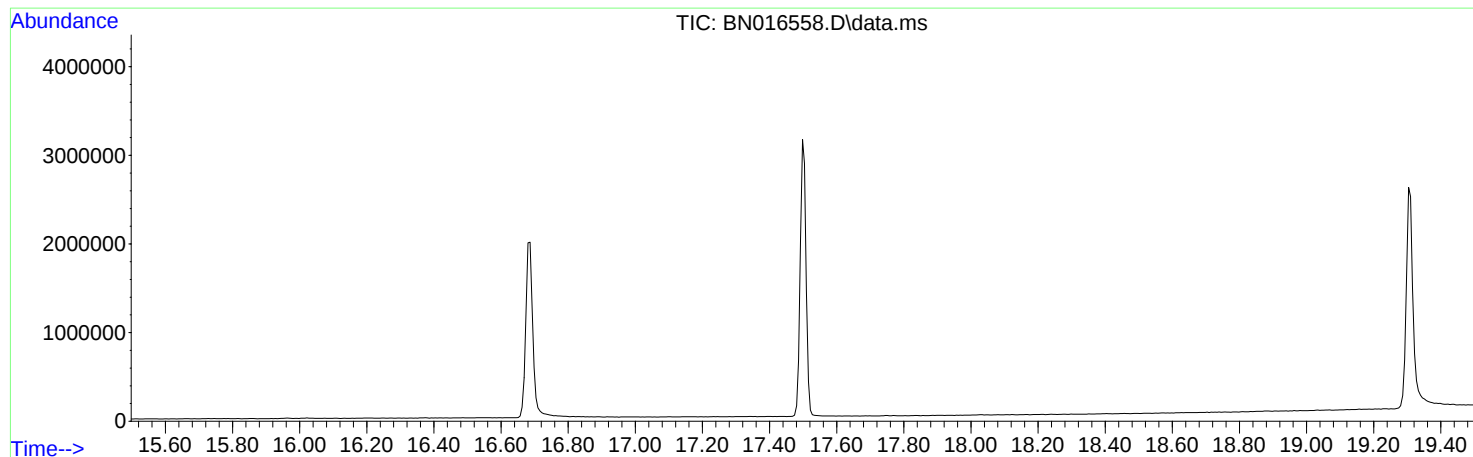




AutoFind: Scans 2449, 2450, 2451; Background Corrected with Scan 2443

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.9	119307	PASS
68	69	0.00	2	1.7	1994	PASS
69	198	0.00	100	42.2	120160	PASS
70	69	0.00	2	0.6	746	PASS
127	198	10	80	52.1	148453	PASS
197	198	0.00	2	0.4	1276	PASS
198	198	100	100	100.0	284992	PASS
199	198	5	9	7.0	19954	PASS
275	198	10	60	25.0	71365	PASS
365	198	1	100	3.2	9062	PASS
441	198	0.01	100	14.7	41773	PASS
442	442	50	100	100.0	283285	PASS
443	442	15	24	17.9	50584	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092821\
 Data File : BN016558.D
 Acq On : 28 Sep 2021 15:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 28 17:48:08 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 28 17:48:03 2021
 Response via : Initial Calibration

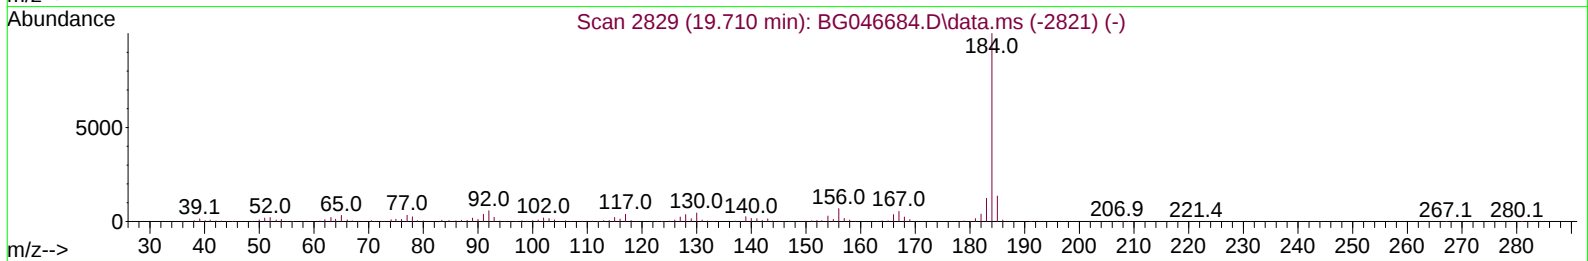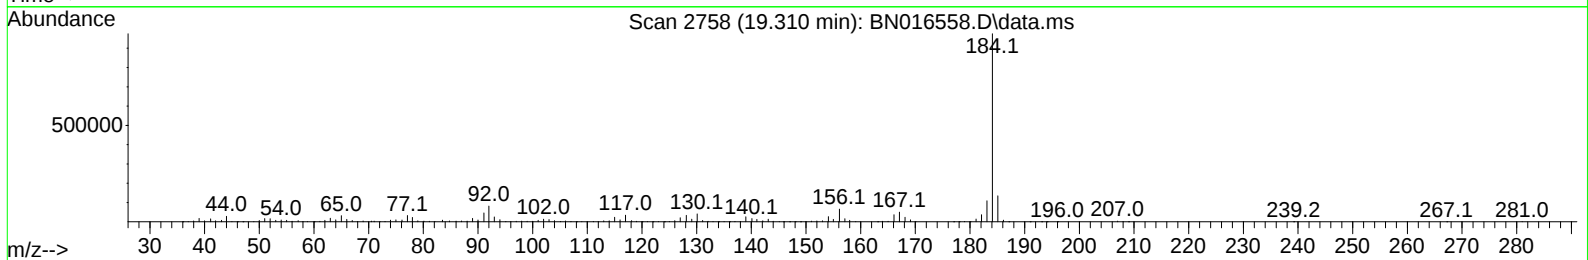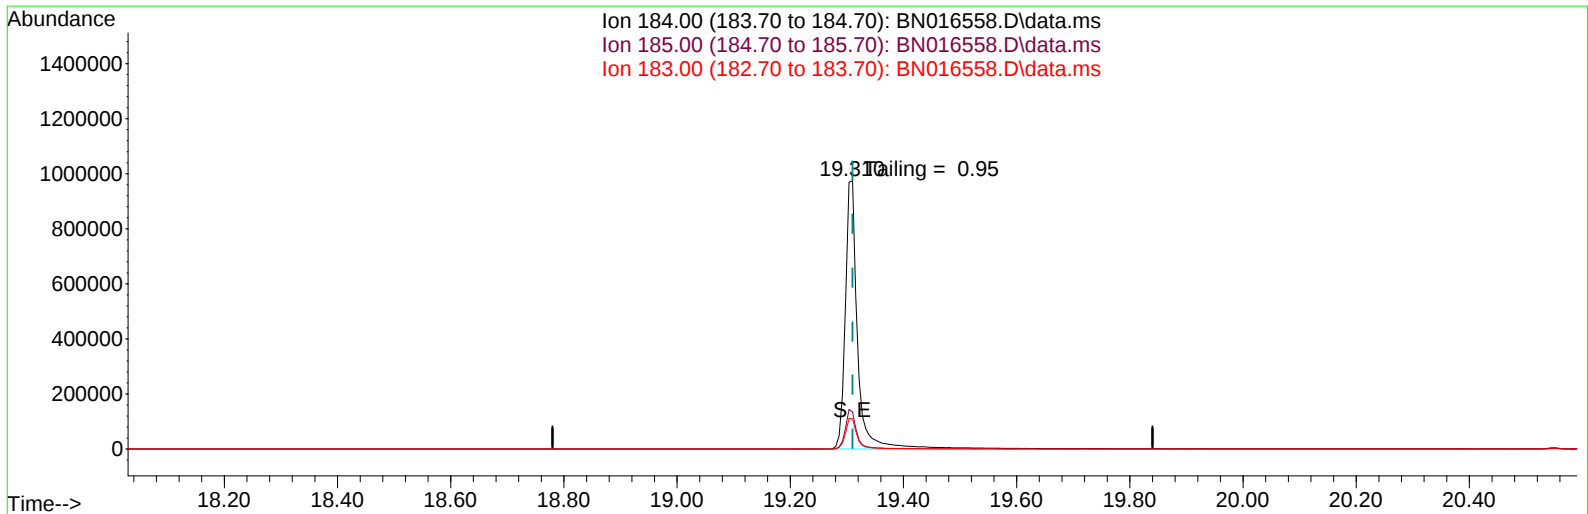

TIC: BN016558.D\data.ms

(77) Benzidine

19.310min (0.000) 153176.07 ng




response 1477895

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.78
183.00	13.20	11.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092821\
 Data File : BN016558.D
 Acq On : 28 Sep 2021 15:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 28 17:48:08 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 28 17:48:03 2021
 Response via : Initial Calibration

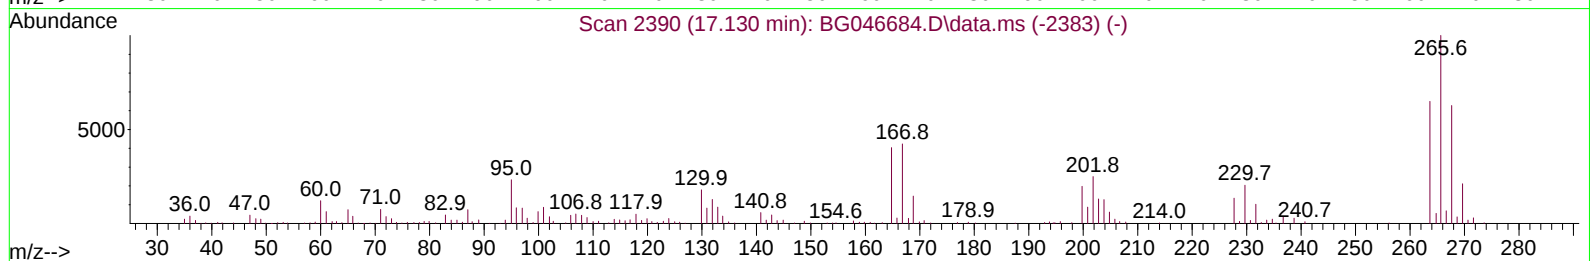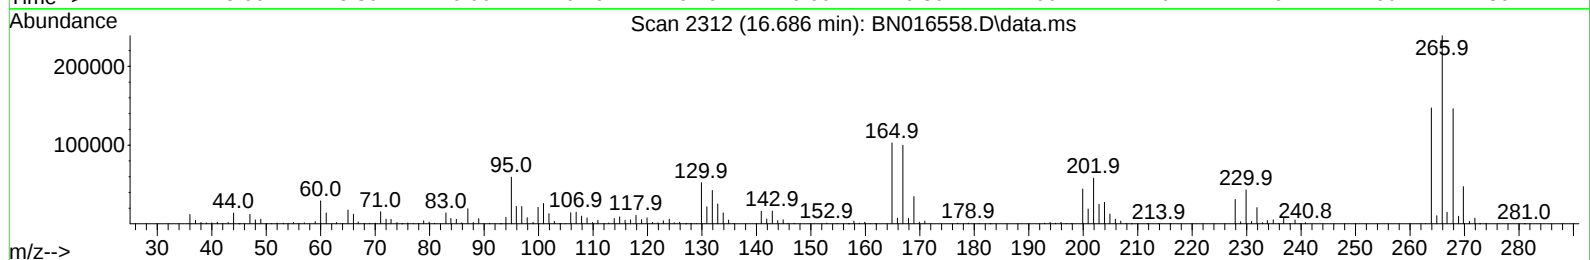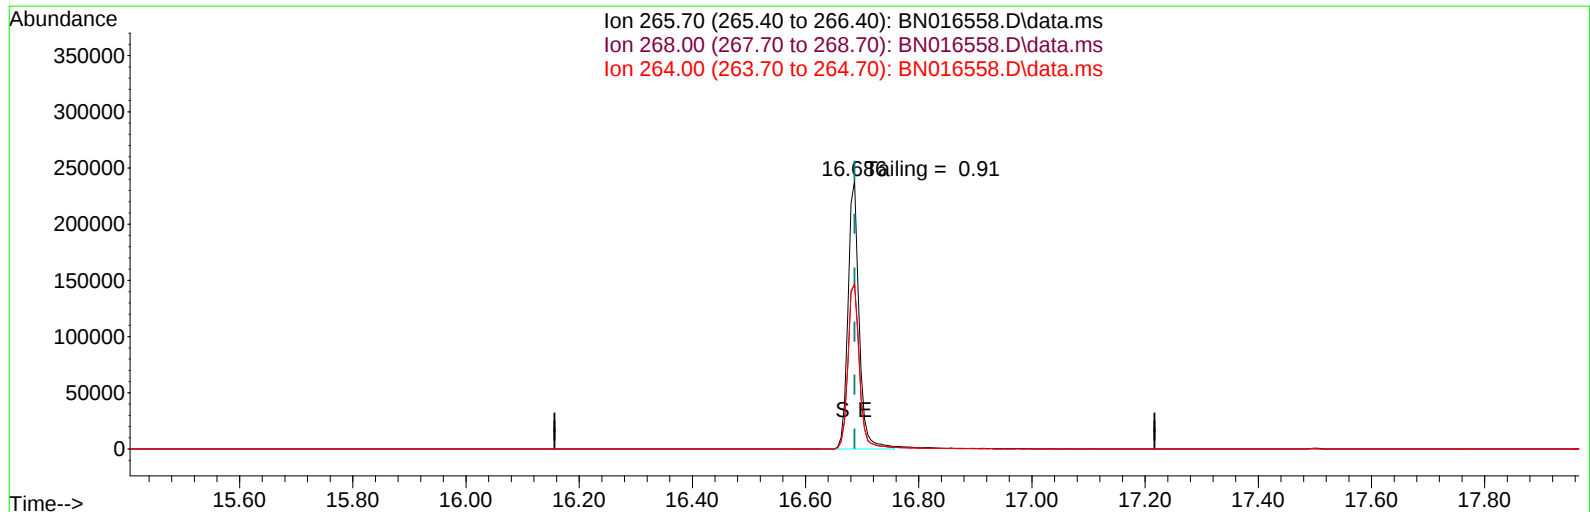

TIC: BN016558.D\data.ms

(70) Pentachlorophenol (C)

16.686min (0.000) 26355.98 ng

response 329902

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.27
264.00	61.60	61.70
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_N
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
9/28/2021	BNA_N	<u>BN016558.D</u>
Compound Name	Response	Retention Time
DDT	685996	20.55
DDD	4169	20.1
DDE	111	19.59
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4280	690276	0.62

Instrument :
BNA_N
ClientSampleId :
DFTPP