

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100121\
 Data File : BN016604.D
 Acq On : 30 Sep 2021 17:20
 Operator : CG/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Quant Time: Sep 30 17:49:24 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 30 15:26:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.642	152	33421	0.40	ng	0.00
7) Naphthalene-d8	10.406	136	132597	0.40	ng	0.00
13) Acenaphthene-d10	14.268	164	68475	0.40	ng	0.00
19) Phenanthrene-d10	17.029	188	121623	0.40	ng	0.00
29) Chrysene-d12	21.238	240	113643	0.40	ng	0.00
35) Perylene-d12	23.488	264	117449	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.254	112	399589	4.66	ng	0.00
5) Phenol-d6	6.821	99	450584	4.91	ng	0.00
8) Nitrobenzene-d5	8.784	82	485411	5.83	ng	0.00
11) 2-Methylnaphthalene-d10	12.003	152	925916	4.78	ng	0.00
14) 2,4,6-Tribromophenol	15.778	330	184550	5.91	ng	0.01
15) 2-Fluorobiphenyl	12.898	172	1298849	4.62	ng	0.00
27) Fluoranthene-d10	19.068	212	1620256	4.86	ng	0.00
31) Terphenyl-d14	19.678	244	1285493	5.20	ng	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.253	88	77133	4.66	ng	# 86
3) n-Nitrosodimethylamine	3.576	42	126572	5.03	ng	99
6) bis(2-Chloroethyl)ether	7.080	93	406227	4.47	ng	99
9) Naphthalene	10.457	128	1674670	4.57	ng	100
10) Hexachlorobutadiene	10.749	225	322539	4.73	ng	# 100
12) 2-Methylnaphthalene	12.078	142	1056475	4.63	ng	99
16) Acenaphthylene	13.989	152	1582152	5.21	ng	100
17) Acenaphthene	14.332	154	975102	4.84	ng	98
18) Fluorene	15.322	166	1168324	4.88	ng	99
20) 4,6-Dinitro-2-methylph...	15.410	198	121584	8.80	ng	# 79
21) 4-Bromophenyl-phenylether	16.226	248	393700	5.24	ng	98
22) Hexachlorobenzene	16.336	284	428643	4.89	ng	99
23) Atrazine	16.506	200	322269	5.85	ng	97
25) Phenanthrene	17.066	178	1760796	4.80	ng	100
26) Anthracene	17.151	178	1655626	5.23	ng	100
28) Fluoranthene	19.097	202	1880034	4.65	ng	99
30) Pyrene	19.460	202	1980595	5.35	ng	100
32) Benzo(a)anthracene	21.217	228	1928673	5.57	ng	100
33) Chrysene	21.270	228	1833727	5.06	ng	99
36) Indeno(1,2,3-cd)pyrene	25.767	276	2233982	5.11	ng	99
37) Benzo(b)fluoranthene	22.810	252	1985292	5.46	ng	100
38) Benzo(k)fluoranthene	22.854	252	1904987	5.18	ng	100
39) Benzo(a)pyrene	23.388	252	1821558	5.36	ng	100
40) Dibenzo(a,h)anthracene	25.791	278	1824093	5.16	ng	100
41) Benzo(g,h,i)perylene	26.466	276	1954181	5.07	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100121\
Data File : BN016604.D
Acq On : 30 Sep 2021 17:20
Operator : CG/JU
Sample : SSTDICC5.0
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Quant Time: Sep 30 17:49:24 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 15:26:45 2021
Response via : Initial Calibration








#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.642 min Scan# 495
 Delta R.T. 0.000 min
 Lab File: BN016604.D
 Acq: 30 Sep 2021 17:20




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:152 Resp: 33421
 Ion Ratio Lower Upper
 152 100
 150 157.5 124.6 186.8
 115 58.5 46.5 69.7



#2
 1,4-Dioxane
 Concen: 4.66 ng
 RT: 3.253 min Scan# 19
 Delta R.T. 0.000 min
 Lab File: BN016604.D
 Acq: 30 Sep 2021 17:20

Tgt Ion: 88 Resp: 77133
 Ion Ratio Lower Upper
 88 100
 43 27.0 37.8 56.8#
 58 73.3 61.3 91.9









#3
n-Nitrosodimethylamine
Concen: 5.03 ng
RT: 3.576 min Scan# 54
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion: 42 Resp: 126572




Ion	Ratio	Lower	Upper
42	100		
74	152.9	121.6	182.4
44	6.5	6.3	9.5




#4
2-Fluorophenol
Concen: 4.66 ng
RT: 5.254 min Scan# 236
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20

Tgt Ion: 112 Resp: 399589

Ion	Ratio	Lower	Upper
112	100		
64	53.9	43.1	64.7
63	27.2	21.6	32.4









#5
Phenol-d6
Concen: 4.91 ng
RT: 6.821 min Scan# 406
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 99 Resp: 450584
Ion Ratio Lower Upper
99 100
42 16.4 13.0 19.6
71 29.6 23.5 35.3



#6
bis(2-Chloroethyl)ether
Concen: 4.47 ng
RT: 7.080 min Scan# 434
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20

Tgt Ion: 93 Resp: 406227
Ion Ratio Lower Upper
93 100
63 73.0 59.1 88.7
95 32.6 26.2 39.4









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.406 min Scan# 733
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	136	Resp:	132597
Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.7	13.1
54	7.2	5.9	8.9
68	6.1	5.0	7.6



#8
Nitrobenzene-d5
Concen: 5.83 ng
RT: 8.784 min Scan# 605
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20

Tgt Ion:	82	Resp:	485411
Ion	Ratio	Lower	Upper
82	100		
128	45.4	33.6	50.4
54	45.1	37.6	56.4









#9
Naphthalene
Concen: 4.57 ng
RT: 10.457 min Scan# 737
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:128 Resp: 1674670
Ion Ratio Lower Upper
128 100
129 11.2 8.8 13.2
127 12.8 10.3 15.5



#10
Hexachlorobutadiene
Concen: 4.73 ng
RT: 10.749 min Scan# 760
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20

Tgt Ion:225 Resp: 322539
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.2 51.0 76.6









#11
2-Methylnaphthalene-d10
Concen: 4.78 ng
RT: 12.003 min Scan# 931
Delta R.T. -0.004 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:152 Resp: 925916
Ion Ratio Lower Upper
152 100
151 20.1 16.2 24.4

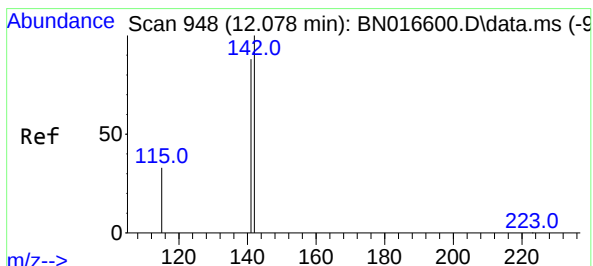

#12
2-Methylnaphthalene
Concen: 4.63 ng
RT: 12.078 min Scan# 948
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20

Tgt Ion:142 Resp: 1056475
Ion Ratio Lower Upper
142 100
141 87.7 70.6 105.8
115 32.7 26.6 39.8









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.268 min Scan# 1183
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:164 Resp: 68475
Ion Ratio Lower Upper
164 100
162 103.4 82.2 123.2
160 47.6 37.7 56.5



#14
2,4,6-Tribromophenol
Concen: 5.91 ng
RT: 15.778 min Scan# 1302
Delta R.T. 0.013 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20

Tgt Ion:330 Resp: 184550
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 30.7 25.2 37.8









#15
2-Fluorobiphenyl
Concen: 4.62 ng
RT: 12.898 min Scan# 1075
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:172 Resp: 1298849




Ion	Ratio	Lower	Upper
172	100		
171	33.2	27.0	40.4
170	21.4	17.4	26.2




#16
Acenaphthylene
Concen: 5.21 ng
RT: 13.989 min Scan# 1161
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20

Tgt Ion:152 Resp: 1582152

Ion	Ratio	Lower	Upper
152	100		
151	19.3	15.5	23.3
153	13.2	10.4	15.6









#17
Acenaphthene
Concen: 4.84 ng
RT: 14.332 min Scan# 1188
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:154 Resp: 975102
Ion Ratio Lower Upper
154 100
153 110.8 90.2 135.2
152 52.7 44.0 66.0



#18
Fluorene
Concen: 4.88 ng
RT: 15.322 min Scan# 1266
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20

Tgt Ion:166 Resp: 1168324
Ion Ratio Lower Upper
166 100
165 95.9 77.9 116.9
167 13.5 10.7 16.1









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.029 min Scan# 1404
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:188 Resp: 121623




Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	6.7	5.0	7.6




#20
4,6-Dinitro-2-methylphenol
Concen: 8.80 ng
RT: 15.410 min Scan# 1273
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20

Tgt Ion:198 Resp: 121584

Ion	Ratio	Lower	Upper
198	100		
182	6.1	11.8	17.8
77	0.0	0.0	0.0









#21
4-Bromophenyl-phenylether
Concen: 5.24 ng
RT: 16.226 min Scan# 1338
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20




Instrument :
BNA_N
ClientSampled :
SSTDICC5.0


Tgt Ion:248 Resp: 393700
Ion Ratio Lower Upper
248 100
250 97.6 78.6 117.8
141 45.8 38.6 57.8



#22
Hexachlorobenzene
Concen: 4.89 ng
RT: 16.336 min Scan# 1347
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20

Tgt Ion:284 Resp: 428643
Ion Ratio Lower Upper
284 100
142 32.3 26.4 39.6
249 29.2 23.4 35.2









#23
Atrazine
Concen: 5.85 ng
RT: 16.506 min Scan# 1361
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:200 Resp: 322269
Ion Ratio Lower Upper
200 100
173 25.6 18.6 27.8
215 48.2 39.4 59.2



#25
Phenanthrene
Concen: 4.80 ng
RT: 17.066 min Scan# 1407
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20

Tgt Ion:178 Resp: 1760796
Ion Ratio Lower Upper
178 100
176 18.8 15.0 22.4
179 15.5 12.2 18.4









#26
 Anthracene
 Concen: 5.23 ng
 RT: 17.151 min Scan# 1414
 Delta R.T. 0.000 min
 Lab File: BN016604.D
 Acq: 30 Sep 2021 17:20

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Tgt Ion:178 Resp: 1655626




Ion	Ratio	Lower	Upper
178	100		
176	18.2	14.6	21.8
179	15.5	12.2	18.4




#27
 Fluoranthene-d10
 Concen: 4.86 ng
 RT: 19.068 min Scan# 1697
 Delta R.T. 0.000 min
 Lab File: BN016604.D
 Acq: 30 Sep 2021 17:20

Tgt Ion:212 Resp: 1620256

Ion	Ratio	Lower	Upper
212	100		
106	13.8	10.6	16.0
104	7.5	5.9	8.9









#28
Fluoranthene
Concen: 4.65 ng
RT: 19.097 min Scan# 1703
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:202 Resp: 1880034
Ion Ratio Lower Upper
202 100
101 11.5 9.0 13.4
203 17.7 13.8 20.6



#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.238 min Scan# 2002
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20

Tgt Ion:240 Resp: 113643
Ion Ratio Lower Upper
240 100
120 6.8 5.0 7.4
236 25.7 20.4 30.6









#30
Pyrene
Concen: 5.35 ng
RT: 19.460 min Scan# 1776
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:202 Resp: 1980595




Ion	Ratio	Lower	Upper
202	100		
200	20.6	16.5	24.7
203	17.8	14.0	21.0




#31
Terphenyl-d14
Concen: 5.20 ng
RT: 19.678 min Scan# 1820
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20

Tgt Ion:244 Resp: 1285493

Ion	Ratio	Lower	Upper
244	100		
212	7.4	6.0	9.0
122	13.2	10.1	15.1









#32
Benzo(a)anthracene
Concen: 5.57 ng
RT: 21.217 min Scan# 2000
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:228 Resp: 1928673
Ion Ratio Lower Upper
228 100
226 27.5 21.9 32.9
229 19.9 15.7 23.5



#33
Chrysene
Concen: 5.06 ng
RT: 21.270 min Scan# 2005
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20


Tgt Ion:228 Resp: 1833727
Ion Ratio Lower Upper
228 100
226 29.9 23.7 35.5
229 19.8 15.5 23.3







#35
Perylene-d12
Concen: 0.40 ng
RT: 23.488 min Scan# 2428
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20


Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0





Tgt Ion:264 Resp: 117449
Ion Ratio Lower Upper
264 100
260 24.5 19.9 29.9
265 23.4 19.2 28.8




#36
Indeno(1,2,3-cd)pyrene
Concen: 5.11 ng
RT: 25.767 min Scan# 3094
Delta R.T. 0.003 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20



Tgt Ion:276 Resp: 2233982
Ion Ratio Lower Upper
276 100
138 24.8 19.5 29.3
277 25.1 19.9 29.9









#37
Benzo(b)fluoranthene
Concen: 5.46 ng
RT: 22.810 min Scan# 2230
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:252 Resp: 1985292
Ion Ratio Lower Upper
252 100
253 22.2 17.8 26.8
125 10.0 8.0 12.0



#38
Benzo(k)fluoranthene
Concen: 5.18 ng
RT: 22.854 min Scan# 2243
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20

Tgt Ion:252 Resp: 1904987
Ion Ratio Lower Upper
252 100
253 22.0 17.8 26.6
125 10.1 8.0 12.0









#39
Benzo(a)pyrene
Concen: 5.36 ng
RT: 23.388 min Scan# 2399
Delta R.T. 0.000 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:252 Resp: 1821558
Ion Ratio Lower Upper
252 100
253 22.2 17.8 26.8
125 10.9 9.0 13.4



#40
Dibenzo(a,h)anthracene
Concen: 5.16 ng
RT: 25.791 min Scan# 3101
Delta R.T. 0.003 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20


Tgt Ion:278 Resp: 1824093
Ion Ratio Lower Upper
278 100
139 16.3 13.1 19.7
279 23.7 19.1 28.7





#41
Benzo(g,h,i)perylene
Concen: 5.07 ng
RT: 26.466 min Scan# 3298
Delta R.T. 0.007 min
Lab File: BN016604.D
Acq: 30 Sep 2021 17:20

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0



Tgt Ion:276 Resp: 1954181
Ion Ratio Lower Upper
276 100
277 23.8 19.0 28.6
138 21.4 16.9 25.3

