

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100121\
 Data File : BN016616.D
 Acq On : 01 Oct 2021 02:23
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Oct 01 06:23:24 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 30 17:56:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.642	152	33291	0.40	ng	0.00
7) Naphthalene-d8	10.407	136	144903	0.40	ng	0.00
13) Acenaphthene-d10	14.269	164	75533	0.40	ng	0.00
19) Phenanthrene-d10	17.017	188	135439	0.40	ng	#-0.01
29) Chrysene-d12	21.227	240	125841	0.40	ng	#-0.01
35) Perylene-d12	23.481	264	132252	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.254	112	29689	0.35	ng	0.00
5) Phenol-d6	6.822	99	31906	0.34	ng	0.00
8) Nitrobenzene-d5	8.784	82	30216	0.32	ng	0.00
11) 2-Methylnaphthalene-d10	12.003	152	79610	0.37	ng	0.00
14) 2,4,6-Tribromophenol	15.766	330	10649	0.31	ng	0.00
15) 2-Fluorobiphenyl	12.898	172	112943	0.37	ng	0.00
27) Fluoranthene-d10	19.063	212	129381	0.36	ng	0.00
31) Terphenyl-d14	19.678	244	109044	0.40	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.253	88	5718	0.37	ng	# 78
3) n-Nitrosodimethylamine	3.576	42	8859	0.36	ng	98
6) bis(2-Chloroethyl)ether	7.080	93	34237	0.38	ng	100
9) Naphthalene	10.457	128	146411	0.37	ng	100
10) Hexachlorobutadiene	10.749	225	28116	0.38	ng	# 100
12) 2-Methylnaphthalene	12.078	142	95219	0.38	ng	99
16) Acenaphthylene	13.990	152	113830	0.34	ng	100
17) Acenaphthene	14.332	154	80961	0.36	ng	99
18) Fluorene	15.322	166	97214	0.37	ng	100
20) 4,6-Dinitro-2-methylph...	15.411	198	3263	0.32	ng	98
21) 4-Bromophenyl-phenylether	16.226	248	30506	0.36	ng	95
22) Hexachlorobenzene	16.324	284	37321	0.38	ng	99
23) Atrazine	16.506	200	18425	0.30	ng	99
24) Pentachlorophenol	16.677	266	10567	0.33	ng	100
25) Phenanthrene	17.066	178	154084	0.38	ng	100
26) Anthracene	17.151	178	123148	0.35	ng	100
28) Fluoranthene	19.093	202	165011	0.38	ng	100
30) Pyrene	19.460	202	162095	0.40	ng	100
32) Benzo(a)anthracene	21.217	228	139962	0.36	ng	98
33) Chrysene	21.270	228	165316	0.42	ng	98
34) Bis(2-ethylhexyl)phtha...	21.164	149	44365	0.29	ng	99
36) Indeno(1,2,3-cd)pyrene	25.757	276	191152	0.41	ng	99
37) Benzo(b)fluoranthene	22.803	252	155467	0.37	ng	100
38) Benzo(k)fluoranthene	22.848	252	169940	0.40	ng	98
39) Benzo(a)pyrene	23.382	252	141604	0.37	ng	100
40) Dibenzo(a,h)anthracene	25.778	278	153266	0.40	ng	99
41) Benzo(g,h,i)perylene	26.452	276	164989	0.40	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100121\
Data File : BN016616.D
Acq On : 01 Oct 2021 02:23
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Oct 01 06:23:24 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 17:56:53 2021
Response via : Initial Calibration



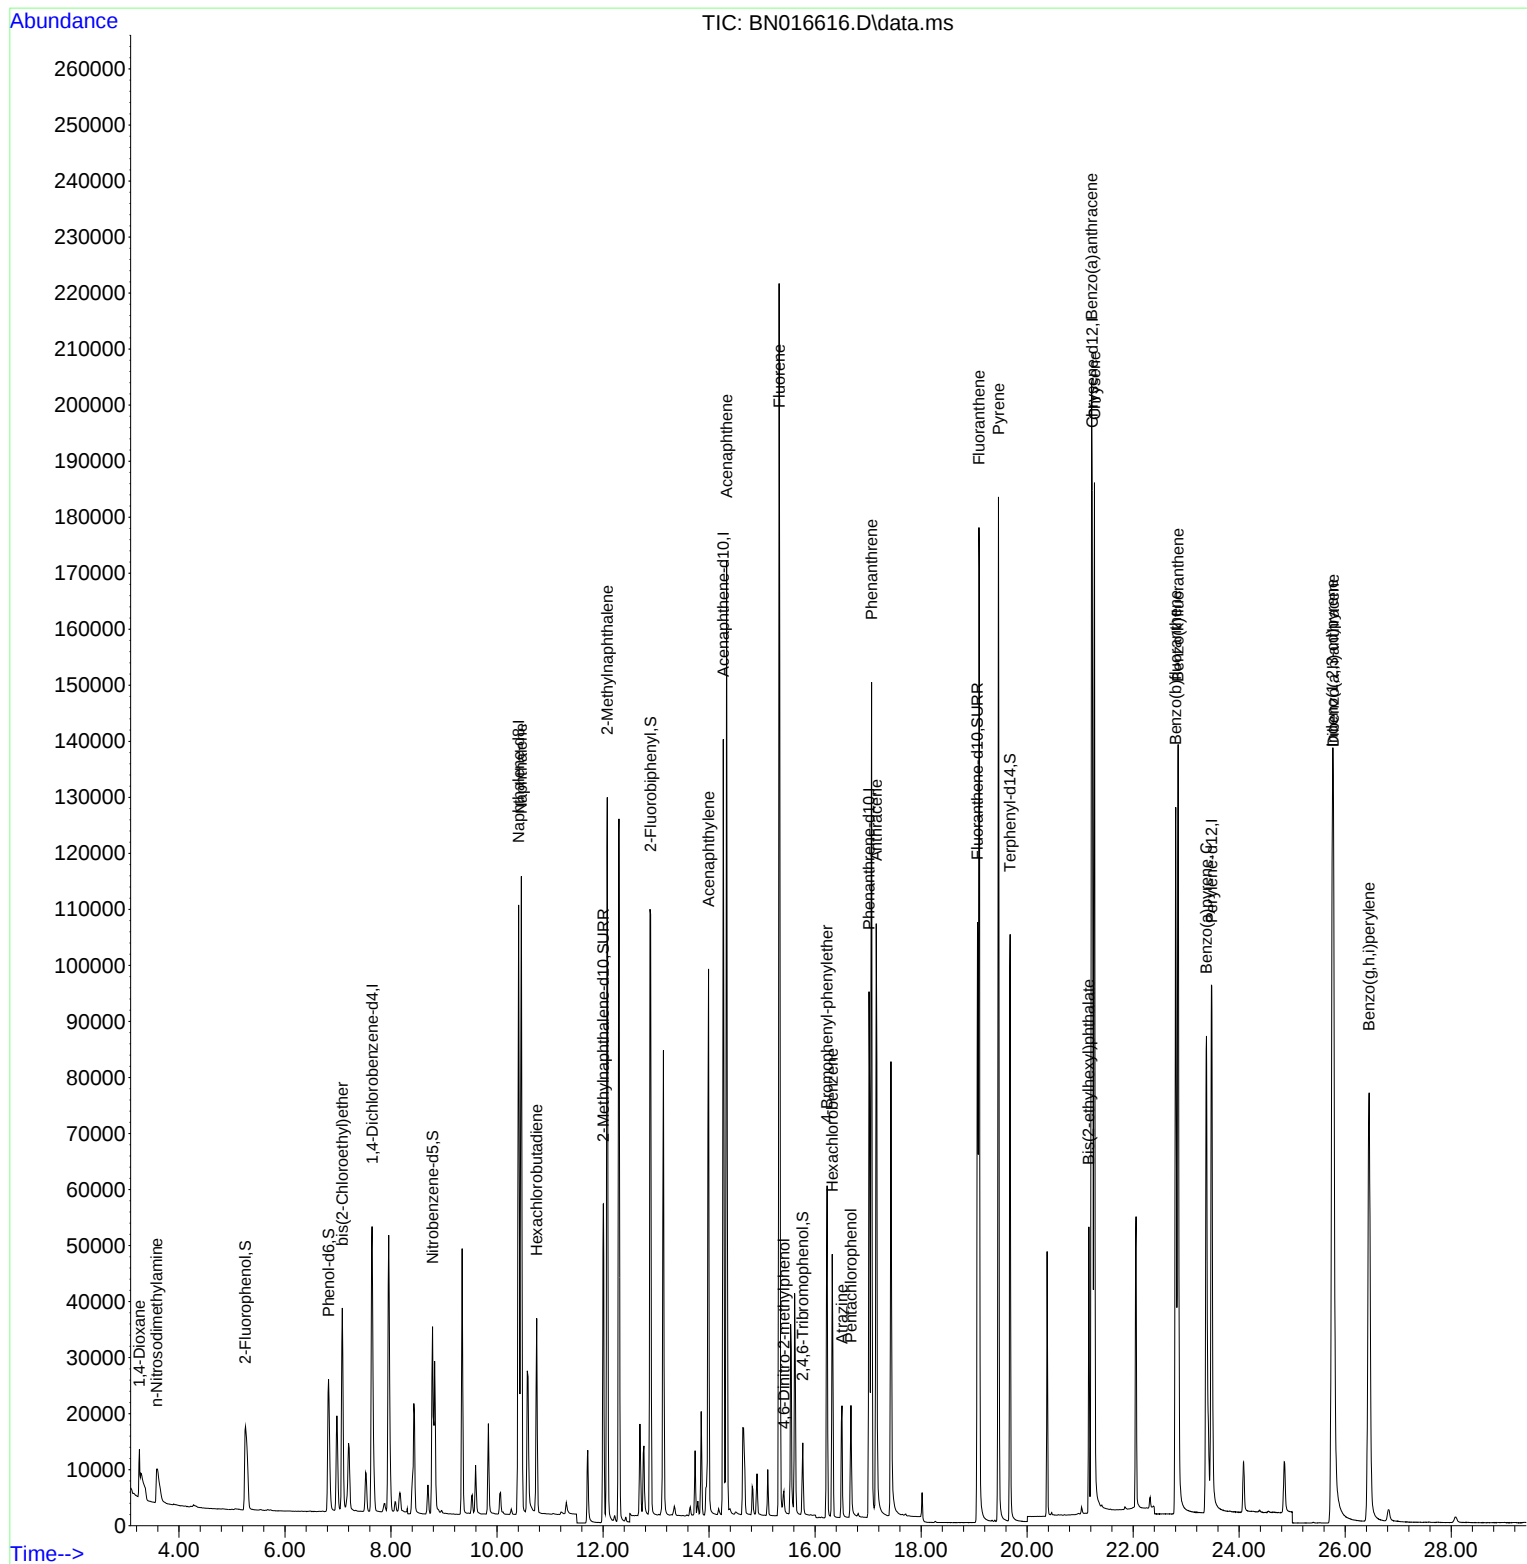




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.642 min Scan# 495
 Delta R.T. 0.000 min
 Lab File: BN016616.D
 Acq: 01 Oct 2021 02:23




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion:152 Resp: 33291
 Ion Ratio Lower Upper
 152 100
 150 155.5 124.6 186.8
 115 57.3 46.5 69.7

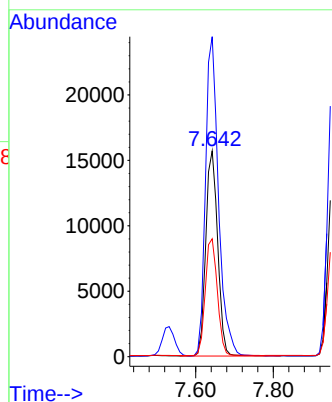

#2
 1,4-Dioxane
 Concen: 0.37 ng
 RT: 3.253 min Scan# 19
 Delta R.T. 0.000 min
 Lab File: BN016616.D
 Acq: 01 Oct 2021 02:23

Tgt Ion: 88 Resp: 5718
 Ion Ratio Lower Upper
 88 100
 43 23.8 37.8 56.8#
 58 65.2 61.3 91.9









#3
n-Nitrosodimethylamine
Concen: 0.36 ng
RT: 3.576 min Scan# 54
Delta R.T. 0.000 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion: 42 Resp: 8859
Ion Ratio Lower Upper
42 100
74 149.8 121.6 182.4
44 6.7 6.3 9.5



#4
2-Fluorophenol
Concen: 0.35 ng
RT: 5.254 min Scan# 236
Delta R.T. 0.000 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23

Tgt Ion: 112 Resp: 29689
Ion Ratio Lower Upper
112 100
64 53.8 43.1 64.7
63 27.2 21.6 32.4


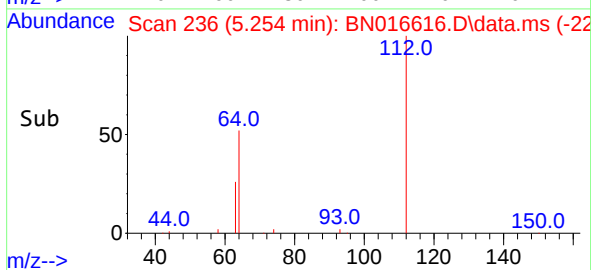






#5
Phenol-d6
Concen: 0.34 ng
RT: 6.822 min Scan# 406
Delta R.T. 0.000 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion: 99 Resp: 31906
Ion Ratio Lower Upper
99 100
42 16.6 13.0 19.6
71 29.5 23.5 35.3

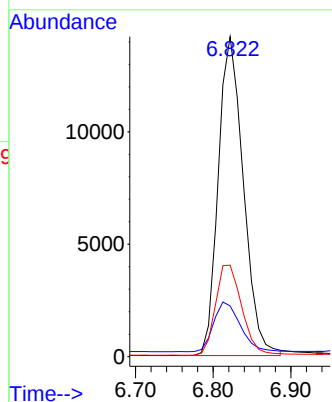

#6
bis(2-Chloroethyl)ether
Concen: 0.38 ng
RT: 7.080 min Scan# 434
Delta R.T. 0.000 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23


Tgt Ion: 93 Resp: 34237
Ion Ratio Lower Upper
93 100
63 73.9 59.1 88.7
95 32.9 26.2 39.4








#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.407 min Scan# 733
Delta R.T. 0.000 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4



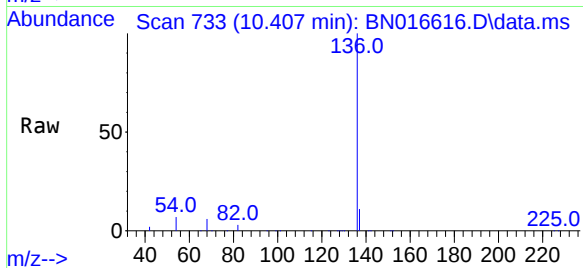



Tgt Ion:	136	Resp:	144903
Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.7	13.1
54	6.6	5.9	8.9
68	5.6	5.0	7.6



#8
Nitrobenzene-d5
Concen: 0.32 ng
RT: 8.784 min Scan# 605
Delta R.T. 0.000 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23

Tgt Ion:	82	Resp:	30216
Ion	Ratio	Lower	Upper
82	100		
128	43.6	33.6	50.4
54	45.5	37.6	56.4


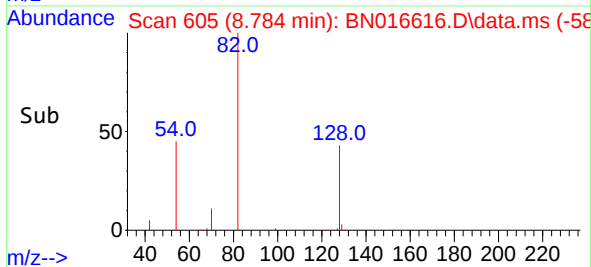

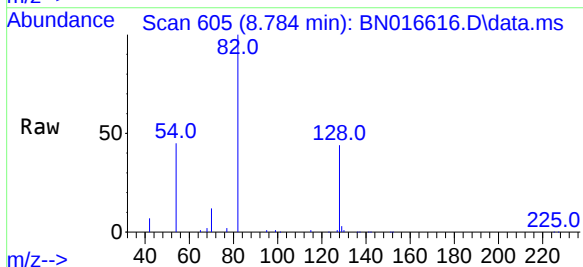




#9
Naphthalene
Concen: 0.37 ng
RT: 10.457 min Scan# 737
Delta R.T. 0.000 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:128 Resp: 146411
Ion Ratio Lower Upper
128 100
129 10.9 8.8 13.2
127 12.9 10.3 15.5

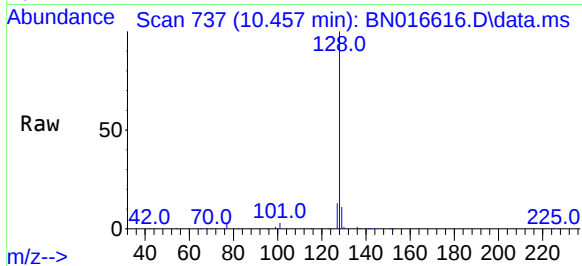

#10
Hexachlorobutadiene
Concen: 0.38 ng
RT: 10.749 min Scan# 760
Delta R.T. 0.000 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23

Tgt Ion:225 Resp: 28116
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.0 51.0 76.6


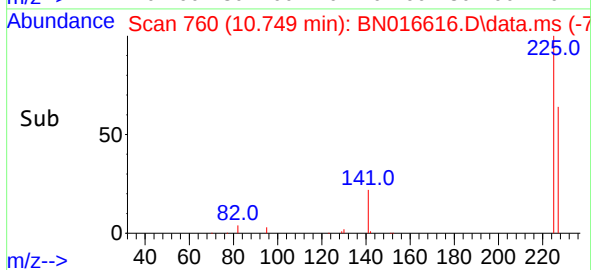

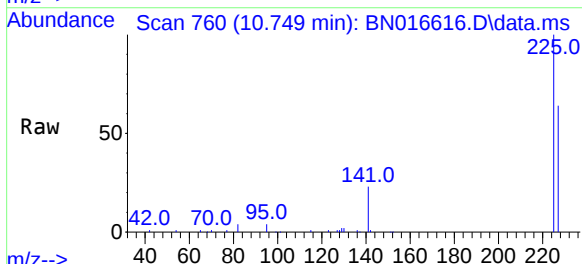


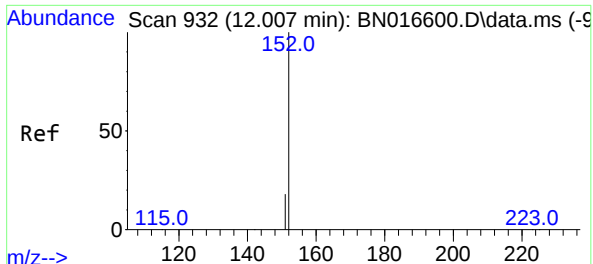

#11
2-Methylnaphthalene-d10
Concen: 0.37 ng
RT: 12.003 min Scan# 931
Delta R.T. -0.004 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 79610
Ion Ratio Lower Upper
152 100
151 20.3 16.2 24.4

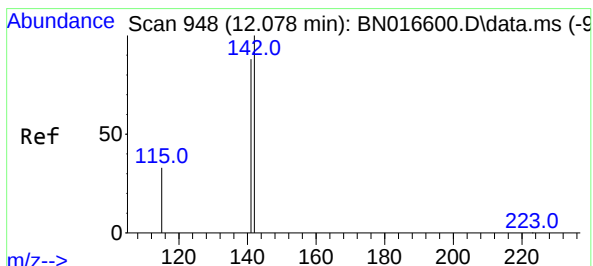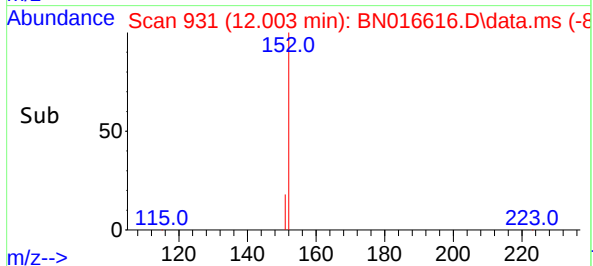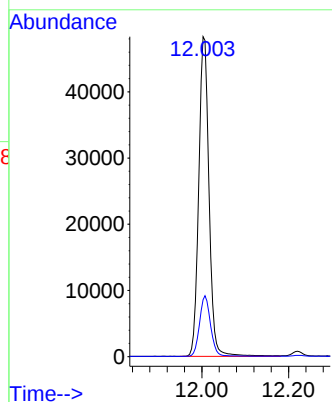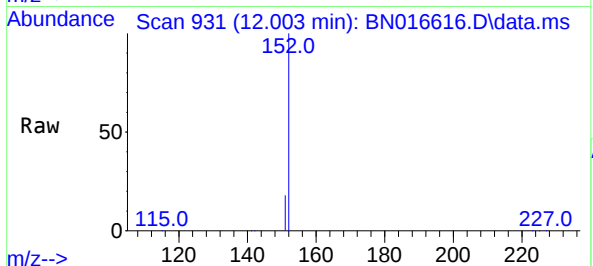

#12
2-Methylnaphthalene
Concen: 0.38 ng
RT: 12.078 min Scan# 948
Delta R.T. 0.000 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23

Tgt Ion:142 Resp: 95219
Ion Ratio Lower Upper
142 100
141 87.5 70.6 105.8
115 32.4 26.6 39.8


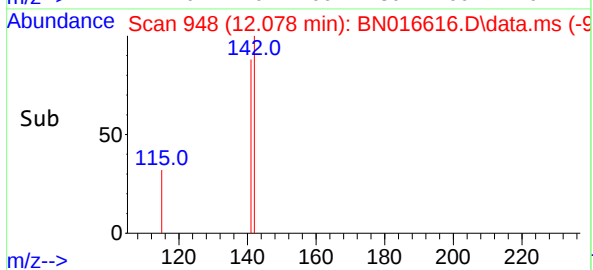
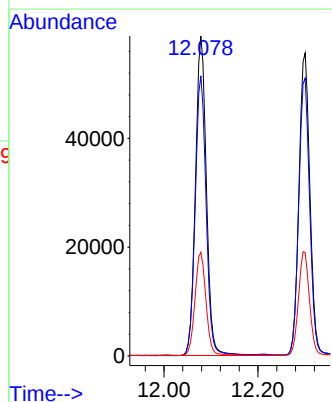
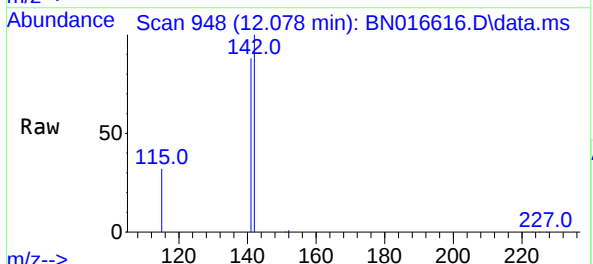




#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.269 min Scan# 1183
Delta R.T. 0.000 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:164 Resp: 75533
Ion Ratio Lower Upper
164 100
162 101.8 82.2 123.2
160 46.3 37.7 56.5

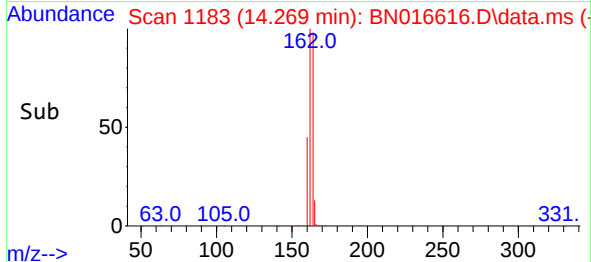

#14
2,4,6-Tribromophenol
Concen: 0.31 ng
RT: 15.766 min Scan# 1301
Delta R.T. 0.000 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23

Tgt Ion:330 Resp: 10649
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 31.0 25.2 37.8


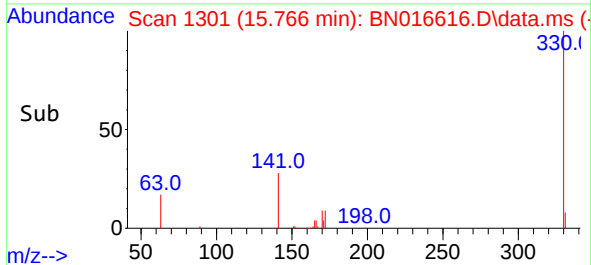

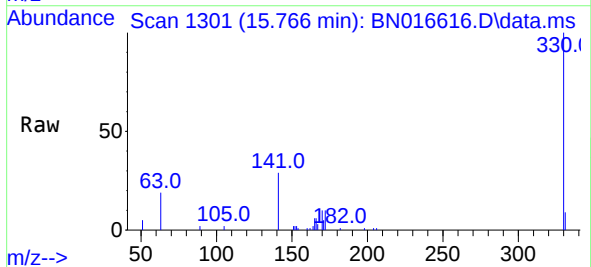




#15
2-Fluorobiphenyl
Concen: 0.37 ng
RT: 12.898 min Scan# 1075
Delta R.T. 0.000 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:172 Resp: 112943
Ion Ratio Lower Upper
172 100
171 33.3 27.0 40.4
170 21.4 17.4 26.2



#16
Acenaphthylene
Concen: 0.34 ng
RT: 13.990 min Scan# 1161
Delta R.T. 0.000 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23

Tgt Ion:152 Resp: 113830
Ion Ratio Lower Upper
152 100
151 19.4 15.5 23.3
153 13.0 10.4 15.6


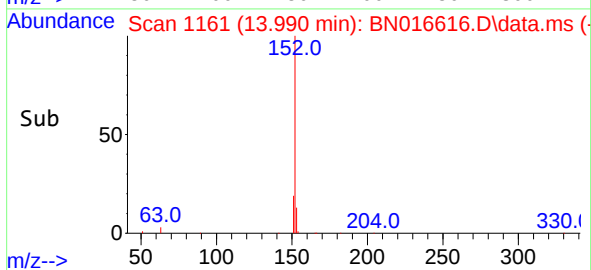






#17
Acenaphthene
Concen: 0.36 ng
RT: 14.332 min Scan# 1188
Delta R.T. 0.000 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:154 Resp: 80961
Ion Ratio Lower Upper
154 100
153 114.0 90.2 135.2
152 56.2 44.0 66.0

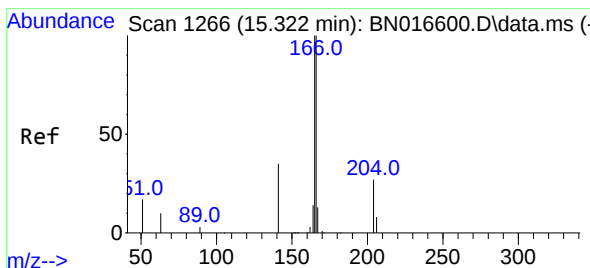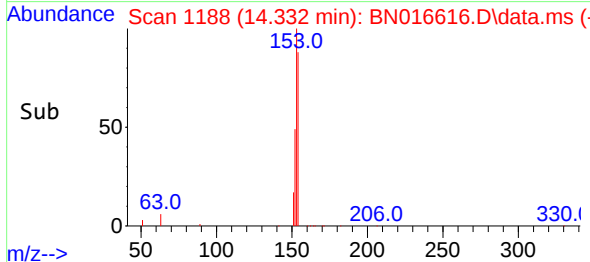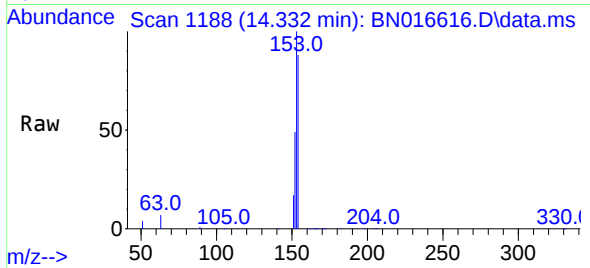

#18
Fluorene
Concen: 0.37 ng
RT: 15.322 min Scan# 1266
Delta R.T. 0.000 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23


Tgt Ion:166 Resp: 97214
Ion Ratio Lower Upper
166 100
165 97.5 77.9 116.9
167 13.4 10.7 16.1

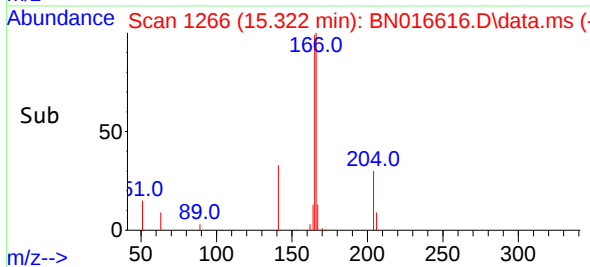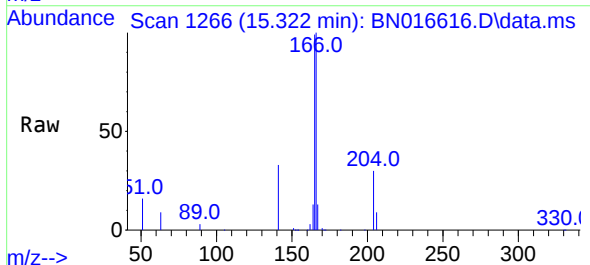






#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.017 min Scan# 1403
Delta R.T. -0.012 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4



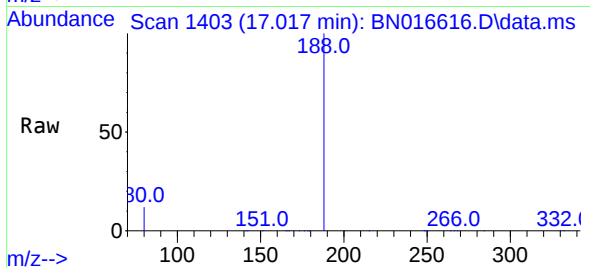



Tgt Ion:188 Resp: 135439
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 12.4 5.0 7.6#

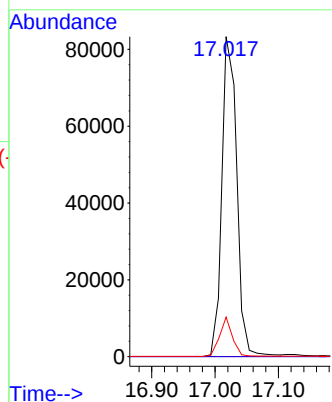

#20
4,6-Dinitro-2-methylphenol
Concen: 0.32 ng
RT: 15.411 min Scan# 1273
Delta R.T. 0.001 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23

Tgt Ion:198 Resp: 3263
Ion Ratio Lower Upper
198 100
182 14.0 11.8 17.8
77 0.0 0.0 0.0


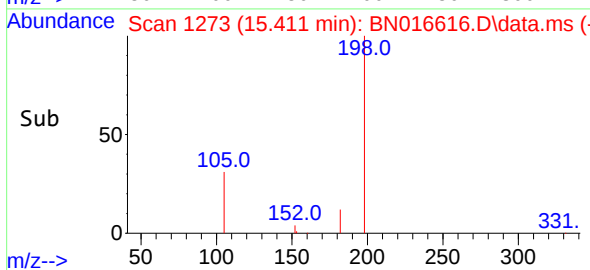






#21
4-Bromophenyl-phenylether
Concen: 0.36 ng
RT: 16.226 min Scan# 1338
Delta R.T. 0.000 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:248 Resp: 30506
Ion Ratio Lower Upper
248 100
250 100.6 78.6 117.8
141 41.9 38.6 57.8



#22
Hexachlorobenzene
Concen: 0.38 ng
RT: 16.324 min Scan# 1346
Delta R.T. -0.012 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23

Tgt Ion:284 Resp: 37321
Ion Ratio Lower Upper
284 100
142 32.6 26.4 39.6
249 29.1 23.4 35.2


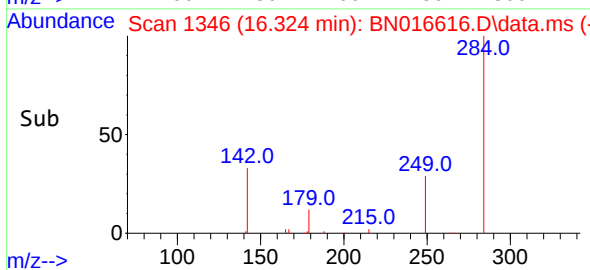






#23
Atrazine
Concen: 0.30 ng
RT: 16.506 min Scan# 1361
Delta R.T. 0.000 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:200 Resp: 18425
Ion Ratio Lower Upper
200 100
173 22.2 18.6 27.8
215 48.8 39.4 59.2



#24
Pentachlorophenol
Concen: 0.33 ng
RT: 16.677 min Scan# 1375
Delta R.T. 0.000 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23

Tgt Ion:266 Resp: 10567
Ion Ratio Lower Upper
266 100
264 62.5 49.8 74.6
268 63.9 51.4 77.2


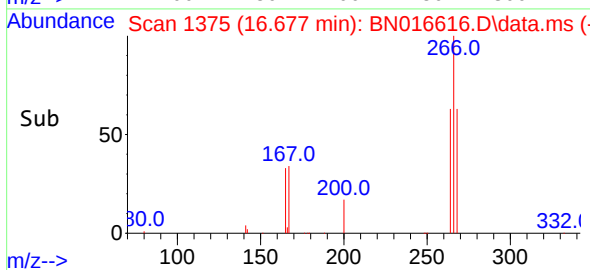






#25
Phenanthrene
Concen: 0.38 ng
RT: 17.066 min Scan# 1407
Delta R.T. 0.000 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:178 Resp: 154084
Ion Ratio Lower Upper
178 100
176 18.9 15.0 22.4
179 15.5 12.2 18.4



#26
Anthracene
Concen: 0.35 ng
RT: 17.151 min Scan# 1414
Delta R.T. 0.000 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23

Tgt Ion:178 Resp: 123148
Ion Ratio Lower Upper
178 100
176 18.2 14.6 21.8
179 15.2 12.2 18.4


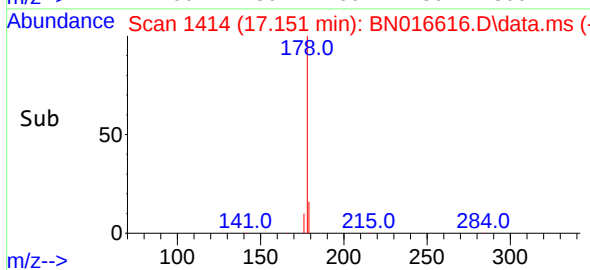






#27
Fluoranthene-d10
Concen: 0.36 ng
RT: 19.063 min Scan# 1696
Delta R.T. -0.005 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:212 Resp: 129381
Ion Ratio Lower Upper
212 100
106 13.4 10.6 16.0
104 7.3 5.9 8.9

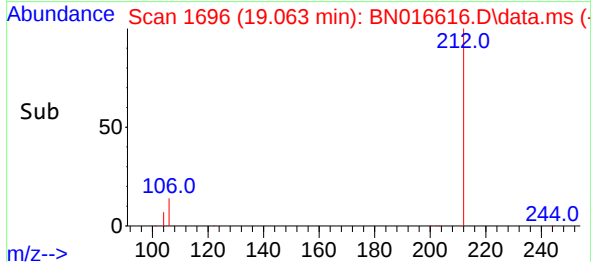

#28
Fluoranthene
Concen: 0.38 ng
RT: 19.093 min Scan# 1702
Delta R.T. -0.005 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23

Tgt Ion:202 Resp: 165011
Ion Ratio Lower Upper
202 100
101 11.1 9.0 13.4
203 17.4 13.8 20.6


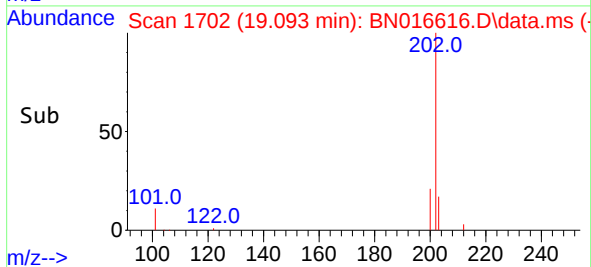

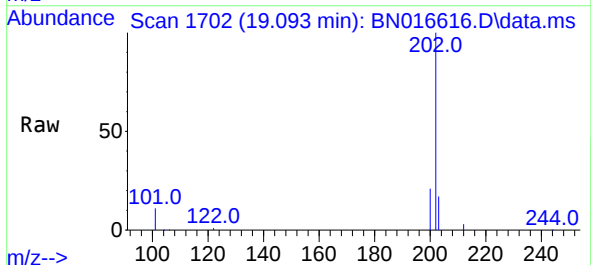




#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.227 min Scan# 2001
Delta R.T. -0.010 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:240 Resp: 125841
Ion Ratio Lower Upper
240 100
120 11.4 5.0 7.4#
236 26.4 20.4 30.6

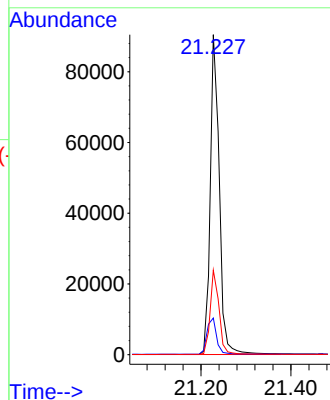

#30
Pyrene
Concen: 0.40 ng
RT: 19.460 min Scan# 1776
Delta R.T. 0.000 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23

Tgt Ion:202 Resp: 162095
Ion Ratio Lower Upper
202 100
200 20.6 16.5 24.7
203 17.4 14.0 21.0


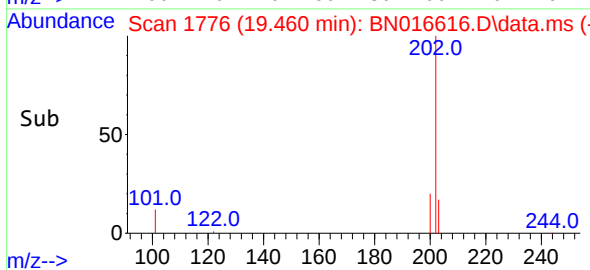
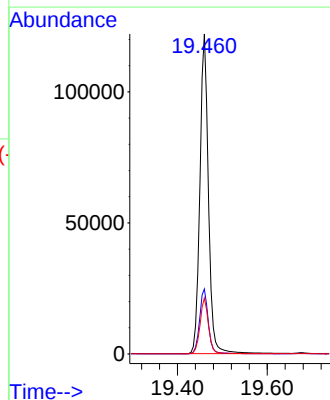





#31
Terphenyl-d14
Concen: 0.40 ng
RT: 19.678 min Scan# 1820
Delta R.T. 0.000 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:244 Resp: 109044
Ion Ratio Lower Upper
244 100
212 7.2 6.0 9.0
122 11.5 10.1 15.1

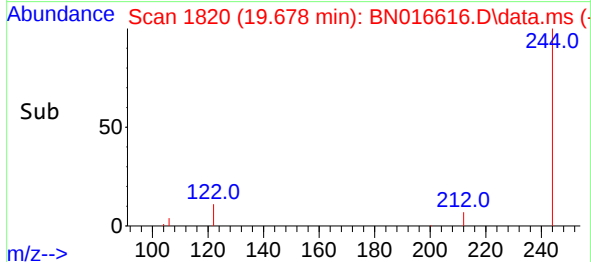

#32
Benzo(a)anthracene
Concen: 0.36 ng
RT: 21.217 min Scan# 2000
Delta R.T. 0.000 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23

Tgt Ion:228 Resp: 139962
Ion Ratio Lower Upper
228 100
226 26.2 21.9 32.9
229 19.9 15.7 23.5



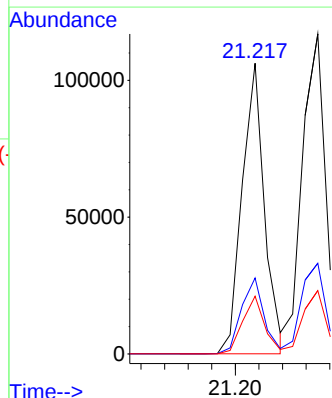





#33
Chrysene
Concen: 0.42 ng
RT: 21.270 min Scan# 2005
Delta R.T. 0.000 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:228 Resp: 165316
Ion Ratio Lower Upper
228 100
226 28.4 23.7 35.5
229 19.8 15.5 23.3



#34
Bis(2-ethylhexyl)phthalate
Concen: 0.29 ng
RT: 21.164 min Scan# 1995
Delta R.T. -0.010 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23


Tgt Ion:149 Resp: 44365
Ion Ratio Lower Upper
149 100
167 27.1 22.2 33.4
279 4.0 3.2 4.8

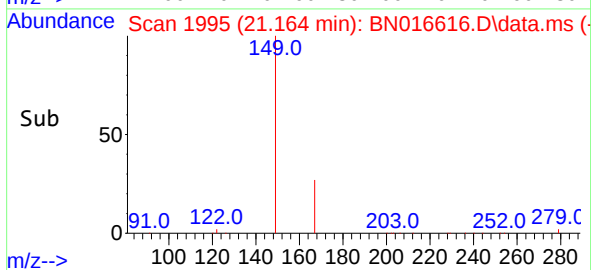






#35
Perylene-d12
Concen: 0.40 ng
RT: 23.481 min Scan# 2426
Delta R.T. -0.007 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4







Tgt Ion:264 Resp: 132252
Ion Ratio Lower Upper
264 100
260 24.6 19.9 29.9
265 23.1 19.2 28.8

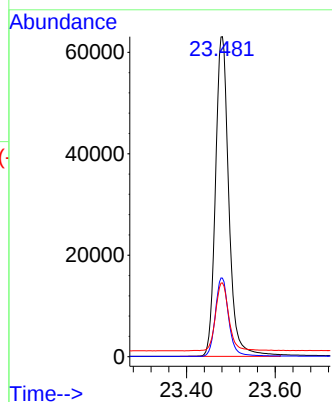

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.41 ng
RT: 25.757 min Scan# 3091
Delta R.T. -0.007 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23


Tgt Ion:276 Resp: 191152
Ion Ratio Lower Upper
276 100
138 25.3 19.5 29.3
277 25.0 19.9 29.9

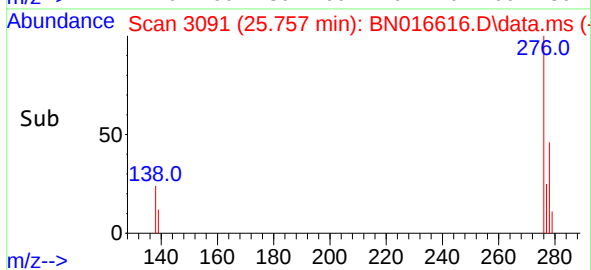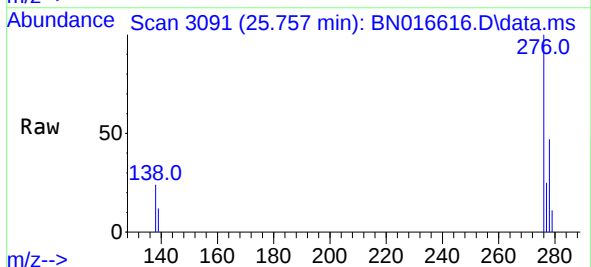






#37
Benzo(b)fluoranthene
Concen: 0.37 ng
RT: 22.803 min Scan# 2228
Delta R.T. -0.007 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4







Tgt Ion:252 Resp: 155467
Ion Ratio Lower Upper
252 100
253 22.3 17.8 26.8
125 9.9 8.0 12.0

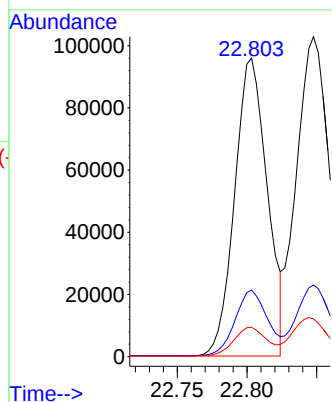

#38
Benzo(k)fluoranthene
Concen: 0.40 ng
RT: 22.848 min Scan# 2241
Delta R.T. -0.007 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23


Tgt Ion:252 Resp: 169940
Ion Ratio Lower Upper
252 100
253 22.4 17.8 26.6
125 11.8 8.0 12.0

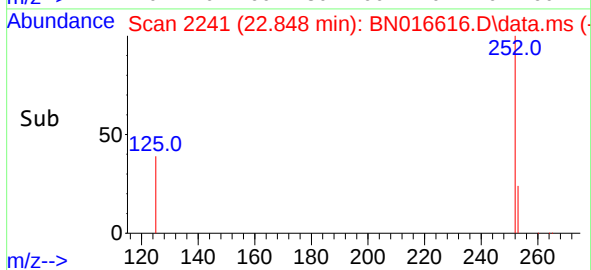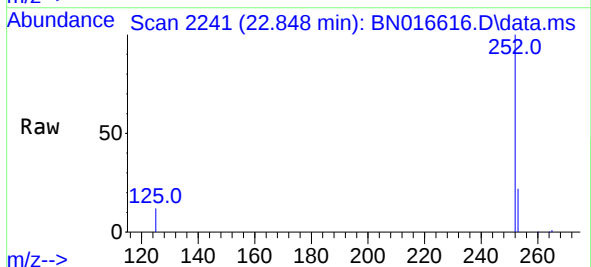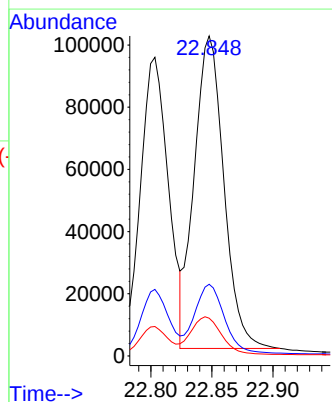






#39
Benzo(a)pyrene
Concen: 0.37 ng
RT: 23.382 min Scan# 2397
Delta R.T. -0.007 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4







Tgt Ion:252 Resp: 141604
Ion Ratio Lower Upper
252 100
253 22.2 17.8 26.8
125 11.0 9.0 13.4

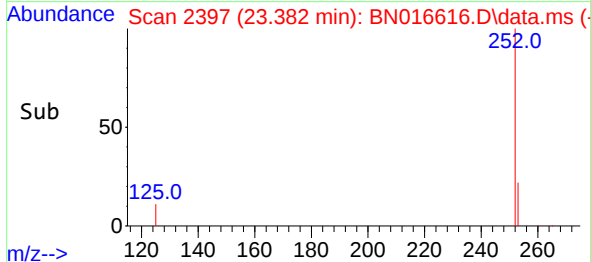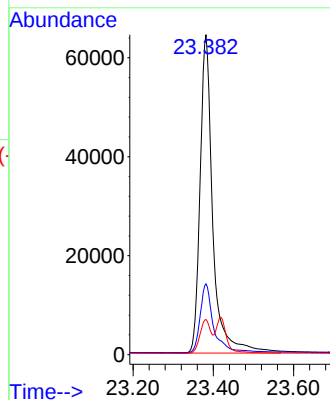

#40
Dibenzo(a,h)anthracene
Concen: 0.40 ng
RT: 25.778 min Scan# 3097
Delta R.T. -0.010 min
Lab File: BN016616.D
Acq: 01 Oct 2021 02:23

Tgt Ion:278 Resp: 153266
Ion Ratio Lower Upper
278 100
139 17.6 13.1 19.7
279 23.8 19.1 28.7

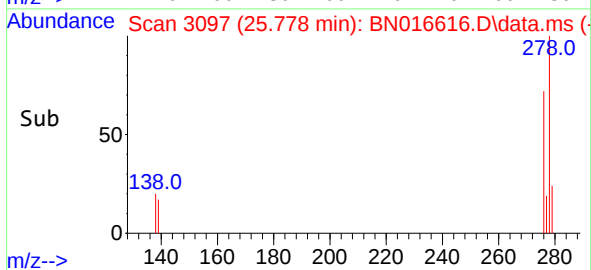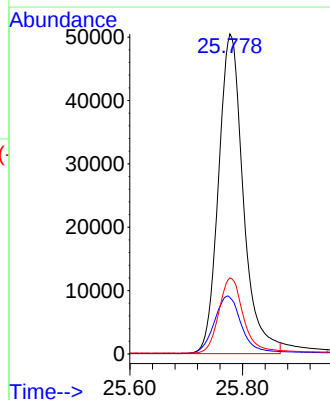

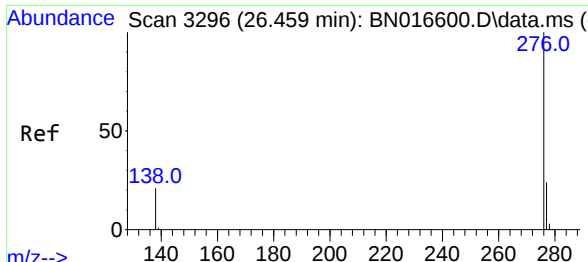

#41
 Benzo(g,h,i)perylene
 Concen: 0.40 ng
 RT: 26.452 min Scan# 3294
 Delta R.T. -0.007 min
 Lab File: BN016616.D
 Acq: 01 Oct 2021 02:23

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Tgt Ion:	276	Resp:	164989
Ion	Ratio	Lower	Upper
276	100		
277	23.6	19.0	28.6
138	21.0	16.9	25.3

