

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100121\
 Data File : BN016629.D
 Acq On : 01 Oct 2021 10:10
 Operator : CG/JU
 Sample : M3833-18
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE126D3-20210920

Quant Time: Oct 01 11:02:24 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 30 17:56:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.642	152	27315	0.40	ng	0.00
7) Naphthalene-d8	10.407	136	124559	0.40	ng	0.00
13) Acenaphthene-d10	14.269	164	66266	0.40	ng	0.00
19) Phenanthrene-d10	17.017	188	129026	0.40	ng	#-0.01
29) Chrysene-d12	21.238	240	117060	0.40	ng	0.00
35) Perylene-d12	23.484	264	116863	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.273	112	7127	0.10	ng	0.02
5) Phenol-d6	6.831	99	4100	0.05	ng	0.00
8) Nitrobenzene-d5	8.784	82	18479	0.23	ng	0.00
11) 2-Methylnaphthalene-d10	12.003	152	54028	0.29	ng	0.00
14) 2,4,6-Tribromophenol	15.766	330	8054	0.27	ng	0.00
15) 2-Fluorobiphenyl	12.898	172	69444	0.26	ng	0.00
27) Fluoranthene-d10	19.063	212	132338	0.39	ng	0.00
31) Terphenyl-d14	19.678	244	97432	0.38	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.263	88	2075	0.17	ng	# 81
34) Bis(2-ethylhexyl)phtha...	21.164	149	17089	0.12	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100121\
Data File : BN016629.D
Acq On : 01 Oct 2021 10:10
Operator : CG/JU
Sample : M3833-18
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE126D3-20210920

Quant Time: Oct 01 11:02:24 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 17:56:53 2021
Response via : Initial Calibration

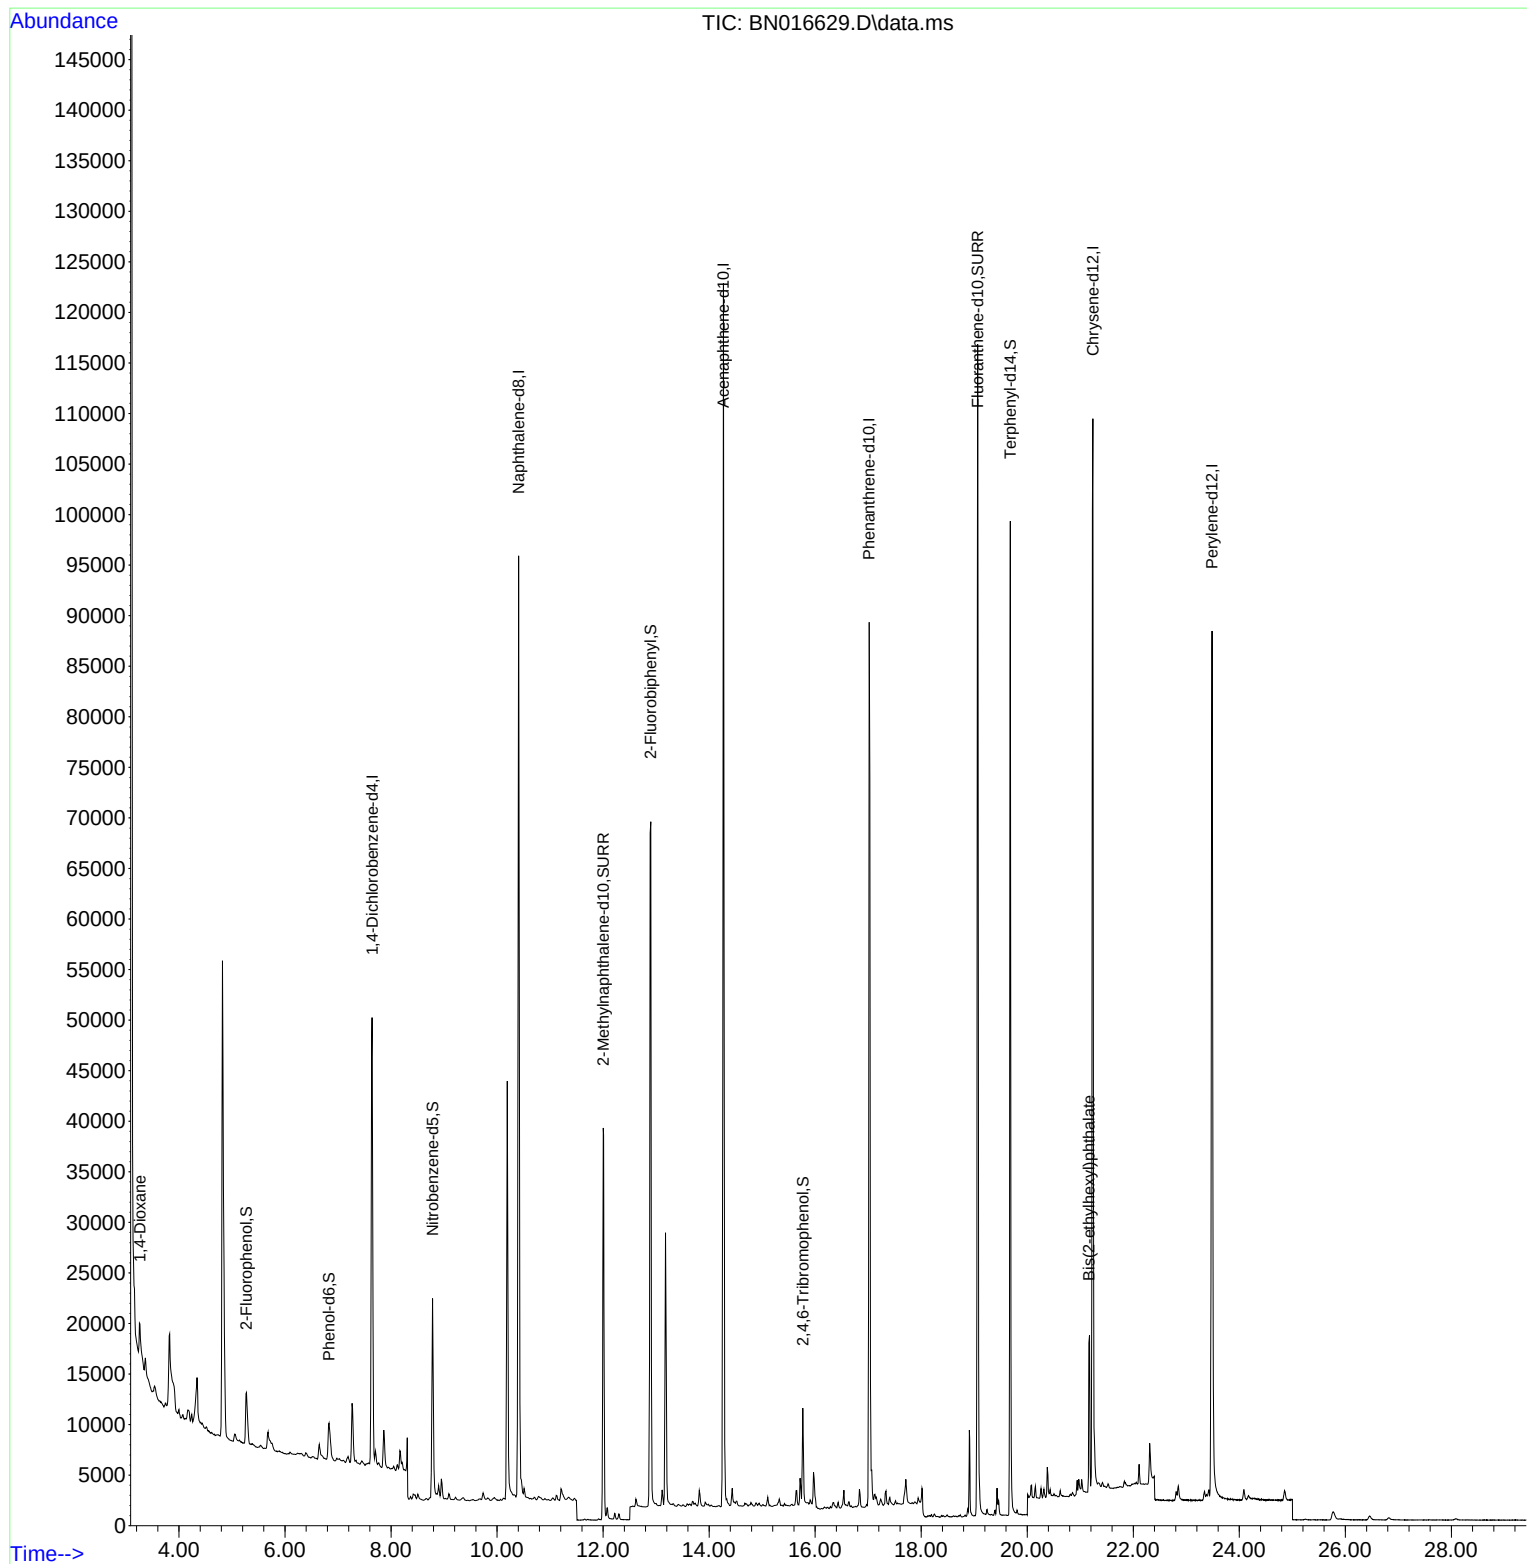




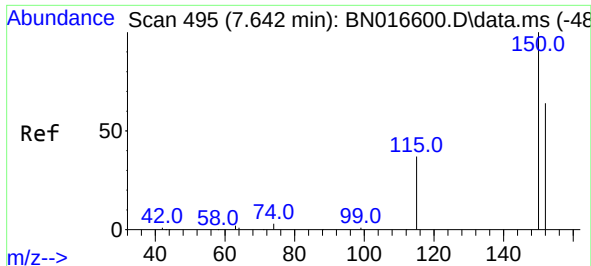


#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.642 min Scan# 495
 Delta R.T. 0.000 min
 Lab File: BN016629.D
 Acq: 01 Oct 2021 10:10

Instrument :
 BNA_N
 ClientSampleId :
 RE126D3-20210920

Tgt Ion: 152 Resp: 27315




Ion	Ratio	Lower	Upper
152	100		
150	154.2	124.6	186.8
115	57.9	46.5	69.7

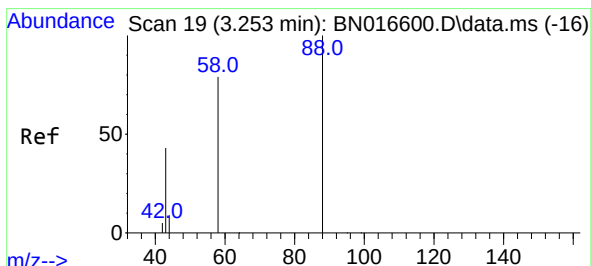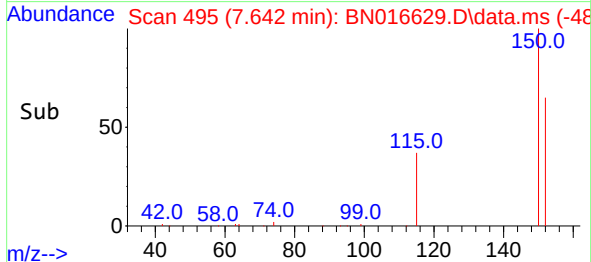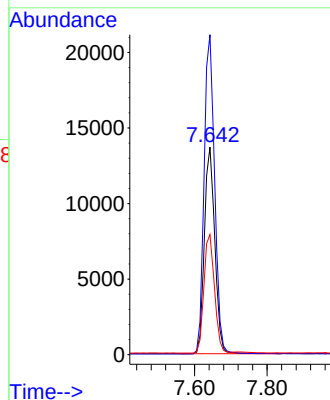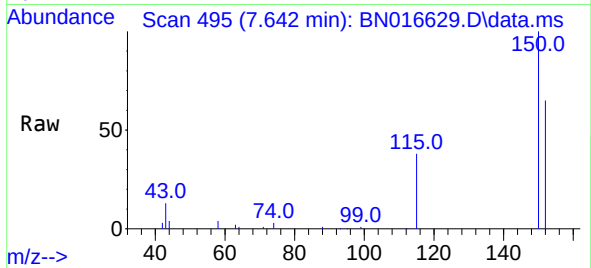


#2
 1,4-Dioxane
 Concen: 0.17 ng
 RT: 3.263 min Scan# 20
 Delta R.T. 0.009 min
 Lab File: BN016629.D
 Acq: 01 Oct 2021 10:10

Tgt Ion: 88 Resp: 2075

Ion	Ratio	Lower	Upper
88	100		
43	17.2	37.8	56.8
58	73.5	61.3	91.9


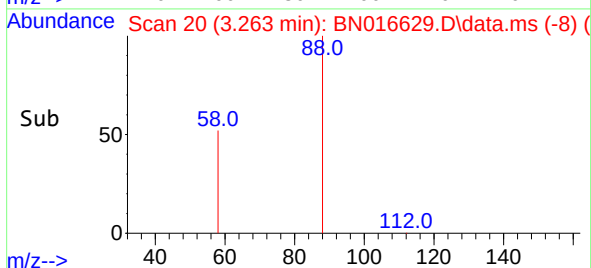
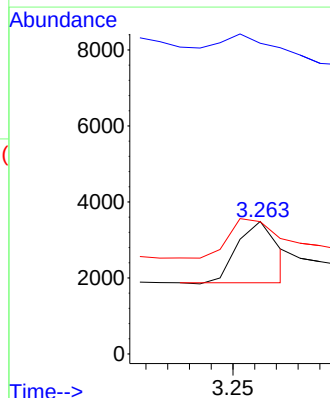
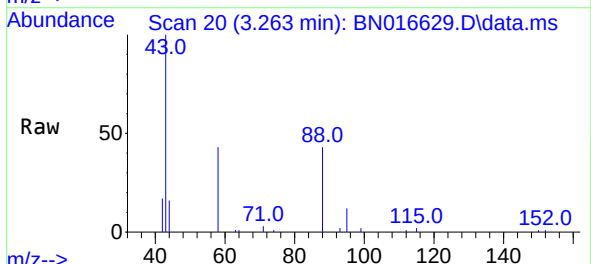


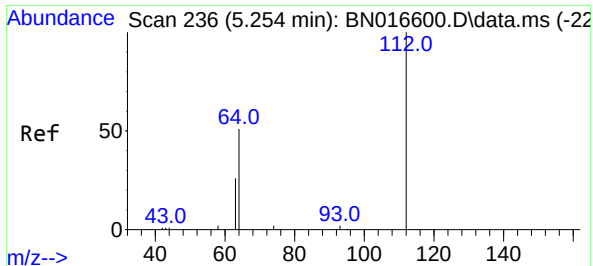

#4
2-Fluorophenol
Concen: 0.10 ng
RT: 5.273 min Scan# 238
Delta R.T. 0.019 min
Lab File: BN016629.D
Acq: 01 Oct 2021 10:10




Instrument :
BNA_N
ClientSampleId :
RE126D3-20210920


Tgt Ion: 112 Resp: 7127
Ion Ratio Lower Upper
112 100
64 54.7 43.1 64.7
63 27.9 21.6 32.4

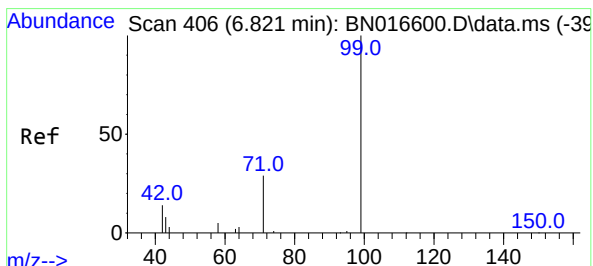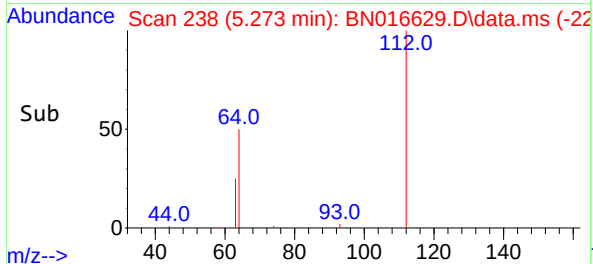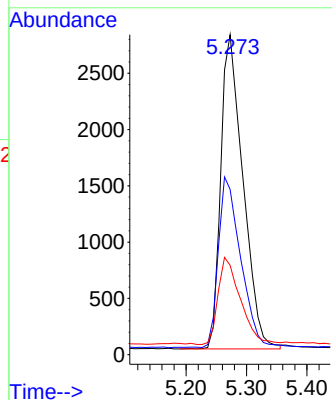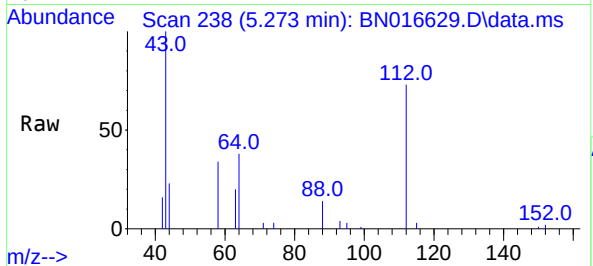

#5
Phenol-d6
Concen: 0.05 ng
RT: 6.831 min Scan# 407
Delta R.T. 0.009 min
Lab File: BN016629.D
Acq: 01 Oct 2021 10:10


Tgt Ion: 99 Resp: 4100
Ion Ratio Lower Upper
99 100
42 20.7 13.0 19.6#
71 37.6 23.5 35.3#

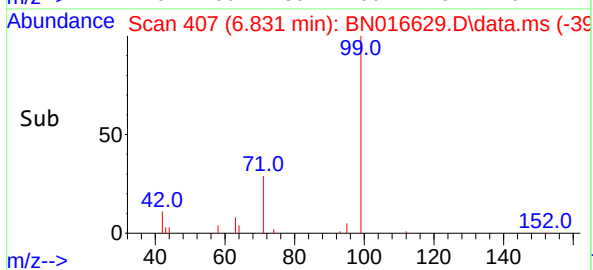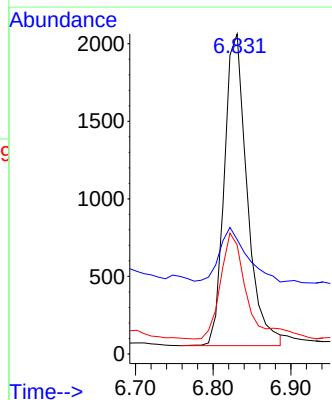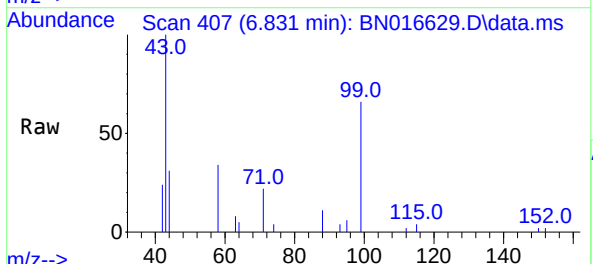



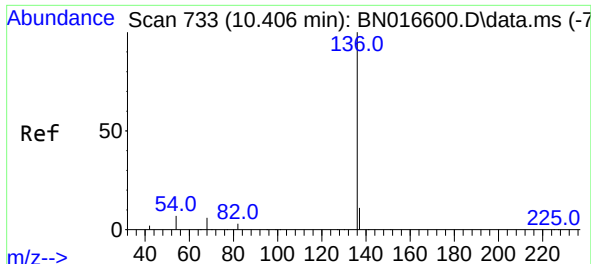


#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.407 min Scan# 733
Delta R.T. 0.000 min
Lab File: BN016629.D
Acq: 01 Oct 2021 10:10

Instrument :
BNA_N
ClientSampleId :
RE126D3-20210920



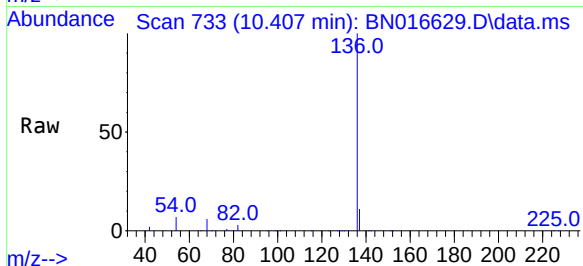



Tgt Ion:	136	Resp:	124559
Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.7	13.1
54	6.6	5.9	8.9
68	5.7	5.0	7.6

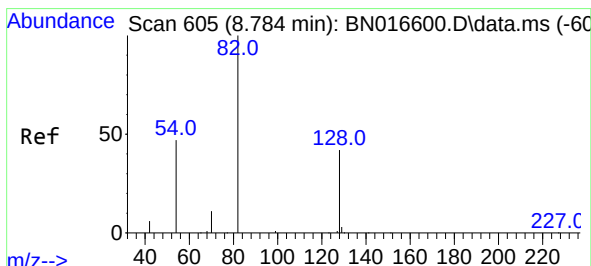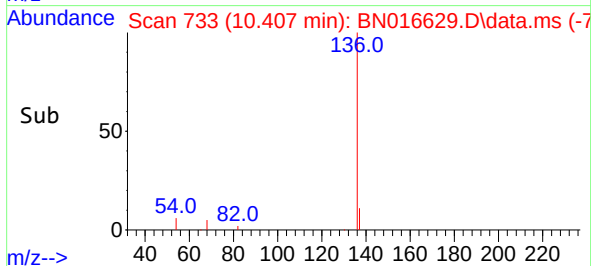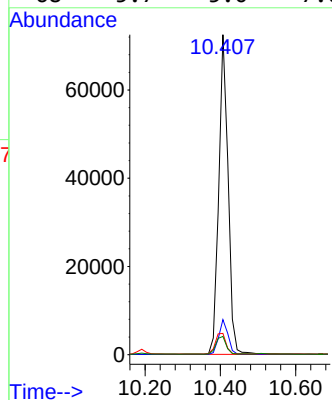

#8
Nitrobenzene-d5
Concen: 0.23 ng
RT: 8.784 min Scan# 605
Delta R.T. 0.000 min
Lab File: BN016629.D
Acq: 01 Oct 2021 10:10

Tgt Ion:	82	Resp:	18479
Ion	Ratio	Lower	Upper
82	100		
128	43.4	33.6	50.4
54	47.1	37.6	56.4


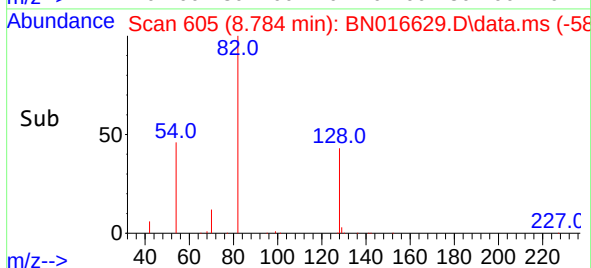
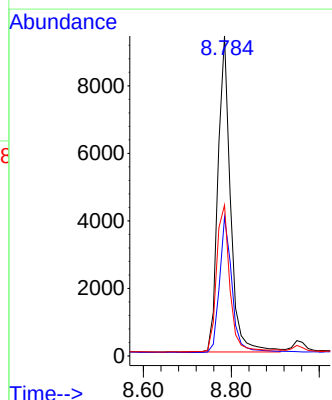
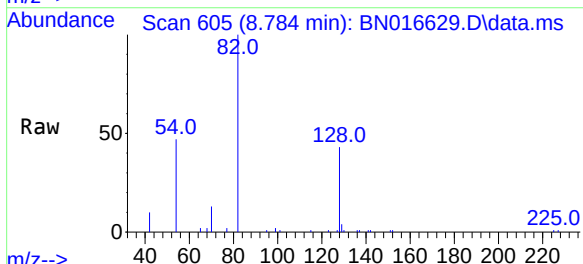


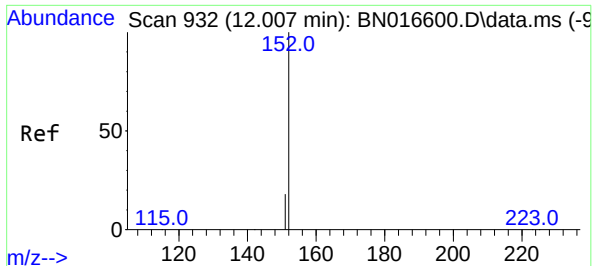

#11
2-Methylnaphthalene-d10
Concen: 0.29 ng
RT: 12.003 min Scan# 931
Delta R.T. -0.004 min
Lab File: BN016629.D
Acq: 01 Oct 2021 10:10




Instrument :
BNA_N
ClientSampleId :
RE126D3-20210920


Tgt Ion:152 Resp: 54028
Ion Ratio Lower Upper
152 100
151 20.6 16.2 24.4

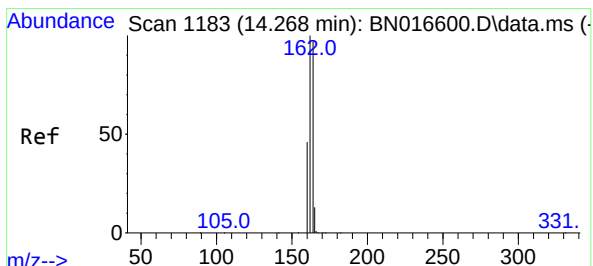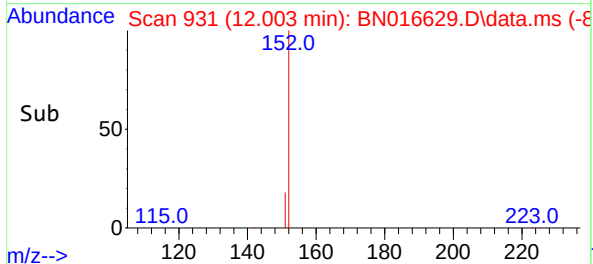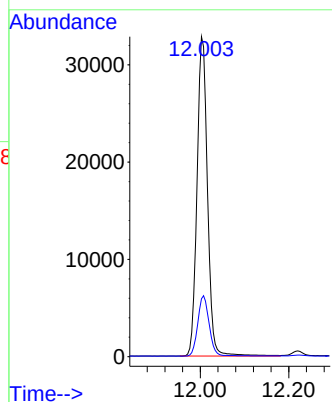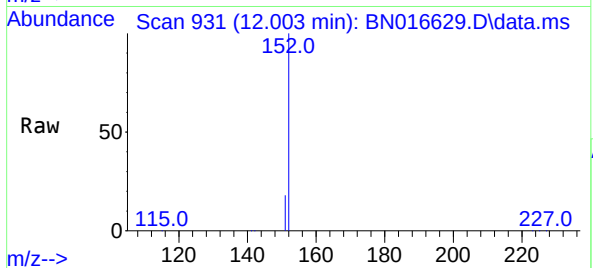

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.269 min Scan# 1183
Delta R.T. 0.000 min
Lab File: BN016629.D
Acq: 01 Oct 2021 10:10

Tgt Ion:164 Resp: 66266
Ion Ratio Lower Upper
164 100
162 102.5 82.2 123.2
160 46.5 37.7 56.5


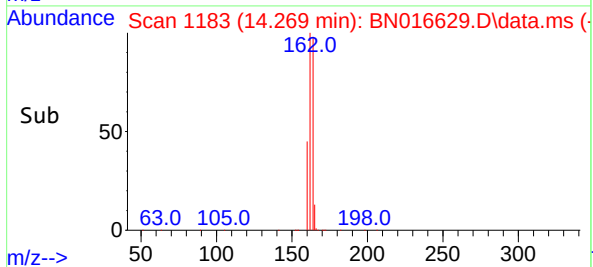
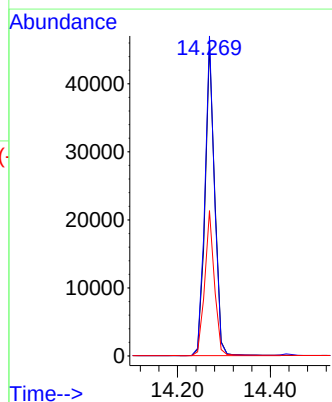
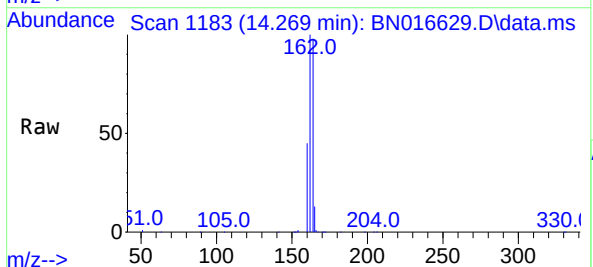


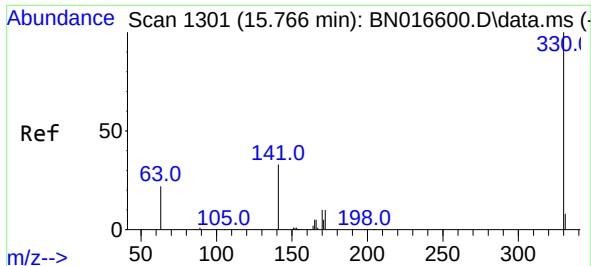

#14
2,4,6-Tribromophenol
Concen: 0.27 ng
RT: 15.766 min Scan# 1301
Delta R.T. 0.000 min
Lab File: BN016629.D
Acq: 01 Oct 2021 10:10




Instrument :
BNA_N
ClientSampleId :
RE126D3-20210920


Tgt Ion:330 Resp: 8054
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 30.8 25.2 37.8

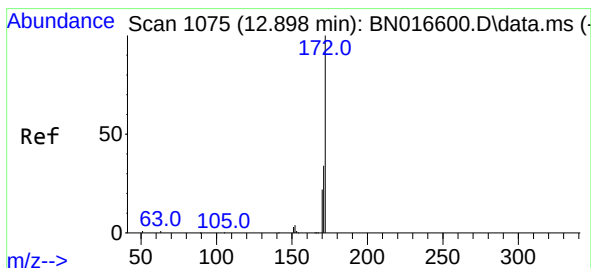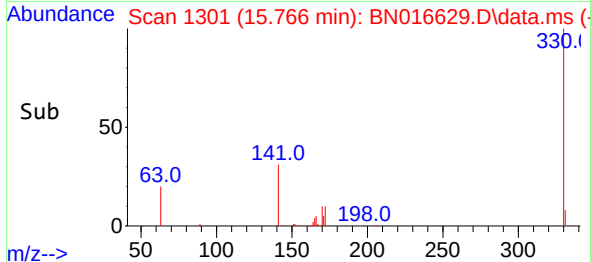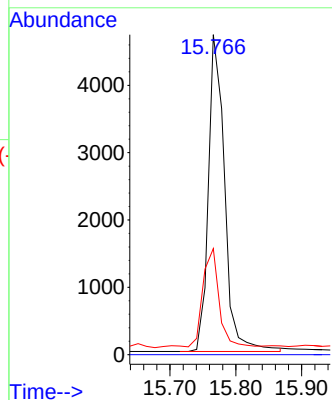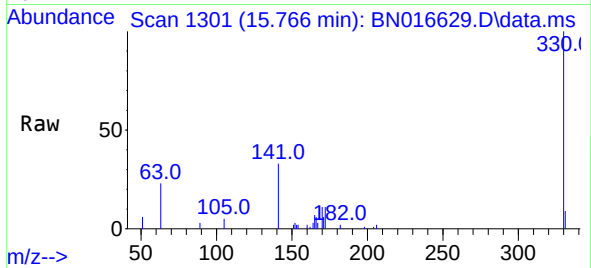

#15
2-Fluorobiphenyl
Concen: 0.26 ng
RT: 12.898 min Scan# 1075
Delta R.T. 0.000 min
Lab File: BN016629.D
Acq: 01 Oct 2021 10:10

Tgt Ion:172 Resp: 69444
Ion Ratio Lower Upper
172 100
171 33.2 27.0 40.4
170 21.3 17.4 26.2


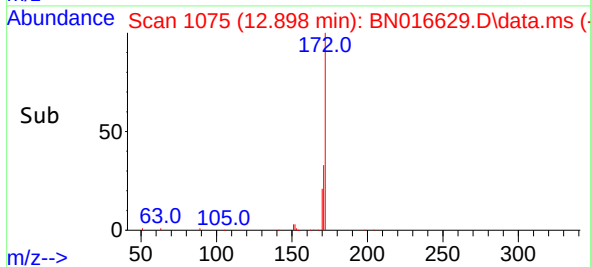
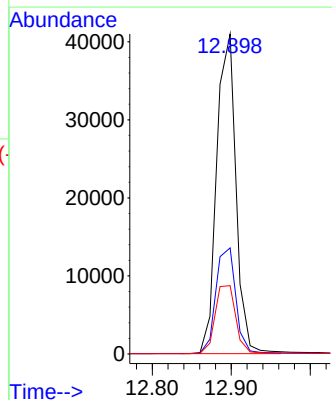
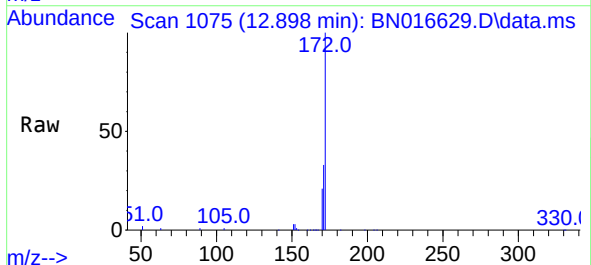


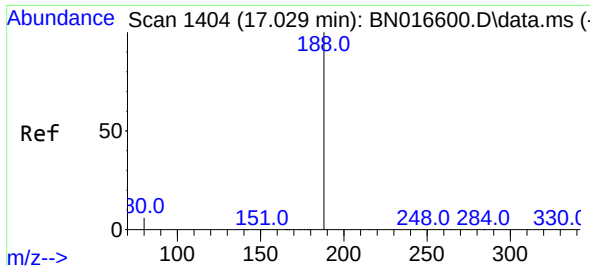

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.017 min Scan# 1403
Delta R.T. -0.012 min
Lab File: BN016629.D
Acq: 01 Oct 2021 10:10




Instrument :
BNA_N
ClientSampleId :
RE126D3-20210920


Tgt Ion:188 Resp: 129026
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 12.3 5.0 7.6#

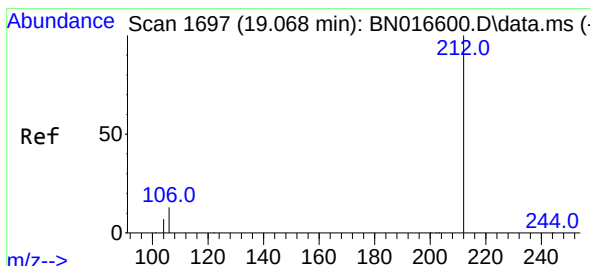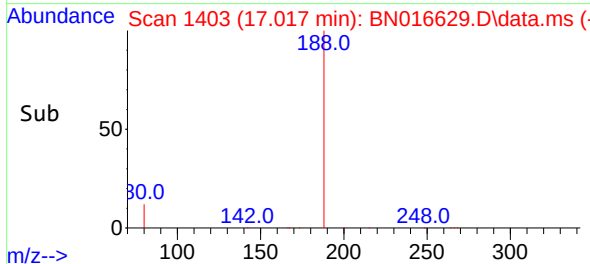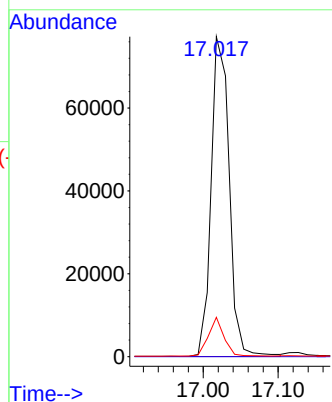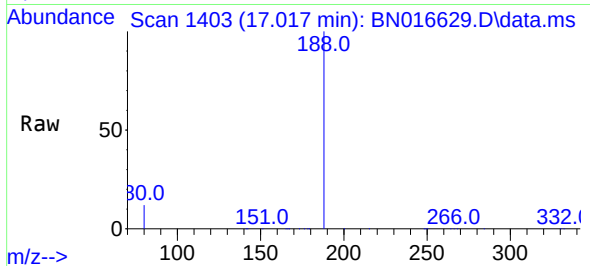

#27
Fluoranthene-d10
Concen: 0.39 ng
RT: 19.063 min Scan# 1696
Delta R.T. -0.005 min
Lab File: BN016629.D
Acq: 01 Oct 2021 10:10

Tgt Ion:212 Resp: 132338
Ion Ratio Lower Upper
212 100
106 13.3 10.6 16.0
104 7.2 5.9 8.9


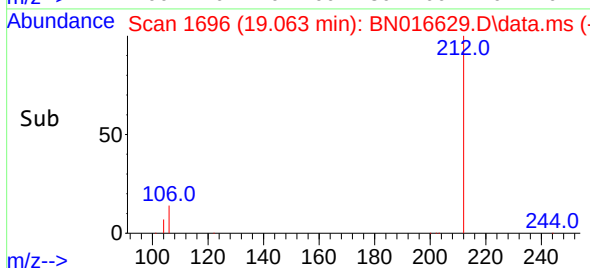
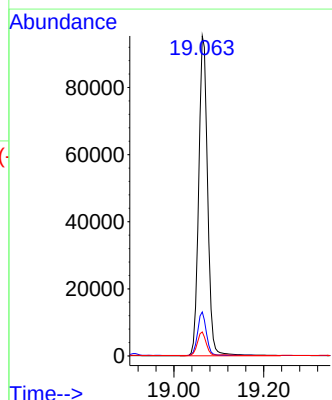
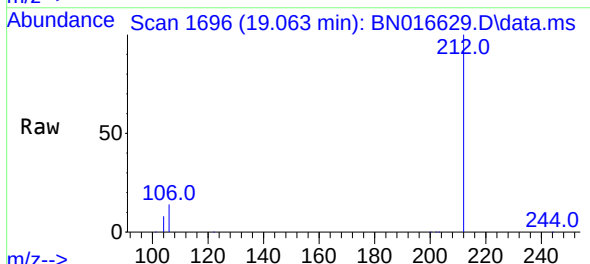


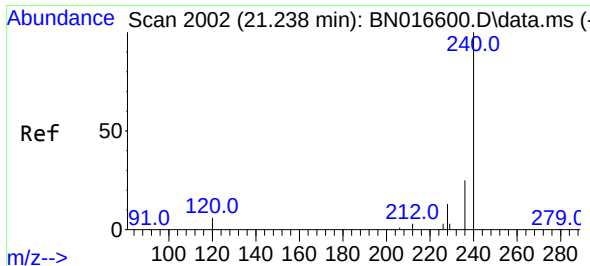

#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.238 min Scan# 2002
Delta R.T. 0.000 min
Lab File: BN016629.D
Acq: 01 Oct 2021 10:10




Instrument :
BNA_N
ClientSampleId :
RE126D3-20210920


Tgt Ion:240 Resp: 117060
Ion Ratio Lower Upper
240 100
120 6.0 5.0 7.4
236 25.3 20.4 30.6

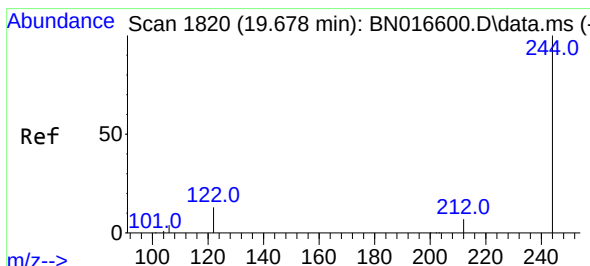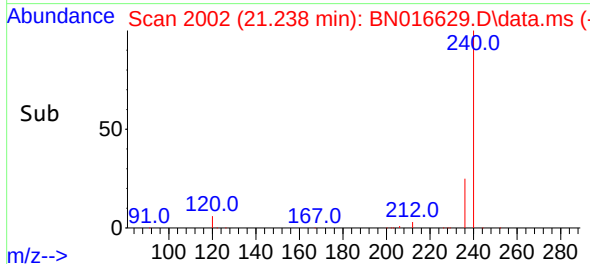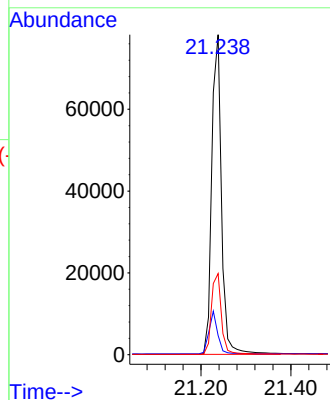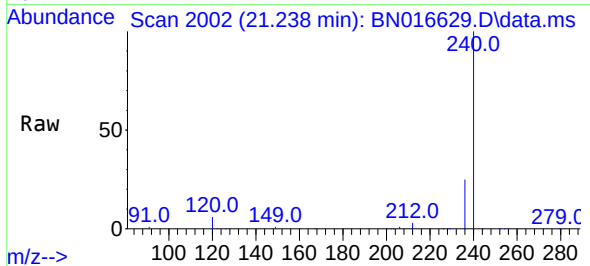

#31
Terphenyl-d14
Concen: 0.38 ng
RT: 19.678 min Scan# 1820
Delta R.T. 0.000 min
Lab File: BN016629.D
Acq: 01 Oct 2021 10:10

Tgt Ion:244 Resp: 97432
Ion Ratio Lower Upper
244 100
212 7.3 6.0 9.0
122 11.8 10.1 15.1


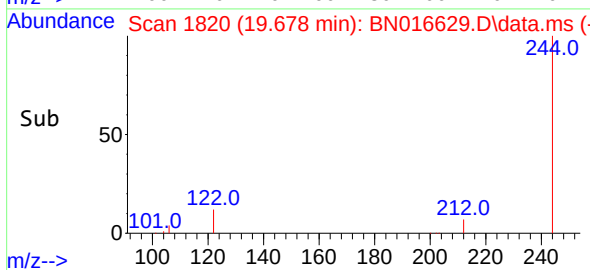
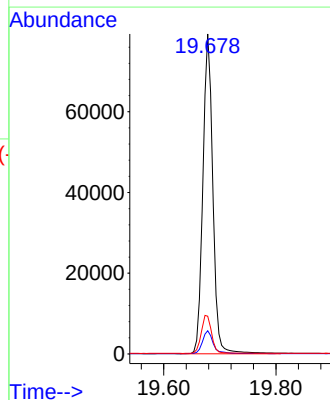
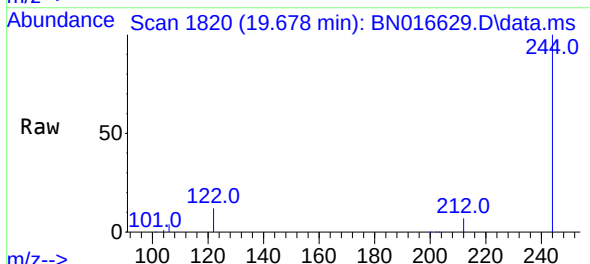


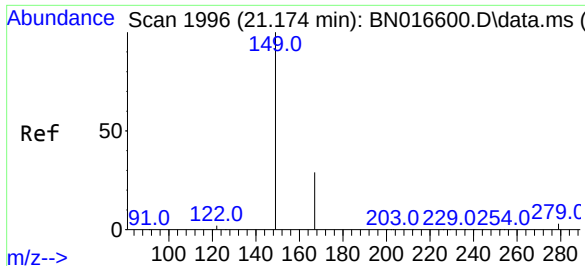

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.12 ng
RT: 21.164 min Scan# 1995
Delta R.T. -0.010 min
Lab File: BN016629.D
Acq: 01 Oct 2021 10:10

Instrument :
BNA_N
ClientSampleId :
RE126D3-20210920

Tgt Ion:149 Resp: 17089
Ion Ratio Lower Upper
149 100
167 27.0 22.2 33.4
279 4.4 3.2 4.8

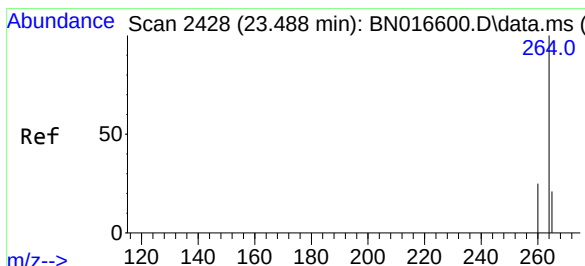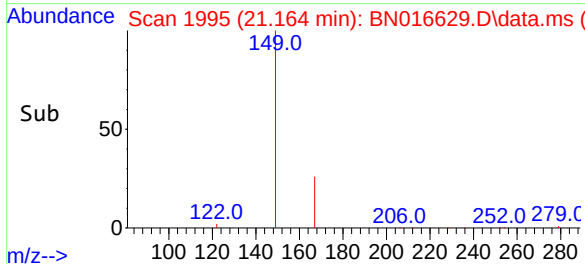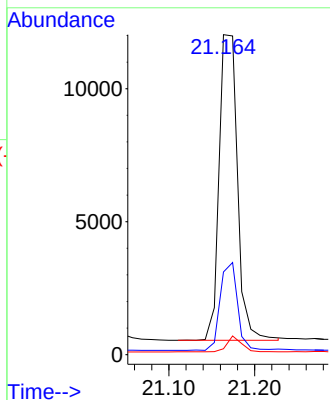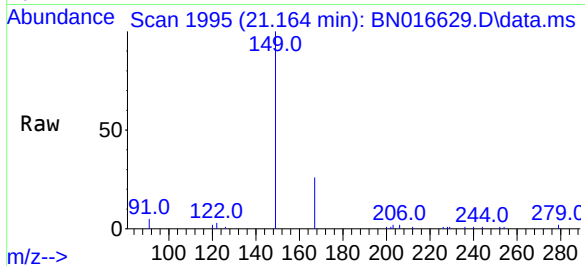

#35
Perylene-d12
Concen: 0.40 ng
RT: 23.484 min Scan# 2427
Delta R.T. -0.003 min
Lab File: BN016629.D
Acq: 01 Oct 2021 10:10

Tgt Ion:264 Resp: 116863
Ion Ratio Lower Upper
264 100
260 24.6 19.9 29.9
265 23.4 19.2 28.8

