

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100121\
 Data File : BN016631.D
 Acq On : 01 Oct 2021 11:22
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 34 Sample Multiplier: 1


Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Quant Time: Oct 01 11:51:32 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 30 17:56:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.642	152	33937	0.40	ng	0.00
7) Naphthalene-d8	10.406	136	150398	0.40	ng	0.00
13) Acenaphthene-d10	14.268	164	79386	0.40	ng	0.00
19) Phenanthrene-d10	17.017	188	144390	0.40	ng	#-0.01
29) Chrysene-d12	21.238	240	138091	0.40	ng	0.00
35) Perylene-d12	23.484	264	144795	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.263	112	31713	0.37	ng	0.00
5) Phenol-d6	6.821	99	34583	0.37	ng	0.00
8) Nitrobenzene-d5	8.784	82	32675	0.33	ng	0.00
11) 2-Methylnaphthalene-d10	12.002	152	82551	0.37	ng	0.00
14) 2,4,6-Tribromophenol	15.766	330	12391	0.34	ng	0.00
15) 2-Fluorobiphenyl	12.898	172	117727	0.37	ng	0.00
27) Fluoranthene-d10	19.068	212	141926	0.37	ng	0.00
31) Terphenyl-d14	19.678	244	118355	0.39	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.253	88	5770	0.37	ng	# 89
3) n-Nitrosodimethylamine	3.594	42	9268	0.37	ng	99
6) bis(2-Chloroethyl)ether	7.080	93	35394	0.38	ng	100
9) Naphthalene	10.457	128	151041	0.37	ng	100
10) Hexachlorobutadiene	10.749	225	28996	0.38	ng	# 100
12) 2-Methylnaphthalene	12.078	142	98548	0.38	ng	99
16) Acenaphthylene	13.989	152	122594	0.35	ng	100
17) Acenaphthene	14.332	154	86019	0.37	ng	100
18) Fluorene	15.322	166	102709	0.37	ng	100
20) 4,6-Dinitro-2-methylph...	15.410	198	2575	0.27	ng	99
21) 4-Bromophenyl-phenylether	16.226	248	32168	0.36	ng	94
22) Hexachlorobenzene	16.324	284	39465	0.38	ng	99
23) Atrazine	16.506	200	21562	0.33	ng	99
24) Pentachlorophenol	16.677	266	13084	0.38	ng	100
25) Phenanthrene	17.066	178	163218	0.38	ng	100
26) Anthracene	17.151	178	132902	0.35	ng	100
28) Fluoranthene	19.092	202	179139	0.38	ng	100
30) Pyrene	19.460	202	177432	0.40	ng	100
32) Benzo(a)anthracene	21.217	228	162510	0.38	ng	99
33) Chrysene	21.270	228	172549	0.40	ng	99
34) Bis(2-ethylhexyl)phtha...	21.163	149	61172	0.36	ng	99
36) Indeno(1,2,3-cd)pyrene	25.760	276	207158	0.40	ng	100
37) Benzo(b)fluoranthene	22.806	252	172581	0.37	ng	100
38) Benzo(k)fluoranthene	22.851	252	182899	0.40	ng	99
39) Benzo(a)pyrene	23.381	252	158048	0.38	ng	100
40) Dibenzo(a,h)anthracene	25.781	278	166159	0.40	ng	99
41) Benzo(g,h,i)perylene	26.452	276	179773	0.39	ng	100




(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.642 min Scan# 495
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:152 Resp: 33937
Ion Ratio Lower Upper
152 100
150 155.5 124.6 186.8
115 57.9 46.5 69.7



#2
1,4-Dioxane
Concen: 0.37 ng
RT: 3.253 min Scan# 19
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22

Tgt Ion: 88 Resp: 5770
Ion Ratio Lower Upper
88 100
43 28.7 37.8 56.8#
58 75.9 61.3 91.9









#3
n-Nitrosodimethylamine
Concen: 0.37 ng
RT: 3.594 min Scan# 56
Delta R.T. 0.018 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion: 42 Resp: 9268
Ion Ratio Lower Upper
42 100
74 150.6 121.6 182.4
44 8.3 6.3 9.5



#4
2-Fluorophenol
Concen: 0.37 ng
RT: 5.263 min Scan# 237
Delta R.T. 0.009 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22

Tgt Ion: 112 Resp: 31713
Ion Ratio Lower Upper
112 100
64 54.0 43.1 64.7
63 27.3 21.6 32.4









#5
Phenol-d6
Concen: 0.37 ng
RT: 6.821 min Scan# 406
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion: 99 Resp: 34583
Ion Ratio Lower Upper
99 100
42 16.5 13.0 19.6
71 29.7 23.5 35.3



#6
bis(2-Chloroethyl)ether
Concen: 0.38 ng
RT: 7.080 min Scan# 434
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22


Tgt Ion: 93 Resp: 35394
Ion Ratio Lower Upper
93 100
63 74.1 59.1 88.7
95 32.8 26.2 39.4








#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.406 min Scan# 733
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC





Tgt Ion:136 Resp: 150398
Ion Ratio Lower Upper
136 100
137 10.8 8.7 13.1
54 6.5 5.9 8.9
68 5.5 5.0 7.6




#8
Nitrobenzene-d5
Concen: 0.33 ng
RT: 8.784 min Scan# 605
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22



Tgt Ion: 82 Resp: 32675
Ion Ratio Lower Upper
82 100
128 44.0 33.6 50.4
54 45.3 37.6 56.4









#9
Naphthalene
Concen: 0.37 ng
RT: 10.457 min Scan# 737
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:128 Resp: 151041
Ion Ratio Lower Upper
128 100
129 11.0 8.8 13.2
127 12.9 10.3 15.5



#10
Hexachlorobutadiene
Concen: 0.38 ng
RT: 10.749 min Scan# 760
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22

Tgt Ion:225 Resp: 28996
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.8 51.0 76.6









#11
2-Methylnaphthalene-d10
Concen: 0.37 ng
RT: 12.002 min Scan# 931
Delta R.T. -0.004 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:152 Resp: 82551
Ion Ratio Lower Upper
152 100
151 20.3 16.2 24.4

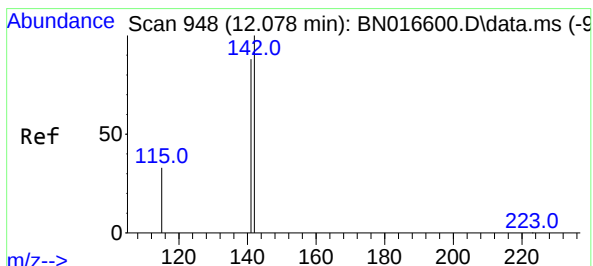

#12
2-Methylnaphthalene
Concen: 0.38 ng
RT: 12.078 min Scan# 948
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22

Tgt Ion:142 Resp: 98548
Ion Ratio Lower Upper
142 100
141 87.1 70.6 105.8
115 32.0 26.6 39.8









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.268 min Scan# 1183
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:164 Resp: 79386
Ion Ratio Lower Upper
164 100
162 101.5 82.2 123.2
160 46.0 37.7 56.5



#14
2,4,6-Tribromophenol
Concen: 0.34 ng
RT: 15.766 min Scan# 1301
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22

Tgt Ion:330 Resp: 12391
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 30.9 25.2 37.8









#15
2-Fluorobiphenyl
Concen: 0.37 ng
RT: 12.898 min Scan# 1075
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:172 Resp: 117727
Ion Ratio Lower Upper
172 100
171 33.3 27.0 40.4
170 21.5 17.4 26.2



#16
Acenaphthylene
Concen: 0.35 ng
RT: 13.989 min Scan# 1161
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22

Tgt Ion:152 Resp: 122594
Ion Ratio Lower Upper
152 100
151 19.3 15.5 23.3
153 13.1 10.4 15.6









#17
Acenaphthene
Concen: 0.37 ng
RT: 14.332 min Scan# 1188
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:154 Resp: 86019
Ion Ratio Lower Upper
154 100
153 112.3 90.2 135.2
152 54.8 44.0 66.0



#18
Fluorene
Concen: 0.37 ng
RT: 15.322 min Scan# 1266
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22

Tgt Ion:166 Resp: 102709
Ion Ratio Lower Upper
166 100
165 97.4 77.9 116.9
167 13.5 10.7 16.1









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.017 min Scan# 1403
Delta R.T. -0.012 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:188 Resp: 144390
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 12.3 5.0 7.6#



#20
4,6-Dinitro-2-methylphenol
Concen: 0.27 ng
RT: 15.410 min Scan# 1273
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22

Tgt Ion:198 Resp: 2575
Ion Ratio Lower Upper
198 100
182 14.3 11.8 17.8
77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 0.36 ng
RT: 16.226 min Scan# 1338
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:248 Resp: 32168
Ion Ratio Lower Upper
248 100
250 102.3 78.6 117.8
141 41.0 38.6 57.8



#22
Hexachlorobenzene
Concen: 0.38 ng
RT: 16.324 min Scan# 1346
Delta R.T. -0.012 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22

Tgt Ion:284 Resp: 39465
Ion Ratio Lower Upper
284 100
142 32.2 26.4 39.6
249 28.9 23.4 35.2









#23
Atrazine
Concen: 0.33 ng
RT: 16.506 min Scan# 1361
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:200 Resp: 21562
Ion Ratio Lower Upper
200 100
173 21.9 18.6 27.8
215 49.7 39.4 59.2



#24
Pentachlorophenol
Concen: 0.38 ng
RT: 16.677 min Scan# 1375
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22

Tgt Ion:266 Resp: 13084
Ion Ratio Lower Upper
266 100
264 62.5 49.8 74.6
268 64.4 51.4 77.2









#25
Phenanthrene
Concen: 0.38 ng
RT: 17.066 min Scan# 1407
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:178 Resp: 163218
Ion Ratio Lower Upper
178 100
176 18.7 15.0 22.4
179 15.6 12.2 18.4



#26
Anthracene
Concen: 0.35 ng
RT: 17.151 min Scan# 1414
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22

Tgt Ion:178 Resp: 132902
Ion Ratio Lower Upper
178 100
176 18.3 14.6 21.8
179 15.4 12.2 18.4









#27
Fluoranthene-d10
Concen: 0.37 ng
RT: 19.068 min Scan# 1697
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:212 Resp: 141926
Ion Ratio Lower Upper
212 100
106 13.2 10.6 16.0
104 7.3 5.9 8.9



#28
Fluoranthene
Concen: 0.38 ng
RT: 19.092 min Scan# 1702
Delta R.T. -0.005 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22

Tgt Ion:202 Resp: 179139
Ion Ratio Lower Upper
202 100
101 11.0 9.0 13.4
203 17.3 13.8 20.6









#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.238 min Scan# 2002
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:240 Resp: 138091
Ion Ratio Lower Upper
240 100
120 5.6 5.0 7.4
236 25.2 20.4 30.6



#30
Pyrene
Concen: 0.40 ng
RT: 19.460 min Scan# 1776
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22

Tgt Ion:202 Resp: 177432
Ion Ratio Lower Upper
202 100
200 20.6 16.5 24.7
203 17.5 14.0 21.0









#31
Terphenyl-d14
Concen: 0.39 ng
RT: 19.678 min Scan# 1820
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:244 Resp: 118355
Ion Ratio Lower Upper
244 100
212 7.2 6.0 9.0
122 11.3 10.1 15.1



#32
Benzo(a)anthracene
Concen: 0.38 ng
RT: 21.217 min Scan# 2000
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22

Tgt Ion:228 Resp: 162510
Ion Ratio Lower Upper
228 100
226 26.7 21.9 32.9
229 19.6 15.7 23.5









#33
Chrysene
Concen: 0.40 ng
RT: 21.270 min Scan# 2005
Delta R.T. 0.000 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:228 Resp: 172549




Ion	Ratio	Lower	Upper
228	100		
226	29.3	23.7	35.5
229	19.6	15.5	23.3




#34
Bis(2-ethylhexyl)phthalate
Concen: 0.36 ng
RT: 21.163 min Scan# 1995
Delta R.T. -0.011 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22

Tgt Ion:149 Resp: 61172


Ion	Ratio	Lower	Upper
149	100		
167	27.4	22.2	33.4
279	4.0	3.2	4.8








#35
Perylene-d12
Concen: 0.40 ng
RT: 23.484 min Scan# 2427
Delta R.T. -0.003 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC







Tgt Ion:264 Resp: 144795
Ion Ratio Lower Upper
264 100
260 24.5 19.9 29.9
265 22.6 19.2 28.8



#36
Indeno(1,2,3-cd)pyrene
Concen: 0.40 ng
RT: 25.760 min Scan# 3092
Delta R.T. -0.003 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22

Tgt Ion:276 Resp: 207158
Ion Ratio Lower Upper
276 100
138 24.8 19.5 29.3
277 25.0 19.9 29.9









#37
Benzo(b)fluoranthene
Concen: 0.37 ng
RT: 22.806 min Scan# 2229
Delta R.T. -0.003 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:252 Resp: 172581
Ion Ratio Lower Upper
252 100
253 22.0 17.8 26.8
125 9.9 8.0 12.0



#38
Benzo(k)fluoranthene
Concen: 0.40 ng
RT: 22.851 min Scan# 2242
Delta R.T. -0.003 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22


Tgt Ion:252 Resp: 182899
Ion Ratio Lower Upper
252 100
253 22.4 17.8 26.6
125 11.3 8.0 12.0








#39
Benzo(a)pyrene
Concen: 0.38 ng
RT: 23.381 min Scan# 2397
Delta R.T. -0.007 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC







Tgt Ion:252 Resp: 158048
Ion Ratio Lower Upper
252 100
253 22.1 17.8 26.8
125 10.9 9.0 13.4



#40
Dibenzo(a,h)anthracene
Concen: 0.40 ng
RT: 25.781 min Scan# 3098
Delta R.T. -0.007 min
Lab File: BN016631.D
Acq: 01 Oct 2021 11:22

Tgt Ion:278 Resp: 166159
Ion Ratio Lower Upper
278 100
139 17.4 13.1 19.7
279 23.7 19.1 28.7



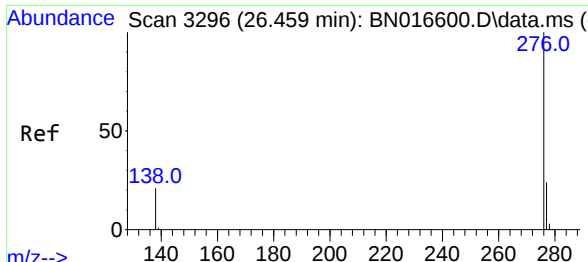

#41
 Benzo(g,h,i)perylene
 Concen: 0.39 ng
 RT: 26.452 min Scan# 3294
 Delta R.T. -0.007 min
 Lab File: BN016631.D
 Acq: 01 Oct 2021 11:22

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Tgt Ion:276 Resp: 179773
 Ion Ratio Lower Upper
 276 100
 277 23.8 19.0 28.6
 138 21.0 16.9 25.3

