
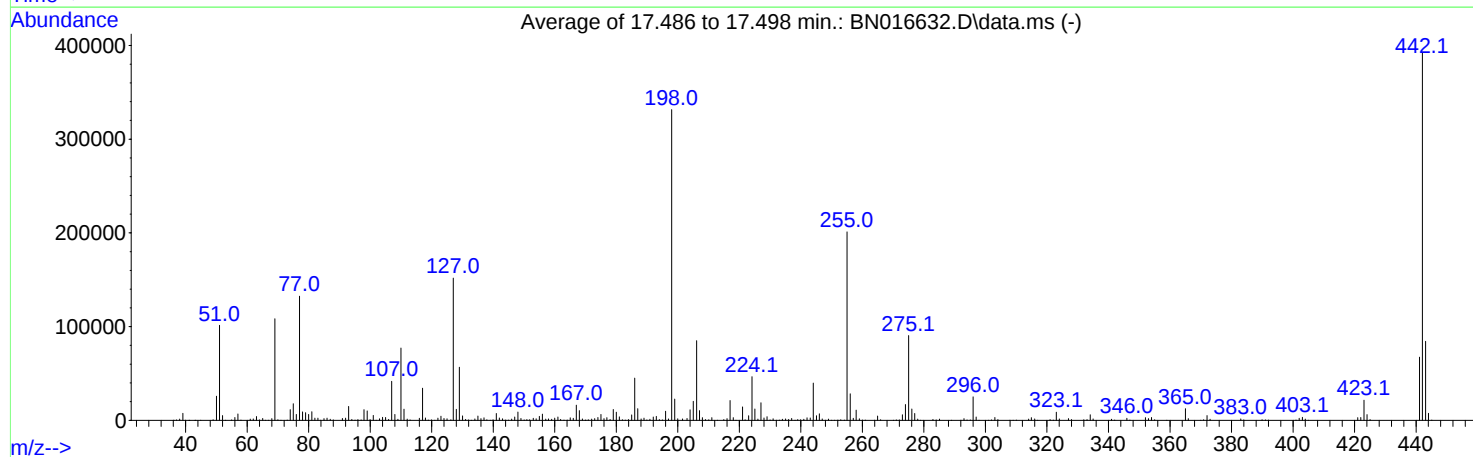


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100121\
 Data File : BN016632.D
 Acq On : 01 Oct 2021 12:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 01 13:35:26 2021

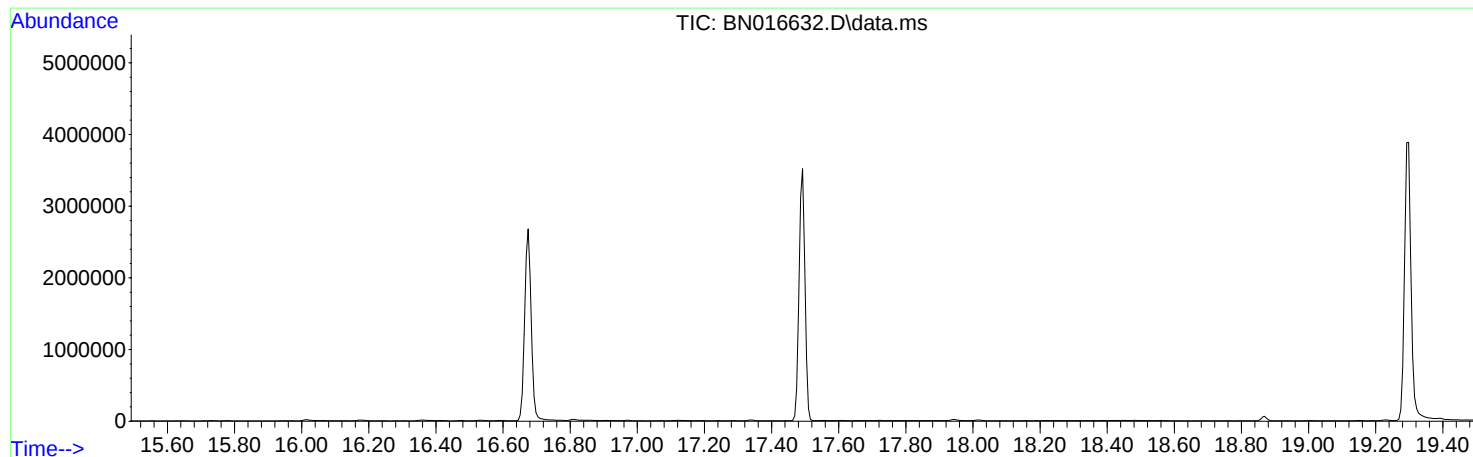

AutoFind: Scans 2448, 2449, 2450; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.6	101371	PASS
68	69	0.00	2	1.7	1808	PASS
69	198	0.00	100	32.7	108491	PASS
70	69	0.00	2	0.6	672	PASS
127	198	10	80	45.8	151739	PASS
197	198	0.00	2	0.5	1626	PASS
198	198	100	100	100.0	331584	PASS
199	198	5	9	6.9	22790	PASS
275	198	10	60	27.3	90539	PASS
365	198	1	100	3.8	12436	PASS
441	198	0.01	100	20.4	67509	PASS
442	442	50	100	100.0	392469	PASS
443	442	15	24	21.5	84341	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/1/2021	BNA_N	<u>BN016632.D</u>
Compound Name	Response	Retention Time
DDT	1170026	20.539
DDD	14042	20.098
DDE	1329	19.586
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15371	1185397	1.30

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100121\
Data File : BN016632.D
Acq On : 01 Oct 2021 12:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 06 05:02:56 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

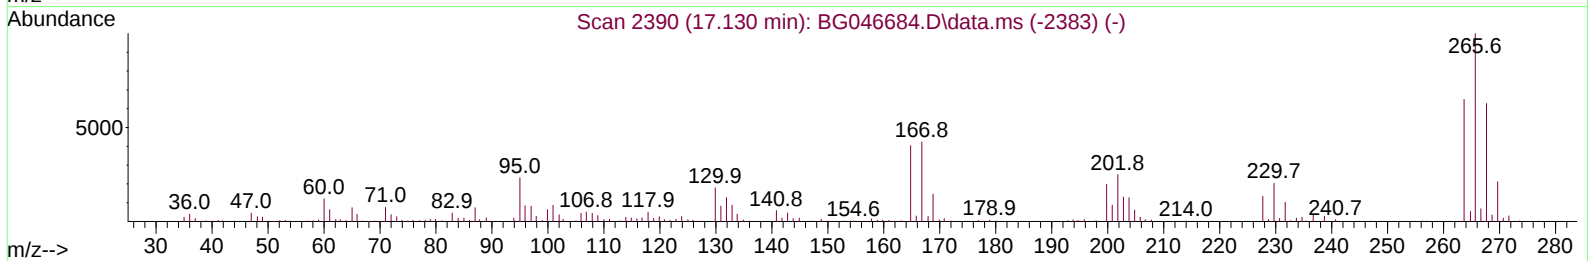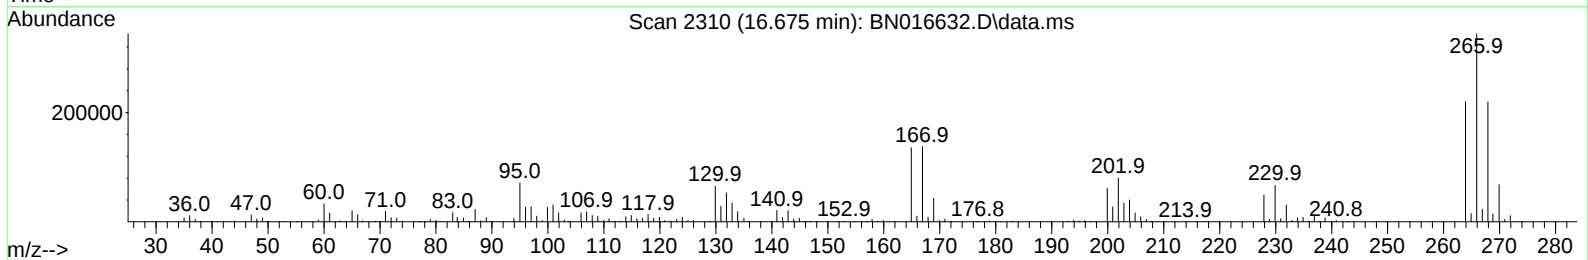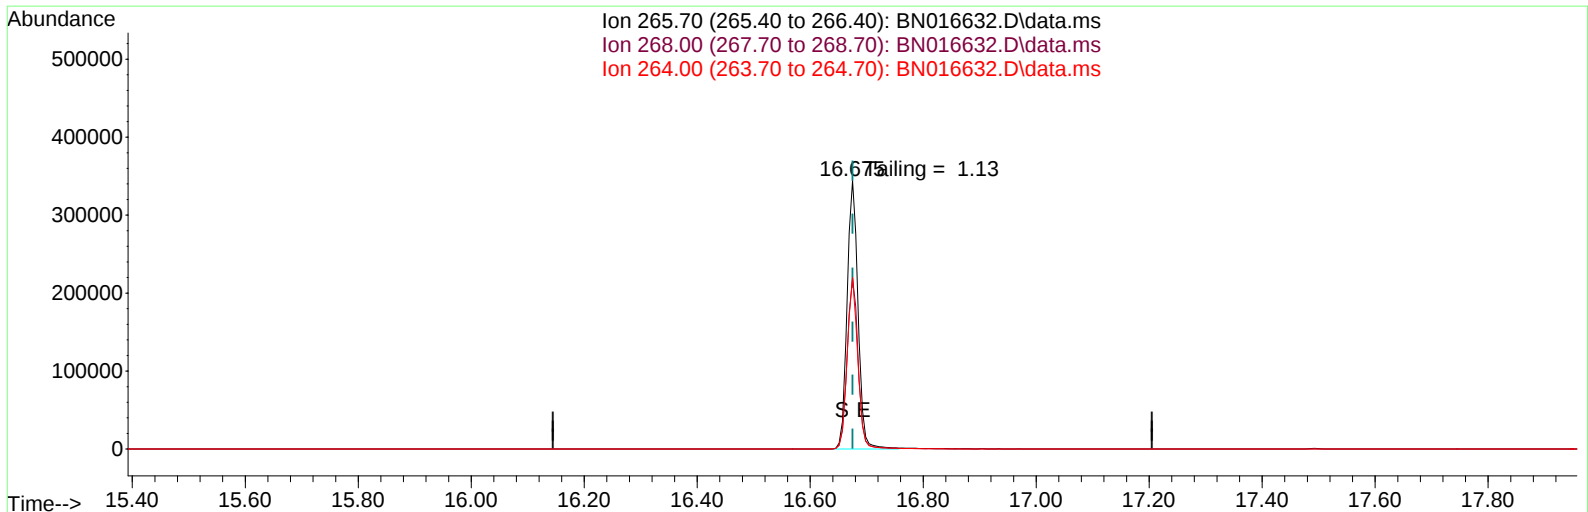

TIC: BN016632.D\data.ms

(70) Pentachlorophenol (C)

16.675min (+ 0.000) 28622.33 ng




response 465639

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.65
264.00	61.60	63.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100121\
Data File : BN016632.D
Acq On : 01 Oct 2021 12:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 06 05:02:56 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

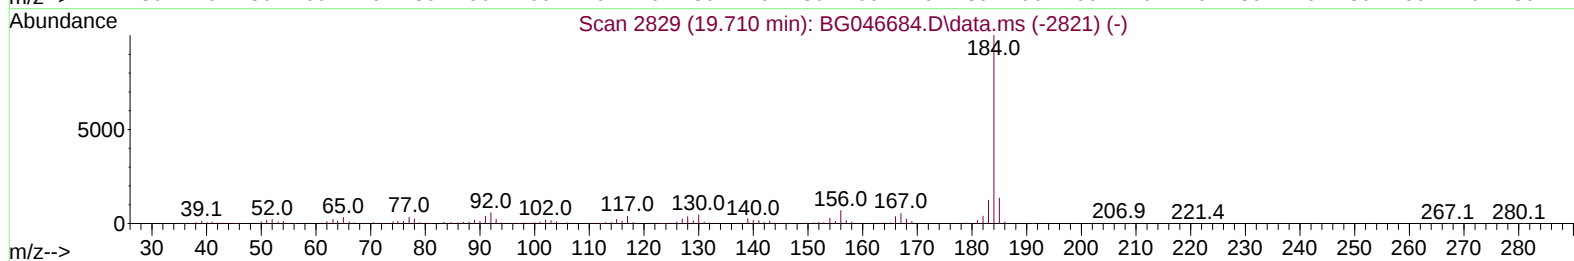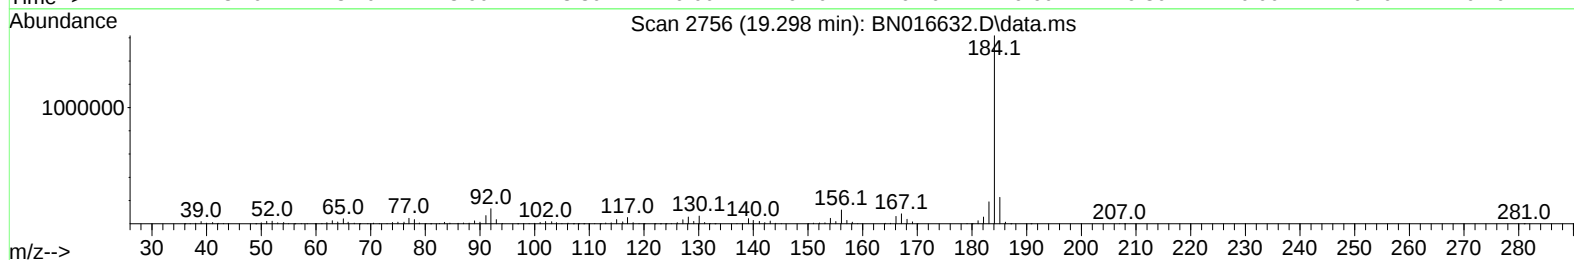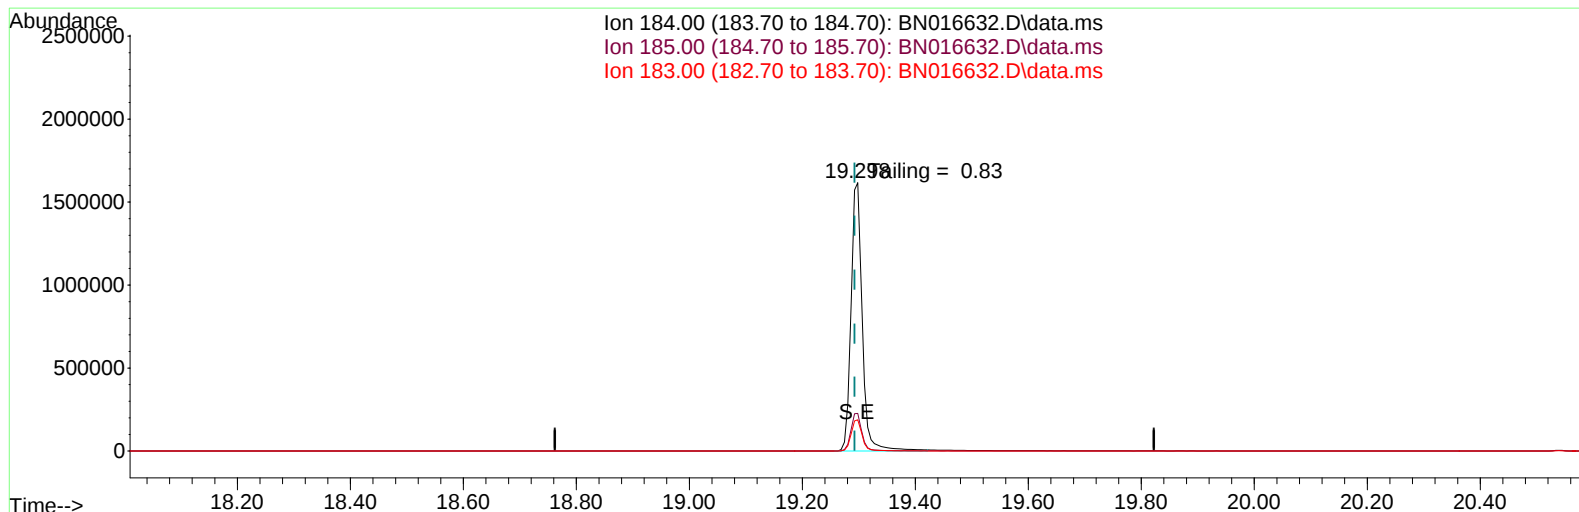

TIC: BN016632.D\data.ms

(77) Benzidine

19.298min (+ 0.006) 0.00 ng

response 2260650

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.06
183.00	13.20	11.65
0.00	0.00	0.00