
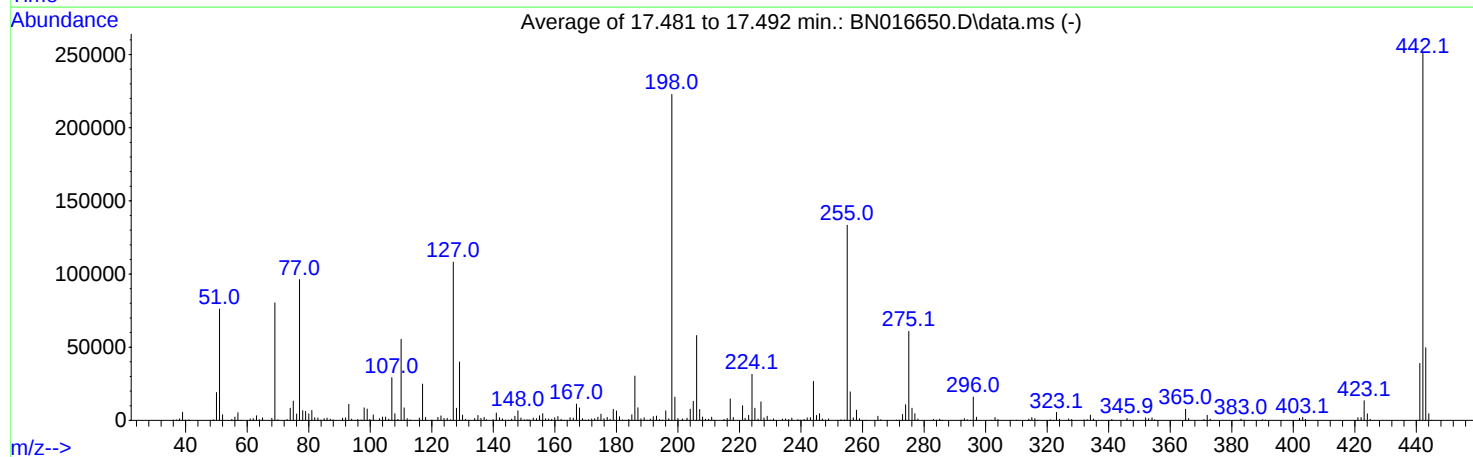


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100121\
 Data File : BN016650.D
 Acq On : 02 Oct 2021 01:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 01 13:35:26 2021

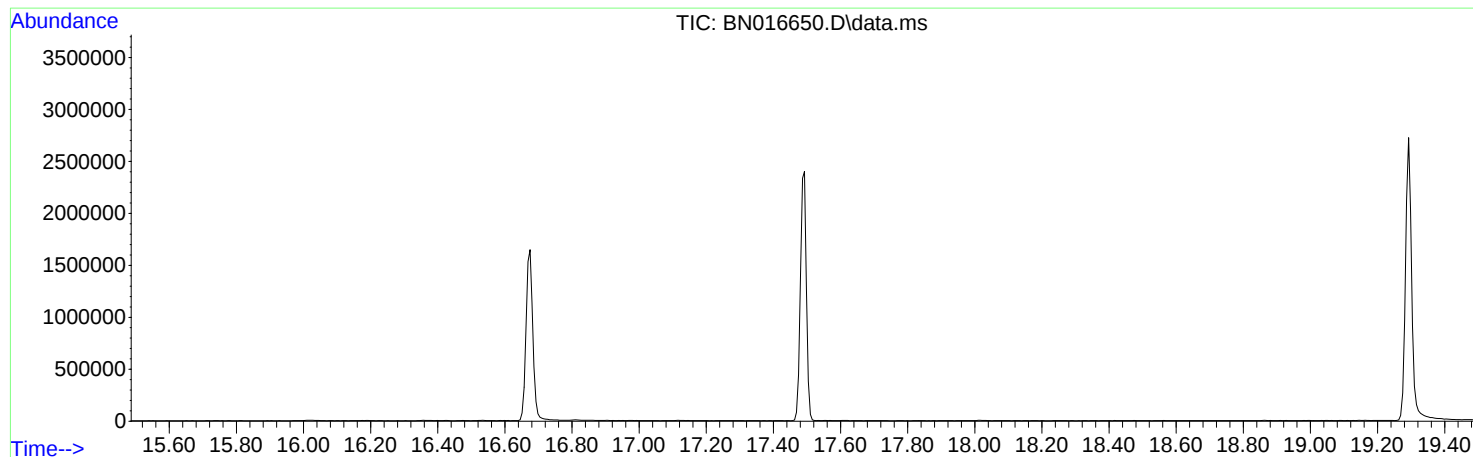




AutoFind: Scans 2447, 2448, 2449; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	76083	PASS
68	69	0.00	2	1.8	1433	PASS
69	198	0.00	100	36.1	80397	PASS
70	69	0.00	2	0.6	458	PASS
127	198	10	80	48.5	108123	PASS
197	198	0.00	2	0.5	1113	PASS
198	198	100	100	100.0	222805	PASS
199	198	5	9	7.1	15840	PASS
275	198	10	60	27.3	60843	PASS
365	198	1	100	3.4	7680	PASS
441	198	0.01	100	17.5	38952	PASS
442	442	50	100	100.0	251413	PASS
443	442	15	24	19.7	49624	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100121\
Data File : BN016650.D
Acq On : 02 Oct 2021 01:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 02 04:28:53 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

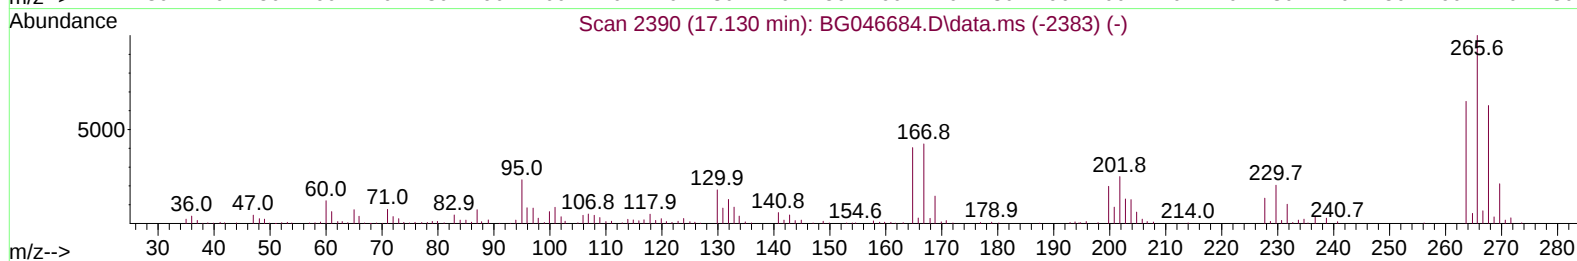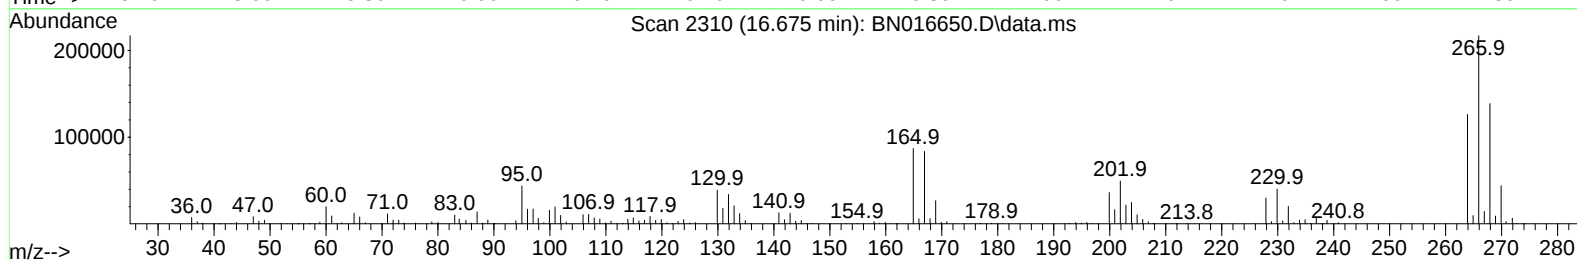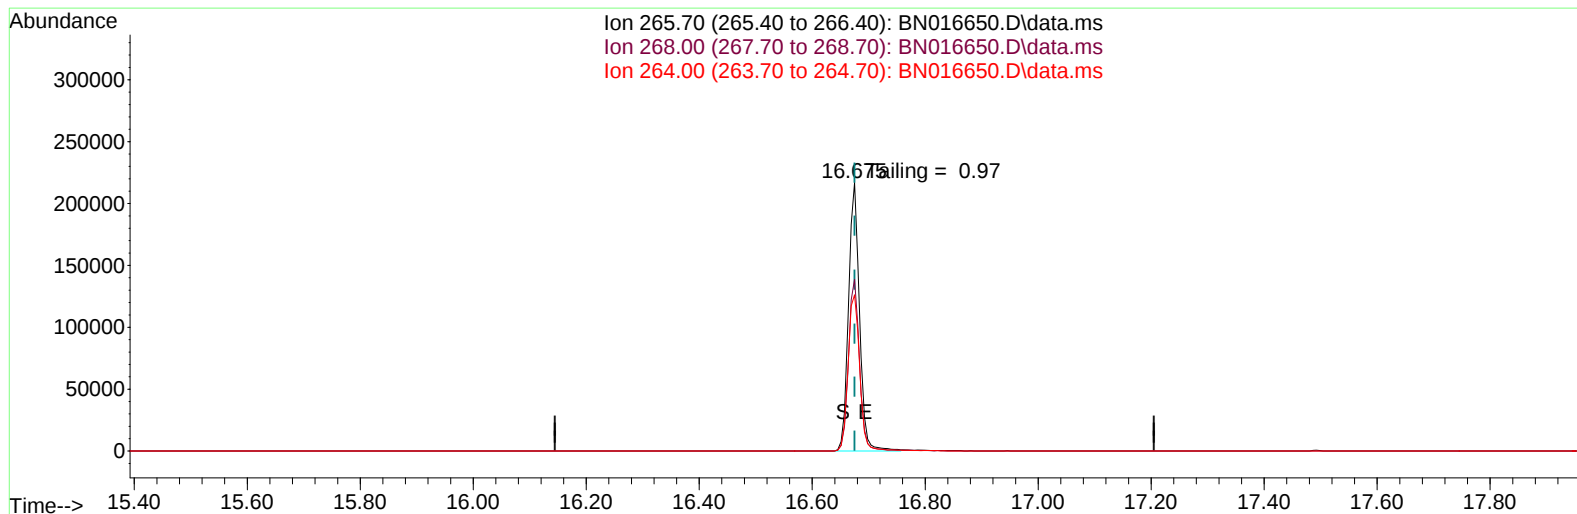

TIC: BN016650.D\data.ms

(70) Pentachlorophenol (C)

16.675min (+ 0.000) 25377.77 ng




response 294356

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.97
264.00	61.60	58.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100121\
Data File : BN016650.D
Acq On : 02 Oct 2021 01:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 02 04:28:53 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

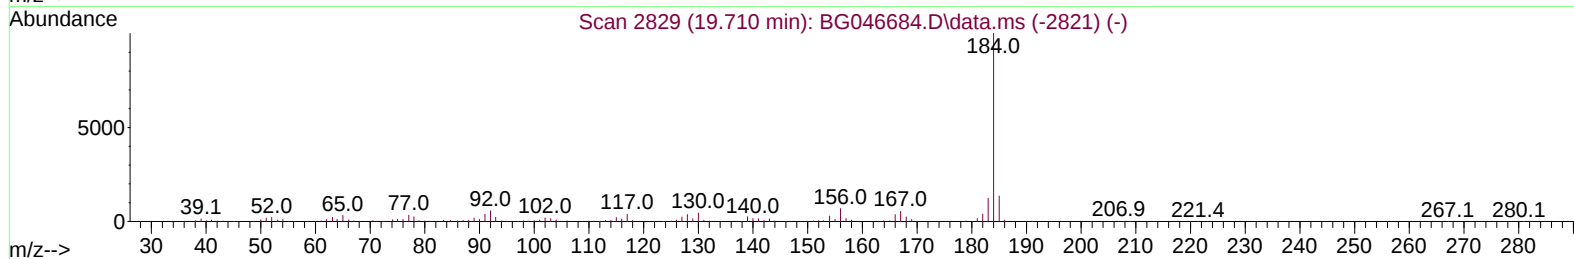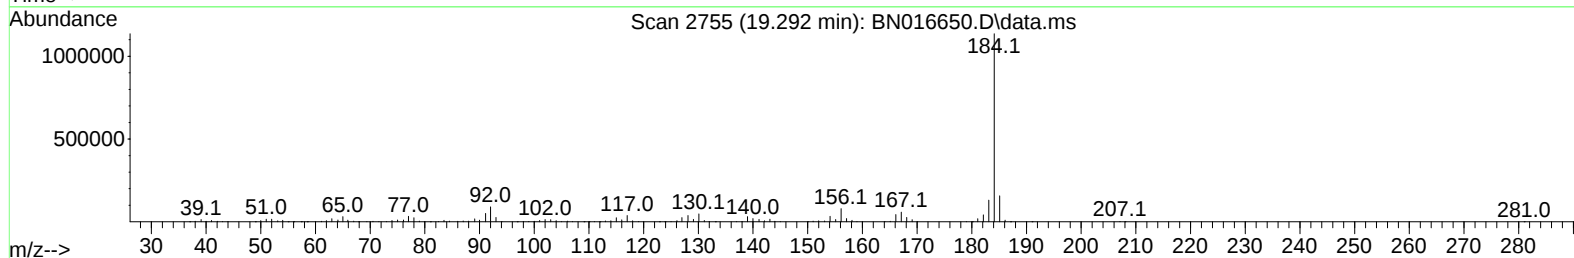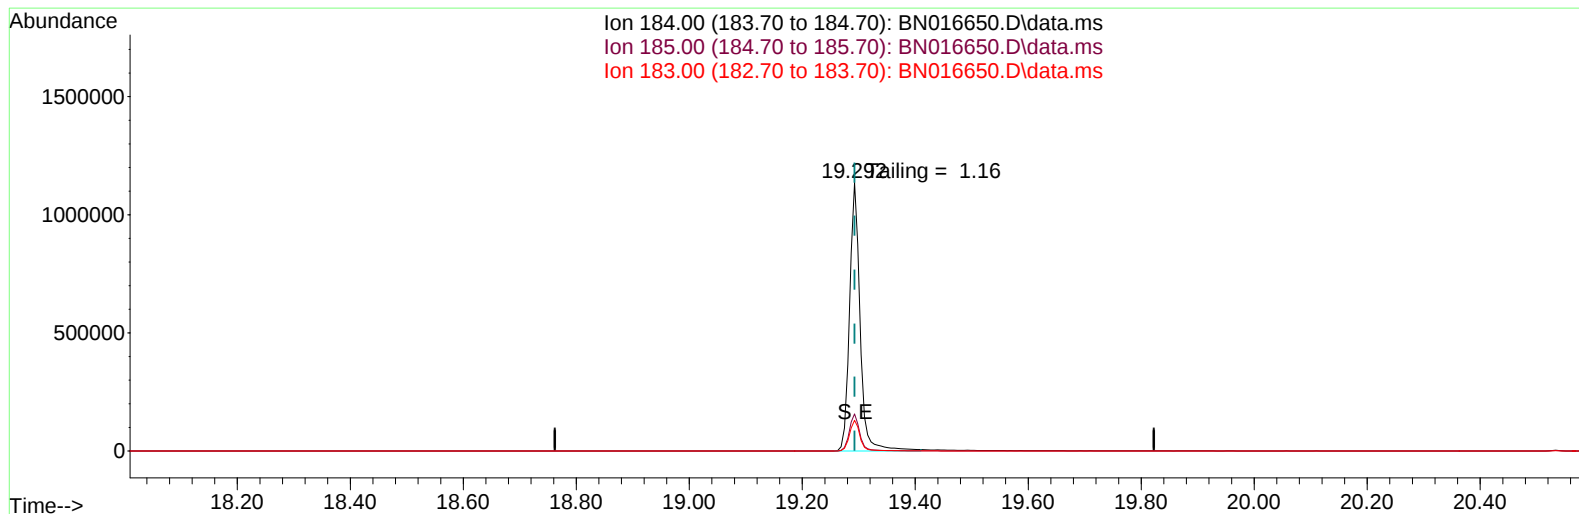

TIC: BN016650.D\data.ms

(77) Benzidine

19.292min (+ 0.000) 0.00 ng

response 1485130

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.82
183.00	13.20	11.48
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/1/2021	BNA_N	<u>BN016650.D</u>
Compound Name	Response	Retention Time
DDT	766121	20.533
DDD	18838	20.092
DDE	495	19.581
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19333	785454	2.46