
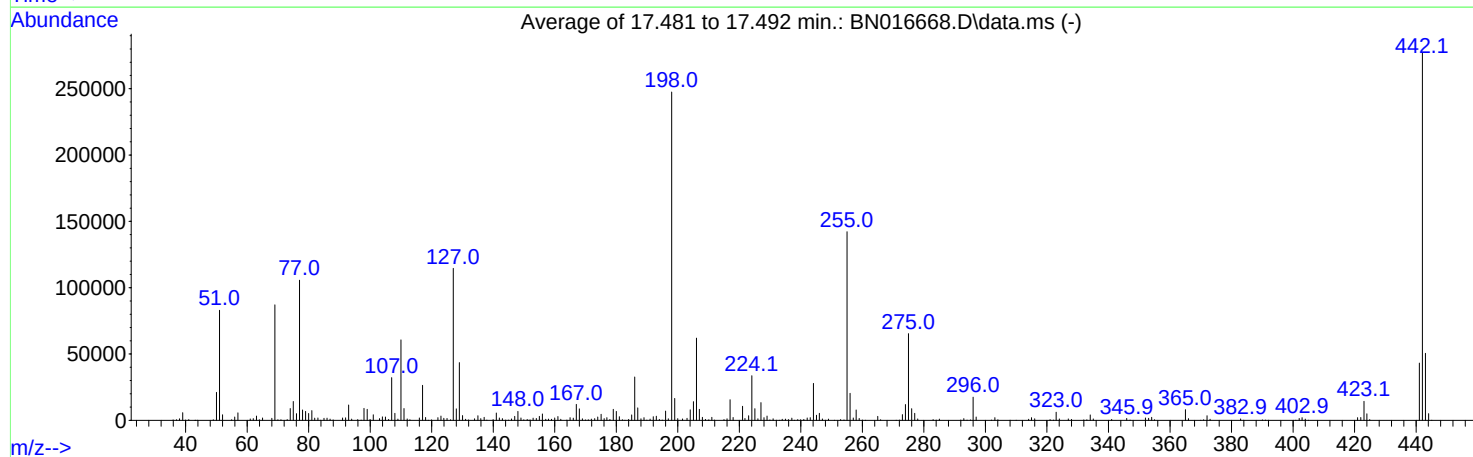


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100121\
 Data File : BN016668.D
 Acq On : 02 Oct 2021 12:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 01 13:35:26 2021

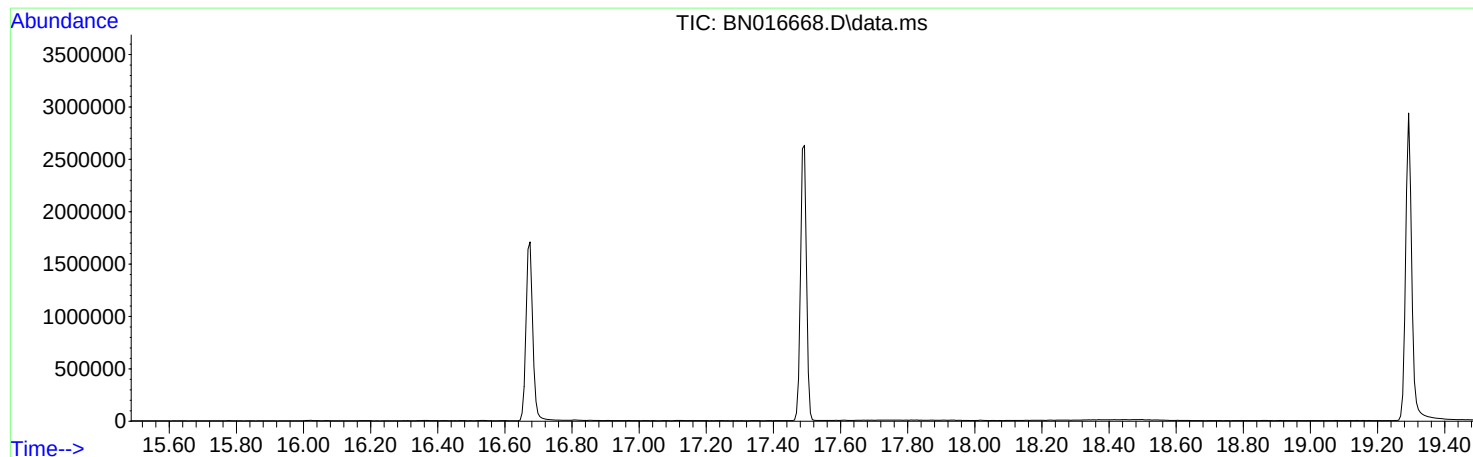




AutoFind: Scans 2447, 2448, 2449; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	83032	PASS
68	69	0.00	2	1.8	1601	PASS
69	198	0.00	100	35.2	87040	PASS
70	69	0.00	2	0.6	526	PASS
127	198	10	80	46.3	114557	PASS
197	198	0.00	2	0.5	1242	PASS
198	198	100	100	100.0	247552	PASS
199	198	5	9	6.7	16564	PASS
275	198	10	60	26.4	65400	PASS
365	198	1	100	3.3	8065	PASS
441	198	0.01	100	17.5	43235	PASS
442	442	50	100	100.0	277312	PASS
443	442	15	24	18.2	50557	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100121\
Data File : BN016668.D
Acq On : 02 Oct 2021 12:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 04 05:43:14 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

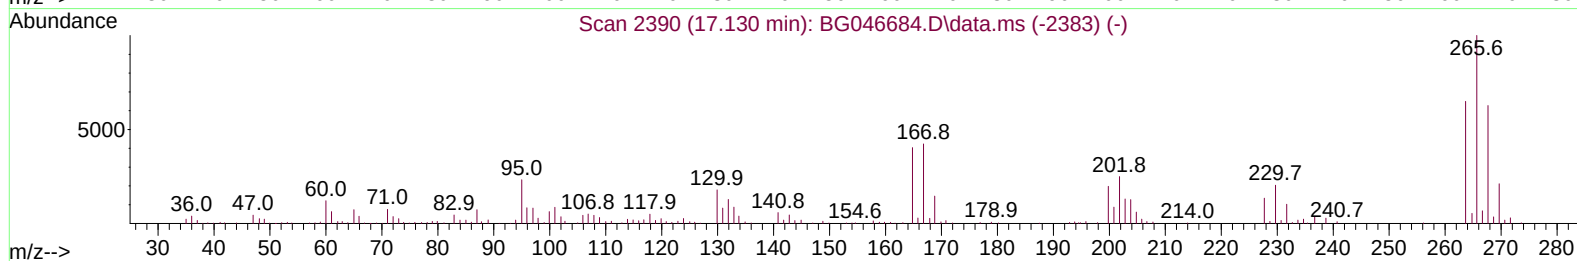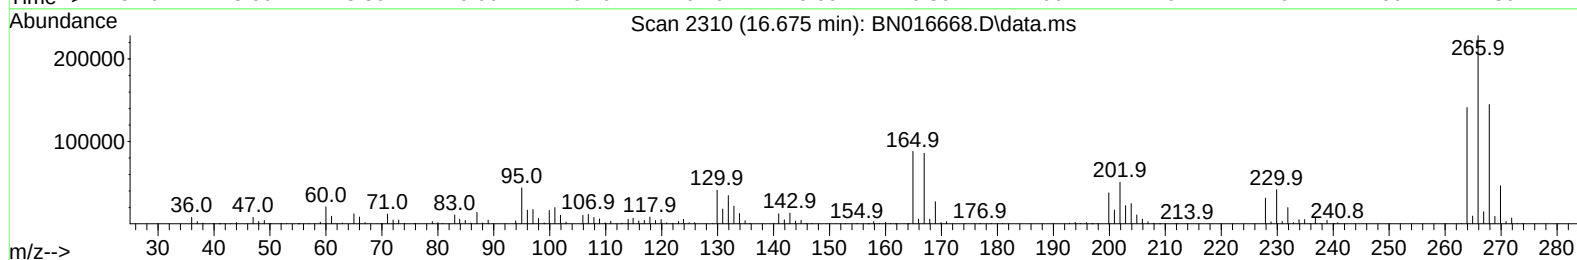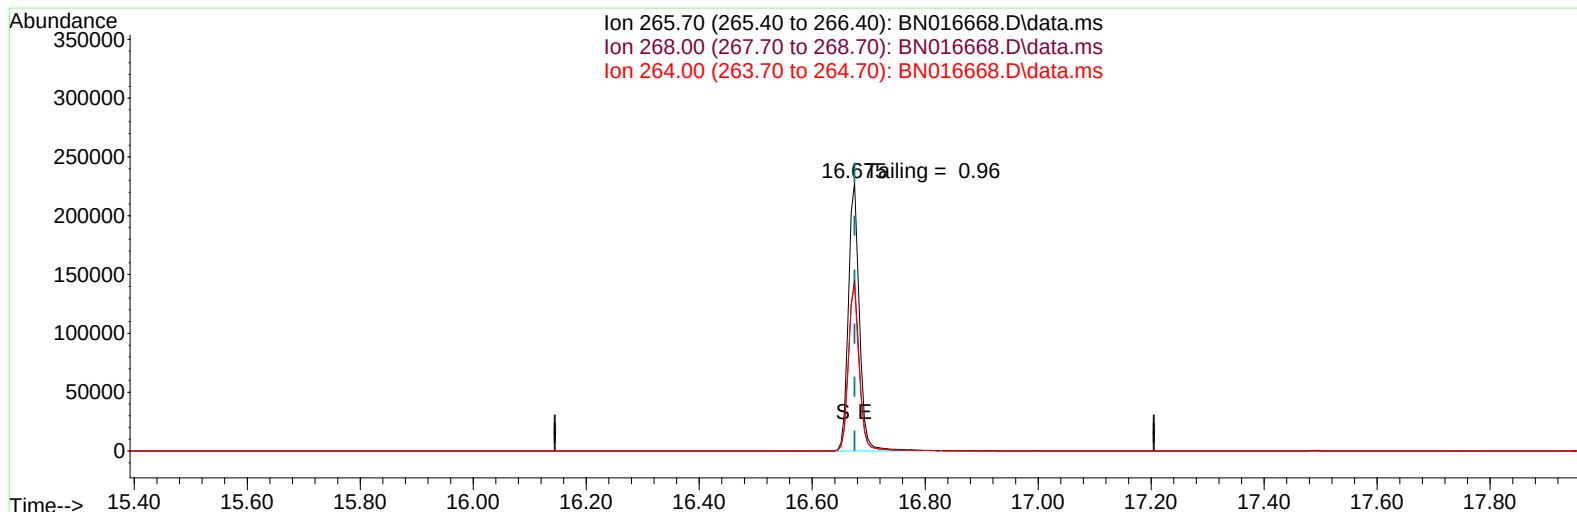

TIC: BN016668.D\data.ms

(70) Pentachlorophenol (C)

16.675min (+ 0.000) 25093.01 ng




response 311927

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.48
264.00	61.60	61.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100121\
Data File : BN016668.D
Acq On : 02 Oct 2021 12:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 04 05:43:14 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

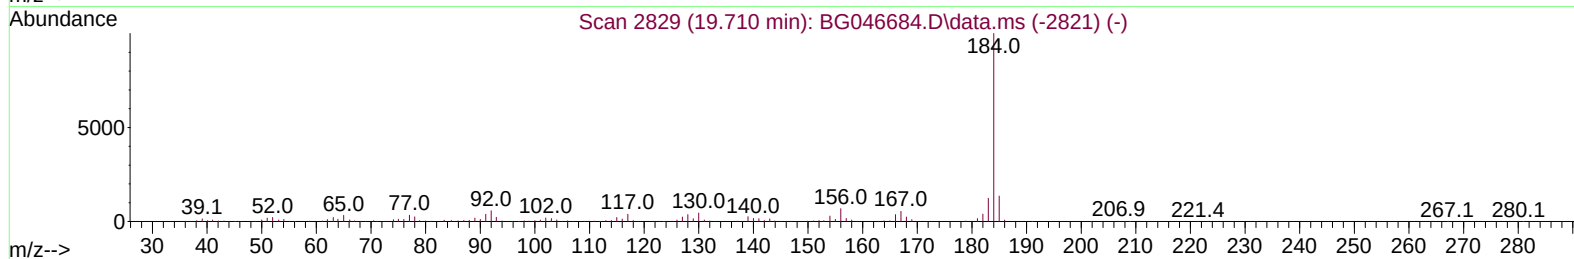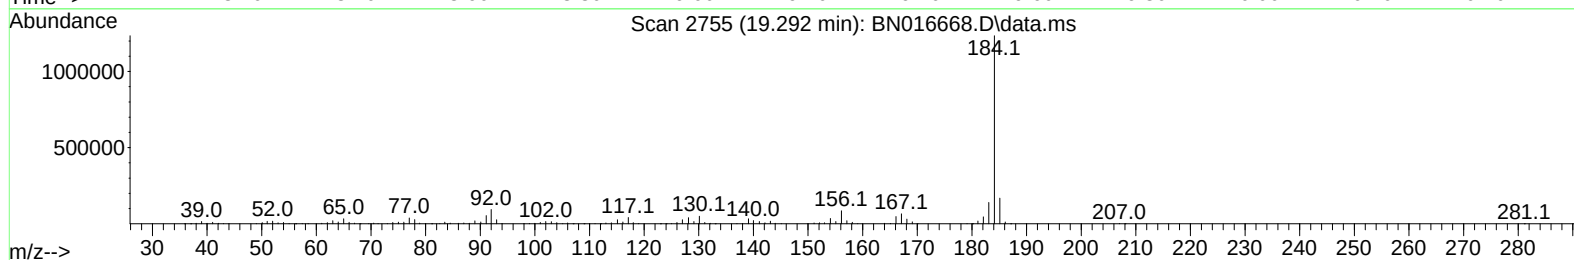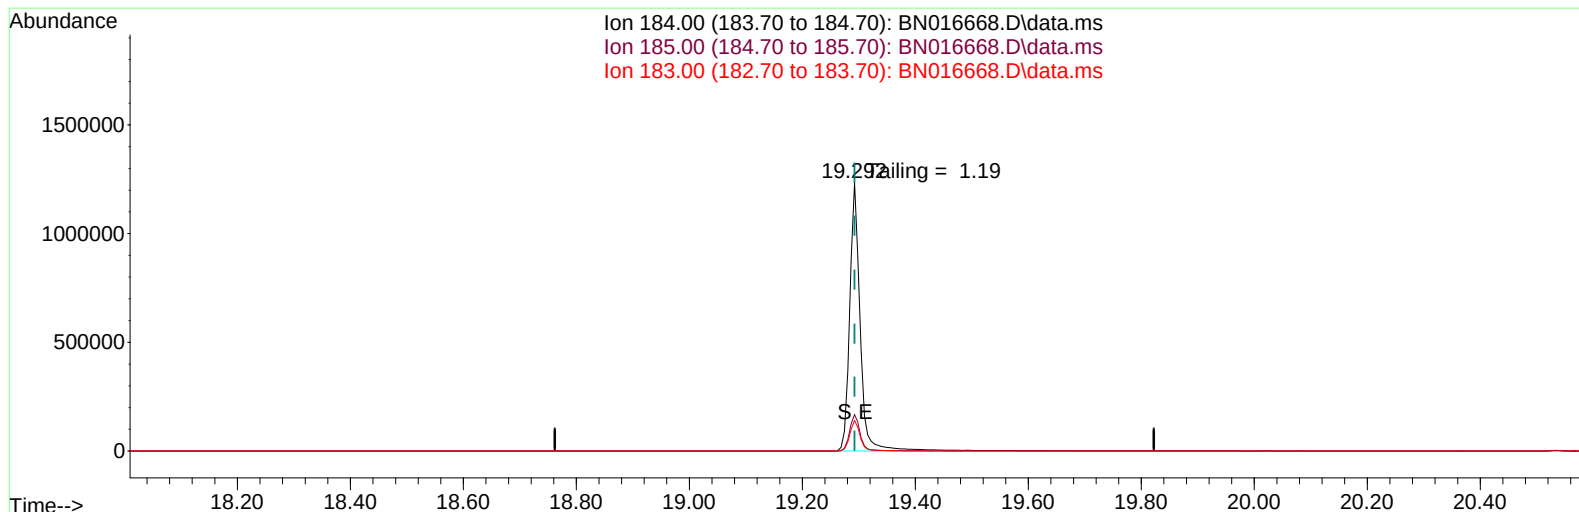

TIC: BN016668.D\data.ms

(77) Benzidine

19.292min (+ 0.000) 0.00 ng

response 1603854

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.63
183.00	13.20	11.39
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/1/2021	BNA_N	<u>BN016668.D</u>
Compound Name	Response	Retention Time
DDT	809135	20.533
DDD	15598	20.092
DDE	112	19.586
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15710	824845	1.90