
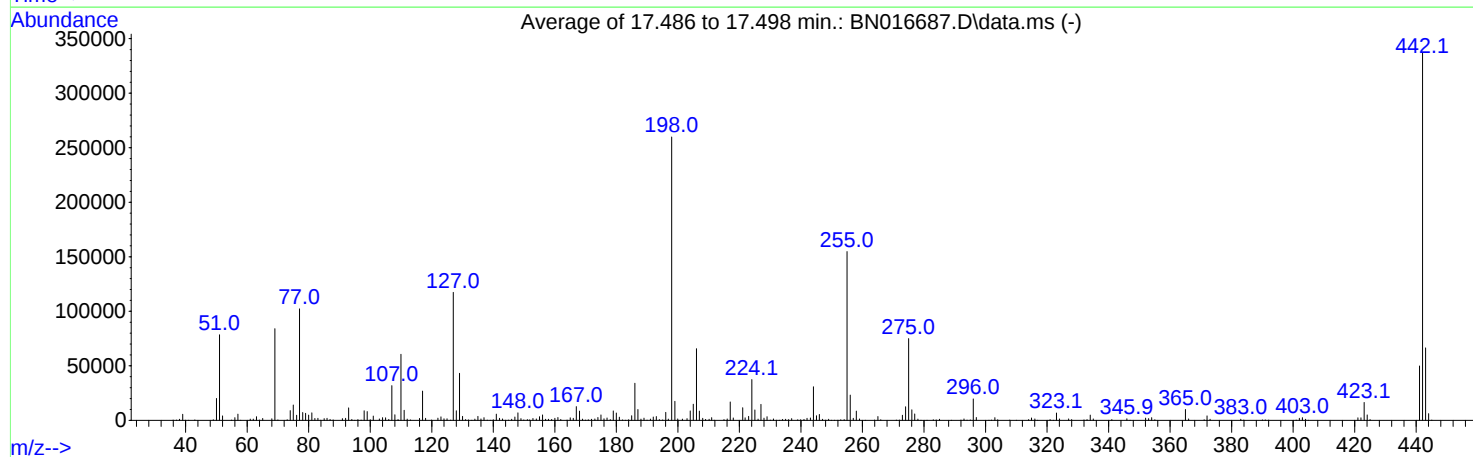


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100121\
 Data File : BN016687.D
 Acq On : 03 Oct 2021 01:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 01 13:35:26 2021

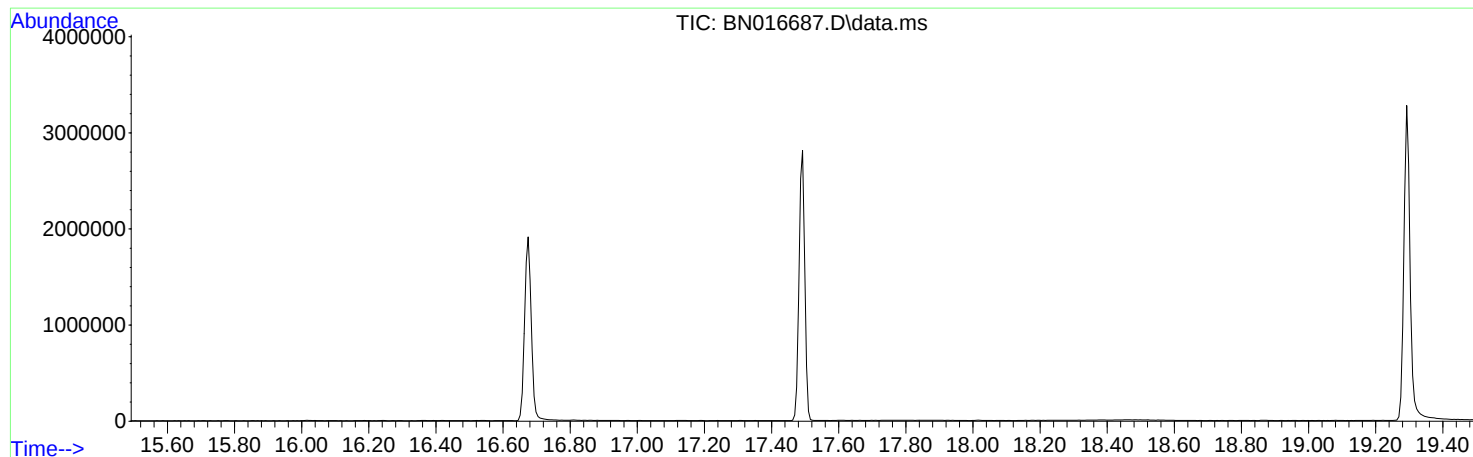




AutoFind: Scans 2448, 2449, 2450; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.2	78445	PASS
68	69	0.00	2	1.7	1461	PASS
69	198	0.00	100	32.3	84043	PASS
70	69	0.00	2	0.6	514	PASS
127	198	10	80	45.2	117360	PASS
197	198	0.00	2	0.5	1253	PASS
198	198	100	100	100.0	259861	PASS
199	198	5	9	6.7	17408	PASS
275	198	10	60	28.9	74984	PASS
365	198	1	100	3.8	9996	PASS
441	198	0.01	100	19.2	49832	PASS
442	442	50	100	100.0	337323	PASS
443	442	15	24	19.7	66515	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100121\
Data File : BN016687.D
Acq On : 03 Oct 2021 01:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 04 05:48:38 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

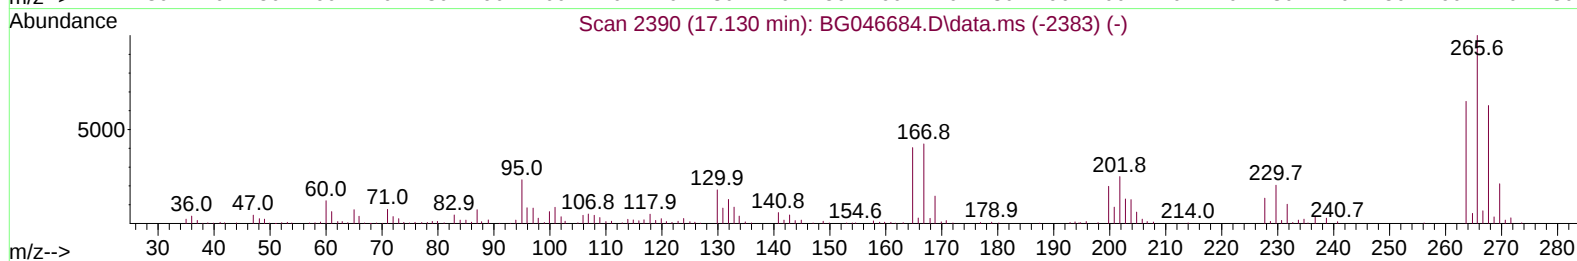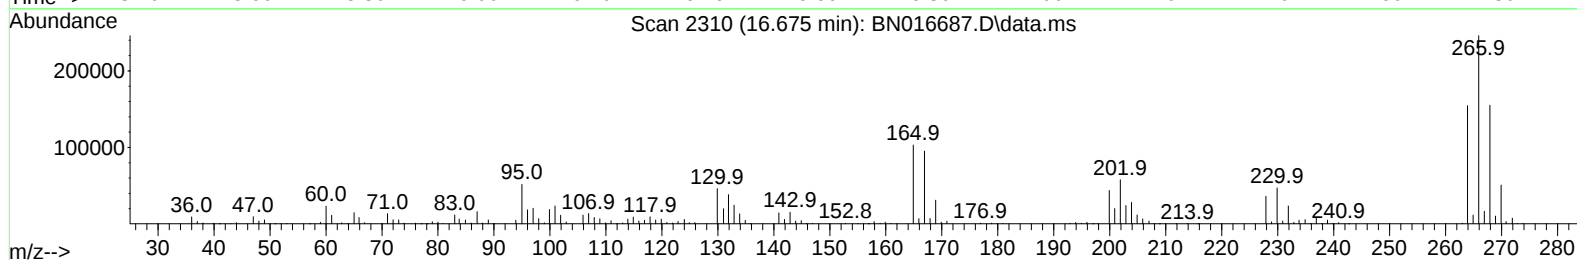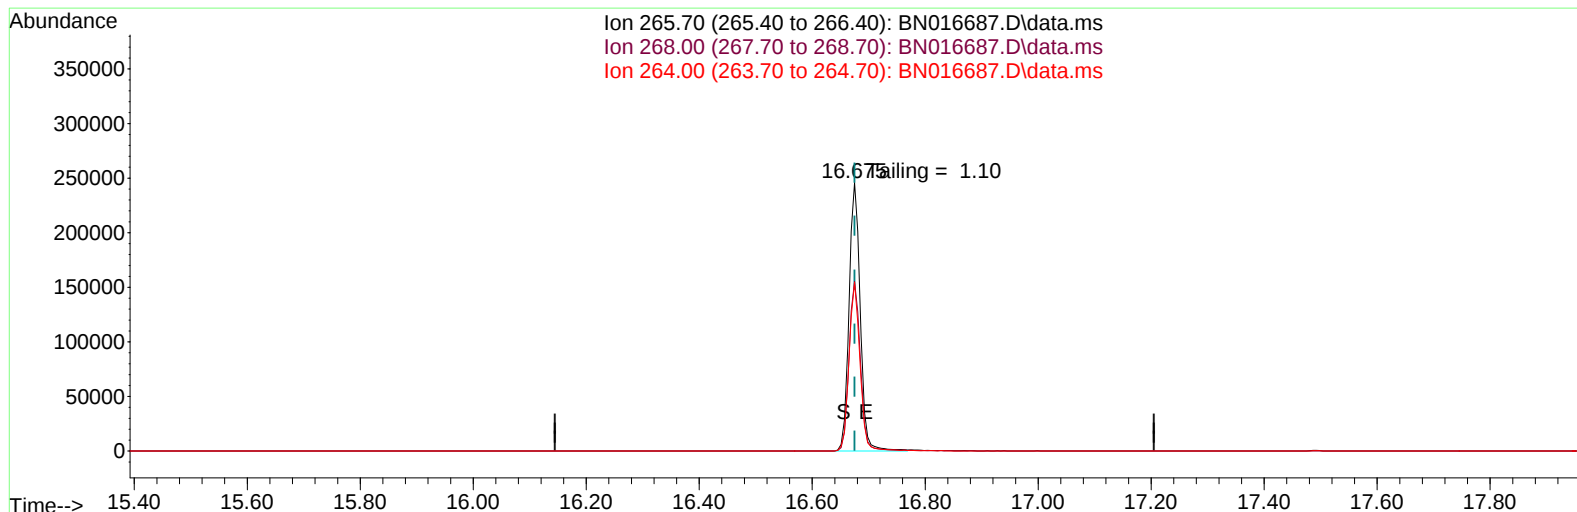

TIC: BN016687.D\data.ms

(70) Pentachlorophenol (C)

16.675min (+ 0.000) 29077.44 ng m




response 339094

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.14
264.00	61.60	62.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100121\
Data File : BN016687.D
Acq On : 03 Oct 2021 01:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 04 05:48:38 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

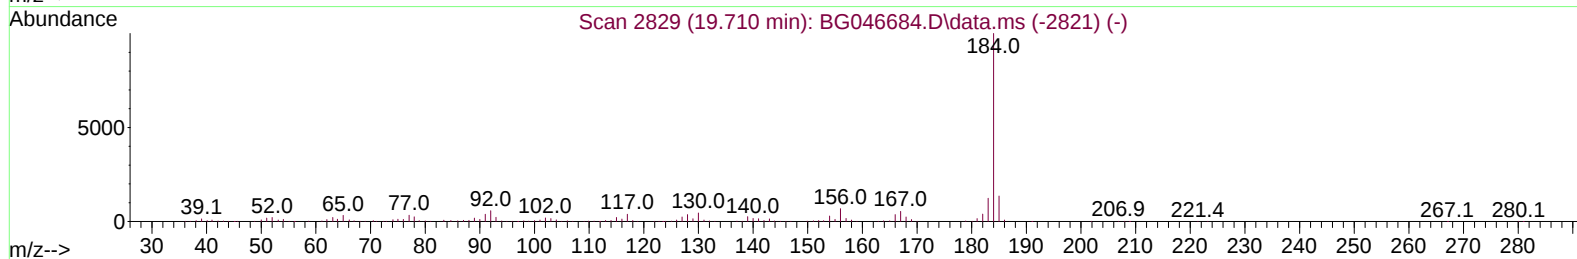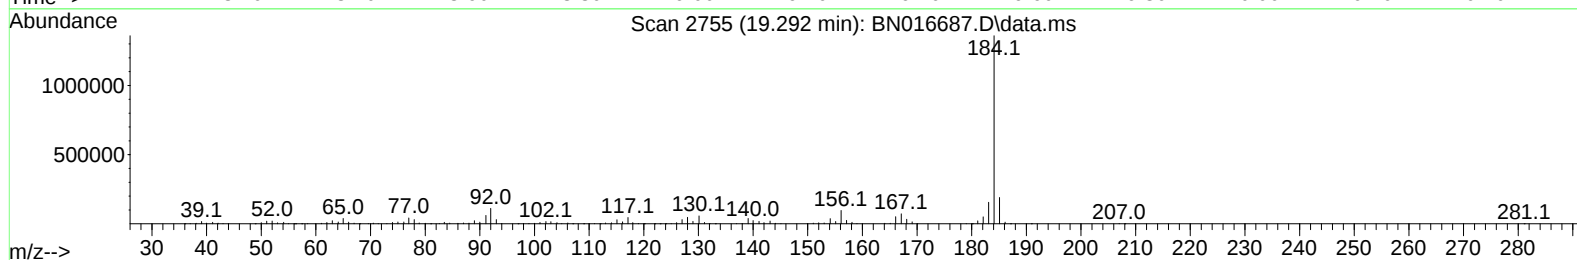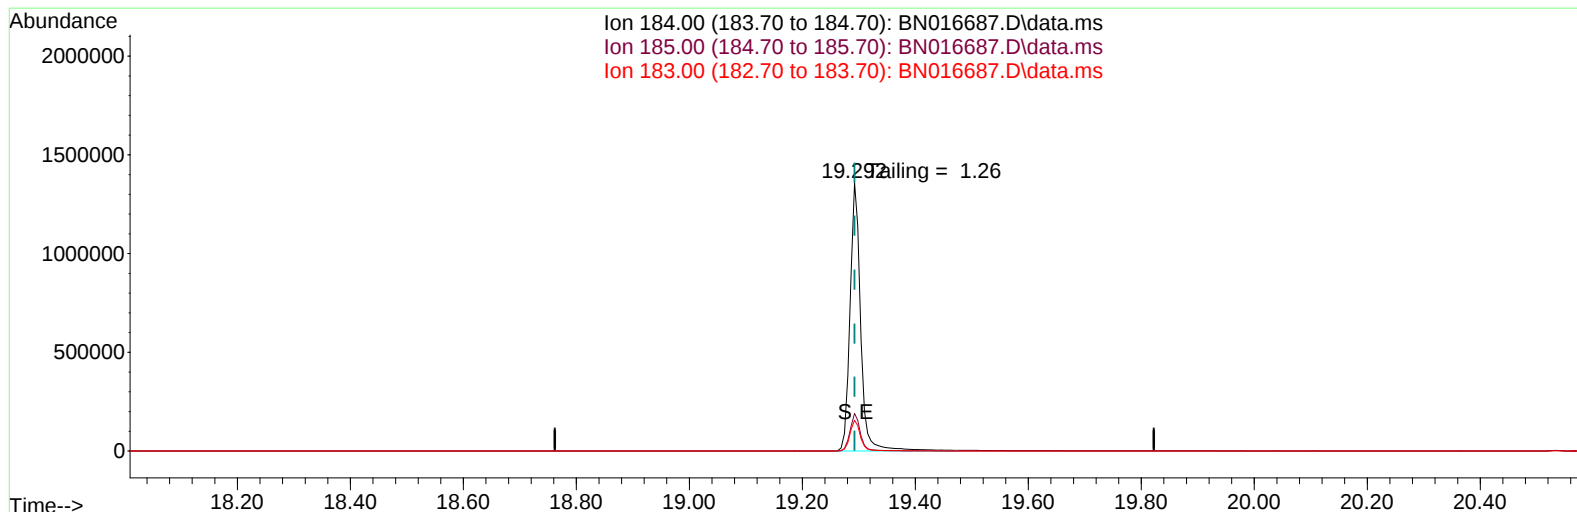

TIC: BN016687.D\data.ms

(77) Benzidine

19.292min (+ 0.000) 0.00 ng

response 1803928

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.00
183.00	13.20	11.45
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/1/2021	BNA_N	<u>BN016687.D</u>
Compound Name	Response	Retention Time
DDT	869891	20.533
DDD	28943	20.092
DDE	319	19.58
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
29262	899153	3.25