


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100622\
 Data File : BN022014.D
 Acq On : 06 Oct 2022 10:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 04 01:32:21 2022

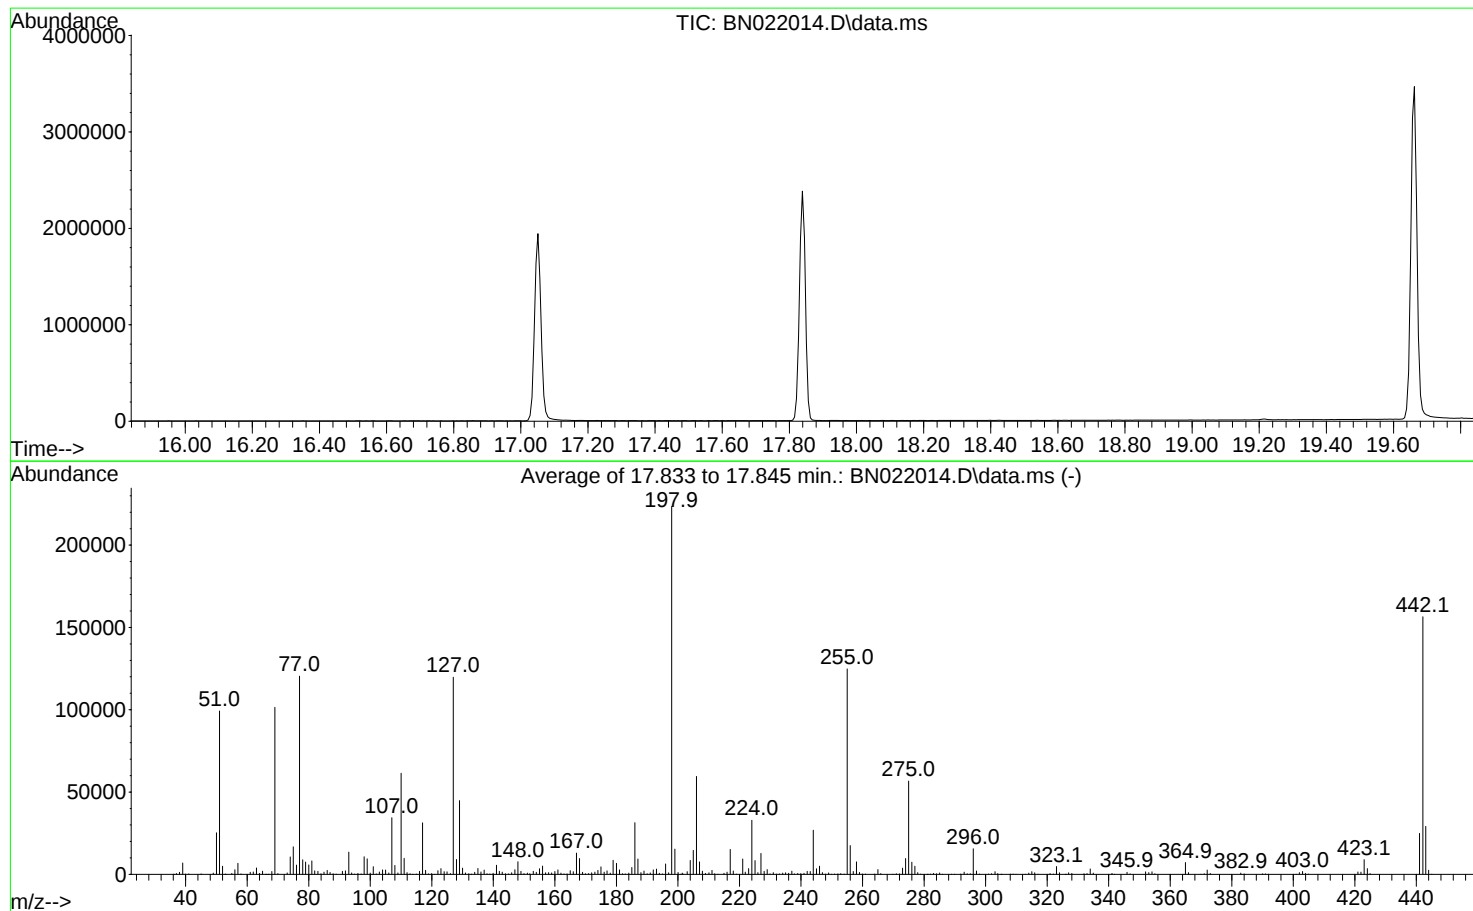




AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.4	99203	PASS
68	69	0.00	2	1.7	1714	PASS
69	198	0.00	100	45.4	101456	PASS
70	69	0.00	2	0.5	495	PASS
127	198	10	80	53.6	119765	PASS
197	198	0.00	2	0.5	1020	PASS
198	198	100	100	100.0	223467	PASS
199	198	5	9	6.9	15348	PASS
275	198	10	60	25.4	56683	PASS
365	198	1	100	3.2	7156	PASS
441	198	0.01	100	11.1	24872	PASS
442	442	50	100	100.0	156469	PASS
443	442	15	24	18.6	29133	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100622\
 Data File : BN022014.D
 Acq On : 06 Oct 2022 10:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Oct 07 05:43:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 07 05:43:37 2022
 Response via : Initial Calibration

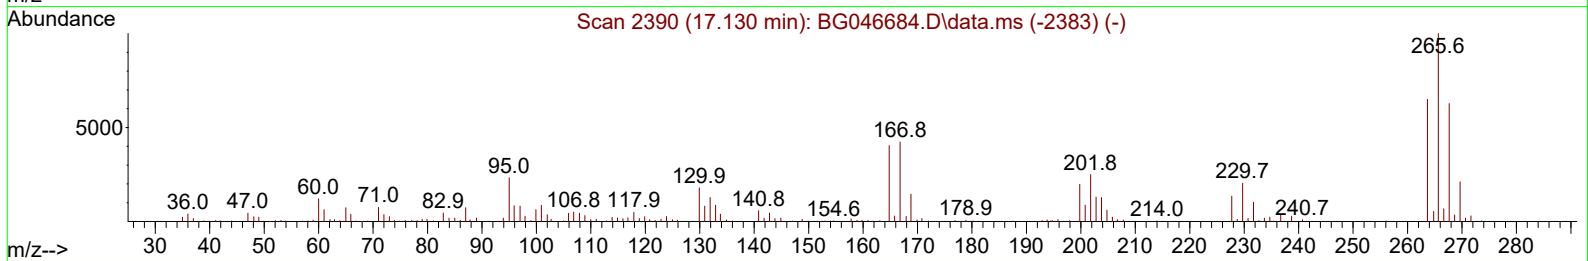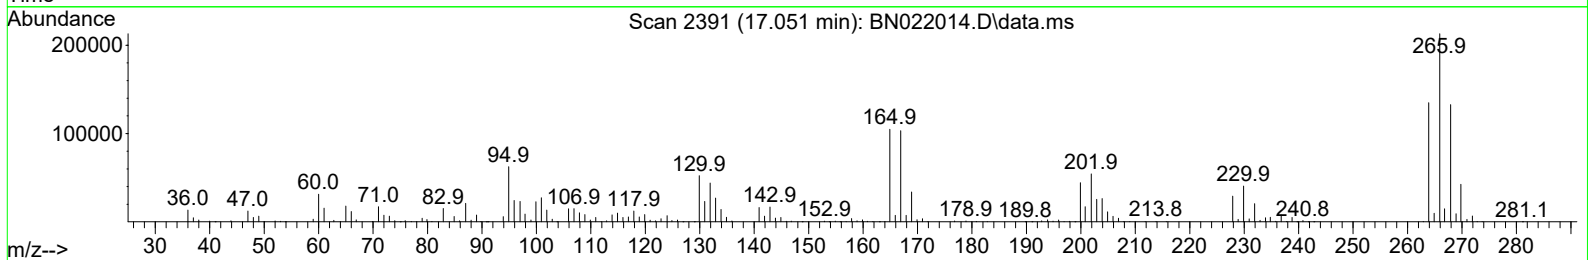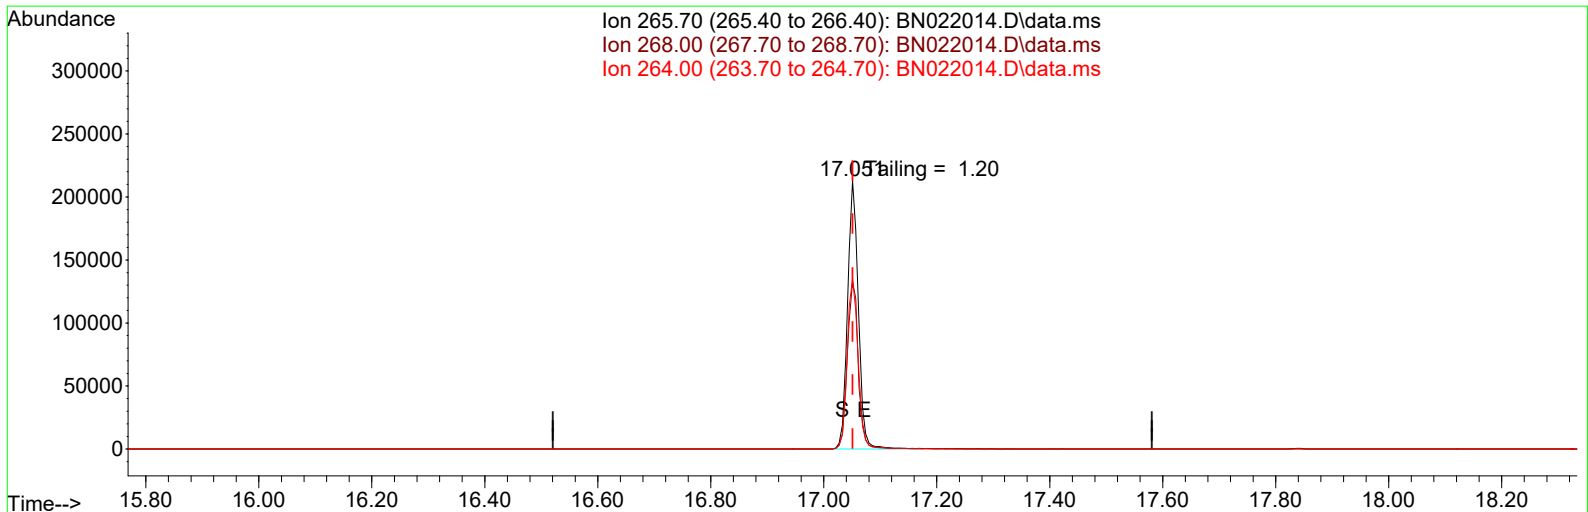

TIC: BN022014.D\data.ms

(70) Pentachlorophenol (C)

17.051min (0.000) 22407.16 ng




response 283815

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.29
264.00	61.60	63.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100622\
Data File : BN022014.D
Acq On : 06 Oct 2022 10:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 07 05:43:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 07 05:43:37 2022
Response via : Initial Calibration

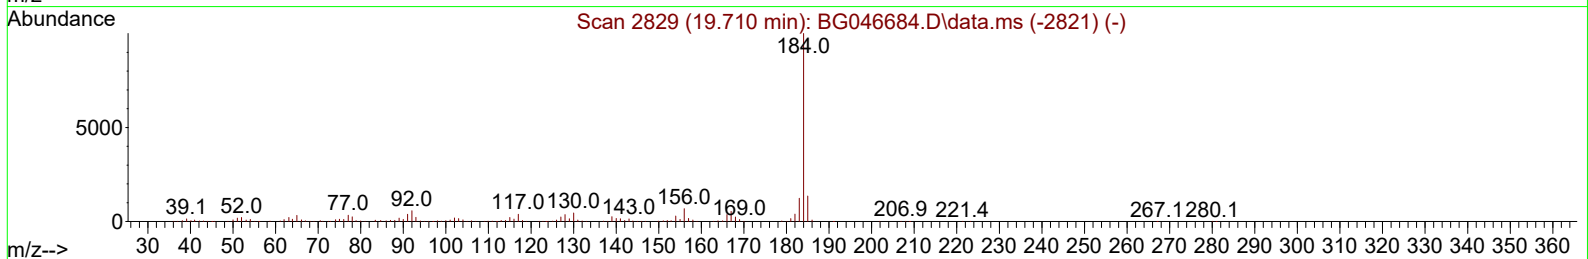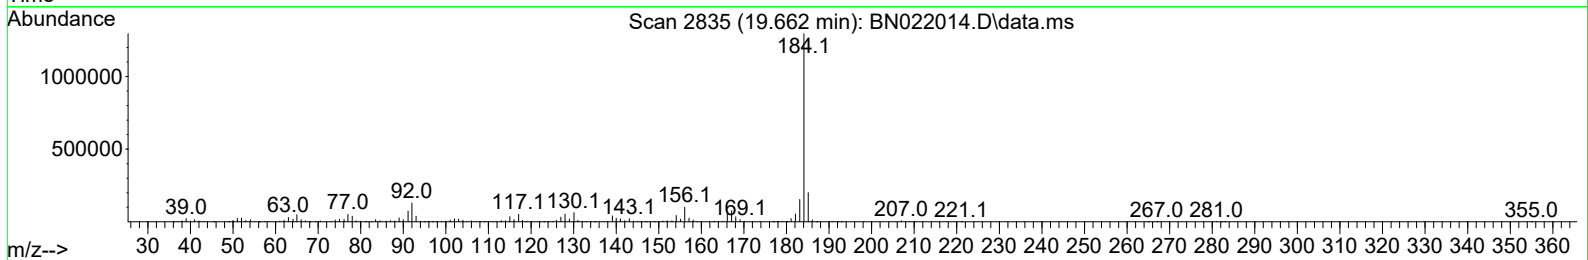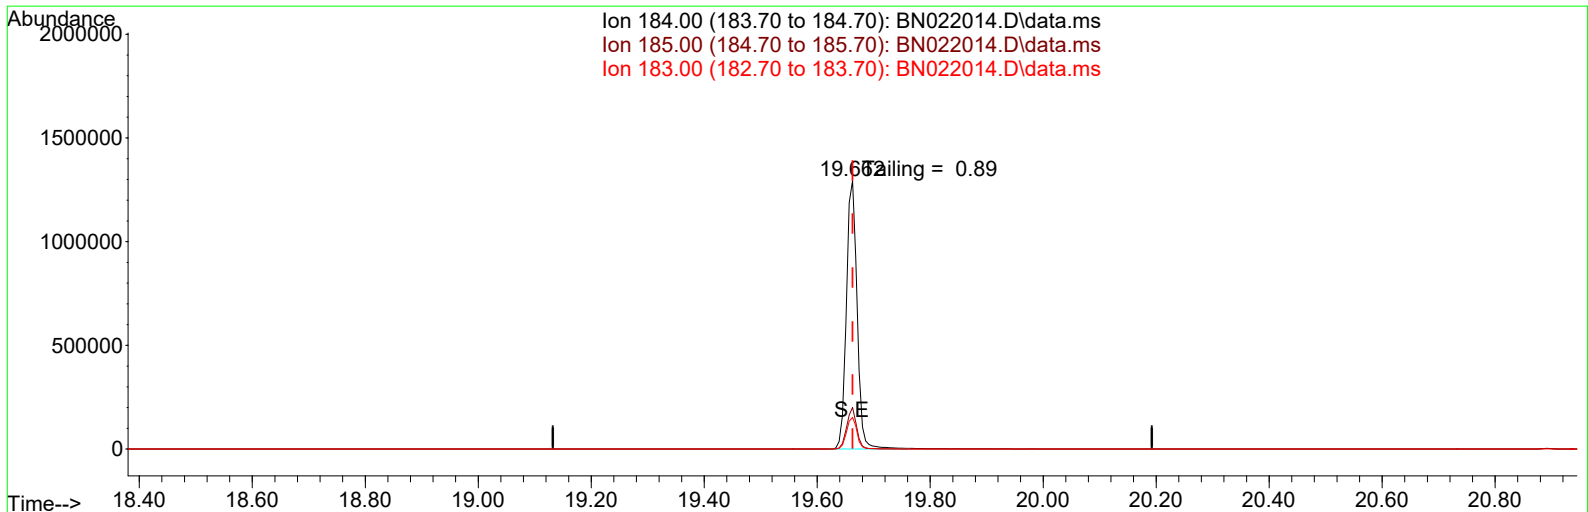

TIC: BN022014.D\data.ms

(77) Benzidine

19.662min (0.000) 0.00 ng

response 1715859

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.50
183.00	13.20	11.84
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/6/2022	BNA_N	<u>BN022014.D</u>
Compound Name	Response	Retention Time
DDT	807774	20.892
DDD	7990	20.451
DDE	414	19.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8404	816178	1.03

Instrument :
BNA_N
ClientSampleId :
DFTPP