
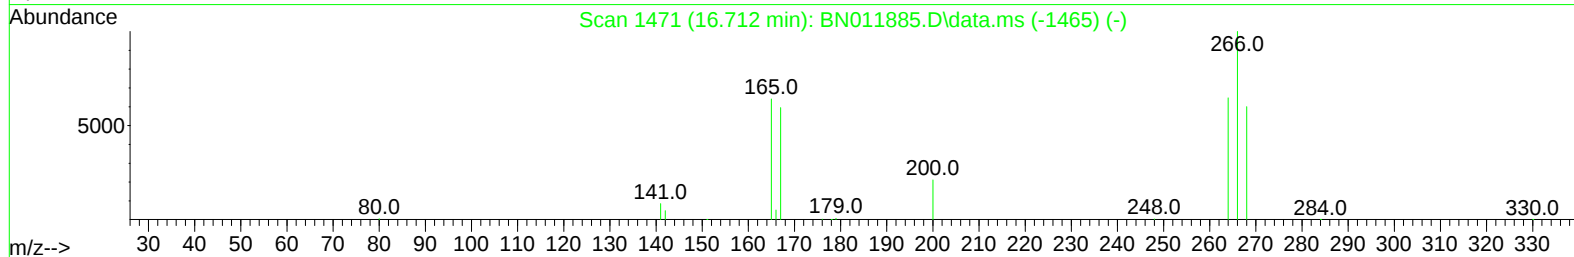
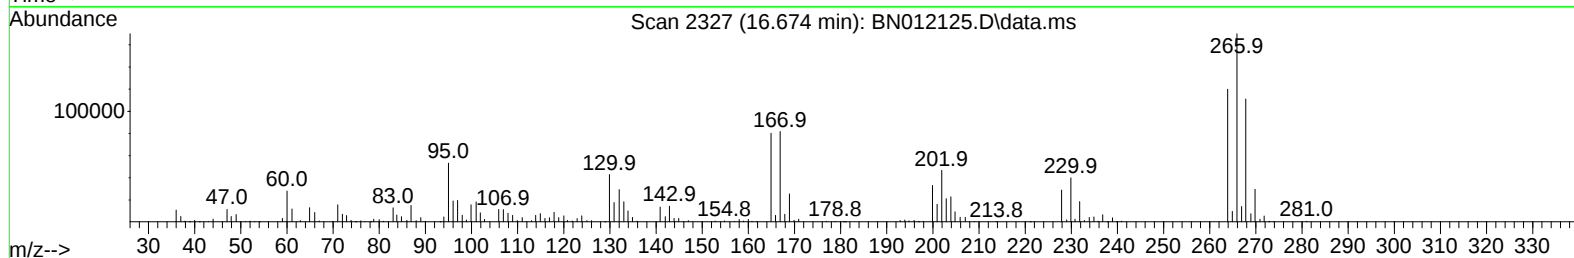


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101020\
Data File : BN012125.D
Acq On : 09 Oct 2020 16:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 10 04:30:40 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 09 18:10:29 2020
Response via : Initial Calibration

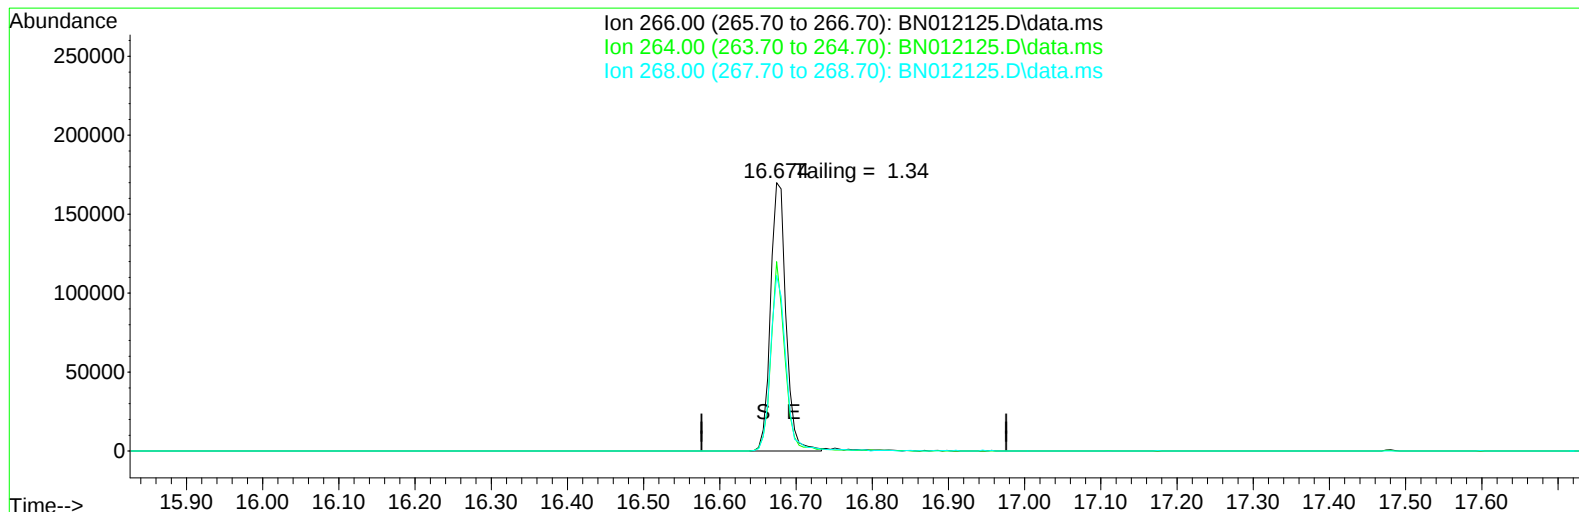

TIC: BN012125.D\data.ms

(24) Pentachlorophenol

16.676min (-16.676) 0.00 ng

response 0

Ion	Exp%	Act%
266.00	100.00	0.00
264.00	64.00	0.00#
268.00	65.50	0.00#
0.00	0.00	0.00