
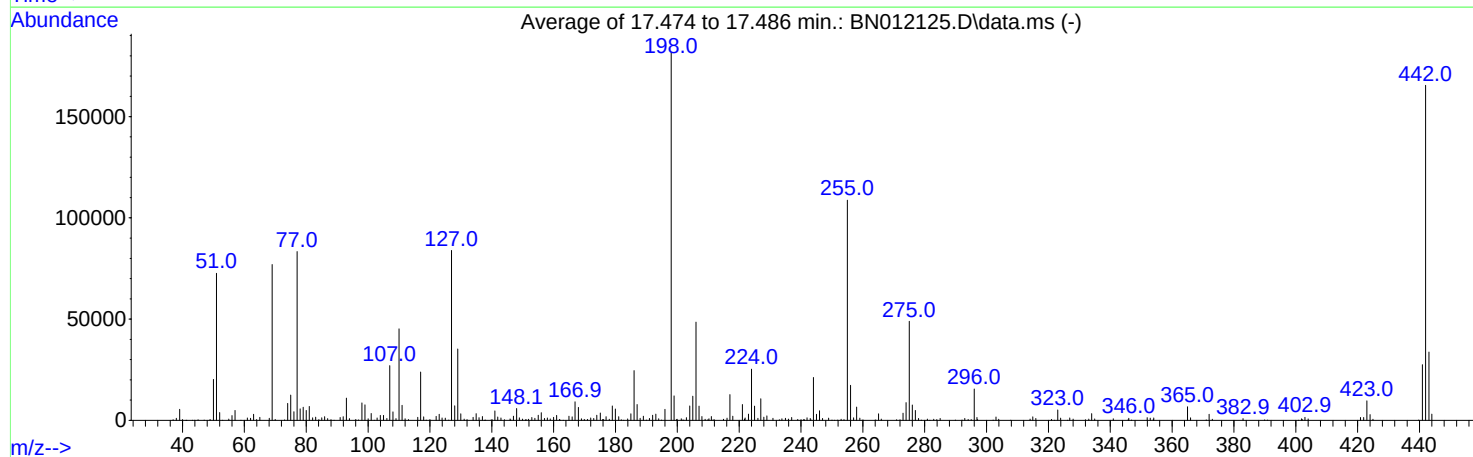


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101020\
Data File : BN012125.D
Acq On : 09 Oct 2020 16:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 12 11:15:56 2020

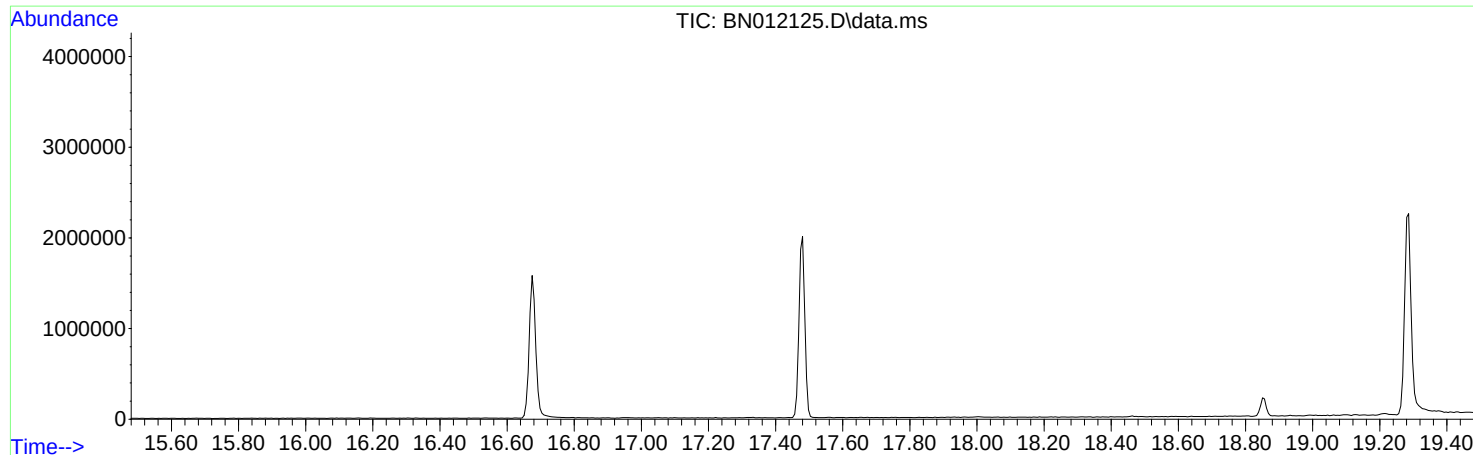

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	72627	PASS
68	69	0.00	2	1.3	1030	PASS
69	198	0.00	100	42.4	76936	PASS
70	69	0.00	2	0.6	440	PASS
127	198	10	80	46.2	83888	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	181653	PASS
199	198	5	9	6.6	12061	PASS
275	198	10	60	26.9	48901	PASS
365	198	1	100	3.7	6703	PASS
441	198	0.01	100	15.1	27501	PASS
442	198	50	100	91.1	165440	PASS
443	442	15	24	20.4	33728	PASS