

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102221\
 Data File : BN017074.D
 Acq On : 22 Oct 2021 15:56
 Operator : CG/JU
 Sample : M4207-12
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B86

Quant Time: Oct 22 16:25:15 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN101921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 22 15:39:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.548	152	1910	0.400	ng/ul	0.00
4) Naphthalene-d8	10.315	136	7983	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.197	164	4926	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.952	188	11334	0.400	ng/ul	0.00
17) Chrysene-d12	21.164	240	10893	0.400	ng/ul	0.00
23) Perylene-d12	23.376	264	14228	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.071	96	9304	4.482	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.921	152	3469	0.305	ng/ul	0.00
18) Fluoranthene-d10	18.993	212	12635	0.470	ng/ul	0.00
Target Compounds						
15) Phenanthrene	16.990	178	748	0.021	ng/ul#	Qvalue 81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102221\
Data File : BN017074.D
Acq On : 22 Oct 2021 15:56
Operator : CG/JU
Sample : M4207-12
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B86


Quant Time: Oct 22 16:25:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN101921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 22 15:39:11 2021
Response via : Initial Calibration

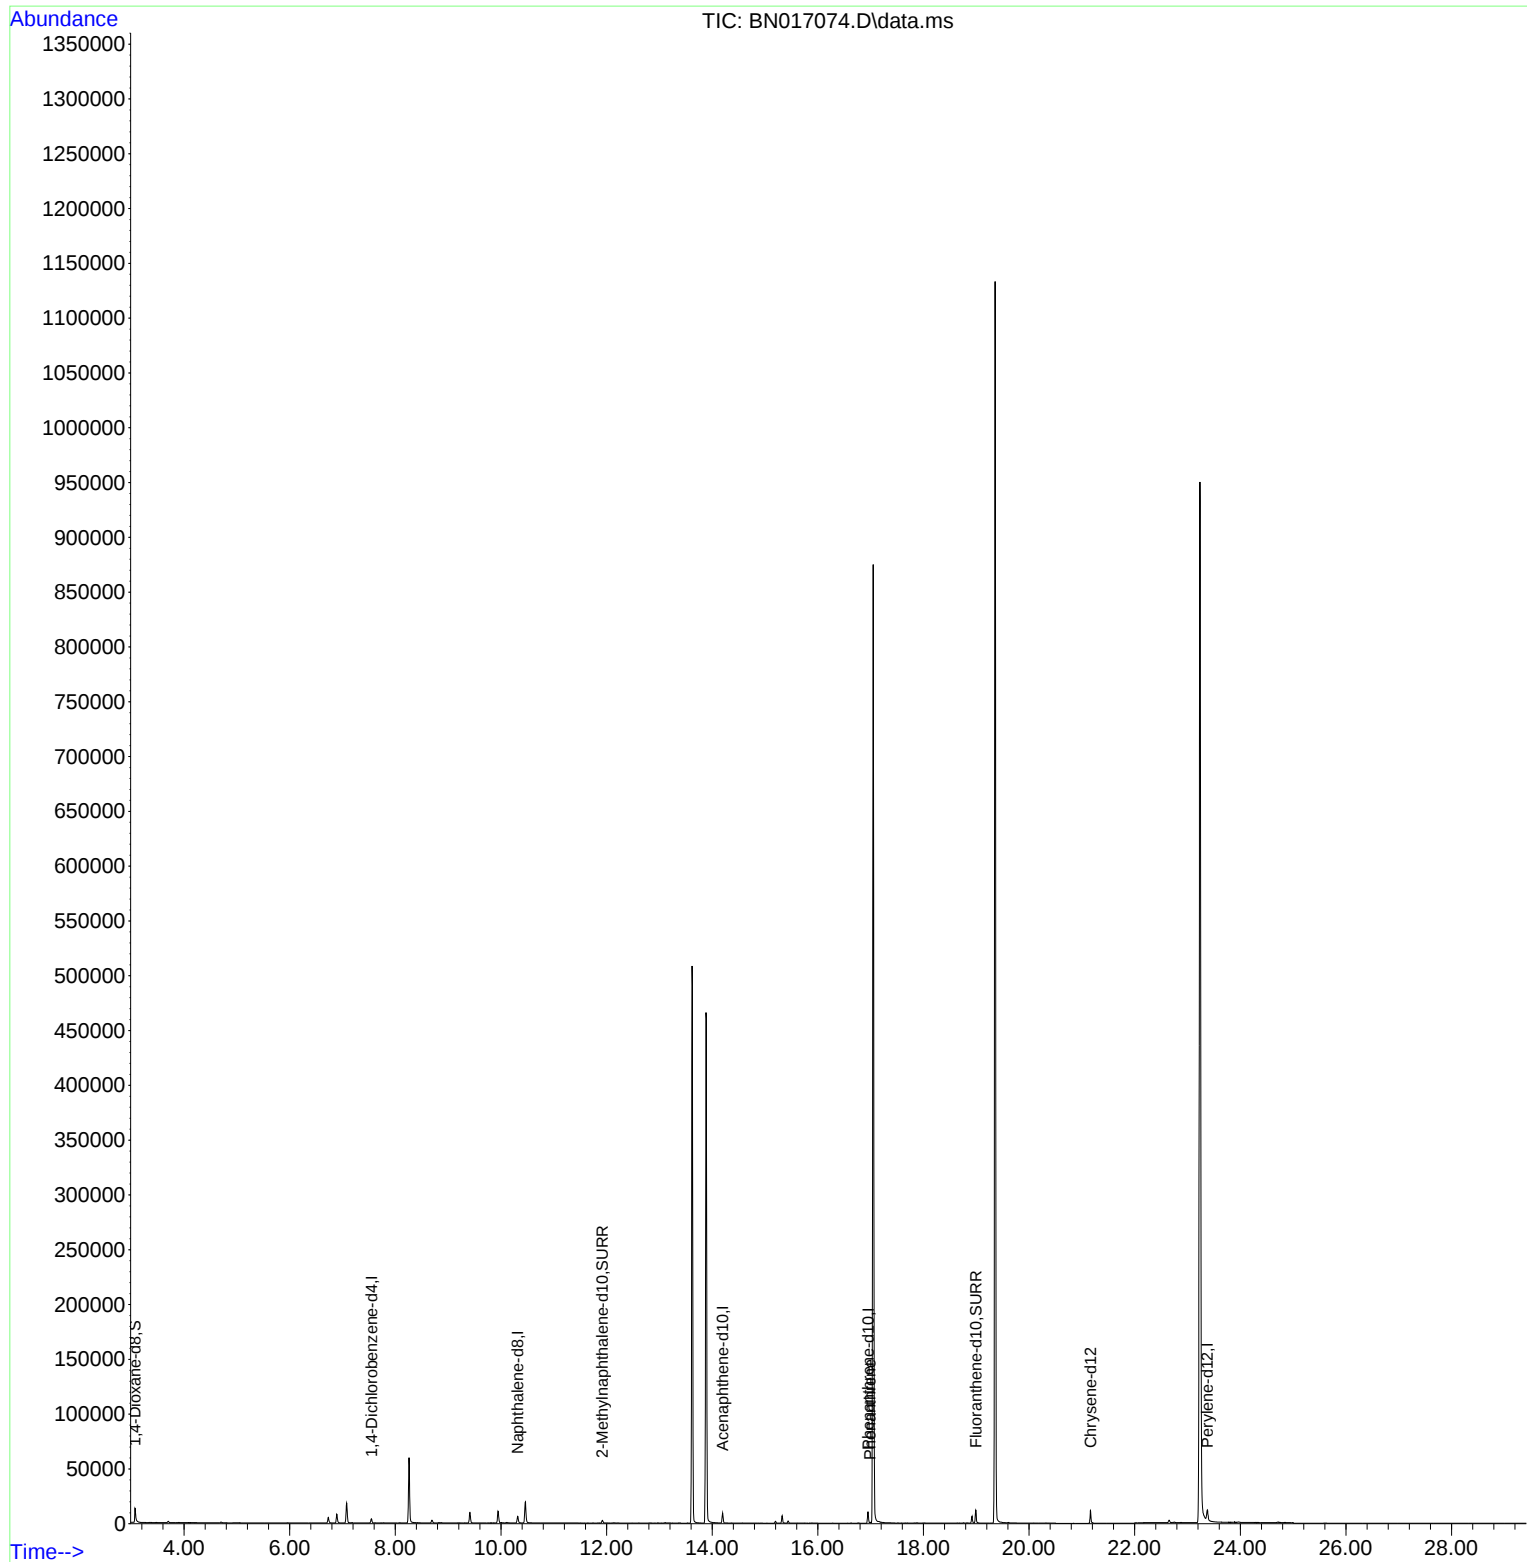

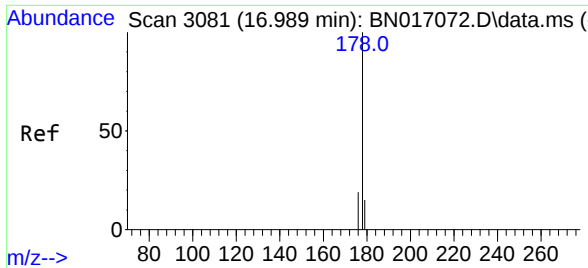

#15
 Phenanthrene
 Concen: 0.021 ng/ul
 RT: 16.990 min Scan# 3081
 Delta R.T. 0.000 min
 Lab File: BN017074.D
 Acq: 22 Oct 2021 15:56

Instrument :
 BNA_N
 ClientSampleId :
 C0B86

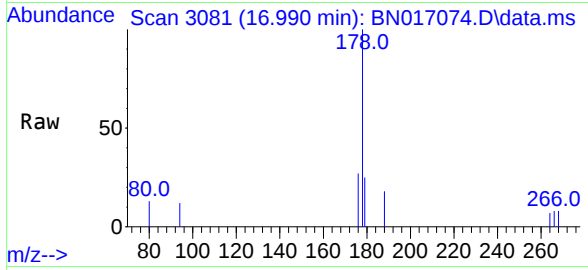

Tgt Ion:	178	Resp:	748
Ion	Ratio	Lower	Upper
178	100		
179	25.2	12.6	19.0#
176	27.2	15.9	23.9#

