
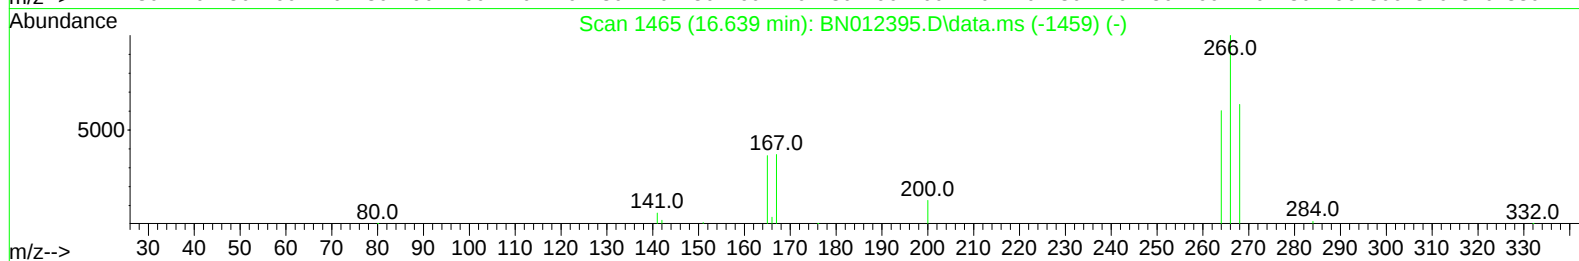
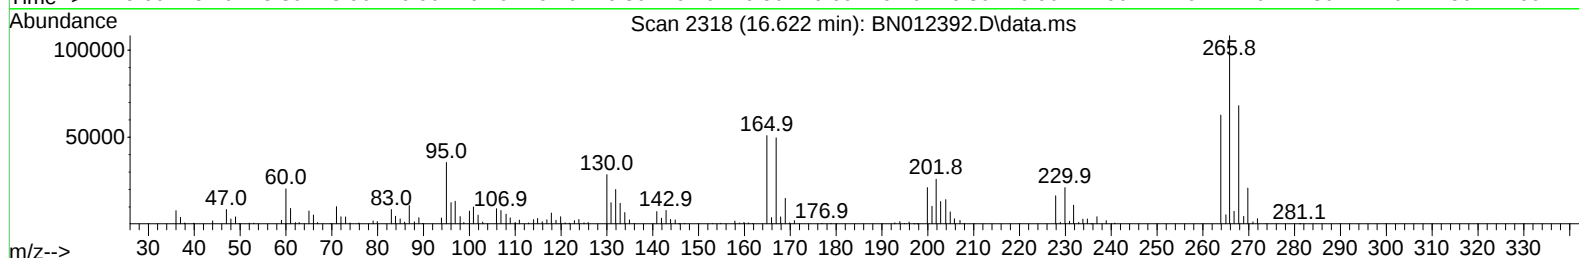


Quant Time: Oct 27 03:14:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN102620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 26 15:06:07 2020
Response via : Initial Calibration

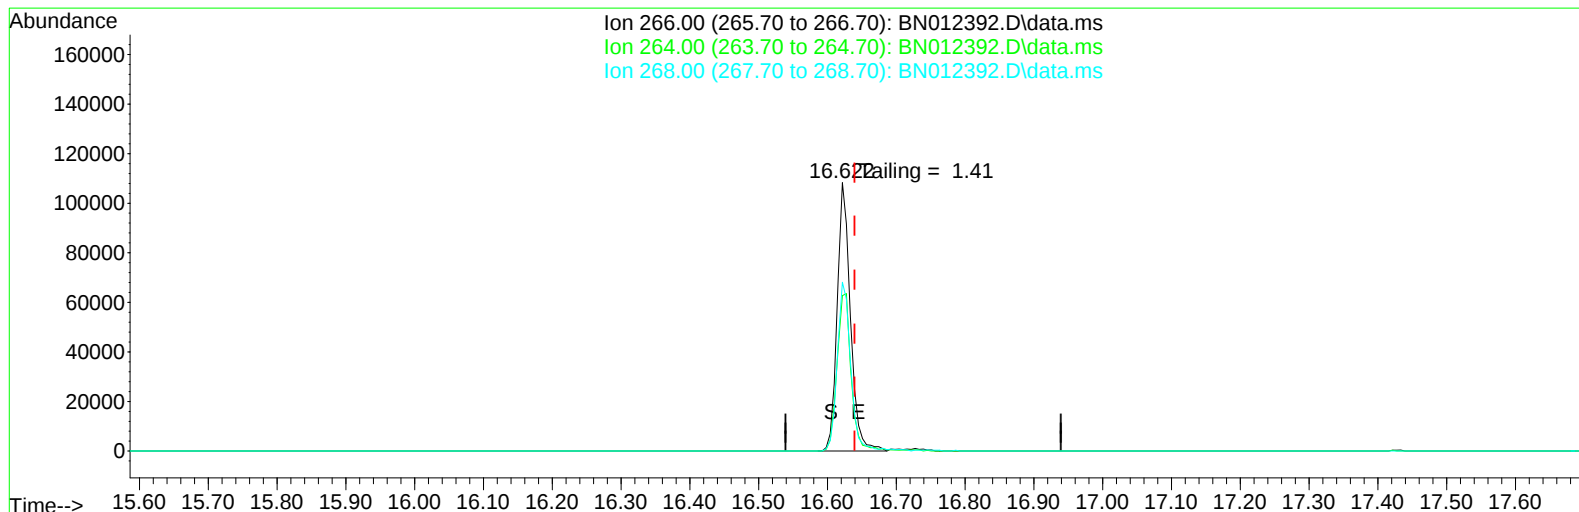

TIC: BN012392.D\data.ms

16.622min (-0.018) 0.00 ng

response **144425**

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	63.60	62.95
268.00	64.40	63.56
0.00	0.00	0.00