
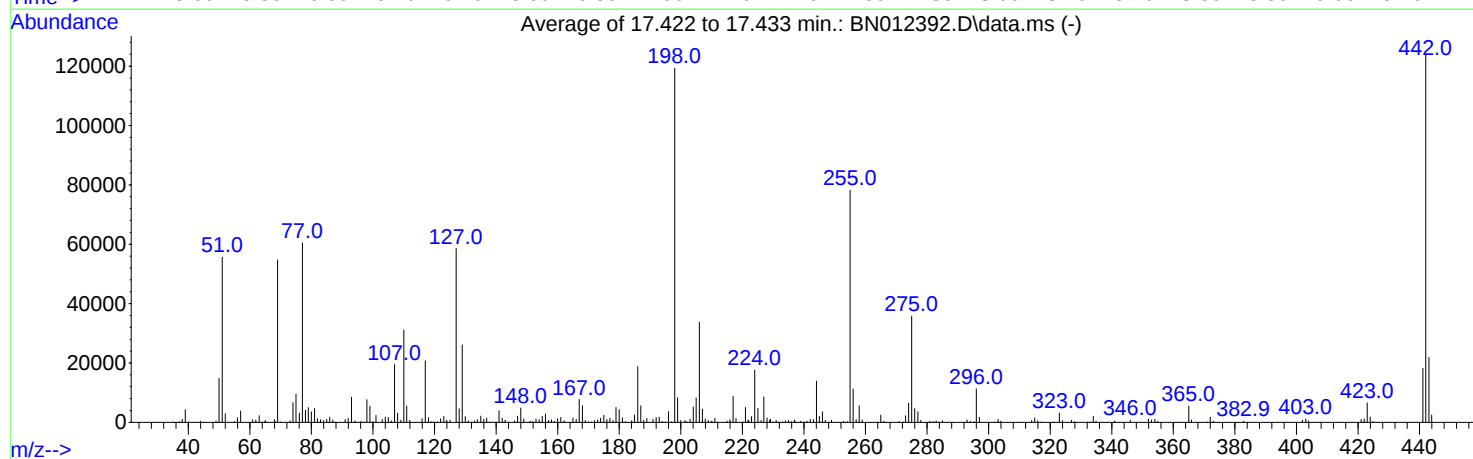


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102620\
Data File : BN012392.D
Acq On : 26 Oct 2020 10:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN102620.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 27 11:36:24 2020

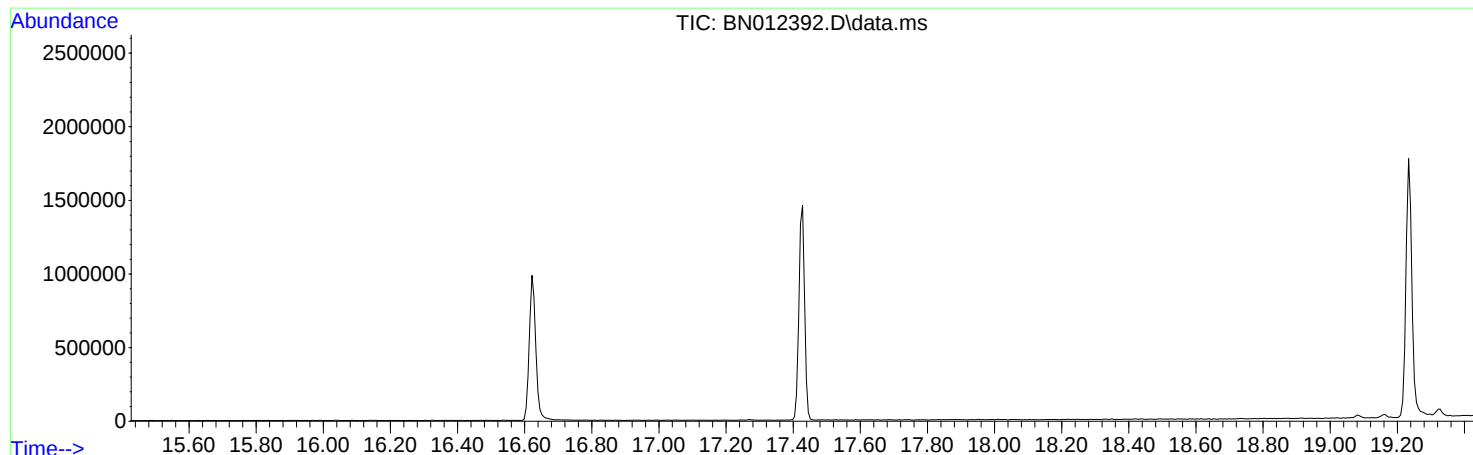

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.6	55635	PASS
68	69	0.00	2	1.7	921	PASS
69	198	0.00	100	45.9	54725	PASS
70	69	0.00	2	0.2	112	PASS
127	198	10	80	49.1	58563	PASS
197	198	0.00	2	0.2	236	PASS
198	198	100	100	100.0	119317	PASS
199	198	5	9	7.0	8305	PASS
275	198	10	60	30.0	35765	PASS
365	198	1	100	4.6	5467	PASS
441	198	0.01	100	15.2	18146	PASS
442	442	100	100	100.0	123917	PASS
443	442	15	24	17.6	21864	PASS