

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN111020\
 Data File : BN012542.D
 Acq On : 10 Nov 2020 21:28
 Operator : CG/JU
 Sample : PB132685BL
 Misc : PBBL-W-02
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK685

Quant Time: Nov 11 00:52:22 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN111020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 10 14:27:13 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.47	152	744	0.40	ng/ul	0.00
4) Naphthalene-d8	10.26	136	2627	0.40	ng/ul	0.02
9) Acenaphthene-d10	14.13	164	1504	0.40	ng/ul	0.00
13) Phenanthrene-d10	16.88	188	2829	0.40	ng/ul	0.00
19) Chrysene-d12	21.08	240	2733	0.40	ng/ul	0.00
23) Perylene-d12	23.19	264	2999	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.01	96	683	0.68	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.88	152	1120	0.30	ng/ul	0.04
17) Fluoranthene-d10	18.91	212	2845	0.40	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.02	88	75	0.074	ng/ul#	Ovalue 55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN111020\
Data File : BN012542.D
Acq On : 10 Nov 2020 21:28
Operator : CG/JU
Sample : PB132685BL
Misc : PBBL-W-02
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK685

Quant Time: Nov 11 00:52:22 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN111020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 10 14:27:13 2020
Response via : Initial Calibration

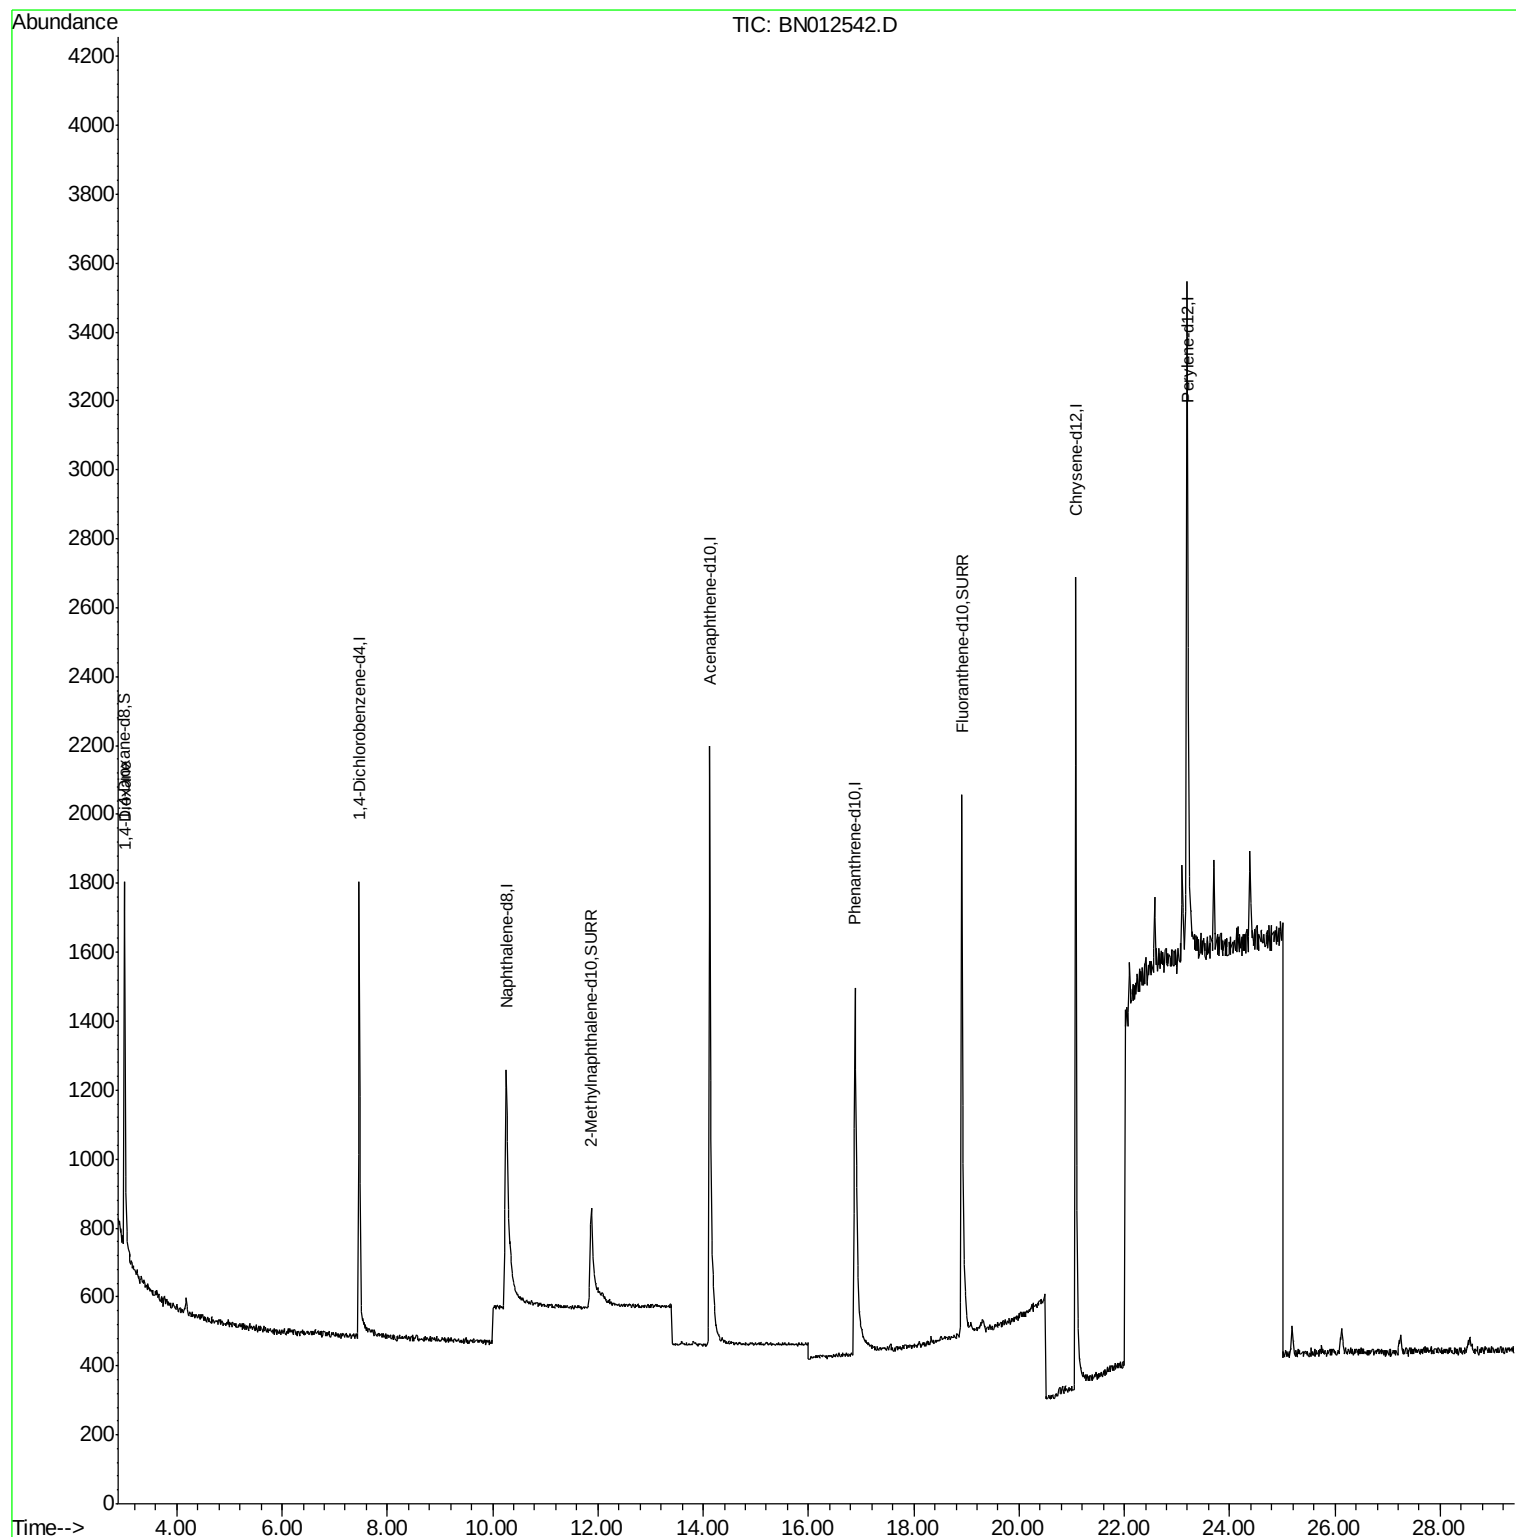

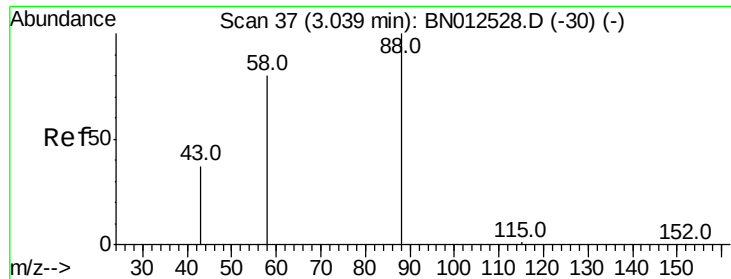

#2

1,4-Dioxane

Concen: 0.074 ng/ul

RT: 3.02 min Scan# 32

Delta R.T. -0.02 min

Lab File: BN012542.D

Acq: 10 Nov 2020 21:28

Instrument :

BNA_N

ClientSampleId :

SBLK685

Tot Ion: 88 Resp: 75

Ion Ratio Lower Upper

88 100

43 35.4 42.7 64.1#

58 22.1 57.3 85.9#

