
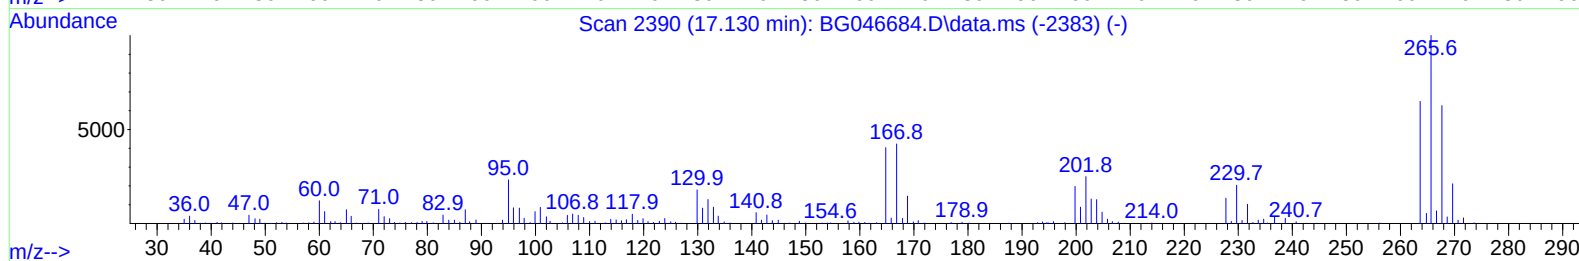
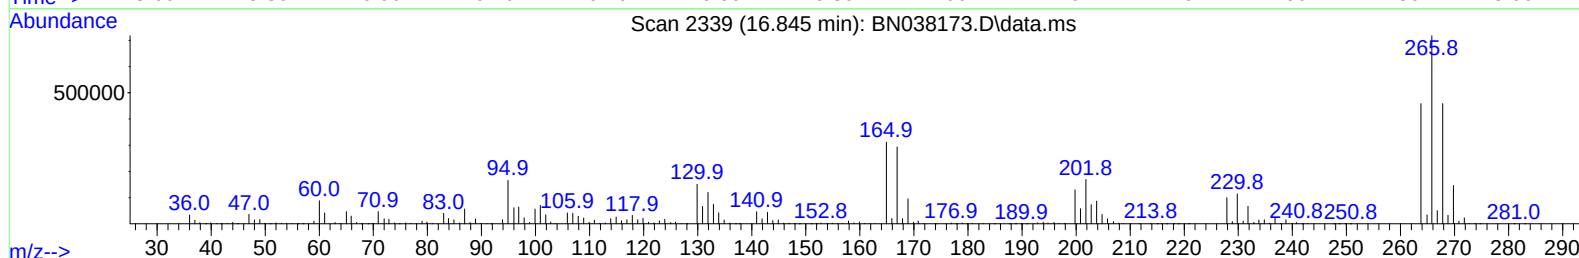


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111025\
Data File : BN038173.D
Acq On : 10 Nov 2025 09:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 10:10:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 10 10:10:34 2025
Response via : Initial Calibration

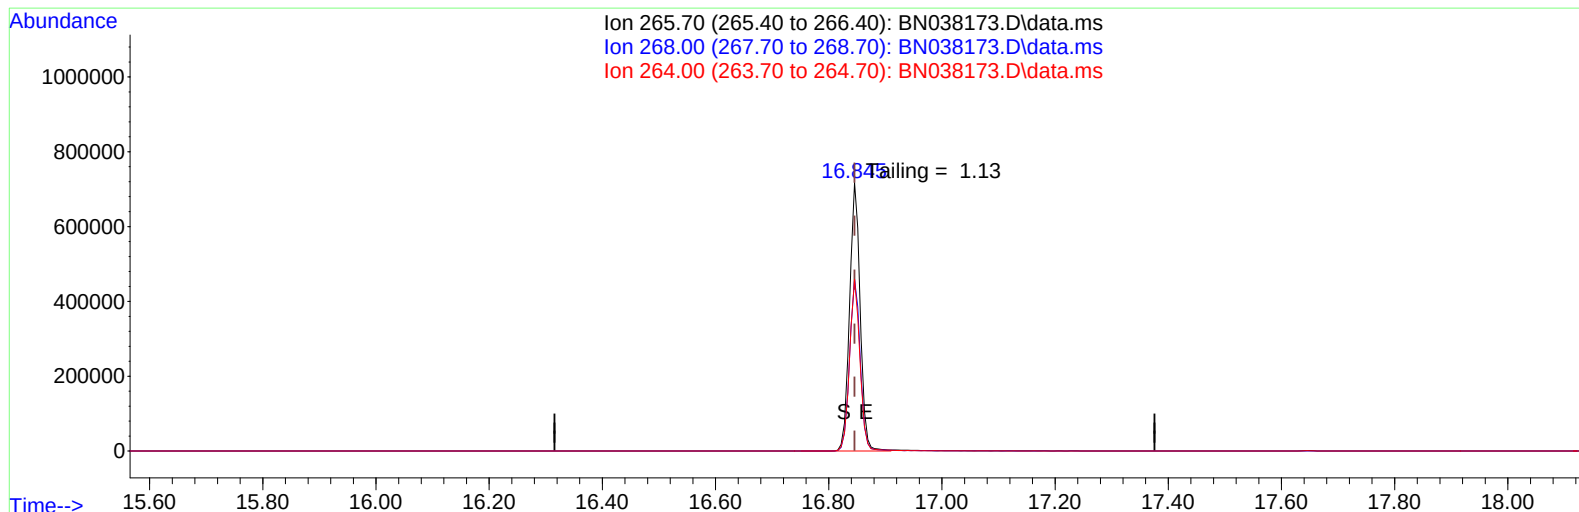

TIC: BN038173.D\data.ms

(70) Pentachlorophenol (C)




16.845min (0.000) 277.71 ng

response 940981

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.90
264.00	61.60	63.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111025\
Data File : BN038173.D
Acq On : 10 Nov 2025 09:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 10:10:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 10 10:10:34 2025
Response via : Initial Calibration

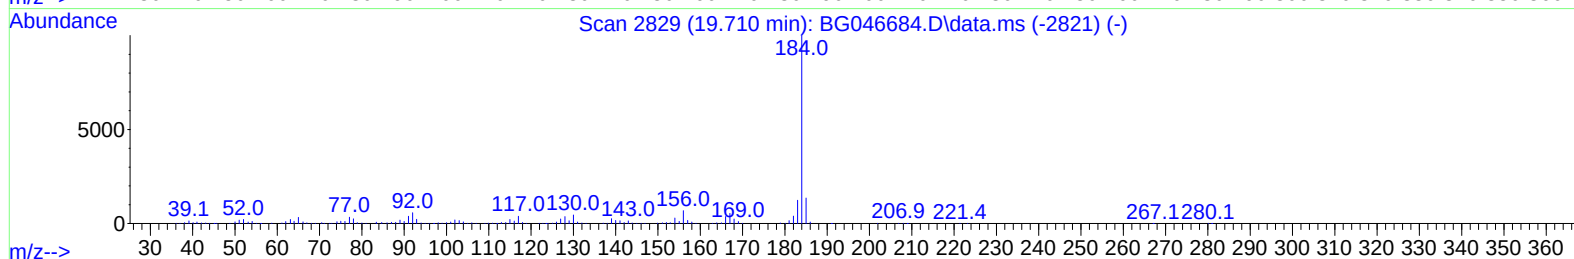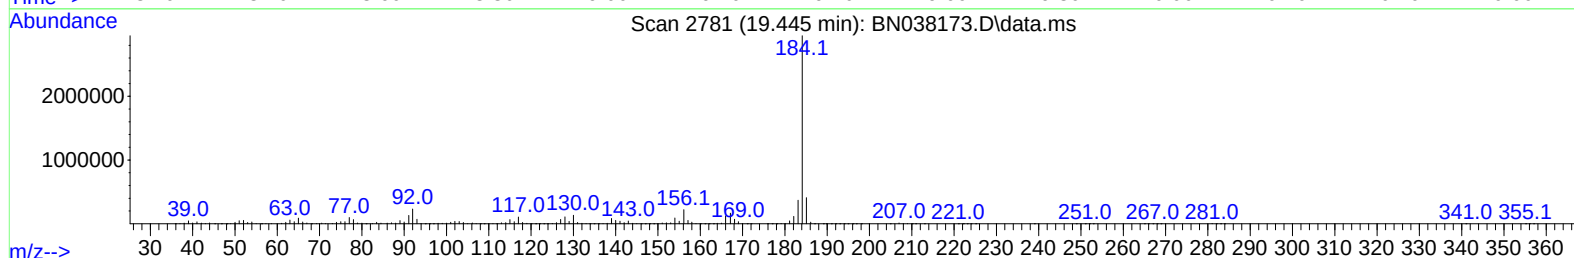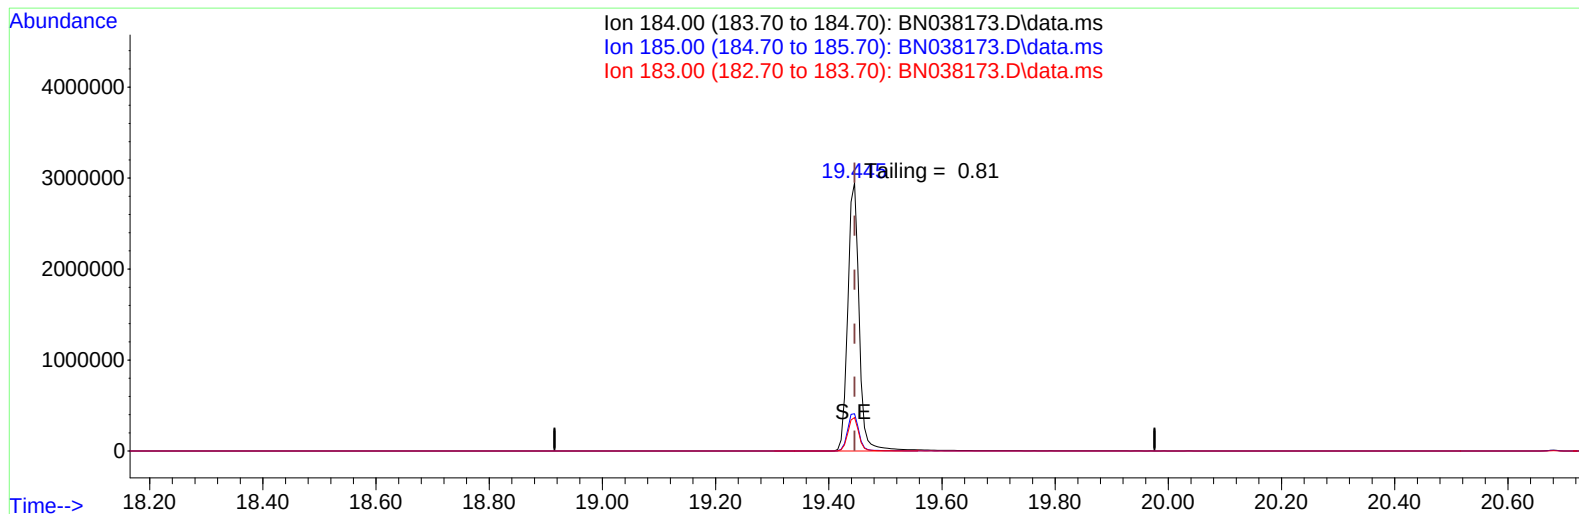

TIC: BN038173.D\data.ms

(77) Benzidine

19.445min (0.000) 280.15 ng

response 4168590

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.90
183.00	13.20	12.49
0.00	0.00	0.00