
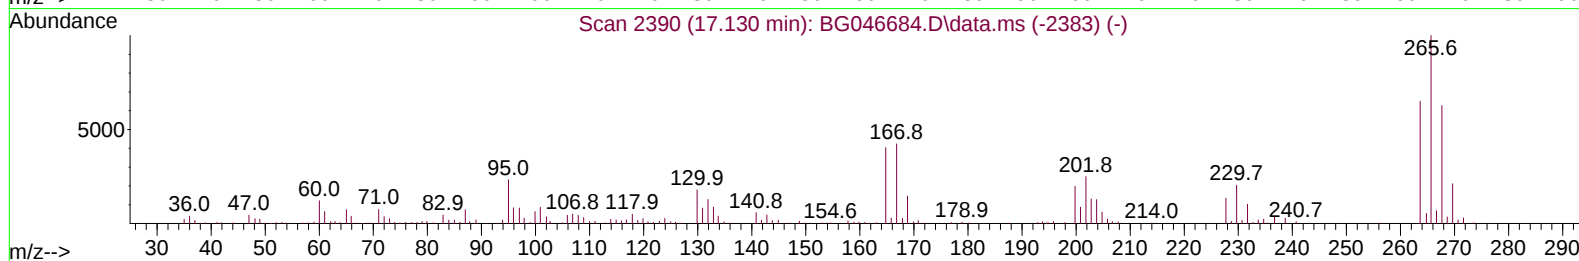
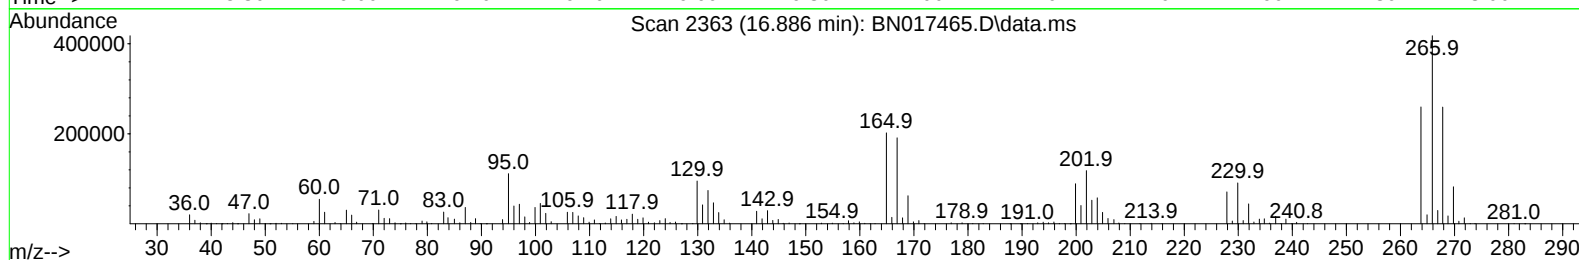


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111621\
Data File : BN017465.D
Acq On : 16 Nov 2021 07:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 15:53:11 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 16 15:52:55 2021
Response via : Initial Calibration

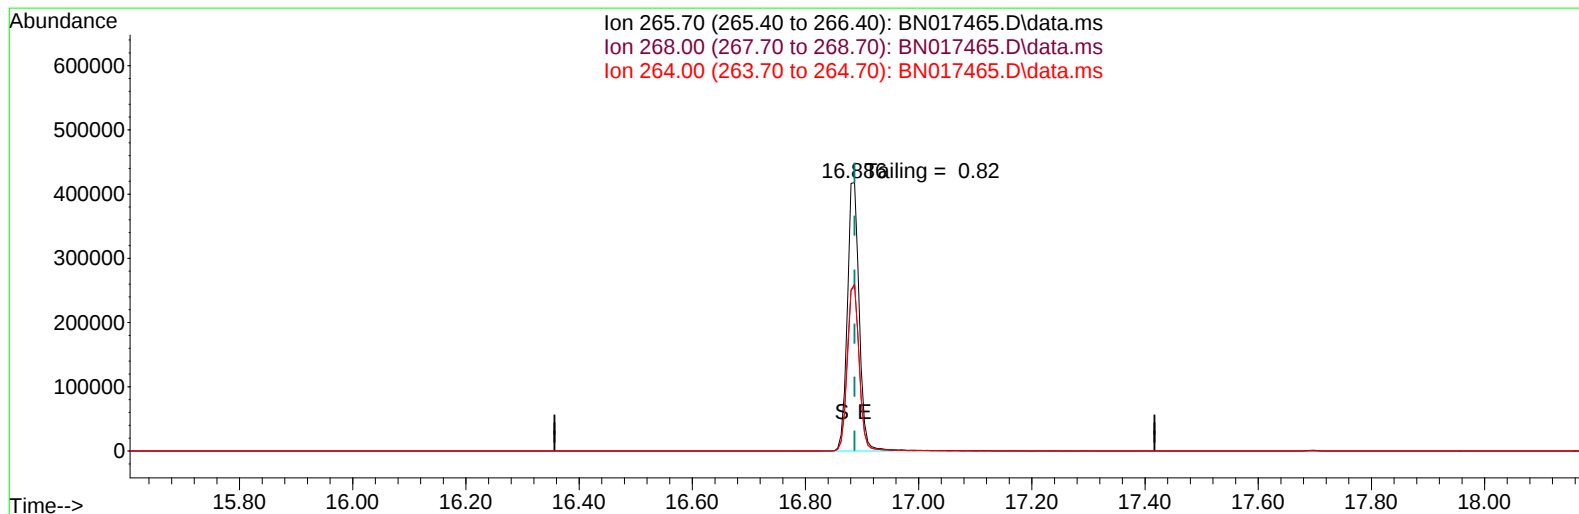

TIC: BN017465.D\data.ms

(70) Pentachlorophenol (C)




16.886min (0.000) 20465.43 ng

response 610148

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.05
264.00	61.60	62.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111621\
Data File : BN017465.D
Acq On : 16 Nov 2021 07:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 15:53:11 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 16 15:52:55 2021
Response via : Initial Calibration

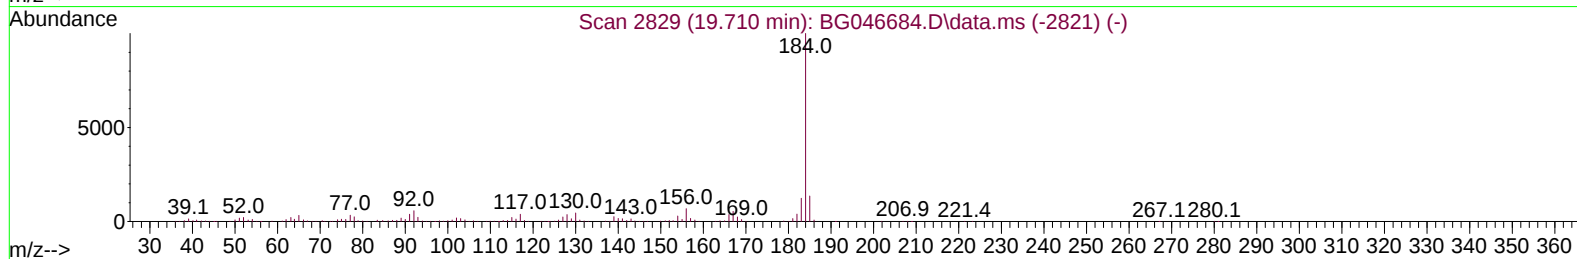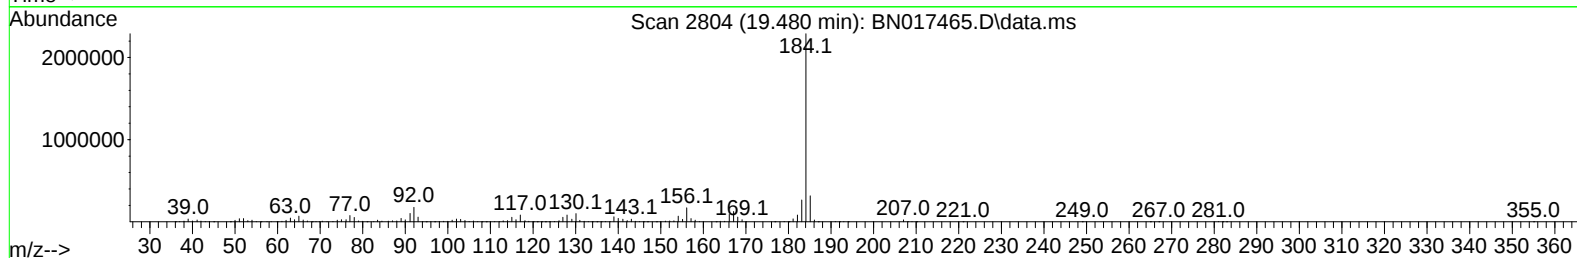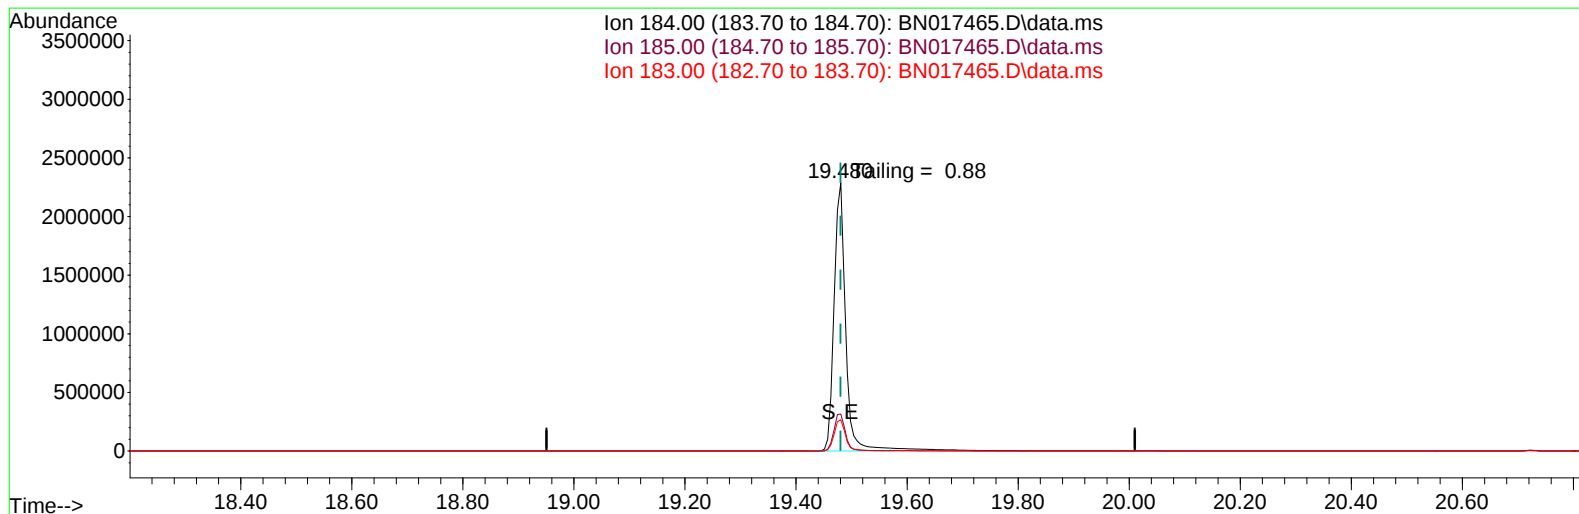

TIC: BN017465.D\data.ms

(77) Benzidine

19.480min (0.000) 0.00 ng

response 3383978

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.82
183.00	13.20	11.62
0.00	0.00	0.00