
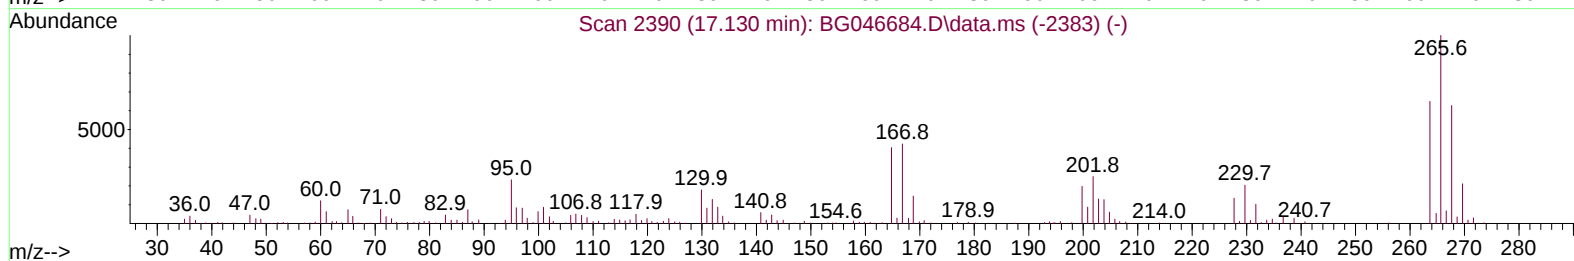
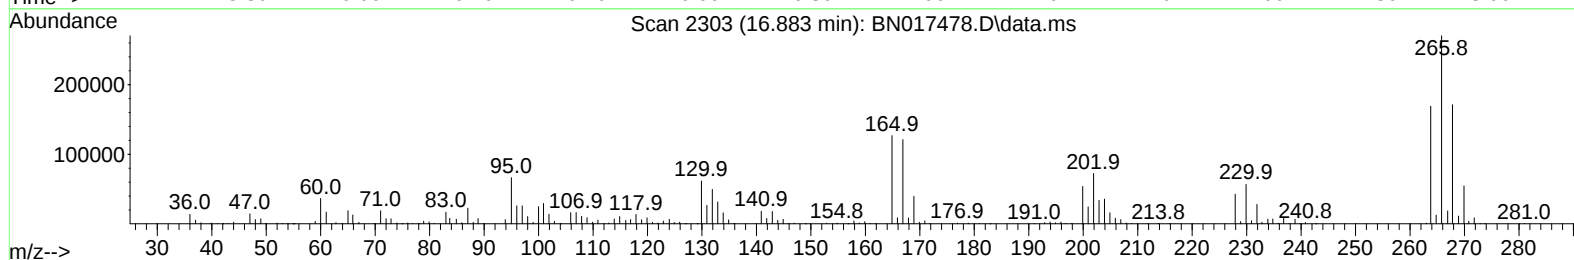


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111621\
 Data File : BN017478.D
 Acq On : 16 Nov 2021 19:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 03:12:56 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 17 03:12:51 2021
 Response via : Initial Calibration

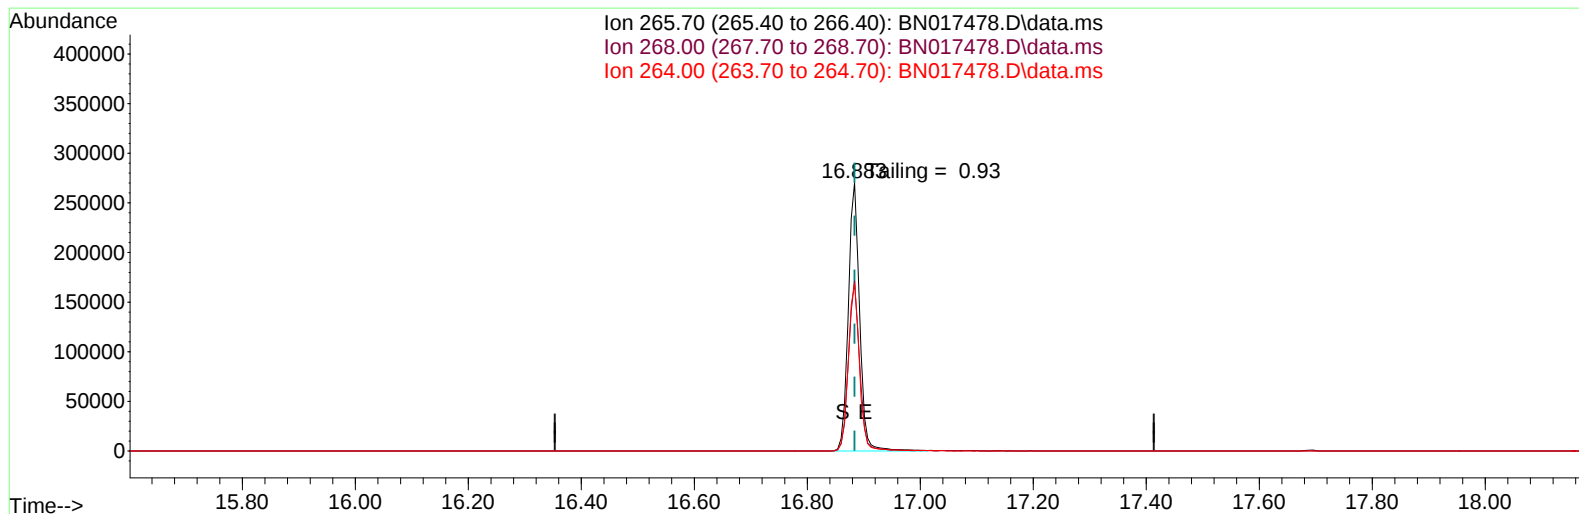

TIC: BN017478.D\data.ms

(70) Pentachlorophenol (C)




16.883min (0.000) 17508.06 ng

response 376885

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.36
264.00	61.60	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111621\
Data File : BN017478.D
Acq On : 16 Nov 2021 19:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 03:12:56 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 17 03:12:51 2021
Response via : Initial Calibration

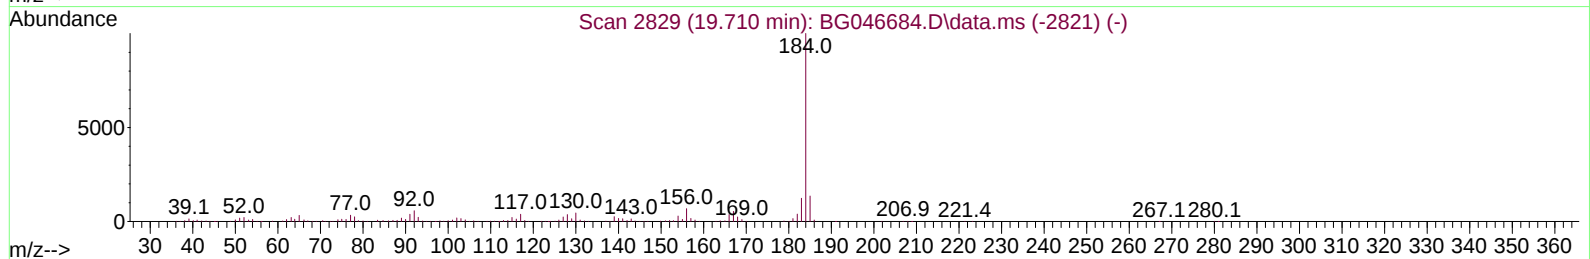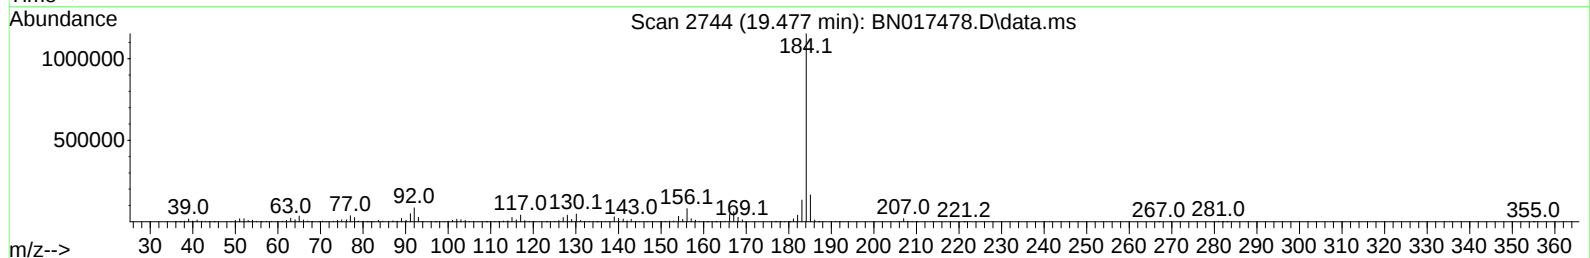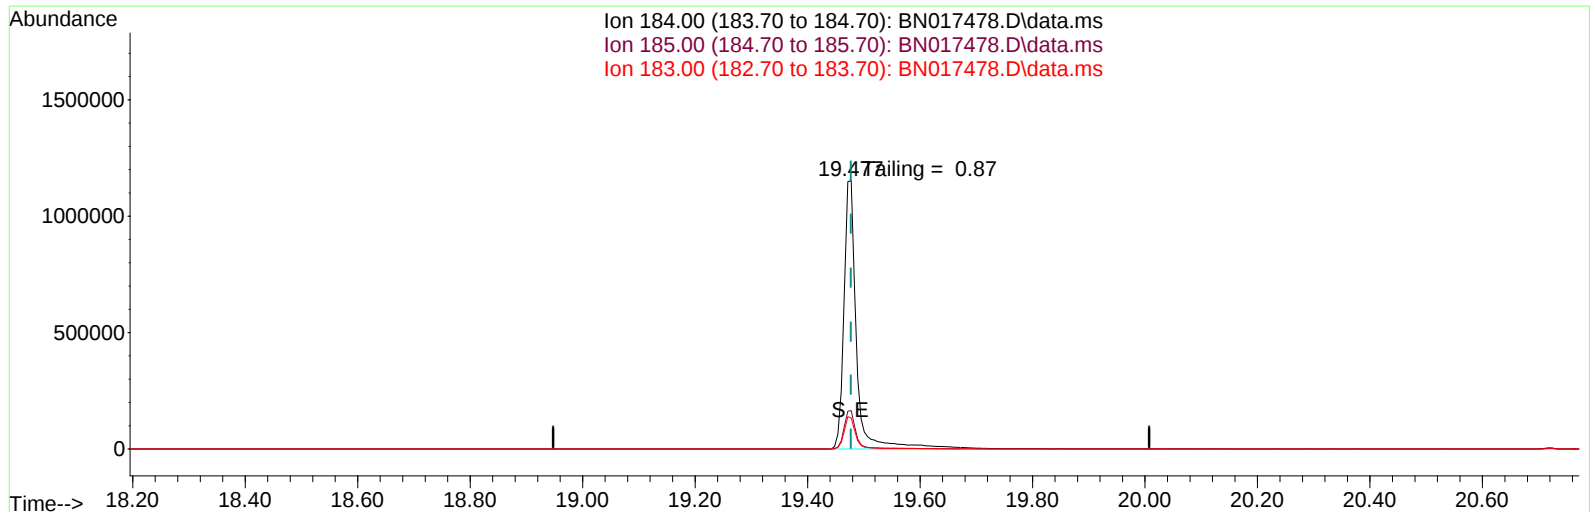

TIC: BN017478.D\data.ms

(77) Benzidine

19.477min (0.000) 0.00 ng

response 1809970

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.32
183.00	13.20	11.57
0.00	0.00	0.00