
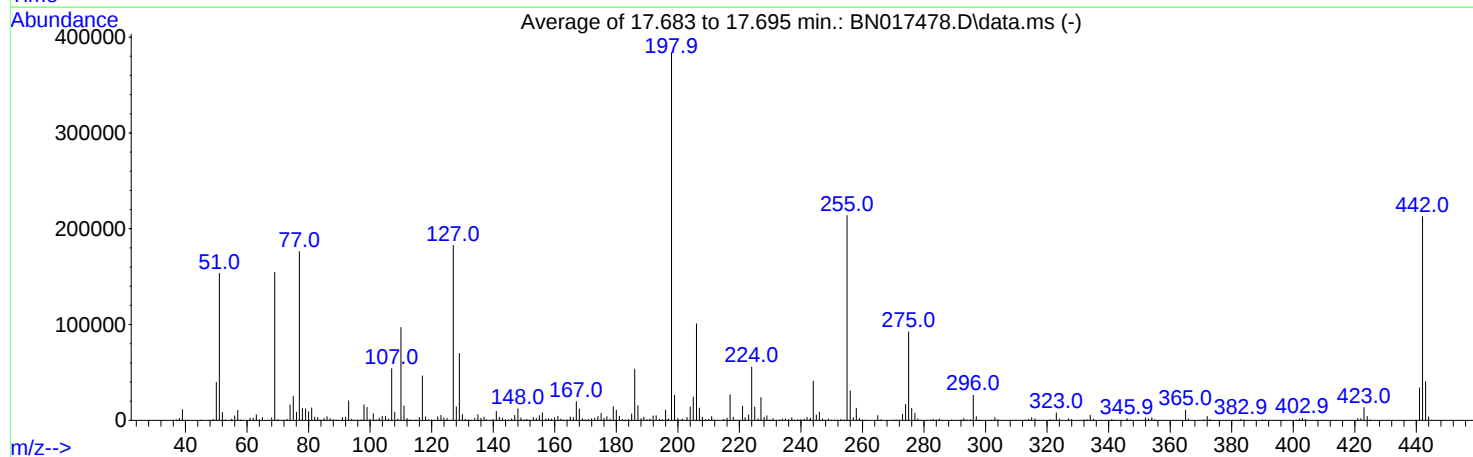


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111621\
 Data File : BN017478.D
 Acq On : 16 Nov 2021 19:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN111621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 16 14:06:59 2021

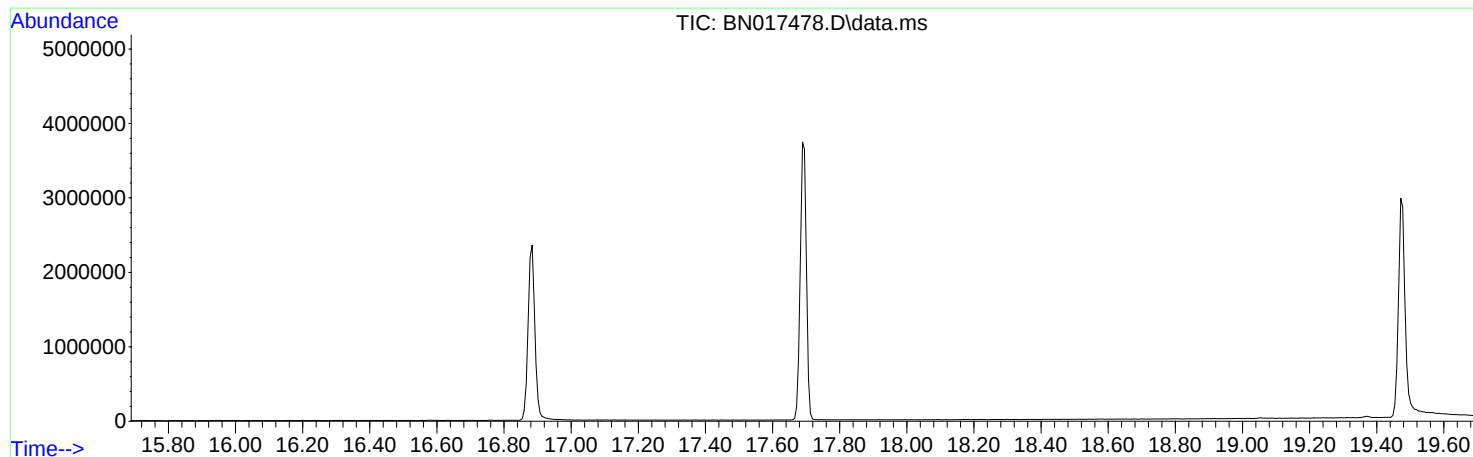




AutoFind: Scans 2439, 2440, 2441; Background Corrected with Scan 2433

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	153453	PASS
68	69	0.00	2	1.7	2613	PASS
69	198	0.00	100	40.2	154483	PASS
70	69	0.00	2	0.5	849	PASS
127	198	10	80	47.5	182464	PASS
197	198	0.00	2	0.4	1435	PASS
198	198	100	100	100.0	383936	PASS
199	198	5	9	6.9	26389	PASS
275	198	10	60	24.1	92427	PASS
365	198	1	100	2.8	10678	PASS
441	198	0.01	100	8.8	33872	PASS
442	442	50	100	100.0	212816	PASS
443	442	15	24	19.1	40555	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111621\
 Data File : BN017478.D
 Acq On : 16 Nov 2021 19:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Nov 17 03:12:56 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 17 03:12:51 2021
 Response via : Initial Calibration

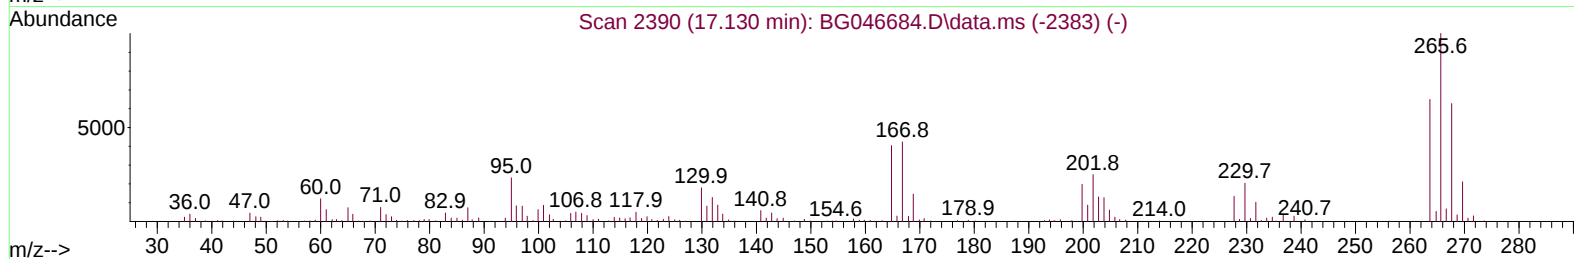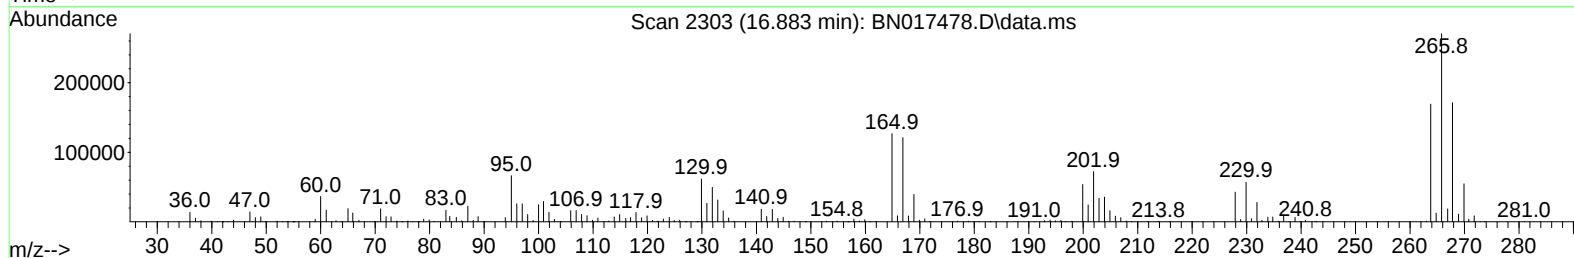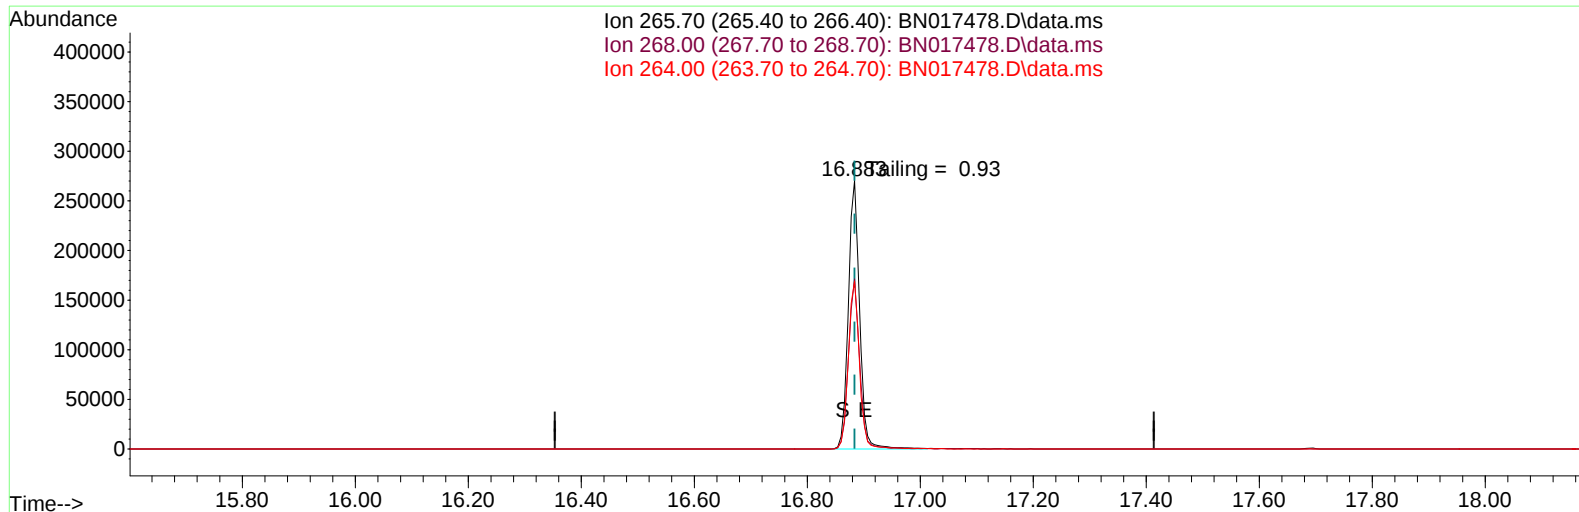

TIC: BN017478.D\data.ms

(70) Pentachlorophenol (C)

16.883min (0.000) 17508.06 ng




response 376885

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.36
264.00	61.60	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111621\
Data File : BN017478.D
Acq On : 16 Nov 2021 19:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 17 03:12:56 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 17 03:12:51 2021
Response via : Initial Calibration

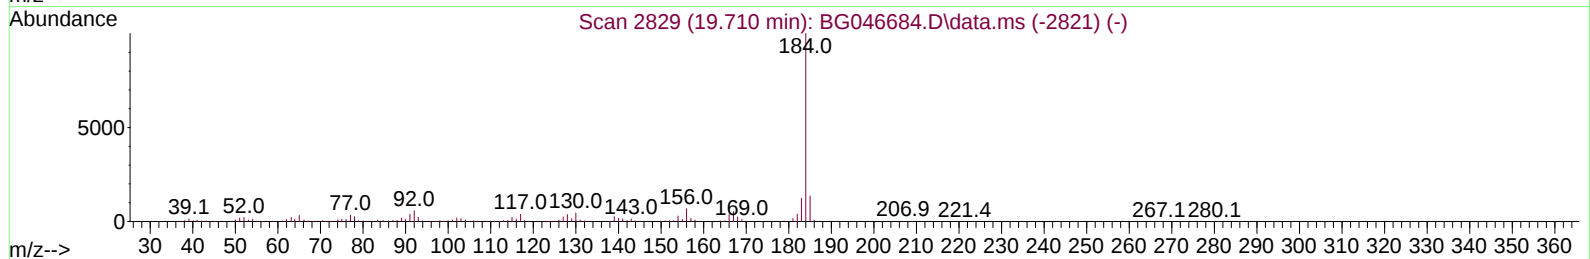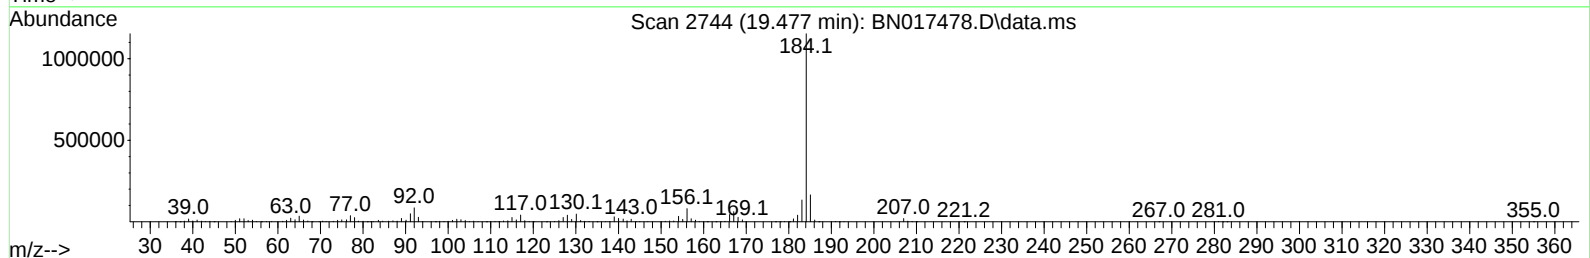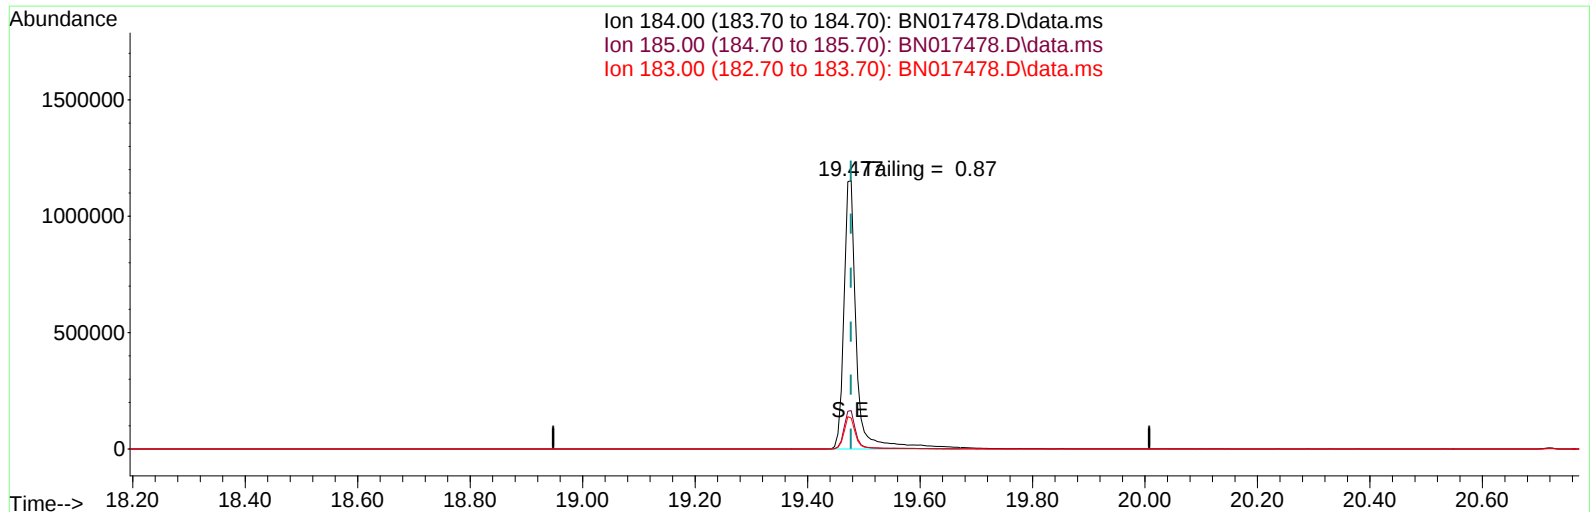

TIC: BN017478.D\data.ms

(77) Benzidine

19.477min (0.000) 0.00 ng

response 1809970

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.32
183.00	13.20	11.57
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_N
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
11/16/2021	BNA_N	<u>BN017478.D</u>
Compound Name	Response	Retention Time
DDT	1109649	20.719
DDD	24562	20.277
DDE	992	19.772
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25554	1135203	2.25