

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112822\
 Data File : BN022914.D
 Acq On : 28 Nov 2022 11:54
 Operator : CG/JU
 Sample : PB149073BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Nov 29 01:10:52 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 28 03:16:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.065	152	7243	0.400	ng/ul	0.00
4) Naphthalene-d8	10.887	136	21007	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.705	164	11844	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.453	188	25092	0.400	ng/ul	0.00
17) Chrysene-d12	21.636	240	15841	0.400	ng/ul	0.00
23) Perylene-d12	24.127	264	13360	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.408	96	56486	6.499	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.470	152	10517	0.329	ng/ul	0.00
18) Fluoranthene-d10	19.476	212	21556	0.368	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.700	166	3995	0.076	ng/ul#	12
20) Pyrene	19.843	202	3436	0.043	ng/ul#	1
26) Benzo(a)pyrene	23.966	252	6244	0.121	ng/ul#	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112822\
Data File : BN022914.D
Acq On : 28 Nov 2022 11:54
Operator : CG/JU
Sample : PB149073BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Nov 29 01:10:52 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 28 03:16:56 2022
Response via : Initial Calibration




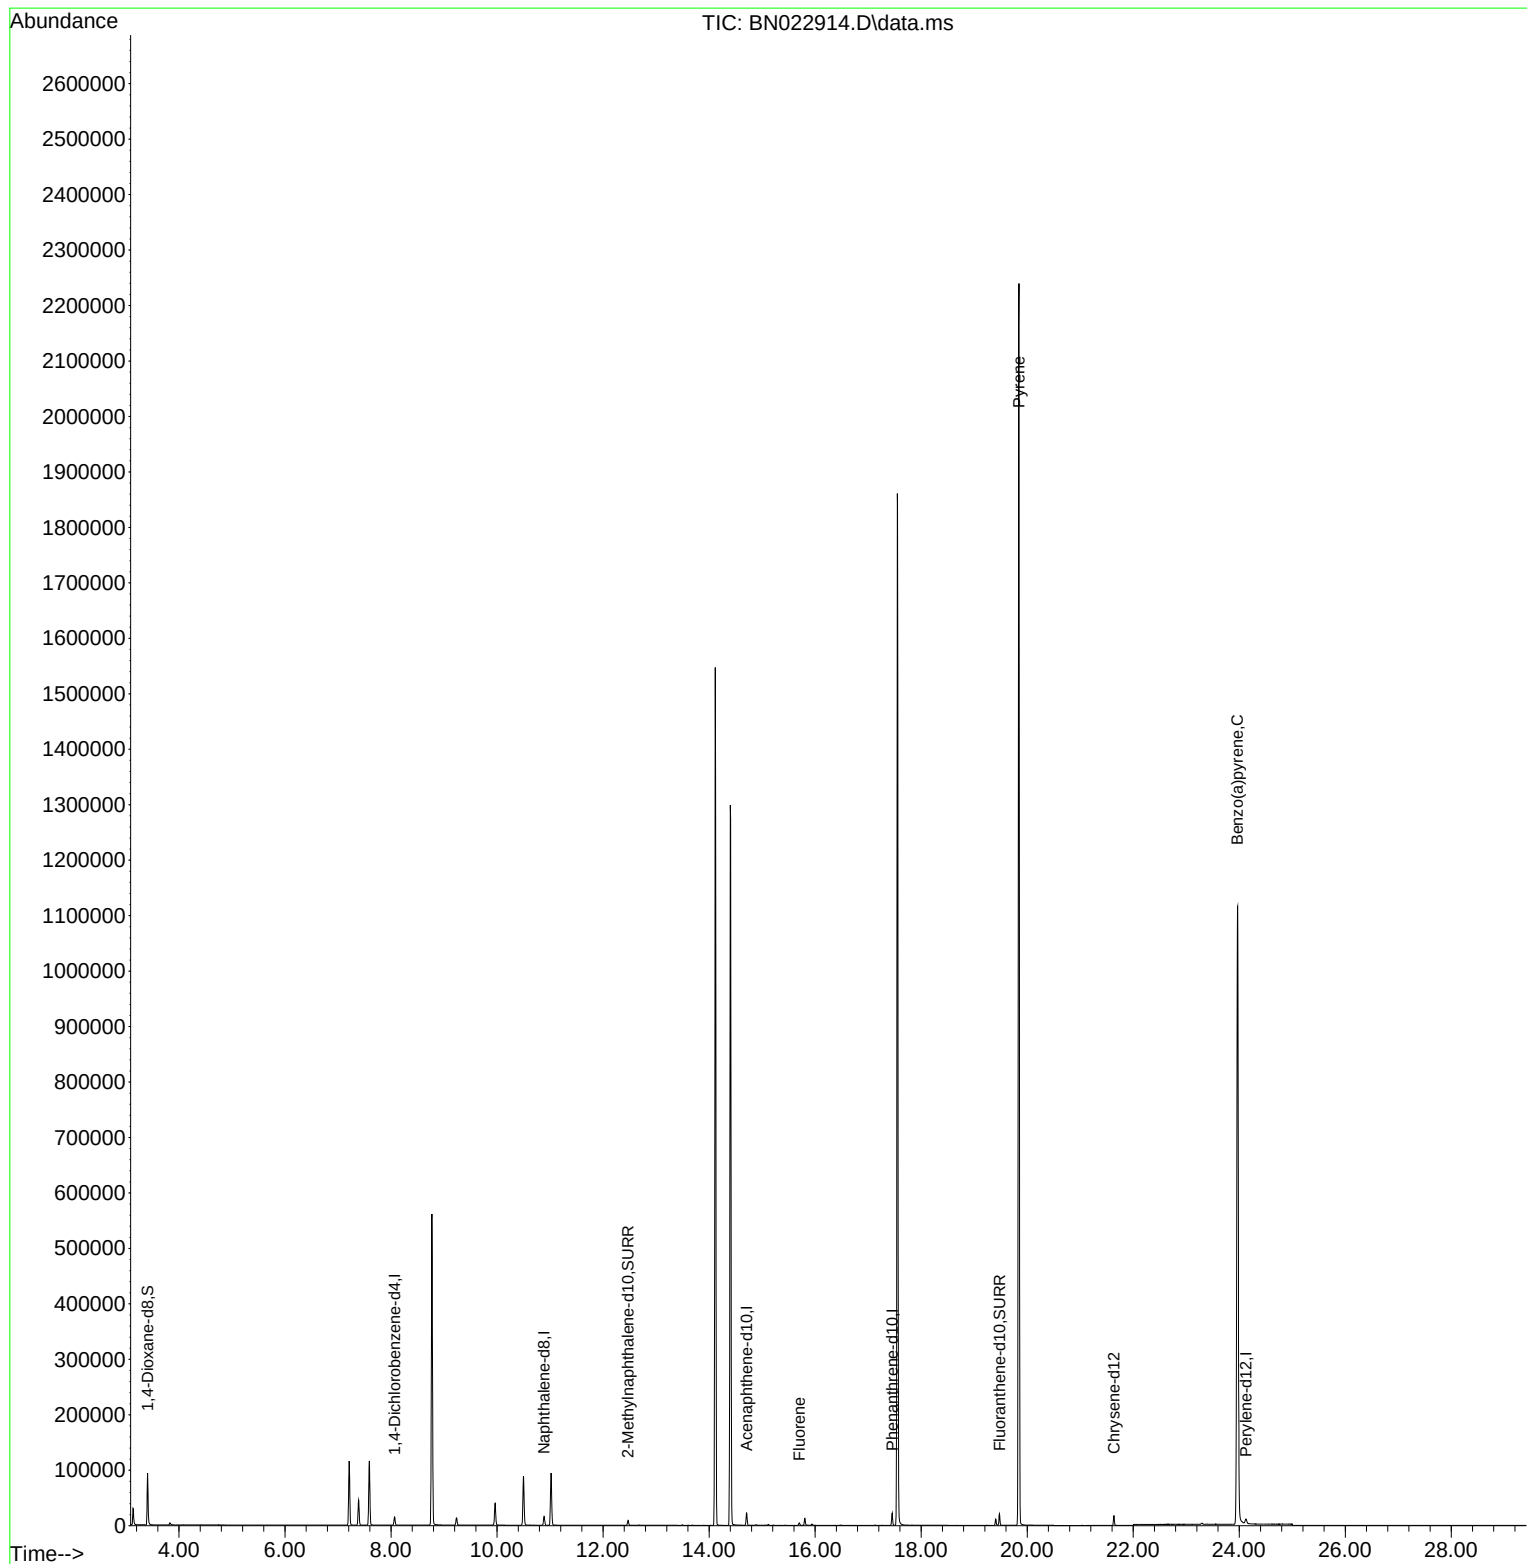


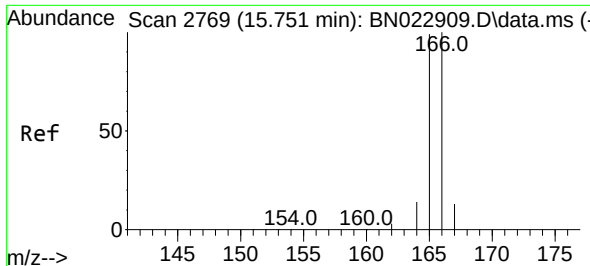

#12
Fluorene
Concen: 0.076 ng/ul
RT: 15.700 min Scan# 21
Delta R.T. -0.056 min
Lab File: BN022914.D
Acq: 28 Nov 2022 11:54




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:166 Resp: 3995
Ion Ratio Lower Upper
166 100
165 6.7 78.7 118.1#
167 34.1 10.8 16.2#

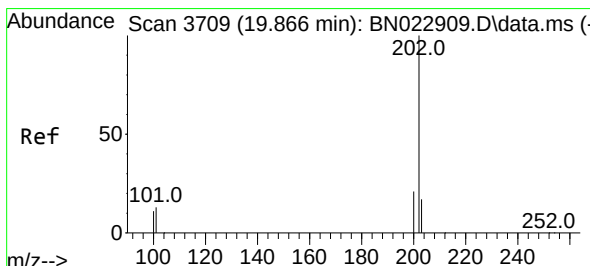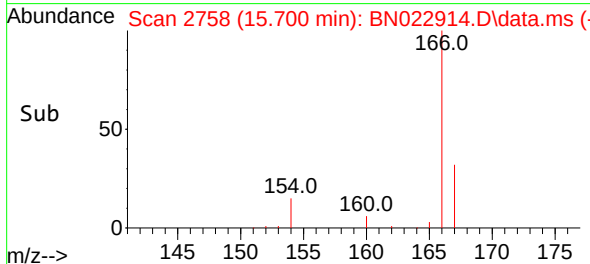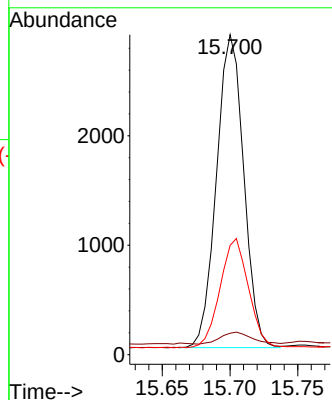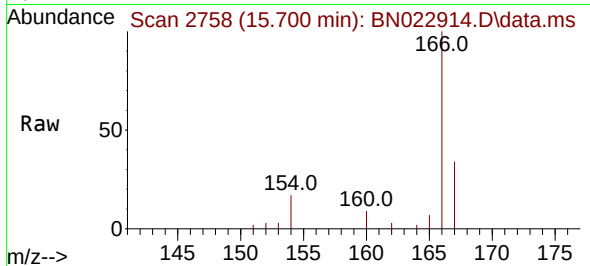

#20
Pyrene
Concen: 0.043 ng/ul
RT: 19.843 min Scan# 3704
Delta R.T. -0.028 min
Lab File: BN022914.D
Acq: 28 Nov 2022 11:54

Tgt Ion:202 Resp: 3436
Ion Ratio Lower Upper
202 100
101 154.8 10.6 16.0#
100 1134.3 8.2 12.4#

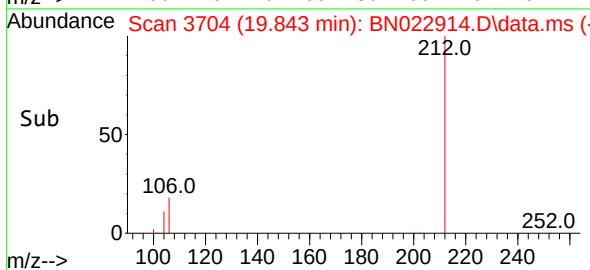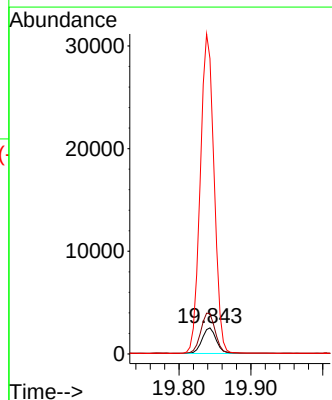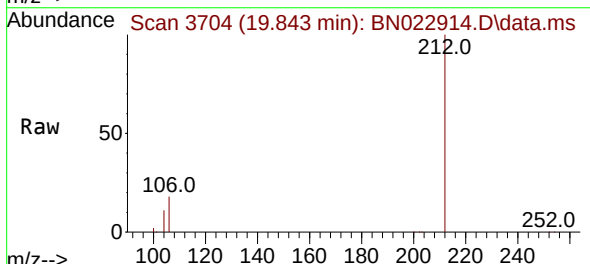

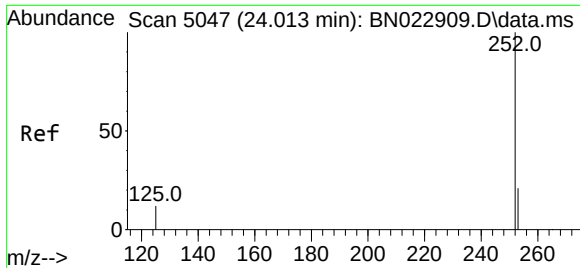

#26

Benzo(a)pyrene

Concen: 0.121 ng/ul

RT: 23.966 min Scan# 50

Delta R.T. -0.047 min


Lab File: BN022914.D

Acq: 28 Nov 2022 11:54

Instrument :

BNA_N

ClientSampleId :

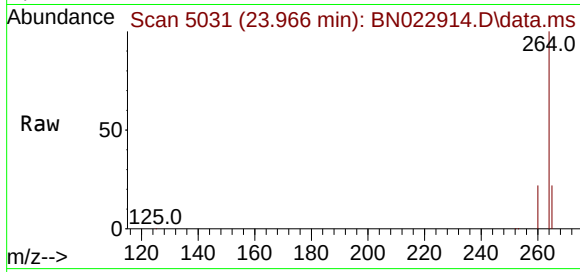

Tgt Ion:252 Resp: 6244

Ion Ratio Lower Upper

252 100

253 35.6 19.7 29.5#

125 32.2 13.7 20.5#

