

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112822\
 Data File : BN022920.D
 Acq On : 28 Nov 2022 15:36
 Operator : CG/JU
 Sample : N5591-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C9827

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 11/29/2022
 Supervised By :mohammad ahmed 11/30/2022

Quant Time: Nov 29 01:12:05 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 28 03:16:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.065	152	7903	0.400	ng/ul	0.00
4) Naphthalene-d8	10.887	136	23864	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.705	164	13483	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.453	188	28734	0.400	ng/ul	0.00
17) Chrysene-d12	21.635	240	17146	0.400	ng/ul	0.00
23) Perylene-d12	24.123	264	12983	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.408	96	40865	4.309	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.470	152	9747	0.268	ng/ul	0.00
18) Fluoranthene-d10	19.476	212	21167	0.334	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.936	128	2710	0.037	ng/ul#	91
7) 2-Methylnaphthalene	12.542	142	1682	0.037	ng/ul	98
8) 1-Methylnaphthalene	12.762	142	1160	0.025	ng/ul	99
15) Phenanthrene	17.491	178	9048	0.092	ng/ul	98
19) Fluoranthene	19.504	202	12430	0.140	ng/ul	96
20) Pyrene	19.866	202	8528m	0.098	ng/ul	
21) Benzo(a)anthracene	21.617	228	1671	0.025	ng/ul#	87
22) Chrysene	21.673	228	3718	0.052	ng/ul#	94
24) Benzo(b)fluoranthene	23.362	252	4115m	0.063	ng/ul	
27) Indeno(1,2,3-cd)pyrene	26.729	276	1268	0.021	ng/ul#	100
29) Benzo(g,h,i)perylene	27.534	276	1115	0.021	ng/ul#	56

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112822\
Data File : BN022920.D
Acq On : 28 Nov 2022 15:36
Operator : CG/JU
Sample : N5591-15
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C9827

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022


Quant Time: Nov 29 01:12:05 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 28 03:16:56 2022
Response via : Initial Calibration

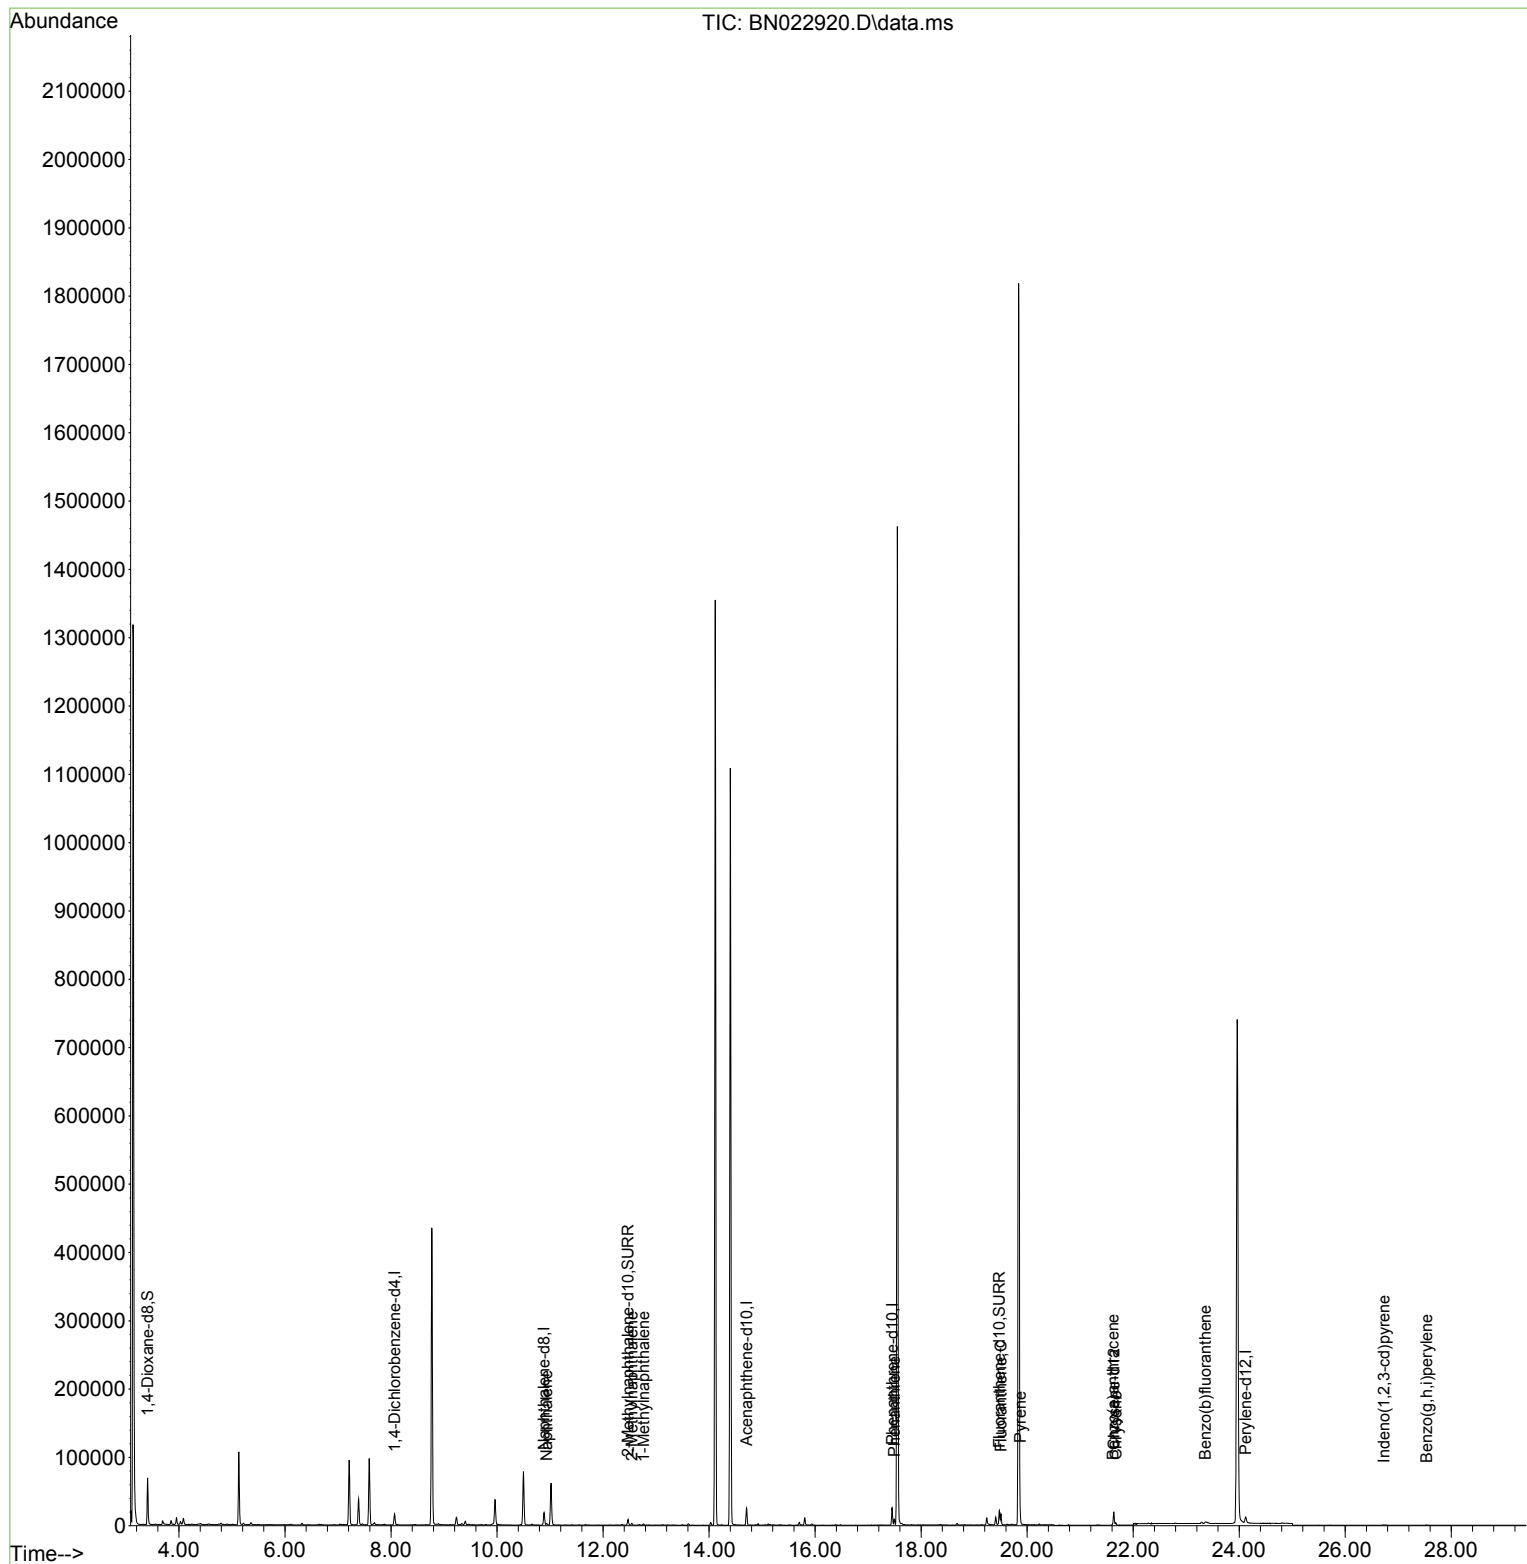

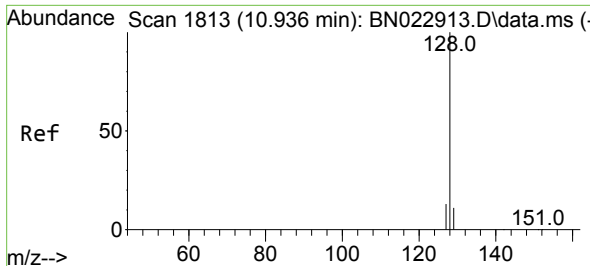

#5
Naphthalene
Concen: 0.037 ng/ul
RT: 10.936 min Scan# 1813
Delta R.T. -0.006 min
Lab File: BN022920.D
Acq: 28 Nov 2022 15:36




Instrument :
BNA_N
ClientSampleId :
C9827

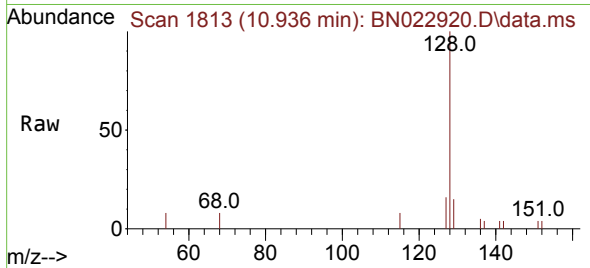

Tgt Ion:128 Resp: 2710
Ion Ratio Lower Upper
128 100
129 15.4 9.0 13.6
127 16.1 10.6 16.0




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022

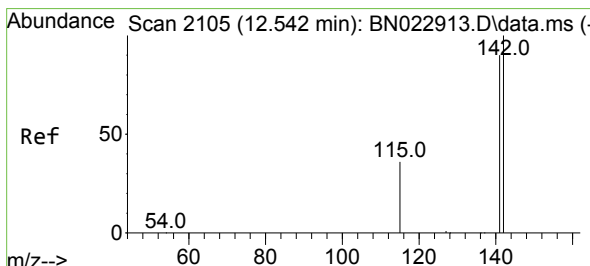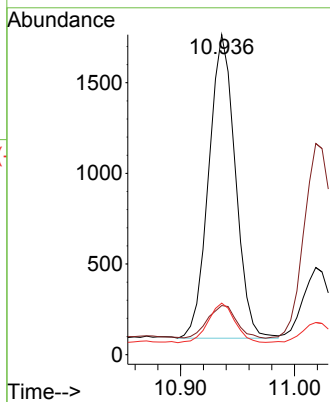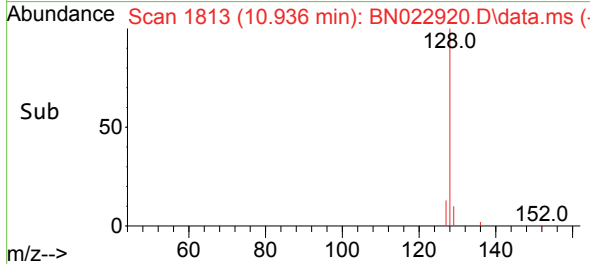

#7
2-Methylnaphthalene
Concen: 0.037 ng/ul
RT: 12.542 min Scan# 2105
Delta R.T. -0.006 min
Lab File: BN022920.D
Acq: 28 Nov 2022 15:36


Tgt Ion:142 Resp: 1682
Ion Ratio Lower Upper
142 100
141 87.8 71.6 107.4

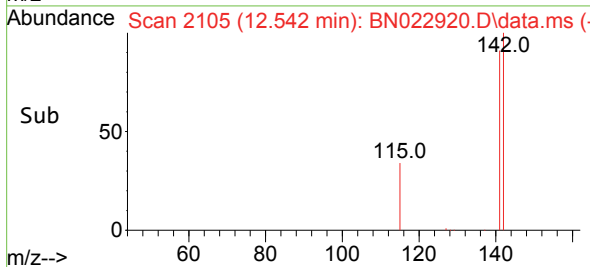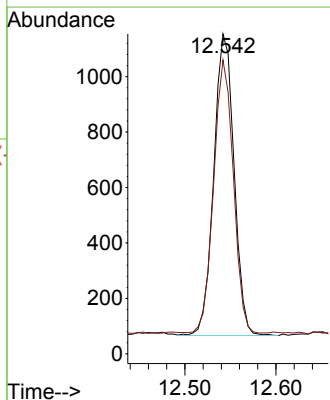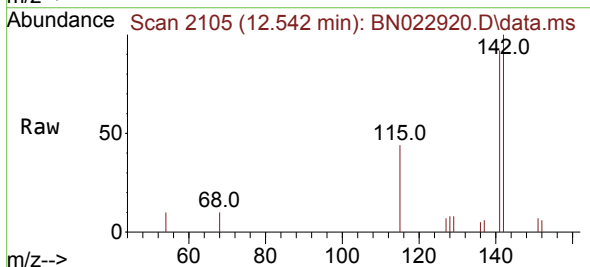

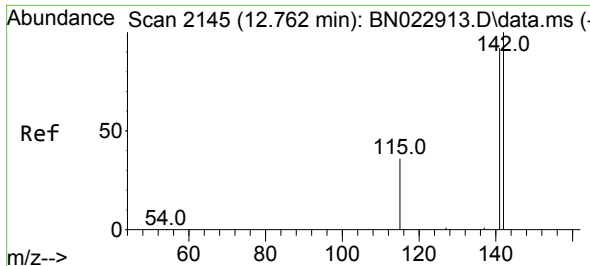

#8
1-Methylnaphthalene
Concen: 0.025 ng/ul
RT: 12.762 min Scan# 2145
Delta R.T. -0.006 min
Lab File: BN022920.D
Acq: 28 Nov 2022 15:36




Instrument :
BNA_N
ClientSampleId :
C9827

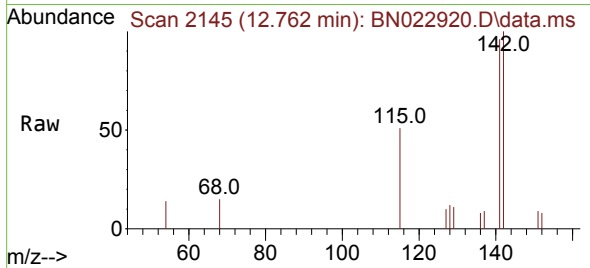


Tgt Ion:142 Resp: 1160
Ion Ratio Lower Upper
142 100
141 93.5 73.8 110.6

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022

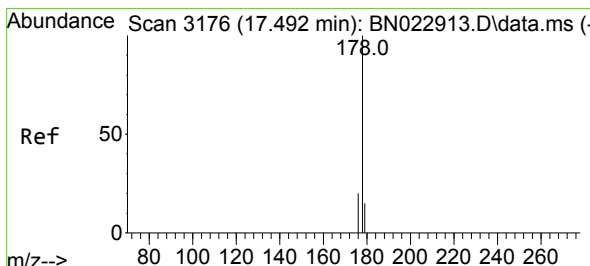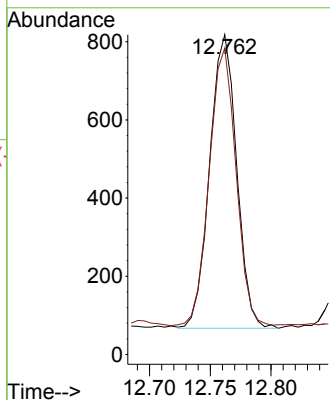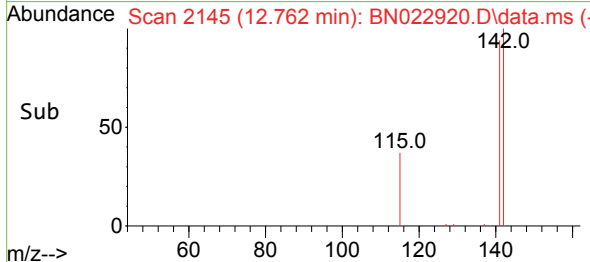


#15
Phenanthrene
Concen: 0.092 ng/ul
RT: 17.491 min Scan# 3176
Delta R.T. -0.004 min
Lab File: BN022920.D
Acq: 28 Nov 2022 15:36

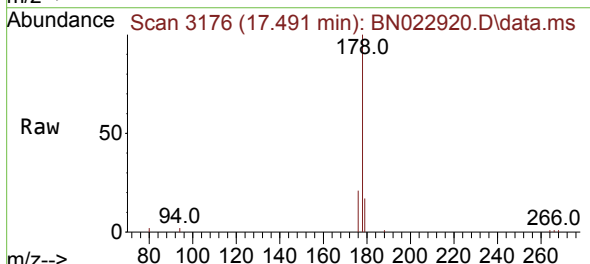

Tgt Ion:178 Resp: 9048
Ion Ratio Lower Upper
178 100
179 16.8 12.5 18.7
176 20.7 15.9 23.9

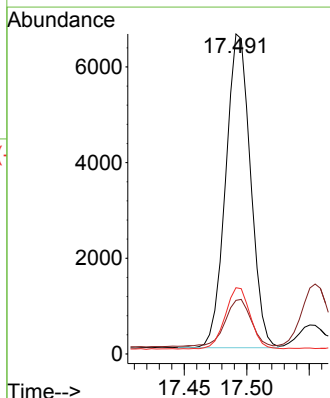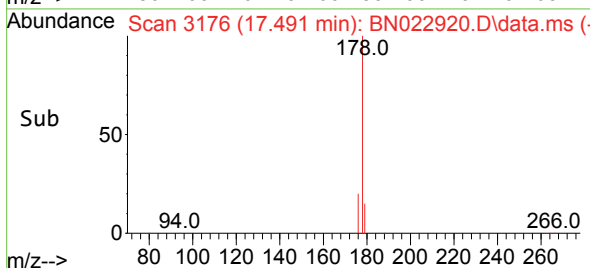

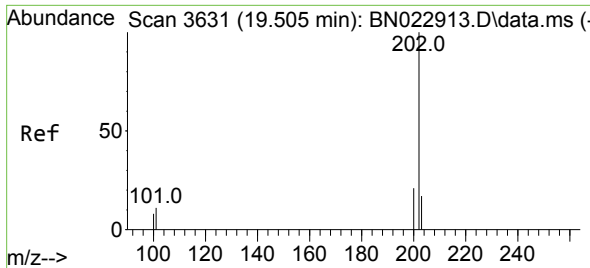

#19

Fluoranthene

Concen: 0.140 ng/ul

RT: 19.504 min Scan# 3631

Delta R.T. -0.005 min

Lab File: BN022920.D

Acq: 28 Nov 2022 15:36

Instrument :

BNA_N

ClientSampleId :





C9827

Tgt Ion:202	Resp:	12430
Ion Ratio	Lower	Upper
202	100	
101	12.9	9.2 13.8
100	10.0	6.9 10.3

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022

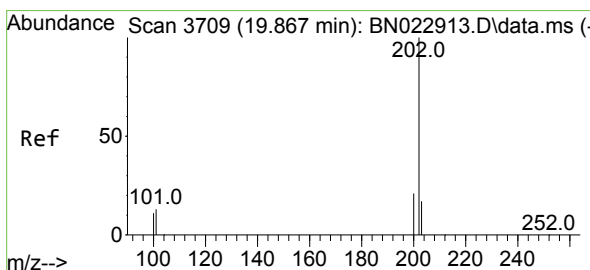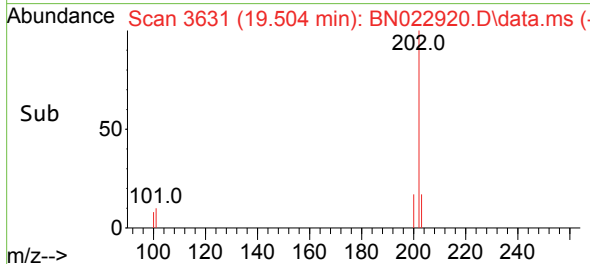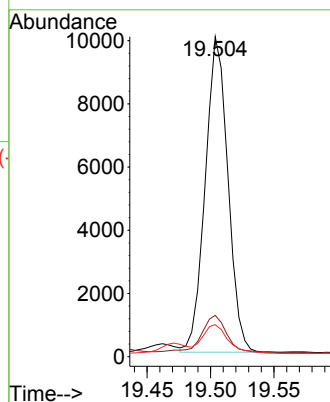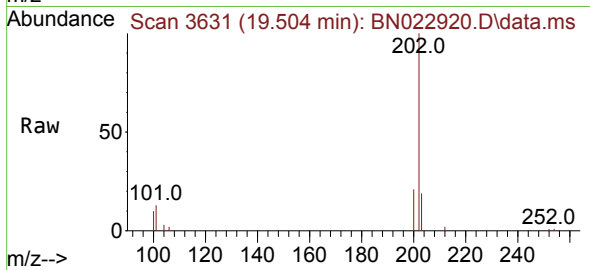

#20

Pyrene

Concen: 0.098 ng/ul m




RT: 19.866 min Scan# 3709


Delta R.T. -0.005 min

Lab File: BN022920.D

Acq: 28 Nov 2022 15:36


Tgt Ion:202	Resp:	8528
Ion Ratio	Lower	Upper
202	100	
101	16.2	10.6 16.0#
100	14.6	8.2 12.4#

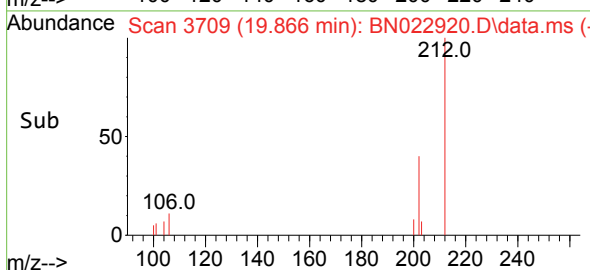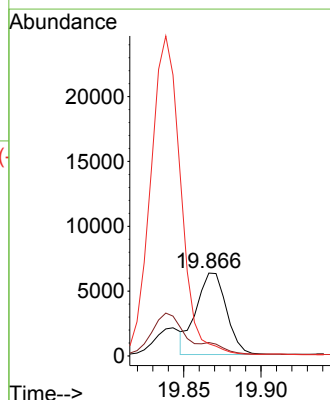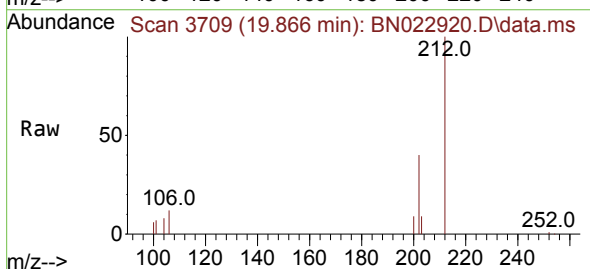

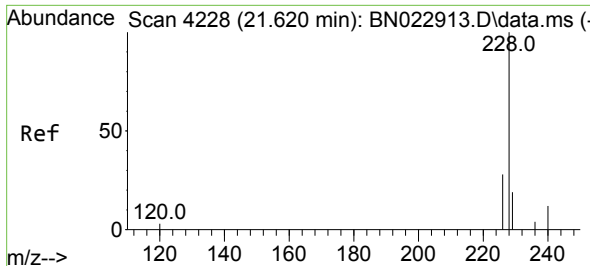

#21
Benzo(a)anthracene
Concen: 0.025 ng/u1
RT: 21.617 min Scan# 4227
Delta R.T. -0.001 min
Lab File: BN022920.D
Acq: 28 Nov 2022 15:36




Instrument :
BNA_N
ClientSampleId :
C9827

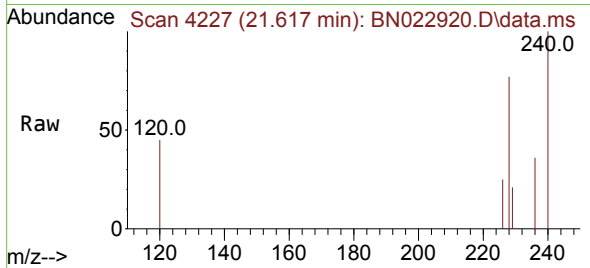

Tgt Ion:228 Resp: 167
Ion Ratio Lower Upper
228 100
229 27.0 15.5 23.3
226 33.0 22.2 33.4




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022

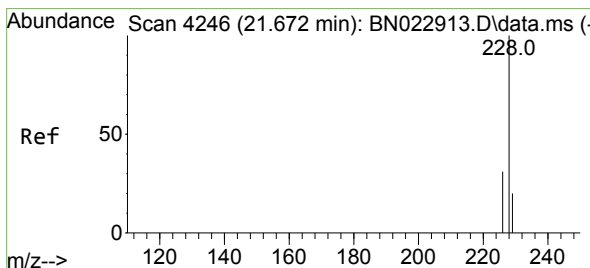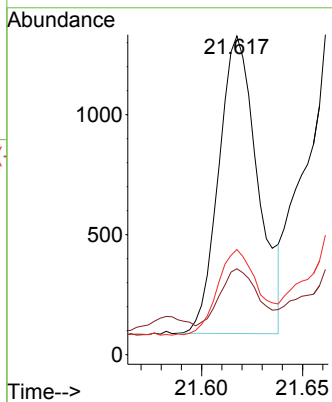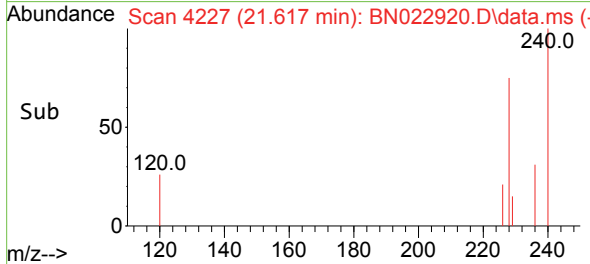

#22
Chrysene
Concen: 0.052 ng/u1
RT: 21.673 min Scan# 4246
Delta R.T. -0.001 min
Lab File: BN022920.D
Acq: 28 Nov 2022 15:36


Tgt Ion:228 Resp: 3718
Ion Ratio Lower Upper
228 100
226 32.4 24.6 37.0
229 24.4 15.8 23.8

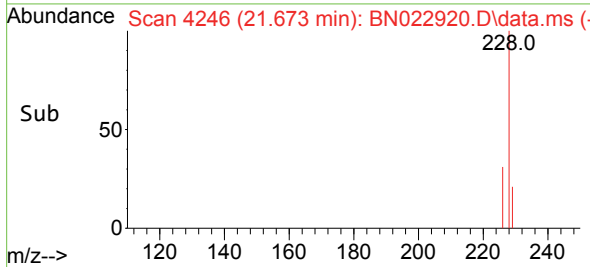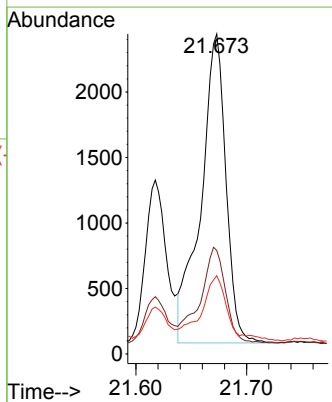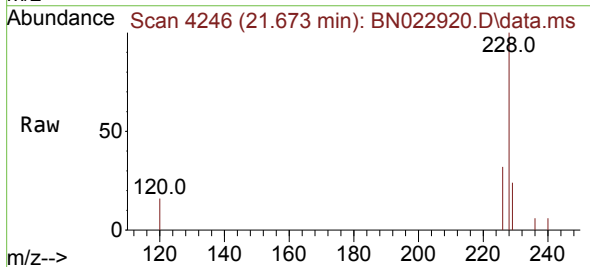

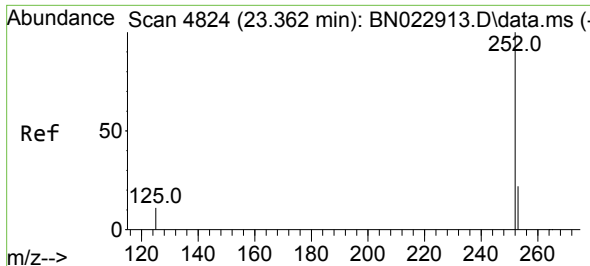

#24
Benzo(b)fluoranthene
Concen: 0.063 ng/ul m
RT: 23.362 min Scan# 4824
Delta R.T. -0.001 min
Lab File: BN022920.D
Acq: 28 Nov 2022 15:36




Instrument :
BNA_N
ClientSampleId :
C9827

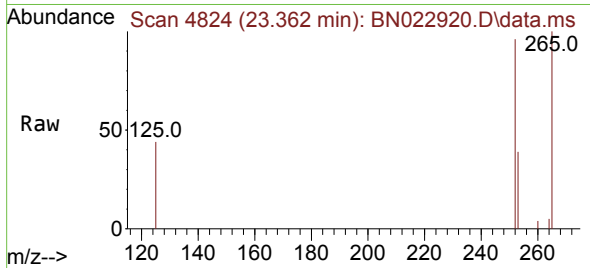


Tgt Ion:252 Resp: 411
Ion Ratio Lower Upper
252 100
253 40.6 0.0 46.0
125 45.3 0.0 28.6

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022

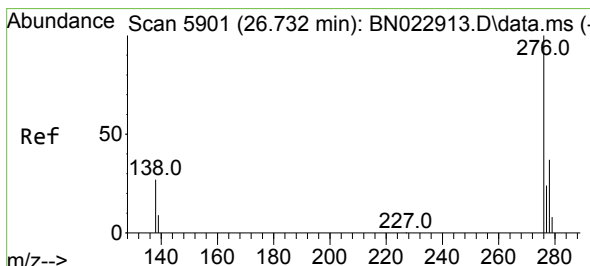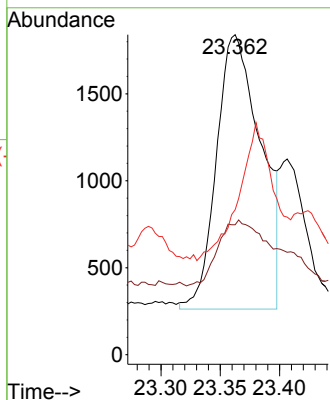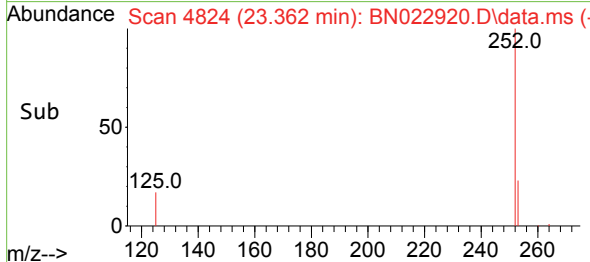


#27
Indeno(1,2,3-cd)pyrene
Concen: 0.021 ng/ul
RT: 26.729 min Scan# 5900
Delta R.T. -0.012 min
Lab File: BN022920.D
Acq: 28 Nov 2022 15:36

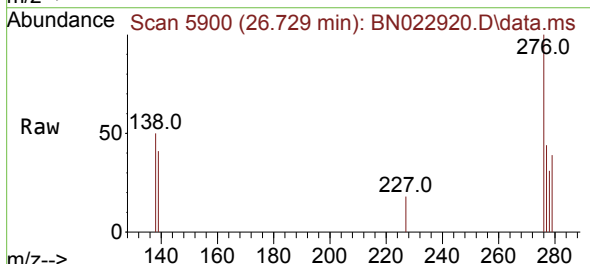


Tgt Ion:276 Resp: 1268
Ion Ratio Lower Upper
276 100
138 0.0 0.0 0.0
227 0.2 0.0 0.0#

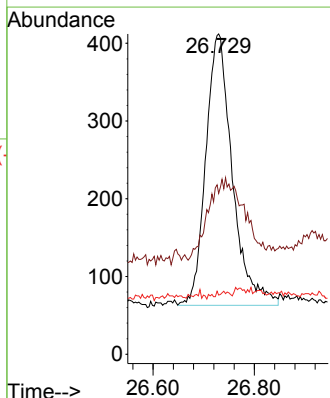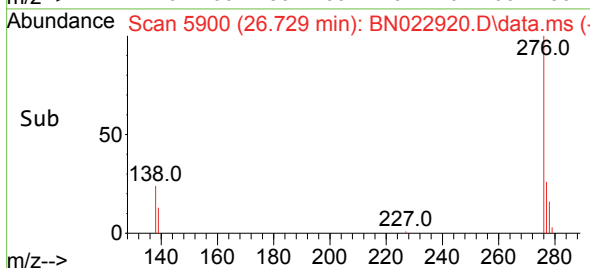

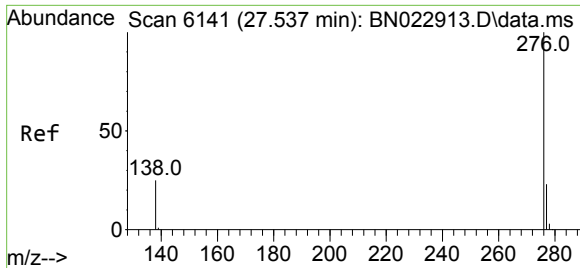

#29
Benzo(g,h,i)perylene
Concen: 0.021 ng/ul
RT: 27.534 min Scan# 6140
Delta R.T. -0.005 min
Lab File: BN022920.D
Acq: 28 Nov 2022 15:36

Instrument :
BNA_N
ClientSampleId :
C9827

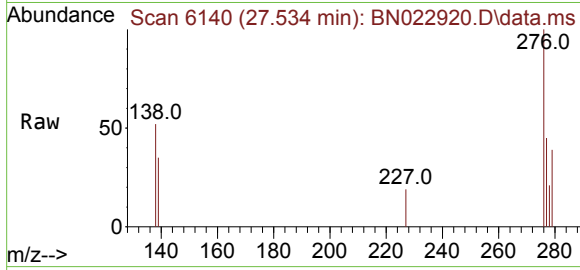

Tgt Ion:276 Resp: 111
Ion Ratio Lower Upper
276 100
138 51.8 22.1 33.1
277 45.0 19.4 29.2

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022

