
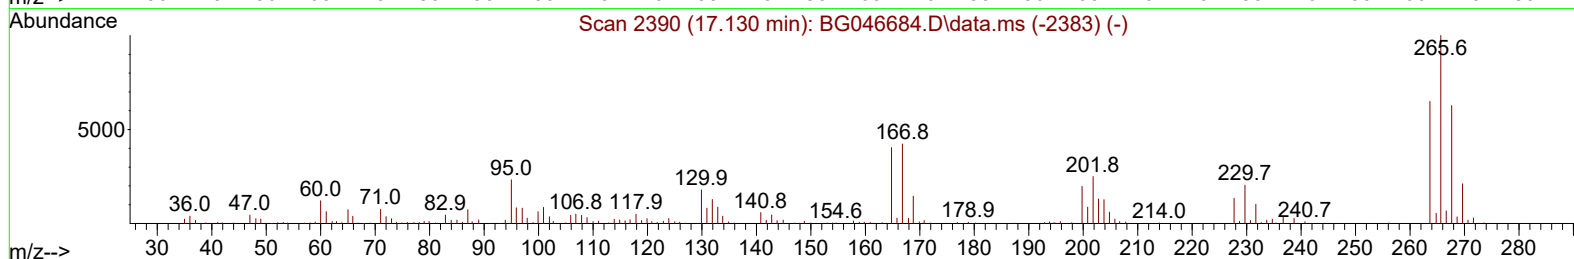
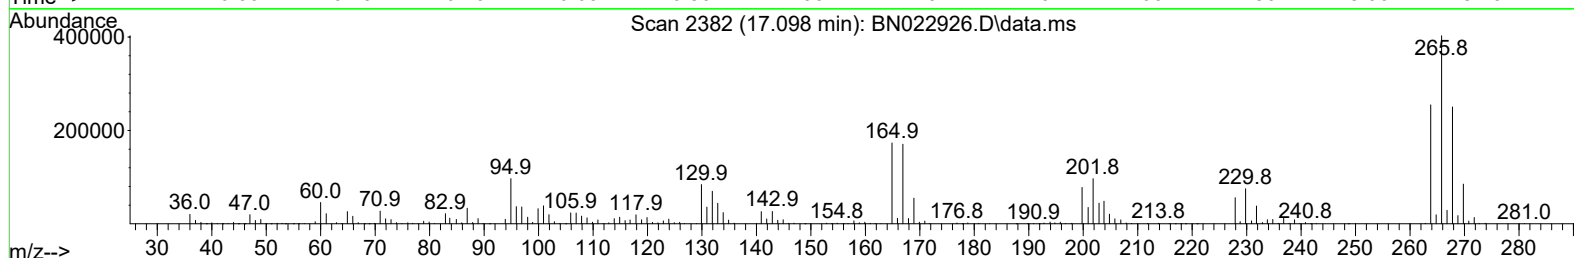


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112922\
Data File : BN022926.D
Acq On : 28 Nov 2022 21:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 29 07:30:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 07:30:31 2022
Response via : Initial Calibration

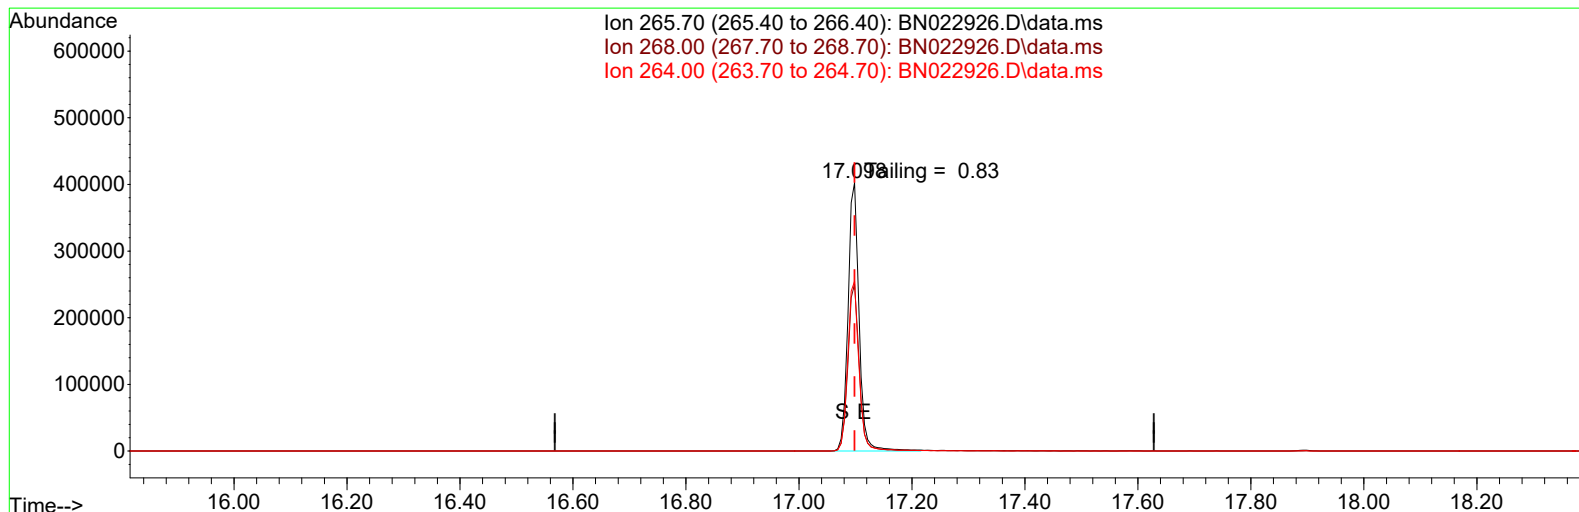

TIC: BN022926.D\data.ms

(70) Pentachlorophenol (C)




17.098min (0.000) 20243.05 ng

response **549346**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.17
264.00	61.60	63.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112922\
Data File : BN022926.D
Acq On : 28 Nov 2022 21:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 29 07:30:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 07:30:31 2022
Response via : Initial Calibration

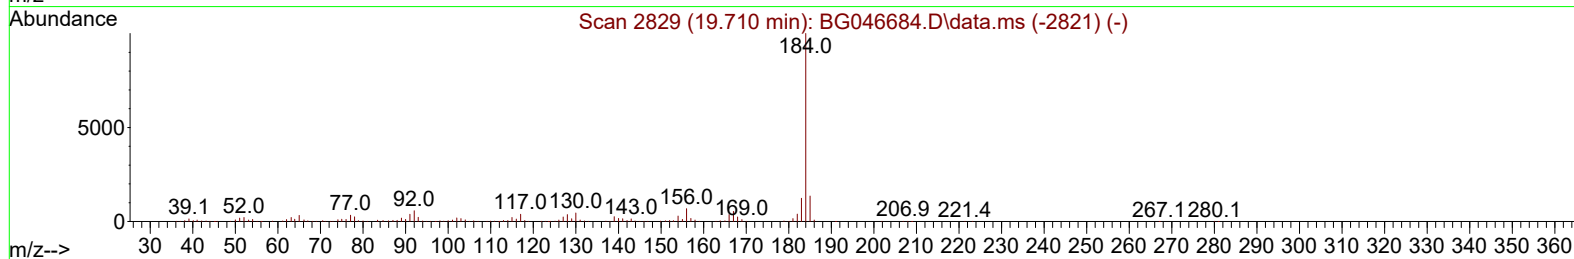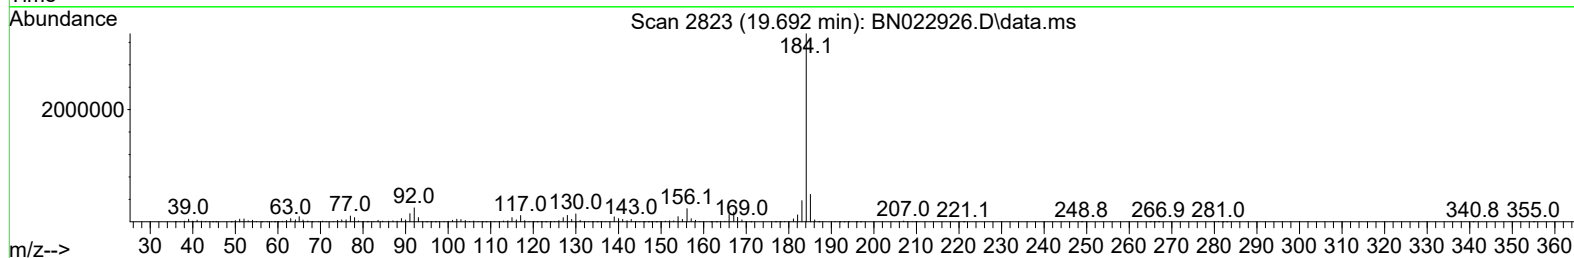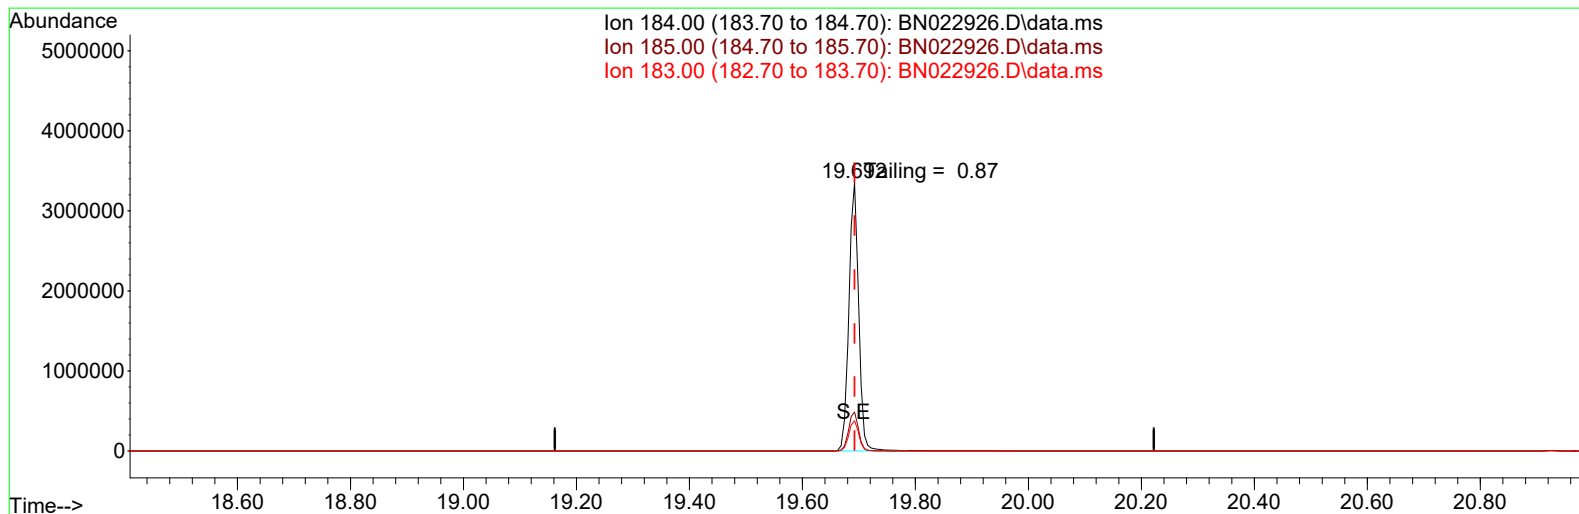

TIC: BN022926.D\data.ms

(77) Benzidine

19.692min (0.000) 0.00 ng

response 4065797

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.55
183.00	13.20	11.26
0.00	0.00	0.00