
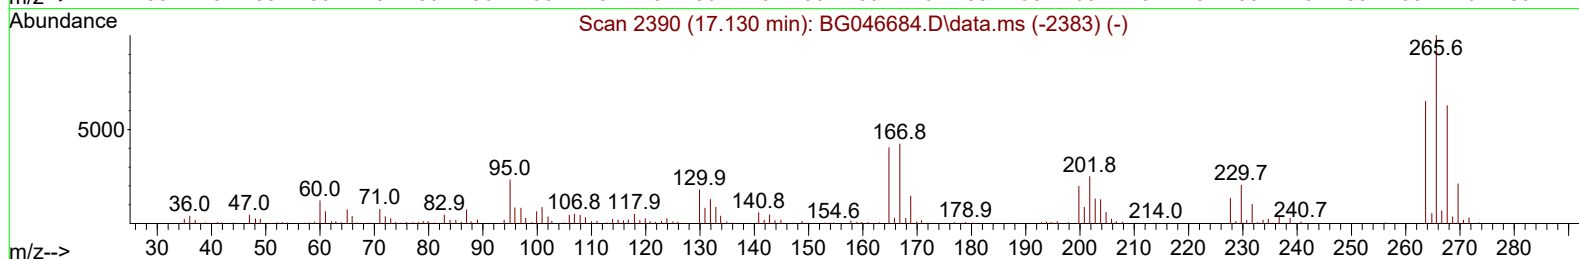
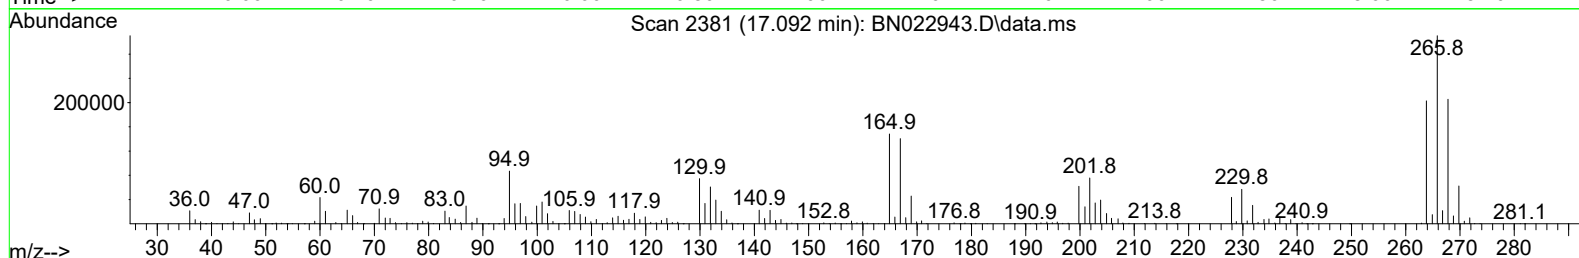


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112922\
Data File : BN022943.D
Acq On : 29 Nov 2022 08:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 30 05:40:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 30 05:40:21 2022
Response via : Initial Calibration

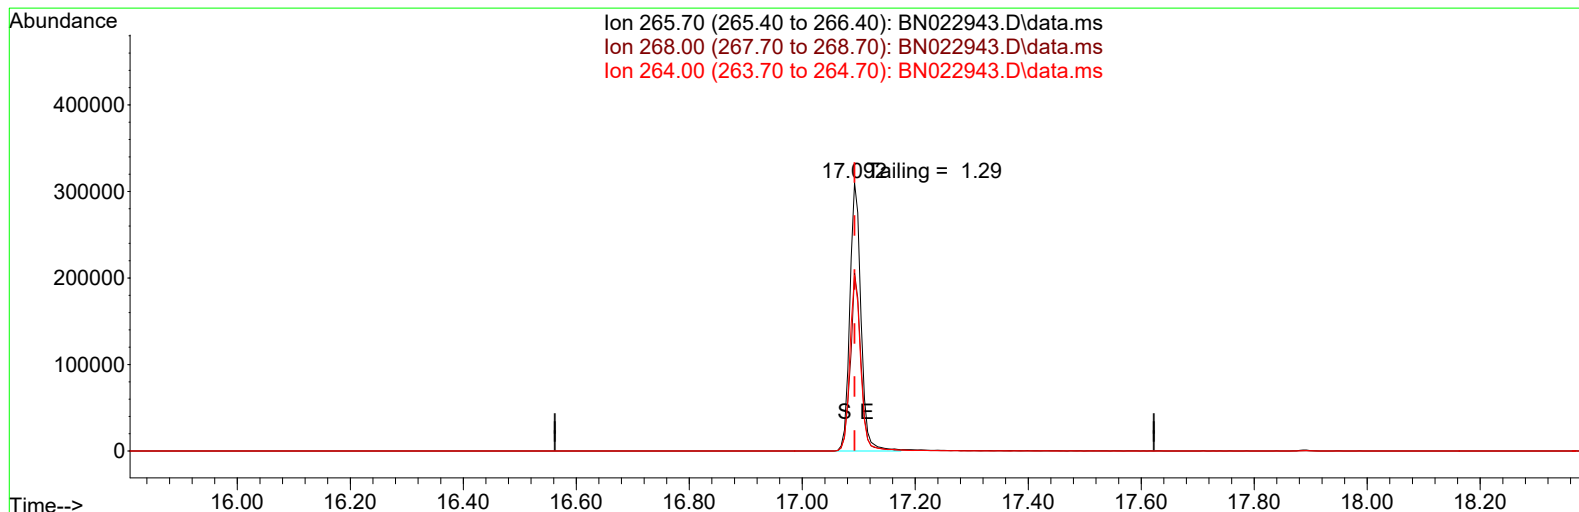

TIC: BN022943.D\data.ms

(70) Pentachlorophenol (C)




17.092min (0.000) 16449.87 ng

response 430530

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.23
264.00	61.60	65.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112922\
Data File : BN022943.D
Acq On : 29 Nov 2022 08:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 30 05:40:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 30 05:40:21 2022
Response via : Initial Calibration

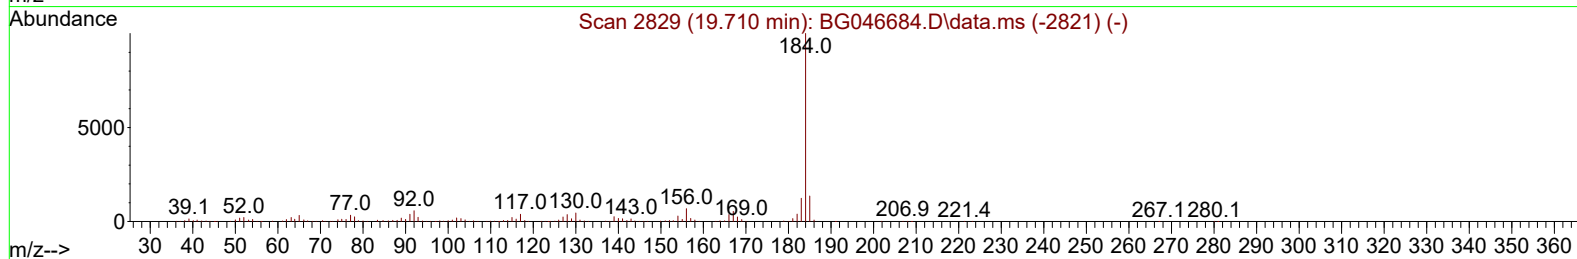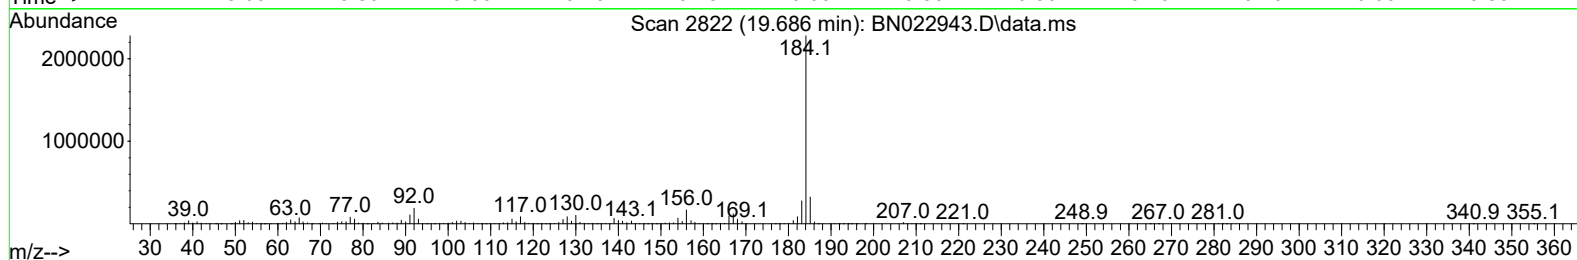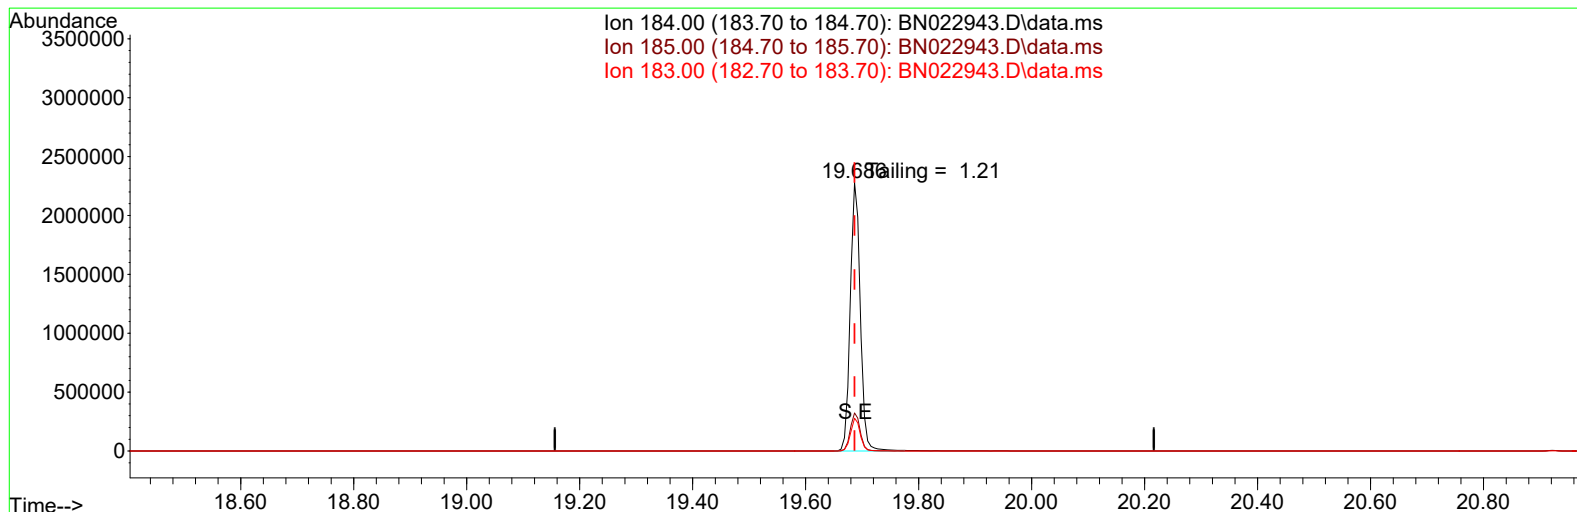

TIC: BN022943.D\data.ms

(77) Benzidine

19.686min (0.000) 0.00 ng

response 2830903

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.20
183.00	13.20	12.22
0.00	0.00	0.00