
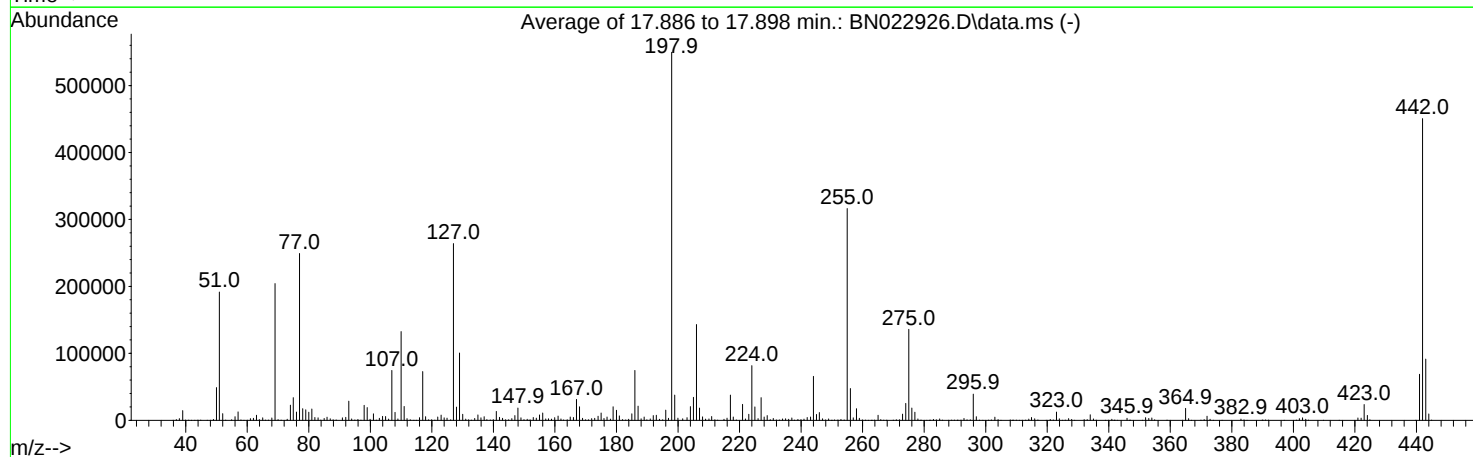


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112922\
 Data File : BN022926.D
 Acq On : 28 Nov 2022 21:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 29 05:14:21 2022

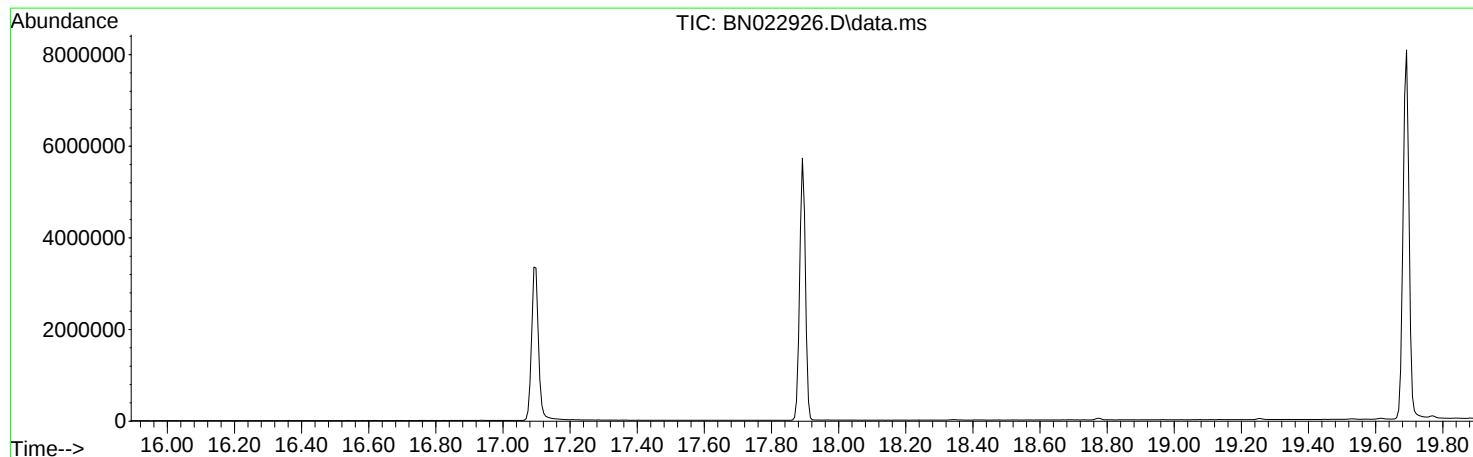




AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	191582	PASS
68	69	0.00	2	1.7	3568	PASS
69	198	0.00	100	37.2	204373	PASS
70	69	0.00	2	0.6	1187	PASS
127	198	10	80	48.1	264043	PASS
197	198	0.00	2	0.6	3041	PASS
198	198	100	100	100.0	549504	PASS
199	198	5	9	6.9	37731	PASS
275	198	10	60	24.7	135784	PASS
365	198	1	100	3.3	17951	PASS
441	198	0.01	100	12.5	68621	PASS
442	442	50	100	100.0	450560	PASS
443	442	15	24	20.3	91424	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112922\  
Data File : BN022926.D  
Acq On    : 28 Nov 2022   21:12  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 29 07:30:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 07:30:31 2022
Response via : Initial Calibration

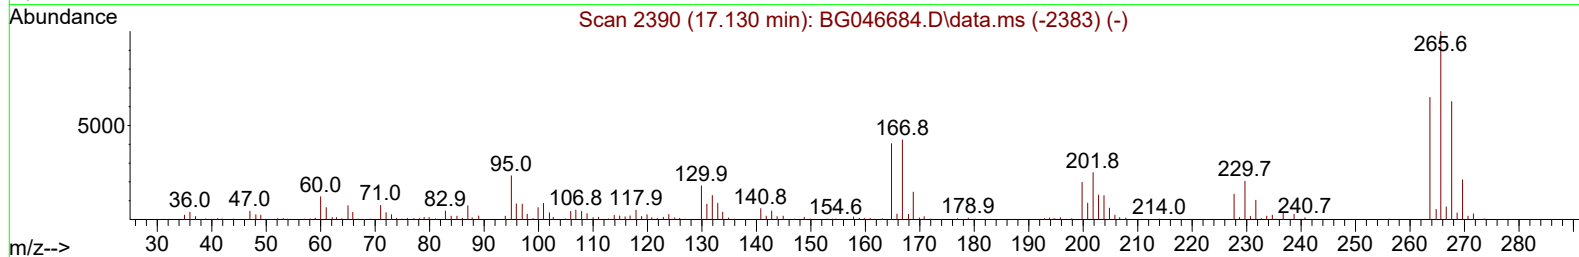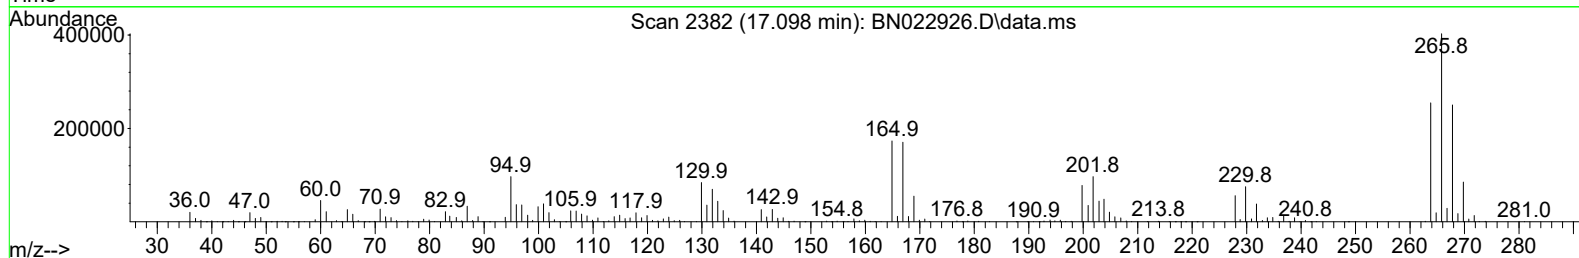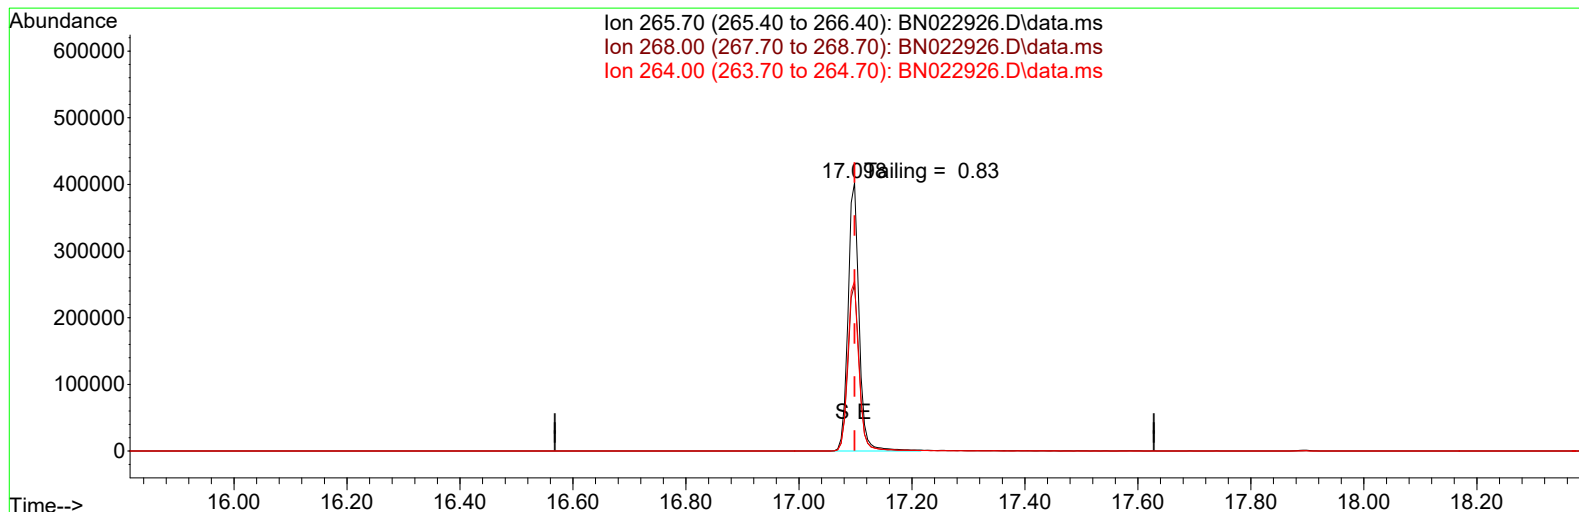

TIC: BN022926.D\data.ms

(70) Pentachlorophenol (C)

17.098min (0.000) 20243.05 ng




response **549346**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.17
264.00	61.60	63.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112922\
Data File : BN022926.D
Acq On : 28 Nov 2022 21:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 29 07:30:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 07:30:31 2022
Response via : Initial Calibration

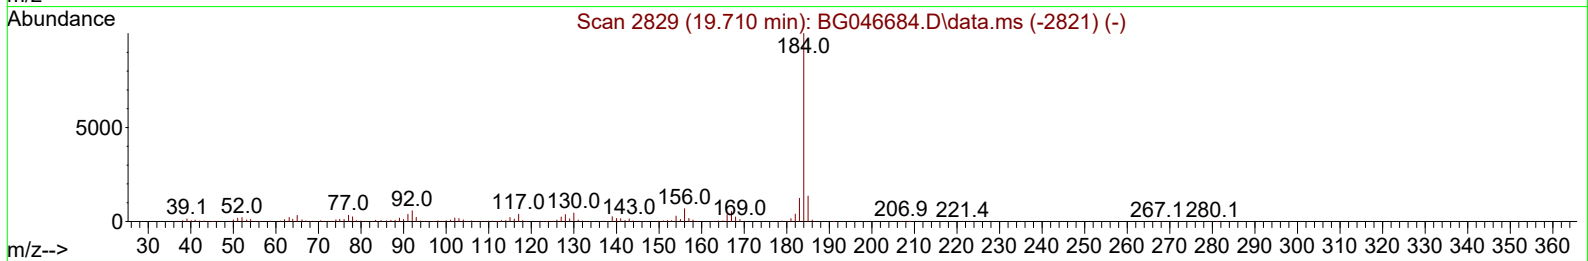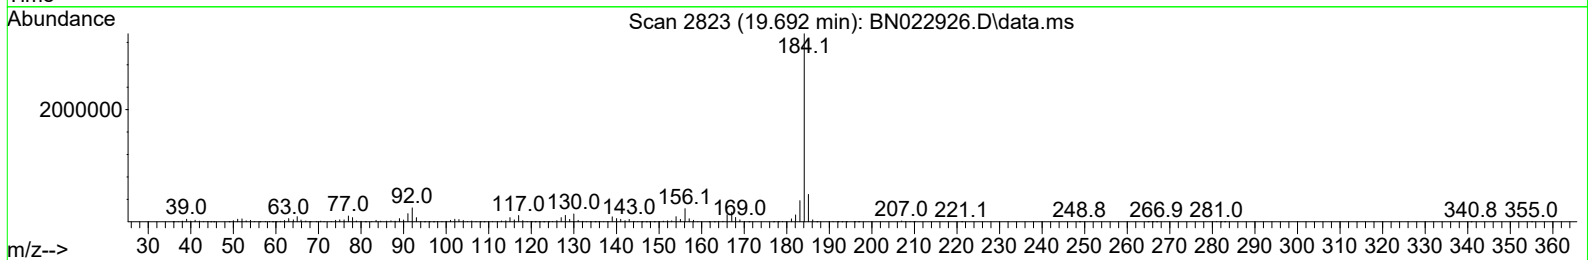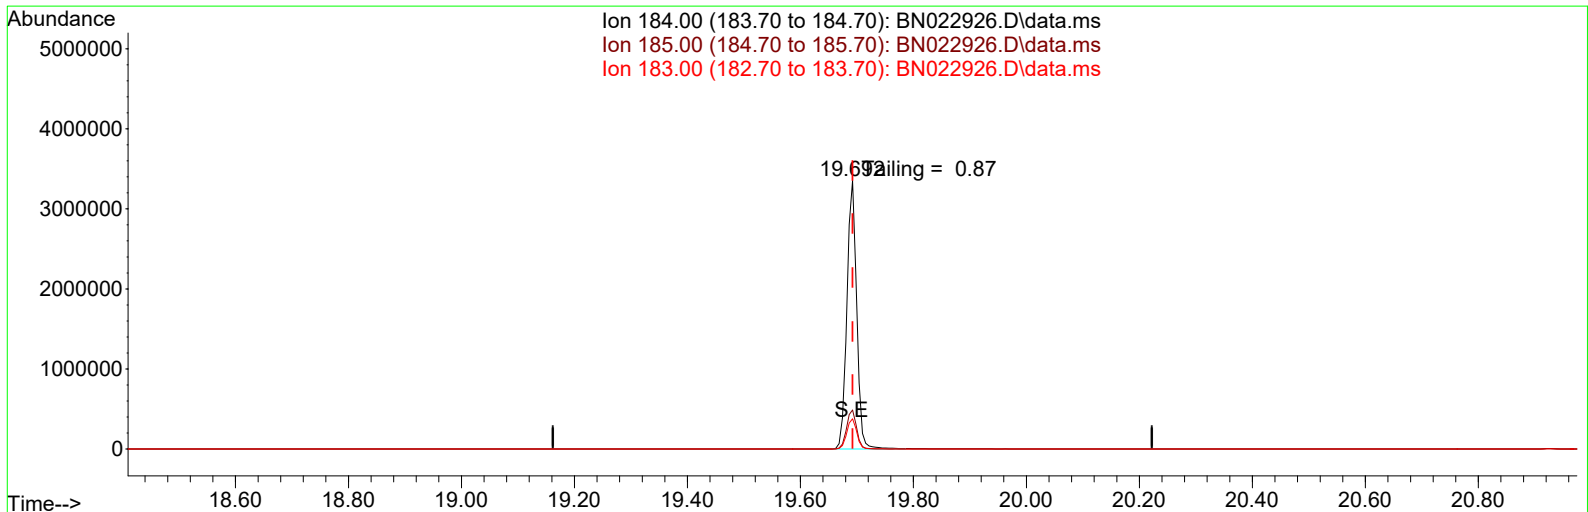

TIC: BN022926.D\data.ms

(77) Benzidine

19.692min (0.000) 0.00 ng

response 4065797

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.55
183.00	13.20	11.26
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/29/2022	BNA_N	<u>BN022926.D</u>
Compound Name	Response	Retention Time
DDT	1780818	20.927
DDD	35779	20.486
DDE	1019	19.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
36798	1817616	2.02

Instrument :
BNA_N
ClientSampleId :
DFTPP