
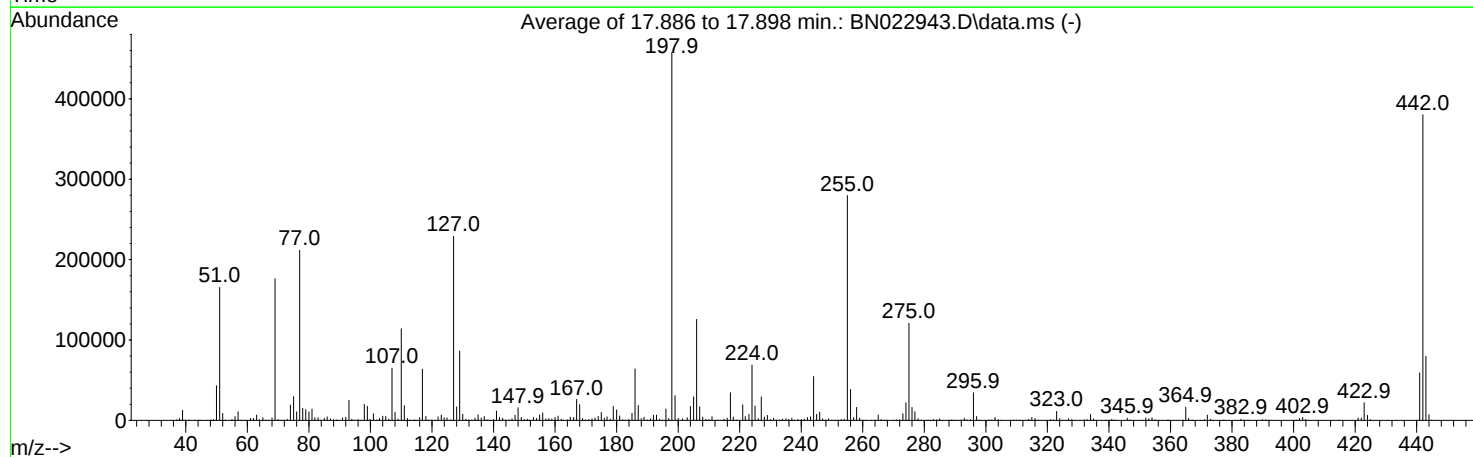


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112922\
 Data File : BN022943.D
 Acq On : 29 Nov 2022 08:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 30 00:45:21 2022

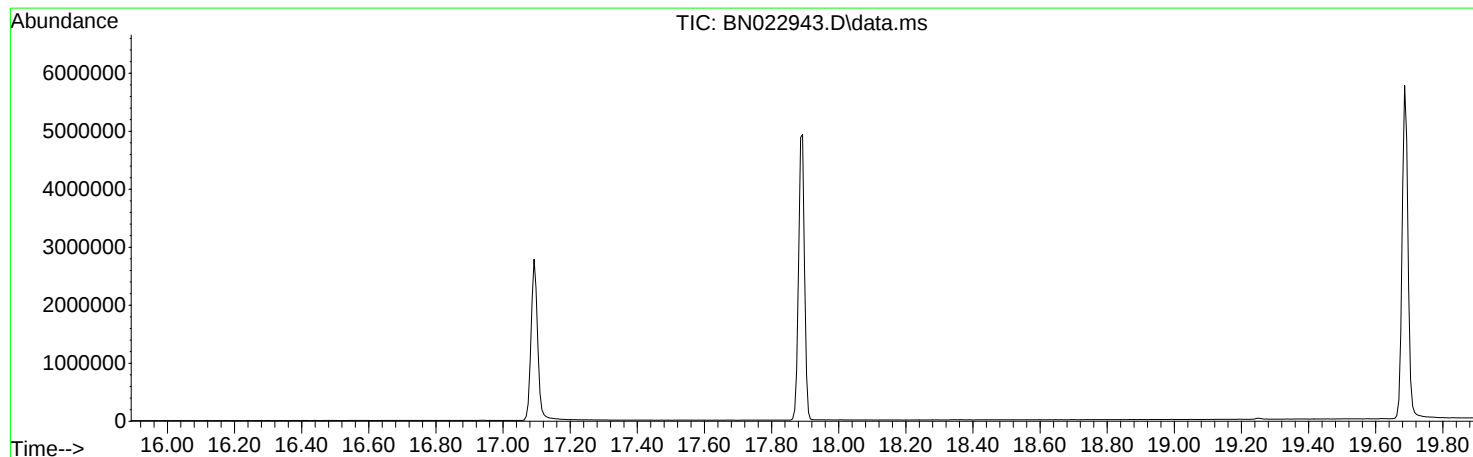




AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	165424	PASS
68	69	0.00	2	1.7	2963	PASS
69	198	0.00	100	38.5	176120	PASS
70	69	0.00	2	0.5	932	PASS
127	198	10	80	50.0	228920	PASS
197	198	0.00	2	0.5	2384	PASS
198	198	100	100	100.0	457643	PASS
199	198	5	9	6.7	30787	PASS
275	198	10	60	26.4	120885	PASS
365	198	1	100	3.6	16250	PASS
441	198	0.01	100	12.9	59216	PASS
442	442	50	100	100.0	380288	PASS
443	442	15	24	21.0	79827	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112922\
Data File : BN022943.D
Acq On : 29 Nov 2022 08:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 30 05:40:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 30 05:40:21 2022
Response via : Initial Calibration

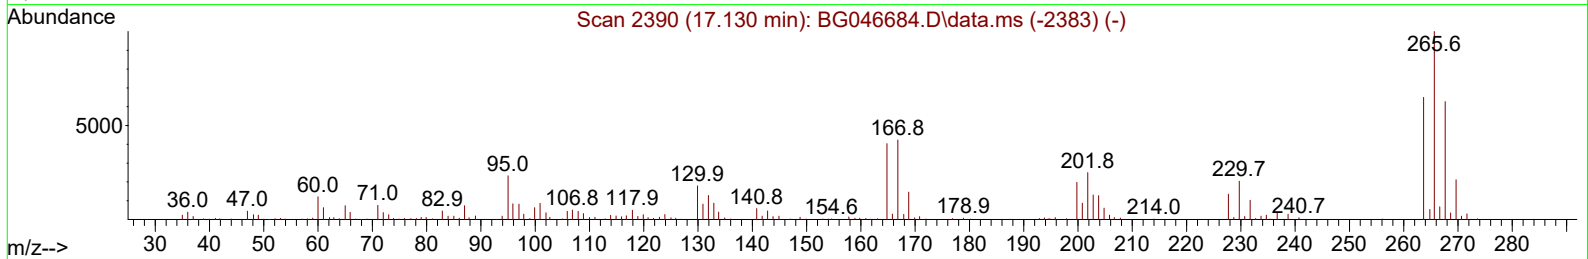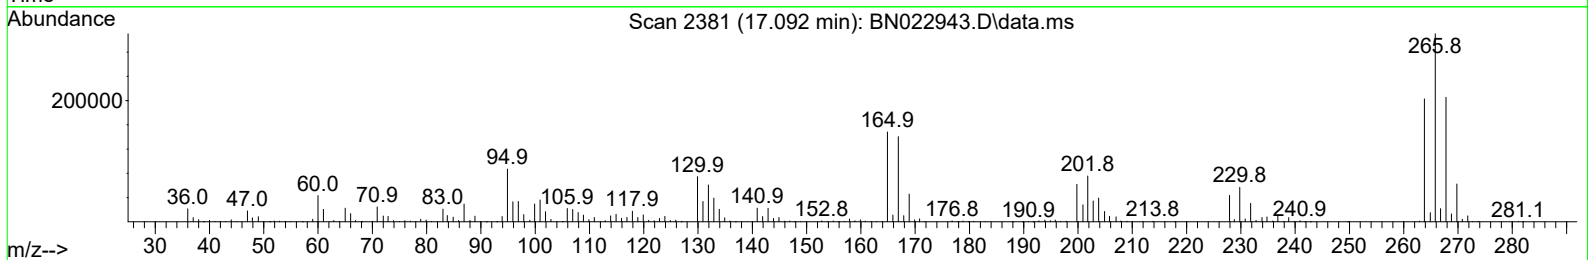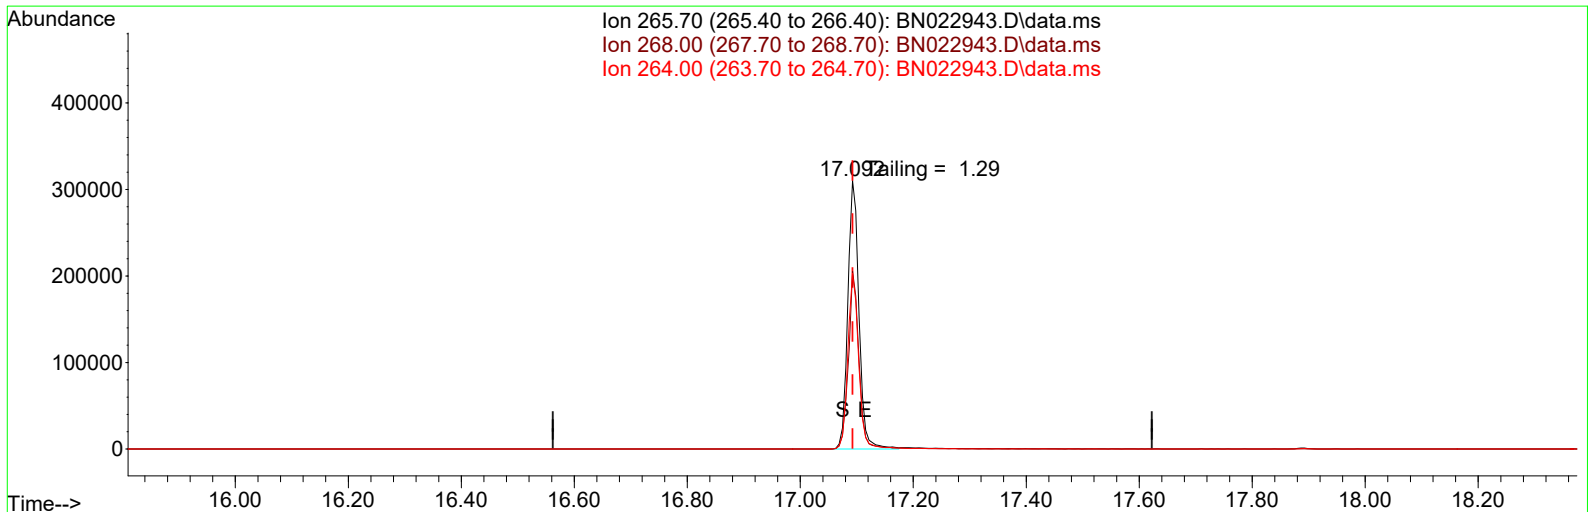

TIC: BN022943.D\data.ms

(70) Pentachlorophenol (C)

17.092min (0.000) 16449.87 ng




response 430530

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.23
264.00	61.60	65.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112922\
Data File : BN022943.D
Acq On : 29 Nov 2022 08:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 30 05:40:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 30 05:40:21 2022
Response via : Initial Calibration

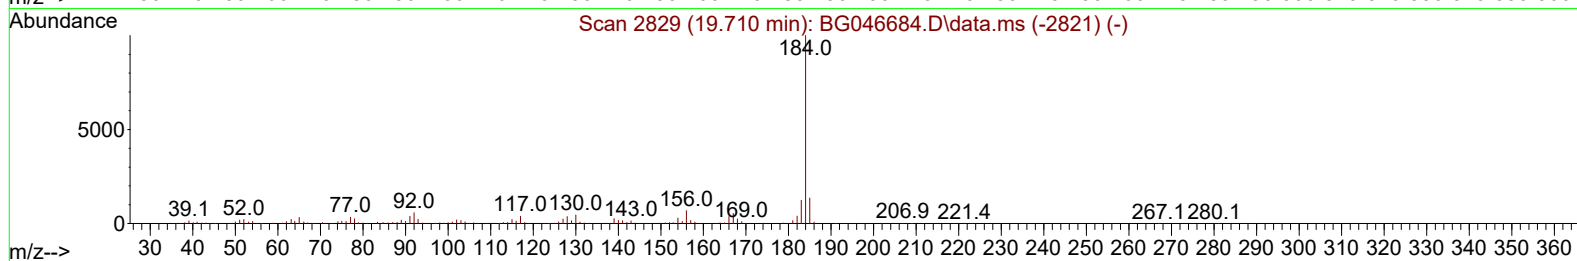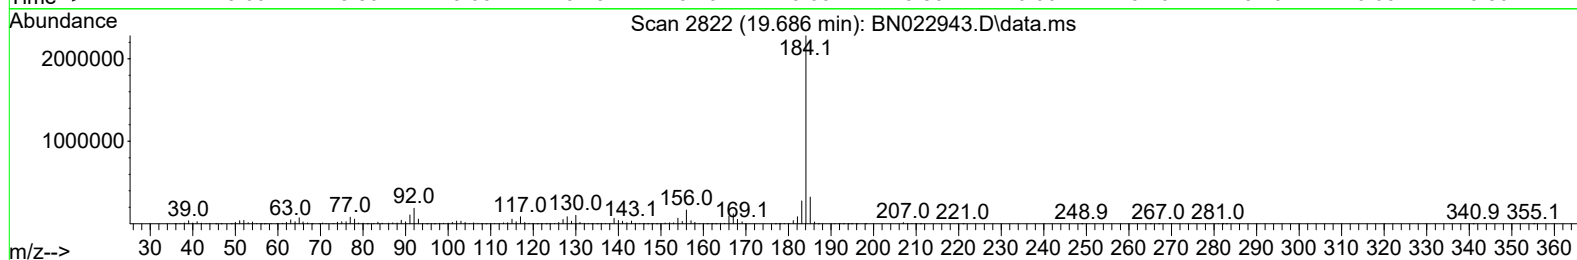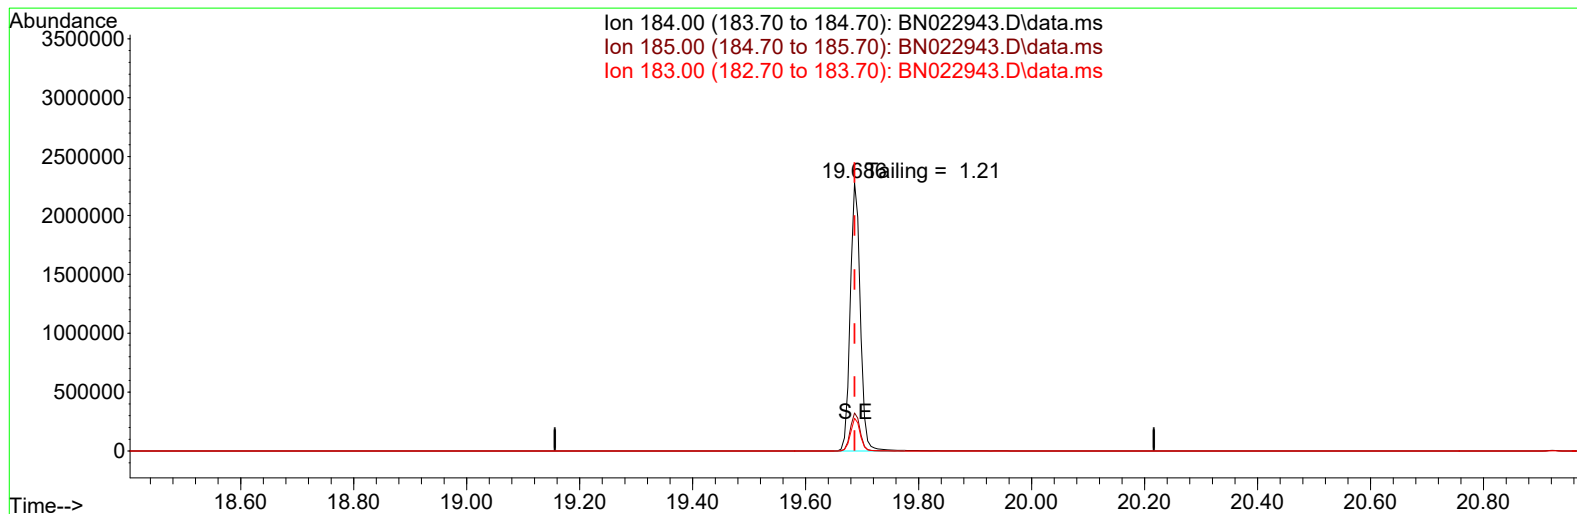

TIC: BN022943.D\data.ms

(77) Benzidine

19.686min (0.000) 0.00 ng

response 2830903

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.20
183.00	13.20	12.22
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/29/2022	BNA_N	<u>BN022943.D</u>
Compound Name	Response	Retention Time
DDT	1324105	20.922
DDD	18216	20.48
DDE	427	19.975
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18643	1342748	1.39

Instrument :
BNA_N
ClientSampleId :
DFTPP