
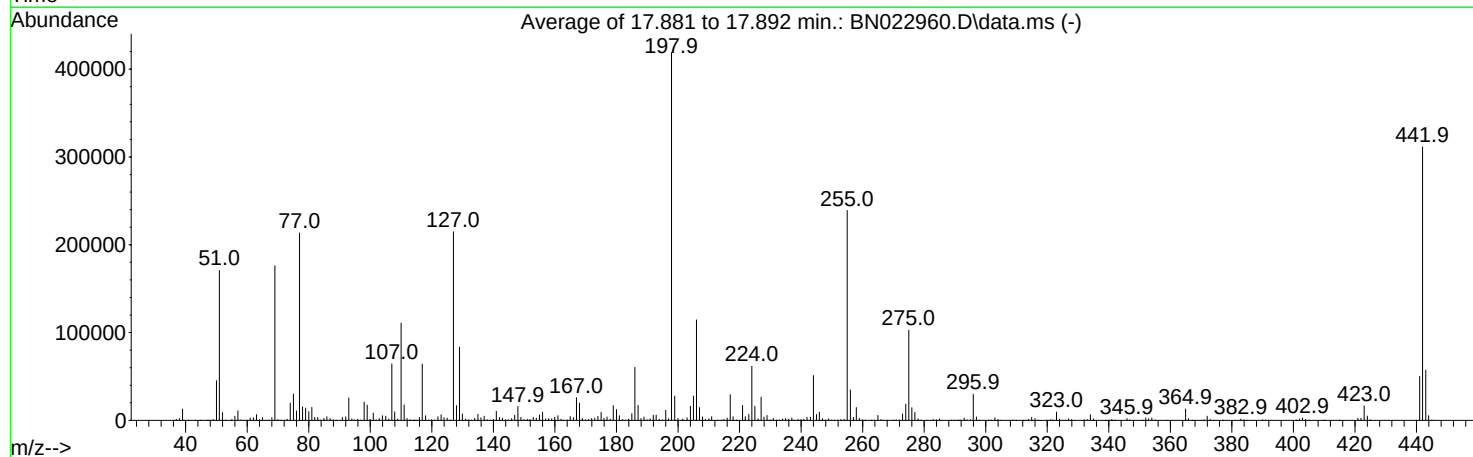


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112922\
 Data File : BN022960.D
 Acq On : 29 Nov 2022 20:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 30 00:45:21 2022

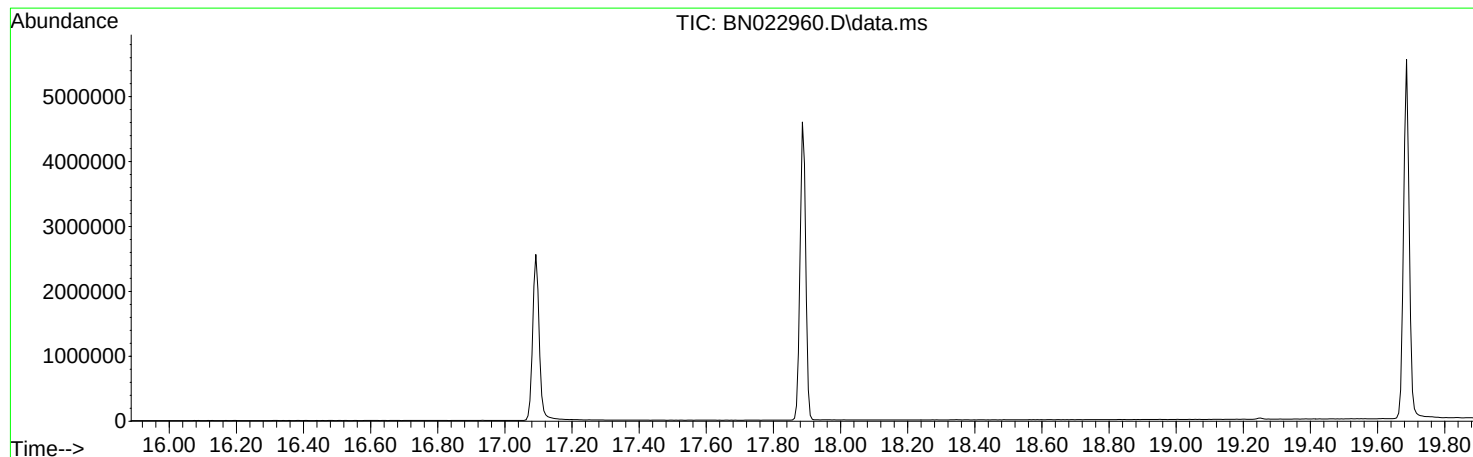




AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.8	170783	PASS
68	69	0.00	2	1.8	3122	PASS
69	198	0.00	100	42.0	176107	PASS
70	69	0.00	2	0.6	979	PASS
127	198	10	80	51.3	214933	PASS
197	198	0.00	2	0.5	1894	PASS
198	198	100	100	100.0	418965	PASS
199	198	5	9	6.6	27795	PASS
275	198	10	60	24.5	102757	PASS
365	198	1	100	3.1	13024	PASS
441	198	0.01	100	12.0	50163	PASS
442	442	50	100	100.0	311445	PASS
443	442	15	24	18.3	57149	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112922\
 Data File : BN022960.D
 Acq On : 29 Nov 2022 20:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Nov 30 05:41:44 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 30 05:40:21 2022
 Response via : Initial Calibration

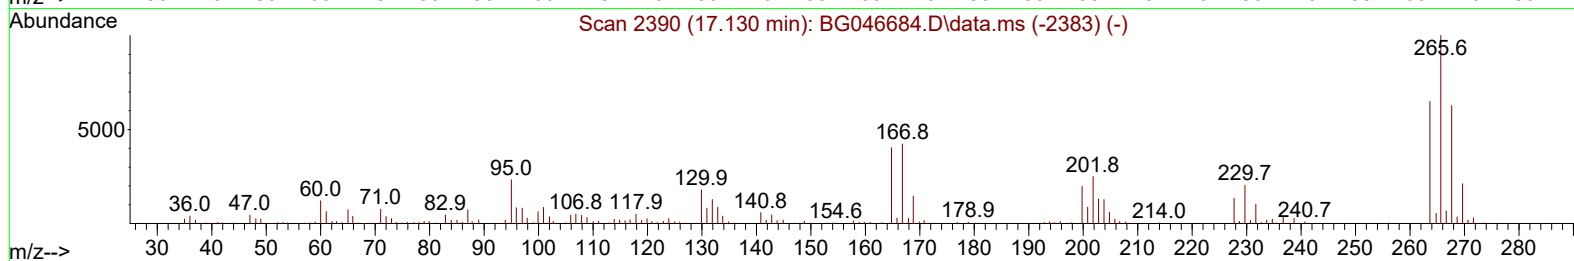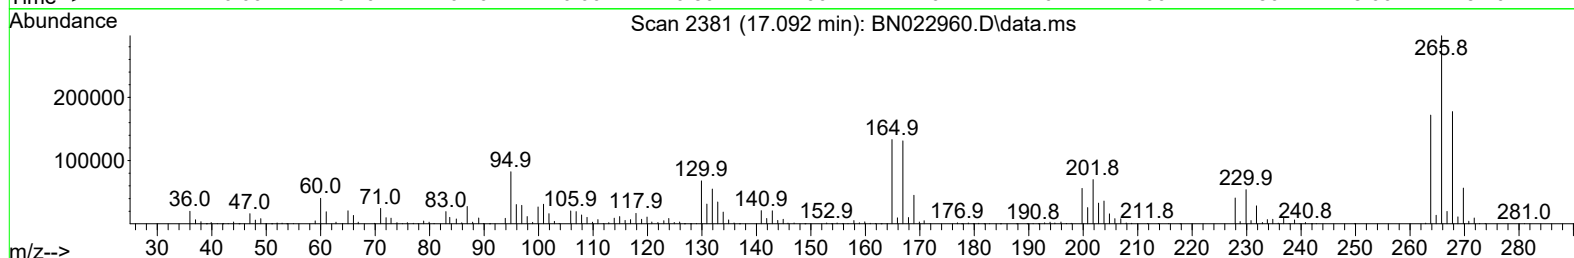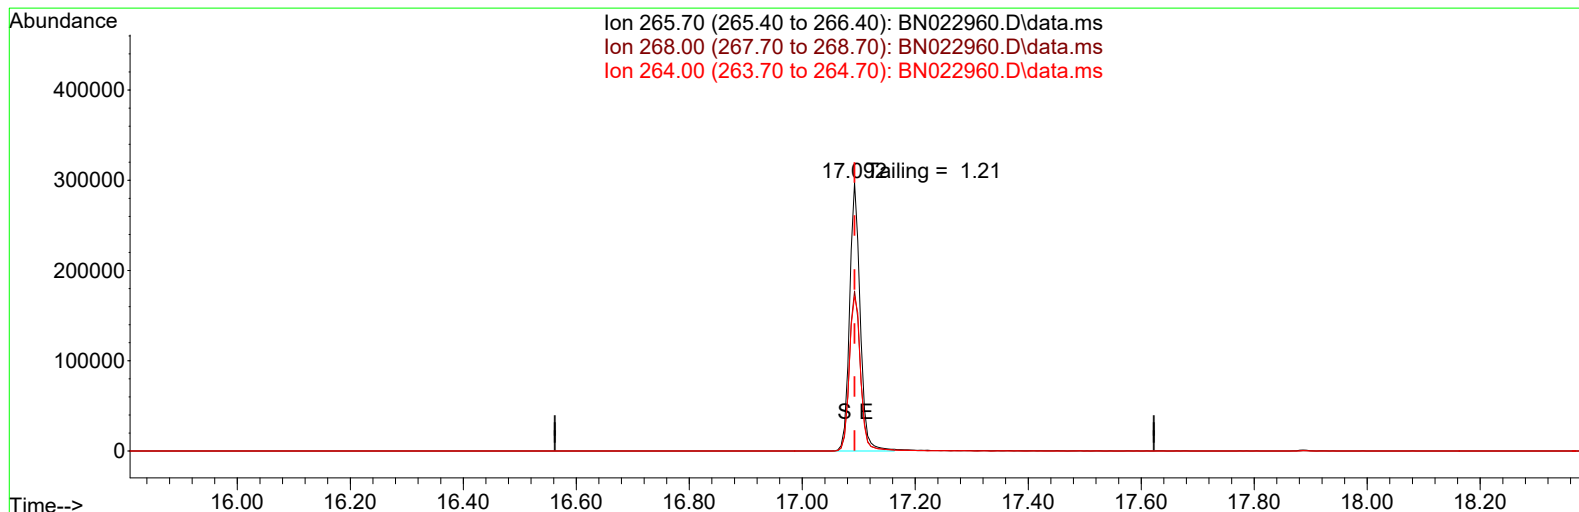

TIC: BN022960.D\data.ms

(70) Pentachlorophenol (C)

17.092min (-0.000) 17555.12 ng




response 390435

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.65
264.00	61.60	57.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112922\
Data File : BN022960.D
Acq On : 29 Nov 2022 20:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 30 05:41:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 30 05:40:21 2022
Response via : Initial Calibration

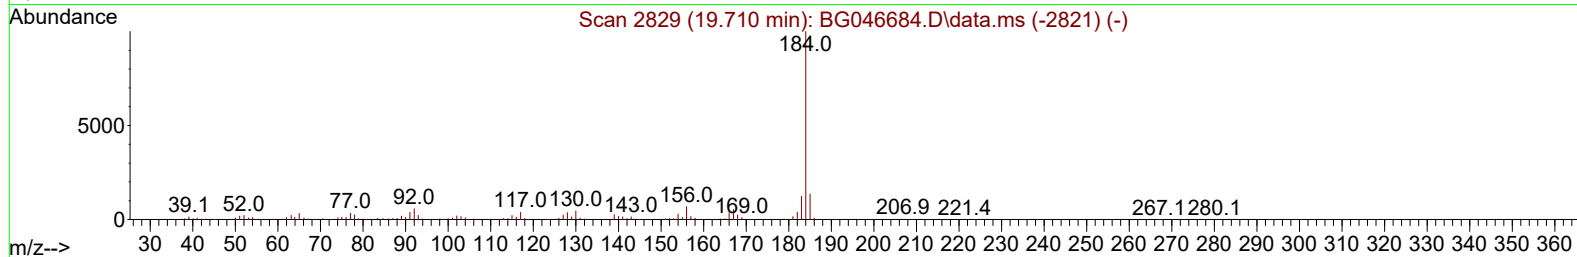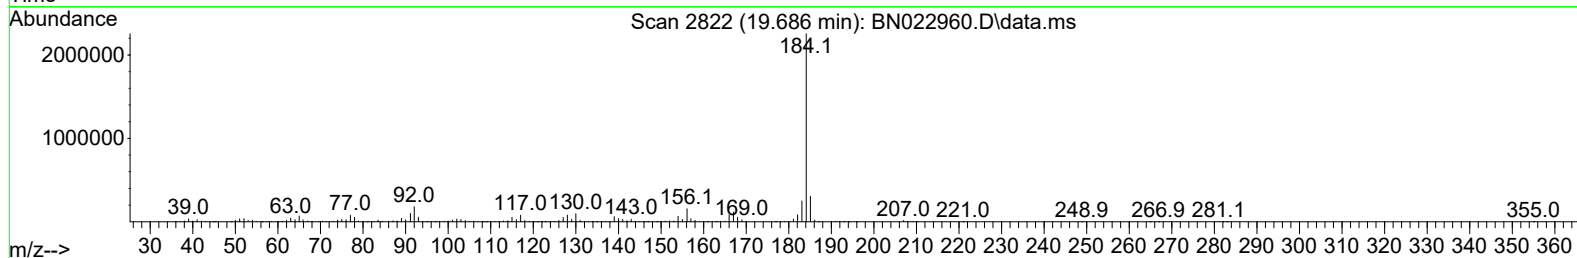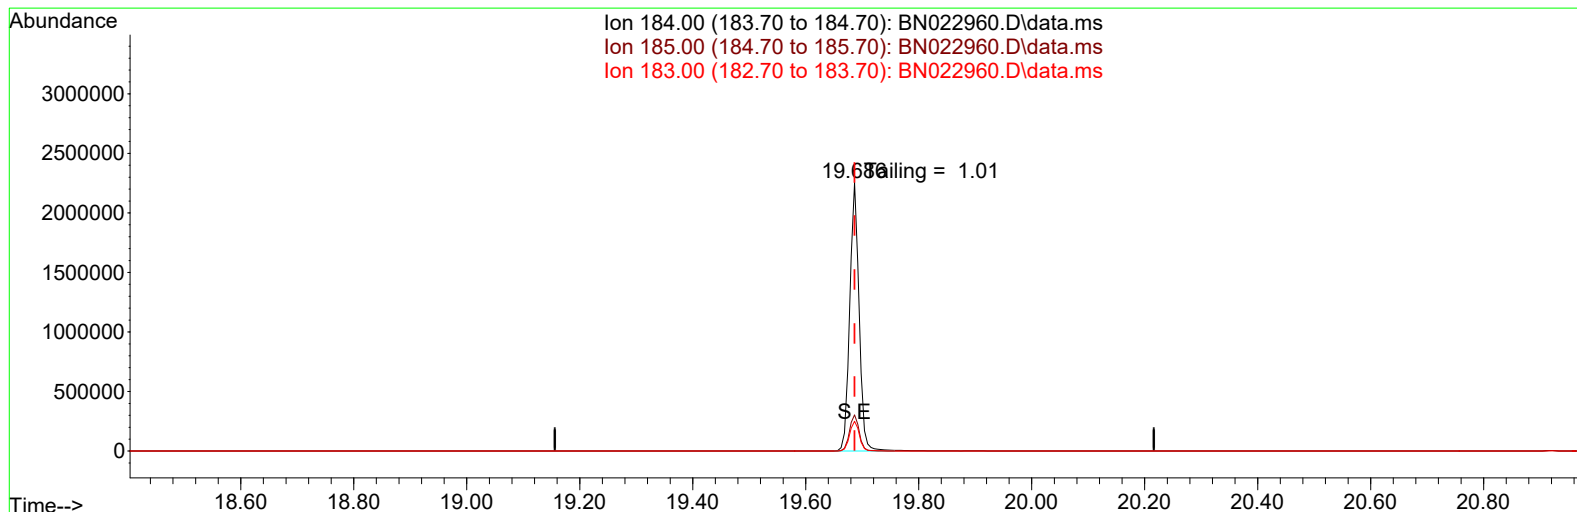

TIC: BN022960.D\data.ms

(77) Benzidine

19.686min (-0.000) 0.00 ng

response 2605372

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.51
183.00	13.20	11.09
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/29/2022	BNA_N	<u>BN022960.D</u>
Compound Name	Response	Retention Time
DDT	1180648	20.922
DDD	15752	20.474
DDE	547	19.969
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16299	1196947	1.36

Instrument :
BNA_N
ClientSampleId :
DFTPP