

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120320\
 Data File : BN012853.D
 Acq On : 03 Dec 2020 18:56
 Operator : CG/JU
 Sample : L4866-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BC1

Quant Time: Dec 04 00:18:25 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 04 00:14:34 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	828	0.40	ng/ul	0.00
2) Naphthalene-d8	10.16	136	3361	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.07	164	2123	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.82
16) Chrysene-d12	21.05	240	3626	0.40	ng/ul	0.00
20) Perylene-d12	23.15	264	3980	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.77	152	2340	0.47	ng/ul	0.00
14) Fluoranthene-d10	18.86	212	5150	0.00	ng/ul	0.00
Target Compounds				Ovalue		
9) Fluorene	15.07	166	1044	0.110	ng/ul#	17
17) Pyrene	19.23	202	1144	0.067	ng/ul#	1
23) Benzo(a)pyrene	23.02	252	2431	0.142	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120320\
Data File : BN012853.D
Acq On : 03 Dec 2020 18:56
Operator : CG/JU
Sample : L4866-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BC1

Quant Time: Dec 04 00:18:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 04 00:14:34 2020
Response via : Initial Calibration

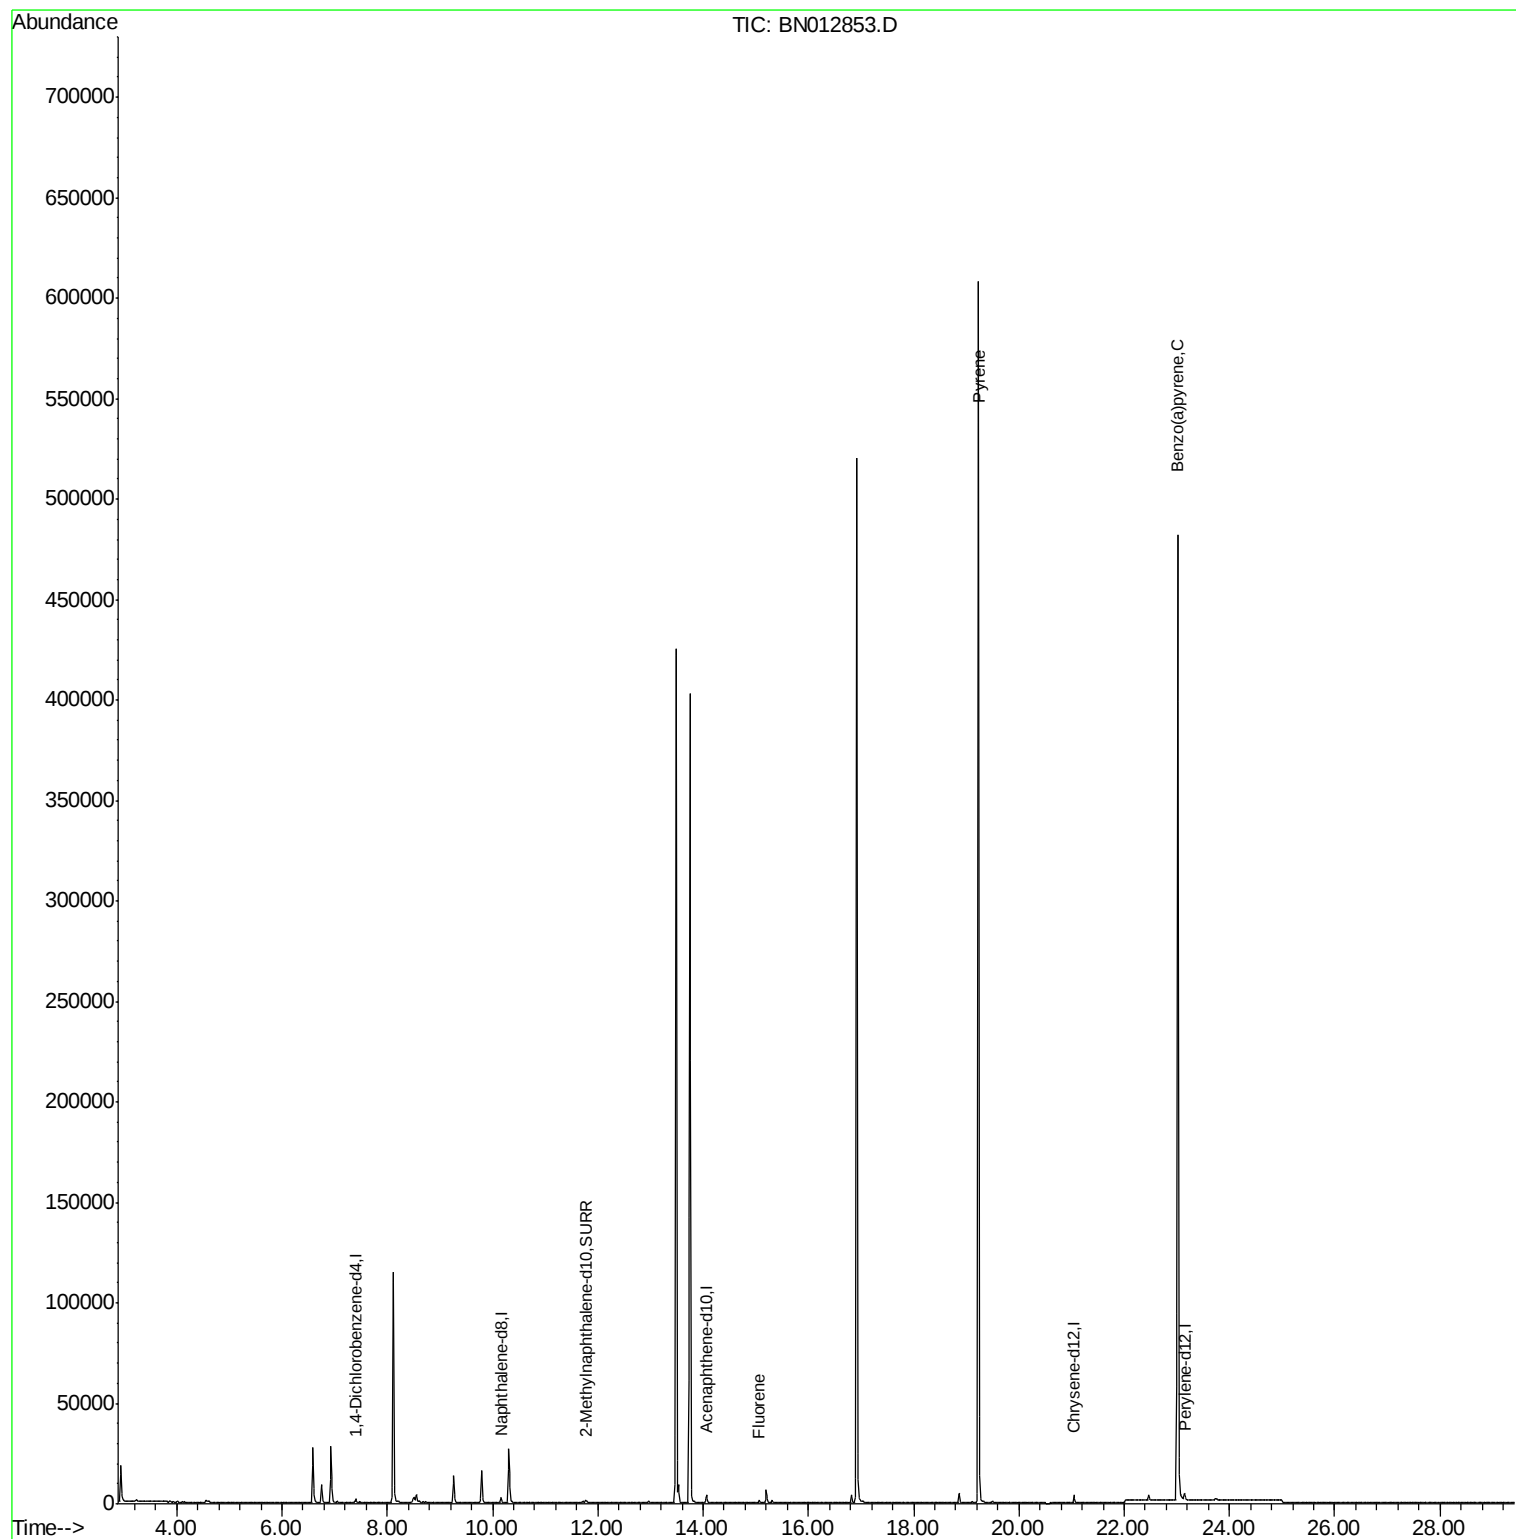

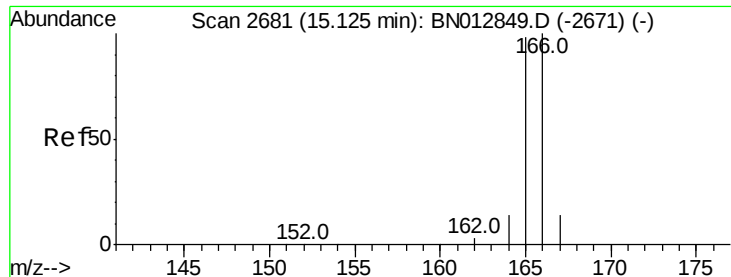

#9

Fluorene

Concen: 0.110 ng/ul

RT: 15.07 min Scan# 2669

Delta R.T. -0.06 min

Lab File: BN012853.D

Acq: 03 Dec 2020 18:56

Instrument :

BNA_N

ClientSampleId :

C0BC1





Tot Ion:166 Resp: 1044

Ion Ratio Lower Upper

166 100

165 9.9 79.8 119.8#

167 34.6 13.8 20.8#

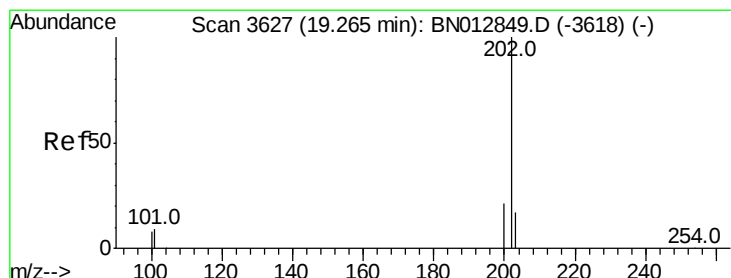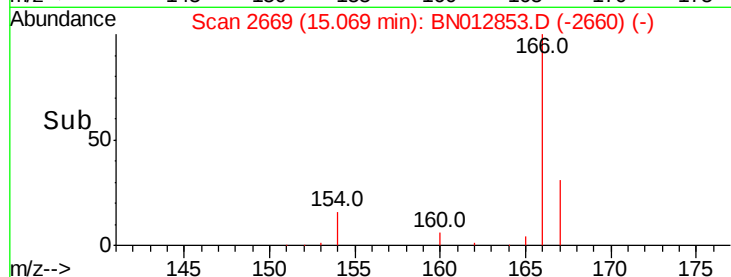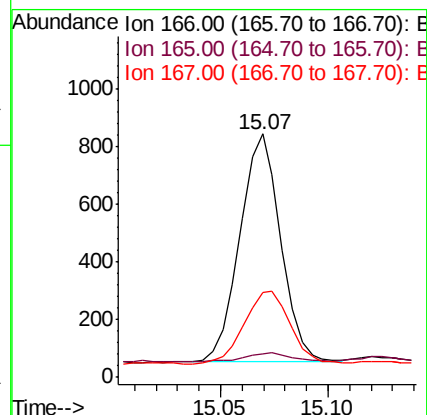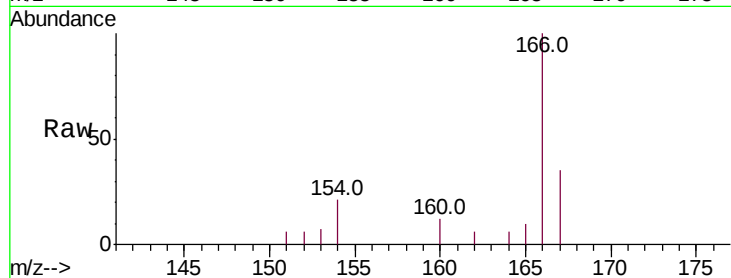

#17

Pyrene

Concen: 0.067 ng/ul

RT: 19.23 min Scan# 3620

Delta R.T. -0.03 min

Lab File: BN012853.D

Acq: 03 Dec 2020 18:56




Tgt Ion:202 Resp: 1144


Ion Ratio Lower Upper

202 100

101 198.1 9.1 13.7#

100 1406.7 7.5 11.3#

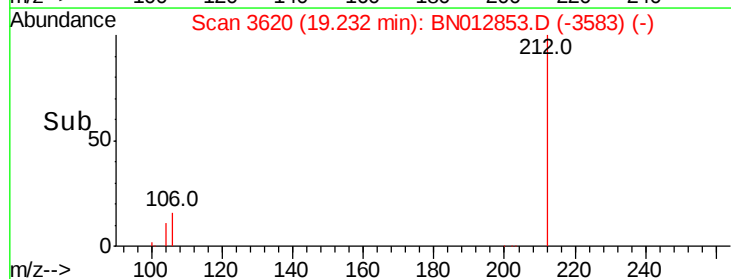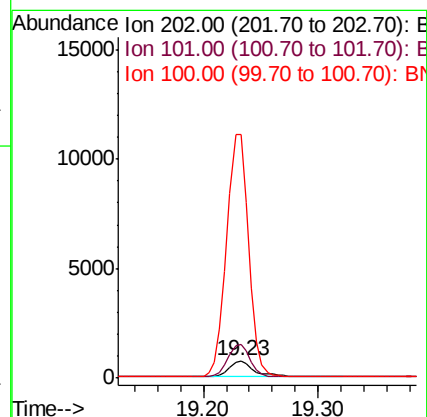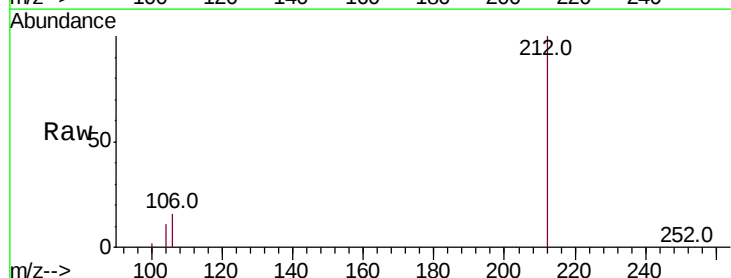

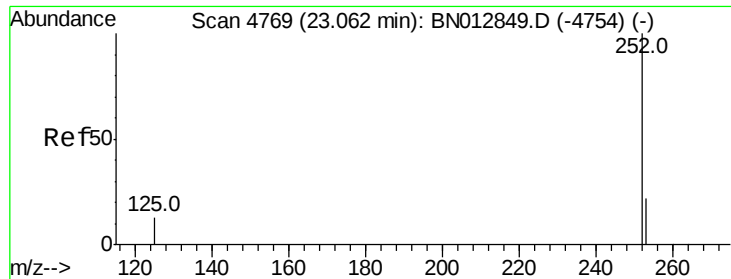

#23

Benzo(a)pyrene

Concen: 0.142 ng/ul

RT: 23.02 min Scan# 4753

Delta R.T. -0.04 min

Lab File: BN012853.D

Acq: 03 Dec 2020 18:56

Instrument :

BNA_N

ClientSampleId :

C0BC1


Tot Ion:252 Resp: 2431

Ion Ratio Lower Upper

252 100

253 43.7 26.5 39.7#

125 38.3 14.2 21.2#

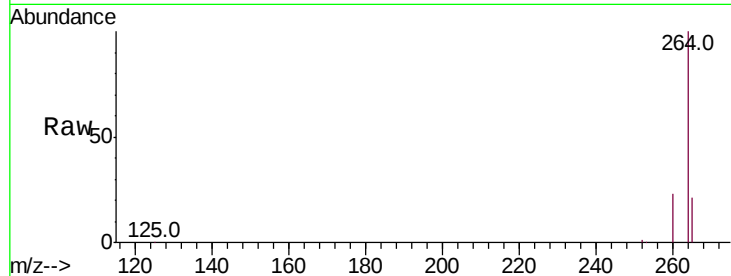

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

