

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120320\
 Data File : BN012855.D
 Acq On : 03 Dec 2020 20:08
 Operator : CG/JU
 Sample : L4866-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BC8

Quant Time: Dec 04 00:18:31 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 04 00:14:34 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	578	0.40	ng/ul	0.00
2) Naphthalene-d8	10.16	136	2340	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.06	164	1454	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.82
16) Chrysene-d12	21.05	240	2524	0.40	ng/ul	0.00
20) Perylene-d12	23.15	264	2872	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.77	152	1438	0.41	ng/ul	0.00
14) Fluoranthene-d10	18.86	212	3149	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.23	202	750	0.063	ng/ul#	1
23) Benzo(a)pyrene	23.01	252	1595	0.129	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120320\
Data File : BN012855.D
Acq On : 03 Dec 2020 20:08
Operator : CG/JU
Sample : L4866-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BC8

Quant Time: Dec 04 00:18:31 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 04 00:14:34 2020
Response via : Initial Calibration




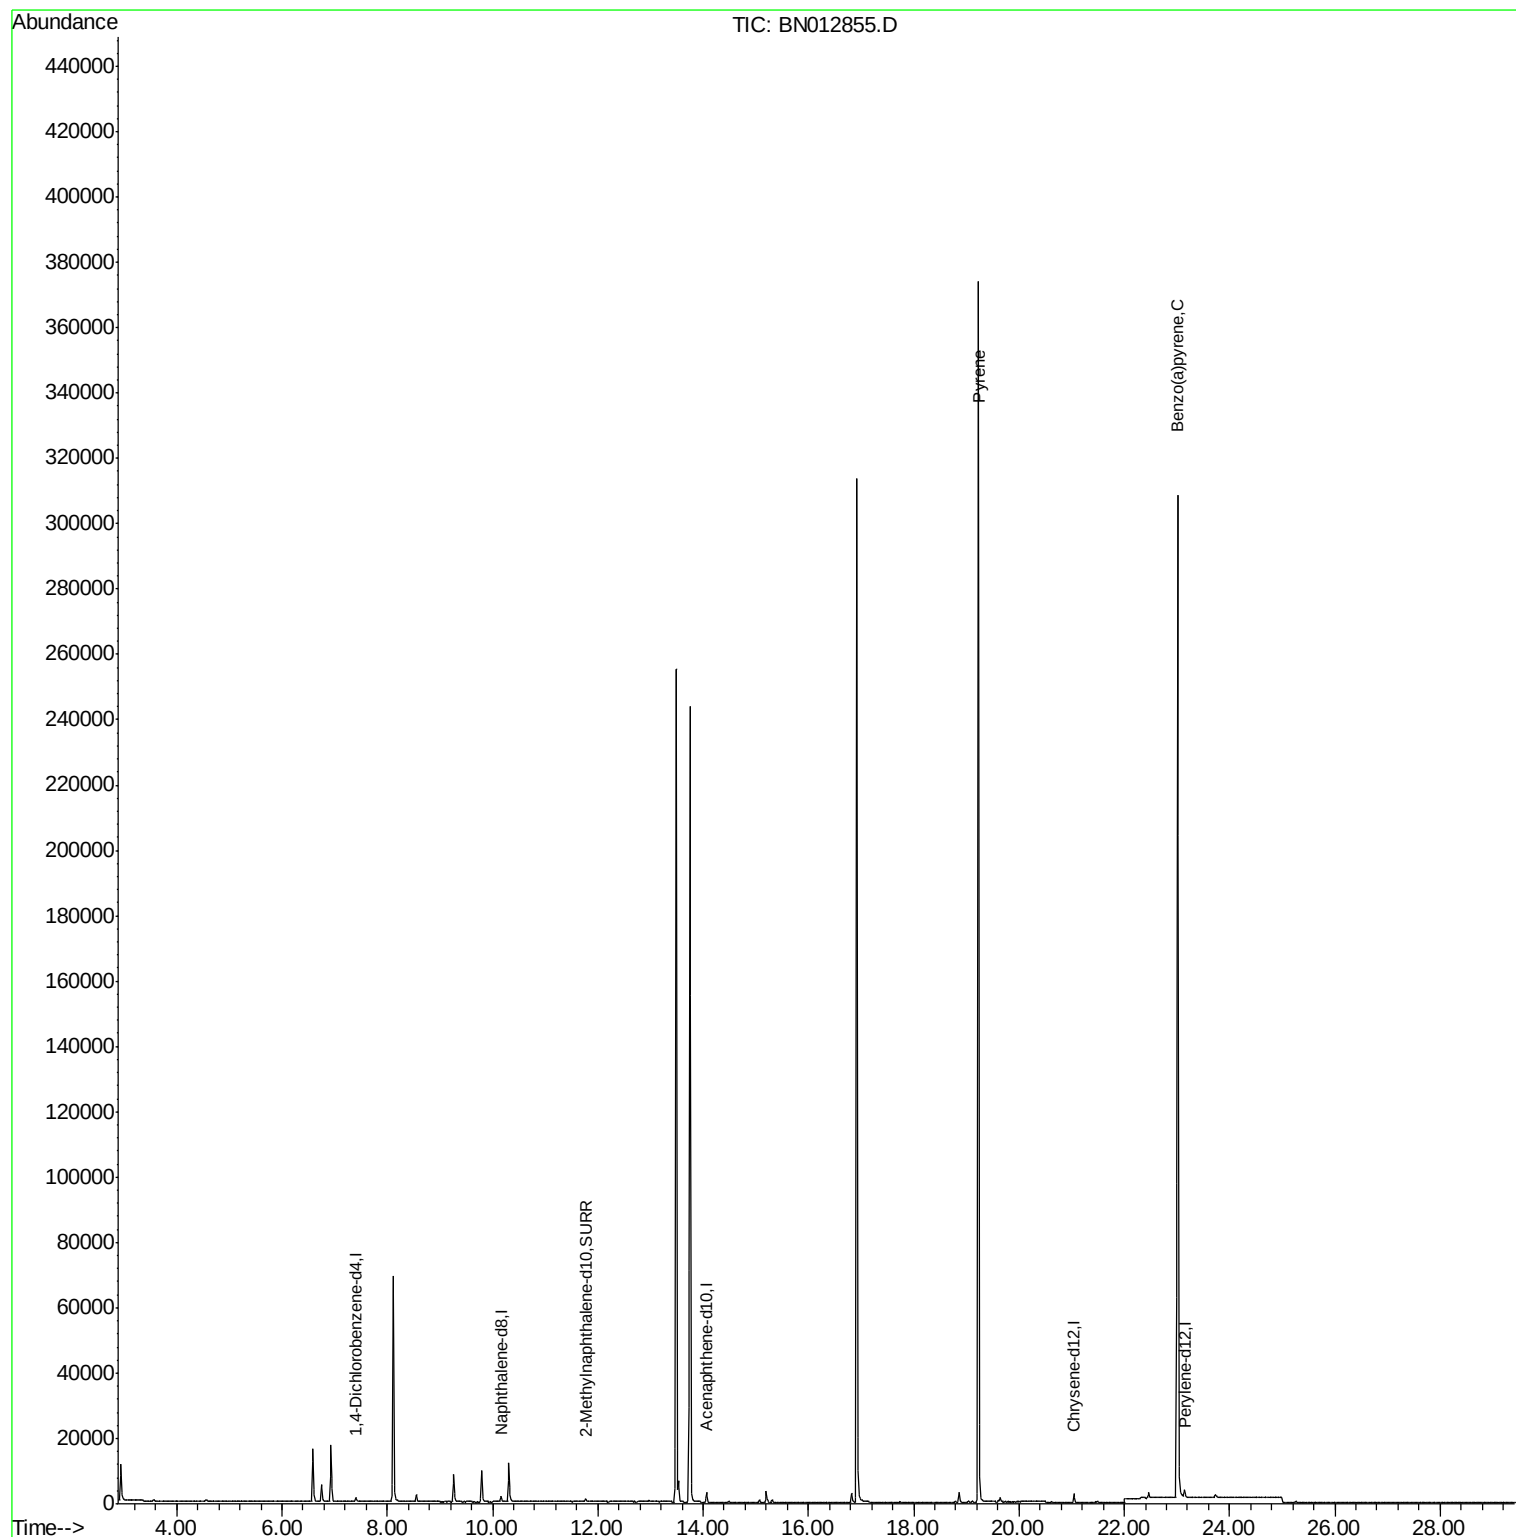


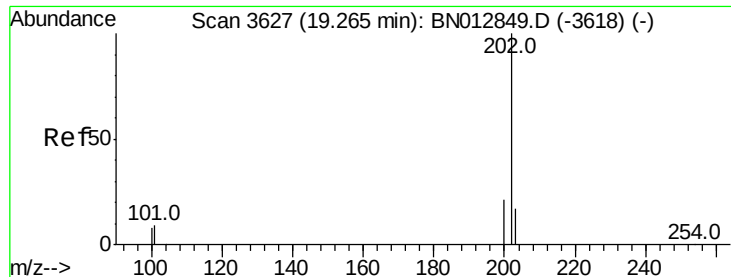

#17
Pvrene
Concen: 0.063 ng/ul
RT: 19.23 min Scan# 3620
Delta R.T. -0.03 min
Lab File: BN012855.D
Acq: 03 Dec 2020 20:08

Instrument :
BNA_N
ClientSampleId :
C0BC8

Tot Ion:202 Resp: 750
Ion Ratio Lower Upper
202 100
101 198.6 9.1 13.7#
100 1366.5 7.5 11.3#

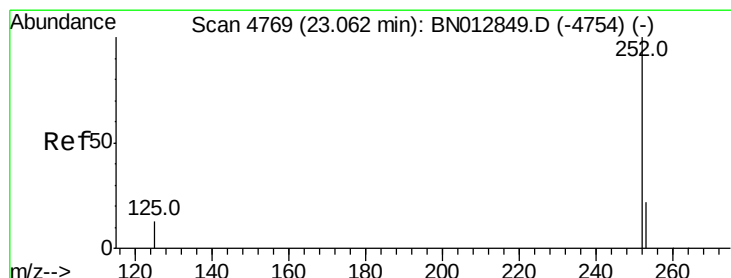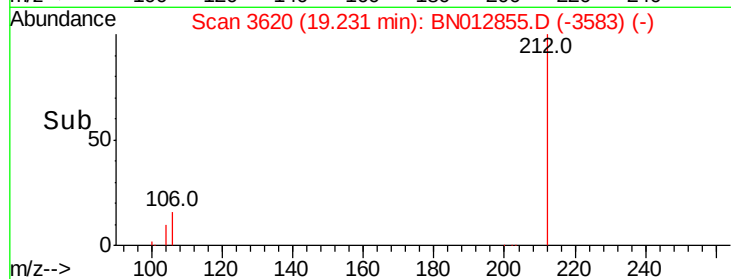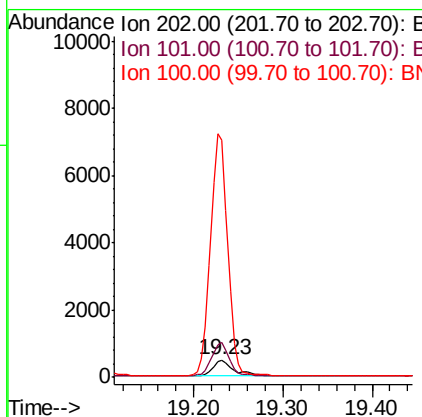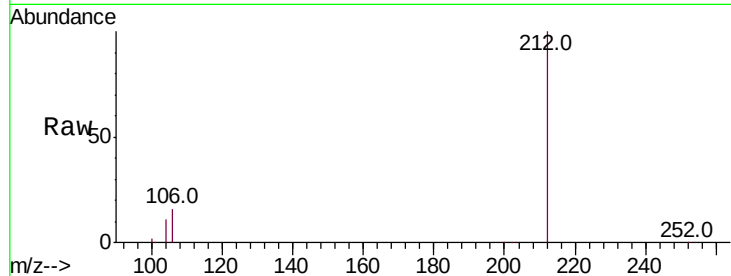

#23
Benzo(a)pyrene
Concen: 0.129 ng/ul
RT: 23.01 min Scan# 4752
Delta R.T. -0.04 min
Lab File: BN012855.D
Acq: 03 Dec 2020 20:08

Tgt Ion:252 Resp: 1595
Ion Ratio Lower Upper
252 100
253 49.2 26.5 39.7#
125 40.1 14.2 21.2#

