

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120320\
 Data File : BN012856.D
 Acq On : 03 Dec 2020 20:44
 Operator : CG/JU
 Sample : L4866-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BE1

Quant Time: Dec 04 00:18:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 04 00:14:34 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	553	0.40	ng/ul	0.00
2) Naphthalene-d8	10.16	136	2218	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.07	164	1372	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.82
16) Chrysene-d12	21.04	240	2408	0.40	ng/ul	0.00
20) Perylene-d12	23.15	264	2798	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.77	152	1361	0.41	ng/ul	0.00
14) Fluoranthene-d10	18.87	212	2979	0.00	ng/ul	0.00
Target Compounds						
					Ovalue	
9) Fluorene	15.07	166	605	0.099	ng/ul#	20
17) Pyrene	19.23	202	702	0.062	ng/ul#	1
23) Benzo(a)pyrene	23.01	252	1472	0.123	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120320\
Data File : BN012856.D
Acq On : 03 Dec 2020 20:44
Operator : CG/JU
Sample : L4866-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BE1

Quant Time: Dec 04 00:18:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 04 00:14:34 2020
Response via : Initial Calibration




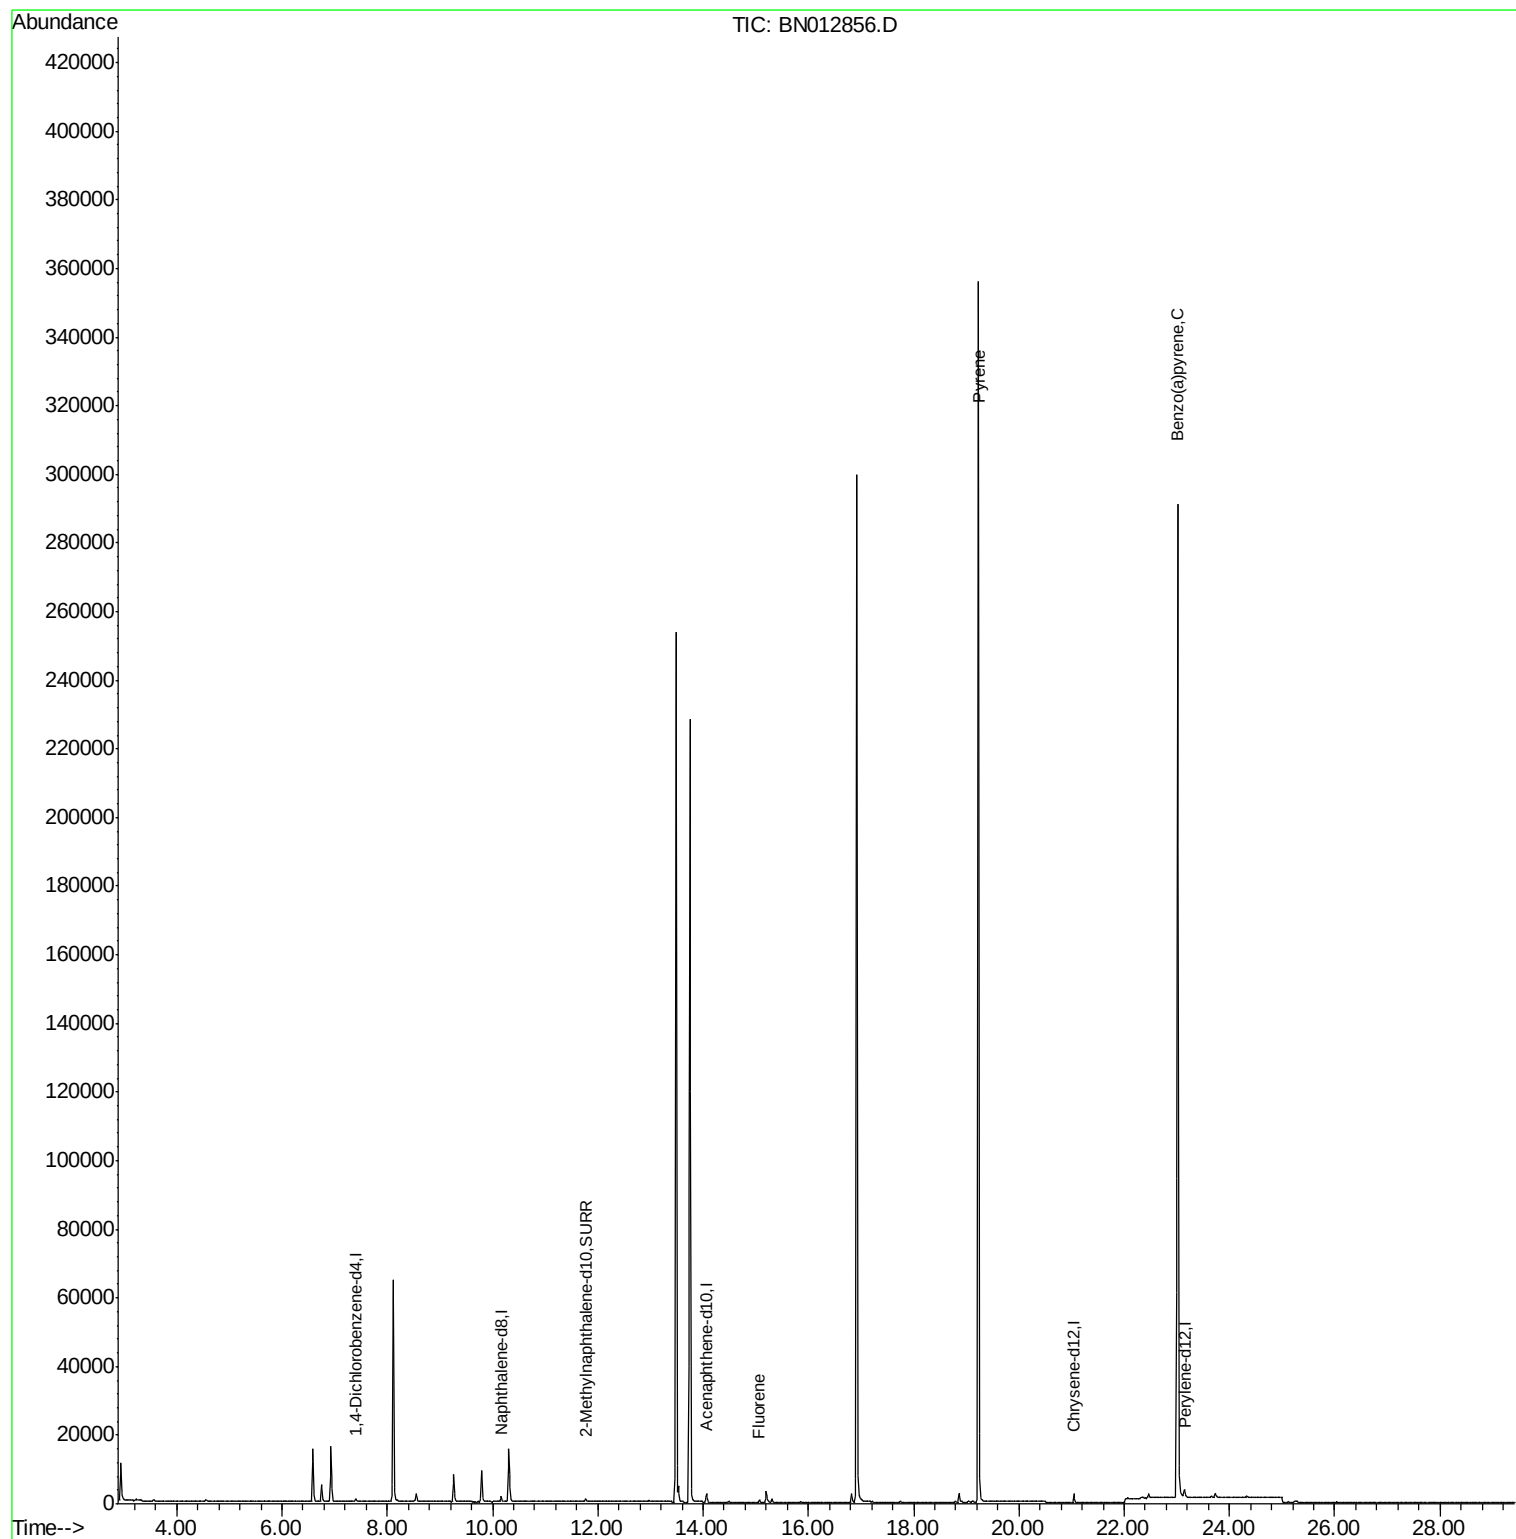


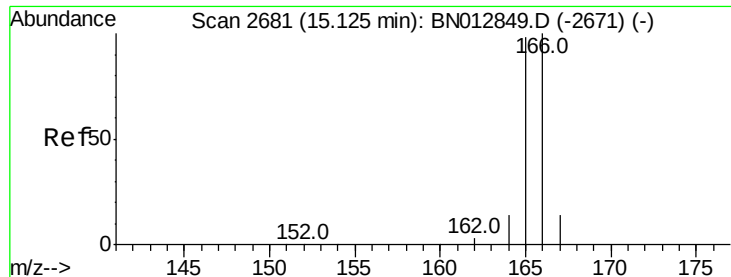

#9
Fluorene
 Concen: 0.099 ng/ul
 RT: 15.07 min Scan# 2669
 Delta R.T. -0.06 min
 Lab File: BN012856.D
 Acq: 03 Dec 2020 20:44




Instrument :
 BNA_N
 ClientSampleId :
 C0BE1


Tot Ion:166 Resp: 605
 Ion Ratio Lower Upper
 166 100
 165 14.4 79.8 119.8#
 167 39.2 13.8 20.8#

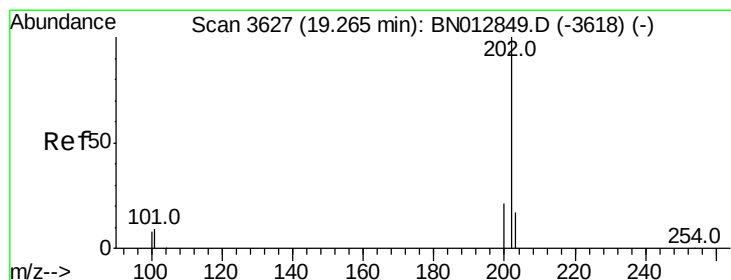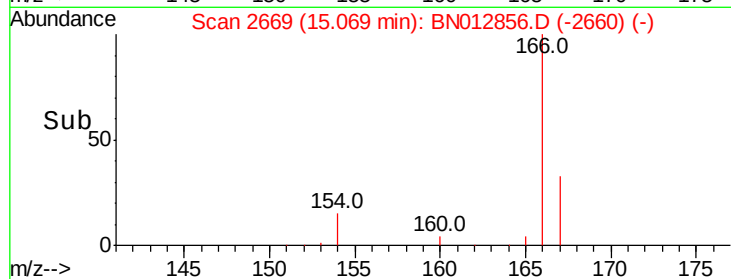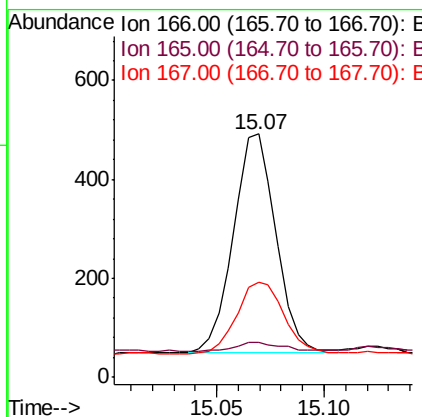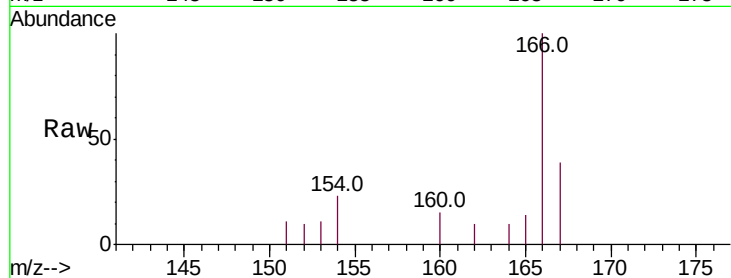

#17
Pyrene
 Concen: 0.062 ng/ul
 RT: 19.23 min Scan# 3620
 Delta R.T. -0.03 min
 Lab File: BN012856.D
 Acq: 03 Dec 2020 20:44

Tgt Ion:202 Resp: 702
 Ion Ratio Lower Upper
 202 100
 101 197.3 9.1 13.7#
 100 1338.1 7.5 11.3#

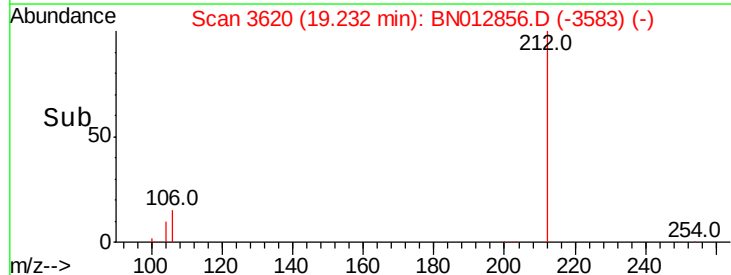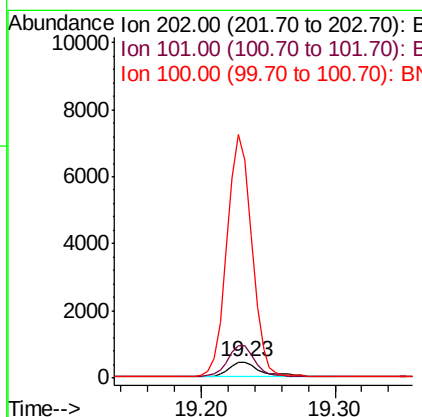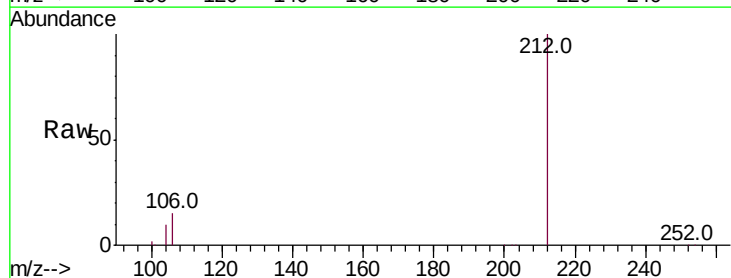

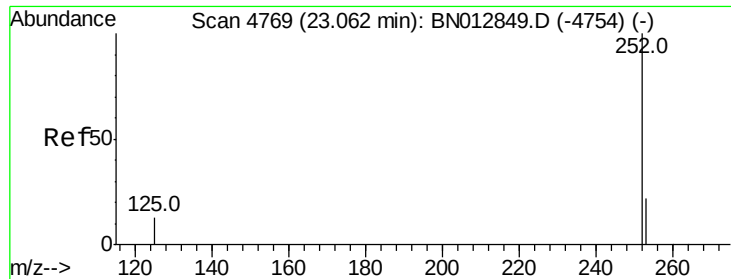

#23

Benzo(a)pyrene

Concen: 0.123 ng/ul

RT: 23.01 min Scan# 4752

Delta R.T. -0.04 min

Lab File: BN012856.D

Acq: 03 Dec 2020 20:44

Instrument :

BNA_N

ClientSampleId :

C0BE1


Tot Ion: 252 Resp: 1472

Ion Ratio Lower Upper

252 100

253 48.9 26.5 39.7#

125 42.7 14.2 21.2#

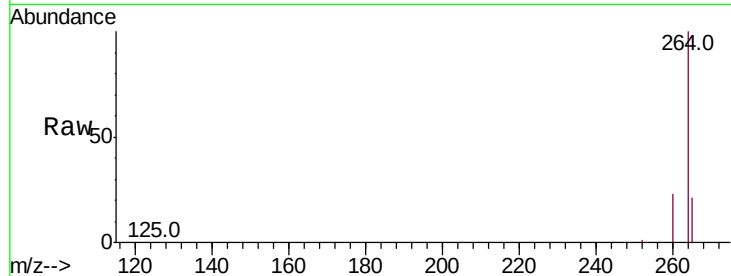

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

