

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120320\
 Data File : BN012858.D
 Acq On : 03 Dec 2020 21:56
 Operator : CG/JU
 Sample : L4866-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BE0

Quant Time: Dec 04 00:18:45 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 04 00:14:34 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	664	0.40	ng/ul	0.00
2) Naphthalene-d8	10.16	136	2726	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.07	164	1714	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.82
16) Chrysene-d12	21.04	240	2943	0.40	ng/ul	0.00
20) Perylene-d12	23.14	264	3390	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.77	152	1742	0.43	ng/ul	0.00
14) Fluoranthene-d10	18.86	212	3943	0.00	ng/ul	0.00
Target Compounds				Ovalue		
9) Fluorene	15.07	166	813	0.106	ng/ul#	18
17) Pyrene	19.23	202	908	0.065	ng/ul#	1
23) Benzo(a)pyrene	23.01	252	1938	0.133	ng/ul#	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120320\
Data File : BN012858.D
Acq On : 03 Dec 2020 21:56
Operator : CG/JU
Sample : L4866-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BE0

Quant Time: Dec 04 00:18:45 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 04 00:14:34 2020
Response via : Initial Calibration




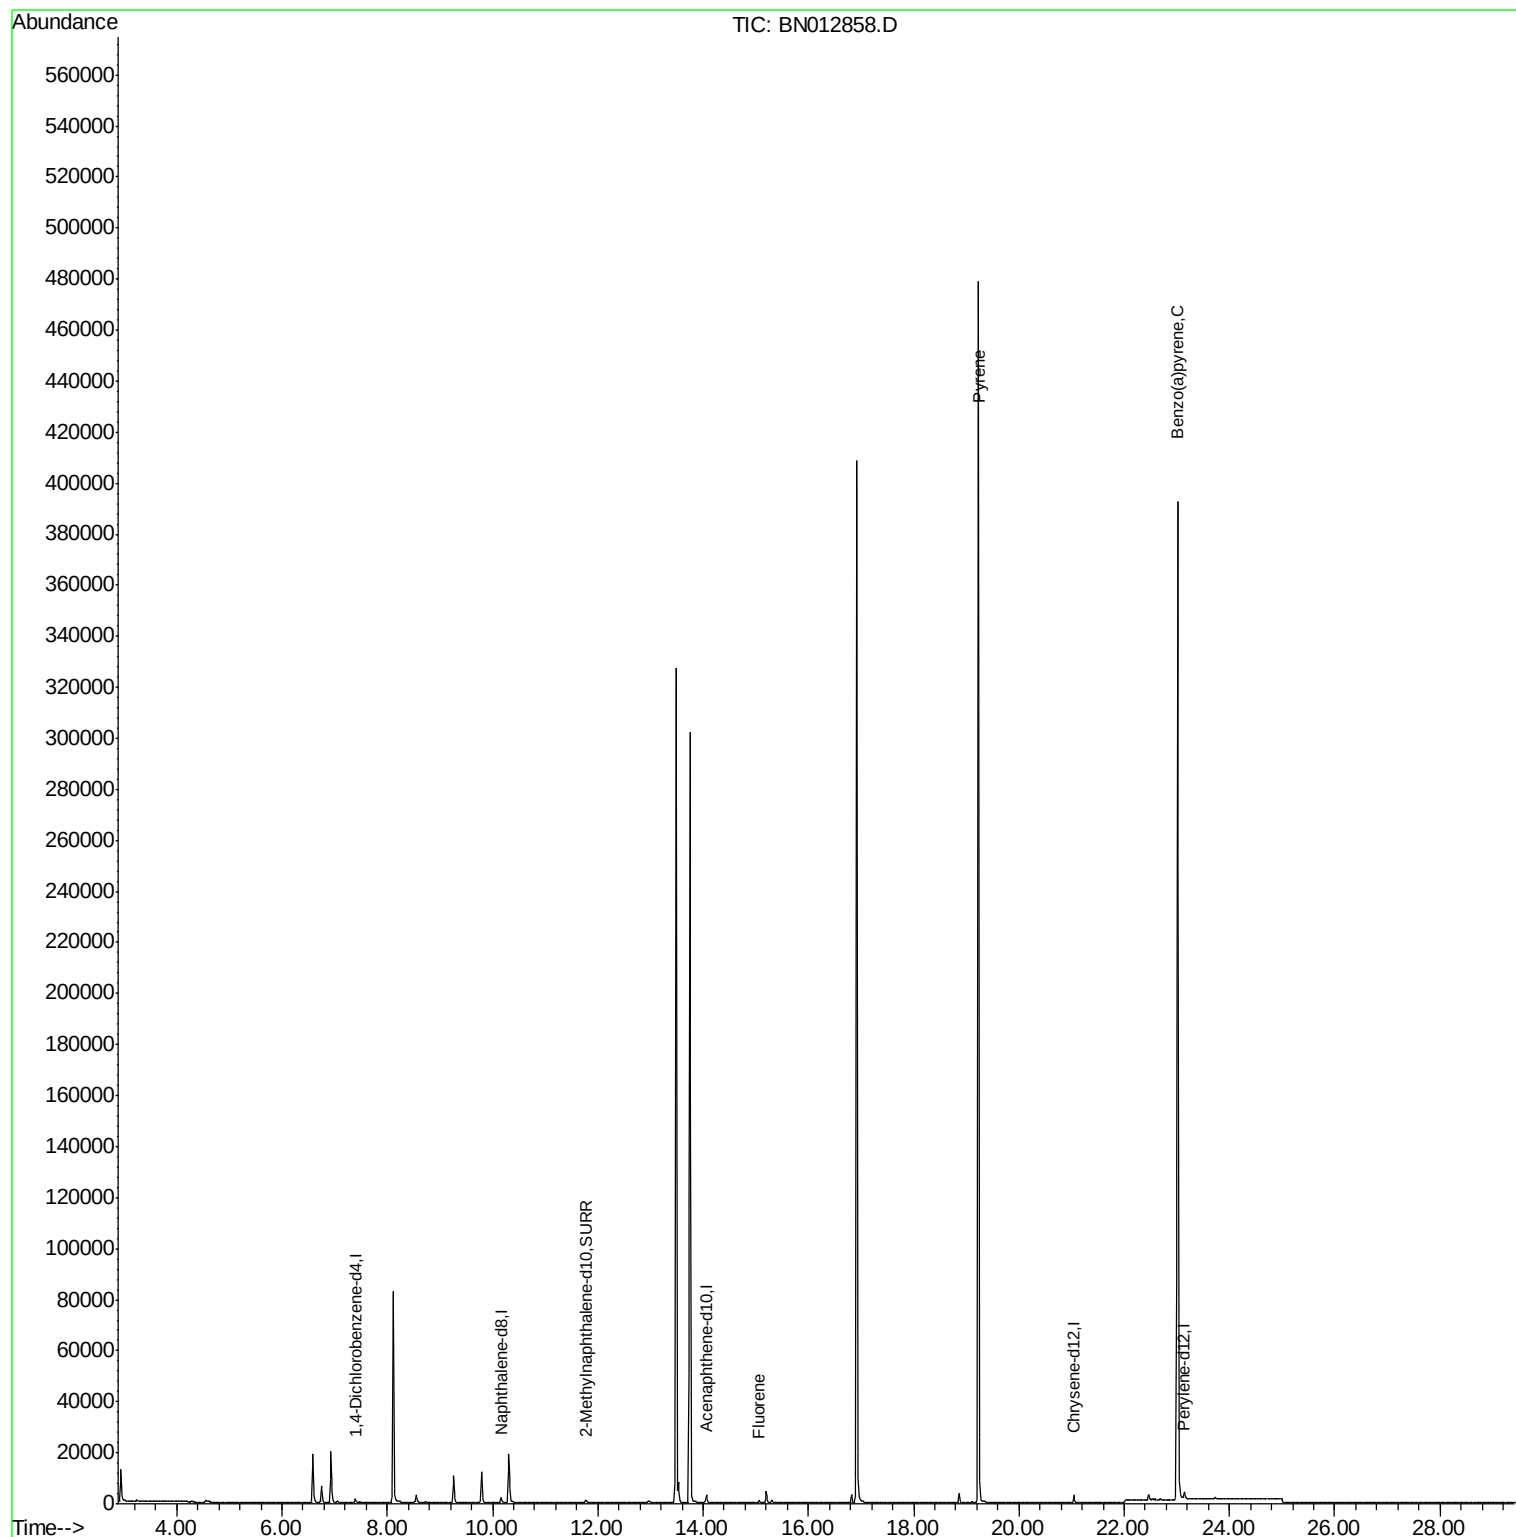


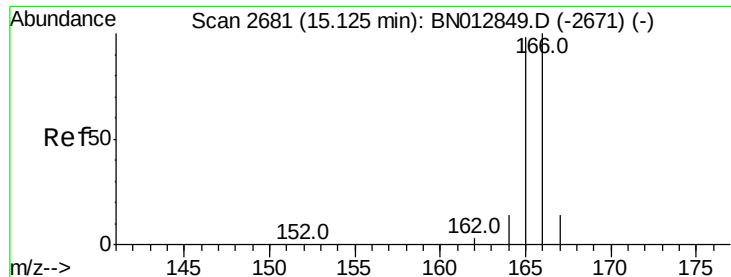

#9
Fluorene
 Concen: 0.106 ng/ul
 RT: 15.07 min Scan# 2669
 Delta R.T. -0.06 min
 Lab File: BN012858.D
 Acq: 03 Dec 2020 21:56




Instrument :
 BNA_N
 ClientSampleId :
 C0BE0


Tot Ion:166 Resp: 813
 Ion Ratio Lower Upper
 166 100
 165 11.6 79.8 119.8#
 167 38.4 13.8 20.8#

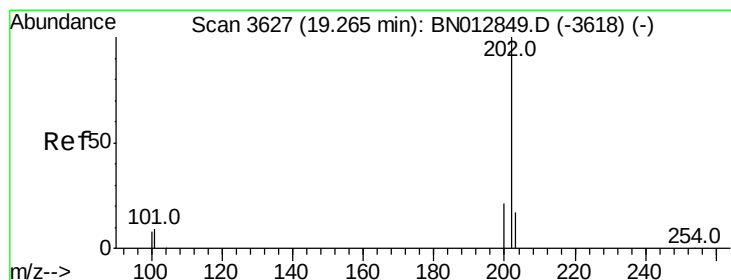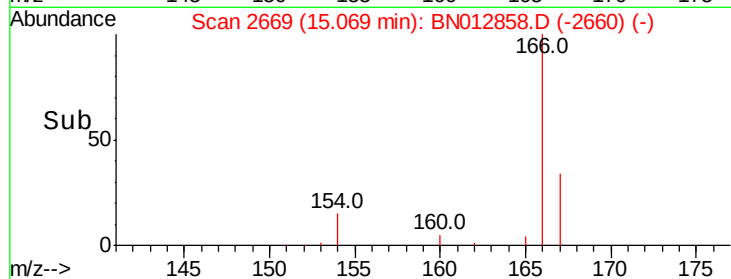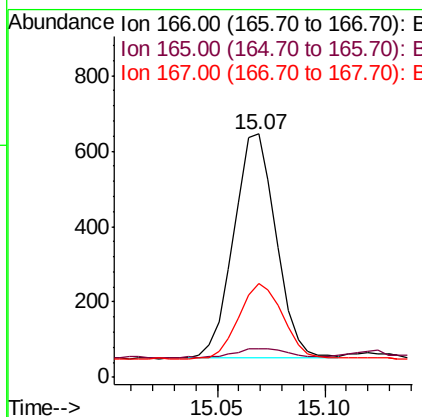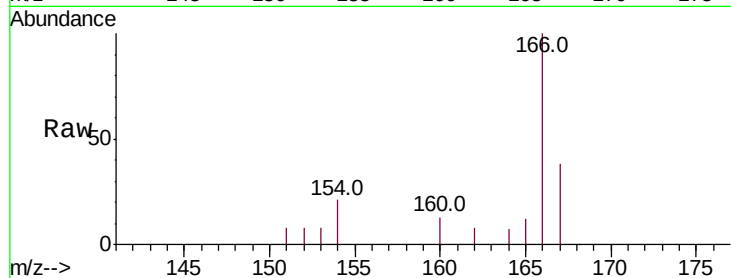

#17
Pyrene
 Concen: 0.065 ng/ul
 RT: 19.23 min Scan# 3620
 Delta R.T. -0.03 min
 Lab File: BN012858.D
 Acq: 03 Dec 2020 21:56

Tgt Ion:202 Resp: 908
 Ion Ratio Lower Upper
 202 100
 101 197.1 9.1 13.7#
 100 1374.8 7.5 11.3#

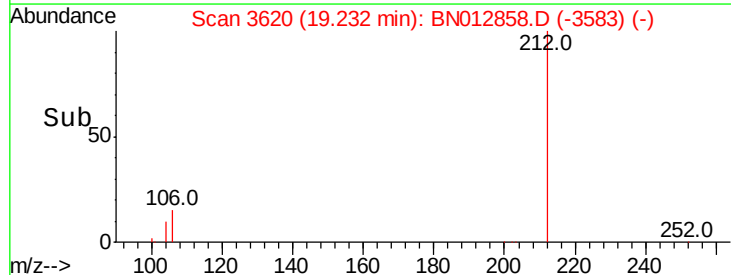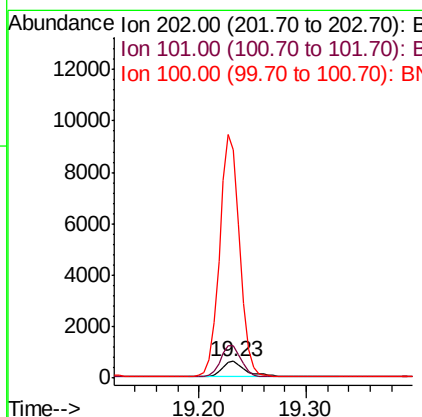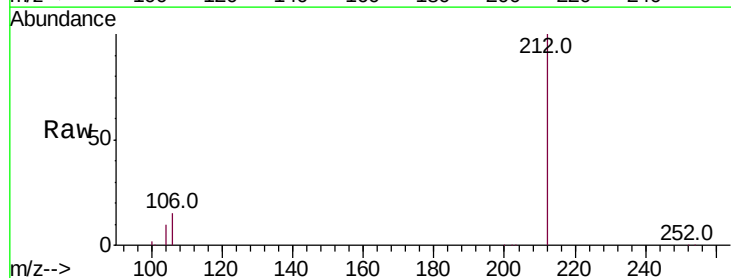

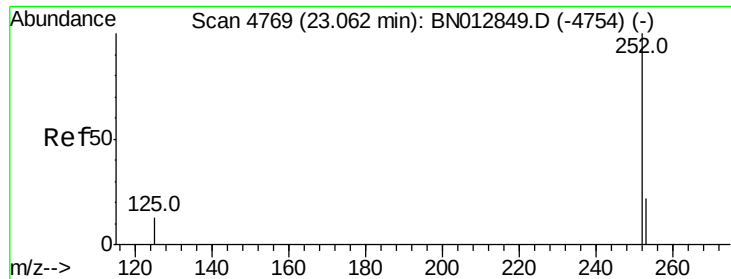

#23

Benzo(a)pyrene

Concen: 0.133 ng/ul

RT: 23.01 min Scan# 4752

Delta R.T. -0.04 min

Lab File: BN012858.D

Acq: 03 Dec 2020 21:56

Instrument :

BNA_N

ClientSampleId :

C0BE0


Tot Ion: 252 Resp: 1938

Ion Ratio Lower Upper

252 100

253 44.6 26.5 39.7#

125 38.5 14.2 21.2#

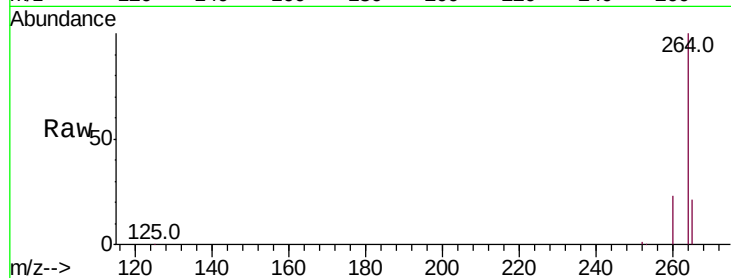

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

