


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120320\
Data File : BN012854.D
Acq On : 03 Dec 2020 19:32
Operator : CG/JU
Sample : L4866-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BE4

Manual Integrations
APPROVED

mohammad
12/7/2020 8:51:14 AM

Quant Time: Dec 04 00:29:15 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 04 00:14:34 2020
Response via : Initial Calibration

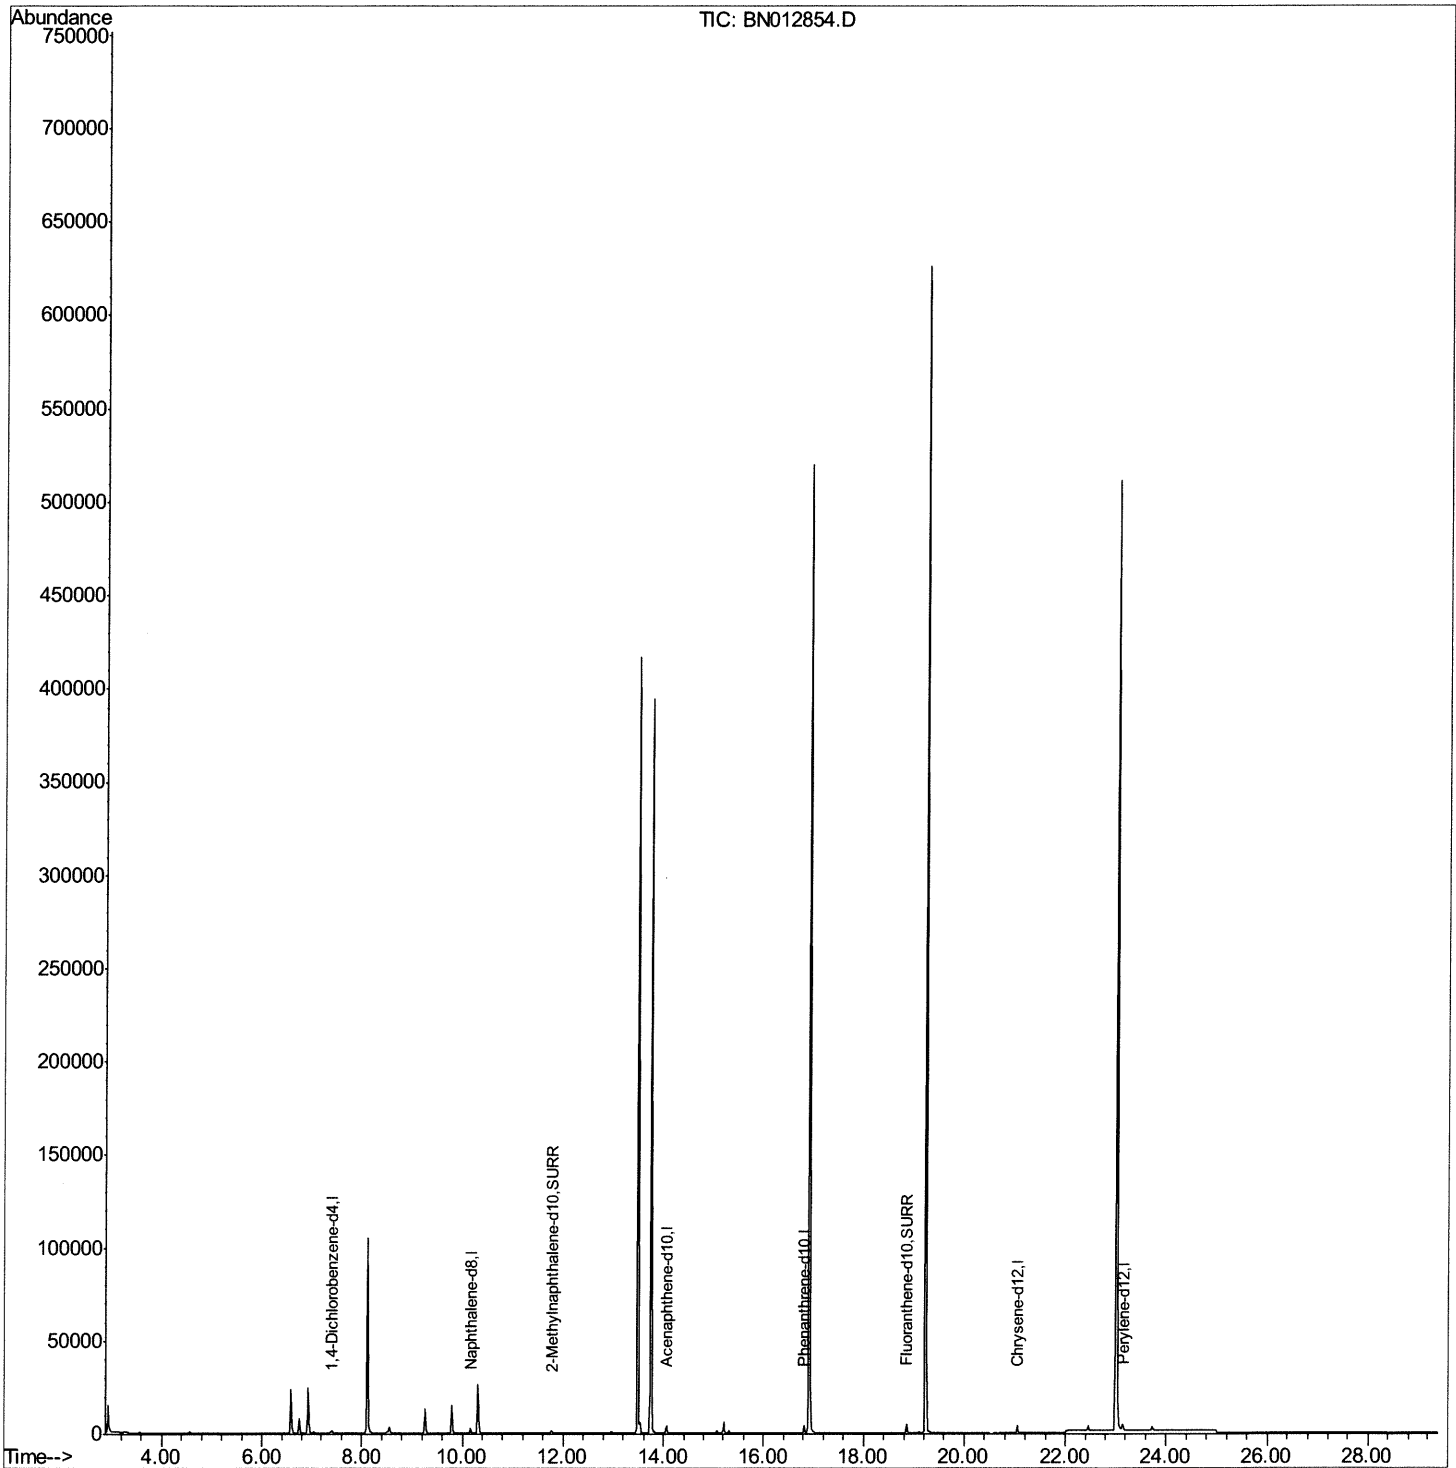

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120320\
 Data File : BN012854.D
 Acq On : 03 Dec 2020 19:32
 Operator : CG/JU
 Sample : L4866-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BE4

Manual Integrations
 APPROVED

mohammad
 12/7/2020 8:51:14 AM

Quant Time: Dec 04 00:18:28 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 04 00:14:34 2020
 Response via : Initial Calibration

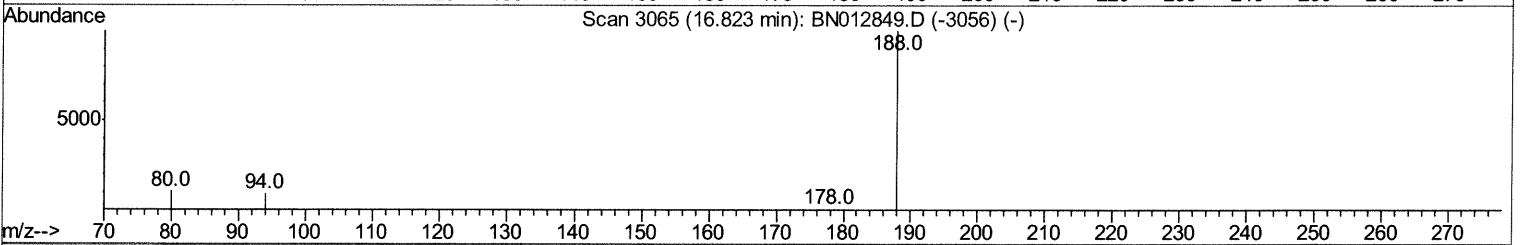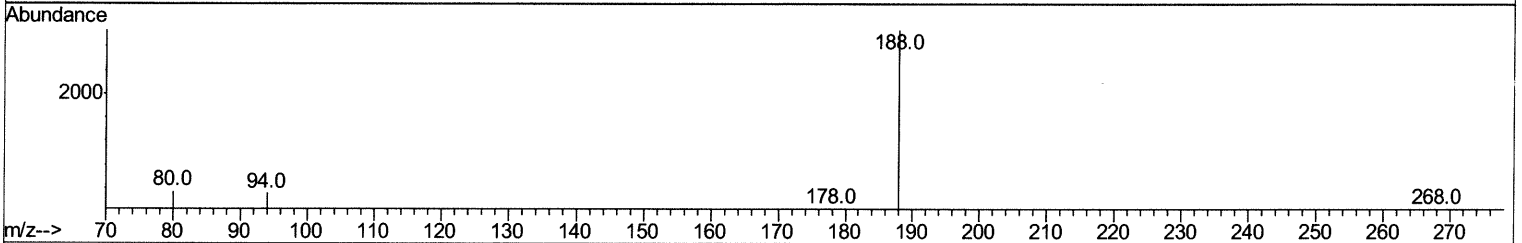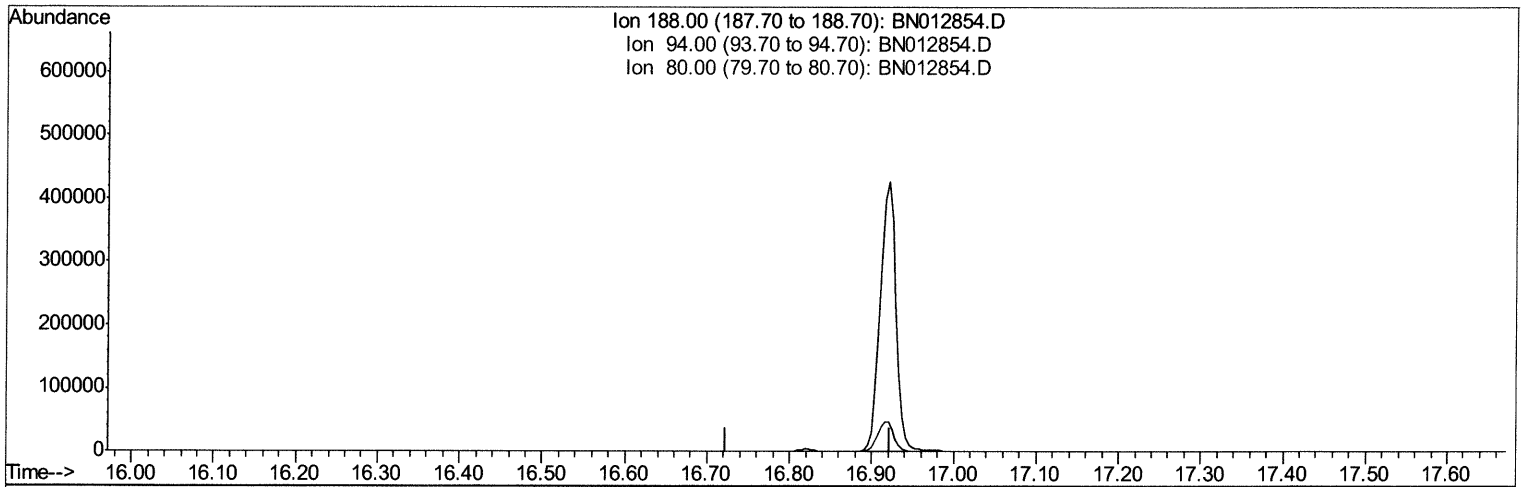

TIC: BN012854.D

(10) Phenanthrene-d10 (I)

16.823min (-16.823) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.40	0.00#
80.00	12.40	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120320\
 Data File : BN012854.D
 Acq On : 03 Dec 2020 19:32
 Operator : CG/JU
 Sample : L4866-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BE4

Manual Integrations
 APPROVED

mohammad
 12/7/2020 8:51:14 AM

Quant Time: Dec 04 00:18:28 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 04 00:14:34 2020
 Response via : Initial Calibration

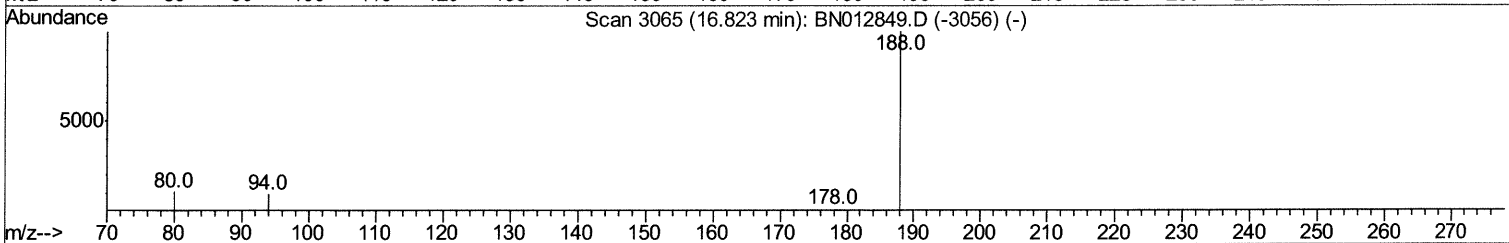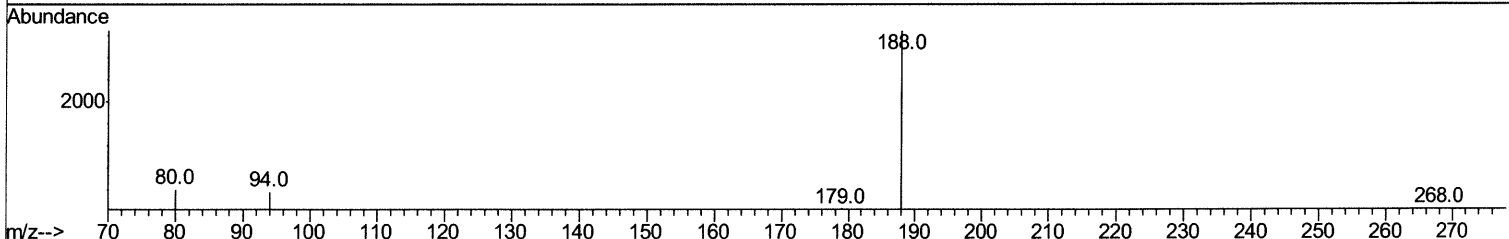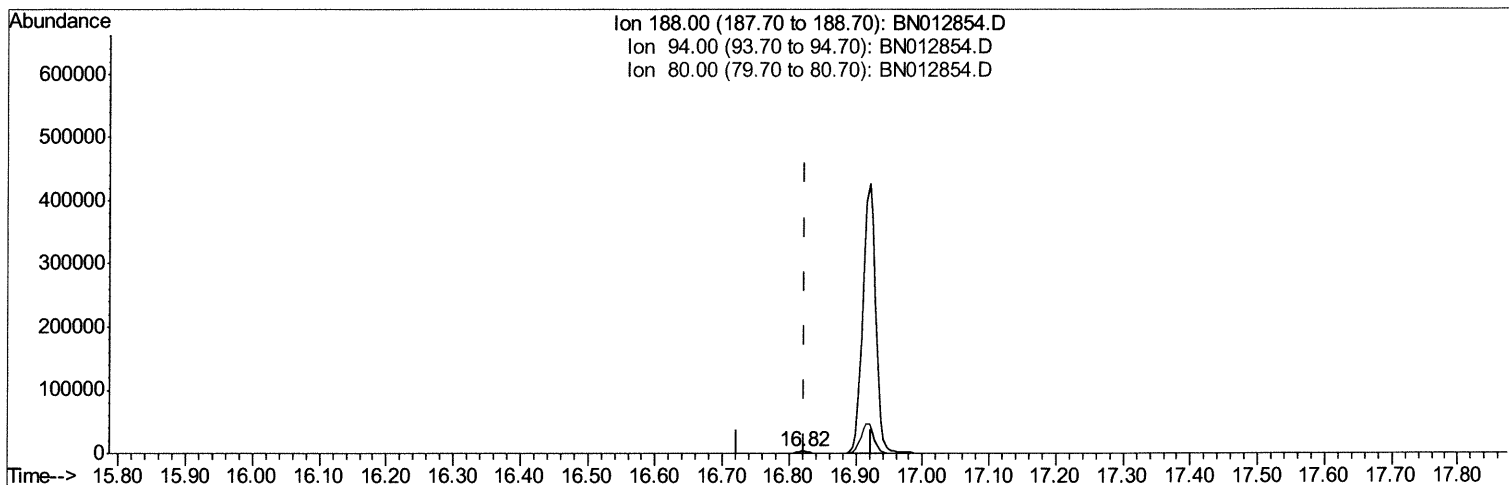

TIC: BN012854.D

(10) Phenanthrene-d10 (I)

16.819min (-0.004) 0.40ng/ul m 12/07/20 54

response 4492

Ion	Exp%	Act%
188.00	100	100
94.00	11.40	10.83
80.00	12.40	12.53
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120320\
 Data File : BN012854.D
 Acq On : 03 Dec 2020 19:32
 Operator : CG/JU
 Sample : L4866-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BE4

Manual Integrations
 APPROVED

mohammad
 12/7/2020 8:51:14 AM

Quant Time: Dec 04 00:29:15 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 04 00:14:34 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	810	0.40	ng/ul	0.00
2) Naphthalene-d8	10.16	136	3301	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.06	164	2124	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.82	188	4492m>	0.40	ng/ul>	0.00
16) Chrysene-d12	21.04	240	3817	0.40	ng/ul	0.00
20) Perylene-d12	23.15	264	4313	0.40	ng/ul	0.00

12/07/2020

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev (Min)
4) 2-Methylnaphthalene-d10	11.77	152	2219	0.45	ng/ul	0.00
14) Fluoranthene-d10	18.86	212	5240	0.43	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed