

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120522\
 Data File : BN023062.D
 Acq On : 05 Dec 2022 16:38
 Operator : CG/JU
 Sample : SSTDICC3.2
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Quant Time: Dec 06 03:40:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 06 03:35:07 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.049	152	3846	0.400	ng	0.00
7) Naphthalene-d8	10.872	136	11098	0.400	ng	# 0.01
13) Acenaphthene-d10	14.688	164	6789	0.400	ng	0.00
19) Phenanthrene-d10	17.427	188	14901	0.400	ng	0.00
29) Chrysene-d12	21.616	240	15227	0.400	ng	0.00
35) Perylene-d12	24.097	264	11589	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.587	112	26731	2.675	ng	0.00
5) Phenol-d6	7.197	99	37034	2.909	ng	0.00
8) Nitrobenzene-d5	9.206	82	27981	3.246	ng	0.00
11) 2-Methylnaphthalene-d10	12.450	152	85614	3.557	ng	0.00
14) 2,4,6-Tribromophenol	16.173	330	10335	3.153	ng	0.00
15) 2-Fluorobiphenyl	13.319	172	100274	3.229	ng	0.00
27) Fluoranthene-d10	19.460	212	150371	3.715	ng	0.00
31) Terphenyl-d14	20.058	244	98812	2.762	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.427	88	14547	2.980	ng	99
3) n-Nitrosodimethylamine	3.752	42	17201	3.269	ng	# 95
6) bis(2-Chloroethyl)ether	7.464	93	39677	3.319	ng	99
9) Naphthalene	10.915	128	112169	3.282	ng	98
10) Hexachlorobutadiene	11.203	225	20525	2.925	ng	# 100
12) 2-Methylnaphthalene	12.140	142	22056	3.162	ng	# 87
16) Acenaphthylene	14.410	152	121484	3.380	ng	100
17) Acenaphthene	14.752	154	81779	3.458	ng	98
18) Fluorene	15.726	166	101393	3.347	ng	98
20) 4,6-Dinitro-2-methylph...	15.801	198	8944	5.370	ng	# 80
21) 4-Bromophenyl-phenylether	16.620	248	33003	3.068	ng	97
22) Hexachlorobenzene	16.744	284	40288	3.068	ng	99
23) Atrazine	16.893	200	23188	3.057	ng	# 87
24) Pentachlorophenol	17.079	266	13164	3.662	ng	100
25) Phenanthrene	17.476	178	174967	3.377	ng	99
26) Anthracene	17.563	178	155026	3.447	ng	100
28) Fluoranthene	19.490	202	207860	3.773	ng	99
30) Pyrene	19.852	202	211709	2.671	ng	99
32) Benzo(a)anthracene	21.598	228	193195	3.140	ng	99
33) Chrysene	21.652	228	206511	3.236	ng	100
34) Bis(2-ethylhexyl)phtha...	21.527	149	74129	3.000	ng	# 98
36) Indeno(1,2,3-cd)pyrene	26.693	276	228734	4.757	ng	100
37) Benzo(b)fluoranthene	23.340	252	186889	3.613	ng	# 93
38) Benzo(k)fluoranthene	23.387	252	194703	3.475	ng	# 92
39) Benzo(a)pyrene	23.989	252	151077	3.826	ng	# 88
40) Dibenzo(a,h)anthracene	26.711	278	183681	4.810	ng	96
41) Benzo(g,h,i)perylene	27.491	276	190461	4.629	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120522\
 Data File : BN023062.D
 Acq On : 05 Dec 2022 16:38
 Operator : CG/JU
 Sample : SSTDICC3.2
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Quant Time: Dec 06 03:40:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 06 03:35:07 2022
 Response via : Initial Calibration









#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 8.049 min Scan# 688
 Delta R.T. 0.000 min
 Lab File: BN023062.D
 Acq: 05 Dec 2022 16:38




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2


Tgt Ion:152 Resp: 3846
 Ion Ratio Lower Upper
 152 100
 150 155.0 122.3 183.5
 115 61.1 48.6 72.8



#2
 1,4-Dioxane
 Concen: 2.980 ng
 RT: 3.427 min Scan# 48
 Delta R.T. 0.000 min
 Lab File: BN023062.D
 Acq: 05 Dec 2022 16:38

Tgt Ion: 88 Resp: 14547
 Ion Ratio Lower Upper
 88 100
 43 30.8 25.4 38.2
 58 71.7 58.2 87.4









#3
 n-Nitrosodimethylamine
 Concen: 3.269 ng
 RT: 3.752 min Scan# 91
 Delta R.T. -0.007 min
 Lab File: BN023062.D
 Acq: 05 Dec 2022 16:38




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2


Tgt Ion: 42 Resp: 17201
 Ion Ratio Lower Upper
 42 100
 74 113.5 87.4 131.0
 44 7.3 10.4 15.6#



#4
 2-Fluorophenol
 Concen: 2.675 ng
 RT: 5.587 min Scan# 347
 Delta R.T. 0.007 min
 Lab File: BN023062.D
 Acq: 05 Dec 2022 16:38

Tgt Ion: 112 Resp: 26731
 Ion Ratio Lower Upper
 112 100
 64 57.4 46.2 69.4
 63 31.6 25.1 37.7









#5
Phenol-d6
Concen: 2.909 ng
RT: 7.197 min Scan# 51
Delta R.T. -0.000 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion: 99 Resp: 37034
Ion Ratio Lower Upper
99 100
42 22.1 18.1 27.1
71 34.7 28.2 42.2



#6
bis(2-Chloroethyl)ether
Concen: 3.319 ng
RT: 7.464 min Scan# 607
Delta R.T. -0.000 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38

Tgt Ion: 93 Resp: 39677
Ion Ratio Lower Upper
93 100
63 76.1 61.4 92.2
95 32.1 25.9 38.9









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.872 min Scan# 90
Delta R.T. 0.011 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:	136	Resp:	11098
Ion	Ratio	Lower	Upper
136	100		
137	11.5	9.4	14.2
54	6.9	8.8	13.2#
68	5.6	7.0	10.6#



#8
Nitrobenzene-d5
Concen: 3.246 ng
RT: 9.206 min Scan# 808
Delta R.T. -0.000 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38

Tgt Ion:	82	Resp:	27981
Ion	Ratio	Lower	Upper
82	100		
128	34.7	29.9	44.9
54	53.9	44.2	66.2





#9

Naphthalene

Concen: 3.282 ng

RT: 10.915 min Scan# 9

Delta R.T. -0.000 min

Lab File: BN023062.D

Acq: 05 Dec 2022 16:38

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:128 Resp: 112169

Ion Ratio Lower Upper

128 100

129 10.9 9.2 13.8

127 13.0 10.9 16.3



#10

Hexachlorobutadiene

Concen: 2.925 ng

RT: 11.203 min Scan# 995

Delta R.T. -0.000 min

Lab File: BN023062.D

Acq: 05 Dec 2022 16:38




Tgt Ion:225 Resp: 20525


Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 63.5 50.8 76.2









#11
2-Methylnaphthalene-d10
Concen: 3.557 ng
RT: 12.450 min Scan# 1190
Delta R.T. -0.000 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:152 Resp: 85614
Ion Ratio Lower Upper
152 100
151 19.5 18.9 28.3



#12
2-Methylnaphthalene
Concen: 3.162 ng
RT: 12.140 min Scan# 1190
Delta R.T. -0.000 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38

Tgt Ion:142 Resp: 22056
Ion Ratio Lower Upper
142 100
141 11.1 12.3 18.5#
115 2.5 6.9 10.3#







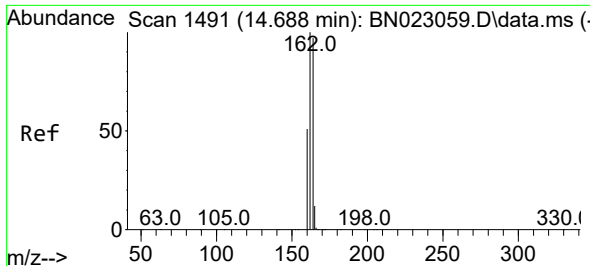

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.688 min Scan# 1491
Delta R.T. -0.000 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:164 Resp: 6789
Ion Ratio Lower Upper
164 100
162 103.0 82.7 124.1
160 53.0 42.6 63.8

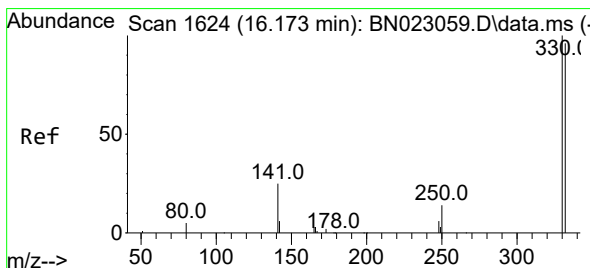

#14
2,4,6-Tribromophenol
Concen: 3.153 ng
RT: 16.173 min Scan# 1624
Delta R.T. -0.000 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38

Tgt Ion:330 Resp: 10335
Ion Ratio Lower Upper
330 100
332 96.3 77.1 115.7
141 41.8 36.7 55.1









#15
2-Fluorobiphenyl
Concen: 3.229 ng
RT: 13.319 min Scan# 1363
Delta R.T. -0.000 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:172 Resp: 100274
Ion Ratio Lower Upper
172 100
171 33.6 27.3 40.9
170 22.7 18.3 27.5



#16
Acenaphthylene
Concen: 3.380 ng
RT: 14.410 min Scan# 1465
Delta R.T. -0.000 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38

Tgt Ion:152 Resp: 121484
Ion Ratio Lower Upper
152 100
151 19.4 15.7 23.5
153 12.9 10.4 15.6









#17
Acenaphthene
Concen: 3.458 ng
RT: 14.752 min Scan# 1497
Delta R.T. -0.000 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:154 Resp: 81779
Ion Ratio Lower Upper
154 100
153 109.1 88.2 132.4
152 57.1 48.2 72.2



#18
Fluorene
Concen: 3.347 ng
RT: 15.726 min Scan# 1588
Delta R.T. -0.000 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38

Tgt Ion:166 Resp: 101393
Ion Ratio Lower Upper
166 100
165 100.9 82.2 123.4
167 13.3 11.4 17.0









#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.427 min Scan# 1725
Delta R.T. -0.000 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:188 Resp: 14901
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 17.1 13.3 19.9



#20
4,6-Dinitro-2-methylphenol
Concen: 5.370 ng
RT: 15.801 min Scan# 1594
Delta R.T. -0.000 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38

Tgt Ion:198 Resp: 8944
Ion Ratio Lower Upper
198 100
51 42.7 51.8 77.6#
105 44.5 40.7 61.1









#21
4-Bromophenyl-phenylether
Concen: 3.068 ng
RT: 16.620 min Scan# 1660
Delta R.T. -0.000 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:248 Resp: 33003
Ion Ratio Lower Upper
248 100
250 93.9 75.8 113.6
141 72.2 54.3 81.5



#22
Hexachlorobenzene
Concen: 3.068 ng
RT: 16.744 min Scan# 1670
Delta R.T. -0.000 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38

Tgt Ion:284 Resp: 40288
Ion Ratio Lower Upper
284 100
142 39.7 32.6 48.8
249 30.5 24.7 37.1





#23

Atrazine

Concen: 3.057 ng

RT: 16.893 min Scan# 1

Delta R.T. 0.012 min

Lab File: BN023062.D

Acq: 05 Dec 2022 16:38

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:200 Resp: 23188

Ion Ratio Lower Upper

200 100

173 20.0 28.4 42.6#

215 47.4 36.6 55.0



#24

Pentachlorophenol

Concen: 3.662 ng

RT: 17.079 min Scan# 1697

Delta R.T. -0.000 min

Lab File: BN023062.D

Acq: 05 Dec 2022 16:38




Tgt Ion:266 Resp: 13164


Ion Ratio Lower Upper

266 100

264 62.3 49.6 74.4

268 63.3 50.8 76.2









#25
Phenanthrene
Concen: 3.377 ng
RT: 17.476 min Scan# 1729
Delta R.T. -0.000 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:178 Resp: 174967
Ion Ratio Lower Upper
178 100
176 19.3 15.3 22.9
179 15.1 12.4 18.6



#26
Anthracene
Concen: 3.447 ng
RT: 17.563 min Scan# 1736
Delta R.T. -0.000 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38

Tgt Ion:178 Resp: 155026
Ion Ratio Lower Upper
178 100
176 18.6 15.0 22.4
179 15.2 12.4 18.6









#27
Fluoranthene-d10
Concen: 3.715 ng
RT: 19.460 min Scan# 2116
Delta R.T. -0.000 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:212 Resp: 150371
Ion Ratio Lower Upper
212 100
106 16.5 13.3 19.9
104 9.4 7.7 11.5



#28
Fluoranthene
Concen: 3.773 ng
RT: 19.490 min Scan# 2123
Delta R.T. -0.000 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38

Tgt Ion:202 Resp: 207860
Ion Ratio Lower Upper
202 100
101 12.7 10.5 15.7
203 17.3 13.8 20.6









#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.616 min Scan# 2425
Delta R.T. -0.000 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:240 Resp: 15227
Ion Ratio Lower Upper
240 100
120 17.3 14.2 21.4
236 28.2 22.8 34.2



#30
Pyrene
Concen: 2.671 ng
RT: 19.852 min Scan# 2209
Delta R.T. -0.000 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38

Tgt Ion:202 Resp: 211709
Ion Ratio Lower Upper
202 100
200 20.5 16.7 25.1
203 17.3 14.3 21.5



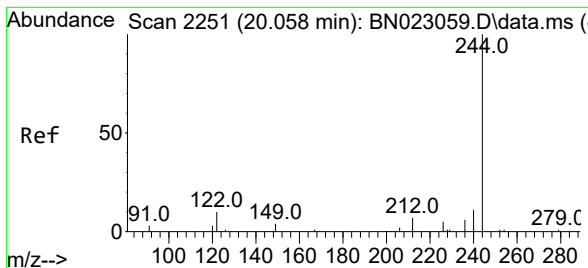

#31

Terphenyl-d14

Concen: 2.762 ng

RT: 20.058 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN023062.D

Acq: 05 Dec 2022 16:38

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:244 Resp: 98812

Ion Ratio Lower Upper

244 100

212 7.3 6.2 9.2

122 8.9 7.7 11.5

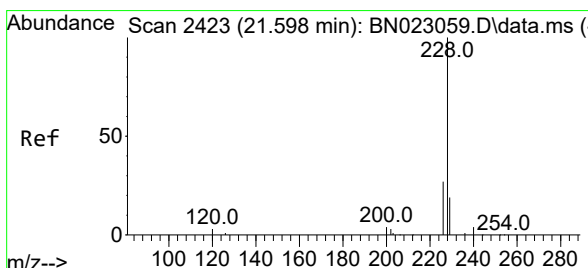

#32

Benzo(a)anthracene

Concen: 3.140 ng

RT: 21.598 min Scan# 2423

Delta R.T. -0.000 min

Lab File: BN023062.D

Acq: 05 Dec 2022 16:38




Tgt Ion:228 Resp: 193195


Ion Ratio Lower Upper

228 100

226 28.2 22.2 33.4

229 19.3 15.7 23.5



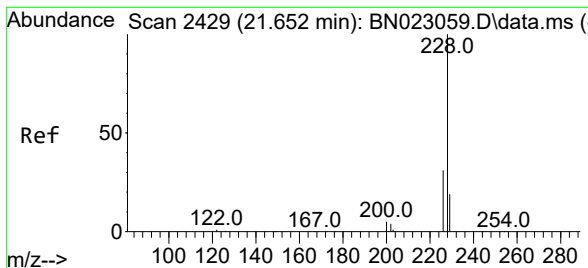

#33

Chrysene

Concen: 3.236 ng

RT: 21.652 min Scan# 2429

Delta R.T. -0.000 min

Lab File: BN023062.D

Acq: 05 Dec 2022 16:38

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:228 Resp: 206511

Ion Ratio Lower Upper

228 100

226 31.1 25.0 37.6

229 19.3 15.4 23.0

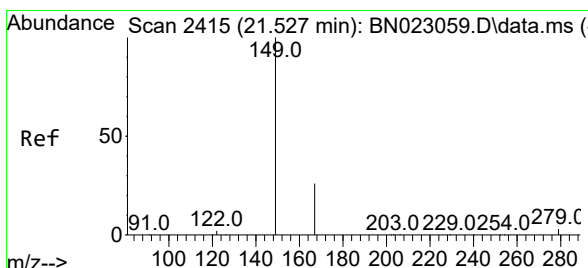

#34

Bis(2-ethylhexyl)phthalate

Concen: 3.000 ng

RT: 21.527 min Scan# 2415

Delta R.T. -0.000 min

Lab File: BN023062.D

Acq: 05 Dec 2022 16:38




Tgt Ion:149 Resp: 74129


Ion Ratio Lower Upper

149 100

167 25.5 19.5 29.3


279 2.5 2.6 4.0#








#35
Perylene-d12
Concen: 0.400 ng
RT: 24.097 min Scan# 3092
Delta R.T. -0.000 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2







Tgt Ion:264 Resp: 11589
Ion Ratio Lower Upper
264 100
260 26.8 21.0 31.4
265 54.9 45.0 67.6



#36
Indeno(1,2,3-cd)pyrene
Concen: 4.757 ng
RT: 26.693 min Scan# 3980
Delta R.T. -0.000 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38

Tgt Ion:276 Resp: 228734
Ion Ratio Lower Upper
276 100
138 30.3 24.4 36.6
277 24.8 19.8 29.8









#37
Benzo(b)fluoranthene
Concen: 3.613 ng
RT: 23.340 min Scan# 2833
Delta R.T. -0.000 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:252 Resp: 186889
Ion Ratio Lower Upper
252 100
253 21.7 19.5 29.3
125 12.3 13.4 20.2#



#38
Benzo(k)fluoranthene
Concen: 3.475 ng
RT: 23.387 min Scan# 2849
Delta R.T. -0.003 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38

Tgt Ion:252 Resp: 194703
Ion Ratio Lower Upper
252 100
253 21.5 19.4 29.2
125 12.3 13.5 20.3#





#39

Benzo(a)pyrene

Concen: 3.826 ng

RT: 23.989 min Scan# 3055

Delta R.T. 0.003 min

Lab File: BN023062.D

Acq: 05 Dec 2022 16:38

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:252 Resp: 151077

Ion Ratio Lower Upper

252 100

253 21.7 20.7 31.1

125 13.8 17.1 25.7#



#40

Dibenzo(a,h)anthracene

Concen: 4.810 ng

RT: 26.711 min Scan# 3986

Delta R.T. -0.006 min

Lab File: BN023062.D

Acq: 05 Dec 2022 16:38




Tgt Ion:278 Resp: 183681


Ion Ratio Lower Upper

278 100

139 20.3 17.2 25.8


279 23.3 20.6 31.0



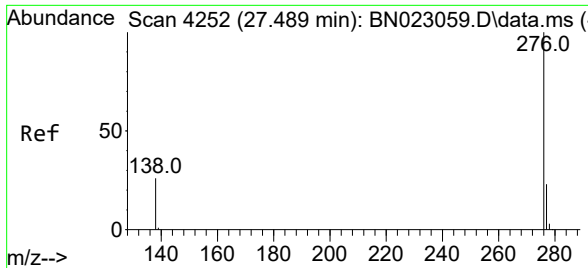

#41
Benzo(g,h,i)perylene
Concen: 4.629 ng
RT: 27.491 min Scan# 41
Delta R.T. 0.003 min
Lab File: BN023062.D
Acq: 05 Dec 2022 16:38

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2



Tgt Ion:276 Resp: 190461
Ion Ratio Lower Upper
276 100
277 23.7 19.7 29.5
138 26.1 22.2 33.4

