

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120522\
 Data File : BN023063.D
 Acq On : 05 Dec 2022 17:15
 Operator : CG/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Quant Time: Dec 06 03:40:48 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 06 03:35:07 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.049	152	4289	0.400	ng	0.00
7) Naphthalene-d8	10.872	136	11691	0.400	ng	# 0.01
13) Acenaphthene-d10	14.688	164	7173	0.400	ng	0.00
19) Phenanthrene-d10	17.439	188	15480	0.400	ng	# 0.01
29) Chrysene-d12	21.616	240	16045	0.400	ng	0.00
35) Perylene-d12	24.097	264	12453	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.587	112	46097	4.136	ng	0.00
5) Phenol-d6	7.197	99	63921	4.503	ng	0.00
8) Nitrobenzene-d5	9.206	82	47429	5.222	ng	0.00
11) 2-Methylnaphthalene-d10	12.450	152	143761	5.669	ng	0.00
14) 2,4,6-Tribromophenol	16.173	330	17347	5.009	ng	0.00
15) 2-Fluorobiphenyl	13.319	172	161274	4.915	ng	0.00
27) Fluoranthene-d10	19.464	212	246763	5.869	ng	0.00
31) Terphenyl-d14	20.058	244	165571	4.393	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.427	88	24390	4.481	ng	98
3) n-Nitrosodimethylamine	3.752	42	29312	4.995	ng	# 92
6) bis(2-Chloroethyl)ether	7.464	93	64945	4.872	ng	100
9) Naphthalene	10.914	128	183910	5.108	ng	99
10) Hexachlorobutadiene	11.213	225	33143	4.484	ng	# 99
12) 2-Methylnaphthalene	12.144	142	38826	5.285	ng	# 86
16) Acenaphthylene	14.410	152	201047	5.294	ng	100
17) Acenaphthene	14.752	154	132843	5.317	ng	96
18) Fluorene	15.726	166	162944	5.092	ng	95
20) 4,6-Dinitro-2-methylph...	15.801	198	15296	8.841	ng	# 80
21) 4-Bromophenyl-phenylether	16.620	248	52635	4.710	ng	96
22) Hexachlorobenzene	16.744	284	62733	4.599	ng	100
23) Atrazine	16.893	200	38434	4.878	ng	# 87
24) Pentachlorophenol	17.079	266	22436	6.008	ng	99
25) Phenanthrene	17.476	178	280800	5.217	ng	100
26) Anthracene	17.563	178	253998	5.437	ng	100
28) Fluoranthene	19.494	202	331091	5.785	ng	99
30) Pyrene	19.856	202	344928	4.129	ng	99
32) Benzo(a)anthracene	21.598	228	319996	4.935	ng	100
33) Chrysene	21.652	228	332591	4.946	ng	99
34) Bis(2-ethylhexyl)phtha...	21.526	149	124209	4.770	ng	# 97
36) Indeno(1,2,3-cd)pyrene	26.690	276	381489	7.383	ng	99
37) Benzo(b)fluoranthene	23.340	252	308007	5.541	ng	# 93
38) Benzo(k)fluoranthene	23.387	252	317724	5.277	ng	# 92
39) Benzo(a)pyrene	23.986	252	256901	6.055	ng	# 88
40) Dibenzo(a,h)anthracene	26.714	278	302539	7.373	ng	96
41) Benzo(g,h,i)perylene	27.488	276	312020	7.057	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120522\
Data File : BN023063.D
Acq On : 05 Dec 2022 17:15
Operator : CG/JU
Sample : SSTDICC5.0
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Quant Time: Dec 06 03:40:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 06 03:35:07 2022
Response via : Initial Calibration

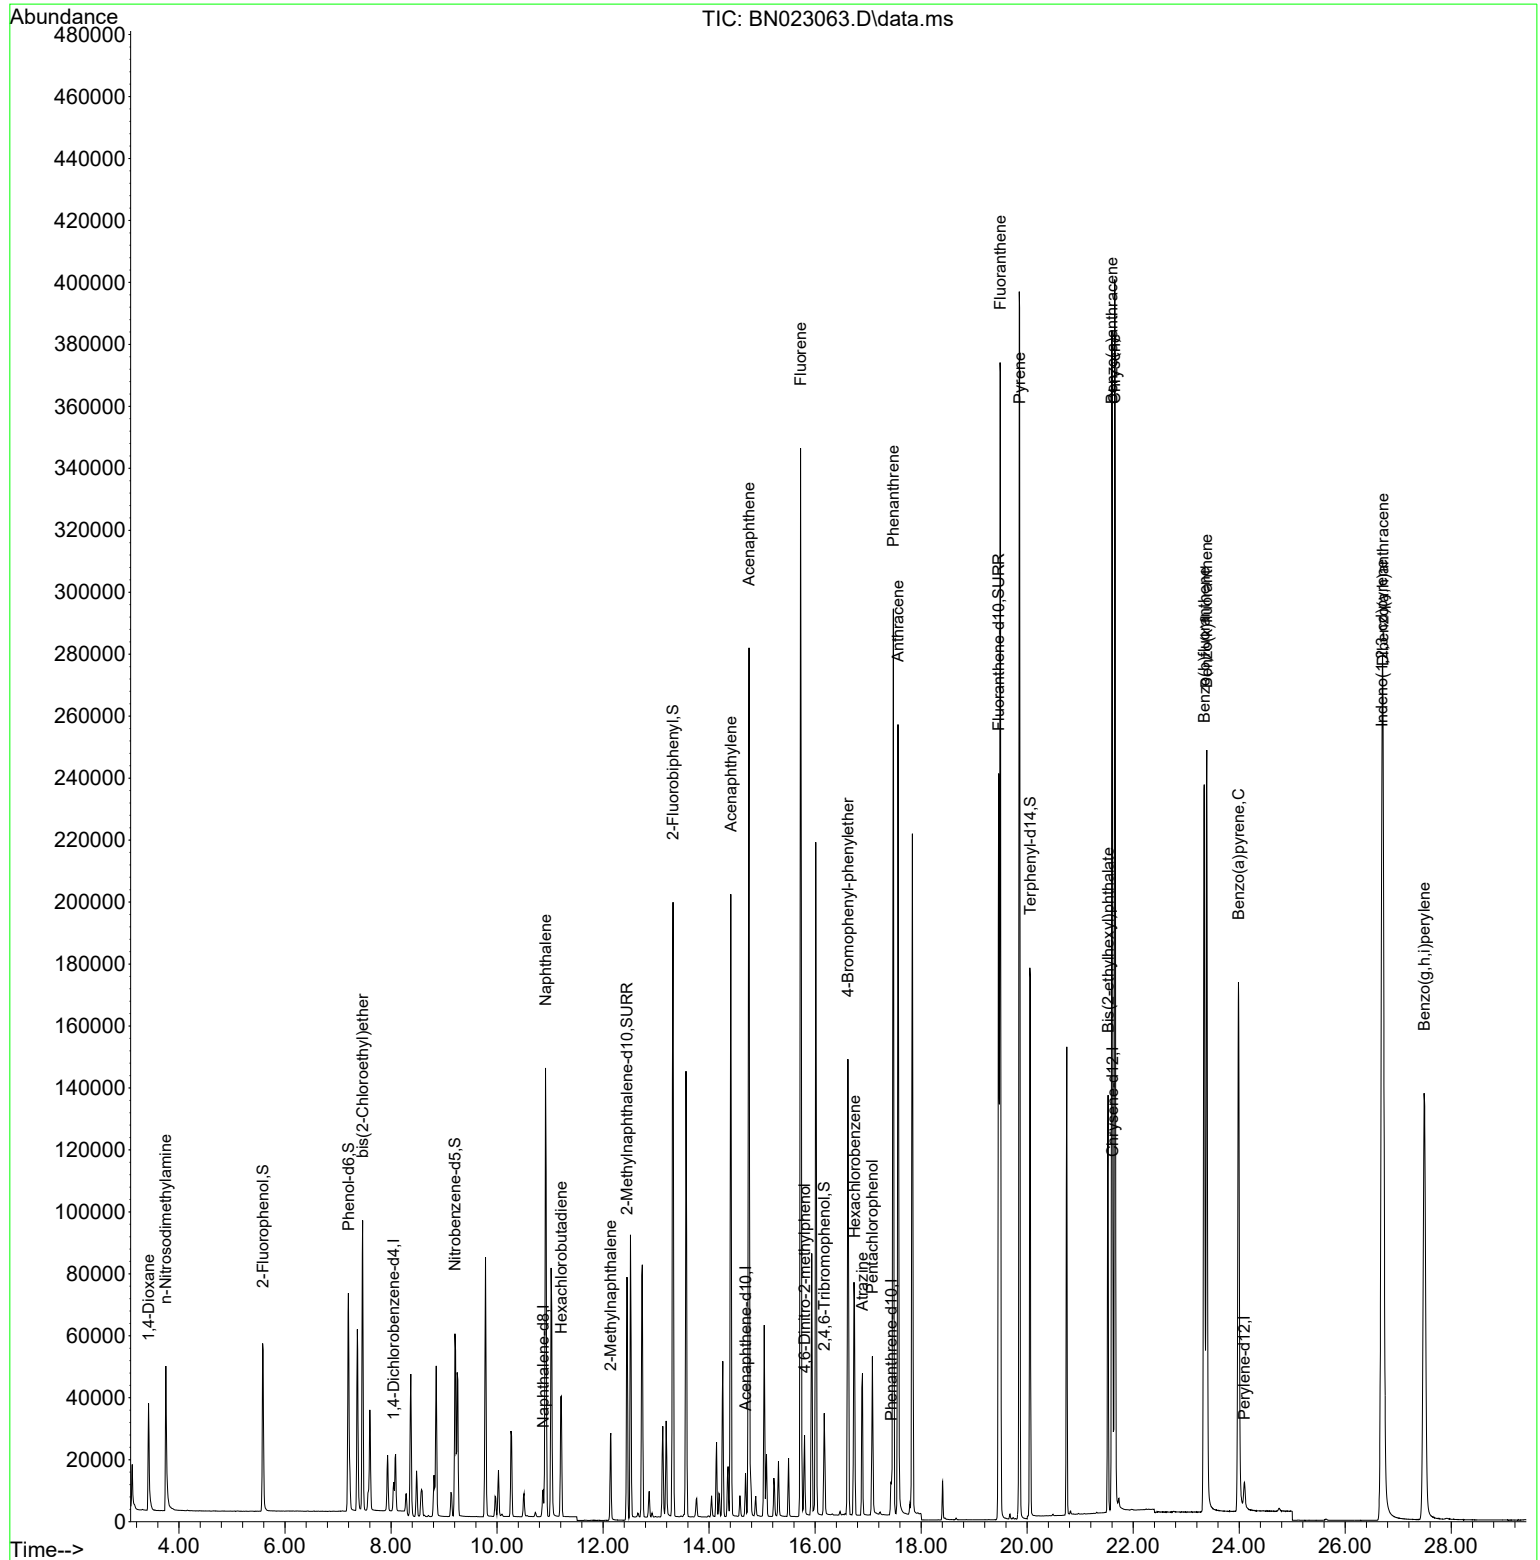






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 8.049 min Scan# 688
 Delta R.T. 0.000 min
 Lab File: BN023063.D
 Acq: 05 Dec 2022 17:15


Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

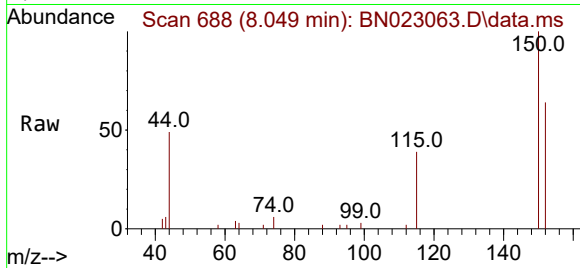



Tgt Ion:152 Resp: 4289
 Ion Ratio Lower Upper
 152 100
 150 155.2 122.3 183.5
 115 60.8 48.6 72.8

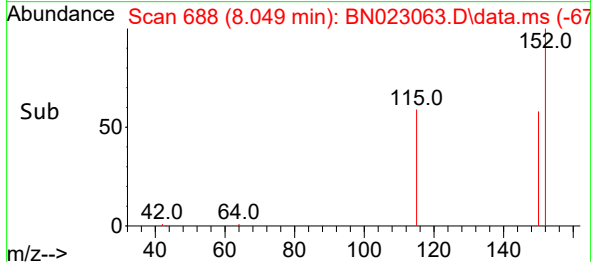


#2
 1,4-Dioxane
 Concen: 4.481 ng
 RT: 3.427 min Scan# 48
 Delta R.T. 0.000 min
 Lab File: BN023063.D
 Acq: 05 Dec 2022 17:15

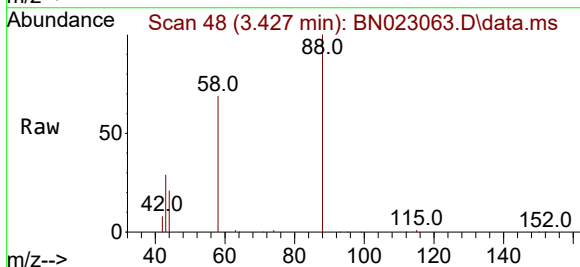

Tgt Ion: 88 Resp: 24390
 Ion Ratio Lower Upper
 88 100
 43 30.2 25.4 38.2
 58 71.6 58.2 87.4



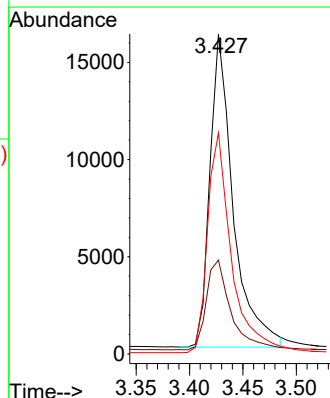
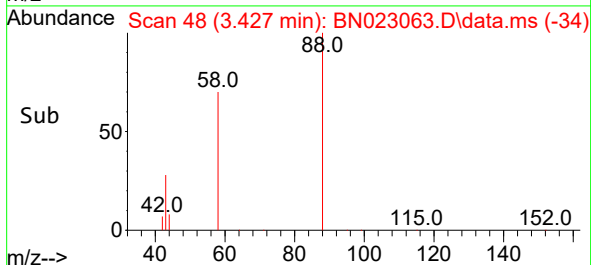




#3
n-Nitrosodimethylamine
Concen: 4.995 ng
RT: 3.752 min Scan# 91
Delta R.T. -0.007 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 42 Resp: 29312
Ion Ratio Lower Upper
42 100
74 117.2 87.4 131.0
44 7.3 10.4 15.6#

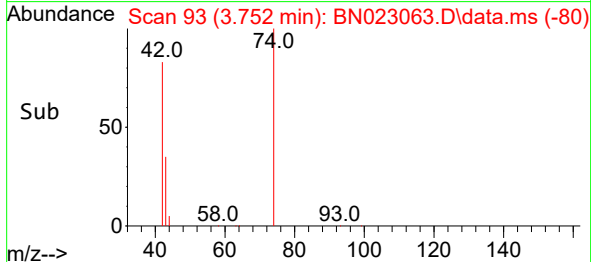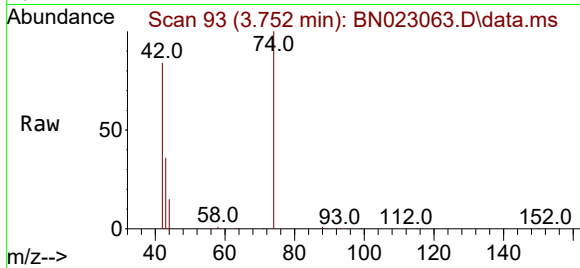

#4
2-Fluorophenol
Concen: 4.136 ng
RT: 5.587 min Scan# 347
Delta R.T. 0.007 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15

Tgt Ion: 112 Resp: 46097
Ion Ratio Lower Upper
112 100
64 57.0 46.2 69.4
63 31.0 25.1 37.7




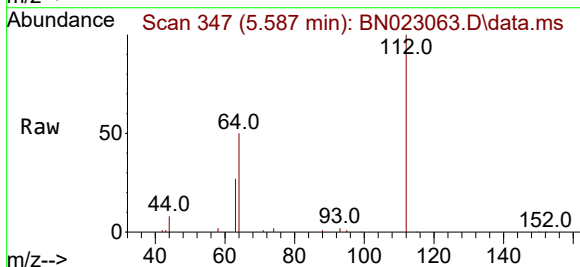




#5
Phenol-d6
Concen: 4.503 ng
RT: 7.197 min Scan# 51
Delta R.T. -0.000 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 99 Resp: 63921
Ion Ratio Lower Upper
99 100
42 21.5 18.1 27.1
71 34.3 28.2 42.2



#6
bis(2-Chloroethyl)ether
Concen: 4.872 ng
RT: 7.464 min Scan# 607
Delta R.T. -0.000 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15

Tgt Ion: 93 Resp: 64945
Ion Ratio Lower Upper
93 100
63 76.4 61.4 92.2
95 32.4 25.9 38.9









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.872 min Scan# 964
Delta R.T. 0.011 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	136	Resp:	11691
Ion Ratio	Lower	Upper	
136	100		
137	11.5	9.4	14.2
54	7.2	8.8	13.2#
68	6.1	7.0	10.6#

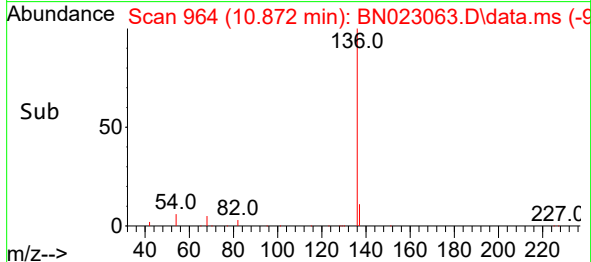

#8
Nitrobenzene-d5
Concen: 5.222 ng
RT: 9.206 min Scan# 808
Delta R.T. -0.000 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15

Tgt Ion:	82	Resp:	47429
Ion Ratio	Lower	Upper	
82	100		
128	34.1	29.9	44.9
54	54.8	44.2	66.2

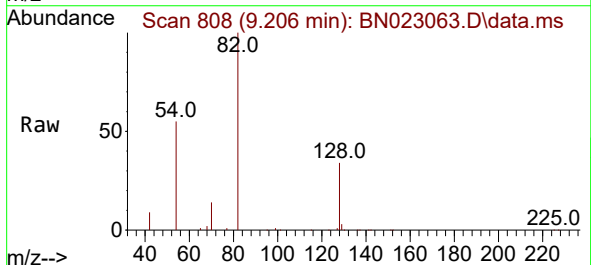



#9

Naphthalene

Concen: 5.108 ng

RT: 10.914 min Scan# 9

Delta R.T. -0.000 min

Lab File: BN023063.D

Acq: 05 Dec 2022 17:15

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:128 Resp: 183910

Ion Ratio Lower Upper

128 100

129 10.9 9.2 13.8

127 13.0 10.9 16.3



#10

Hexachlorobutadiene

Concen: 4.484 ng

RT: 11.213 min Scan# 996

Delta R.T. 0.011 min

Lab File: BN023063.D

Acq: 05 Dec 2022 17:15




Tgt Ion:225 Resp: 33143


Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 63.9 50.8 76.2









#11
2-Methylnaphthalene-d10
Concen: 5.669 ng
RT: 12.450 min Scan# 1191
Delta R.T. -0.000 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:152 Resp: 143761
Ion Ratio Lower Upper
152 100
151 20.8 18.9 28.3



#12
2-Methylnaphthalene
Concen: 5.285 ng
RT: 12.144 min Scan# 1191
Delta R.T. 0.004 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15

Tgt Ion:142 Resp: 38826
Ion Ratio Lower Upper
142 100
141 10.6 12.3 18.5#
115 2.2 6.9 10.3#







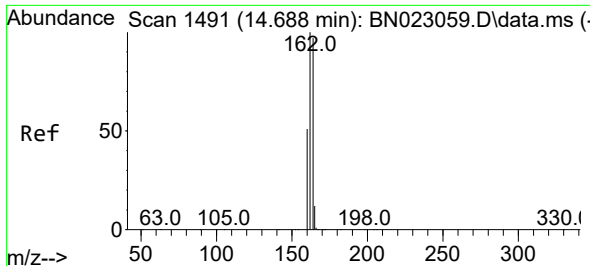

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.688 min Scan# 1491
Delta R.T. -0.000 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:164 Resp: 7173
Ion Ratio Lower Upper
164 100
162 102.6 82.7 124.1
160 50.9 42.6 63.8

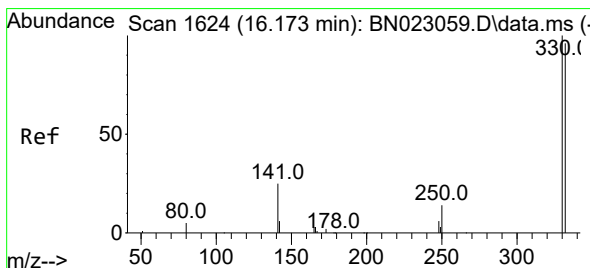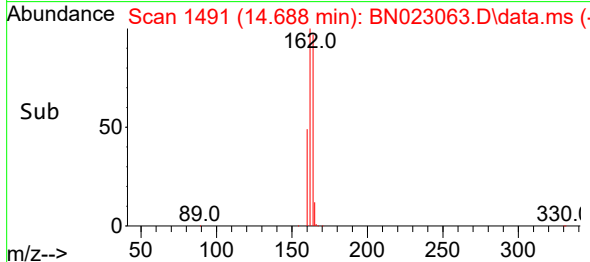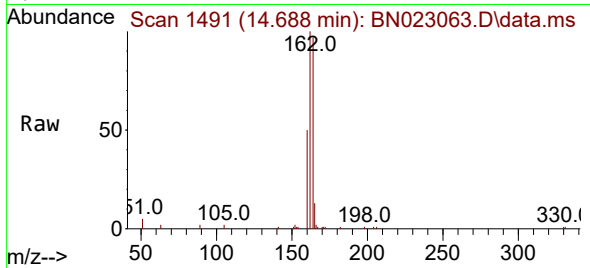

#14
2,4,6-Tribromophenol
Concen: 5.009 ng
RT: 16.173 min Scan# 1624
Delta R.T. -0.000 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15

Tgt Ion:330 Resp: 17347
Ion Ratio Lower Upper
330 100
332 95.8 77.1 115.7
141 41.4 36.7 55.1


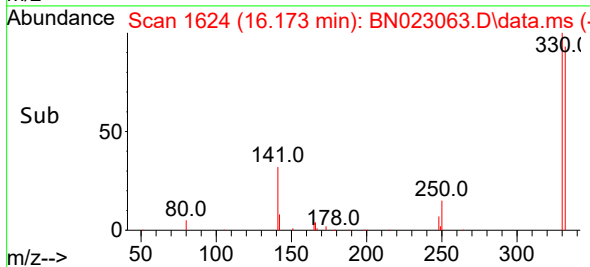

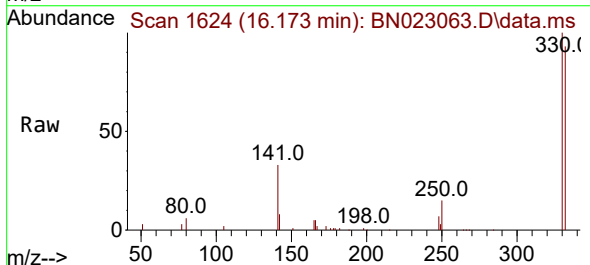




#15
2-Fluorobiphenyl
Concen: 4.915 ng
RT: 13.319 min Scan# 1363
Delta R.T. -0.000 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:172 Resp: 161274
Ion Ratio Lower Upper
172 100
171 33.9 27.3 40.9
170 22.5 18.3 27.5

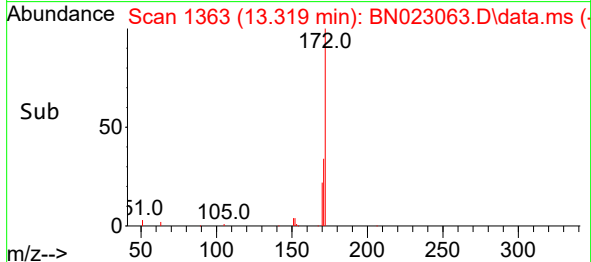

#16
Acenaphthylene
Concen: 5.294 ng
RT: 14.410 min Scan# 1465
Delta R.T. -0.000 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15

Tgt Ion:152 Resp: 201047
Ion Ratio Lower Upper
152 100
151 19.3 15.7 23.5
153 13.0 10.4 15.6




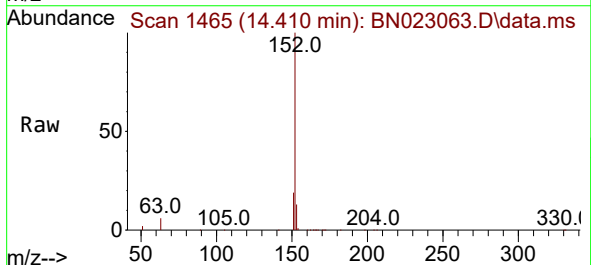




#17
Acenaphthene
Concen: 5.317 ng
RT: 14.752 min Scan# 1497
Delta R.T. -0.000 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:154 Resp: 132843
Ion Ratio Lower Upper
154 100
153 108.3 88.2 132.4
152 55.3 48.2 72.2



#18
Fluorene
Concen: 5.092 ng
RT: 15.726 min Scan# 1588
Delta R.T. -0.000 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15

Tgt Ion:166 Resp: 162944
Ion Ratio Lower Upper
166 100
165 97.9 82.2 123.4
167 13.2 11.4 17.0









#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.439 min Scan# 1726
Delta R.T. 0.012 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:188 Resp: 15480
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.3 13.3 19.9#



#20
4,6-Dinitro-2-methylphenol
Concen: 8.841 ng
RT: 15.801 min Scan# 1594
Delta R.T. -0.000 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15

Tgt Ion:198 Resp: 15296
Ion Ratio Lower Upper
198 100
51 42.2 51.8 77.6#
105 43.9 40.7 61.1









#21
4-Bromophenyl-phenylether
Concen: 4.710 ng
RT: 16.620 min Scan# 1660
Delta R.T. -0.000 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:248 Resp: 52635
Ion Ratio Lower Upper
248 100
250 93.8 75.8 113.6
141 75.1 54.3 81.5

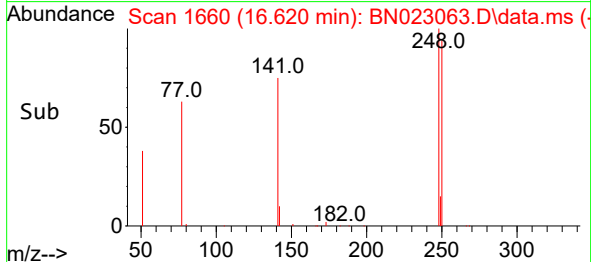

#22
Hexachlorobenzene
Concen: 4.599 ng
RT: 16.744 min Scan# 1670
Delta R.T. -0.000 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15

Tgt Ion:284 Resp: 62733
Ion Ratio Lower Upper
284 100
142 40.4 32.6 48.8
249 30.7 24.7 37.1

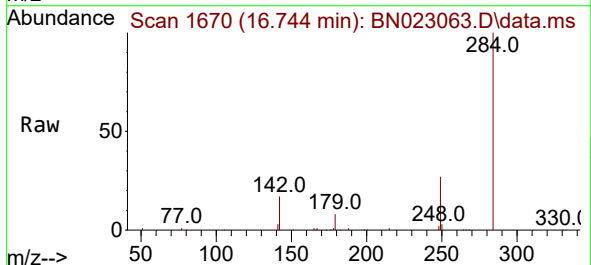



#23

Atrazine

Concen: 4.878 ng

RT: 16.893 min Scan# 1682

Delta R.T. 0.012 min

Lab File: BN023063.D

Acq: 05 Dec 2022 17:15

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:200 Resp: 38434

Ion Ratio Lower Upper

200 100

173 20.4 28.4 42.6#

215 47.3 36.6 55.0

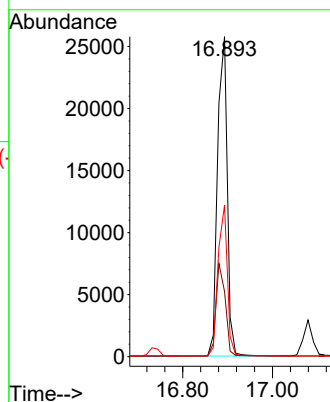

#24

Pentachlorophenol

Concen: 6.008 ng

RT: 17.079 min Scan# 1697

Delta R.T. -0.000 min

Lab File: BN023063.D

Acq: 05 Dec 2022 17:15




Tgt Ion:266 Resp: 22436


Ion Ratio Lower Upper

266 100

264 62.8 49.6 74.4

268 64.2 50.8 76.2



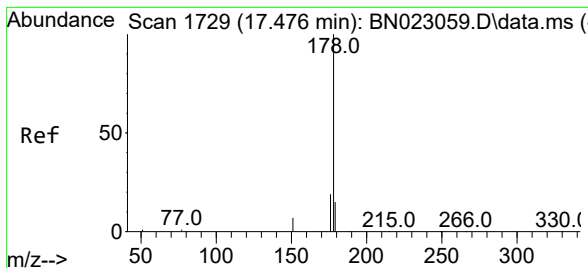

#25

Phenanthrene

Concen: 5.217 ng

RT: 17.476 min Scan# 1729

Delta R.T. -0.000 min

Lab File: BN023063.D

Acq: 05 Dec 2022 17:15

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:178 Resp: 280800

Ion Ratio Lower Upper

178 100

176 19.1 15.3 22.9

179 15.1 12.4 18.6

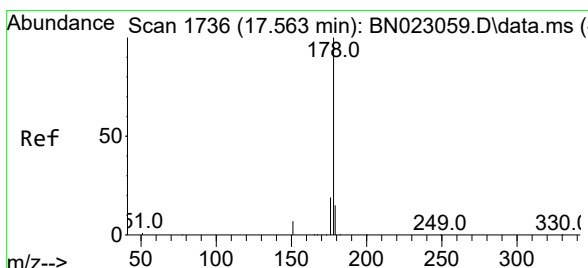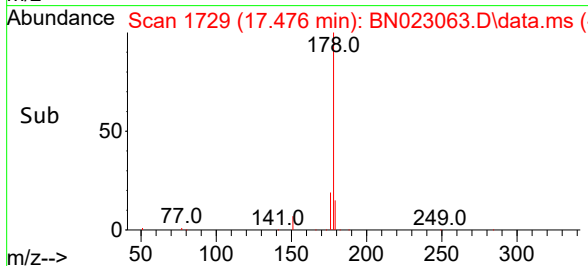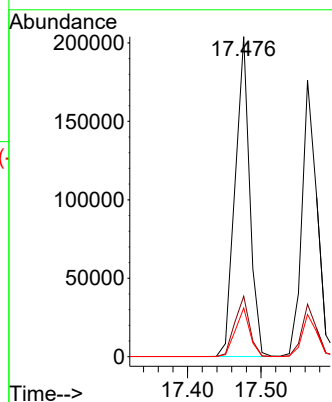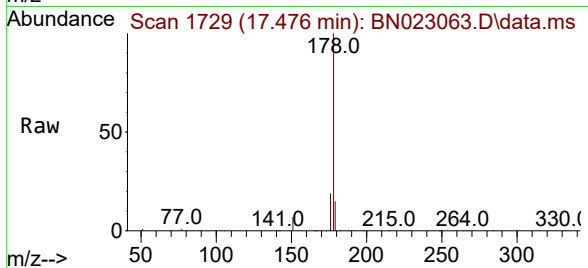

#26

Anthracene

Concen: 5.437 ng

RT: 17.563 min Scan# 1736

Delta R.T. -0.000 min

Lab File: BN023063.D

Acq: 05 Dec 2022 17:15




Tgt Ion:178 Resp: 253998


Ion Ratio Lower Upper

178 100

176 18.6 15.0 22.4

179 15.4 12.4 18.6


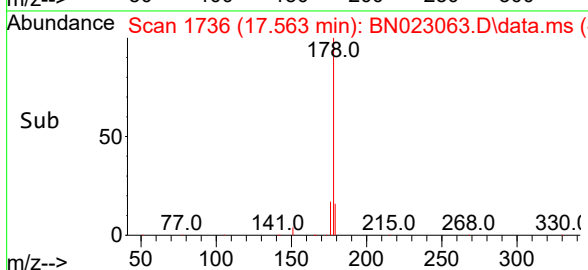

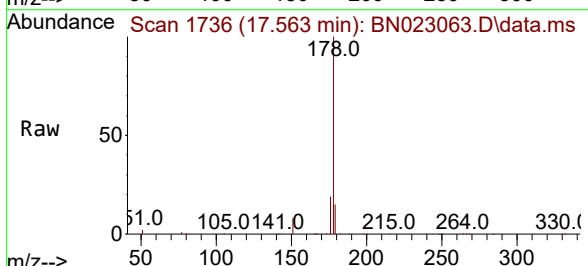




#27
Fluoranthene-d10
Concen: 5.869 ng
RT: 19.464 min Scan# 2116
Delta R.T. 0.004 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:212 Resp: 246763
Ion Ratio Lower Upper
212 100
106 16.3 13.3 19.9
104 9.2 7.7 11.5

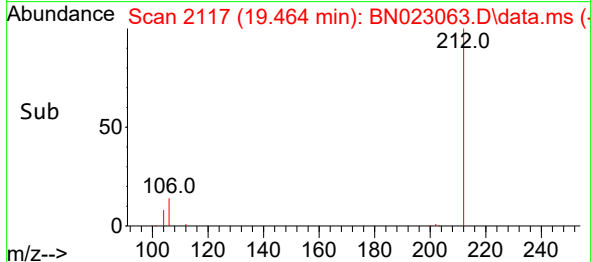

#28
Fluoranthene
Concen: 5.785 ng
RT: 19.494 min Scan# 2124
Delta R.T. 0.004 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15

Tgt Ion:202 Resp: 331091
Ion Ratio Lower Upper
202 100
101 12.6 10.5 15.7
203 17.2 13.8 20.6




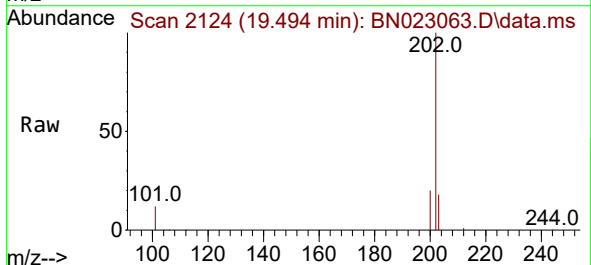




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.616 min Scan# 2425
Delta R.T. -0.000 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:240 Resp: 16045
Ion Ratio Lower Upper
240 100
120 16.3 14.2 21.4
236 28.1 22.8 34.2



#30
Pyrene
Concen: 4.129 ng
RT: 19.856 min Scan# 2210
Delta R.T. 0.004 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15

Tgt Ion:202 Resp: 344928
Ion Ratio Lower Upper
202 100
200 20.5 16.7 25.1
203 17.3 14.3 21.5



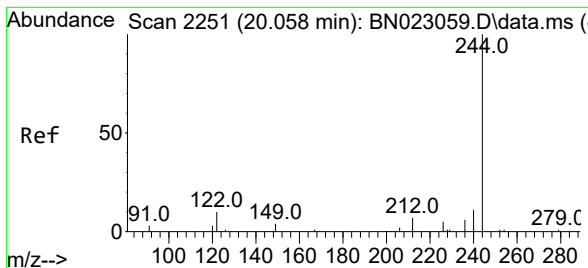

#31

Terphenyl-d14

Concen: 4.393 ng

RT: 20.058 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN023063.D

Acq: 05 Dec 2022 17:15

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:244 Resp: 165571

Ion Ratio Lower Upper

244 100

212 7.2 6.2 9.2

122 9.3 7.7 11.5

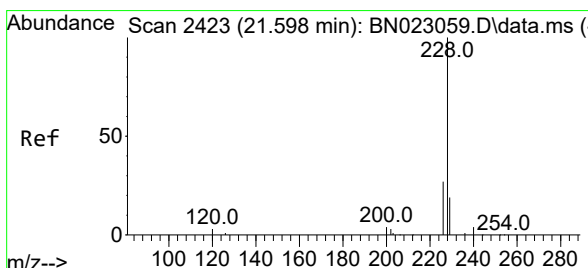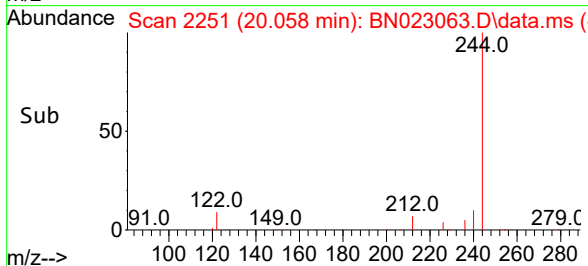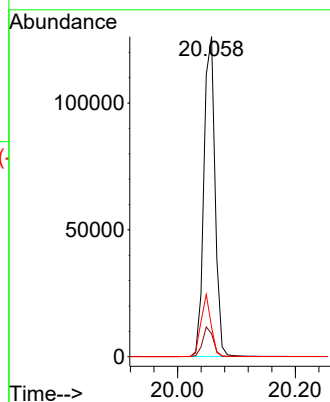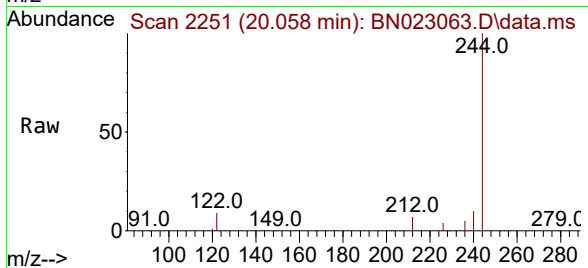

#32

Benzo(a)anthracene

Concen: 4.935 ng

RT: 21.598 min Scan# 2423

Delta R.T. -0.000 min

Lab File: BN023063.D

Acq: 05 Dec 2022 17:15




Tgt Ion:228 Resp: 319996


Ion Ratio Lower Upper

228 100

226 27.7 22.2 33.4

229 19.4 15.7 23.5


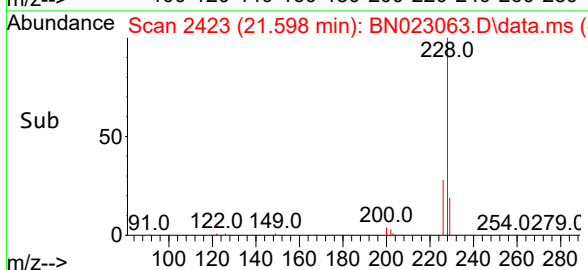

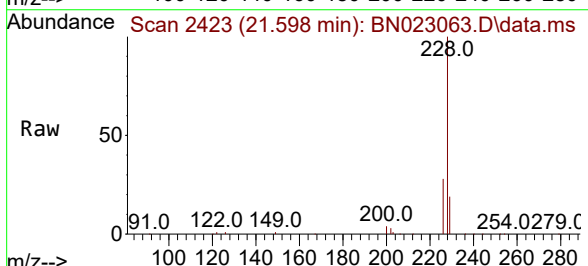


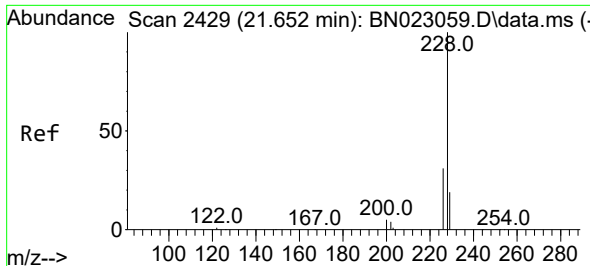

#33
Chrysene
Concen: 4.946 ng
RT: 21.652 min Scan# 2429
Delta R.T. -0.000 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:228 Resp: 332591
Ion Ratio Lower Upper
228 100
226 30.4 25.0 37.6
229 19.1 15.4 23.0

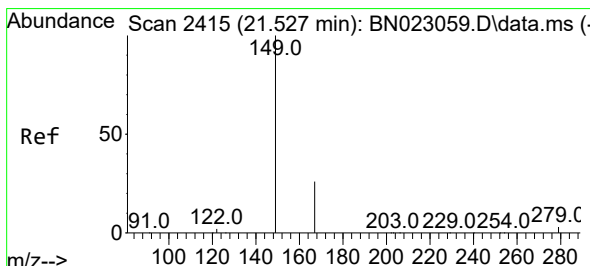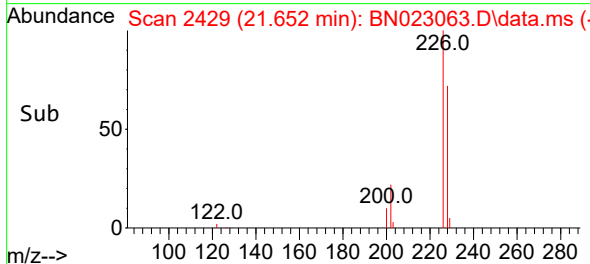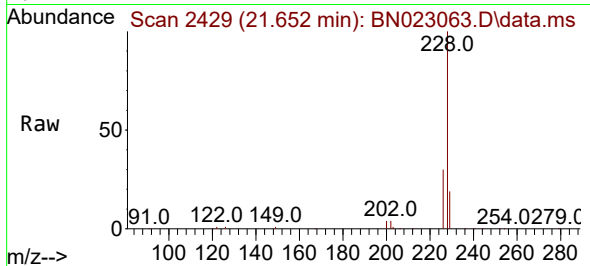

#34
Bis(2-ethylhexyl)phthalate
Concen: 4.770 ng
RT: 21.526 min Scan# 2415
Delta R.T. -0.000 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15

Tgt Ion:149 Resp: 124209
Ion Ratio Lower Upper
149 100
167 26.0 19.5 29.3
279 2.6 2.6 4.0#

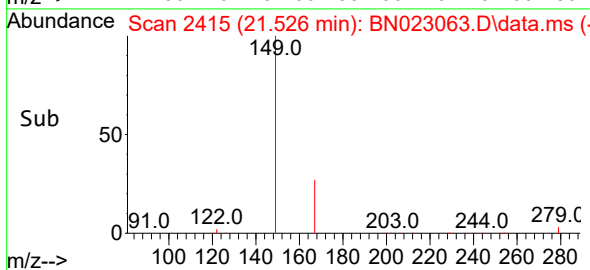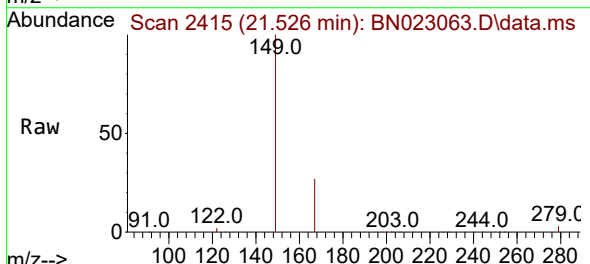



#35

Perylene-d12

Concen: 0.400 ng

RT: 24.097 min Scan# 3092

Delta R.T. -0.000 min

Lab File: BN023063.D


Acq: 05 Dec 2022 17:15

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0






Tgt Ion:264 Resp: 12453

Ion Ratio Lower Upper

264 100

260 26.4 21.0 31.4

265 56.0 45.0 67.6

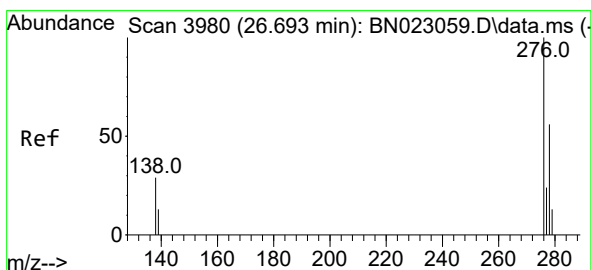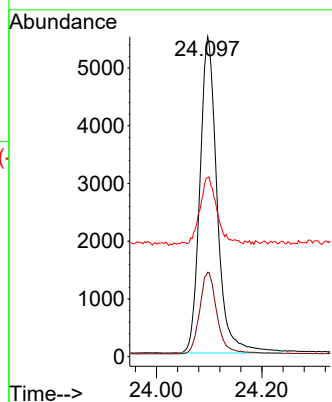

#36

Indeno(1,2,3-cd)pyrene

Concen: 7.383 ng

RT: 26.690 min Scan# 3979

Delta R.T. -0.003 min

Lab File: BN023063.D

Acq: 05 Dec 2022 17:15




Tgt Ion:276 Resp: 381489


Ion Ratio Lower Upper

276 100

138 29.9 24.4 36.6

277 24.7 19.8 29.8




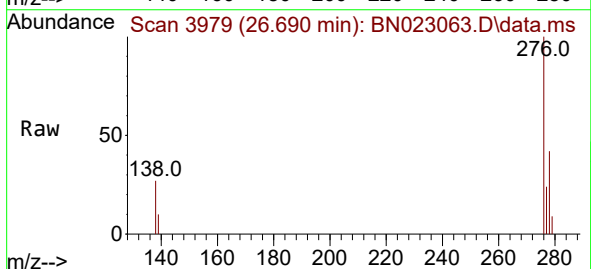




#37
Benzo(b)fluoranthene
Concen: 5.541 ng
RT: 23.340 min Scan# 2833
Delta R.T. -0.000 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:252 Resp: 308007
Ion Ratio Lower Upper
252 100
253 22.0 19.5 29.3
125 12.1 13.4 20.2#

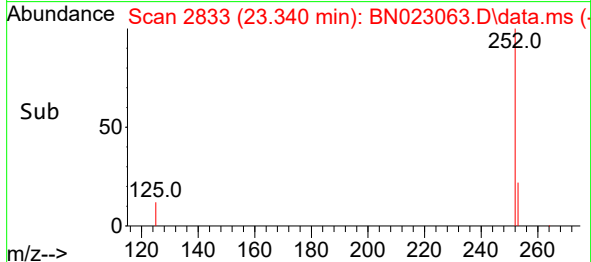

#38
Benzo(k)fluoranthene
Concen: 5.277 ng
RT: 23.387 min Scan# 2849
Delta R.T. -0.003 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15


Tgt Ion:252 Resp: 317724
Ion Ratio Lower Upper
252 100
253 21.7 19.4 29.2
125 11.9 13.5 20.3#

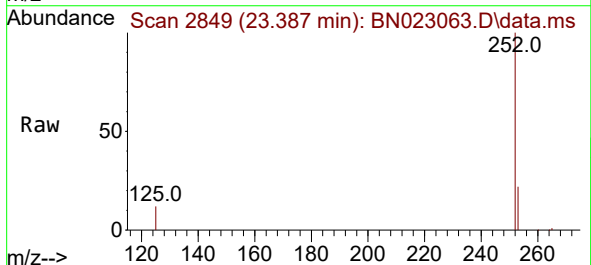






#39
Benzo(a)pyrene
Concen: 6.055 ng
RT: 23.986 min Scan# 3054
Delta R.T. -0.000 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15


Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0





Tgt Ion:252 Resp: 256901
Ion Ratio Lower Upper
252 100
253 21.4 20.7 31.1
125 13.7 17.1 25.7#

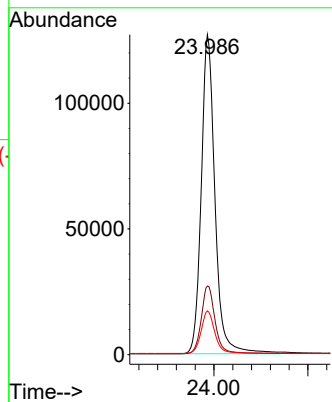


#40
Dibenzo(a,h)anthracene
Concen: 7.373 ng
RT: 26.714 min Scan# 3987
Delta R.T. -0.003 min
Lab File: BN023063.D
Acq: 05 Dec 2022 17:15

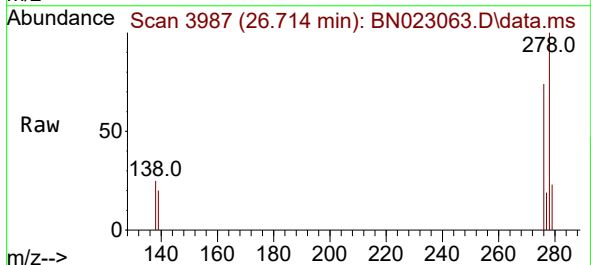

Tgt Ion:278 Resp: 302539
Ion Ratio Lower Upper
278 100
139 20.0 17.2 25.8
279 23.2 20.6 31.0



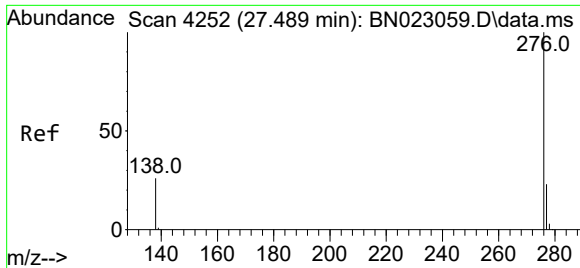

#41
 Benzo(g,h,i)perylene
 Concen: 7.057 ng
 RT: 27.488 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: BN023063.D
 Acq: 05 Dec 2022 17:15

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Tgt Ion:276 Resp: 312020
 Ion Ratio Lower Upper
 276 100
 277 23.5 19.7 29.5
 138 25.6 22.2 33.4

