
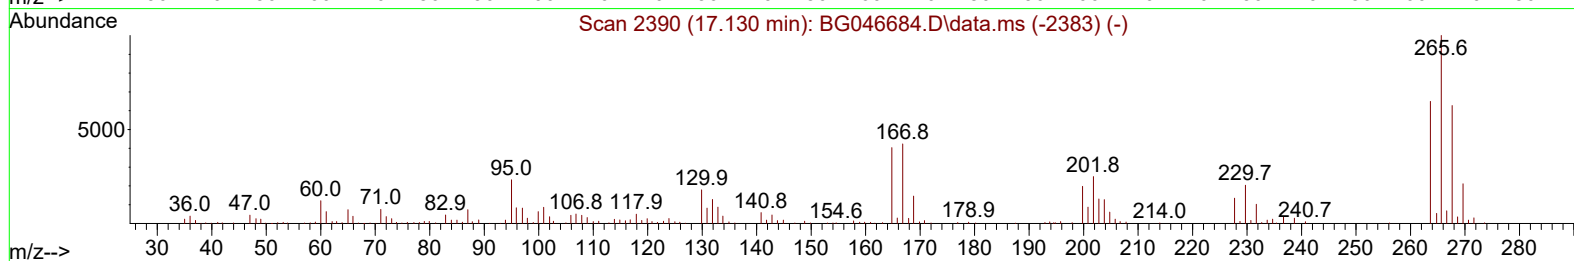
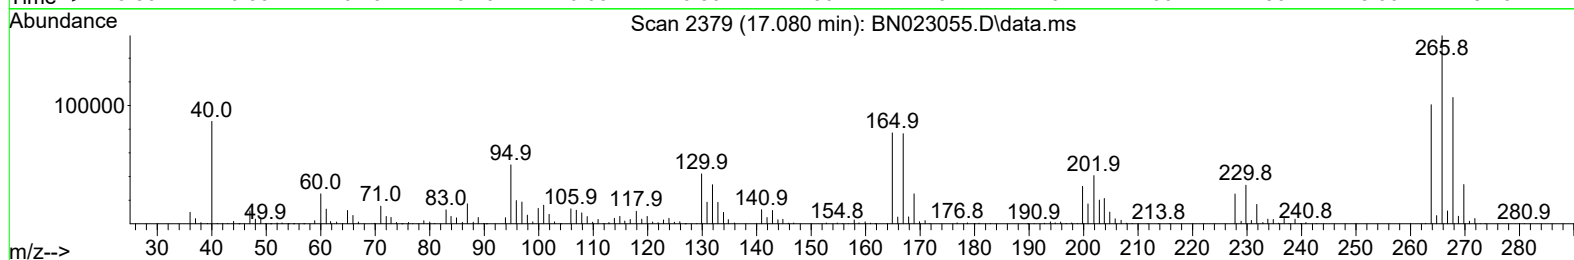


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120522\
 Data File : BN023055.D
 Acq On : 05 Dec 2022 12:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 06:15:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 06 06:15:26 2022
 Response via : Initial Calibration

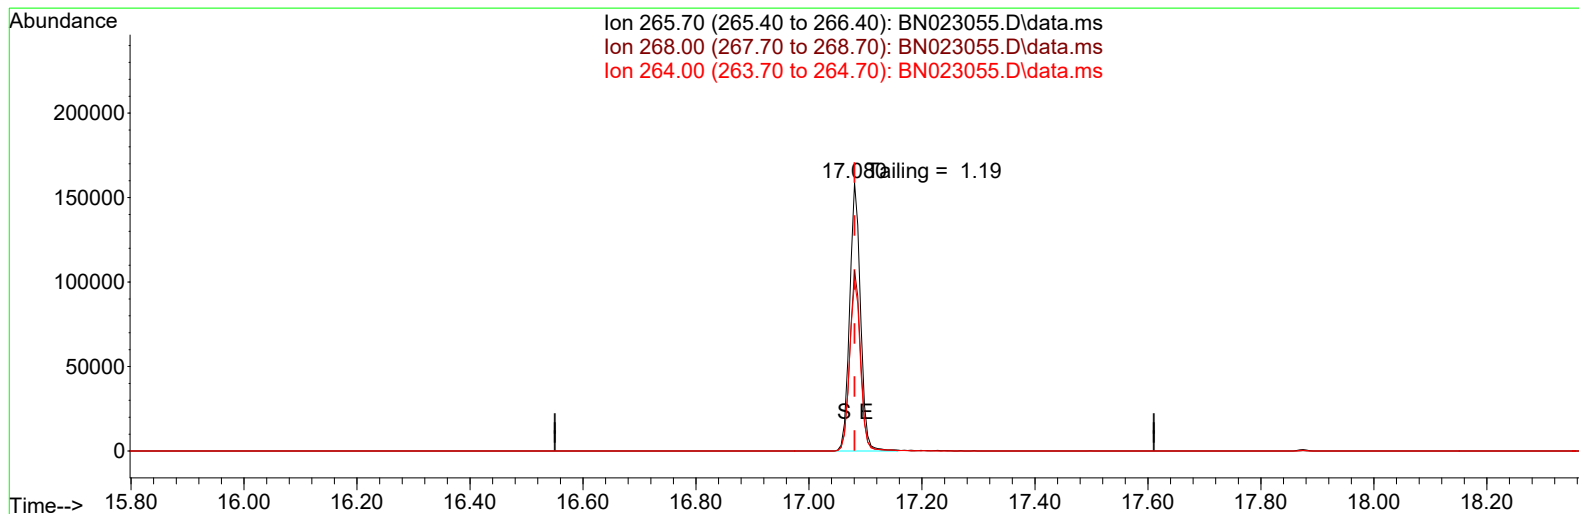

TIC: BN023055.D\data.ms

(70) Pentachlorophenol (C)




17.080min (0.000) 14226.77 ng

response 212578

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.18
264.00	61.60	63.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120522\
Data File : BN023055.D
Acq On : 05 Dec 2022 12:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 06:15:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 06 06:15:26 2022
Response via : Initial Calibration

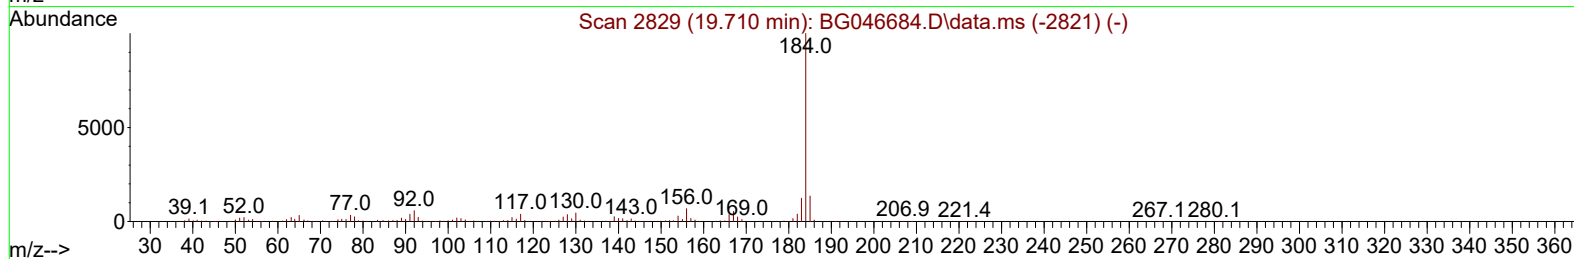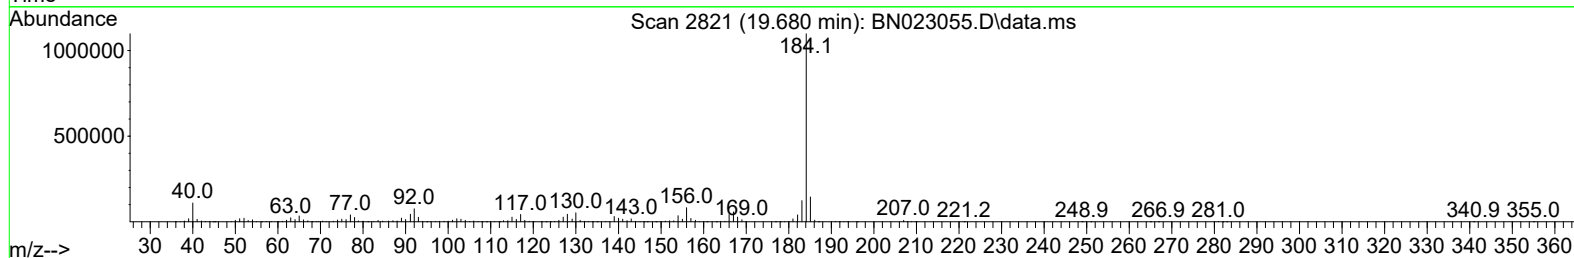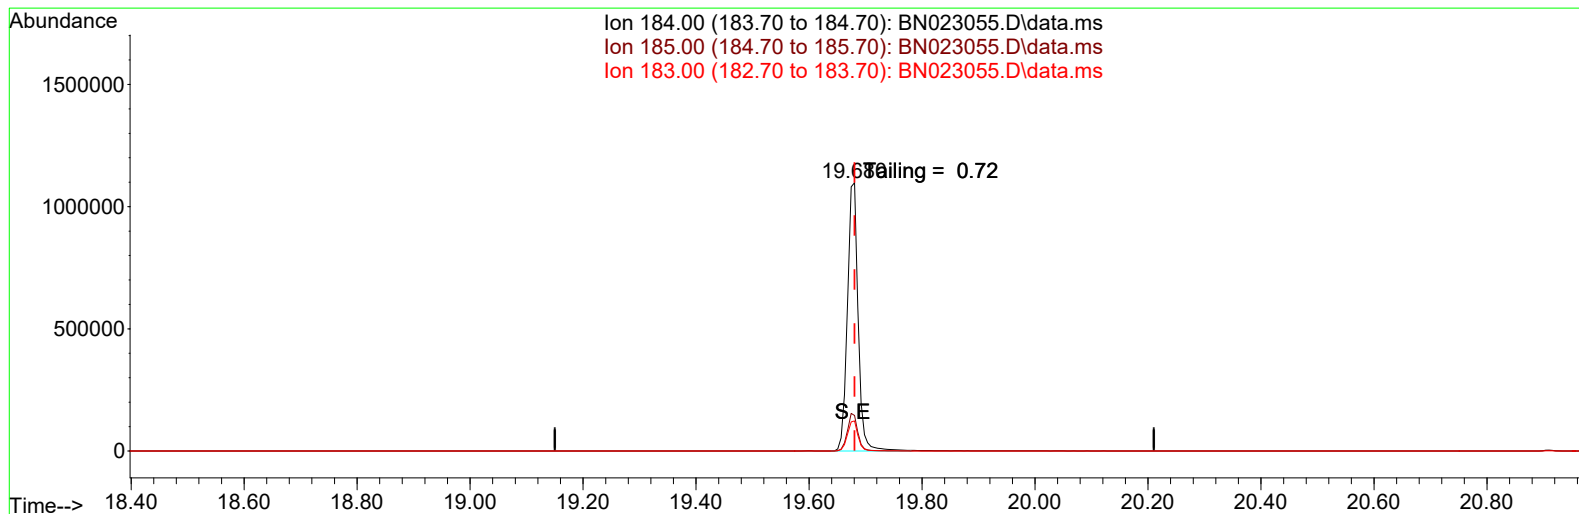

TIC: BN023055.D\data.ms

(77) Benzidine

19.680min (0.000) 0.00 ng

response 1459800

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.22
183.00	13.20	11.21
0.00	0.00	0.00