

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120522\
 Data File : BN023061.D
 Acq On : 05 Dec 2022 16:01
 Operator : CG/JU
 Sample : SSTDICC1.6
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Quant Time: Dec 06 03:40:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 06 03:35:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.049	152	3490	0.400	ng	0.00
7) Naphthalene-d8	10.861	136	10371	0.400	ng	0.00
13) Acenaphthene-d10	14.688	164	6184	0.400	ng	0.00
19) Phenanthrene-d10	17.427	188	13405	0.400	ng	0.00
29) Chrysene-d12	21.625	240	12450	0.400	ng	# 0.00
35) Perylene-d12	24.103	264	9349	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.579	112	12358	1.363	ng	0.00
5) Phenol-d6	7.197	99	16602	1.437	ng	0.00
8) Nitrobenzene-d5	9.206	82	12575	1.561	ng	0.00
11) 2-Methylnaphthalene-d10	12.450	152	37689	1.676	ng	0.00
14) 2,4,6-Tribromophenol	16.173	330	4159	1.393	ng	0.00
15) 2-Fluorobiphenyl	13.319	172	45713	1.616	ng	0.00
27) Fluoranthene-d10	19.464	212	62867	1.727	ng	0.00
31) Terphenyl-d14	20.058	244	41743	1.427	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.427	88	6932	1.565	ng	99
3) n-Nitrosodimethylamine	3.752	42	7937	1.662	ng	# 97
6) bis(2-Chloroethyl)ether	7.464	93	18852	1.738	ng	99
9) Naphthalene	10.915	128	52117	1.632	ng	98
10) Hexachlorobutadiene	11.203	225	9863	1.504	ng	# 100
12) 2-Methylnaphthalene	12.140	142	8772	1.346	ng	# 88
16) Acenaphthylene	14.410	152	51057	1.559	ng	99
17) Acenaphthene	14.752	154	35849	1.664	ng	99
18) Fluorene	15.726	166	45094	1.634	ng	95
20) 4,6-Dinitro-2-methylph...	15.801	198	3552	2.371	ng	# 79
21) 4-Bromophenyl-phenylether	16.620	248	14497	1.498	ng	97
22) Hexachlorobenzene	16.744	284	18377	1.556	ng	100
23) Atrazine	16.881	200	9388	1.376	ng	97
24) Pentachlorophenol	17.079	266	5230	1.617	ng	100
25) Phenanthrene	17.476	178	77763	1.668	ng	99
26) Anthracene	17.563	178	65622	1.622	ng	100
28) Fluoranthene	19.494	202	89135	1.798	ng	100
30) Pyrene	19.857	202	90283	1.393	ng	98
32) Benzo(a)anthracene	21.607	228	77021	1.531	ng	99
33) Chrysene	21.661	228	85872	1.646	ng	98
34) Bis(2-ethylhexyl)phtha...	21.527	149	27810	1.376	ng	# 98
36) Indeno(1,2,3-cd)pyrene	26.696	276	87907	2.266	ng	99
37) Benzo(b)fluoranthene	23.343	252	74162	1.777	ng	# 94
38) Benzo(k)fluoranthene	23.392	252	78261	1.731	ng	# 94
39) Benzo(a)pyrene	23.992	252	58386	1.833	ng	# 91
40) Dibenzo(a,h)anthracene	26.720	278	70777	2.297	ng	97
41) Benzo(g,h,i)perylene	27.494	276	72470	2.183	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120522\
Data File : BN023061.D
Acq On : 05 Dec 2022 16:01
Operator : CG/JU
Sample : SSTDICC1.6
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Quant Time: Dec 06 03:40:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 06 03:35:07 2022
Response via : Initial Calibration




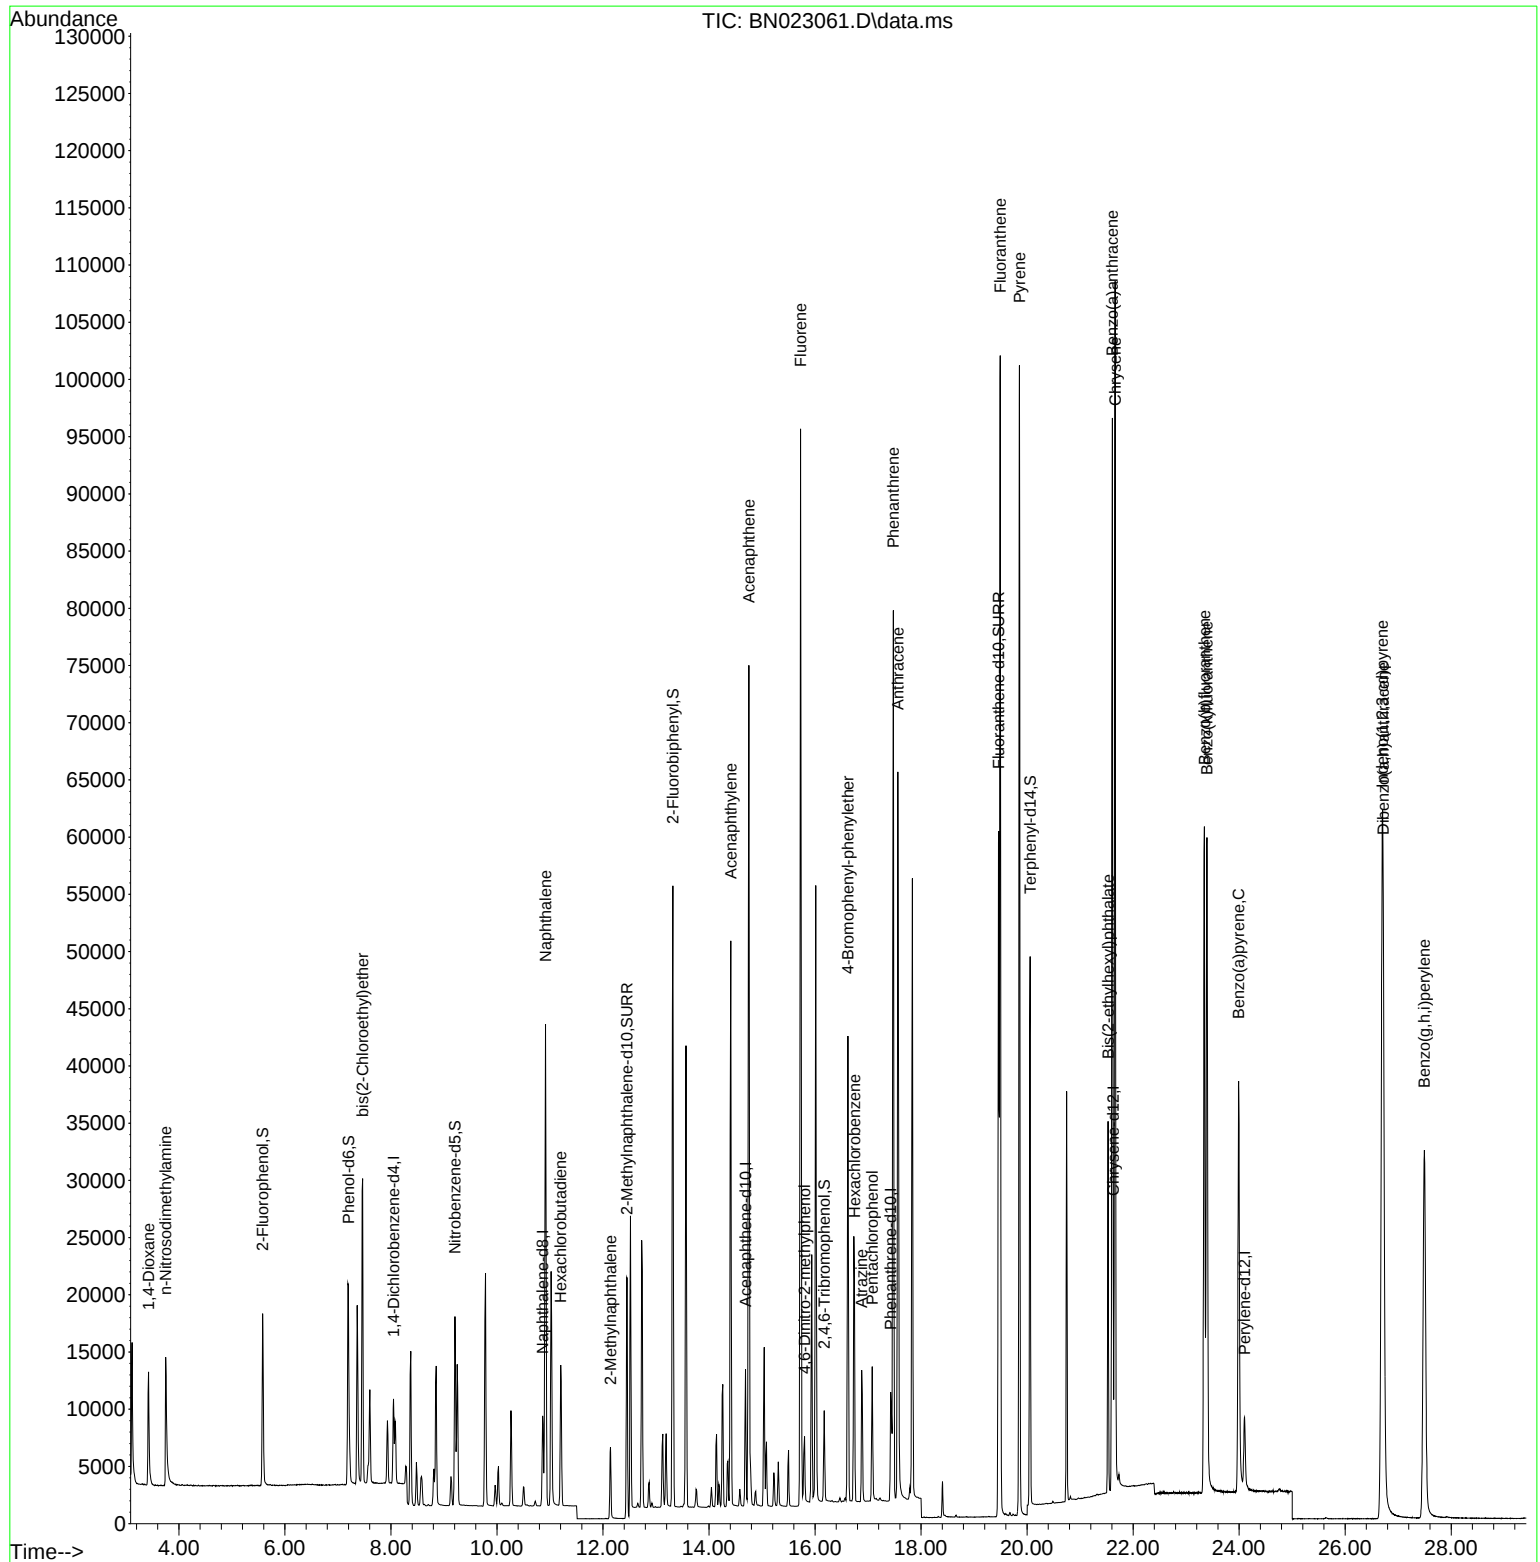




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 8.049 min Scan# 68
 Delta R.T. 0.000 min
 Lab File: BN023061.D
 Acq: 05 Dec 2022 16:01




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6


Tgt Ion:152 Resp: 3490
 Ion Ratio Lower Upper
 152 100
 150 153.9 122.3 183.5
 115 61.7 48.6 72.8

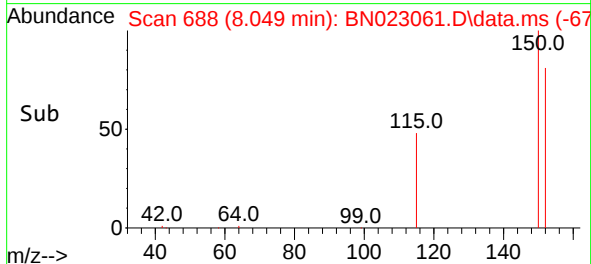

#2
 1,4-Dioxane
 Concen: 1.565 ng
 RT: 3.427 min Scan# 48
 Delta R.T. 0.000 min
 Lab File: BN023061.D
 Acq: 05 Dec 2022 16:01

Tgt Ion: 88 Resp: 6932
 Ion Ratio Lower Upper
 88 100
 43 30.8 25.4 38.2
 58 71.7 58.2 87.4


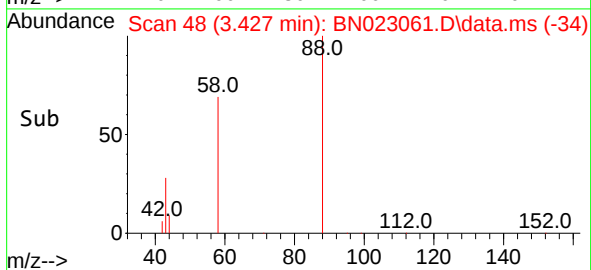




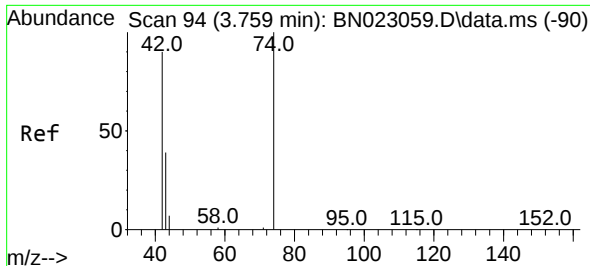

#3
n-Nitrosodimethylamine
Concen: 1.662 ng
RT: 3.752 min Scan# 93
Delta R.T. -0.007 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion: 42 Resp: 7937
Ion Ratio Lower Upper
42 100
74 111.5 87.4 131.0
44 7.5 10.4 15.6#

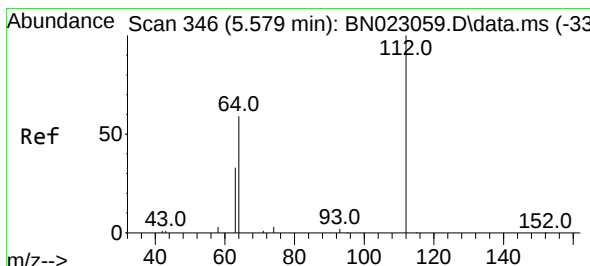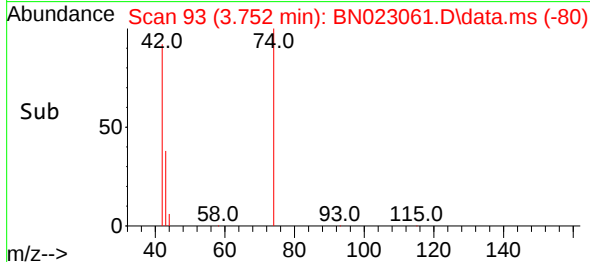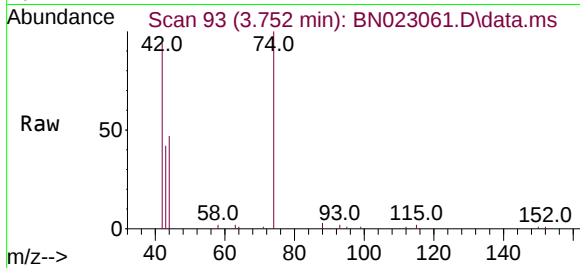

#4
2-Fluorophenol
Concen: 1.363 ng
RT: 5.579 min Scan# 346
Delta R.T. 0.000 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01

Tgt Ion: 112 Resp: 12358
Ion Ratio Lower Upper
112 100
64 57.3 46.2 69.4
63 31.5 25.1 37.7


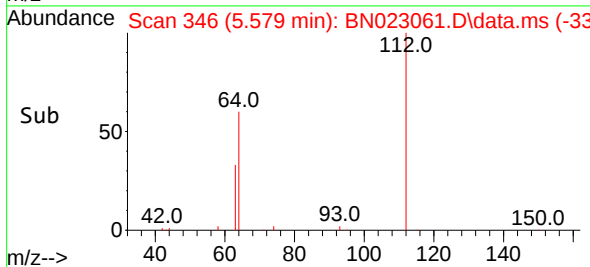

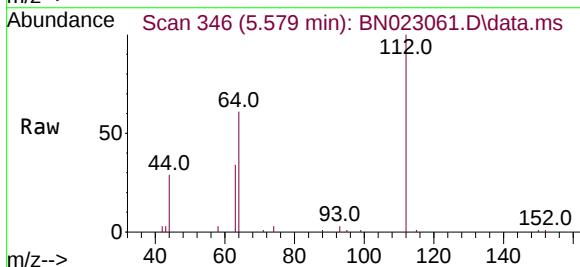


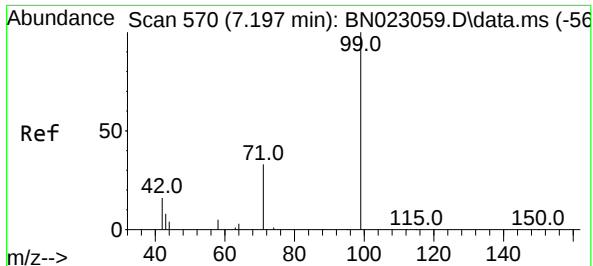

#5
Phenol-d6
Concen: 1.437 ng
RT: 7.197 min Scan# 51
Delta R.T. 0.000 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion: 99 Resp: 16602
Ion Ratio Lower Upper
99 100
42 22.4 18.1 27.1
71 34.7 28.2 42.2

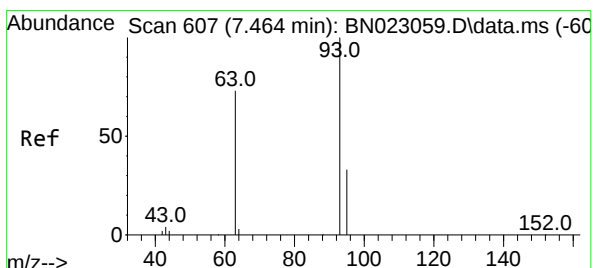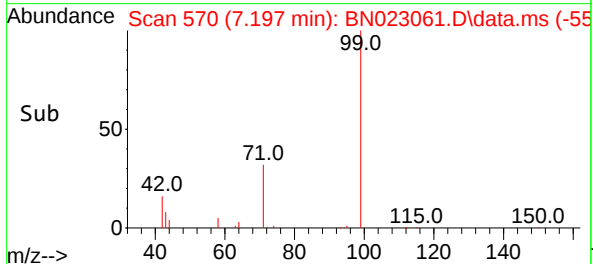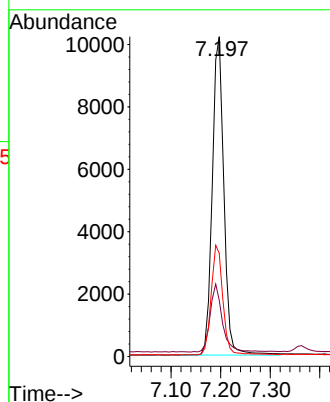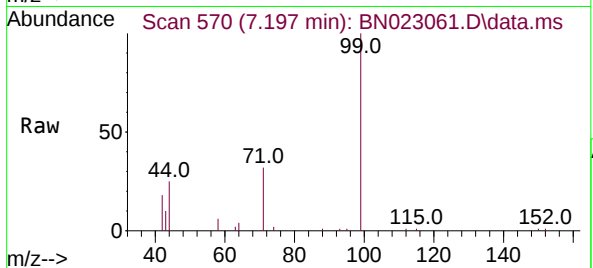

#6
bis(2-Chloroethyl)ether
Concen: 1.738 ng
RT: 7.464 min Scan# 607
Delta R.T. 0.000 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01

Tgt Ion: 93 Resp: 18852
Ion Ratio Lower Upper
93 100
63 76.1 61.4 92.2
95 32.1 25.9 38.9


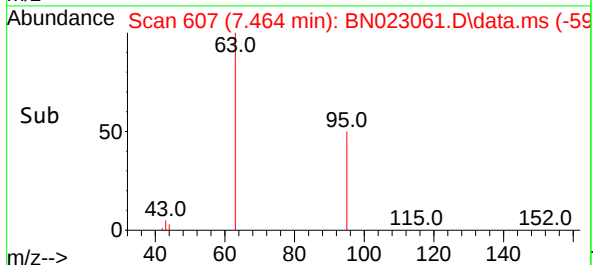
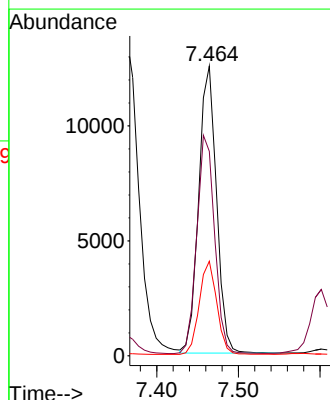
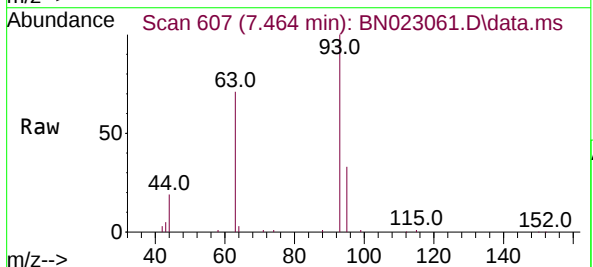




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.861 min Scan# 963
Delta R.T. 0.000 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	136	Resp:	10371
Ion Ratio	Lower	Upper	
136	100		
137	11.8	9.4	14.2
54	11.1	8.8	13.2
68	8.5	7.0	10.6

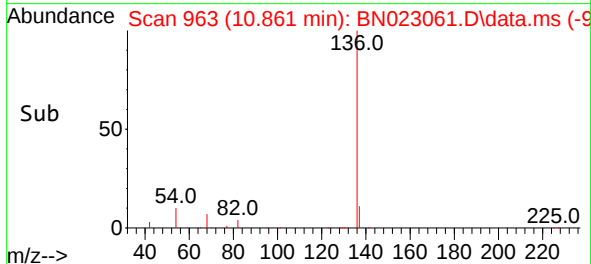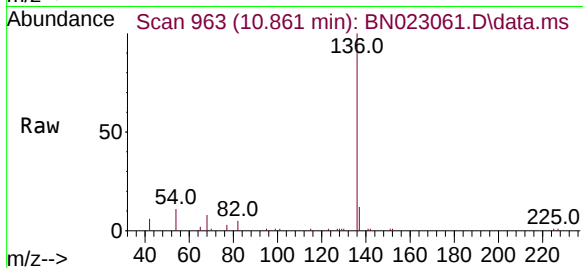

#8
Nitrobenzene-d5
Concen: 1.561 ng
RT: 9.206 min Scan# 808
Delta R.T. 0.000 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01

Tgt Ion:	82	Resp:	12575
Ion Ratio	Lower	Upper	
82	100		
128	34.7	29.9	44.9
54	54.7	44.2	66.2




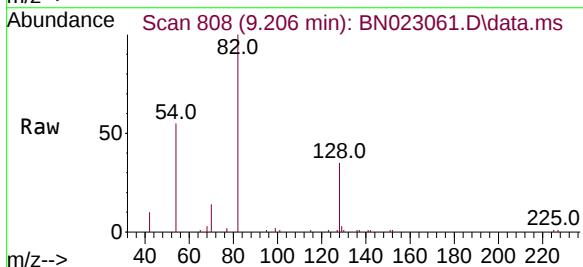


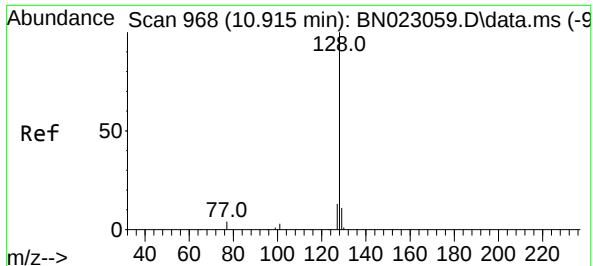

#9
Naphthalene
Concen: 1.632 ng
RT: 10.915 min Scan# 968
Delta R.T. 0.000 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:128 Resp: 52117
Ion Ratio Lower Upper
128 100
129 10.8 9.2 13.8
127 13.0 10.9 16.3

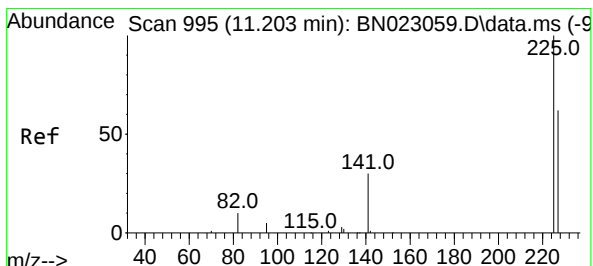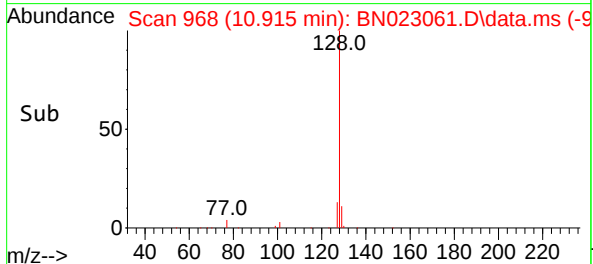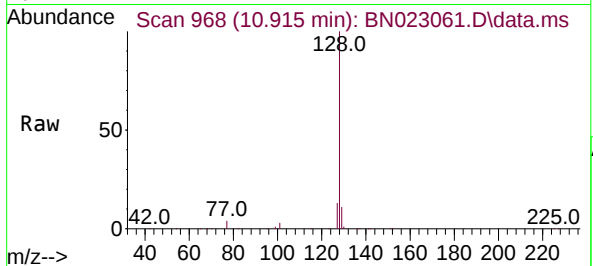

#10
Hexachlorobutadiene
Concen: 1.504 ng
RT: 11.203 min Scan# 995
Delta R.T. 0.000 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01

Tgt Ion:225 Resp: 9863
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.3 50.8 76.2


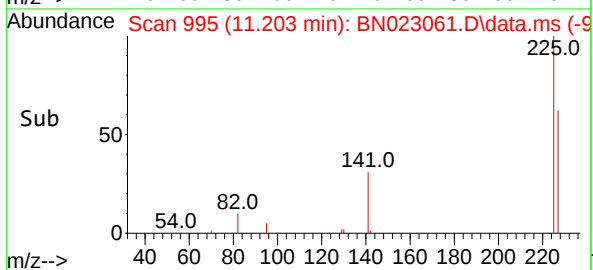

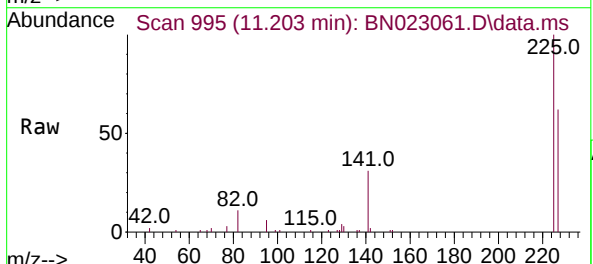




#11
2-Methylnaphthalene-d10
Concen: 1.676 ng
RT: 12.450 min Scan# 1190
Delta R.T. 0.000 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:152 Resp: 37689
Ion Ratio Lower Upper
152 100
151 17.1 18.9 28.3#

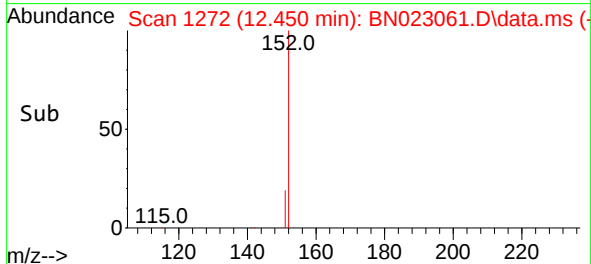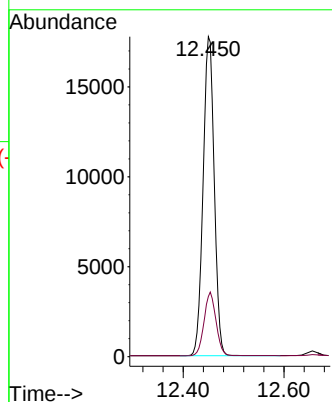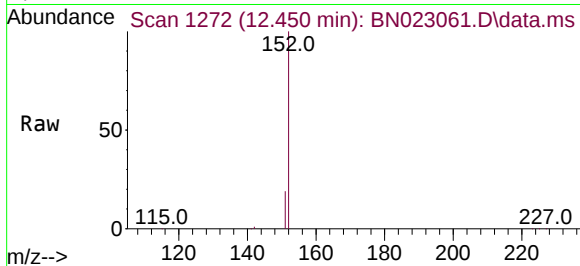

#12
2-Methylnaphthalene
Concen: 1.346 ng
RT: 12.140 min Scan# 1190
Delta R.T. 0.000 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01

Tgt Ion:142 Resp: 8772
Ion Ratio Lower Upper
142 100
141 11.2 12.3 18.5#
115 3.3 6.9 10.3#




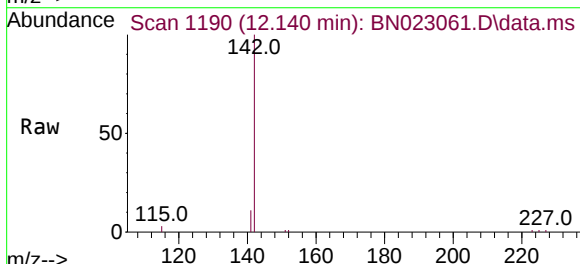


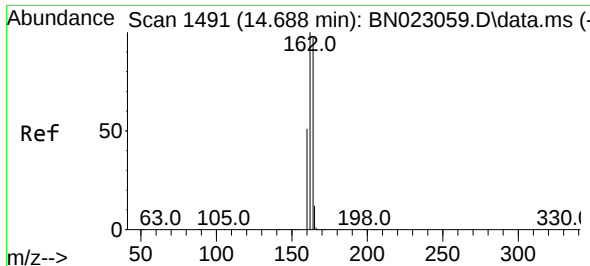

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.688 min Scan# 1491
Delta R.T. 0.000 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:164 Resp: 6184
Ion Ratio Lower Upper
164 100
162 104.1 82.7 124.1
160 54.0 42.6 63.8

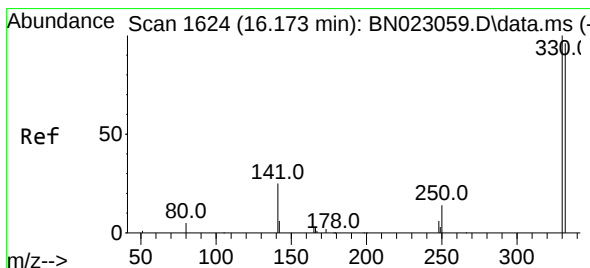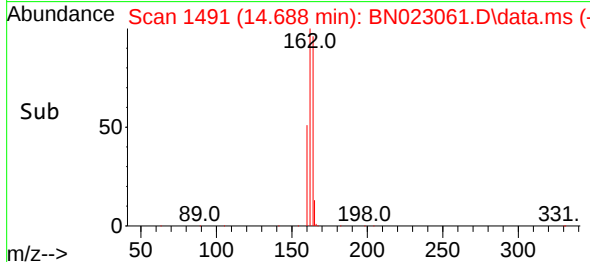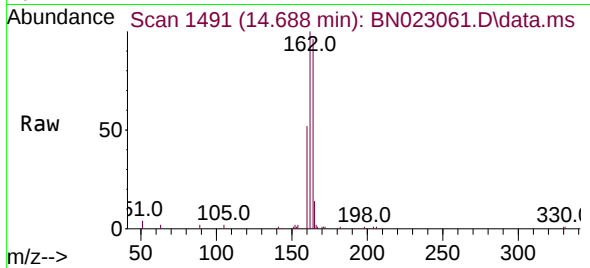

#14
2,4,6-Tribromophenol
Concen: 1.393 ng
RT: 16.173 min Scan# 1624
Delta R.T. 0.000 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01

Tgt Ion:330 Resp: 4159
Ion Ratio Lower Upper
330 100
332 97.6 77.1 115.7
141 42.3 36.7 55.1


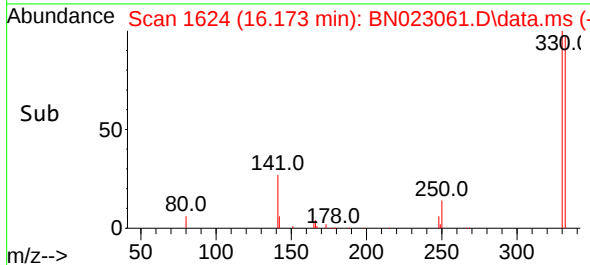

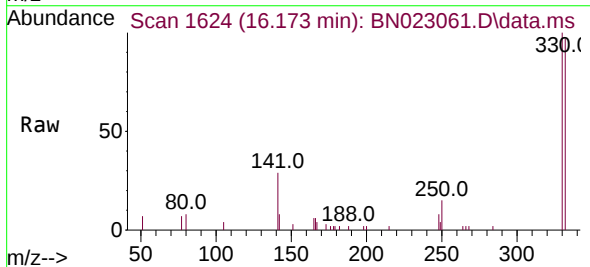




#15
2-Fluorobiphenyl
Concen: 1.616 ng
RT: 13.319 min Scan# 1363
Delta R.T. 0.000 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:172 Resp: 45713
Ion Ratio Lower Upper
172 100
171 33.9 27.3 40.9
170 22.6 18.3 27.5

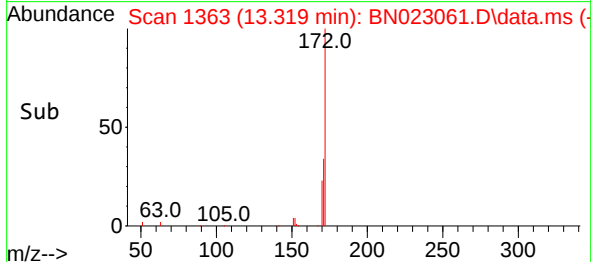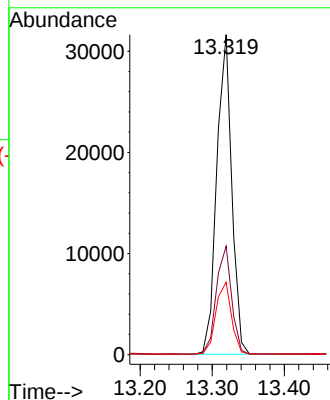

#16
Acenaphthylene
Concen: 1.559 ng
RT: 14.410 min Scan# 1465
Delta R.T. 0.000 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01

Tgt Ion:152 Resp: 51057
Ion Ratio Lower Upper
152 100
151 19.3 15.7 23.5
153 12.9 10.4 15.6



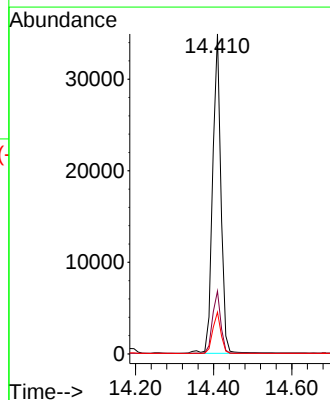
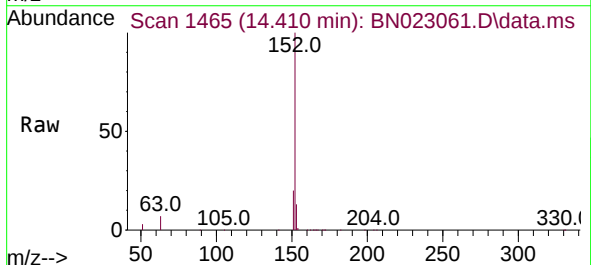




#17
Acenaphthene
Concen: 1.664 ng
RT: 14.752 min Scan# 1497
Delta R.T. 0.000 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:154 Resp: 35849
Ion Ratio Lower Upper
154 100
153 110.1 88.2 132.4
152 59.3 48.2 72.2

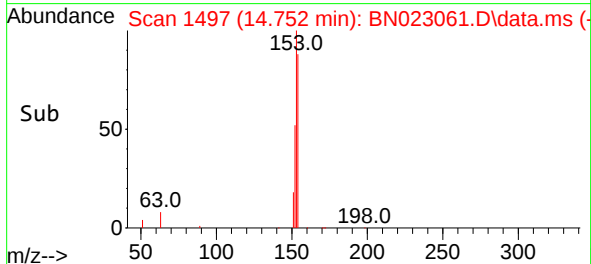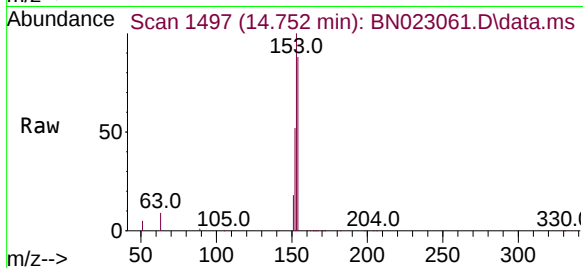

#18
Fluorene
Concen: 1.634 ng
RT: 15.726 min Scan# 1588
Delta R.T. 0.000 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01

Tgt Ion:166 Resp: 45094
Ion Ratio Lower Upper
166 100
165 97.4 82.2 123.4
167 13.6 11.4 17.0

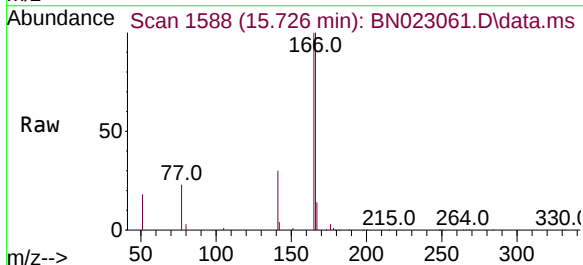



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.427 min Scan# 1725

Delta R.T. 0.000 min

Lab File: BN023061.D

Acq: 05 Dec 2022 16:01

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:188 Resp: 13405

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 17.4 13.3 19.9

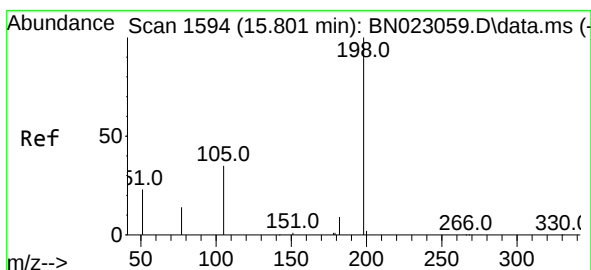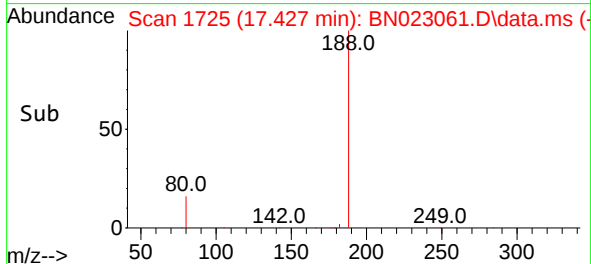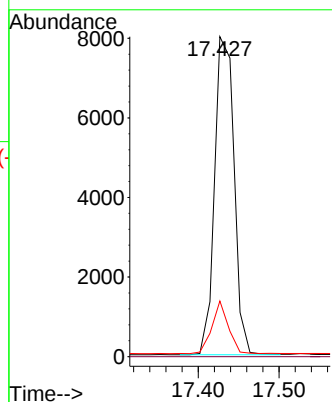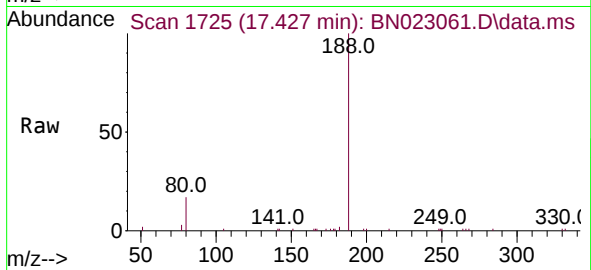

#20

4,6-Dinitro-2-methylphenol

Concen: 2.371 ng

RT: 15.801 min Scan# 1594

Delta R.T. 0.000 min

Lab File: BN023061.D

Acq: 05 Dec 2022 16:01




Tgt Ion:198 Resp: 3552


Ion Ratio Lower Upper

198 100

51 41.7 51.8 77.6#

105 43.1 40.7 61.1









#21
4-Bromophenyl-phenylether
Concen: 1.498 ng
RT: 16.620 min Scan# 1660
Delta R.T. 0.000 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:248 Resp: 14497
Ion Ratio Lower Upper
248 100
250 92.5 75.8 113.6
141 71.6 54.3 81.5

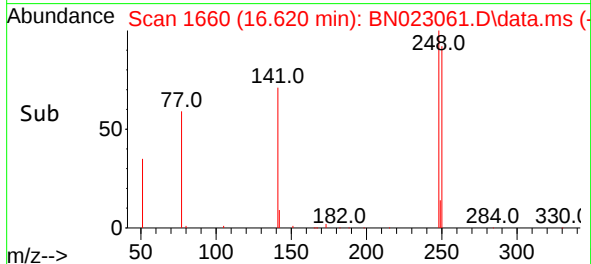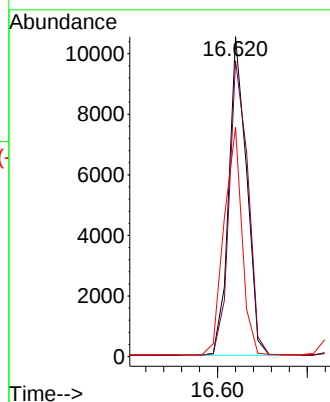

#22
Hexachlorobenzene
Concen: 1.556 ng
RT: 16.744 min Scan# 1670
Delta R.T. 0.000 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01

Tgt Ion:284 Resp: 18377
Ion Ratio Lower Upper
284 100
142 40.8 32.6 48.8
249 30.7 24.7 37.1

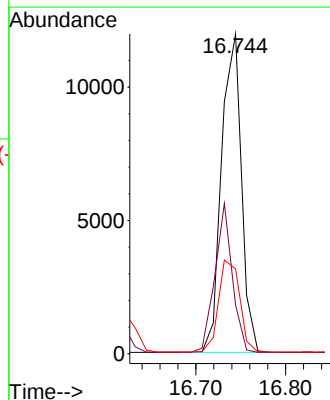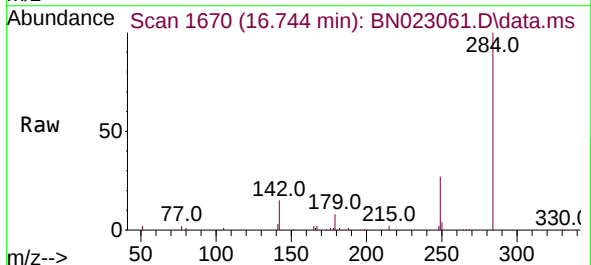



#23

Atrazine

Concen: 1.376 ng

RT: 16.881 min Scan# 1681

Delta R.T. 0.000 min

Lab File: BN023061.D

Acq: 05 Dec 2022 16:01

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:200 Resp: 9388

Ion Ratio Lower Upper

200 100

173 33.9 28.4 42.6

215 43.6 36.6 55.0

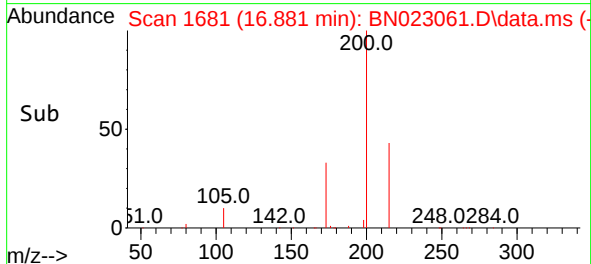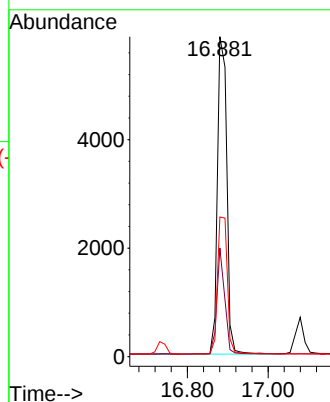

#24

Pentachlorophenol

Concen: 1.617 ng

RT: 17.079 min Scan# 1697

Delta R.T. 0.000 min

Lab File: BN023061.D

Acq: 05 Dec 2022 16:01




Tgt Ion:266 Resp: 5230


Ion Ratio Lower Upper

266 100

264 62.2 49.6 74.4

268 63.0 50.8 76.2


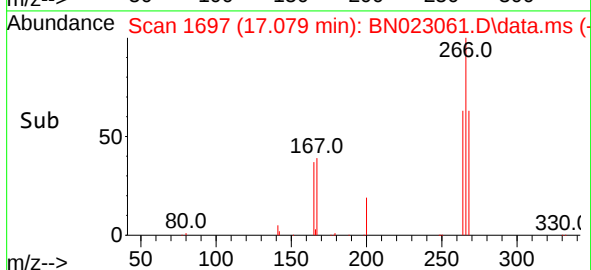
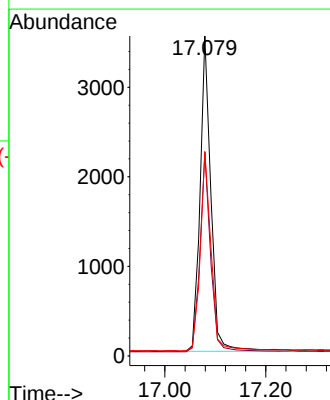



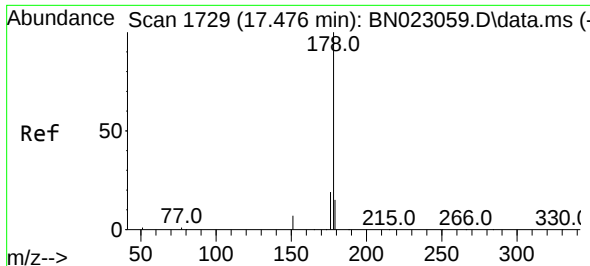

#25
Phenanthrene
Concen: 1.668 ng
RT: 17.476 min Scan# 1729
Delta R.T. 0.000 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:178 Resp: 77763
Ion Ratio Lower Upper
178 100
176 19.3 15.3 22.9
179 15.1 12.4 18.6

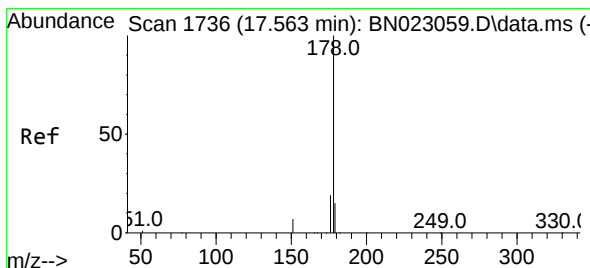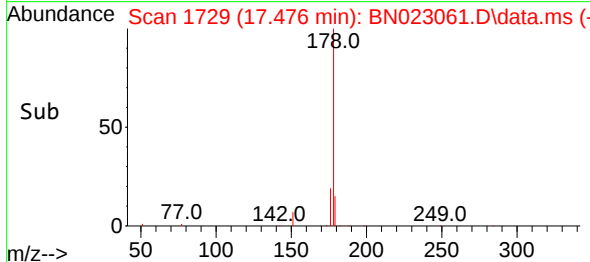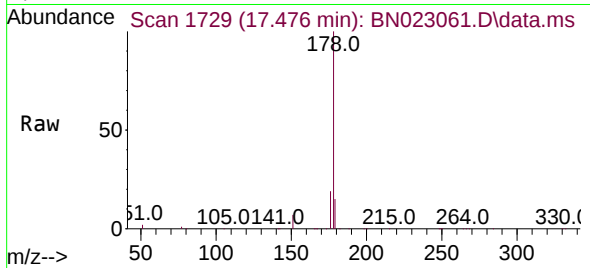

#26
Anthracene
Concen: 1.622 ng
RT: 17.563 min Scan# 1736
Delta R.T. 0.000 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01

Tgt Ion:178 Resp: 65622
Ion Ratio Lower Upper
178 100
176 18.7 15.0 22.4
179 15.3 12.4 18.6


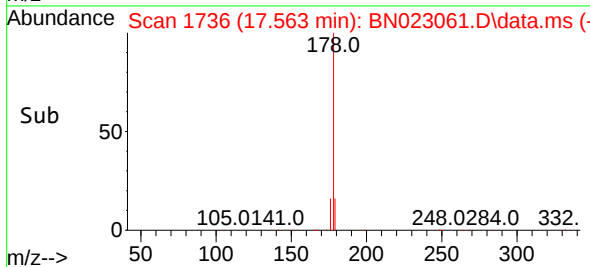

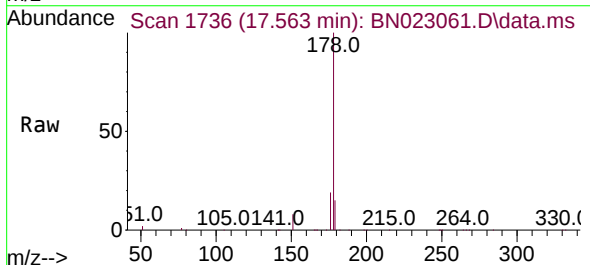




#27
Fluoranthene-d10
Concen: 1.727 ng
RT: 19.464 min Scan# 2116
Delta R.T. 0.004 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:212 Resp: 62867
Ion Ratio Lower Upper
212 100
106 16.8 13.3 19.9
104 9.6 7.7 11.5

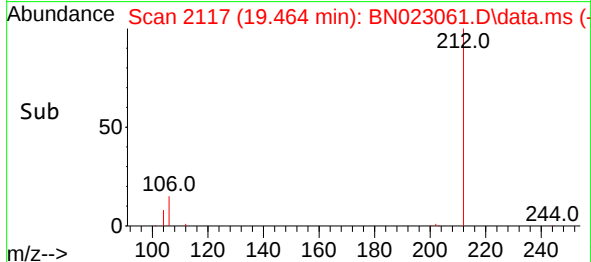

#28
Fluoranthene
Concen: 1.798 ng
RT: 19.494 min Scan# 2124
Delta R.T. 0.004 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01

Tgt Ion:202 Resp: 89135
Ion Ratio Lower Upper
202 100
101 12.9 10.5 15.7
203 17.1 13.8 20.6

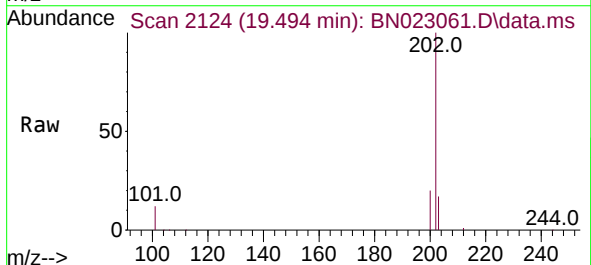



#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.625 min Scan# 2425

Delta R.T. 0.009 min

Lab File: BN023061.D

Acq: 05 Dec 2022 16:01

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:240 Resp: 12450

Ion Ratio Lower Upper

240 100

120 12.5 14.2 21.4#

236 27.9 22.8 34.2

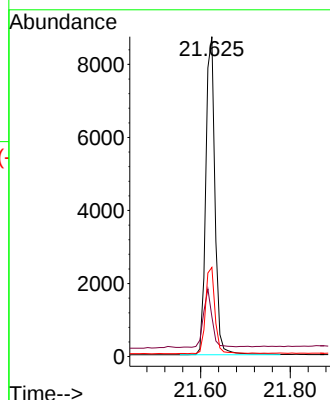

#30

Pyrene

Concen: 1.393 ng

RT: 19.857 min Scan# 2210

Delta R.T. 0.004 min

Lab File: BN023061.D

Acq: 05 Dec 2022 16:01




Tgt Ion:202 Resp: 90283


Ion Ratio Lower Upper

202 100

200 20.1 16.7 25.1

203 16.9 14.3 21.5


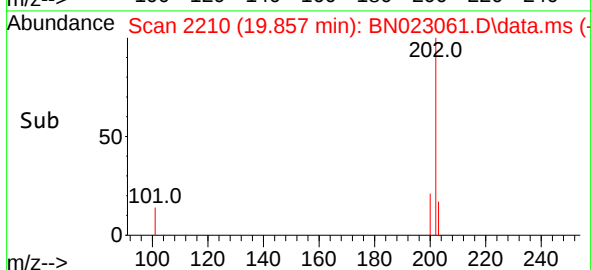
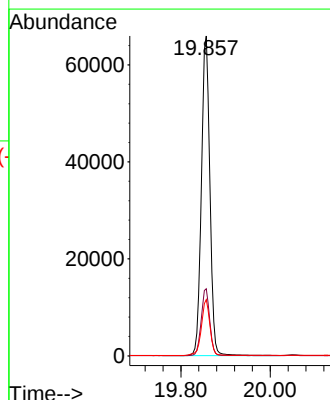



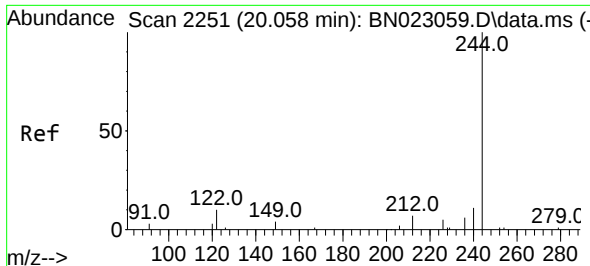

#31
 Terphenyl-d14
 Concen: 1.427 ng
 RT: 20.058 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BN023061.D
 Acq: 05 Dec 2022 16:01




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6


Tgt Ion:244 Resp: 41743
 Ion Ratio Lower Upper
 244 100
 212 8.0 6.2 9.2
 122 10.8 7.7 11.5

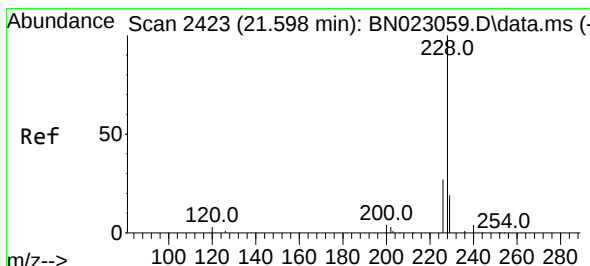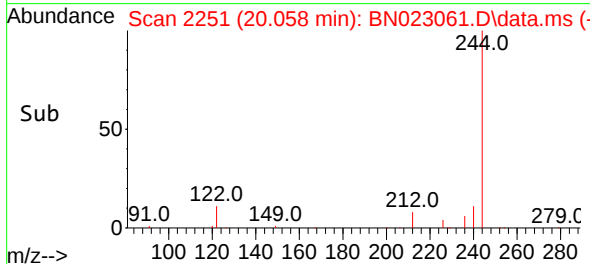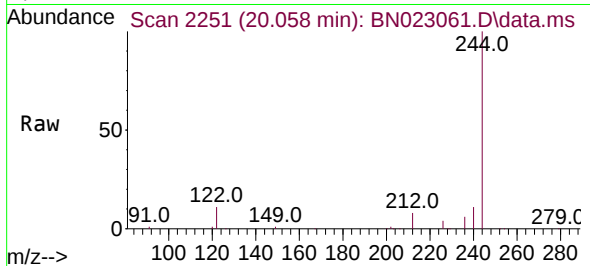

#32
 Benzo(a)anthracene
 Concen: 1.531 ng
 RT: 21.607 min Scan# 2424
 Delta R.T. 0.009 min
 Lab File: BN023061.D
 Acq: 05 Dec 2022 16:01

Tgt Ion:228 Resp: 77021
 Ion Ratio Lower Upper
 228 100
 226 26.8 22.2 33.4
 229 19.6 15.7 23.5

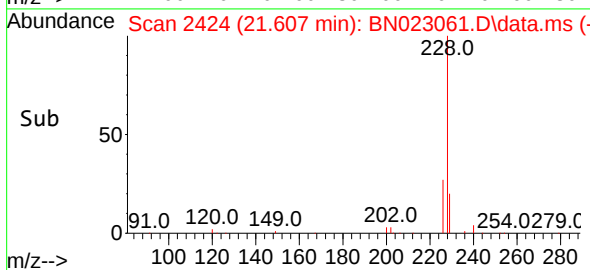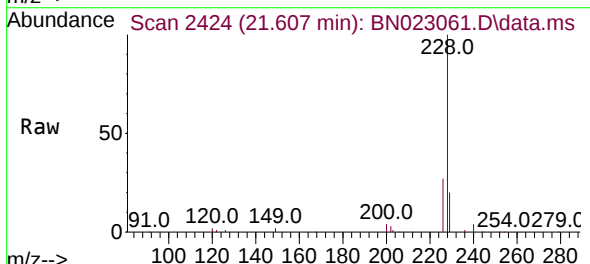

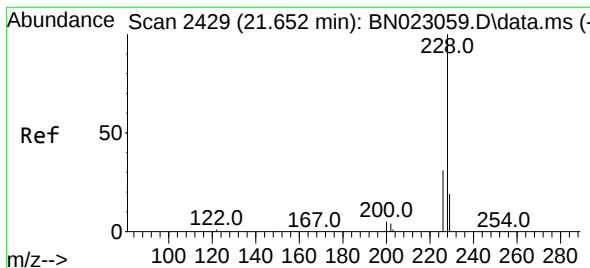

#33

Chrysene

Concen: 1.646 ng

RT: 21.661 min Scan# 24

Delta R.T. 0.009 min

Lab File: BN023061.D

Acq: 05 Dec 2022 16:01

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:228 Resp: 85872

Ion Ratio Lower Upper

228 100

226 30.1 25.0 37.6

229 19.4 15.4 23.0

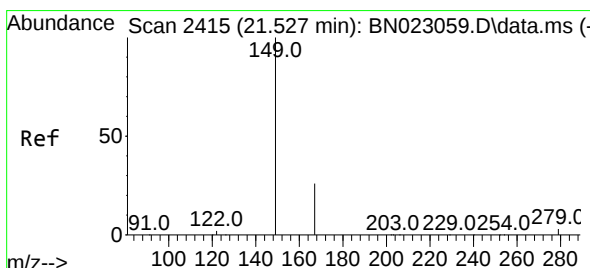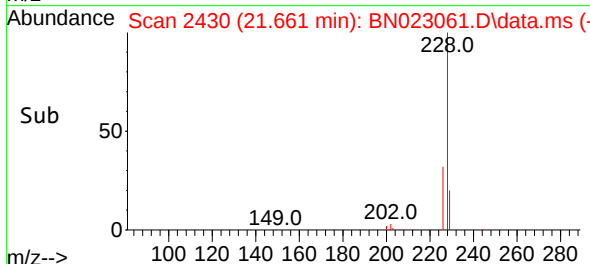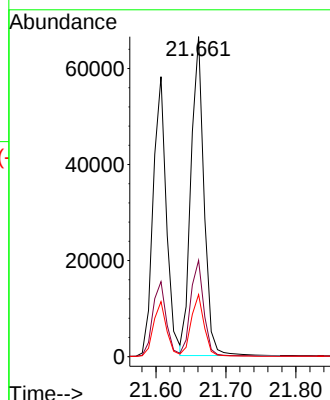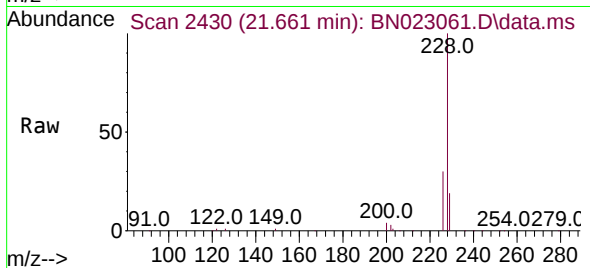

#34

Bis(2-ethylhexyl)phthalate

Concen: 1.376 ng

RT: 21.527 min Scan# 2415

Delta R.T. 0.000 min

Lab File: BN023061.D

Acq: 05 Dec 2022 16:01




Tgt Ion:149 Resp: 27810


Ion Ratio Lower Upper

149 100

167 25.2 19.5 29.3


279 2.4 2.6 4.0#

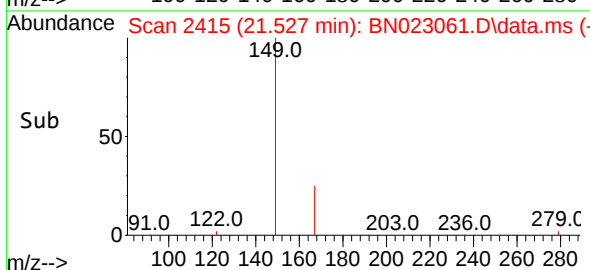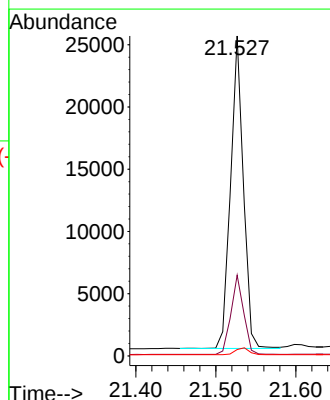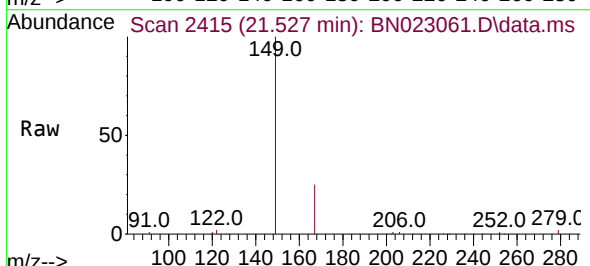






#35
Perylene-d12
Concen: 0.400 ng
RT: 24.103 min Scan# 3094
Delta R.T. 0.006 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6



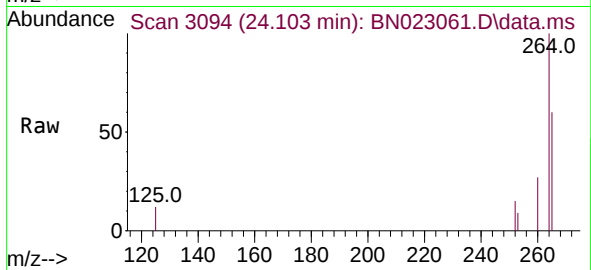



Tgt Ion:264 Resp: 9349
Ion Ratio Lower Upper
264 100
260 26.7 21.0 31.4
265 59.7 45.0 67.6

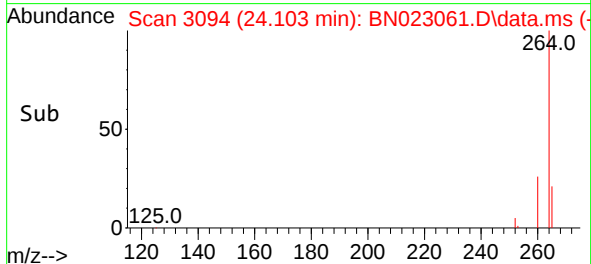

#36
Indeno(1,2,3-cd)pyrene
Concen: 2.266 ng
RT: 26.696 min Scan# 3981
Delta R.T. 0.003 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01

Tgt Ion:276 Resp: 87907
Ion Ratio Lower Upper
276 100
138 31.2 24.4 36.6
277 24.6 19.8 29.8


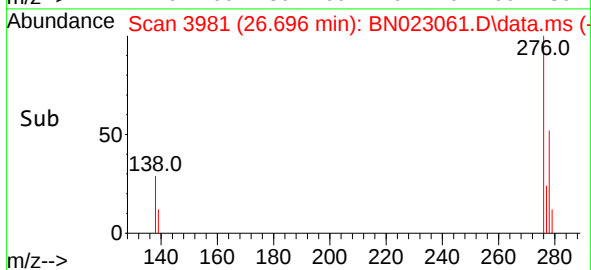






#37
Benzo(b)fluoranthene
Concen: 1.777 ng
RT: 23.343 min Scan# 2833
Delta R.T. 0.003 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:252 Resp: 74162
Ion Ratio Lower Upper
252 100
253 22.3 19.5 29.3
125 13.2 13.4 20.2#

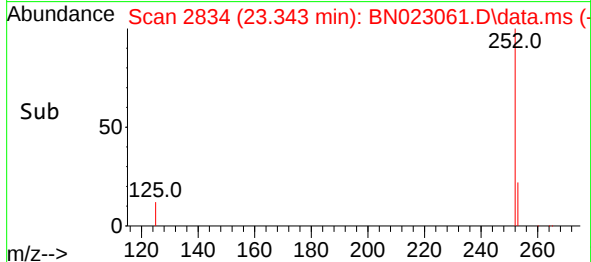

#38
Benzo(k)fluoranthene
Concen: 1.731 ng
RT: 23.392 min Scan# 2851
Delta R.T. 0.003 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01

Tgt Ion:252 Resp: 78261
Ion Ratio Lower Upper
252 100
253 22.3 19.4 29.2
125 13.2 13.5 20.3#




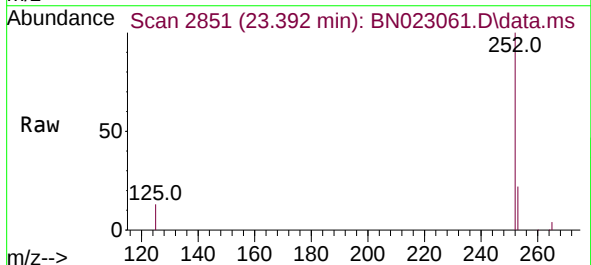




#39
Benzo(a)pyrene
Concen: 1.833 ng
RT: 23.992 min Scan# 3056
Delta R.T. 0.006 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:252 Resp: 58386
Ion Ratio Lower Upper
252 100
253 22.5 20.7 31.1
125 15.5 17.1 25.7#

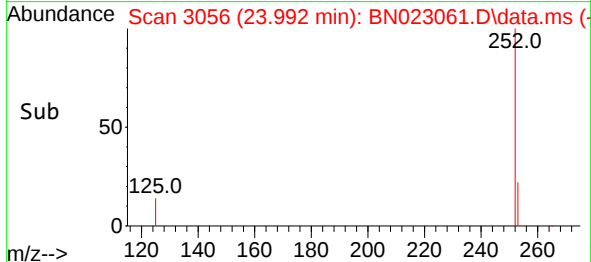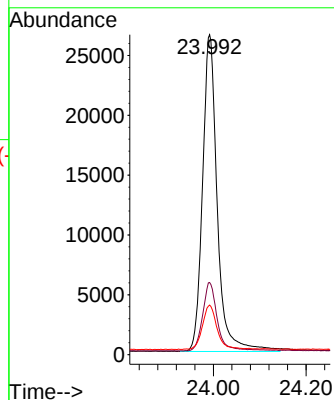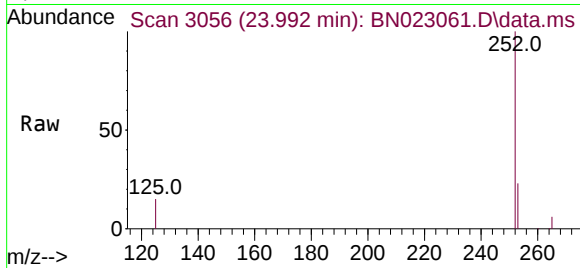

#40
Dibenzo(a,h)anthracene
Concen: 2.297 ng
RT: 26.720 min Scan# 3989
Delta R.T. 0.003 min
Lab File: BN023061.D
Acq: 05 Dec 2022 16:01


Tgt Ion:278 Resp: 70777
Ion Ratio Lower Upper
278 100
139 20.7 17.2 25.8
279 23.4 20.6 31.0

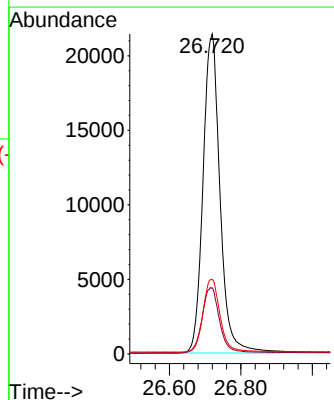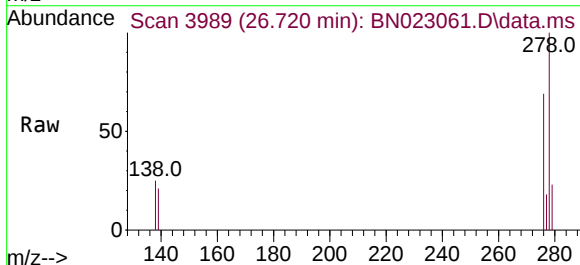

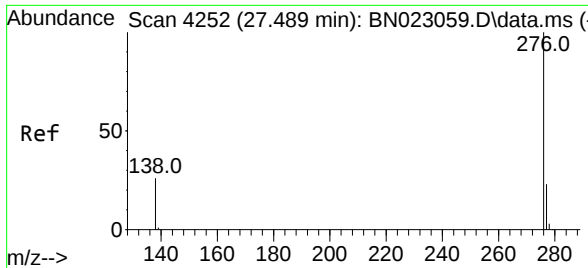

#41
 Benzo(g,h,i)perylene
 Concen: 2.183 ng
 RT: 27.494 min Scan# 41
 Delta R.T. 0.006 min
 Lab File: BN023061.D
 Acq: 05 Dec 2022 16:01

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

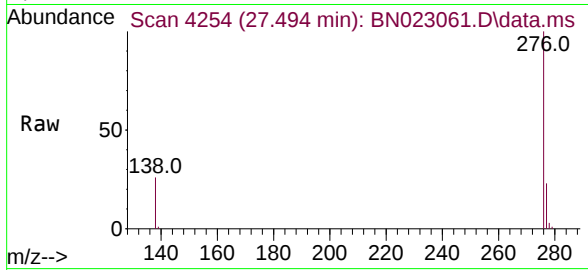

Tgt Ion:276 Resp: 72470
 Ion Ratio Lower Upper
 276 100
 277 23.1 19.7 29.5
 138 26.4 22.2 33.4

