
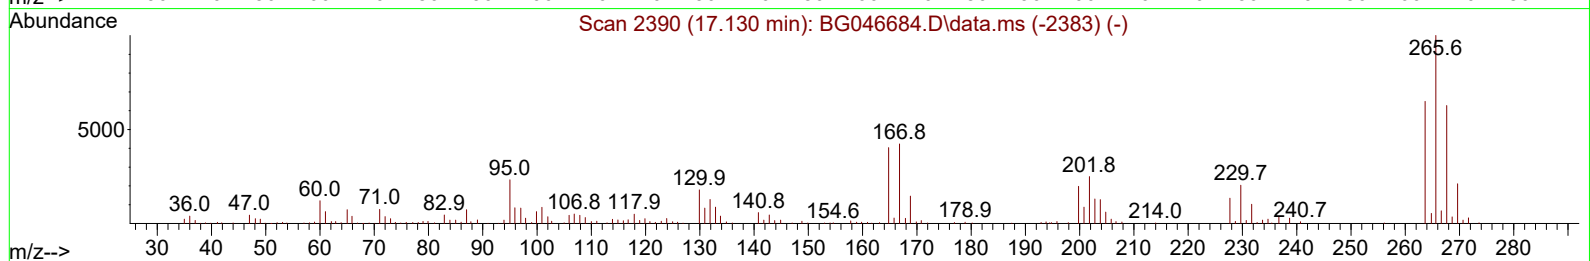
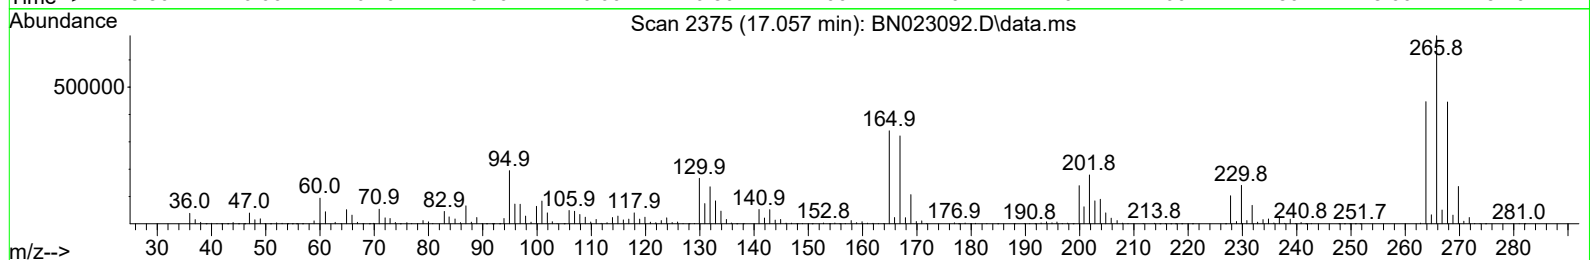


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120822\
Data File : BN023092.D
Acq On : 08 Dec 2022 12:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 09 09:10:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 09 09:10:48 2022
Response via : Initial Calibration

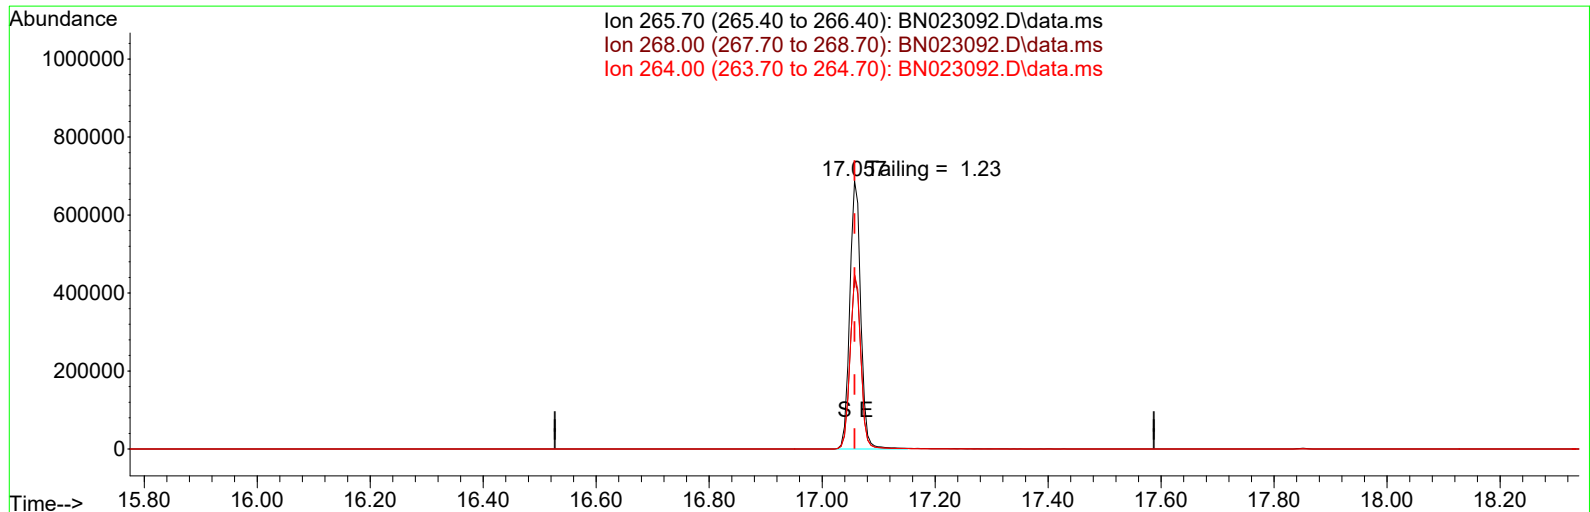

TIC: BN023092.D\data.ms

(70) Pentachlorophenol (C)




17.057min (0.000) 22077.14 ng

response 935928

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.79
264.00	61.60	64.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120822\
Data File : BN023092.D
Acq On : 08 Dec 2022 12:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 09 09:10:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 09 09:10:48 2022
Response via : Initial Calibration

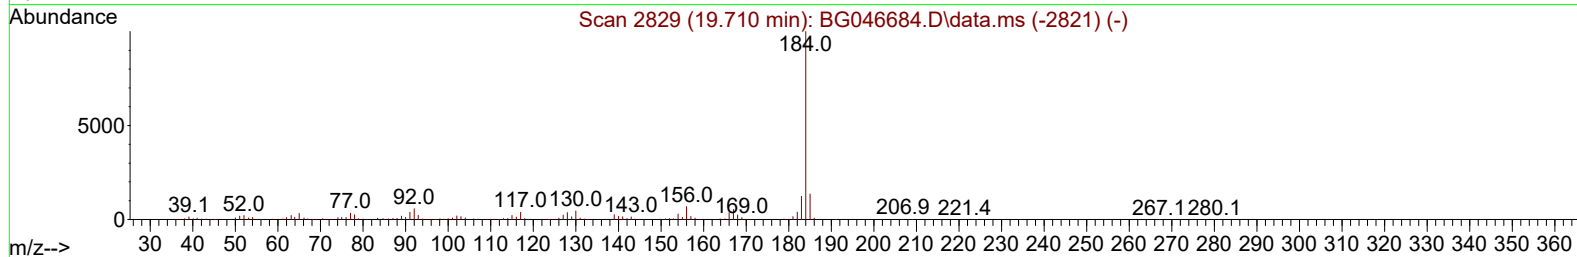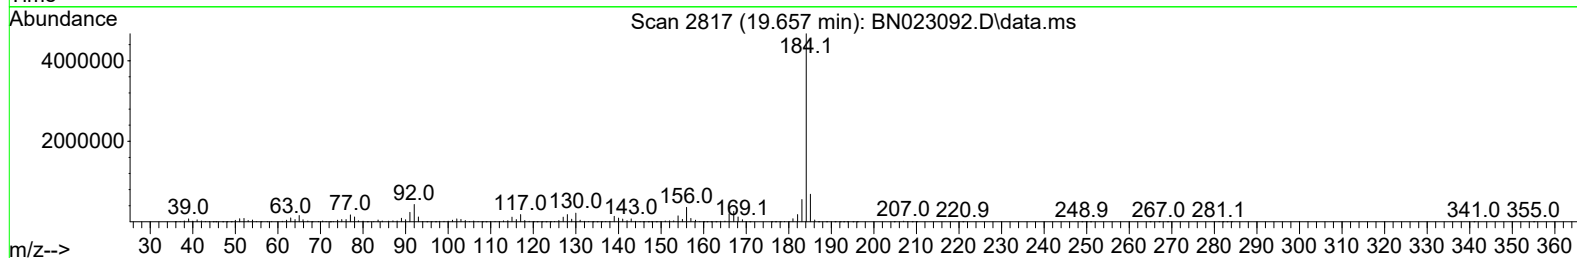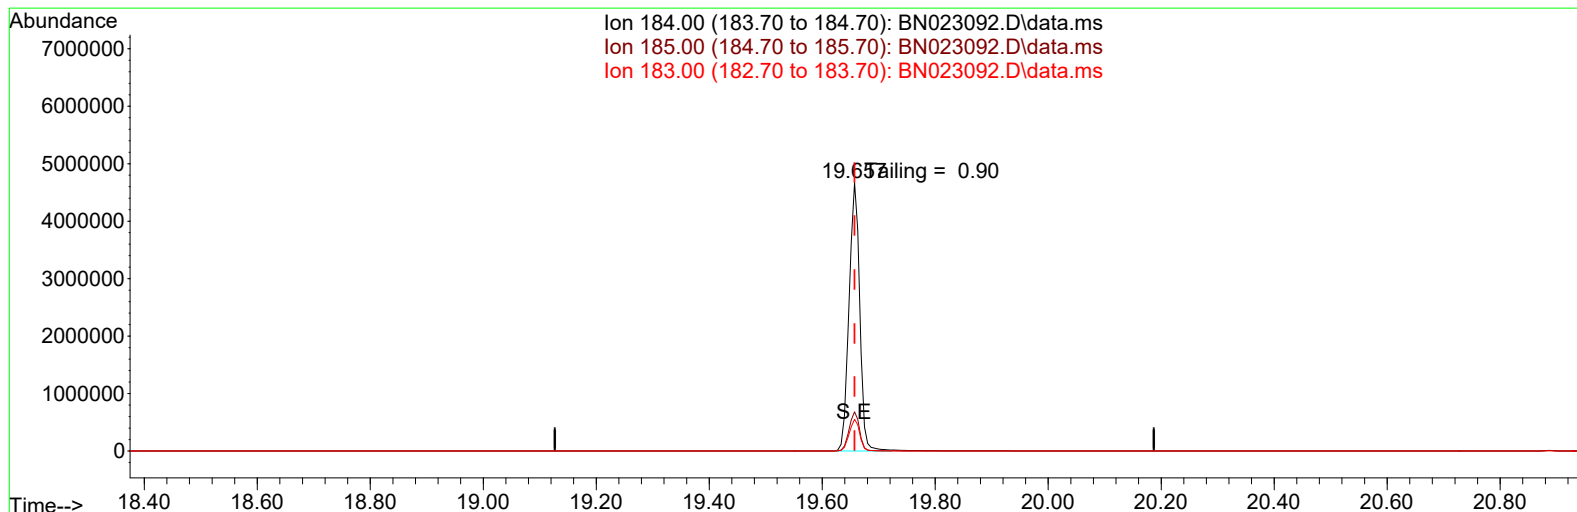

TIC: BN023092.D\data.ms

(77) Benzidine**19.657min (0.000) 3431862.86 ng****response 6135730**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.62
183.00	13.20	11.85
0.00	0.00	0.00