
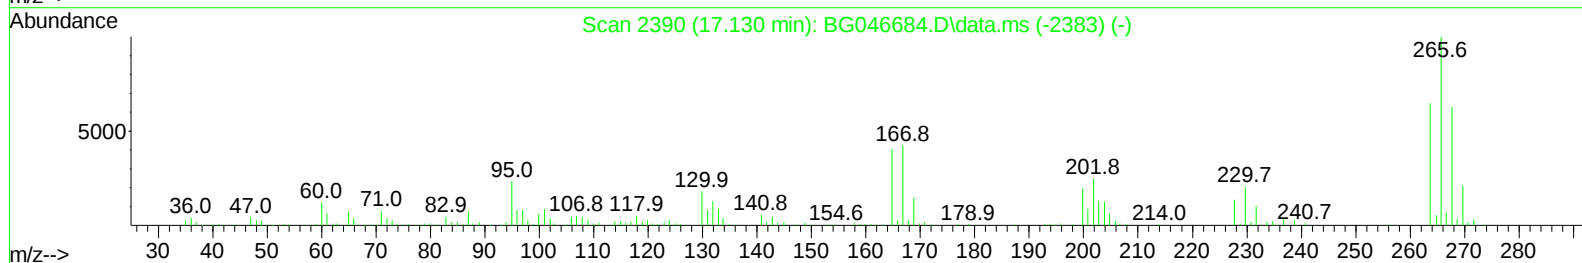
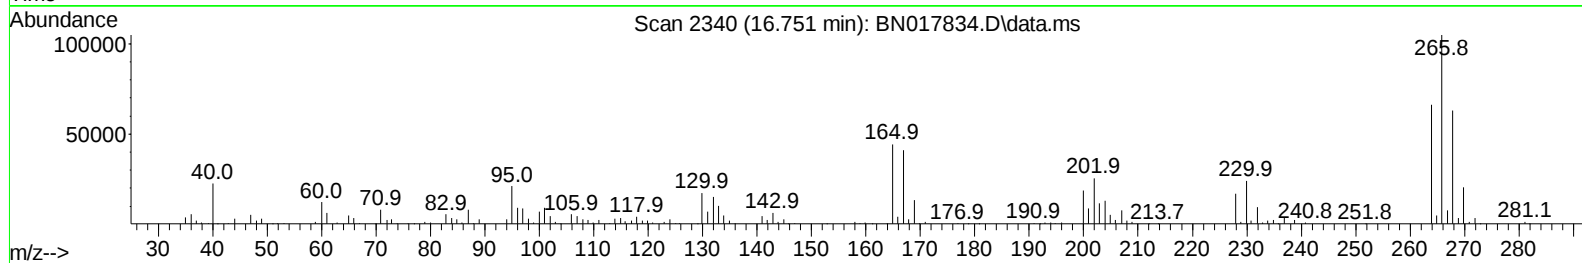


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120921\
Data File : BN017834.D
Acq On : 09 Dec 2021 13:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 08:38:50 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 09 12:31:20 2021
Response via : Initial Calibration

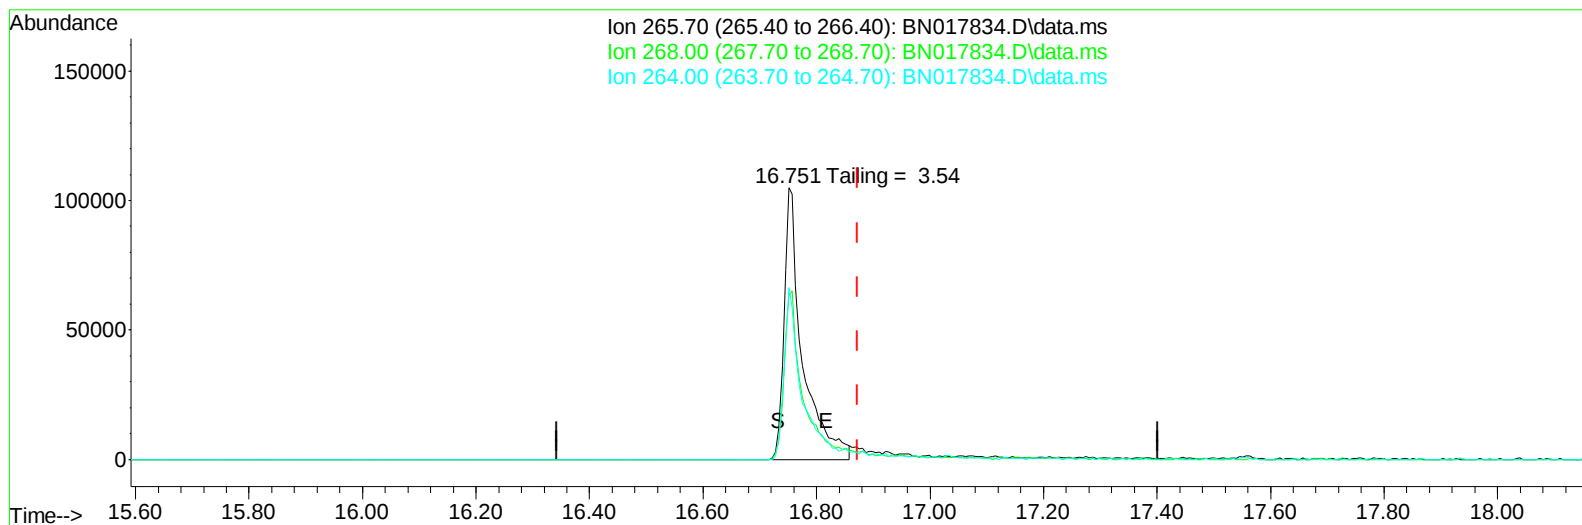




TIC: BN017834.D\data.ms

(70) Pentachlorophenol (C)**16.751min (-0.121) 9192.41 ng****response 249387**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.16
264.00	61.60	63.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120921\
Data File : BN017834.D
Acq On : 09 Dec 2021 13:47
Operator : CG/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 08:38:50 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 09 12:31:20 2021
Response via : Initial Calibration

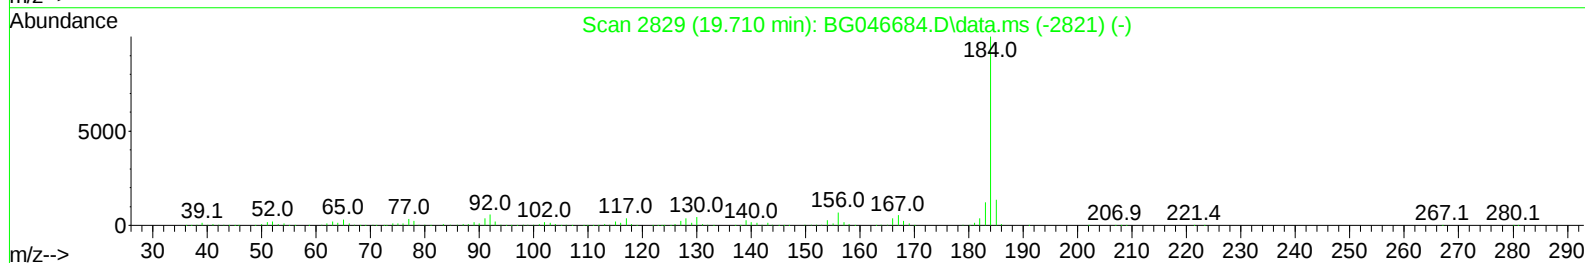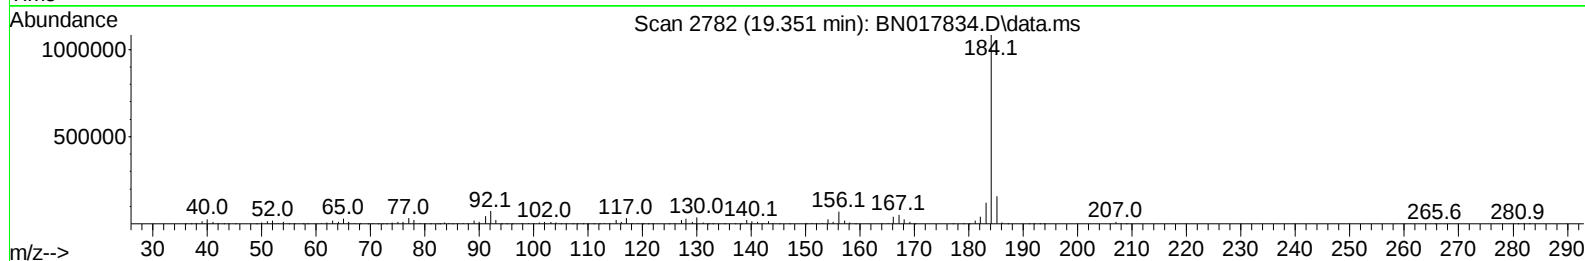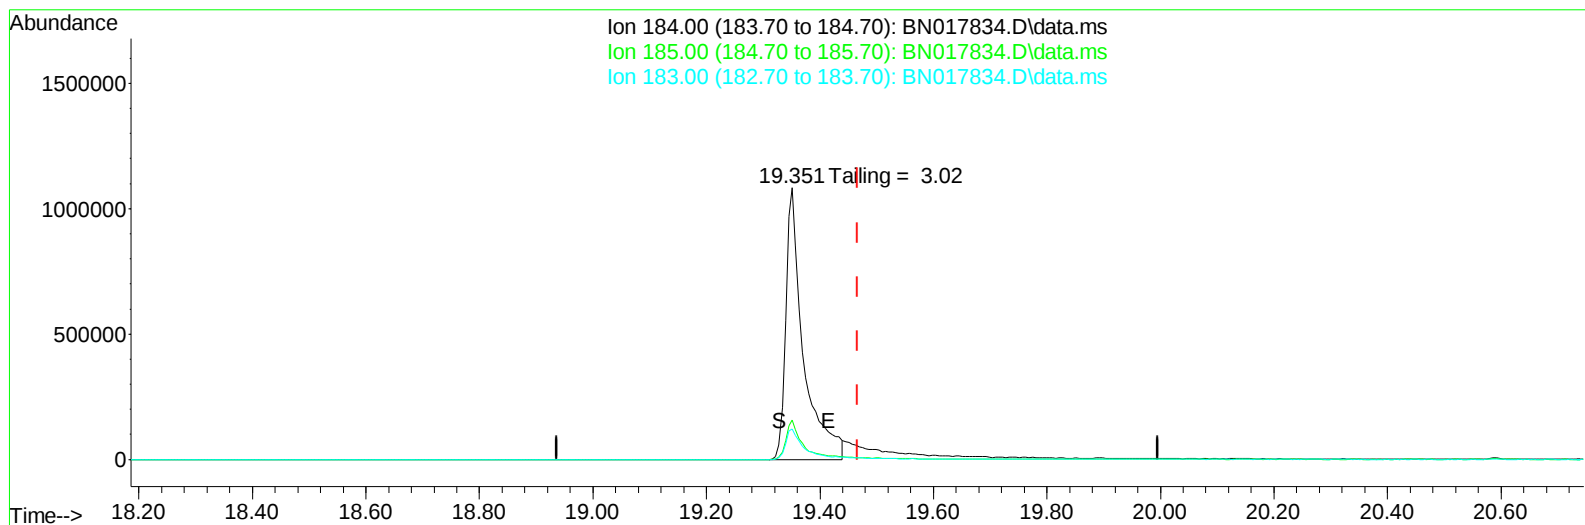

TIC: BN017834.D\data.ms

(77) Benzidine**19.351min (-0.115) 0.00 ng****response 2663192**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.46
183.00	13.20	11.18
0.00	0.00	0.00