
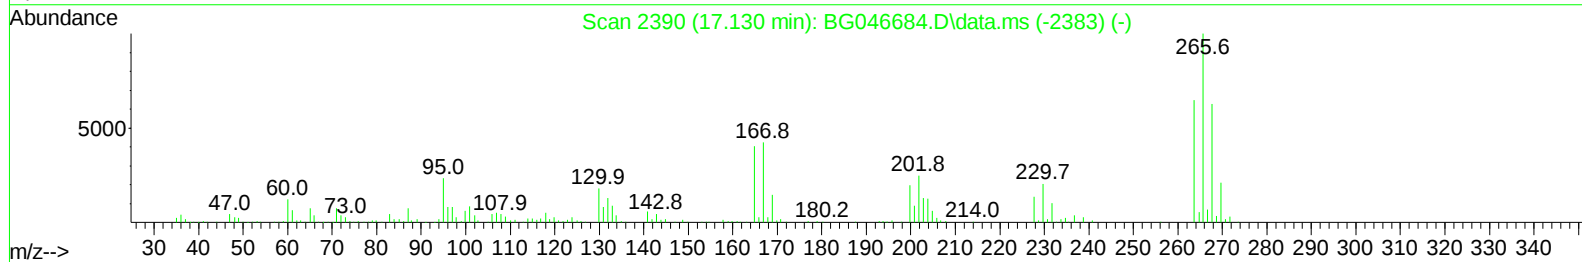
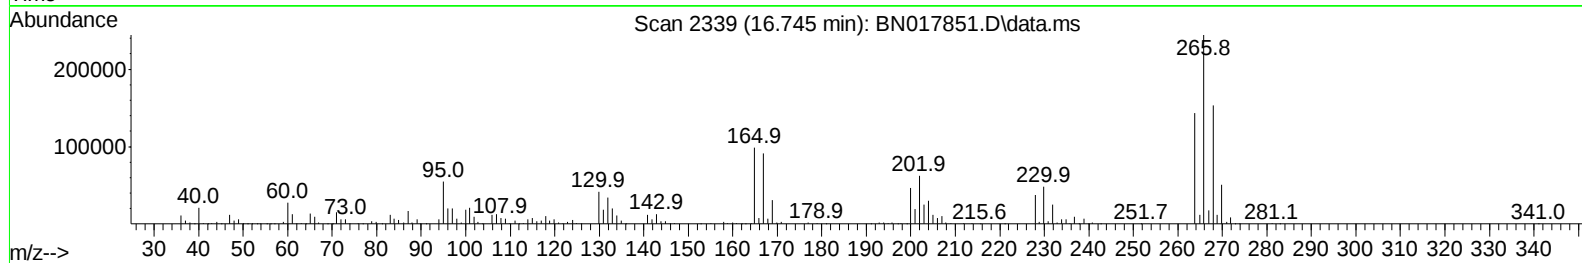


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120921\
Data File : BN017851.D
Acq On : 10 Dec 2021 01:42
Operator : CG/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 08:40:43 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 09 12:31:20 2021
Response via : Initial Calibration

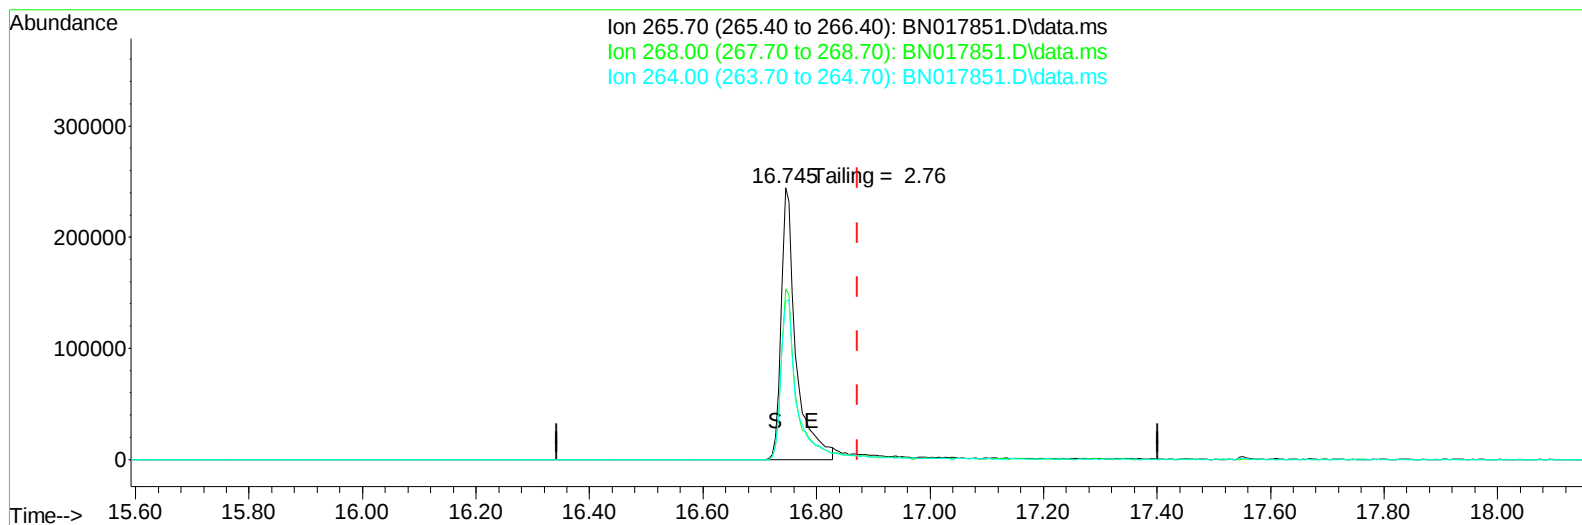

TIC: BN017851.D\data.ms

(70) Pentachlorophenol (C)




16.745min (-0.127) 13697.44 ng

response 467599

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.85
264.00	61.60	58.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120921\
 Data File : BN017851.D
 Acq On : 10 Dec 2021 01:42
 Operator : CG/JU
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 08:40:43 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 09 12:31:20 2021
 Response via : Initial Calibration

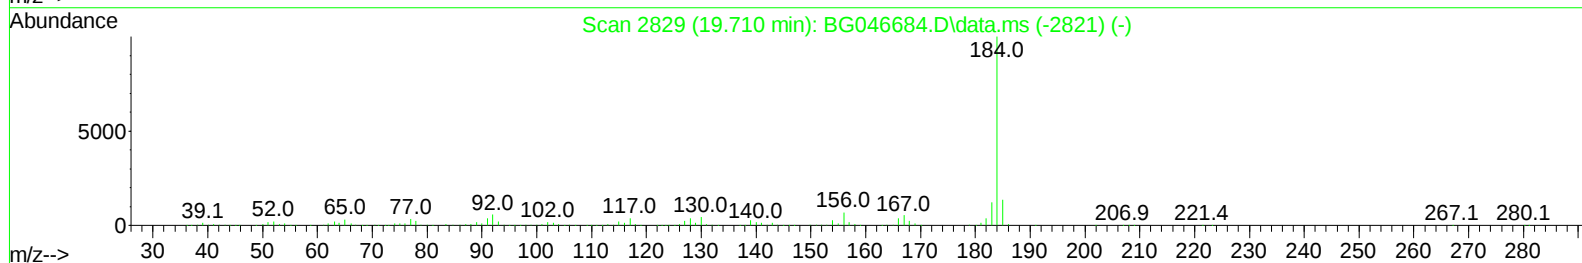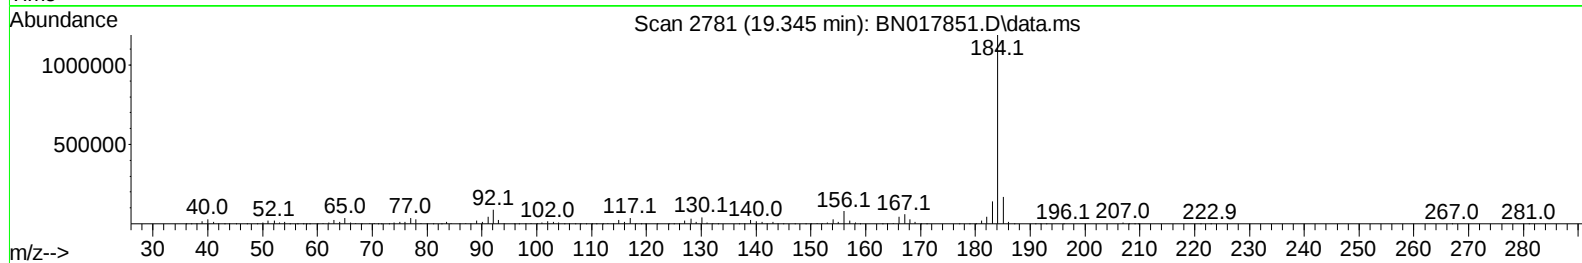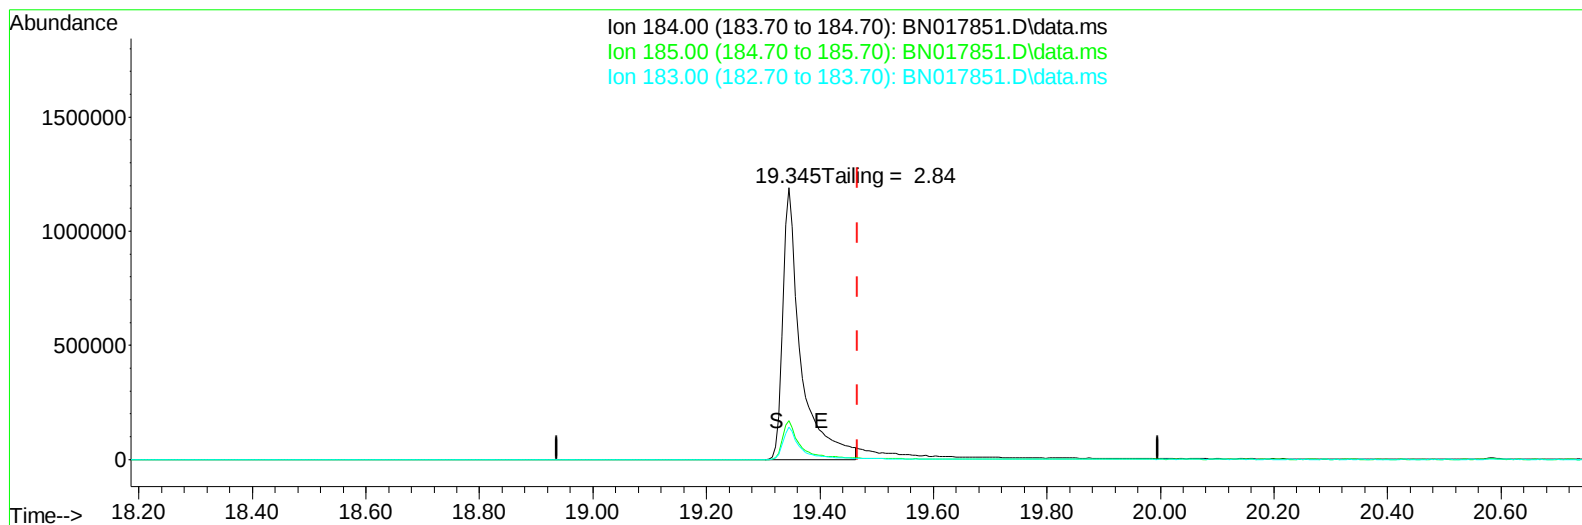

TIC: BN017851.D\data.ms

(77) Benzidine**19.345min (-0.121) 0.00 ng****response 2802502**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.31
183.00	13.20	12.02
0.00	0.00	0.00